

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042421\
 Data File : BN014399.D
 Acq On : 24 Apr 2021 12:44
 Operator : CG/JU
 Sample : PB135930BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK930

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.611	86	89	102	rBV	382342	621170	15.35%	1.567%
2	6.852	634	640	652	rBV	705541	1087939	26.88%	2.745%
3	7.022	664	669	680	rVB	589353	910794	22.51%	2.298%
4	7.216	696	702	714	rVB	770764	1204603	29.77%	3.040%
5	7.681	776	781	790	rVB	504781	805914	19.92%	2.034%
6	8.381	894	900	913	rVB	901928	1394116	34.45%	3.518%
7	8.828	970	976	985	rVB	707502	1175513	29.05%	2.966%
8	9.546	1092	1098	1108	rVB	507729	836656	20.68%	2.111%
9	10.081	1183	1189	1203	rVB	901431	1438073	35.54%	3.629%
10	10.457	1247	1253	1262	rVB	700573	1177334	29.09%	2.971%
11	10.593	1269	1276	1290	rBV	900604	1498387	37.03%	3.781%
12	12.051	1520	1524	1529	rVB3	11920	18653	0.46%	0.047%
13	13.734	1803	1810	1818	rBV	1480254	2054592	50.77%	5.184%
14	14.010	1850	1857	1864	rBV	1953312	2738203	67.67%	6.909%
15	14.322	1902	1910	1917	rBV	994202	1474361	36.43%	3.720%
16	14.516	1936	1943	1961	rBV	598198	850863	21.03%	2.147%
17	15.316	2072	2079	2089	rVB	2260387	3116913	77.02%	7.865%
18	15.434	2093	2099	2109	rVB	453917	611690	15.12%	1.543%
19	15.557	2115	2120	2126	rVB	19159	24709	0.61%	0.062%
20	16.104	2209	2213	2217	rVB4	4844	6117	0.15%	0.015%
21	17.063	2370	2376	2385	rVB	1140149	1609428	39.77%	4.061%
22	17.163	2387	2393	2405	rVV	2422154	3316132	81.95%	8.367%
23	19.098	2718	2722	2726	rBV	14849	19321	0.48%	0.049%
24	19.351	2759	2765	2770	rBV	13976	18307	0.45%	0.046%
25	19.469	2778	2785	2796	rBV	2860519	3865839	95.53%	9.754%
26	21.263	3084	3090	3100	rBV	1412146	1722333	42.56%	4.346%
27	22.827	3353	3356	3362	rVB3	40024	54076	1.34%	0.136%
28	23.345	3437	3444	3459	rBV	2172016	4046674	100.00%	10.211%
29	23.486	3461	3468	3483	rVB2	974998	1840536	45.48%	4.644%
30	24.033	3558	3561	3567	rVB3	56287	92175	2.28%	0.233%


Sum of corrected areas: 39631421

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042421\
Data File : BN014399.D
Acq On : 24 Apr 2021 12:44
Operator : CG/JU
Sample : PB135930BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK930

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

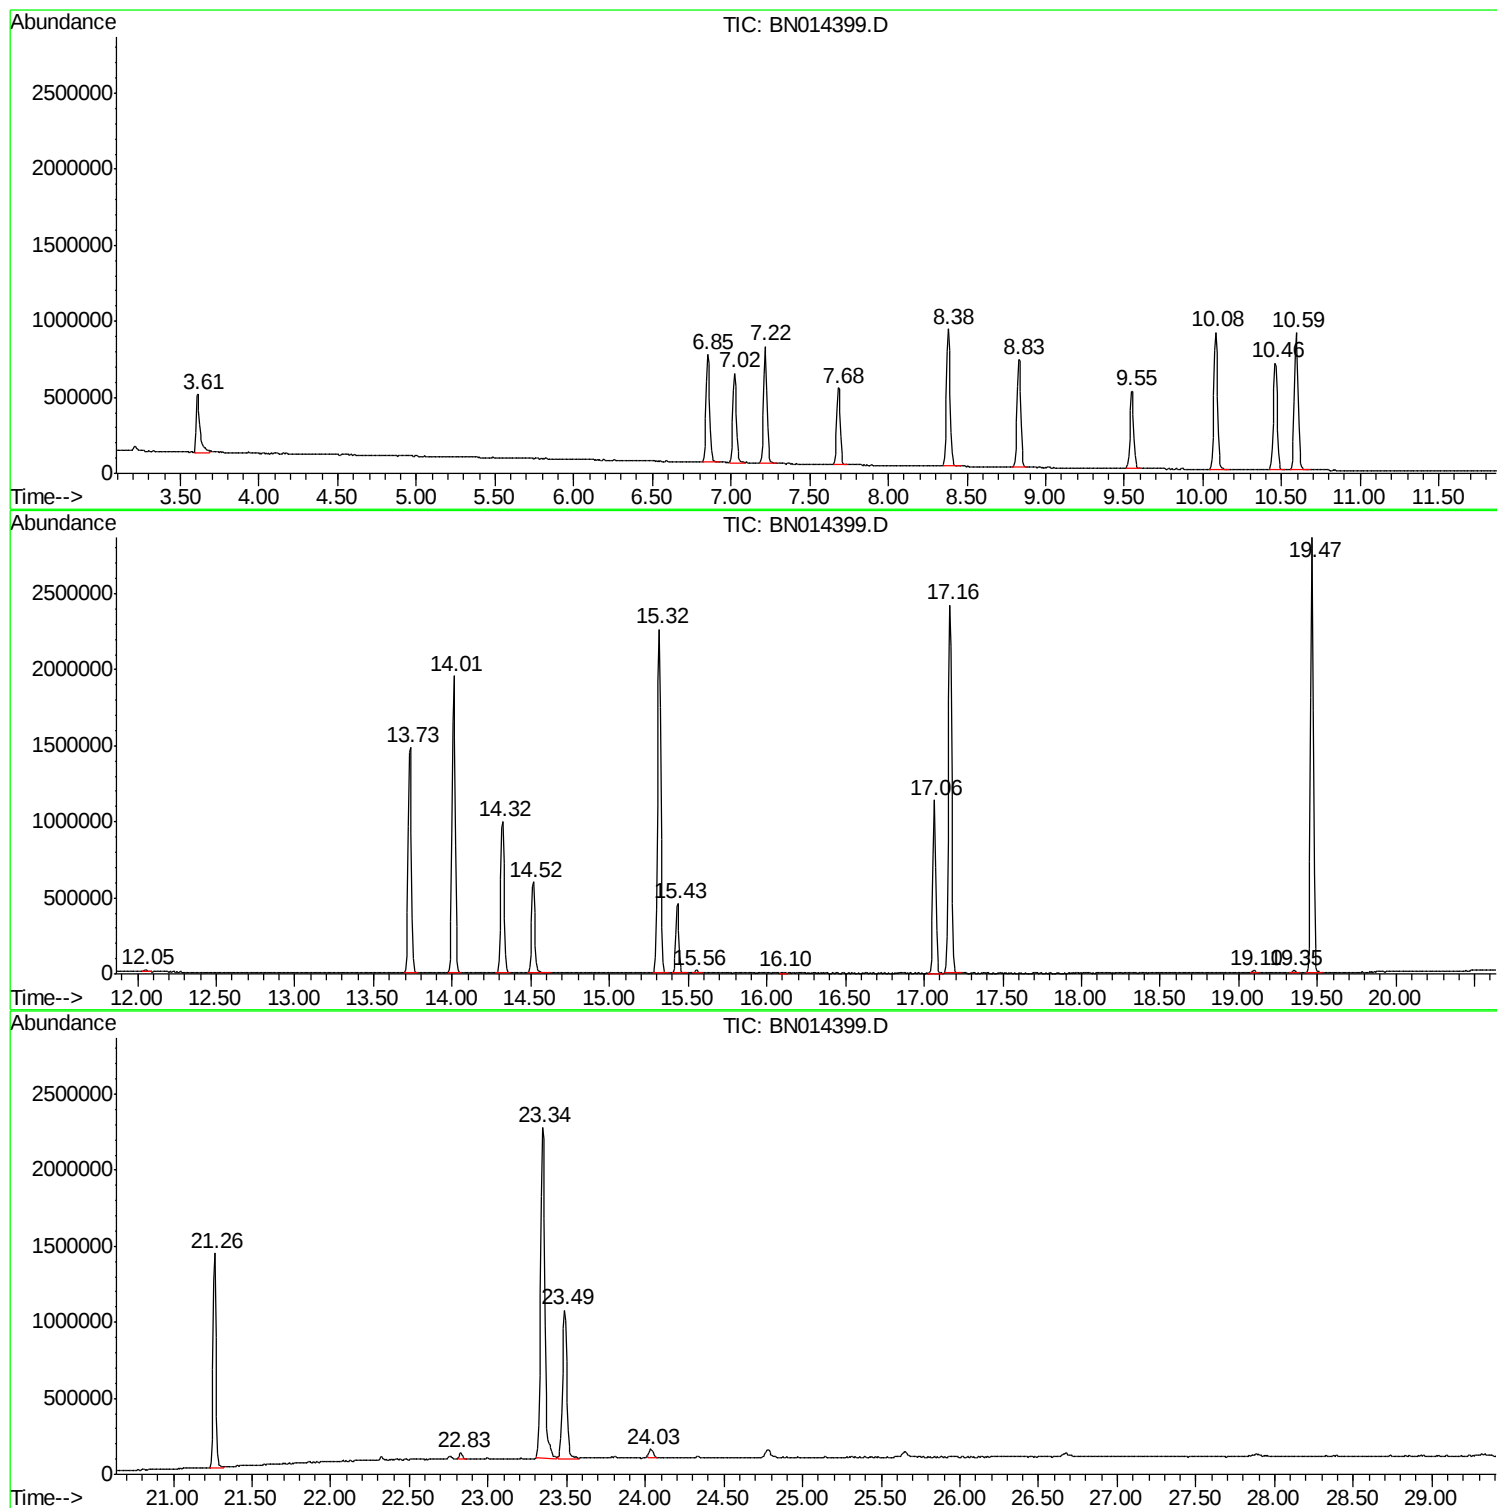

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
Data File : BN014399.D
Acq On : 24 Apr 2021 12:44
Operator : CG/JU
Sample : PB135930BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK930

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
Data File : BN014399.D
Acq On : 24 Apr 2021 12:44
Operator : CG/JU
Sample : PB135930BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK930

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc