

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042421\
 Data File : BN014404.D
 Acq On : 24 Apr 2021 15:42
 Operator : CG/JU
 Sample : M2127-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E0AB0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.852	635	640	643	rBV	140167	236317	6.37%	0.714%
2	7.022	664	669	678	rVB	496127	765125	20.64%	2.313%
3	7.216	696	702	710	rVB	542093	842670	22.73%	2.548%
4	7.681	775	781	789	rVB	465435	737640	19.90%	2.230%
5	8.381	894	900	910	rVB	402079	624194	16.84%	1.887%
6	8.828	970	976	986	rVB	636367	1046627	28.23%	3.164%
7	9.269	1048	1051	1058	rVB	14071	20809	0.56%	0.063%
8	9.546	1092	1098	1111	rVB	443714	718002	19.37%	2.171%
9	10.081	1183	1189	1200	rVB	736243	1171092	31.59%	3.541%
10	10.457	1247	1253	1261	rBV	658598	1080551	29.14%	3.267%
11	10.598	1272	1277	1287	rVB	37269	64717	1.75%	0.196%
12	11.251	1383	1388	1396	rBV2	24257	41617	1.12%	0.126%
13	12.051	1520	1524	1532	rVB2	12767	21559	0.58%	0.065%
14	12.934	1669	1674	1676	rVB5	3052	4282	0.12%	0.013%
15	13.157	1707	1712	1716	rVB2	7261	10150	0.27%	0.031%
16	13.222	1719	1723	1727	rVB2	4643	5702	0.15%	0.017%
17	13.728	1803	1809	1814	rBV	1362152	1848837	49.87%	5.590%
18	13.775	1814	1817	1823	rVB	64881	89826	2.42%	0.272%
19	14.010	1847	1857	1864	rBV	1735108	2520444	67.98%	7.620%
20	14.234	1892	1895	1899	rVB2	6060	7123	0.19%	0.022%
21	14.322	1903	1910	1916	rBV	944014	1371618	36.99%	4.147%
22	14.510	1937	1942	1952	rBV	78327	115223	3.11%	0.348%
23	14.739	1976	1981	1985	rBV5	3161	4246	0.11%	0.013%
24	15.145	2044	2050	2053	rBV2	9820	17677	0.48%	0.053%
25	15.186	2055	2057	2065	rVB4	5836	7072	0.19%	0.021%
26	15.316	2072	2079	2088	rBV	2119371	2944950	79.43%	8.903%
27	15.428	2092	2098	2108	rBV	379846	523412	14.12%	1.582%
28	15.557	2115	2120	2123	rBV	16659	21909	0.59%	0.066%
29	15.692	2138	2143	2145	rVB3	2628	3989	0.11%	0.012%
30	16.051	2199	2204	2206	rVV4	4219	6737	0.18%	0.020%
31	16.104	2210	2213	2220	rVB4	8378	12133	0.33%	0.037%
32	16.222	2228	2233	2236	rBV5	3734	4902	0.13%	0.015%
33	16.316	2245	2249	2253	rBV2	8593	11941	0.32%	0.036%
34	16.410	2258	2265	2268	rBV5	2233	4232	0.11%	0.013%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
 Data File : BN014404.D
 Acq On : 24 Apr 2021 15:42
 Operator : CG/JU
 Sample : M2127-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E0AB0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Title : SVOA CALIBRATION

35	16.816	2326	2334	2336	rBV5	6686	9335	0.25%	0.028%
36	16.845	2336	2339	2344	rVV2	6458	9965	0.27%	0.030%
37	16.898	2344	2348	2351	rVB3	2426	3738	0.10%	0.011%
38	17.063	2370	2376	2384	rBV	1082664	1536663	41.45%	4.646%
39	17.163	2387	2393	2402	rBV	2350490	3200727	86.33%	9.677%
40	17.363	2422	2427	2430	rBV3	3636	4911	0.13%	0.015%
41	17.575	2456	2463	2467	rBV4	2742	4246	0.11%	0.013%
42	17.969	2525	2530	2534	rBV	35740	46746	1.26%	0.141%
43	18.039	2540	2542	2546	rVB	6806	7580	0.20%	0.023%
44	18.145	2554	2560	2564	rBV5	2811	5010	0.14%	0.015%
45	18.480	2613	2617	2623	rBV3	5584	7576	0.20%	0.023%
46	18.745	2656	2662	2667	rBV	38148	51992	1.40%	0.157%
47	19.098	2717	2722	2726	rBV	17636	24798	0.67%	0.075%
48	19.133	2726	2728	2737	rVB6	4327	8059	0.22%	0.024%
49	19.257	2744	2749	2753	rBV2	21986	30545	0.82%	0.092%
50	19.351	2762	2765	2769	rBV	13315	16251	0.44%	0.049%
51	19.463	2778	2784	2793	rBV	2673112	3654857	98.58%	11.050%
52	20.027	2878	2880	2884	rBV4	4794	5457	0.15%	0.016%
53	20.527	2962	2965	2968	rVB4	7064	9080	0.24%	0.027%
54	20.986	3038	3043	3050	rBV4	36012	62683	1.69%	0.190%
55	21.263	3084	3090	3100	rBV	1297437	1617759	43.63%	4.891%
56	21.427	3115	3118	3121	rVB4	14660	16731	0.45%	0.051%
57	21.863	3189	3192	3196	rVB3	26984	32057	0.86%	0.097%
58	22.321	3267	3270	3274	rVB	39614	47378	1.28%	0.143%
59	22.827	3352	3356	3362	rVB2	57915	86061	2.32%	0.260%
60	23.345	3437	3444	3460	rBV	2015917	3707639	100.00%	11.209%
61	23.486	3461	3468	3482	rVB2	906964	1674779	45.17%	5.063%
62	24.033	3556	3561	3567	rVB	79312	134760	3.63%	0.407%
63	24.774	3683	3687	3702	rVB	68977	151863	4.10%	0.459%


Sum of corrected areas: 33076571

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
Data File : BN014404.D
Acq On : 24 Apr 2021 15:42
Operator : CG/JU
Sample : M2127-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0AB0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

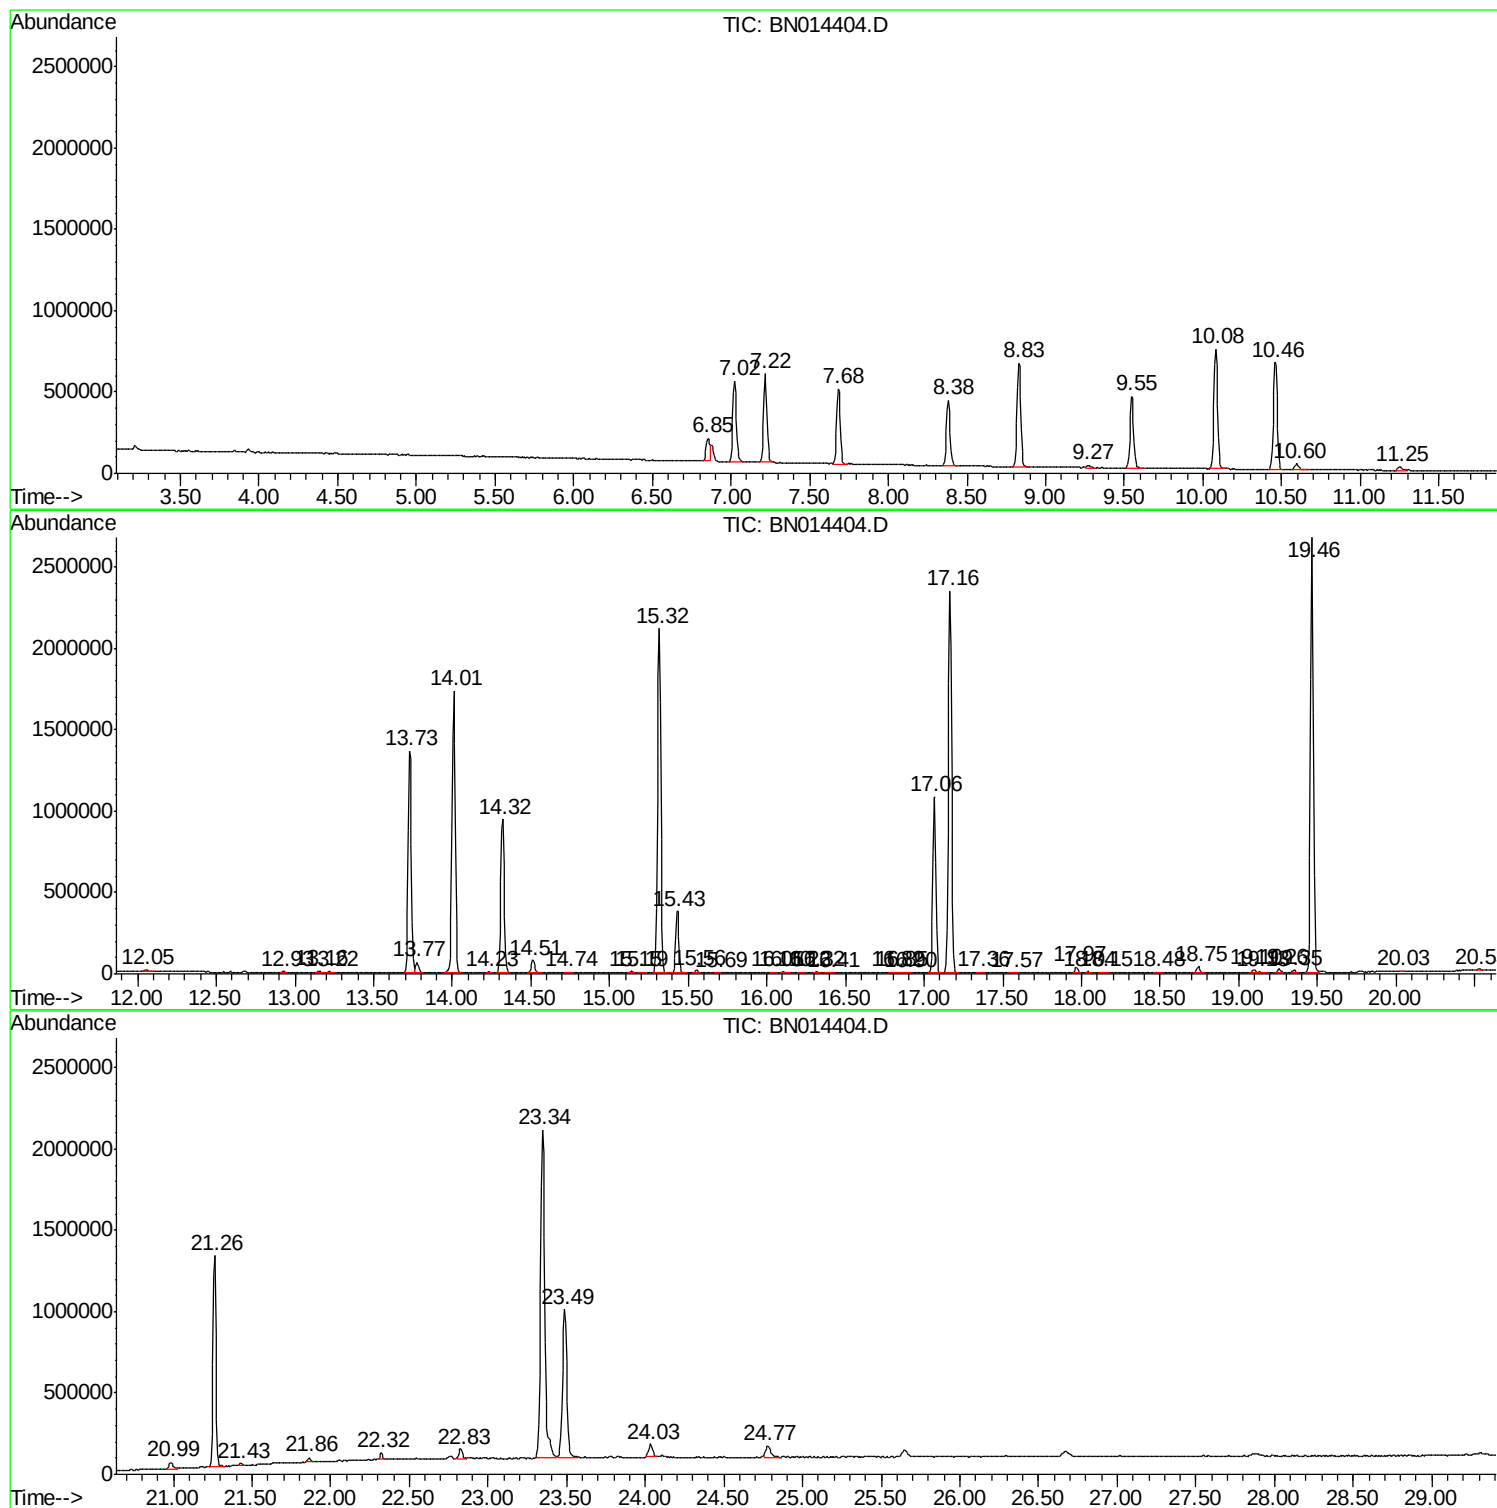

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
Data File : BN014404.D
Acq On : 24 Apr 2021 15:42
Operator : CG/JU
Sample : M2127-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0AB0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
Data File : BN014404.D
Acq On : 24 Apr 2021 15:42
Operator : CG/JU
Sample : M2127-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0AB0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc