

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042421\
 Data File : BN014407.D
 Acq On : 24 Apr 2021 17:29
 Operator : CG/JU
 Sample : PB135931BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK931

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.611	85	89	108	rBV	395844	651918	15.18%	1.539%
2	6.852	634	640	652	rVB	715137	1110416	25.85%	2.621%
3	7.022	663	669	683	rVB	586357	942455	21.94%	2.225%
4	7.216	696	702	712	rBV	776122	1220105	28.40%	2.880%
5	7.681	776	781	789	rVB	544452	862868	20.09%	2.037%
6	8.381	894	900	909	rBV	927559	1433169	33.36%	3.383%
7	8.834	970	977	986	rVB	733008	1231085	28.66%	2.906%
8	9.546	1092	1098	1108	rBV	533102	877814	20.43%	2.072%
9	10.081	1182	1189	1200	rBV	959508	1496717	34.84%	3.533%
10	10.457	1246	1253	1260	rBV	770608	1274186	29.66%	3.008%
11	10.593	1269	1276	1291	rVB	964695	1564687	36.42%	3.693%
12	12.051	1519	1524	1530	rVB	13158	20469	0.48%	0.048%
13	13.734	1803	1810	1822	rVB	1621779	2230009	51.91%	5.264%
14	14.010	1850	1857	1865	rBV	2022505	2919697	67.97%	6.892%
15	14.322	1903	1910	1917	rBV	1122802	1636728	38.10%	3.863%
16	14.516	1936	1943	1954	rBV	662925	911019	21.21%	2.150%
17	15.316	2072	2079	2088	rBV	2490667	3358130	78.17%	7.927%
18	15.433	2092	2099	2110	rBV	475562	663165	15.44%	1.565%
19	15.557	2115	2120	2124	rVB	21558	27731	0.65%	0.065%
20	16.104	2209	2213	2216	rVB2	4944	6083	0.14%	0.014%
21	17.063	2370	2376	2383	rBV	1249286	1786145	41.58%	4.216%
22	17.163	2387	2393	2405	rVB	2566412	3592885	83.64%	8.481%
23	19.098	2717	2722	2728	rBV	14877	19393	0.45%	0.046%
24	19.351	2760	2765	2771	rVB	13527	17750	0.41%	0.042%
25	19.469	2778	2785	2792	rBV	3134072	4194515	97.64%	9.901%
26	21.263	3084	3090	3101	rBV	1539205	1897411	44.17%	4.479%
27	22.827	3353	3356	3360	rVB	31226	38319	0.89%	0.090%
28	23.345	3437	3444	3460	rBV	2397051	4295778	100.00%	10.140%
29	23.486	3461	3468	3479	rVB	1101609	1988654	46.29%	4.694%
30	24.033	3557	3561	3568	rVB2	52280	95338	2.22%	0.225%


Sum of corrected areas: 42364639

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042421\
Data File : BN014407.D
Acq On : 24 Apr 2021 17:29
Operator : CG/JU
Sample : PB135931BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK931

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

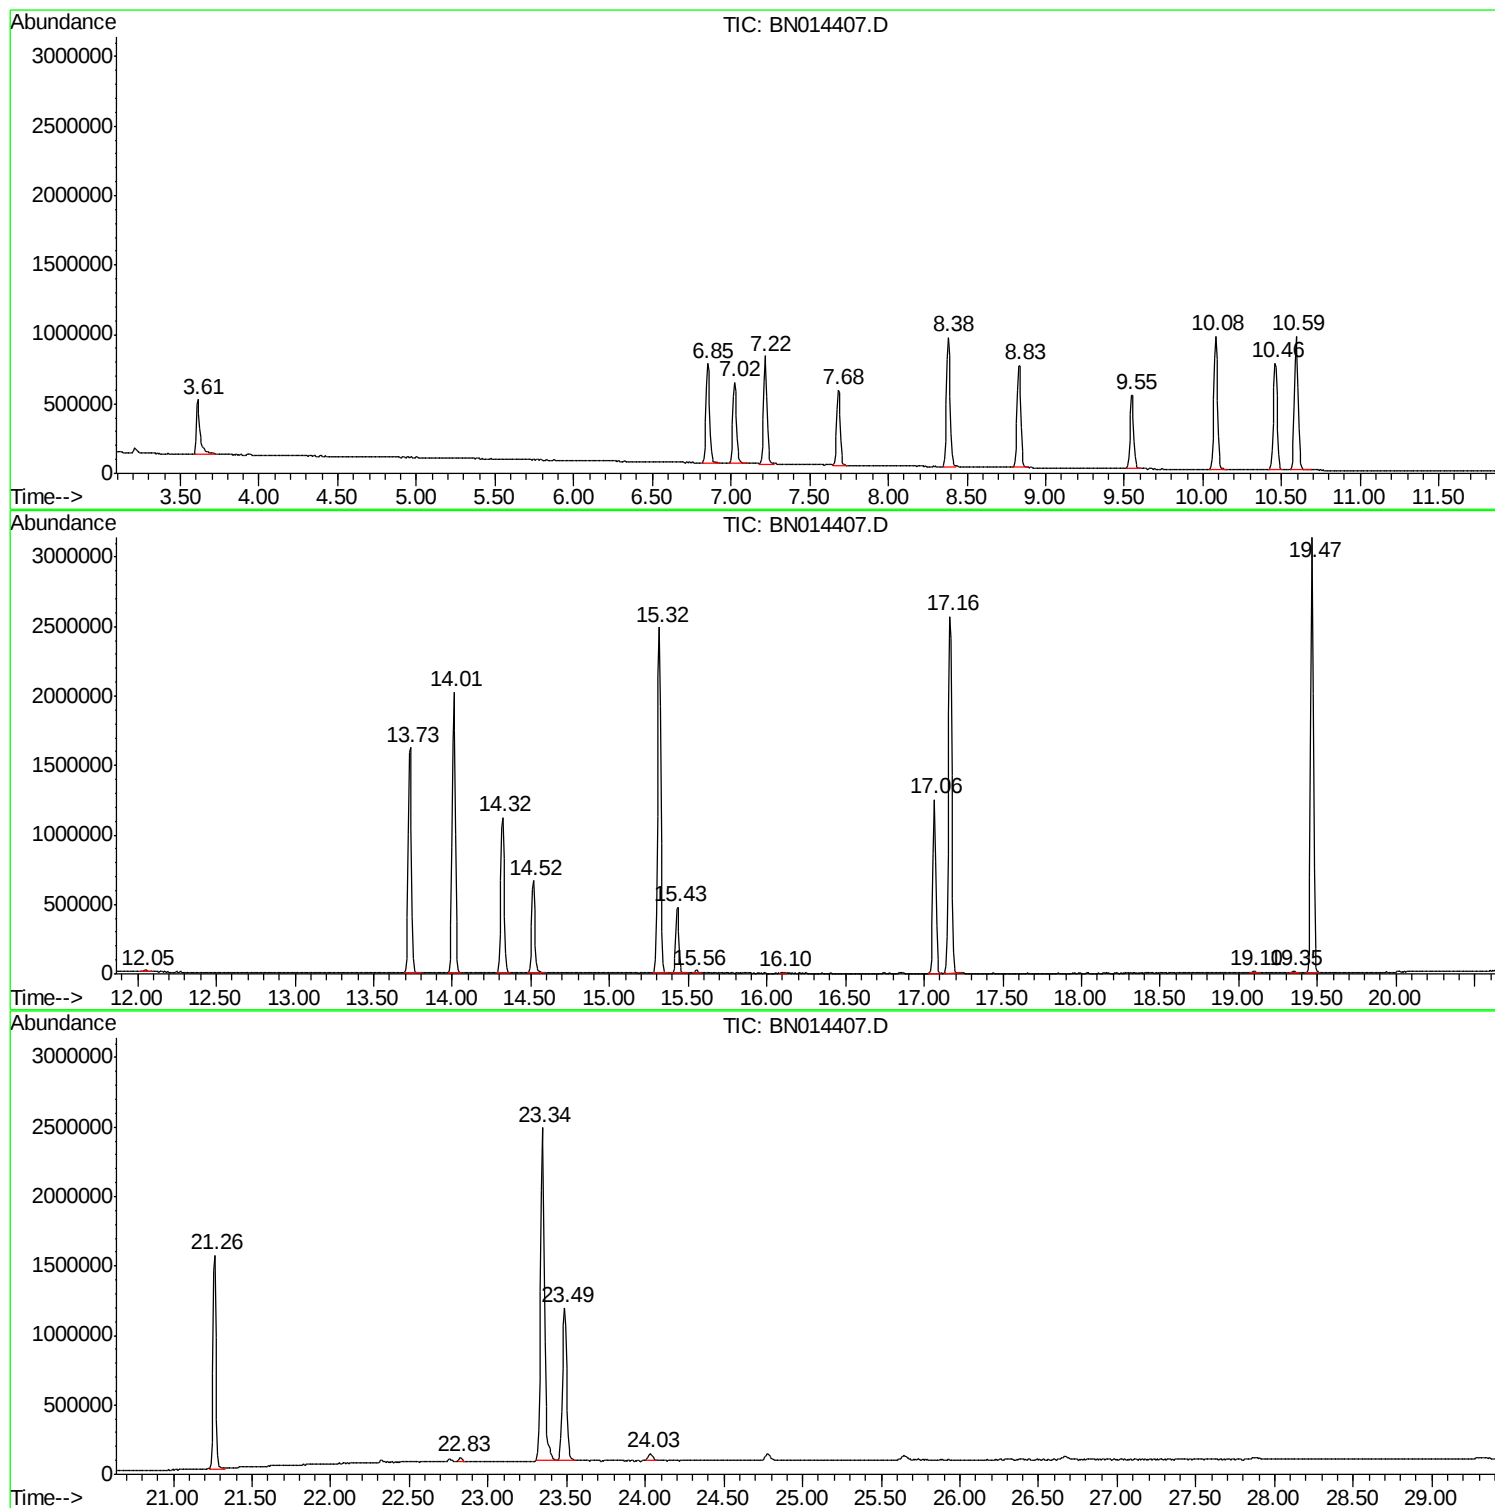

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
Data File : BN014407.D
Acq On : 24 Apr 2021 17:29
Operator : CG/JU
Sample : PB135931BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK931

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
Data File : BN014407.D
Acq On : 24 Apr 2021 17:29
Operator : CG/JU
Sample : PB135931BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK931

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc