

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042421\
 Data File : BN014431.D
 Acq On : 25 Apr 2021 08:54
 Operator : CG/JU
 Sample : PB135971BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK971

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.610	85	89	104	rBV	298574	503474	13.56%	1.356%
2	6.851	634	640	652	rVB	560711	862462	23.23%	2.322%
3	7.022	664	669	679	rVB	460828	725306	19.54%	1.953%
4	7.216	696	702	714	rVB	625008	977995	26.35%	2.633%
5	7.681	775	781	788	rVB	478849	731570	19.71%	1.970%
6	8.381	894	900	912	rVB	761498	1190400	32.07%	3.205%
7	8.828	970	976	986	rVB	632392	1018043	27.42%	2.741%
8	9.545	1092	1098	1107	rBV	424062	680916	18.34%	1.834%
9	10.081	1182	1189	1199	rBV	774504	1263912	34.05%	3.403%
10	10.457	1246	1253	1262	rVB	701345	1157517	31.18%	3.117%
11	10.592	1269	1276	1291	rVB	815899	1336891	36.01%	3.600%
12	12.051	1520	1524	1530	rVB2	11886	18855	0.51%	0.051%
13	13.728	1803	1809	1819	rBV	1490130	1971681	53.11%	5.309%
14	14.010	1850	1857	1864	rBV	1770034	2584223	69.61%	6.959%
15	14.316	1903	1909	1916	rBV2	1022364	1506739	40.59%	4.057%
16	14.510	1936	1942	1961	rBV	536015	758990	20.45%	2.044%
17	15.316	2072	2079	2089	rVB	2133733	3008836	81.05%	8.102%
18	15.427	2093	2098	2108	rBV	374643	492521	13.27%	1.326%
19	15.551	2114	2119	2124	rBV	17433	23522	0.63%	0.063%
20	16.098	2209	2212	2215	rVB3	4922	5585	0.15%	0.015%
21	16.851	2333	2340	2344	rBV2	2776	3875	0.10%	0.010%
22	17.063	2370	2376	2383	rBV	1230903	1660652	44.73%	4.472%
23	17.163	2387	2393	2405	rVB	2341981	3166227	85.29%	8.526%
24	19.098	2716	2722	2727	rBV	17040	22142	0.60%	0.060%
25	19.351	2760	2765	2771	rBV	11862	16634	0.45%	0.045%
26	19.463	2778	2784	2795	rBV	2762825	3616753	97.43%	9.739%
27	20.727	2996	2999	3002	rBV5	4519	7975	0.21%	0.021%
28	21.257	3084	3089	3101	rBV	1511083	1886894	50.83%	5.081%
29	22.315	3267	3269	3276	rVB2	31573	39633	1.07%	0.107%
30	22.821	3351	3355	3363	rVB	52242	69847	1.88%	0.188%
31	23.345	3437	3444	3460	rBV	2034000	3712213	100.00%	9.996%
32	23.480	3461	3467	3476	rVB2	999138	1850784	49.86%	4.984%
33	24.027	3556	3560	3568	rVB	71976	132070	3.56%	0.356%
34	24.774	3682	3687	3694	rVB	66585	132287	3.56%	0.356%

LSC Area Percent Report

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042421\
Data File : BN014431.D
Acq On : 25 Apr 2021 08:54
Operator : CG/JU
Sample : PB135971BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK971

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Title : SVOA CALIBRATION


Sum of corrected areas: 37137424

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042421\
Data File : BN014431.D
Acq On : 25 Apr 2021 08:54
Operator : CG/JU
Sample : PB135971BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK971

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

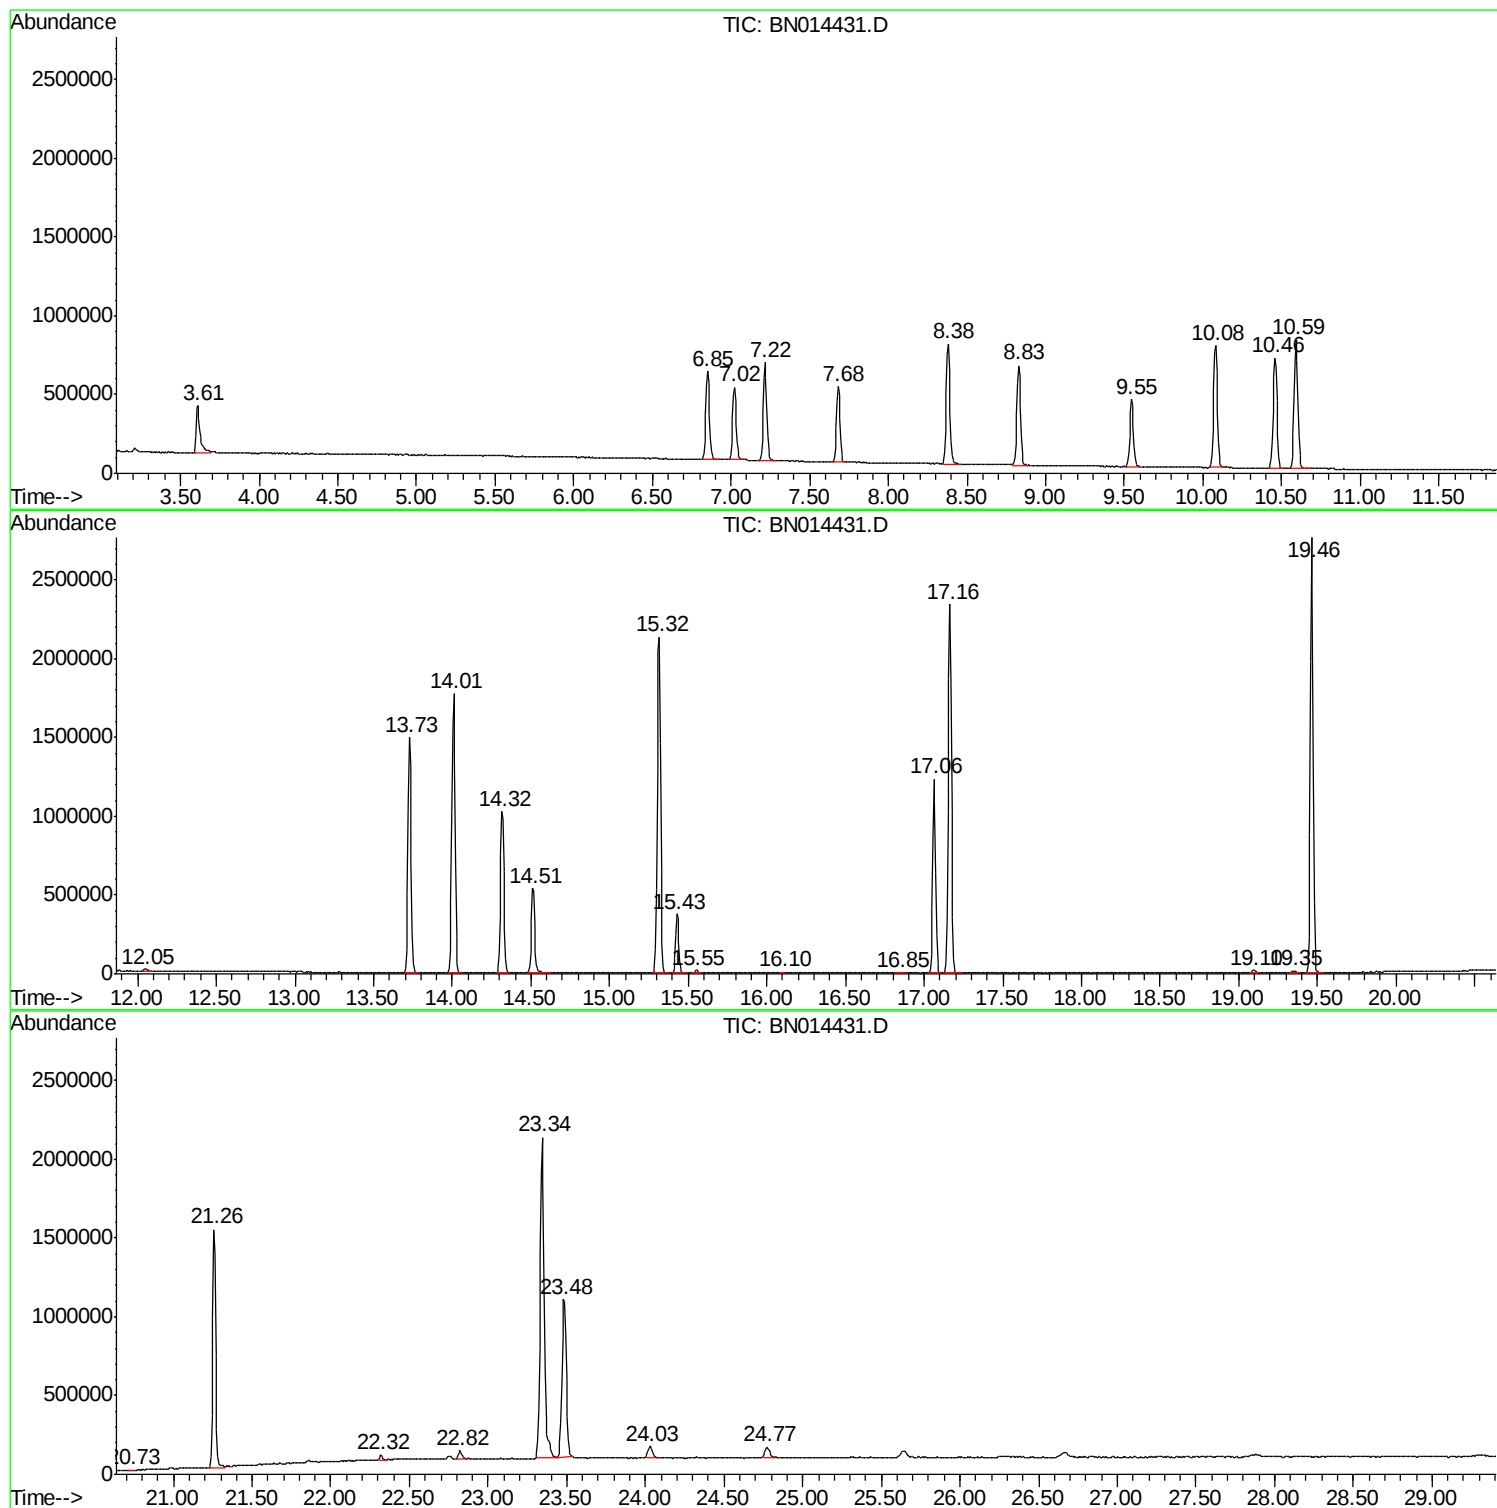

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
Data File : BN014431.D
Acq On : 25 Apr 2021 08:54
Operator : CG/JU
Sample : PB135971BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK971

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
Data File : BN014431.D
Acq On : 25 Apr 2021 08:54
Operator : CG/JU
Sample : PB135971BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK971

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc