

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042421\
 Data File : BN014433.D
 Acq On : 25 Apr 2021 10:05
 Operator : CG/JU
 Sample : M2127-21
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E0AA2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.852	635	640	650	rVB2	116478	225562	6.52%	0.742%
2	7.022	663	669	678	rBV	393218	634188	18.33%	2.085%
3	7.216	696	702	709	rBV	451289	699894	20.22%	2.301%
4	7.681	775	781	790	rVB	435109	672516	19.43%	2.211%
5	8.381	894	900	908	rVB	338262	536784	15.51%	1.765%
6	8.828	970	976	988	rVB	565464	913871	26.41%	3.005%
7	9.546	1092	1098	1110	rVB	382773	600614	17.36%	1.975%
8	10.081	1182	1189	1204	rVB	641884	1059979	30.63%	3.485%
9	10.457	1246	1253	1261	rVB	633786	1044514	30.18%	3.434%
10	10.593	1272	1276	1281	rVB	18830	27681	0.80%	0.091%
11	12.051	1520	1524	1528	rVB	10479	15567	0.45%	0.051%
12	13.151	1708	1711	1714	rVB3	5006	5884	0.17%	0.019%
13	13.728	1803	1809	1814	rBV	1304374	1731908	50.05%	5.694%
14	13.775	1814	1817	1823	rVB	35083	45264	1.31%	0.149%
15	14.010	1847	1857	1864	rBV	1578536	2322835	67.12%	7.637%
16	14.234	1891	1895	1900	rVB2	4633	5696	0.16%	0.019%
17	14.316	1903	1909	1921	rVB	934693	1347292	38.93%	4.430%
18	14.510	1937	1942	1956	rVB	70545	104160	3.01%	0.342%
19	15.128	2044	2047	2053	rBV3	3553	6622	0.19%	0.022%
20	15.187	2053	2057	2061	rVB4	3371	4880	0.14%	0.016%
21	15.310	2072	2078	2086	rVB	1918881	2734284	79.01%	8.990%
22	15.428	2093	2098	2107	rBV	344308	448234	12.95%	1.474%
23	15.551	2115	2119	2123	rBV2	16270	20472	0.59%	0.067%
24	16.051	2199	2204	2206	rBV3	3709	5418	0.16%	0.018%
25	16.098	2209	2212	2219	rVB4	6213	8801	0.25%	0.029%
26	16.316	2243	2249	2252	rBV2	6946	9554	0.28%	0.031%
27	16.845	2336	2339	2343	rVB4	4544	6706	0.19%	0.022%
28	17.063	2370	2376	2384	rVB	1074847	1479894	42.76%	4.866%
29	17.163	2386	2393	2407	rVB	2151966	3004291	86.81%	9.878%
30	17.969	2525	2530	2536	rBV	63561	89912	2.60%	0.296%
31	18.480	2612	2617	2621	rBV3	4078	7444	0.22%	0.024%
32	18.575	2629	2633	2638	rBV3	2530	3816	0.11%	0.013%
33	18.739	2656	2661	2667	rBV	28307	35516	1.03%	0.117%
34	19.092	2717	2721	2726	rBV	15958	22524	0.65%	0.074%

LSC Area Percent Report

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
Data File : BN014433.D
Acq On : 25 Apr 2021 10:05
Operator : CG/JU
Sample : M2127-21
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0AA2

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Title : SVOA CALIBRATION

35	19.257	2741	2749	2757	rBV	43964	69591	2.01%	0.229%
36	19.351	2760	2765	2769	rVB	13639	18984	0.55%	0.062%
37	19.463	2778	2784	2793	rBV	2615729	3460650	100.00%	11.378%
38	20.510	2958	2962	2963	rBV4	4038	4795	0.14%	0.016%
39	20.980	3038	3042	3051	rBV3	56745	101530	2.93%	0.334%
40	21.257	3084	3089	3098	rBV	1330362	1646368	47.57%	5.413%
41	22.316	3267	3269	3275	rVB5	26697	31862	0.92%	0.105%
42	22.821	3352	3355	3361	rVB3	41352	61998	1.79%	0.204%
43	23.345	3436	3444	3458	rBV	1859017	3426108	99.00%	11.265%
44	23.486	3461	3468	3480	rVB2	874591	1633995	47.22%	5.373%
45	24.027	3557	3560	3566	rVB	44293	75551	2.18%	0.248%


Sum of corrected areas: 30414009

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042421\
Data File : BN014433.D
Acq On : 25 Apr 2021 10:05
Operator : CG/JU
Sample : M2127-21
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0AA2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

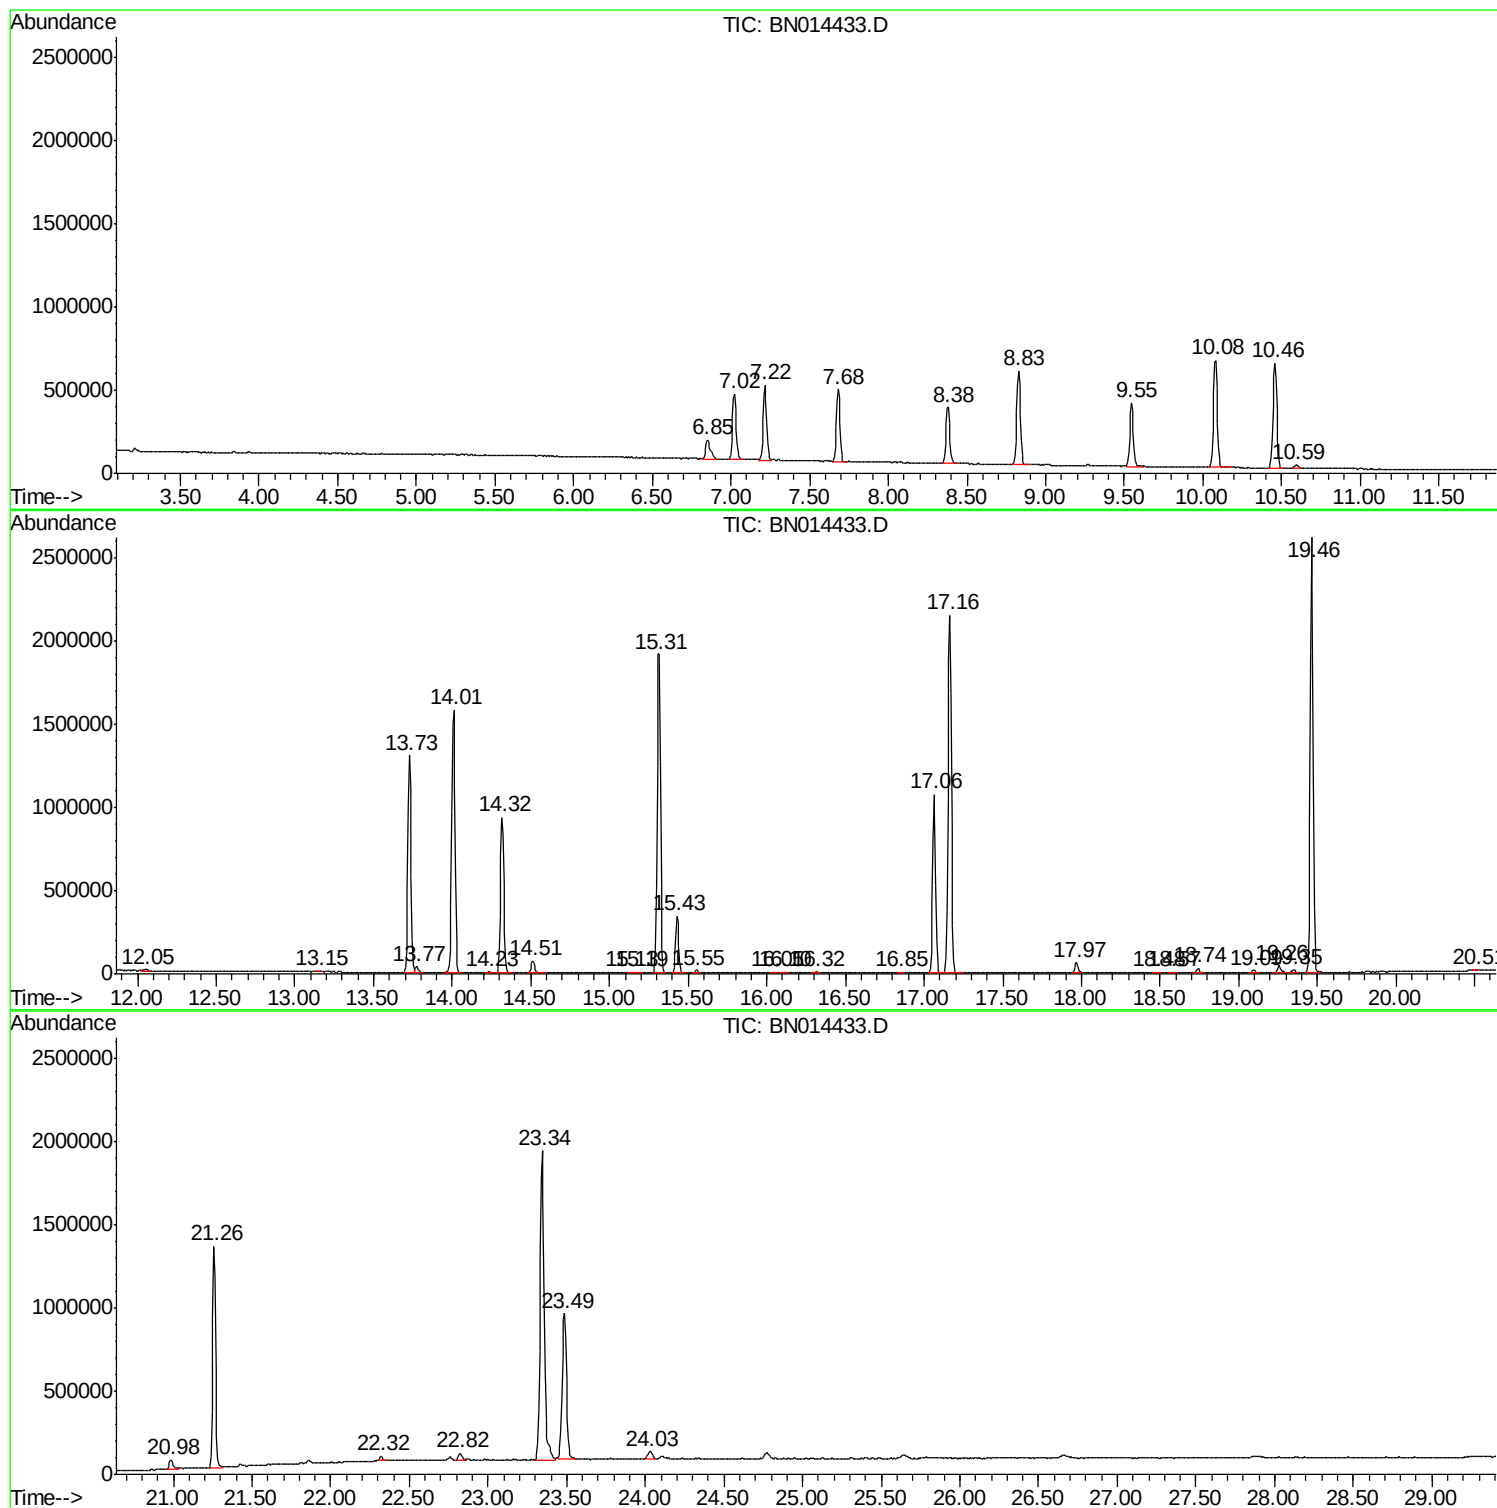

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
Data File : BN014433.D
Acq On : 25 Apr 2021 10:05
Operator : CG/JU
Sample : M2127-21
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0AA2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
Data File : BN014433.D
Acq On : 25 Apr 2021 10:05
Operator : CG/JU
Sample : M2127-21
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0AA2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc