

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042421\
 Data File : BN014434.D
 Acq On : 25 Apr 2021 10:40
 Operator : CG/JU
 Sample : M2127-22
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E0AA3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.852	635	640	649	rVB2	133377	258308	6.78%	0.779%
2	7.022	663	669	682	rVB	438804	712799	18.72%	2.151%
3	7.216	696	702	710	rBV	505738	782095	20.54%	2.360%
4	7.681	775	781	788	rVB	463011	711423	18.68%	2.147%
5	8.375	894	899	911	rVB	383028	623133	16.36%	1.880%
6	8.828	970	976	985	rVB	627880	1008545	26.48%	3.043%
7	9.546	1092	1098	1110	rVB	422811	663865	17.43%	2.003%
8	10.081	1182	1189	1198	rBV	708297	1160192	30.46%	3.501%
9	10.457	1246	1253	1260	rBV	675587	1096363	28.79%	3.308%
10	10.593	1272	1276	1282	rVB	34057	54838	1.44%	0.165%
11	12.051	1520	1524	1531	rVB3	12108	20386	0.54%	0.062%
12	13.151	1708	1711	1714	rBV3	6312	8119	0.21%	0.024%
13	13.728	1803	1809	1814	rBV	1442700	1901028	49.92%	5.736%
14	13.775	1814	1817	1822	rVB	46835	61690	1.62%	0.186%
15	14.010	1846	1857	1867	rVB	1739289	2547891	66.90%	7.688%
16	14.234	1890	1895	1898	rBV4	5866	7646	0.20%	0.023%
17	14.316	1903	1909	1917	rVV	976181	1399272	36.74%	4.222%
18	14.510	1937	1942	1949	rBV	81749	118046	3.10%	0.356%
19	15.134	2043	2048	2053	rBV3	5083	8362	0.22%	0.025%
20	15.187	2053	2057	2061	rVB2	5103	5849	0.15%	0.018%
21	15.310	2072	2078	2089	rVB	2155105	3050332	80.09%	9.204%
22	15.428	2093	2098	2108	rBV	378990	510544	13.41%	1.541%
23	15.551	2115	2119	2123	rBV	15992	19218	0.50%	0.058%
24	16.045	2200	2203	2209	rVV4	3943	8338	0.22%	0.025%
25	16.104	2209	2213	2218	rVB5	7145	11503	0.30%	0.035%
26	16.222	2228	2233	2238	rVB5	3084	4830	0.13%	0.015%
27	16.310	2244	2248	2254	rVB2	8657	12728	0.33%	0.038%
28	16.392	2254	2262	2265	rBV6	1865	4231	0.11%	0.013%
29	16.816	2330	2334	2336	rBV	5482	6920	0.18%	0.021%
30	16.845	2336	2339	2345	rVB3	5403	7622	0.20%	0.023%
31	17.063	2370	2376	2383	rBV	1121990	1538883	40.41%	4.644%
32	17.163	2386	2393	2405	rBV	2471774	3353169	88.04%	10.118%
33	17.963	2525	2529	2536	rBV	45574	63048	1.66%	0.190%
34	18.475	2611	2616	2623	rBV3	5671	10049	0.26%	0.030%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
 Data File : BN014434.D
 Acq On : 25 Apr 2021 10:40
 Operator : CG/JU
 Sample : M2127-22
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E0AA3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Title : SVOA CALIBRATION

35	18.575	2629	2633	2636	rBV4	2496	4059	0.11%	0.012%
36	18.739	2655	2661	2667	rBV	38696	50615	1.33%	0.153%
37	19.098	2715	2722	2726	rBV	19554	27210	0.71%	0.082%
38	19.251	2744	2748	2756	rBV2	31296	45629	1.20%	0.138%
39	19.345	2761	2764	2769	rVV	12403	17527	0.46%	0.053%
40	19.463	2778	2784	2793	rVV	2895906	3804586	99.90%	11.480%
41	20.027	2877	2880	2884	rVB6	3117	4313	0.11%	0.013%
42	20.527	2962	2965	2968	rVB5	3973	3819	0.10%	0.012%
43	20.980	3037	3042	3051	rBV4	40616	79876	2.10%	0.241%
44	21.257	3084	3089	3100	rBV	1334529	1679546	44.10%	5.068%
45	21.427	3115	3118	3123	rBV3	10103	15214	0.40%	0.046%
46	22.316	3267	3269	3274	rVB	25496	31254	0.82%	0.094%
47	22.821	3352	3355	3360	rVB2	38278	49026	1.29%	0.148%
48	23.345	3437	3444	3457	rBV	2024178	3808473	100.00%	11.492%
49	23.486	3461	3468	3478	rVB2	922549	1676336	44.02%	5.058%
50	24.027	3557	3560	3568	rVB2	52987	91294	2.40%	0.275%


Sum of corrected areas: 33140042

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042421\
Data File : BN014434.D
Acq On : 25 Apr 2021 10:40
Operator : CG/JU
Sample : M2127-22
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0AA3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

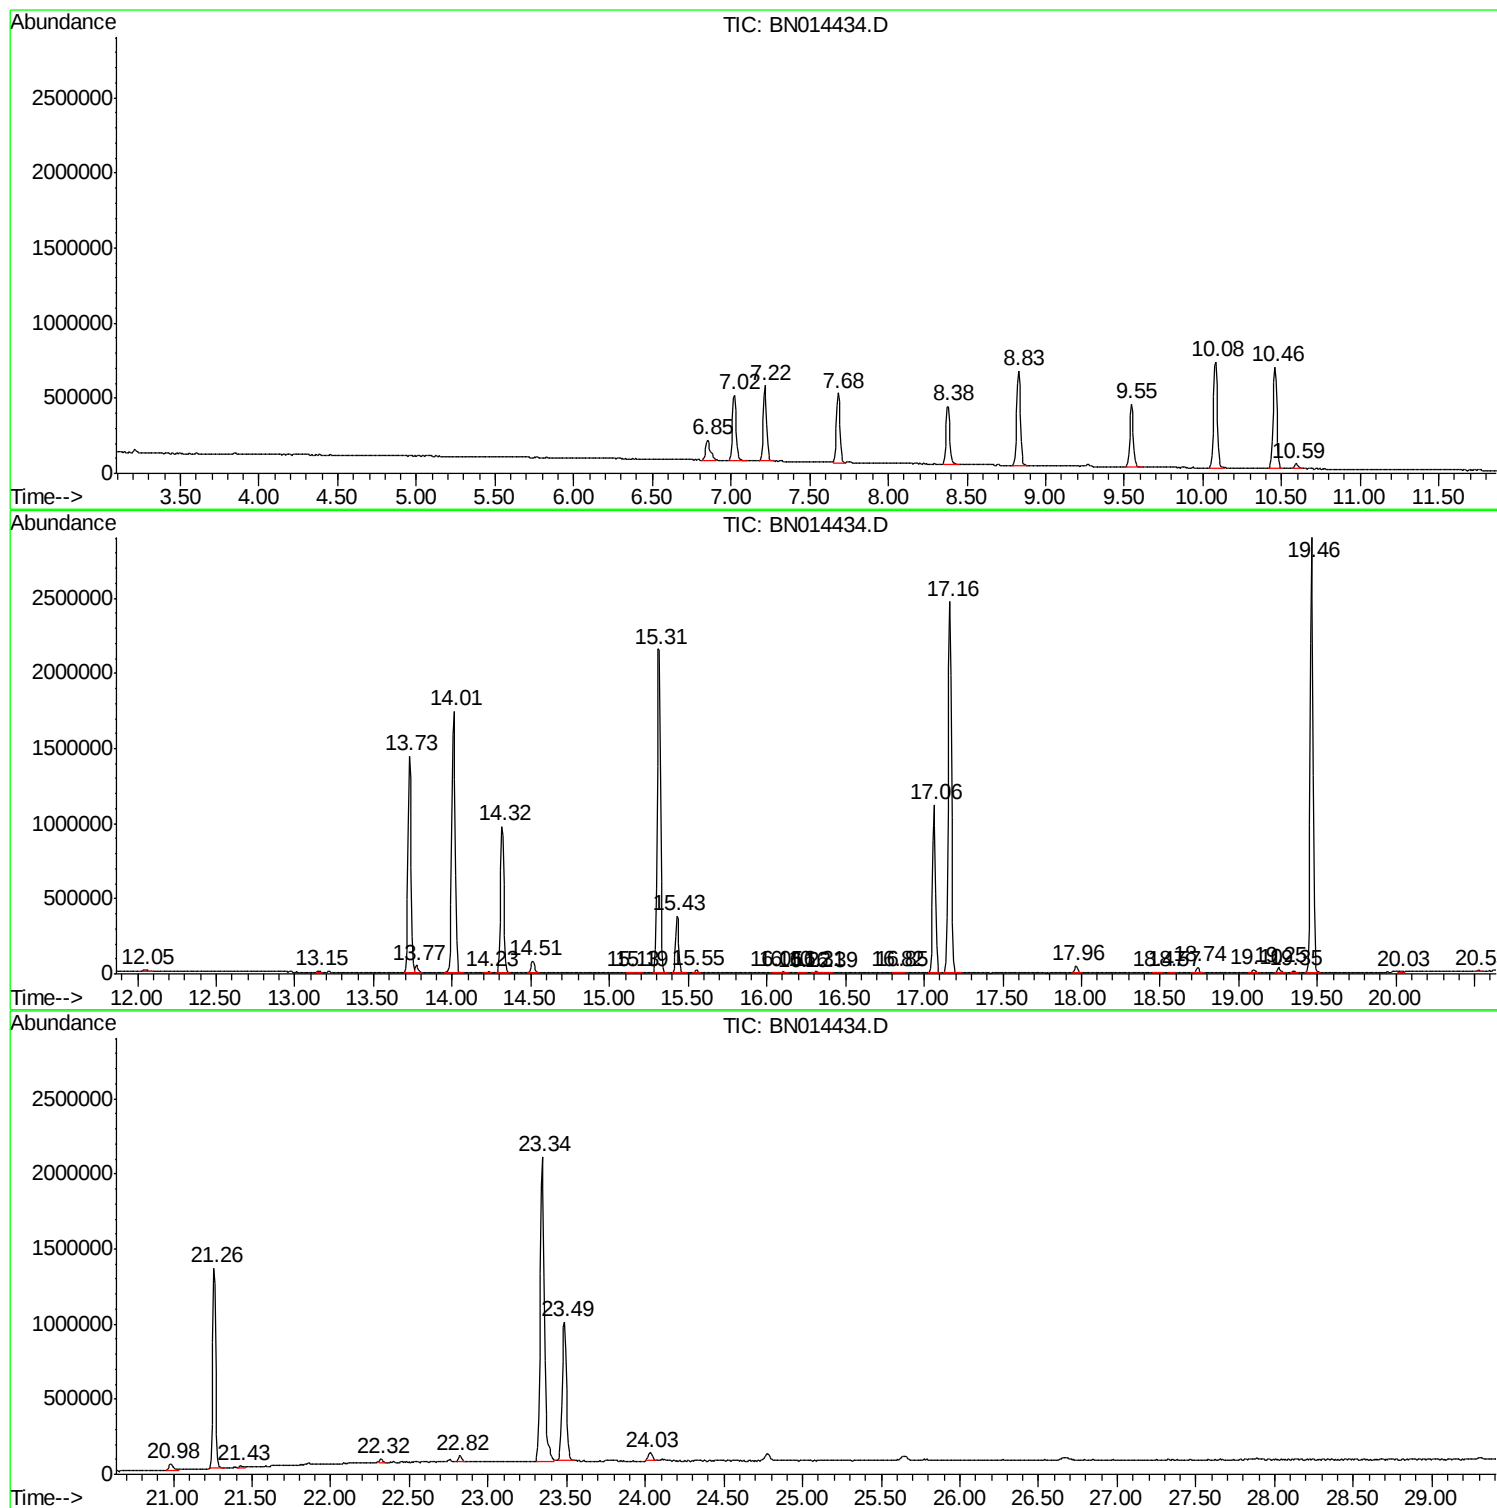

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
Data File : BN014434.D
Acq On : 25 Apr 2021 10:40
Operator : CG/JU
Sample : M2127-22
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0AA3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
Data File : BN014434.D
Acq On : 25 Apr 2021 10:40
Operator : CG/JU
Sample : M2127-22
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0AA3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc