

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042421\
 Data File : BN014435.D
 Acq On : 25 Apr 2021 11:15
 Operator : CG/JU
 Sample : M2127-23
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E0AA4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.851	635	640	641	rBV	132961	168371	4.58%	0.542%
2	6.875	642	644	652	rVB	194094	267745	7.28%	0.862%
3	7.022	663	669	682	rVB	434515	697851	18.98%	2.246%
4	7.216	696	702	710	rBV	487427	746555	20.31%	2.403%
5	7.681	776	781	788	rVB	409836	635797	17.29%	2.046%
6	8.381	894	900	908	rVB	377829	592535	16.12%	1.907%
7	8.828	970	976	987	rVB	598443	963257	26.20%	3.101%
8	9.545	1092	1098	1109	rVB	384438	616533	16.77%	1.984%
9	10.081	1182	1189	1202	rVB	686074	1111834	30.24%	3.579%
10	10.457	1246	1253	1260	rBV	584300	966976	26.30%	3.112%
11	10.592	1272	1276	1282	rVB	25575	41717	1.13%	0.134%
12	12.051	1520	1524	1529	rVB2	10474	16808	0.46%	0.054%
13	13.151	1708	1711	1715	rVB2	5538	6422	0.17%	0.021%
14	13.727	1803	1809	1814	rBV	1318998	1744622	47.45%	5.616%
15	13.774	1814	1817	1824	rVB	105656	134241	3.65%	0.432%
16	14.010	1846	1857	1866	rVB	1661546	2432460	66.16%	7.830%
17	14.233	1891	1895	1898	rBV4	3706	4002	0.11%	0.013%
18	14.316	1903	1909	1918	rVB2	849753	1228374	33.41%	3.954%
19	14.510	1936	1942	1948	rBV	77586	108873	2.96%	0.350%
20	15.127	2044	2047	2053	rBV3	4166	7265	0.20%	0.023%
21	15.186	2053	2057	2060	rVB4	4029	4749	0.13%	0.015%
22	15.310	2072	2078	2085	rBV	1959165	2823562	76.80%	9.088%
23	15.427	2093	2098	2105	rBV	344786	453984	12.35%	1.461%
24	15.551	2114	2119	2123	rBV	15121	19831	0.54%	0.064%
25	16.051	2200	2204	2206	rBV3	3139	3708	0.10%	0.012%
26	16.098	2210	2212	2218	rVB3	5640	7705	0.21%	0.025%
27	16.316	2245	2249	2253	rVB2	6388	8855	0.24%	0.029%
28	16.810	2329	2333	2336	rBV4	3639	5607	0.15%	0.018%
29	16.845	2336	2339	2345	rVV2	4767	8555	0.23%	0.028%
30	17.063	2370	2376	2382	rBV	1027863	1382503	37.60%	4.450%
31	17.163	2386	2393	2404	rVV	2405912	3156334	85.85%	10.160%
32	17.968	2525	2530	2539	rBV	47681	67372	1.83%	0.217%
33	18.033	2539	2541	2545	rVB3	3071	4435	0.12%	0.014%
34	18.474	2612	2616	2621	rBV2	4298	6275	0.17%	0.020%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
 Data File : BN014435.D
 Acq On : 25 Apr 2021 11:15
 Operator : CG/JU
 Sample : M2127-23
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E0AA4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Title : SVOA CALIBRATION

35	18.739	2656	2661	2666	rBV	24727	29526	0.80%	0.095%
36	18.904	2685	2689	2693	rBV4	2662	4668	0.13%	0.015%
37	19.098	2717	2722	2725	rBV	16303	21475	0.58%	0.069%
38	19.257	2742	2749	2756	rBV	34576	48408	1.32%	0.156%
39	19.351	2761	2765	2771	rVB	13947	19330	0.53%	0.062%
40	19.462	2778	2784	2795	rBV	2742156	3676676	100.00%	11.834%
41	20.504	2958	2961	2970	rBV8	6214	13065	0.36%	0.042%
42	20.980	3039	3042	3051	rBV5	24086	41502	1.13%	0.134%
43	21.256	3084	3089	3102	rBV	1235264	1571010	42.73%	5.057%
44	22.821	3352	3355	3359	rVB	25740	35418	0.96%	0.114%
45	23.345	3437	3444	3458	rBV	2088810	3622144	98.52%	11.659%
46	23.486	3461	3468	3477	rVB2	836096	1538704	41.85%	4.953%


Sum of corrected areas: 31067639

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042421\
Data File : BN014435.D
Acq On : 25 Apr 2021 11:15
Operator : CG/JU
Sample : M2127-23
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0AA4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

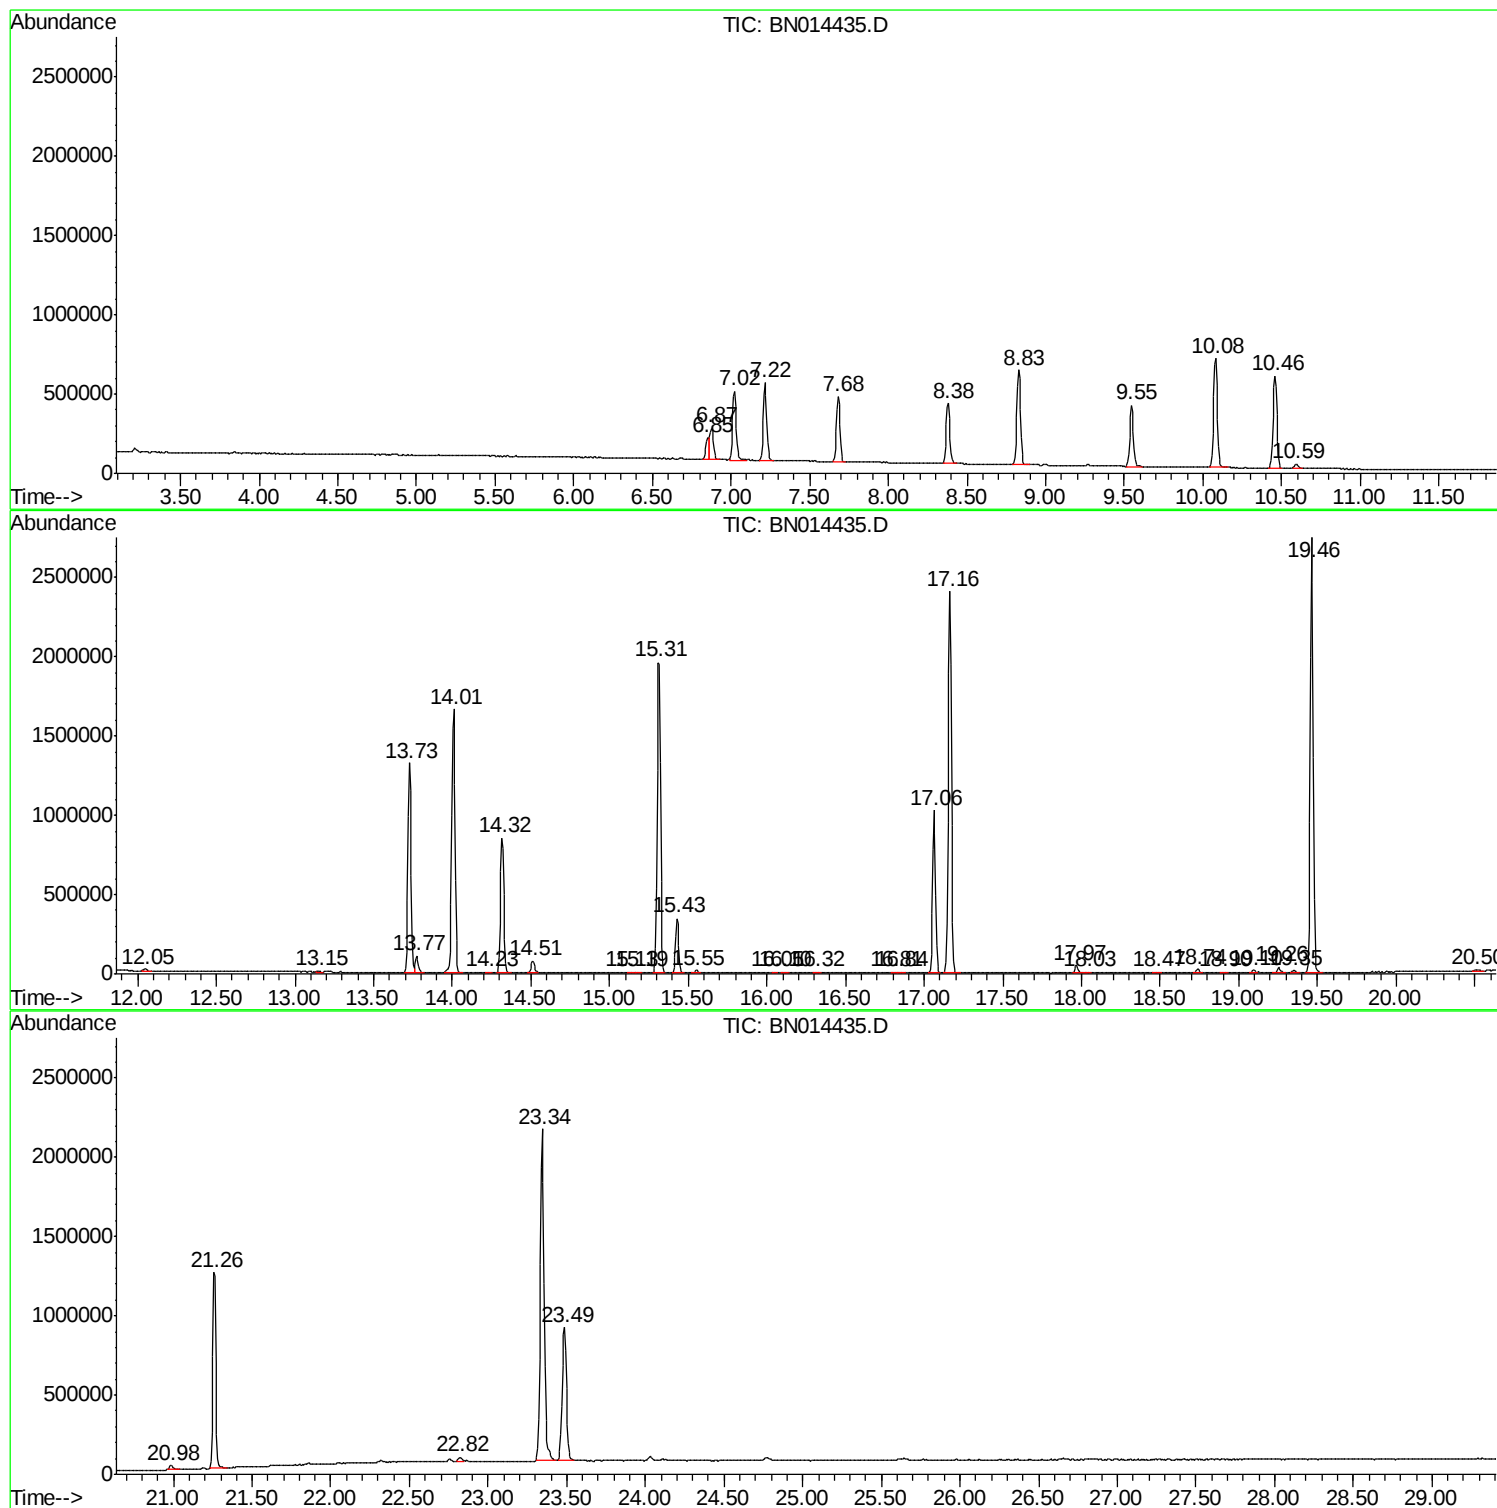

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
Data File : BN014435.D
Acq On : 25 Apr 2021 11:15
Operator : CG/JU
Sample : M2127-23
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0AA4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
Data File : BN014435.D
Acq On : 25 Apr 2021 11:15
Operator : CG/JU
Sample : M2127-23
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0AA4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc