

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
 Data File : BN014436.D
 Acq On : 25 Apr 2021 11:51
 Operator : CG/JU
 Sample : PB135972BL
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK972

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.605	86	88	106	rBV	315386	527448	14.56%	1.549%
2	6.852	634	640	652	rVB	566662	867580	23.96%	2.548%
3	7.022	663	669	682	rVB	461779	737280	20.36%	2.165%
4	7.216	696	702	711	rVB	623990	964469	26.63%	2.833%
5	7.681	775	781	787	rVB	370649	564962	15.60%	1.659%
6	8.381	894	900	913	rVB	743857	1174205	32.42%	3.449%
7	8.828	970	976	985	rVB	637648	1024063	28.28%	3.008%
8	9.546	1092	1098	1113	rVB	412337	660888	18.25%	1.941%
9	10.081	1182	1189	1204	rVB	761774	1246106	34.41%	3.660%
10	10.457	1246	1253	1262	rVB	529032	876805	24.21%	2.575%
11	10.593	1269	1276	1291	rVB	801280	1305768	36.05%	3.835%
12	12.051	1520	1524	1529	rVB	11538	18639	0.51%	0.055%
13	13.728	1803	1809	1820	rVB	1461393	1914084	52.85%	5.622%
14	14.010	1850	1857	1864	rBV	1755201	2571675	71.01%	7.553%
15	14.316	1903	1909	1917	rBV	775676	1107126	30.57%	3.252%
16	14.510	1936	1942	1960	rBV	502818	714509	19.73%	2.098%
17	15.316	2072	2079	2087	rBV	2139445	3011736	83.16%	8.845%
18	15.428	2093	2098	2107	rBV	351399	464471	12.82%	1.364%
19	15.551	2114	2119	2125	rBB	16820	21406	0.59%	0.063%
20	16.098	2205	2212	2217	rVB5	4392	6655	0.18%	0.020%
21	17.063	2370	2376	2384	rVB	939763	1230638	33.98%	3.614%
22	17.163	2386	2393	2403	rBV	2402475	3218274	88.86%	9.452%
23	19.098	2717	2722	2727	rVB2	13302	18889	0.52%	0.055%
24	19.345	2760	2764	2770	rBV	10350	15700	0.43%	0.046%
25	19.463	2778	2784	2792	rBV	2777189	3621608	100.00%	10.636%
26	21.257	3084	3089	3097	rBV	1050466	1303903	36.00%	3.829%
27	23.345	3437	3444	3460	rBV	1966791	3528530	97.43%	10.363%
28	23.480	3461	3467	3481	rVB2	717265	1331555	36.77%	3.911%


Sum of corrected areas: 34048972

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042421\
Data File : BN014436.D
Acq On : 25 Apr 2021 11:51
Operator : CG/JU
Sample : PB135972BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK972

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

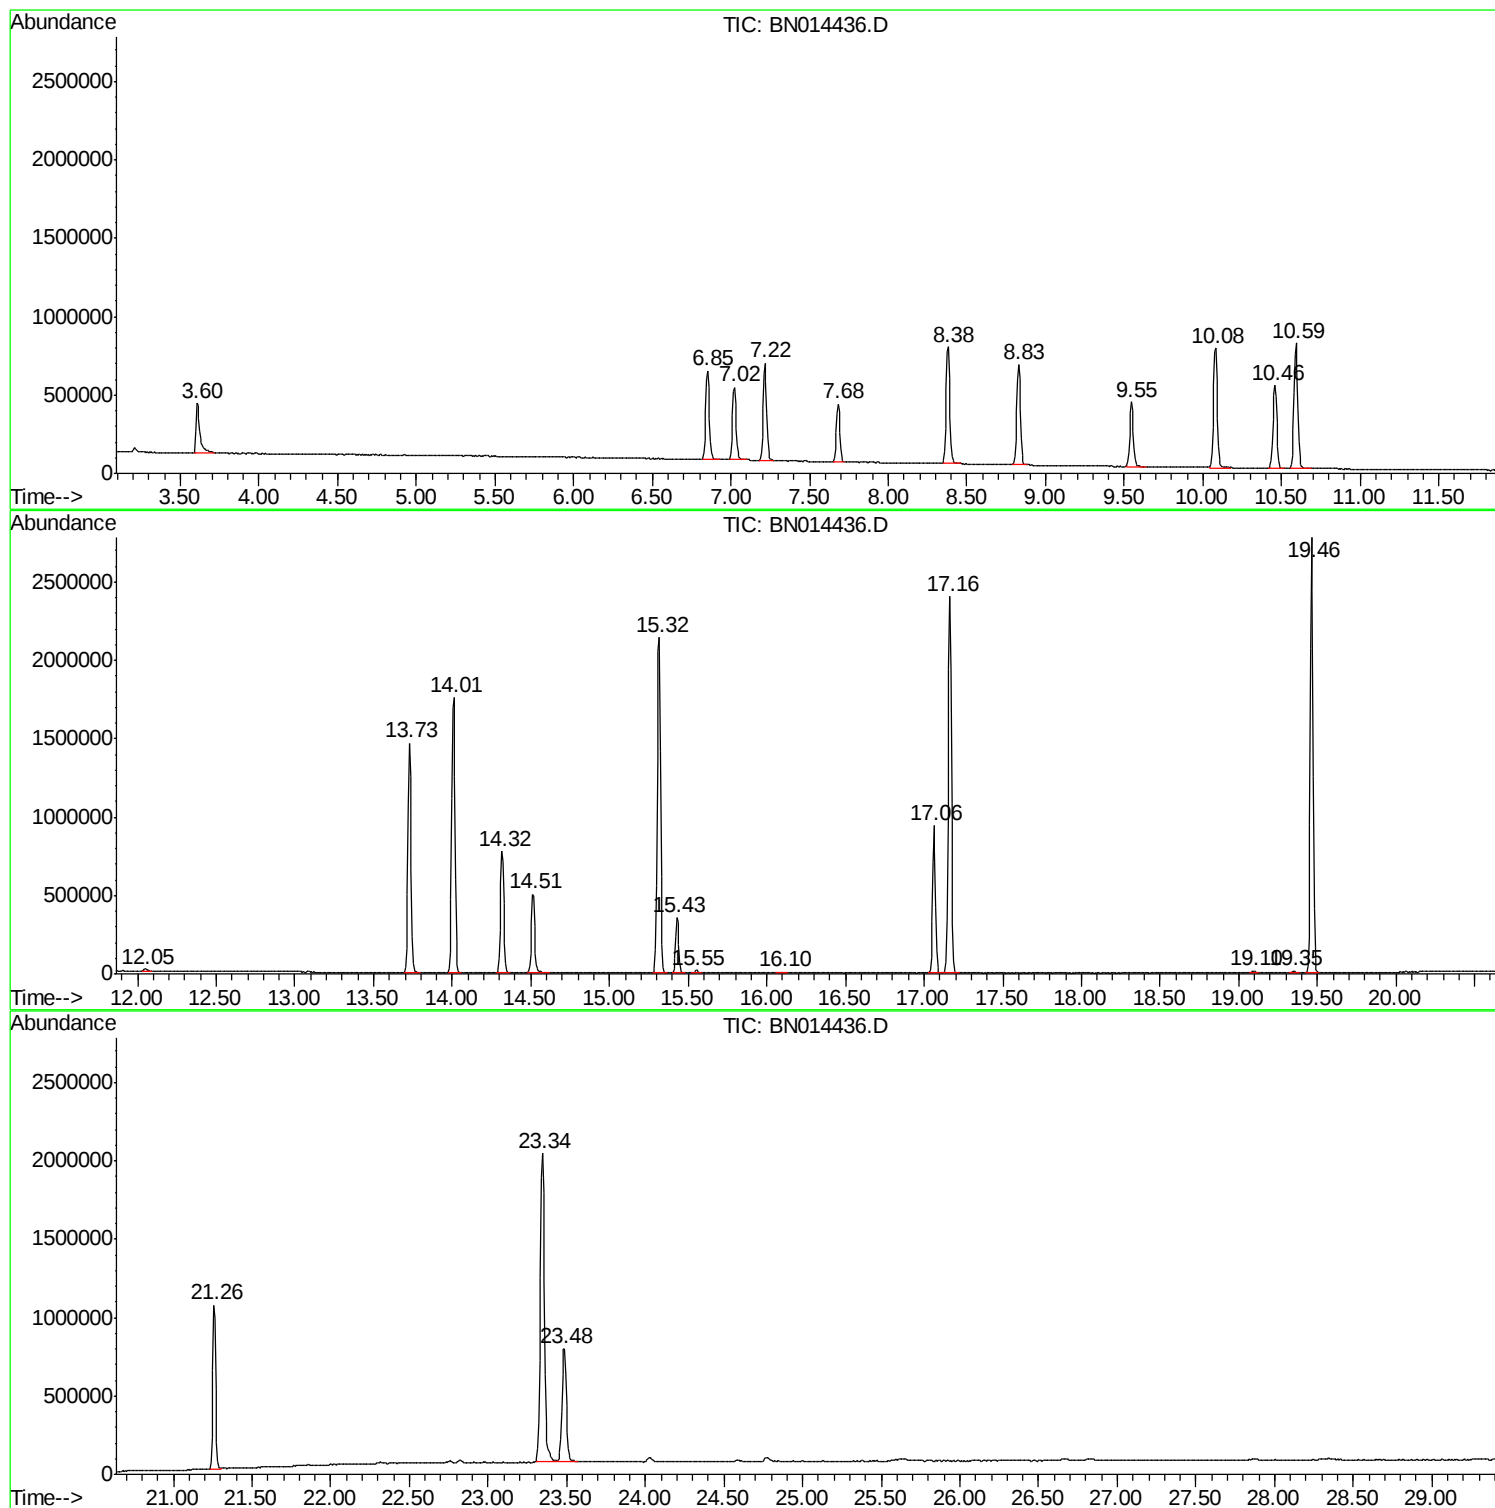

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
Data File : BN014436.D
Acq On : 25 Apr 2021 11:51
Operator : CG/JU
Sample : PB135972BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK972

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
Data File : BN014436.D
Acq On : 25 Apr 2021 11:51
Operator : CG/JU
Sample : PB135972BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK972

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc