

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042523\
 Data File : BN025135.D
 Acq On : 25 Apr 2023 18:22
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTD020283

Quant Time: Apr 26 00:47:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 25 08:52:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.910	152	313254	20.000	ng/u1	0.00
20) Naphthalene-d8	10.728	136	1409438	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.563	164	907575	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.310	188	1993342	20.000	ng/u1	0.00
79) Chrysene-d12	21.510	240	1792535	20.000	ng/u1	0.00
88) Perylene-d12	23.945	264	1889102	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.287	96	64381	7.822	ng/uL	0.00
4) Pyridine-d5	3.716	84	479231	19.445	ng/u1	0.00
7) Phenol-d5	7.075	99	618511	20.252	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.240	67	437970	21.441	ng/u1	0.00
11) 2-Chlorophenol-d4	7.440	132	472934	21.072	ng/u1	0.00
15) 4-Methylphenol-d8	8.628	113	502627	20.731	ng/u1	0.00
21) Nitrobenzene-d5	9.081	128	238927	20.936	ng/u1	0.00
24) 2-Nitrophenol-d4	9.804	143	265370	21.468	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.346	165	483341	21.877	ng/u1	0.00
31) 4-Chloroaniline-d4	10.863	131	726591	21.670	ng/u1	0.00
46) Dimethylphthalate-d6	13.969	166	1552912	22.072	ng/u1	0.00
49) Acenaphthylene-d8	14.257	160	1741481	21.600	ng/u1	0.00
54) 4-Nitrophenol-d4	14.763	143	292389	20.273	ng/u1	0.00
60) Fluorene-d10	15.551	176	1311133	22.072	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.675	200	257601	19.857	ng/u1	0.00
73) Anthracene-d10	17.410	188	2055161	21.952	ng/u1	0.00
81) Pyrene-d10	19.704	212	2349259	22.570	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.792	264	2136687	21.632	ng/u1	0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.328	88	70791	7.970	ng/uL	96
5) Pyridine	3.734	79	515313	20.238	ng/u1	97
6) Benzaldehyde	7.052	77	374076	25.069	ng/u1	97
8) Phenol	7.099	94	657476	20.671	ng/u1	98
10) Bis(2-Chloroethyl)ether	7.334	93	534057	21.388	ng/u1	99
12) 2-Chlorophenol	7.475	128	492196	20.997	ng/u1	99
13) 2-Methylphenol	8.357	108	482729	20.672	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.446	45	1067322	21.768	ng/u1	99
16) Acetophenone	8.746	105	831690	21.694	ng/u1	98
17) N-Nitroso-di-n-propyla...	8.728	70	455622	22.034	ng/u1	99
18) 4-Methylphenol	8.693	108	542069	20.875	ng/u1	98
19) Hexachloroethane	8.999	117	199772	21.116	ng/u1	96
22) Nitrobenzene	9.128	77	665832	21.713	ng/u1	99
23) Isophorone	9.651	82	1226001	21.780	ng/u1	99
25) 2-Nitrophenol	9.840	139	292175	21.912	ng/u1	96
26) 2,4-Dimethylphenol	9.899	107	608651	21.680	ng/u1	99
27) Bis(2-Chloroethoxy)met...	10.134	93	758615	21.656	ng/u1	99
29) 2,4-Dichlorophenol	10.369	162	485793	21.908	ng/u1	99
30) Naphthalene	10.775	128	1706891	21.684	ng/u1	99
32) 4-Chloroaniline	10.893	127	740026	21.803	ng/u1	98
33) Hexachlorobutadiene	11.057	225	296904	22.972	ng/u1	93
34) Caprolactam	11.657	113	103624	13.333	ng/u1	97
35) 4-Chloro-3-methylphenol	12.010	107	569625	21.909	ng/u1	99
36) 2-Methylnaphthalene	12.387	142	1152003	22.144	ng/u1	98


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042523\
 Data File : BN025135.D
 Acq On : 25 Apr 2023 18:22
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTD020283

Quant Time: Apr 26 00:47:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 25 08:52:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.604	142	1149138	22.128	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.757	216	590078	22.290	ng/ul	99
40) Hexachlorocyclopentadiene	12.734	237	264701	16.397	ng/ul	93
41) 2,4,6-Trichlorophenol	12.992	196	399548	22.089	ng/ul	94
42) 2,4,5-Trichlorophenol	13.063	196	440336	22.246	ng/ul	96
43) 1,1'-Biphenyl	13.398	154	1575957	21.794	ng/ul	99
44) 2-Chloronaphthalene	13.440	162	1225761	21.831	ng/ul	98
45) 2-Nitroaniline	13.645	65	424600	21.656	ng/ul	98
47) Dimethylphthalate	14.022	163	1555764	21.977	ng/ul	100
48) 2,6-Dinitrotoluene	14.145	165	307814	22.277	ng/ul	97
50) Acenaphthylene	14.287	152	1918457	21.664	ng/ul	98
51) 3-Nitroaniline	14.475	138	323624	22.287	ng/ul	97
52) Acenaphthene	14.628	153	1344061	21.954	ng/ul	99
53) 2,4-Dinitrophenol	14.675	184	151102	17.008	ng/ul	90
55) 4-Nitrophenol	14.775	109	252885	21.544	ng/ul	95
56) Dibenzofuran	14.957	168	1858766	22.027	ng/ul	97
57) 2,4-Dinitrotoluene	14.928	165	451757	22.586	ng/ul	98
58) 2,3,4,6-Tetrachlorophenol	15.186	232	370274	22.717	ng/ul	99
59) Diethylphthalate	15.381	149	1584938	22.281	ng/ul	100
61) Fluorene	15.610	166	1522546	22.432	ng/ul	98
62) 4-Chlorophenyl-phenyle...	15.604	204	738260	23.368	ng/ul	96
63) 4-Nitroaniline	15.634	138	342298	23.921	ng/ul	96
66) 4,6-Dinitro-2-methylph...	15.692	198	255062	20.072	ng/ul	100
67) N-Nitrosodiphenylamine	15.816	169	1307595	21.622	ng/ul	98
68) 4-Bromophenyl-phenylether	16.498	248	443260	22.123	ng/ul	97
69) Hexachlorobenzene	16.616	284	496629	21.892	ng/ul	97
70) Atrazine	16.769	200	450576	21.896	ng/ul	99
71) Pentachlorophenol	16.957	266	296730	21.044	ng/ul	97
72) Phenanthrene	17.351	178	2414532	21.465	ng/ul	99
74) Anthracene	17.445	178	2456071	21.668	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.363	216	606071	21.377	ng/ul	99
76) Pentachlorobenzene	14.881	250	595251	21.944	ng/ul	98
77) Carbazole	17.716	167	2219521	21.686	ng/ul	98
78) Di-n-butylphthalate	18.275	149	2668211	21.964	ng/ul	99
80) Fluoranthene	19.369	202	2815126	22.566	ng/ul	99
82) Pyrene	19.733	202	2912517	22.180	ng/ul	98
83) Butylbenzylphthalate	20.633	149	1196677	21.951	ng/ul	100
84) 3,3'-Dichlorobenzidine	21.427	252	942726	22.922	ng/ul#	96
85) Benzo(a)anthracene	21.492	228	2872439	22.312	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.410	149	1769016	21.737	ng/ul	99
87) Chrysene	21.545	228	2678072	21.839	ng/ul	98
89) Di-n-octyl phthalate	22.351	149	3035430	23.381	ng/ul	100
90) Benzo(b)fluoranthene	23.198	252	2765118	22.319	ng/ul	98
91) Benzo(k)fluoranthene	23.251	252	2768444	22.710	ng/ul	98
93) Benzo(a)pyrene	23.839	252	2356859	21.729	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	26.480	276	1313800	9.997	ng/ul	97
95) Dibenzo(a,h)anthracene	26.515	278	2386516	21.996	ng/ul	97
96) Benzo(g,h,i)perylene	27.268	276	2239573	21.001	ng/ul	97





(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2
 1,4-Dioxane
 Concen: 7.970 ng/uL
 RT: 3.328 min Scan# 24
 Delta R.T. -0.000 min
 Lab File: BN025135.D
 Acq: 25 Apr 2023 18:22




Instrument :
 BNA_N
 ClientSampleId :
 SST020283


Tgt Ion: 88 Resp: 70791
 Ion Ratio Lower Upper
 88 100
 43 43.1 33.0 49.4
 58 85.6 72.3 108.5

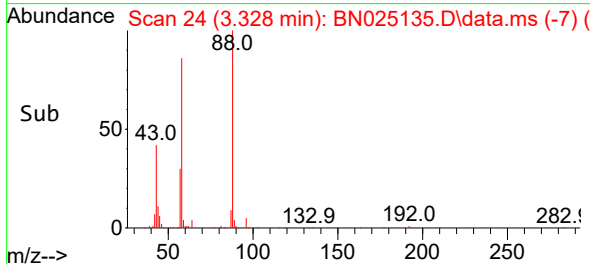

#5
 Pyridine
 Concen: 20.238 ng/uL
 RT: 3.734 min Scan# 93
 Delta R.T. -0.006 min
 Lab File: BN025135.D
 Acq: 25 Apr 2023 18:22

Tgt Ion: 79 Resp: 515313
 Ion Ratio Lower Upper
 79 100
 52 98.0 76.1 114.1
 51 47.2 35.8 53.6


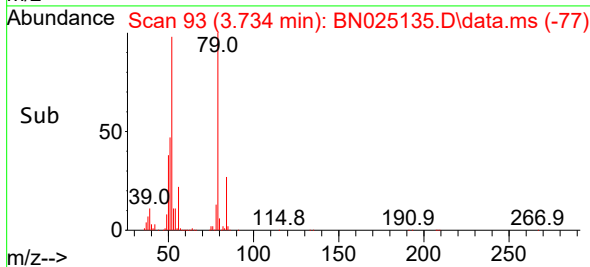

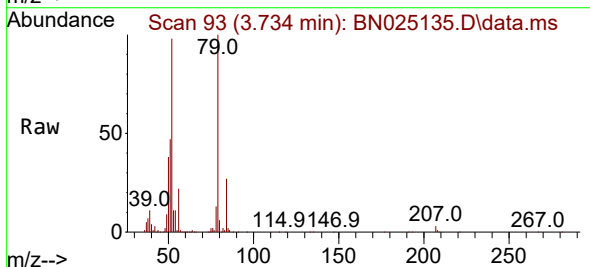




#6
Benzaldehyde
Concen: 25.069 ng/ul
RT: 7.052 min Scan# 657
Delta R.T. -0.000 min
Lab File: BN025135.D
Acq: 25 Apr 2023 18:22




Instrument :
BNA_N
ClientSampleId :
SSTD020283


Tgt Ion: 77 Resp: 374076
Ion Ratio Lower Upper
77 100
105 91.3 74.3 111.5
106 87.0 73.3 109.9

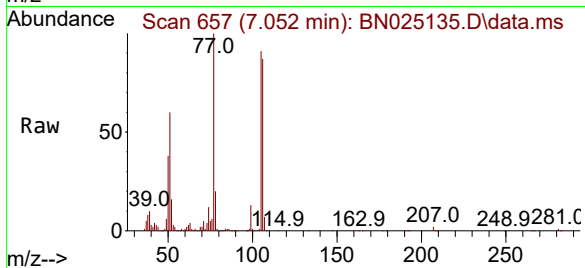

#8
Phenol
Concen: 20.671 ng/ul
RT: 7.099 min Scan# 665
Delta R.T. -0.006 min
Lab File: BN025135.D
Acq: 25 Apr 2023 18:22

Tgt Ion: 94 Resp: 657476
Ion Ratio Lower Upper
94 100
65 32.5 25.1 37.7
66 41.3 31.9 47.9

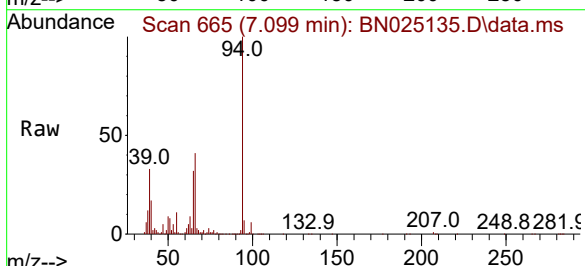







#10
 Bis(2-Chloroethyl)ether
 Concen: 21.388 ng/ul
 RT: 7.334 min Scan# 705
 Delta R.T. -0.006 min
 Lab File: BN025135.D
 Acq: 25 Apr 2023 18:22

Instrument :
 BNA_N
 ClientSampleId :
 SSTD020283

Tgt Ion: 93 Resp: 534057




Ion	Ratio	Lower	Upper
93	100		
63	88.2	70.9	106.3
95	31.3	26.0	39.0

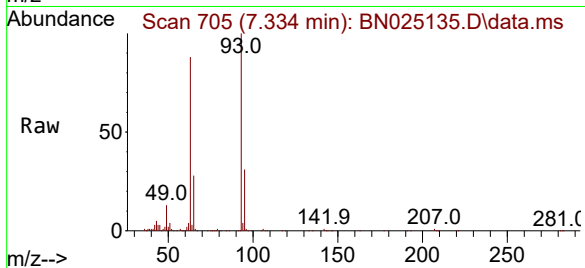


#12
 2-Chlorophenol
 Concen: 20.997 ng/ul
 RT: 7.475 min Scan# 729
 Delta R.T. -0.000 min
 Lab File: BN025135.D
 Acq: 25 Apr 2023 18:22

Tgt Ion:128 Resp: 492196

Ion	Ratio	Lower	Upper
128	100		
64	55.3	44.8	67.2
130	32.4	26.6	39.8

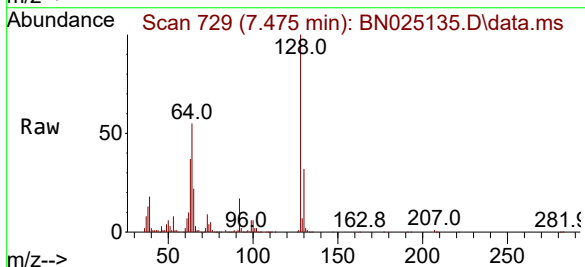



#13

2-Methylphenol

Concen: 20.672 ng/ul

RT: 8.357 min Scan# 81

Delta R.T. -0.006 min

Lab File: BN025135.D

Acq: 25 Apr 2023 18:22

Instrument :

BNA_N

ClientSampleId :





SSTD020283

Tgt Ion:108 Resp: 482729

Ion Ratio Lower Upper

108 100

107 88.3 71.5 107.3

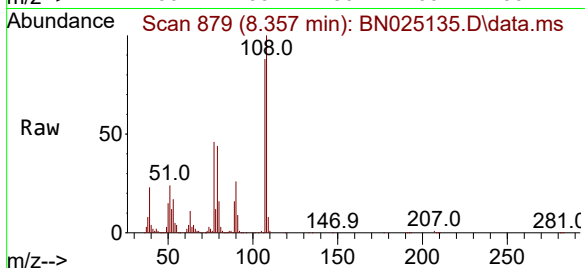

#14

2,2'-oxybis(1-Chloropropane)

Concen: 21.768 ng/ul

RT: 8.446 min Scan# 894

Delta R.T. -0.006 min

Lab File: BN025135.D

Acq: 25 Apr 2023 18:22




Tgt Ion: 45 Resp: 1067322


Ion Ratio Lower Upper

45 100

77 10.2 8.4 12.6

79 7.9 6.6 9.8




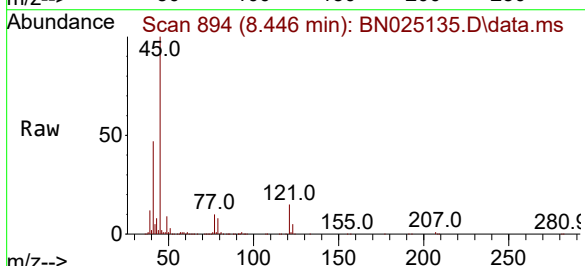




#16
Acetophenone
Concen: 21.694 ng/ul
RT: 8.746 min Scan# 944
Delta R.T. -0.000 min
Lab File: BN025135.D
Acq: 25 Apr 2023 18:22




Instrument :
BNA_N
ClientSampleId :
SSTD020283


Tgt Ion:105 Resp: 831690
Ion Ratio Lower Upper
105 100
77 82.0 64.8 97.2
51 37.9 28.7 43.1



#17
N-Nitroso-di-n-propylamine
Concen: 22.034 ng/ul
RT: 8.728 min Scan# 942
Delta R.T. -0.006 min
Lab File: BN025135.D
Acq: 25 Apr 2023 18:22

Tgt Ion: 70 Resp: 455622
Ion Ratio Lower Upper
70 100
42 81.8 64.2 96.2
101 8.8 7.3 10.9
130 18.8 15.0 22.6









#18
4-Methylphenol
Concen: 20.875 ng/ul
RT: 8.693 min Scan# 91
Delta R.T. -0.000 min
Lab File: BN025135.D
Acq: 25 Apr 2023 18:22




Instrument :
BNA_N
ClientSampleId :
SSTD020283


Tgt Ion:108 Resp: 542069
Ion Ratio Lower Upper
108 100
107 109.4 85.8 128.6

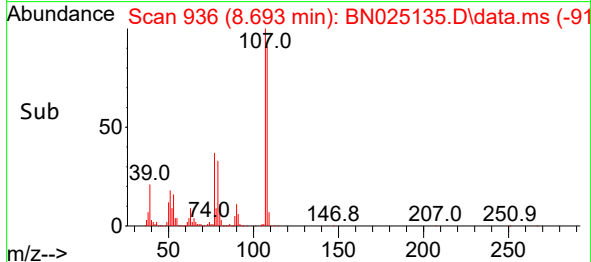

#19
Hexachloroethane
Concen: 21.116 ng/ul
RT: 8.999 min Scan# 988
Delta R.T. -0.000 min
Lab File: BN025135.D
Acq: 25 Apr 2023 18:22

Tgt Ion:117 Resp: 199772
Ion Ratio Lower Upper
117 100
201 94.7 72.2 108.4
199 56.1 46.2 69.4


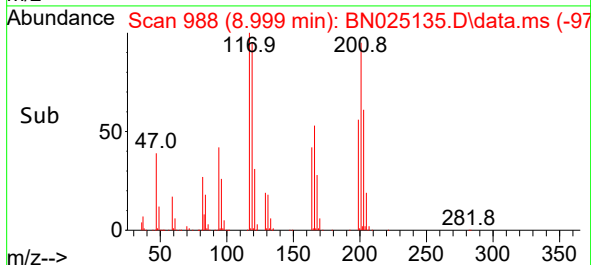
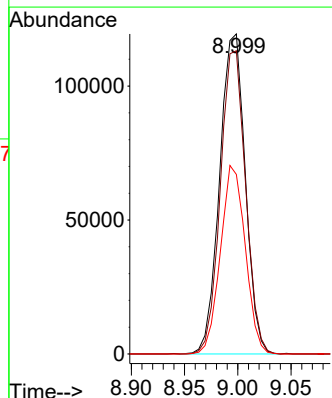





#22
Nitrobenzene
Concen: 21.713 ng/ul
RT: 9.128 min Scan# 1009
Delta R.T. -0.000 min
Lab File: BN025135.D
Acq: 25 Apr 2023 18:22




Instrument :
BNA_N
ClientSampleId :
SSTD020283


Tgt Ion: 77 Resp: 665832
Ion Ratio Lower Upper
77 100
123 40.8 33.5 50.3
65 14.9 11.8 17.8



#23
Isophorone
Concen: 21.780 ng/ul
RT: 9.651 min Scan# 1099
Delta R.T. -0.000 min
Lab File: BN025135.D
Acq: 25 Apr 2023 18:22

Tgt Ion: 82 Resp: 1226001
Ion Ratio Lower Upper
82 100
95 7.1 5.4 8.0
138 16.4 12.8 19.2









#25
2-Nitrophenol
Concen: 21.912 ng/ul
RT: 9.840 min Scan# 1130
Delta R.T. -0.000 min
Lab File: BN025135.D
Acq: 25 Apr 2023 18:22




Instrument :
BNA_N
ClientSampleId :
SSTD020283


Tgt Ion:139 Resp: 292175
Ion Ratio Lower Upper
139 100
65 59.4 49.8 74.8
109 30.1 26.2 39.2

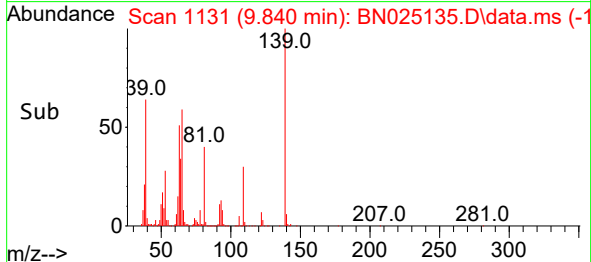

#26
2,4-Dimethylphenol
Concen: 21.680 ng/ul
RT: 9.899 min Scan# 1141
Delta R.T. -0.000 min
Lab File: BN025135.D
Acq: 25 Apr 2023 18:22

Tgt Ion:107 Resp: 608651
Ion Ratio Lower Upper
107 100
121 49.4 39.7 59.5
122 81.8 66.1 99.1









#27
 Bis(2-Chloroethoxy)methane
 Concen: 21.656 ng/ul
 RT: 10.134 min Scan# 1181
 Delta R.T. -0.006 min
 Lab File: BN025135.D
 Acq: 25 Apr 2023 18:22




Instrument :
 BNA_N
 ClientSampleId :
 SSTD020283


Tgt Ion: 93 Resp: 758615
 Ion Ratio Lower Upper
 93 100
 95 31.9 26.1 39.1
 123 10.4 8.5 12.7

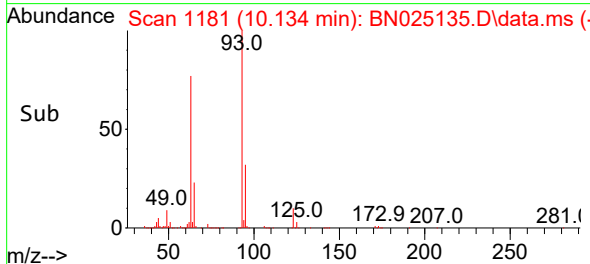

#29
 2,4-Dichlorophenol
 Concen: 21.908 ng/ul
 RT: 10.369 min Scan# 1221
 Delta R.T. -0.006 min
 Lab File: BN025135.D
 Acq: 25 Apr 2023 18:22

Tgt Ion: 162 Resp: 485793
 Ion Ratio Lower Upper
 162 100
 164 63.1 50.9 76.3
 98 39.0 31.0 46.4


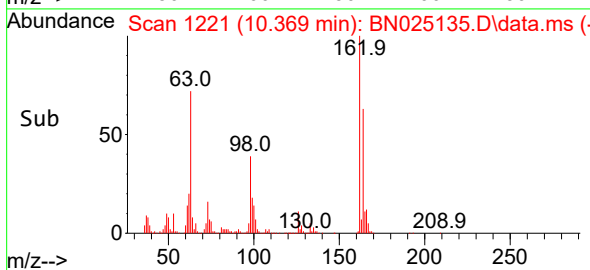

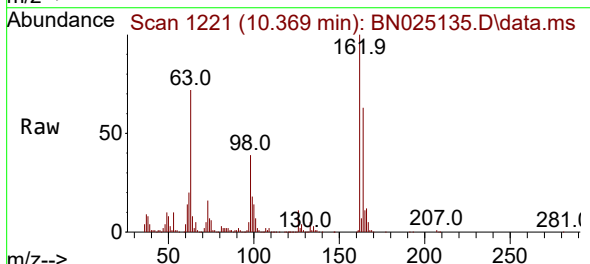




#30
Naphthalene
Concen: 21.684 ng/ul
RT: 10.775 min Scan# 1310
Delta R.T. -0.006 min
Lab File: BN025135.D
Acq: 25 Apr 2023 18:22




Instrument :
BNA_N
ClientSampleId :
SSTD020283


Tgt Ion:128 Resp: 1706891
Ion Ratio Lower Upper
128 100
129 10.4 8.4 12.6
127 12.8 10.7 16.1

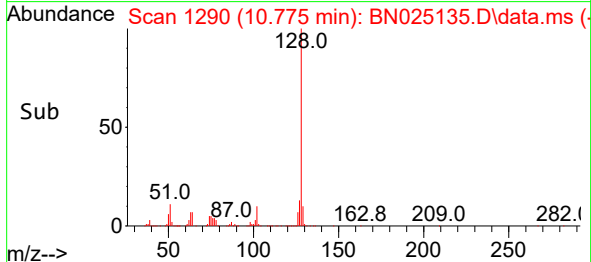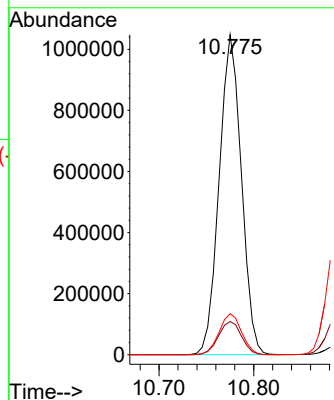

#32
4-Chloroaniline
Concen: 21.803 ng/ul
RT: 10.893 min Scan# 1310
Delta R.T. -0.000 min
Lab File: BN025135.D
Acq: 25 Apr 2023 18:22

Tgt Ion:127 Resp: 740026
Ion Ratio Lower Upper
127 100
129 30.6 25.5 38.3

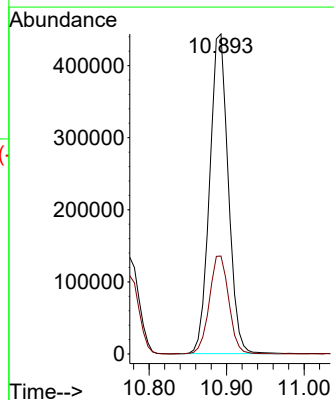



#33

Hexachlorobutadiene

Concen: 22.972 ng/ul

RT: 11.057 min Scan# 1338

Delta R.T. -0.006 min

Lab File: BN025135.D

Acq: 25 Apr 2023 18:22

Instrument :

BNA_N

ClientSampleId :

SSTD020283





Tgt Ion:225 Resp: 296904

Ion Ratio Lower Upper

225 100

223 66.8 45.9 68.9

227 65.5 51.2 76.8

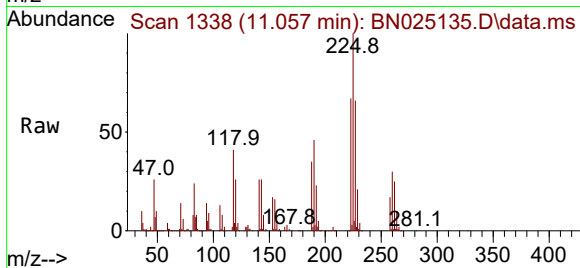

#34

Caprolactam

Concen: 13.333 ng/ul

RT: 11.657 min Scan# 1440

Delta R.T. -0.006 min

Lab File: BN025135.D

Acq: 25 Apr 2023 18:22




Tgt Ion:113 Resp: 103624


Ion Ratio Lower Upper

113 100

55 227.3 188.3 282.5

56 167.5 133.5 200.3




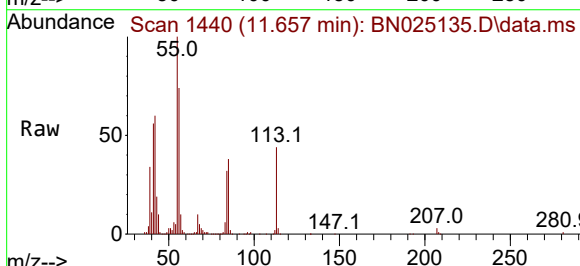




#35
4-Chloro-3-methylphenol
Concen: 21.909 ng/ul
RT: 12.010 min Scan# 1500
Delta R.T. -0.006 min
Lab File: BN025135.D
Acq: 25 Apr 2023 18:22




Instrument :
BNA_N
ClientSampleId :
SSTD020283


Tgt Ion:107 Resp: 569625
Ion Ratio Lower Upper
107 100
144 25.6 19.6 29.4
142 76.8 60.7 91.1



#36
2-Methylnaphthalene
Concen: 22.144 ng/ul
RT: 12.387 min Scan# 1564
Delta R.T. -0.006 min
Lab File: BN025135.D
Acq: 25 Apr 2023 18:22

Tgt Ion:142 Resp: 1152003
Ion Ratio Lower Upper
142 100
141 87.9 71.4 107.2







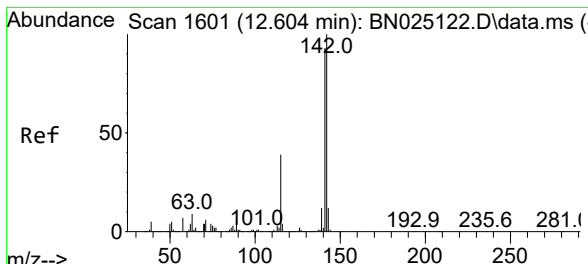

#37
 1-Methylnaphthalene
 Concen: 22.128 ng/ul
 RT: 12.604 min Scan# 1601
 Delta R.T. -0.006 min
 Lab File: BN025135.D
 Acq: 25 Apr 2023 18:22




Instrument :
 BNA_N
 ClientSampleId :
 SSTD020283


Tgt Ion:142 Resp: 1149138
 Ion Ratio Lower Upper
 142 100
 141 92.5 73.5 110.3
 116 4.0 3.1 4.7

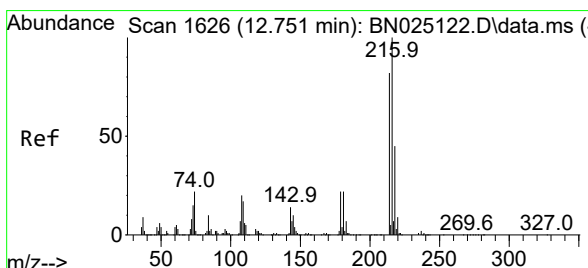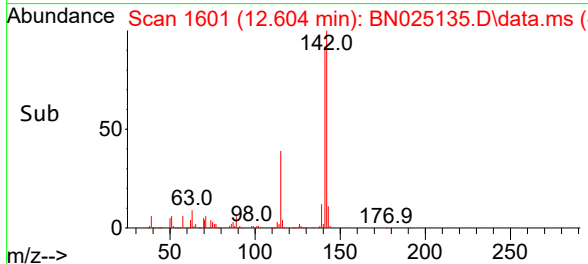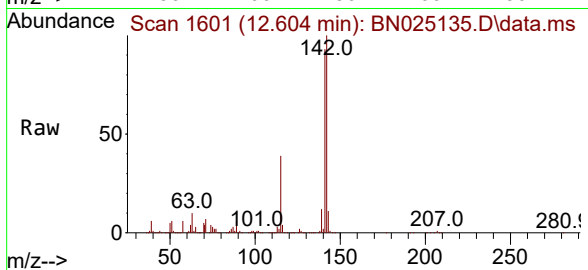

#39
 1,2,4,5-Tetrachlorobenzene
 Concen: 22.290 ng/ul
 RT: 12.757 min Scan# 1627
 Delta R.T. -0.000 min
 Lab File: BN025135.D
 Acq: 25 Apr 2023 18:22

Tgt Ion:216 Resp: 590078
 Ion Ratio Lower Upper
 216 100
 214 78.5 62.2 93.4
 179 21.7 16.8 25.2
 108 19.2 15.0 22.6

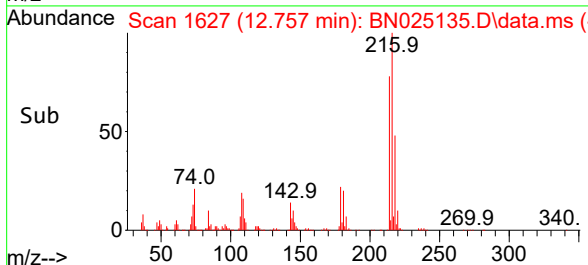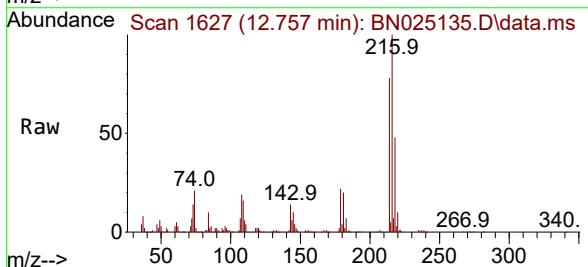



#40

Hexachlorocyclopentadiene

Concen: 16.397 ng/ul

RT: 12.734 min Scan# 1622

Delta R.T. -0.000 min

Lab File: BN025135.D

Acq: 25 Apr 2023 18:22

Instrument :

BNA_N

ClientSampleId :

SSTD020283





Tgt Ion:237 Resp: 264701

Ion Ratio Lower Upper

237 100

235 68.4 49.9 74.9

272 12.6 10.2 15.4



#41

2,4,6-Trichlorophenol

Concen: 22.089 ng/ul

RT: 12.992 min Scan# 1667

Delta R.T. -0.006 min

Lab File: BN025135.D

Acq: 25 Apr 2023 18:22




Tgt Ion:196 Resp: 399548


Ion Ratio Lower Upper

196 100

198 100.4 74.5 111.7

200 31.8 24.3 36.5









#42
2,4,5-Trichlorophenol
Concen: 22.246 ng/ul
RT: 13.063 min Scan# 1
Delta R.T. -0.006 min
Lab File: BN025135.D
Acq: 25 Apr 2023 18:22




Instrument :
BNA_N
ClientSampleId :
SSTD020283


Tgt Ion:196 Resp: 440336
Ion Ratio Lower Upper
196 100
198 92.5 78.2 117.2
200 29.7 24.0 36.0

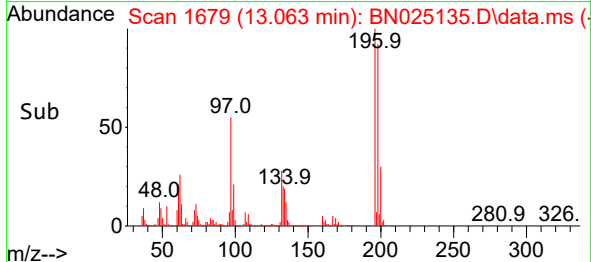

#43
1,1'-Biphenyl
Concen: 21.794 ng/ul
RT: 13.398 min Scan# 1736
Delta R.T. -0.000 min
Lab File: BN025135.D
Acq: 25 Apr 2023 18:22

Tgt Ion:154 Resp: 1575957
Ion Ratio Lower Upper
154 100
153 39.8 32.2 48.2
76 14.3 12.4 18.6

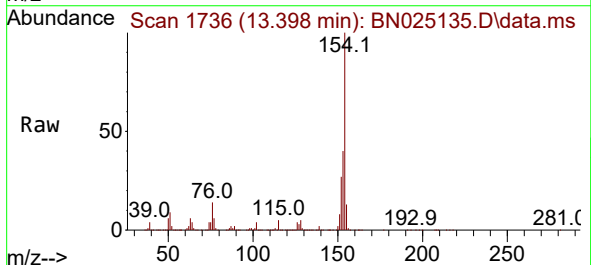




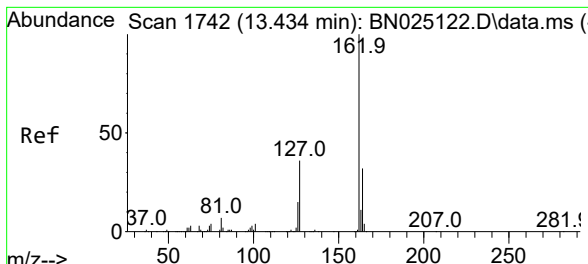


#44
 2-Chloronaphthalene
 Concen: 21.831 ng/ul
 RT: 13.440 min Scan# 1743
 Delta R.T. -0.000 min
 Lab File: BN025135.D
 Acq: 25 Apr 2023 18:22

Instrument :
 BNA_N
 ClientSampleId :
 SSTD020283

Tgt Ion:162 Resp: 1225761




Ion	Ratio	Lower	Upper
162	100		
164	32.3	25.9	38.9
127	39.3	32.9	49.3

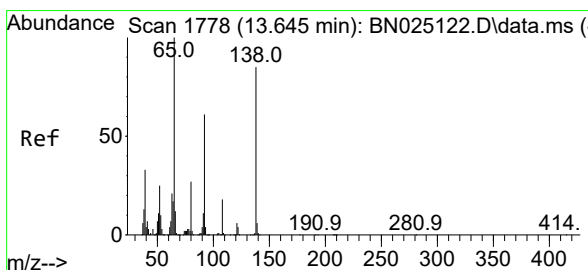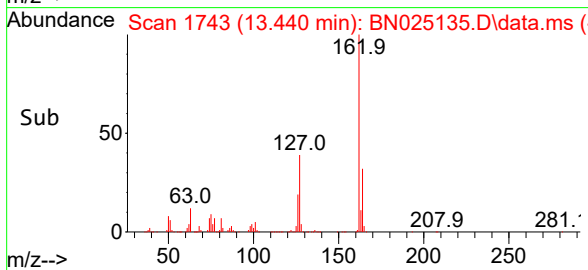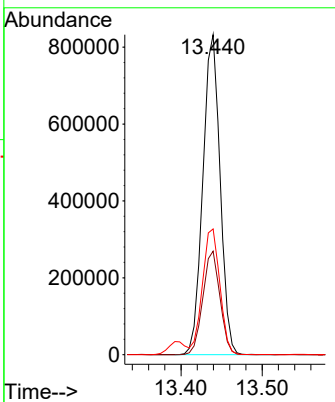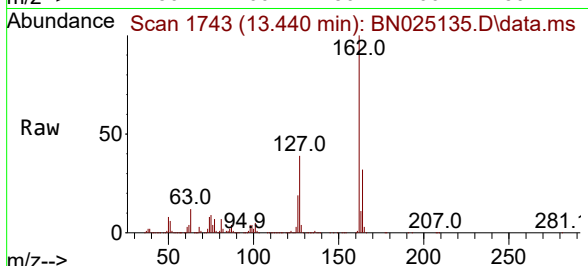


#45
 2-Nitroaniline
 Concen: 21.656 ng/ul
 RT: 13.645 min Scan# 1778
 Delta R.T. -0.006 min
 Lab File: BN025135.D
 Acq: 25 Apr 2023 18:22

Tgt Ion: 65 Resp: 424600

Ion	Ratio	Lower	Upper
65	100		
92	61.3	50.7	76.1
138	89.9	71.4	107.2


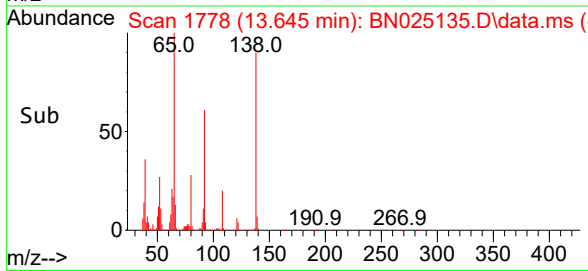
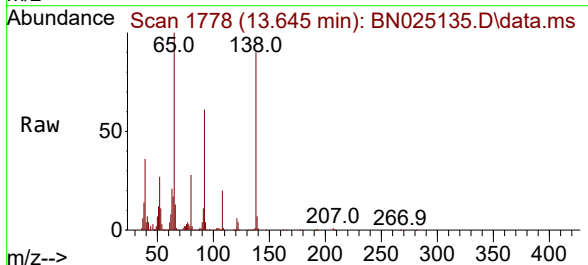
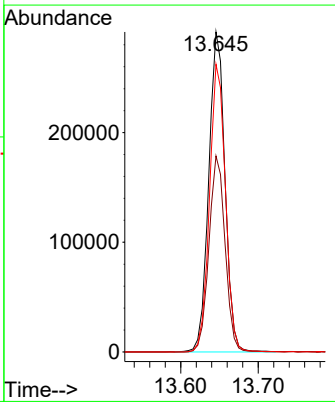




#47
Dimethylphthalate
Concen: 21.977 ng/ul
RT: 14.022 min Scan# 1842
Delta R.T. -0.000 min
Lab File: BN025135.D
Acq: 25 Apr 2023 18:22




Instrument :
BNA_N
ClientSampleId :
SSTD020283


Tgt Ion:163 Resp: 1555764
Ion Ratio Lower Upper
163 100
194 3.9 3.3 4.9
164 10.3 8.2 12.2

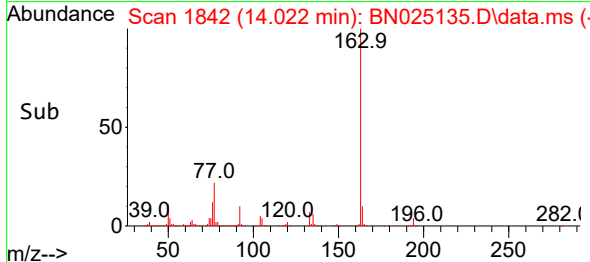

#48
2,6-Dinitrotoluene
Concen: 22.277 ng/ul
RT: 14.145 min Scan# 1863
Delta R.T. -0.000 min
Lab File: BN025135.D
Acq: 25 Apr 2023 18:22

Tgt Ion:165 Resp: 307814
Ion Ratio Lower Upper
165 100
89 65.6 49.8 74.8
121 21.8 17.2 25.8

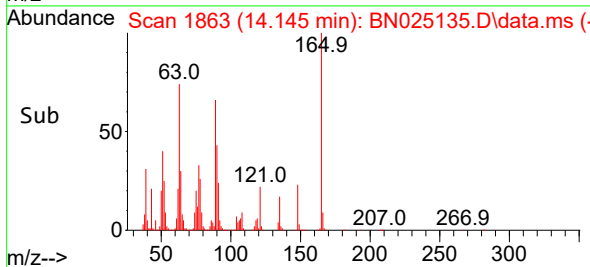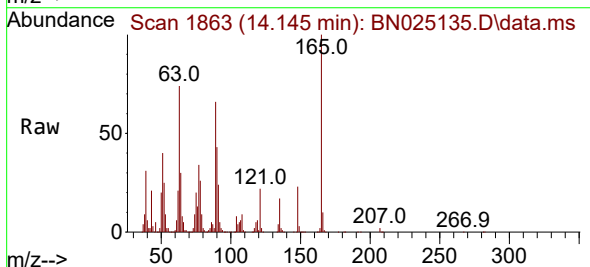



#50

Acenaphthylene

Concen: 21.664 ng/ul

RT: 14.287 min Scan# 1886

Delta R.T. -0.000 min

Lab File: BN025135.D

Acq: 25 Apr 2023 18:22

Instrument :

BNA_N

ClientSampleId :

SSTD020283





Tgt Ion:152 Resp: 1918457

Ion Ratio Lower Upper

152 100

151 19.4 16.2 24.4

153 12.8 10.6 16.0



#51

3-Nitroaniline

Concen: 22.287 ng/ul

RT: 14.475 min Scan# 1919

Delta R.T. -0.000 min

Lab File: BN025135.D

Acq: 25 Apr 2023 18:22




Tgt Ion:138 Resp: 323624


Ion Ratio Lower Upper

138 100

108 10.7 8.6 12.8

92 120.4 99.5 149.3









#52
Acenaphthene
Concen: 21.954 ng/ul
RT: 14.628 min Scan# 1944
Delta R.T. -0.000 min
Lab File: BN025135.D
Acq: 25 Apr 2023 18:22




Instrument :
BNA_N
ClientSampleId :
SSTD020283


Tgt Ion:153 Resp: 1344061
Ion Ratio Lower Upper
153 100
152 46.2 38.8 58.2
154 87.5 70.3 105.5

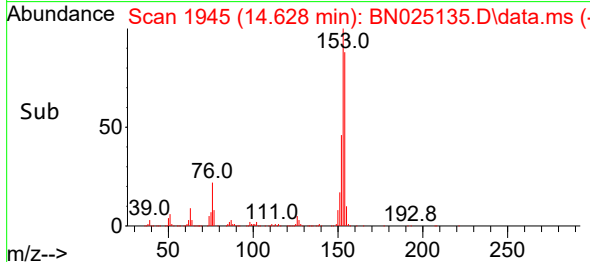

#53
2,4-Dinitrophenol
Concen: 17.008 ng/ul
RT: 14.675 min Scan# 1953
Delta R.T. -0.006 min
Lab File: BN025135.D
Acq: 25 Apr 2023 18:22

Tgt Ion:184 Resp: 151102
Ion Ratio Lower Upper
184 100
63 91.6 62.6 93.8
154 65.5 50.9 76.3


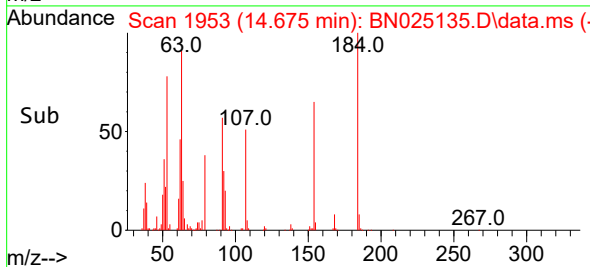

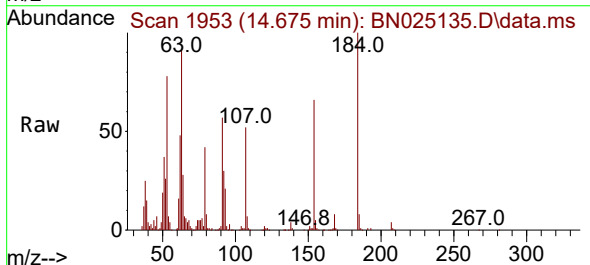




#55
4-Nitrophenol
Concen: 21.544 ng/ul
RT: 14.775 min Scan# 1970
Delta R.T. -0.000 min
Lab File: BN025135.D
Acq: 25 Apr 2023 18:22




Instrument :
BNA_N
ClientSampleId :
SSTD020283


Tgt Ion:109 Resp: 252885
Ion Ratio Lower Upper
109 100
139 124.8 104.3 156.5
65 149.1 124.3 186.5

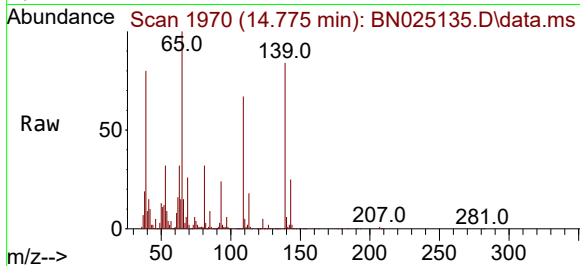

#56
Dibenzofuran
Concen: 22.027 ng/ul
RT: 14.957 min Scan# 2001
Delta R.T. -0.006 min
Lab File: BN025135.D
Acq: 25 Apr 2023 18:22

Tgt Ion:168 Resp: 1858766
Ion Ratio Lower Upper
168 100
139 38.2 32.1 48.1

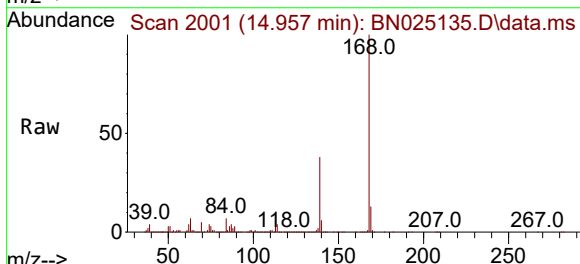



#57

2,4-Dinitrotoluene

Concen: 22.586 ng/ul

RT: 14.928 min Scan# 1996

Delta R.T. -0.006 min

Lab File: BN025135.D

Acq: 25 Apr 2023 18:22

Instrument :

BNA_N

ClientSampleId :

SSTD020283





Tgt Ion:165 Resp: 451757

Ion Ratio Lower Upper

165 100

63 58.1 45.4 68.0

182 2.6 2.2 3.2



#58

2,3,4,6-Tetrachlorophenol

Concen: 22.717 ng/ul

RT: 15.186 min Scan# 2040

Delta R.T. -0.000 min

Lab File: BN025135.D

Acq: 25 Apr 2023 18:22

Tgt Ion:232 Resp: 370274




Ion Ratio Lower Upper


232 100

131 50.3 40.6 61.0

130 3.0 2.2 3.2

166 34.0 27.0 40.4



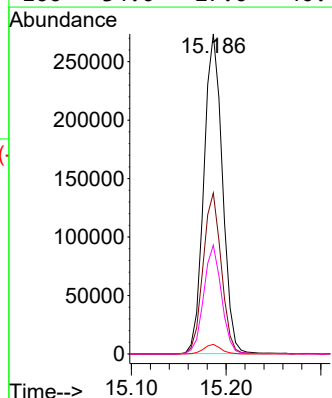





#59
Diethylphthalate
Concen: 22.281 ng/ul
RT: 15.381 min Scan# 2073
Delta R.T. -0.006 min
Lab File: BN025135.D
Acq: 25 Apr 2023 18:22




Instrument :
BNA_N
ClientSampleId :
SSTD020283


Tgt Ion:149 Resp: 1584938
Ion Ratio Lower Upper
149 100
177 20.9 16.6 24.8
150 12.6 10.1 15.1

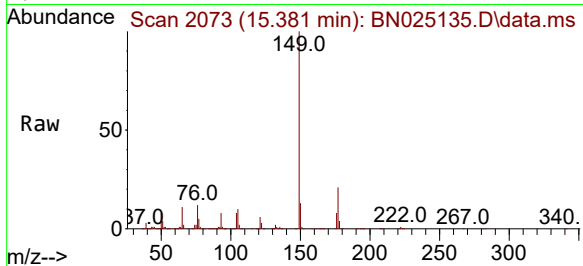

#61
Fluorene
Concen: 22.432 ng/ul
RT: 15.610 min Scan# 2112
Delta R.T. -0.000 min
Lab File: BN025135.D
Acq: 25 Apr 2023 18:22

Tgt Ion:166 Resp: 1522546
Ion Ratio Lower Upper
166 100
165 96.7 79.1 118.7
167 13.5 10.8 16.2




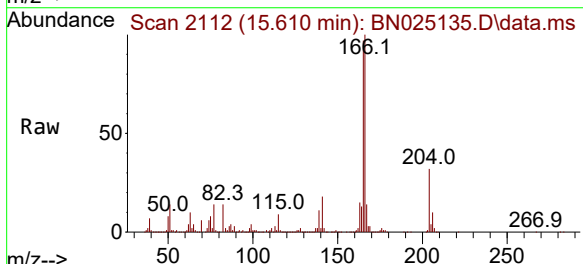




#62
4-Chlorophenyl-phenylether
Concen: 23.368 ng/ul
RT: 15.604 min Scan# 2111
Delta R.T. -0.000 min
Lab File: BN025135.D
Acq: 25 Apr 2023 18:22




Instrument :
BNA_N
ClientSampleId :
SSTD020283


Tgt Ion:204 Resp: 738260
Ion Ratio Lower Upper
204 100
206 32.9 26.0 39.0
141 60.1 51.8 77.8

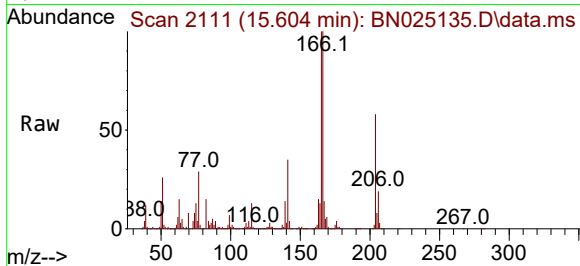

#63
4-Nitroaniline
Concen: 23.921 ng/ul
RT: 15.634 min Scan# 2116
Delta R.T. -0.006 min
Lab File: BN025135.D
Acq: 25 Apr 2023 18:22

Tgt Ion:138 Resp: 342298
Ion Ratio Lower Upper
138 100
92 55.7 43.3 64.9
108 85.4 64.2 96.4




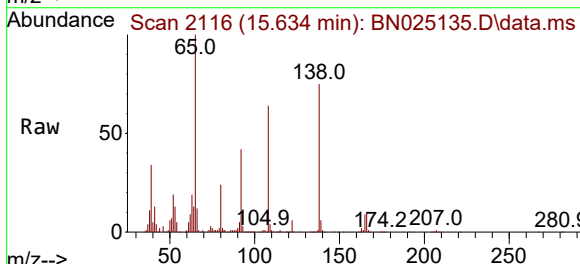




#66
4,6-Dinitro-2-methylphenol
Concen: 20.072 ng/ul
RT: 15.692 min Scan# 2126
Delta R.T. -0.000 min
Lab File: BN025135.D
Acq: 25 Apr 2023 18:22




Instrument :
BNA_N
ClientSampleId :
SSTD020283


Tgt Ion:198 Resp: 255062
Ion Ratio Lower Upper
198 100
182 4.2 3.4 5.0
77 29.7 23.7 35.5

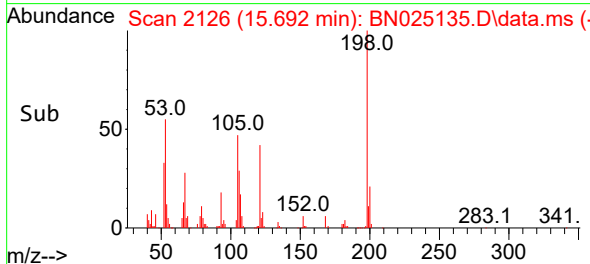

#67
N-Nitrosodiphenylamine
Concen: 21.622 ng/ul
RT: 15.816 min Scan# 2147
Delta R.T. -0.006 min
Lab File: BN025135.D
Acq: 25 Apr 2023 18:22

Tgt Ion:169 Resp: 1307595
Ion Ratio Lower Upper
169 100
168 66.6 54.3 81.5
167 35.3 27.6 41.4


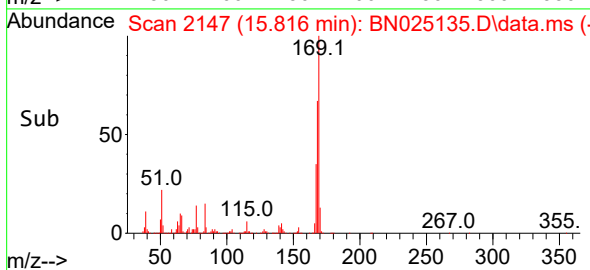

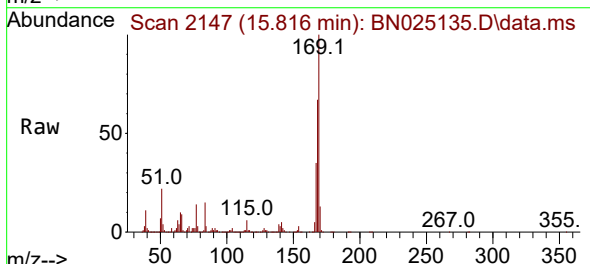


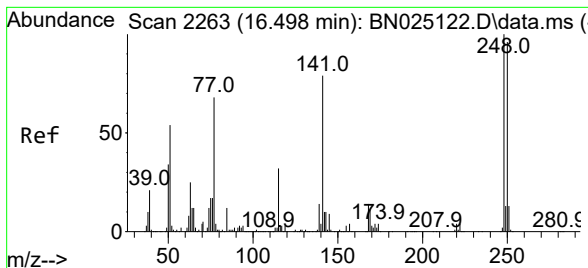

#68
4-Bromophenyl-phenylether
Concen: 22.123 ng/ul
RT: 16.498 min Scan# 21
Delta R.T. -0.000 min
Lab File: BN025135.D
Acq: 25 Apr 2023 18:22




Instrument :
BNA_N
ClientSampleId :
SSTD020283


Tgt Ion:248 Resp: 443260
Ion Ratio Lower Upper
248 100
250 99.9 77.1 115.7
141 79.7 62.3 93.5

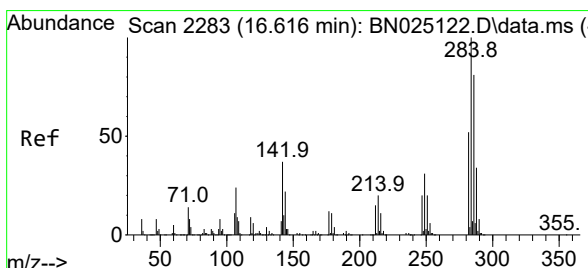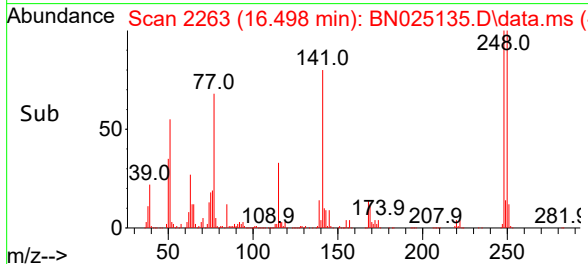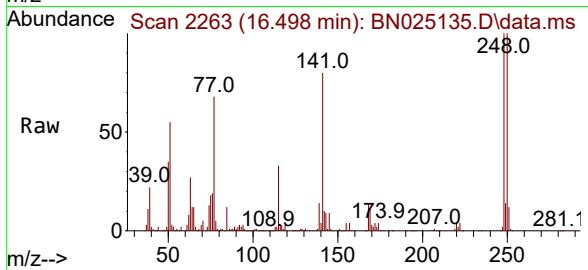

#69
Hexachlorobenzene
Concen: 21.892 ng/ul
RT: 16.616 min Scan# 2283
Delta R.T. -0.000 min
Lab File: BN025135.D
Acq: 25 Apr 2023 18:22

Tgt Ion:284 Resp: 496629
Ion Ratio Lower Upper
284 100
142 37.7 31.0 46.6
249 29.1 25.1 37.7


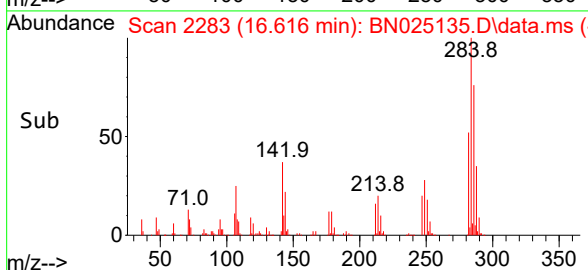

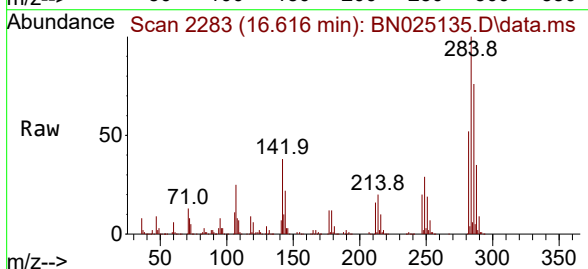




#70
 Atrazine
 Concen: 21.896 ng/ul
 RT: 16.769 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BN025135.D
 Acq: 25 Apr 2023 18:22




Instrument :
 BNA_N
 ClientSampleId :
 SSTD020283


Tgt Ion:200 Resp: 450576
 Ion Ratio Lower Upper
 200 100
 173 25.9 21.4 32.2
 215 47.6 38.2 57.2



#71
 Pentachlorophenol
 Concen: 21.044 ng/ul
 RT: 16.957 min Scan# 2341
 Delta R.T. -0.006 min
 Lab File: BN025135.D
 Acq: 25 Apr 2023 18:22

Tgt Ion:266 Resp: 296730
 Ion Ratio Lower Upper
 266 100
 264 62.6 52.7 79.1
 268 62.0 51.4 77.0





#72

Phenanthrene

Concen: 21.465 ng/ul

RT: 17.351 min Scan# 2408

Delta R.T. -0.000 min

Lab File: BN025135.D

Acq: 25 Apr 2023 18:22

Instrument :

BNA_N

ClientSampleId :

SSTD020283





Tgt Ion:178 Resp: 2414532

Ion Ratio Lower Upper

178 100

179 15.1 12.6 19.0

176 19.3 15.2 22.8



#74

Anthracene

Concen: 21.668 ng/ul

RT: 17.445 min Scan# 2424

Delta R.T. -0.000 min

Lab File: BN025135.D

Acq: 25 Apr 2023 18:22




Tgt Ion:178 Resp: 2456071


Ion Ratio Lower Upper

178 100

179 15.5 12.2 18.4

176 19.1 14.6 21.8





#75

1,2,3,4-Tetrachlorobenzene

Concen: 21.377 ng/uL

RT: 13.363 min Scan# 1730

Delta R.T. -0.000 min

Lab File: BN025135.D

Acq: 25 Apr 2023 18:22

Instrument :

BNA_N

ClientSampleId :

SSTD020283





Tgt Ion:216 Resp: 606071

Ion Ratio Lower Upper

216 100

214 78.0 62.5 93.7

218 48.5 37.7 56.5



#76

Pentachlorobenzene

Concen: 21.944 ng/uL

RT: 14.881 min Scan# 1988

Delta R.T. -0.000 min

Lab File: BN025135.D

Acq: 25 Apr 2023 18:22




Tgt Ion:250 Resp: 595251


Ion Ratio Lower Upper

250 100

248 64.9 50.8 76.2

252 62.8 51.8 77.6

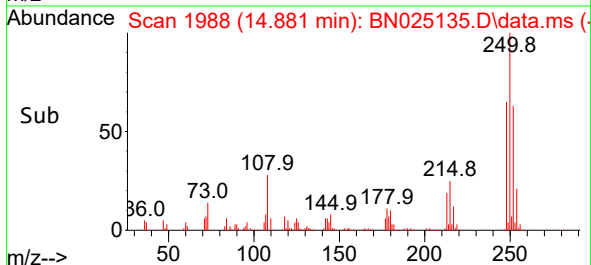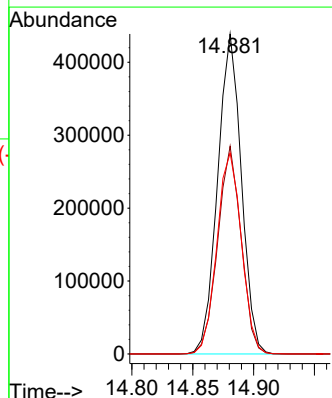



#77

Carbazole

Concen: 21.686 ng/ul

RT: 17.716 min Scan# 2470

Delta R.T. -0.000 min

Lab File: BN025135.D

Acq: 25 Apr 2023 18:22

Instrument :





BNA_N

ClientSampleId :

SSTD020283

Tgt Ion:167 Resp: 2219521

Ion	Ratio	Lower	Upper
167	100		
166	22.2	16.6	24.8
139	13.2	10.2	15.4

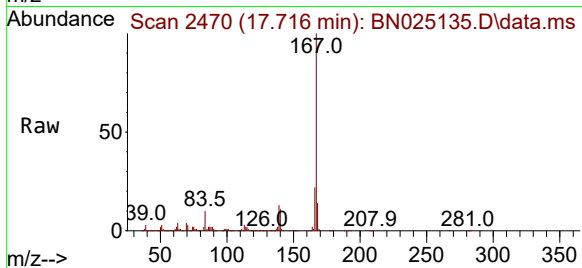

#78

Di-n-butylphthalate

Concen: 21.964 ng/ul

RT: 18.275 min Scan# 2565




Delta R.T. -0.006 min


Lab File: BN025135.D

Acq: 25 Apr 2023 18:22

Tgt Ion:149 Resp: 2668211

Ion	Ratio	Lower	Upper
149	100		
150	8.9	7.4	11.2
104	5.6	4.2	6.4


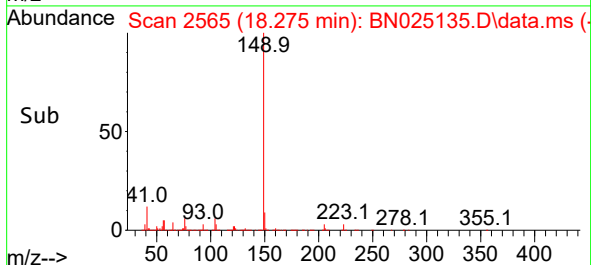

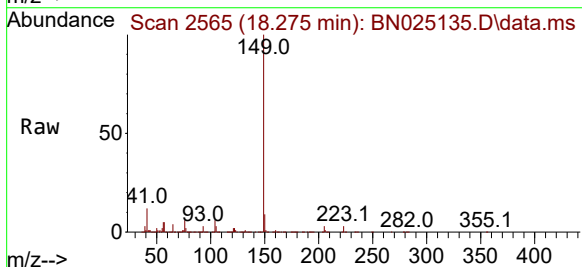




#80
Fluoranthene
Concen: 22.566 ng/ul
RT: 19.369 min Scan# 2751
Delta R.T. -0.000 min
Lab File: BN025135.D
Acq: 25 Apr 2023 18:22




Instrument :
BNA_N
ClientSampleId :
SSTD020283


Tgt Ion:202 Resp: 2815126
Ion Ratio Lower Upper
202 100
101 13.1 10.7 16.1
100 9.9 7.9 11.9

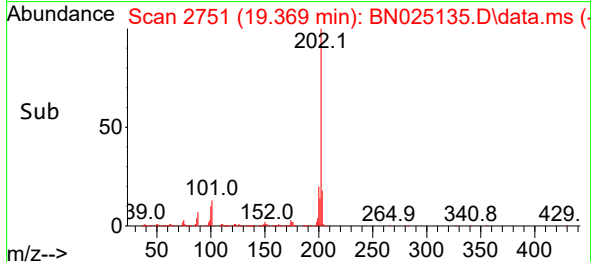

#82
Pyrene
Concen: 22.180 ng/ul
RT: 19.733 min Scan# 2813
Delta R.T. -0.000 min
Lab File: BN025135.D
Acq: 25 Apr 2023 18:22

Tgt Ion:202 Resp: 2912517
Ion Ratio Lower Upper
202 100
101 15.5 13.0 19.6
100 12.6 11.0 16.6




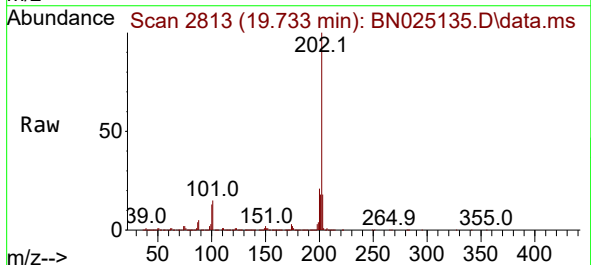




#83
Butylbenzylphthalate
Concen: 21.951 ng/ul
RT: 20.633 min Scan# 2966
Delta R.T. -0.000 min
Lab File: BN025135.D
Acq: 25 Apr 2023 18:22




Instrument :
BNA_N
ClientSampleId :
SSTD020283


Tgt Ion:149 Resp: 1196677
Ion Ratio Lower Upper
149 100
91 77.8 62.6 93.8
206 20.1 16.2 24.2



#84
3,3'-Dichlorobenzidine
Concen: 22.922 ng/ul
RT: 21.427 min Scan# 3101
Delta R.T. -0.000 min
Lab File: BN025135.D
Acq: 25 Apr 2023 18:22

Tgt Ion:252 Resp: 942726
Ion Ratio Lower Upper
252 100
254 62.2 52.2 78.2
126 11.3 11.4 17.2#





#85

Benzo(a)anthracene

Concen: 22.312 ng/ul

RT: 21.492 min Scan# 3112

Delta R.T. -0.000 min

Lab File: BN025135.D

Acq: 25 Apr 2023 18:22

Instrument :

BNA_N

ClientSampleId :

SSTD020283





Tgt Ion:228 Resp: 2872439

Ion Ratio Lower Upper

228 100

229 20.2 16.2 24.2

226 26.5 20.7 31.1



#86

Bis(2-ethylhexyl)phthalate

Concen: 21.737 ng/ul

RT: 21.410 min Scan# 3098

Delta R.T. -0.000 min

Lab File: BN025135.D

Acq: 25 Apr 2023 18:22




Tgt Ion:149 Resp: 1769016


Ion Ratio Lower Upper

149 100

167 27.6 21.8 32.8

279 3.5 2.9 4.3





#87

Chrysene

Concen: 21.839 ng/ul

RT: 21.545 min Scan# 3121

Delta R.T. -0.000 min

Lab File: BN025135.D

Acq: 25 Apr 2023 18:22

Instrument :

BNA_N

ClientSampleId :

SSTD020283





Tgt Ion:228 Resp: 2678072

Ion Ratio Lower Upper

228 100

226 29.5 22.4 33.6

229 18.7 15.6 23.4



#89

Di-n-octyl phthalate

Concen: 23.381 ng/ul




RT: 22.351 min Scan# 3258


Delta R.T. -0.000 min

Lab File: BN025135.D

Acq: 25 Apr 2023 18:22

Tgt Ion:149 Resp: 3035430

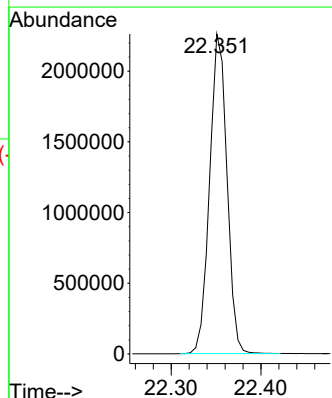



#90

Benzo(b)fluoranthene

Concen: 22.319 ng/ul

RT: 23.198 min Scan# 3402

Delta R.T. -0.000 min

Lab File: BN025135.D

Acq: 25 Apr 2023 18:22

Instrument :

BNA_N

ClientSampleId :

SSTD020283





Tgt Ion:252 Resp: 2765118

Ion Ratio Lower Upper

252 100

253 23.1 19.2 28.8

125 11.8 10.4 15.6



#91

Benzo(k)fluoranthene

Concen: 22.710 ng/ul

RT: 23.251 min Scan# 3411

Delta R.T. 0.006 min

Lab File: BN025135.D

Acq: 25 Apr 2023 18:22




Tgt Ion:252 Resp: 2768444


Ion Ratio Lower Upper

252 100

253 21.8 16.7 25.1

125 11.1 9.3 13.9

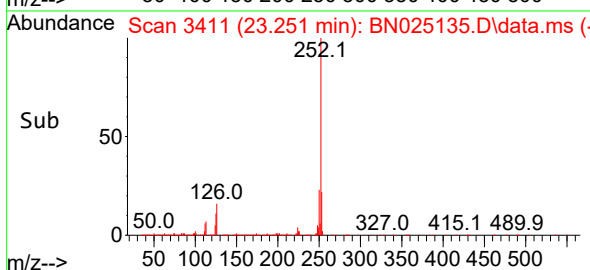



#93

Benzo(a)pyrene

Concen: 21.729 ng/ul

RT: 23.839 min Scan# 3

Delta R.T. 0.006 min

Lab File: BN025135.D

Acq: 25 Apr 2023 18:22

Instrument :

BNA_N

ClientSampleId :

SSTD020283





Tgt Ion:252 Resp: 2356859

Ion Ratio Lower Upper

252 100

253 22.2 17.4 26.0

125 12.7 10.8 16.2



#94

Indeno(1,2,3-cd)pyrene

Concen: 9.997 ng/ul

RT: 26.480 min Scan# 3960

Delta R.T. 0.018 min

Lab File: BN025135.D

Acq: 25 Apr 2023 18:22




Tgt Ion:276 Resp: 1313800


Ion Ratio Lower Upper

276 100

138 24.2 21.9 32.9

277 24.7 19.8 29.6





#95

Dibenzo(a,h)anthracene

Concen: 21.996 ng/ul

RT: 26.515 min Scan# 3959

Delta R.T. 0.029 min

Lab File: BN025135.D

Acq: 25 Apr 2023 18:22

Instrument :

BNA_N

ClientSampleId :

SSTD020283





Tgt Ion:278 Resp: 2386516

Ion Ratio Lower Upper

278 100

139 16.2 14.6 21.8

279 21.9 18.2 27.4

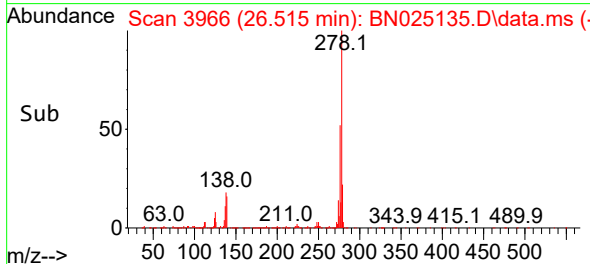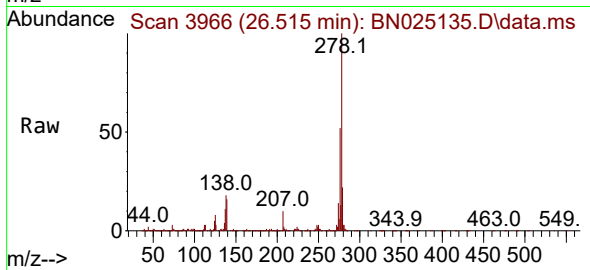

#96

Benzo(g,h,i)perylene

Concen: 21.001 ng/ul

RT: 27.268 min Scan# 4094

Delta R.T. 0.029 min

Lab File: BN025135.D

Acq: 25 Apr 2023 18:22

Tgt Ion:276 Resp: 2239573

Ion Ratio Lower Upper

276 100

138 23.9 19.8 29.8

277 24.4 17.6 26.4

