

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042523\
 Data File : BN025126.D
 Acq On : 25 Apr 2023 12:18
 Operator : CG/JU
 Sample : 02400-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COML6

Quant Time: Apr 26 00:45:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 25 08:52:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.916	152	337304	20.000	ng/u1	0.00
20) Naphthalene-d8	10.728	136	1487205	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.563	164	951664	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.310	188	2041058	20.000	ng/u1	0.00
79) Chrysene-d12	21.504	240	1830573	20.000	ng/u1	0.00
88) Perylene-d12	23.927	264	1773891	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	35183	3.970	ng/uL	0.00
4) Pyridine-d5	3.723	84	207981	7.837	ng/u1	0.00
7) Phenol-d5	7.075	99	187212	5.693	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.240	67	653050	29.690	ng/u1	0.00
11) 2-Chlorophenol-d4	7.440	132	534687	22.125	ng/u1	0.00
15) 4-Methylphenol-d8	8.622	113	365538	14.002	ng/u1	0.00
21) Nitrobenzene-d5	9.081	128	359302	29.838	ng/u1	0.00
24) 2-Nitrophenol-d4	9.805	143	385793	29.579	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.346	165	624875	26.804	ng/u1	0.00
31) 4-Chloroaniline-d4	10.863	131	868849	24.558	ng/u1	0.00
46) Dimethylphthalate-d6	13.969	166	2393085	32.438	ng/u1	0.00
49) Acenaphthylene-d8	14.251	160	2589018	30.624	ng/u1	0.00
54) 4-Nitrophenol-d4	14.757	143	66475	4.396	ng/u1	0.00
60) Fluorene-d10	15.551	176	2025042	32.510	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.675	200	348661	26.249	ng/u1	0.00
73) Anthracene-d10	17.410	188	3324021	34.675	ng/u1	0.00
81) Pyrene-d10	19.704	212	3882890	36.528	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.774	264	3348193	36.099	ng/u1	0.00
Target Compounds						
					Qvalue	
22) Nitrobenzene	9.122	77	81190	2.509	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042523\
Data File : BN025126.D
Acq On : 25 Apr 2023 12:18
Operator : CG/JU
Sample : 02400-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COML6

Quant Time: Apr 26 00:45:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 25 08:52:18 2023
Response via : Initial Calibration

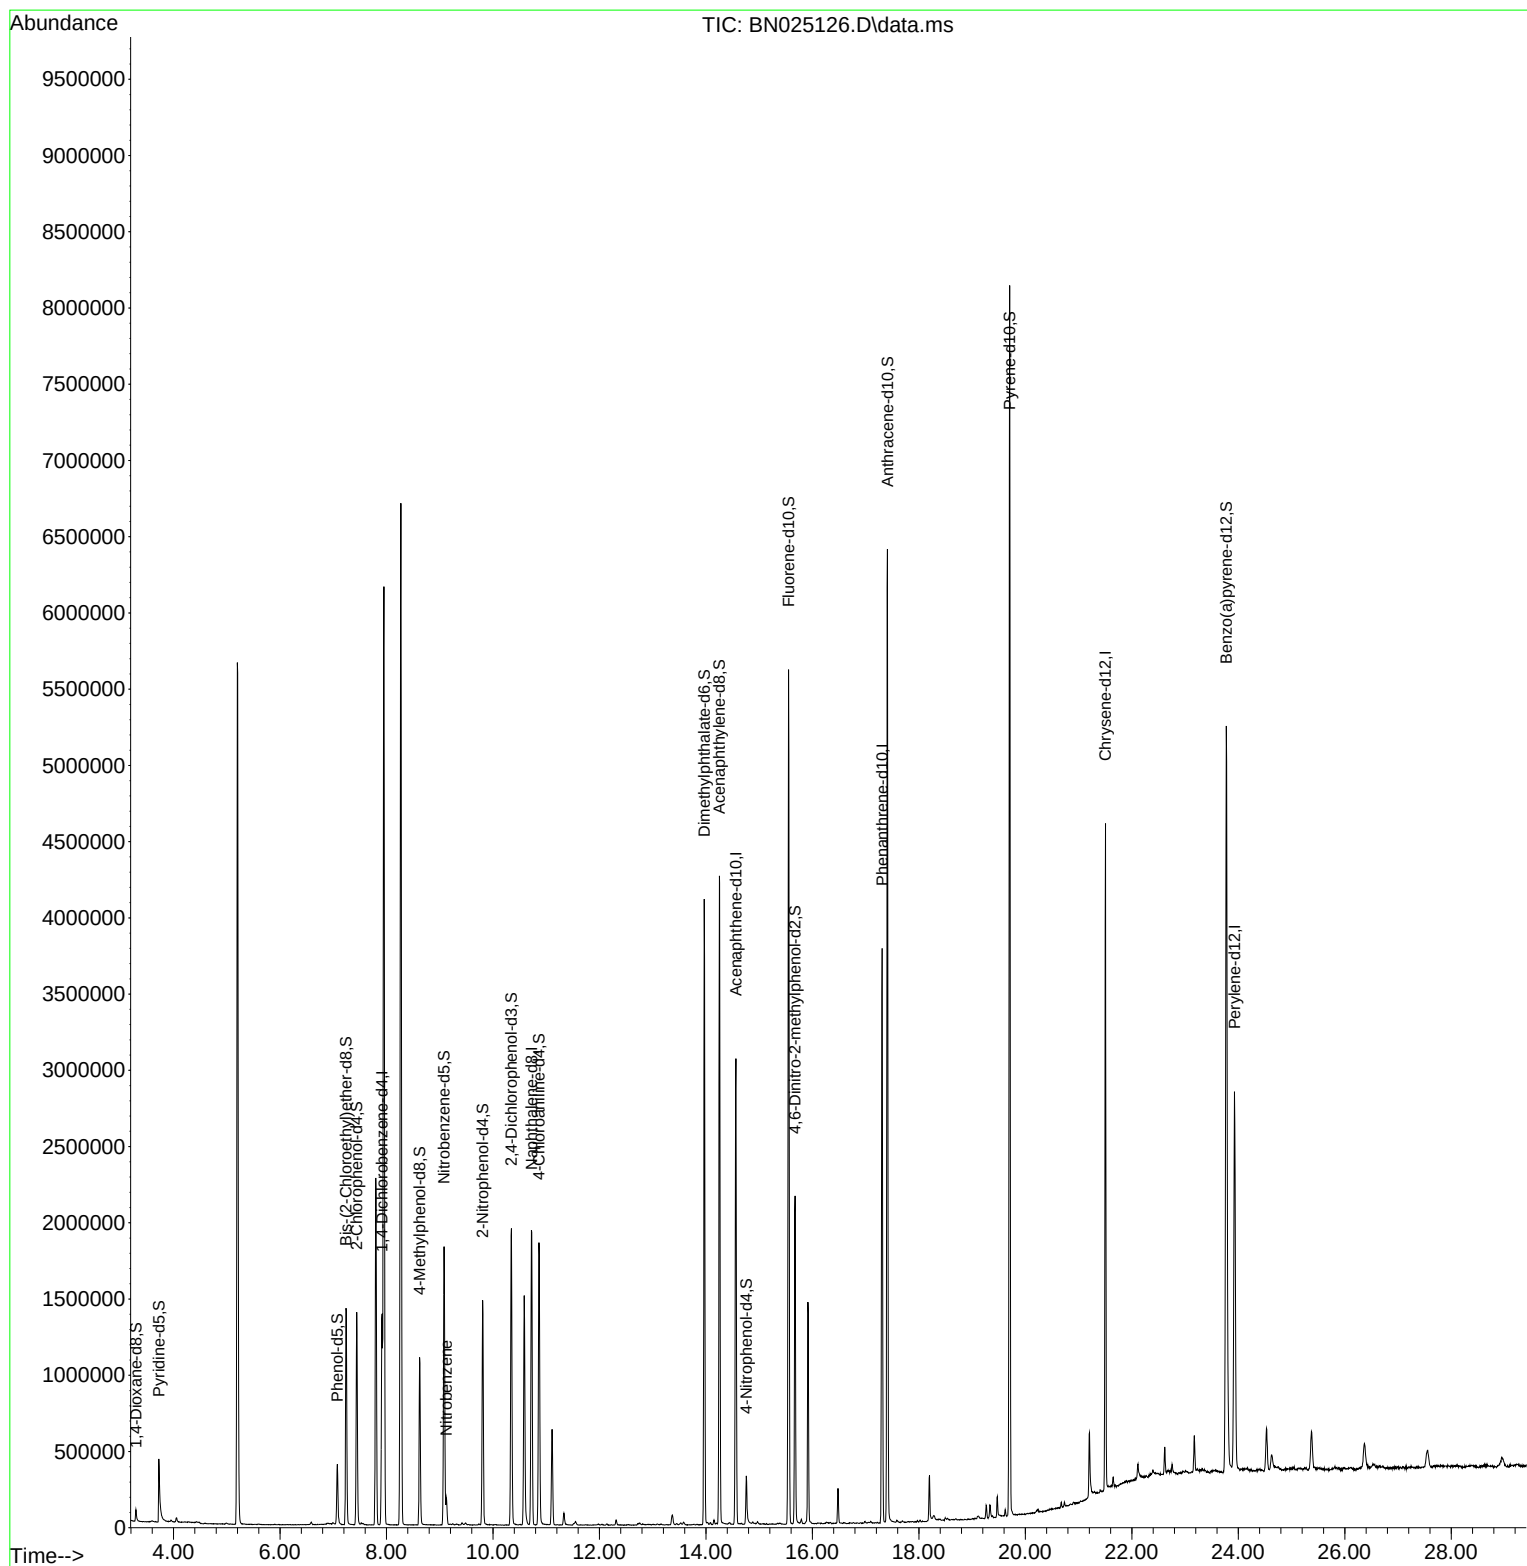

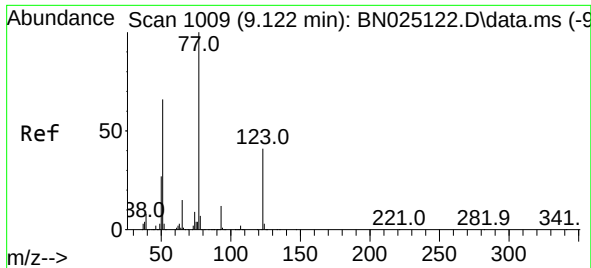

#22
 Nitrobenzene
 Concen: 2.509 ng/ul
 RT: 9.122 min Scan# 10
 Delta R.T. -0.006 min
 Lab File: BN025126.D
 Acq: 25 Apr 2023 12:18

Instrument :
 BNA_N
 ClientSampleId :
 COML6

Tgt Ion: 77	Resp:	81190
Ion	Ratio	Lower Upper
77	100	
123	41.7	33.5 50.3
65	13.8	11.8 17.8

