

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042523\
 Data File : BN025123.D
 Acq On : 25 Apr 2023 10:31
 Operator : CG/JU
 Sample : PB152285BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK285

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Title : SVOA CALIBRATION

Signal : TIC: BN025123.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	14	18	30	rVB	106768	162424	1.67%	0.158%
2	3.587	64	68	75	rBV8	6658	15094	0.16%	0.015%
3	3.717	87	90	116	rBV	1381973	2356513	24.21%	2.298%
4	4.052	142	147	158	rVB	44072	82355	0.85%	0.080%
5	6.952	637	640	646	rBV8	3828	10623	0.11%	0.010%
6	7.075	653	661	680	rVB	1828984	2890375	29.70%	2.819%
7	7.240	683	689	702	rVB	1427472	2233338	22.95%	2.178%
8	7.440	715	723	736	rBV	1783383	2806362	28.84%	2.737%
9	7.910	794	803	814	rBV	1231201	2003301	20.58%	1.954%
10	8.622	916	924	940	rBV	2158950	3480859	35.77%	3.395%
11	9.081	995	1002	1015	rBV	1768601	2854979	29.34%	2.785%
12	9.804	1116	1125	1137	rBV	1510612	2449933	25.17%	2.390%
13	10.340	1207	1216	1229	rBV	2057763	3441375	35.36%	3.357%
14	10.722	1274	1281	1292	rVB	1803510	3002592	30.85%	2.929%
15	10.863	1297	1305	1322	rBV	2335218	3940962	40.49%	3.844%
16	11.969	1488	1493	1502	rVB10	4839	13280	0.14%	0.013%
17	12.316	1545	1552	1557	rBV2	33029	54730	0.56%	0.053%
18	13.969	1826	1833	1845	rBV	3933026	5275102	54.20%	5.145%
19	14.251	1874	1881	1891	rBV	4207949	6080642	62.48%	5.931%
20	14.557	1926	1933	1945	rBV	2659487	4028204	41.39%	3.929%
21	14.757	1960	1967	1988	rBV	2012173	2949833	30.31%	2.877%
22	14.969	2000	2003	2009	rVB8	7706	14225	0.15%	0.014%
23	15.551	2095	2102	2110	rBV	5468238	7549754	77.58%	7.364%
24	15.669	2116	2122	2135	rBV	1721689	2334665	23.99%	2.277%
25	15.786	2138	2142	2152	rVB3	28504	50540	0.52%	0.049%
26	16.334	2230	2235	2239	rBV6	7395	9934	0.10%	0.010%
27	17.304	2394	2400	2409	rBV	3352646	4769178	49.00%	4.652%
28	17.404	2411	2417	2429	rBV2	5900872	8566429	88.02%	8.355%
29	17.581	2443	2447	2452	rVB8	8087	11434	0.12%	0.011%
30	17.686	2462	2465	2471	rBV5	9870	14498	0.15%	0.014%
31	19.263	2729	2733	2740	rBV	66220	95029	0.98%	0.093%
32	19.333	2741	2745	2751	rBV	65863	93312	0.96%	0.091%
33	19.622	2792	2794	2797	rVB3	11827	11358	0.12%	0.011%
34	19.704	2801	2808	2824	rBV	7201077	9732107	100.00%	9.492%
35	21.498	3108	3113	3122	rBV	4042383	4966915	51.04%	4.845%
36	23.780	3494	3501	3517	rBV2	4853452	9295367	95.51%	9.066%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042523\
Data File : BN025123.D
Acq On : 25 Apr 2023 10:31
Operator : CG/JU
Sample : PB152285BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK285

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Title : SVOA CALIBRATION

37 23.939 3520 3528 3541 rVB2 2200075 4877718 50.12% 4.758%




Sum of corrected areas: 102525339

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042523\
Data File : BN025123.D
Acq On : 25 Apr 2023 10:31
Operator : CG/JU
Sample : PB152285BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK285

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

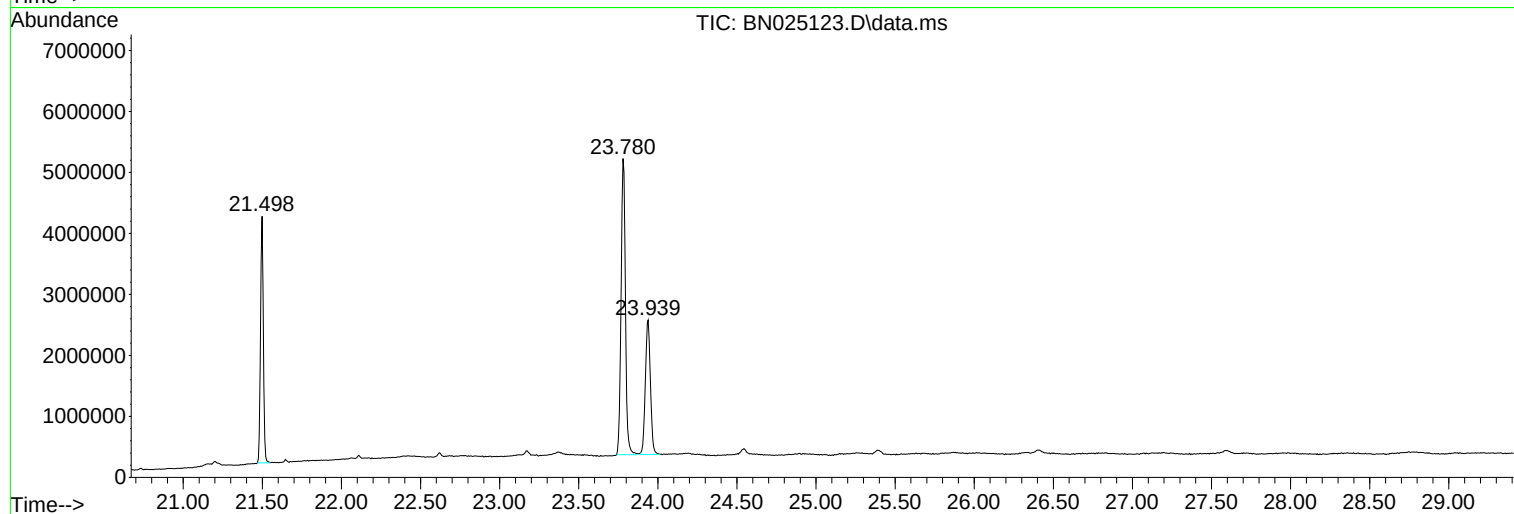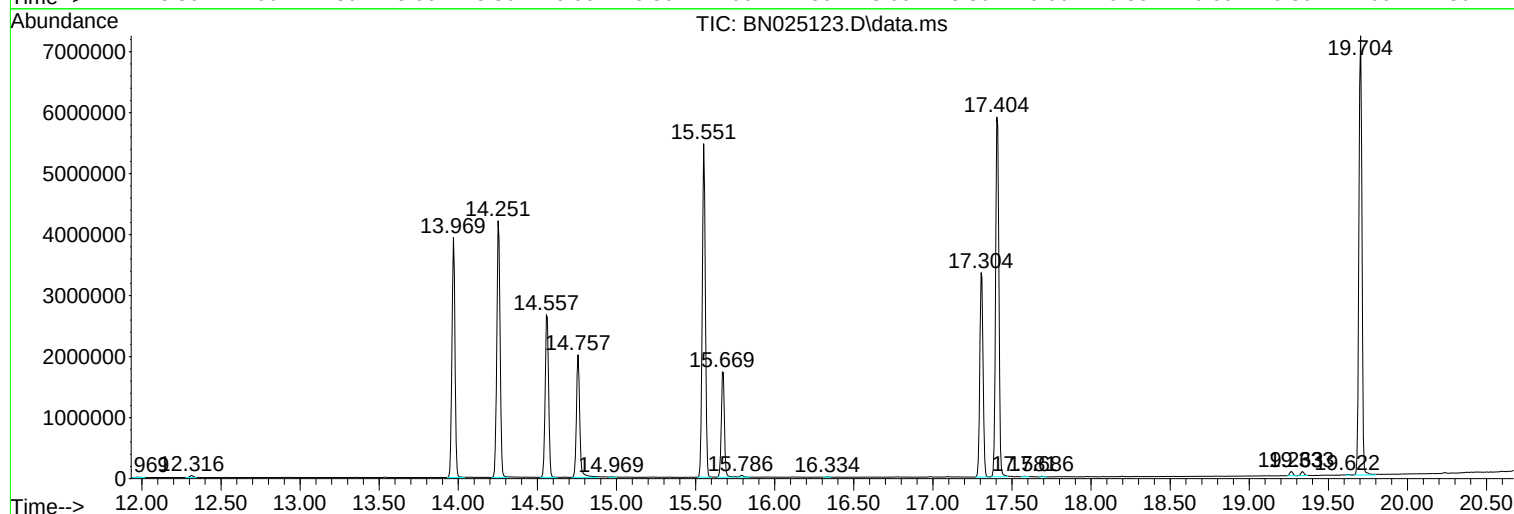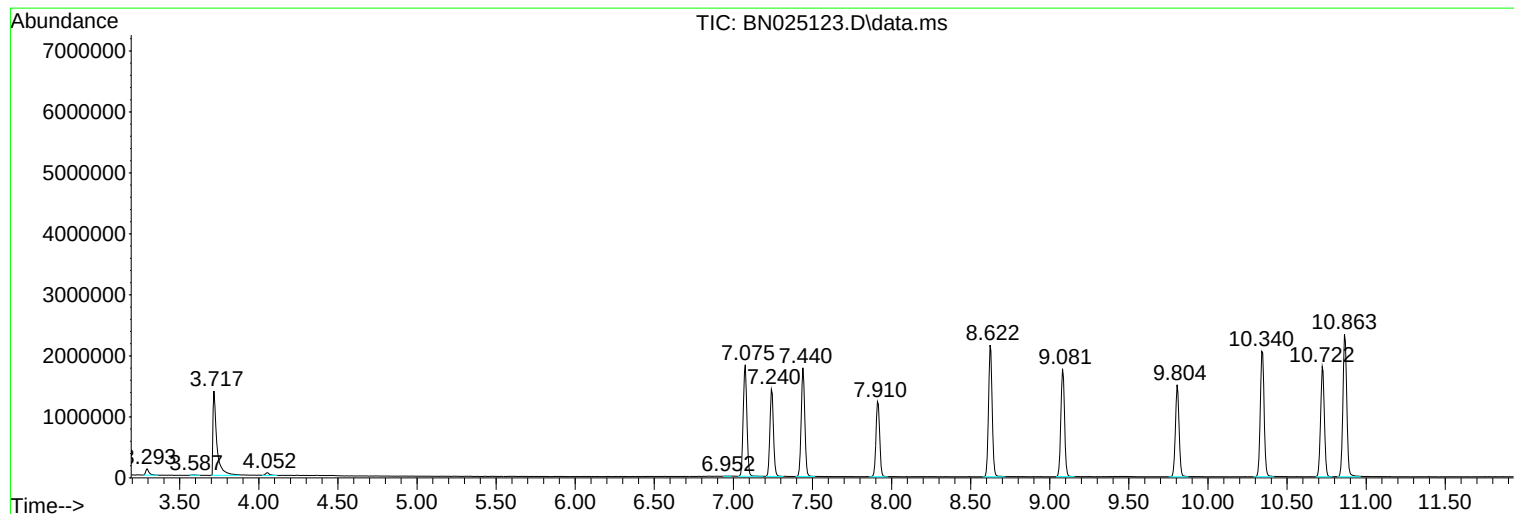

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042523\
Data File : BN025123.D
Acq On : 25 Apr 2023 10:31
Operator : CG/JU
Sample : PB152285BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK285

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042523\
Data File : BN025123.D
Acq On : 25 Apr 2023 10:31
Operator : CG/JU
Sample : PB152285BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK285

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc