
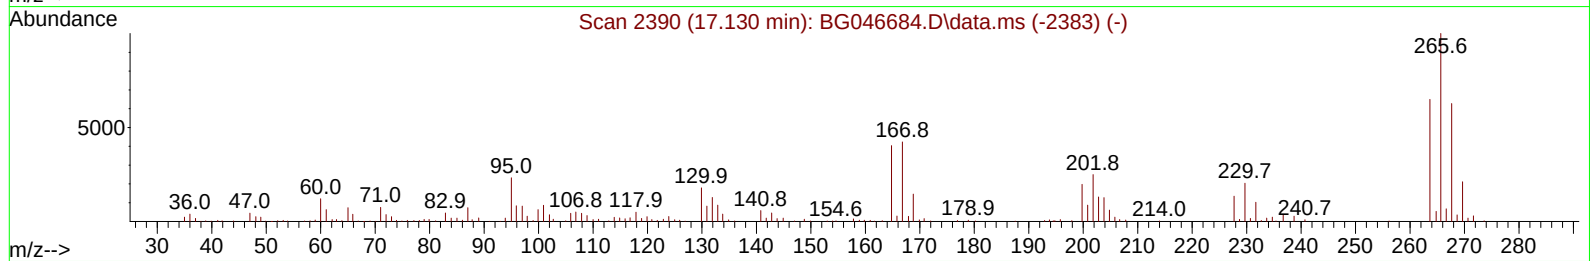
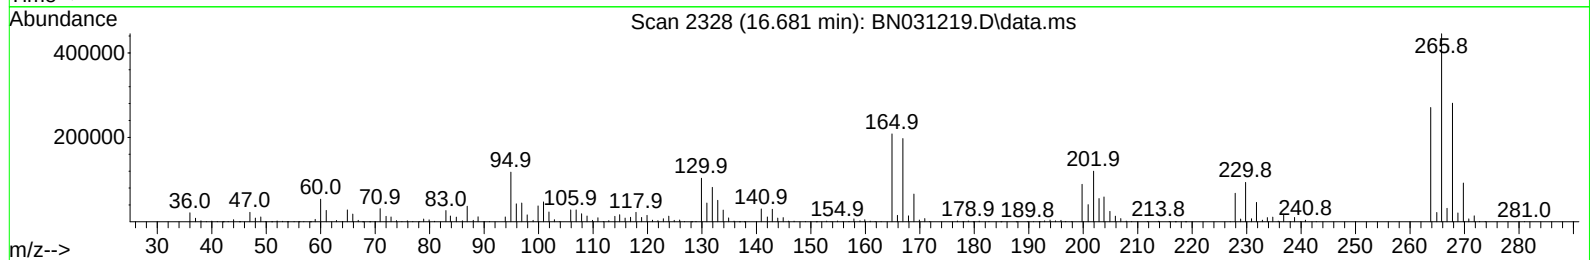


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042524\
Data File : BN031219.D
Acq On : 25 Apr 2024 13:49
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 25 15:56:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 17 01:56:21 2024
Response via : Initial Calibration

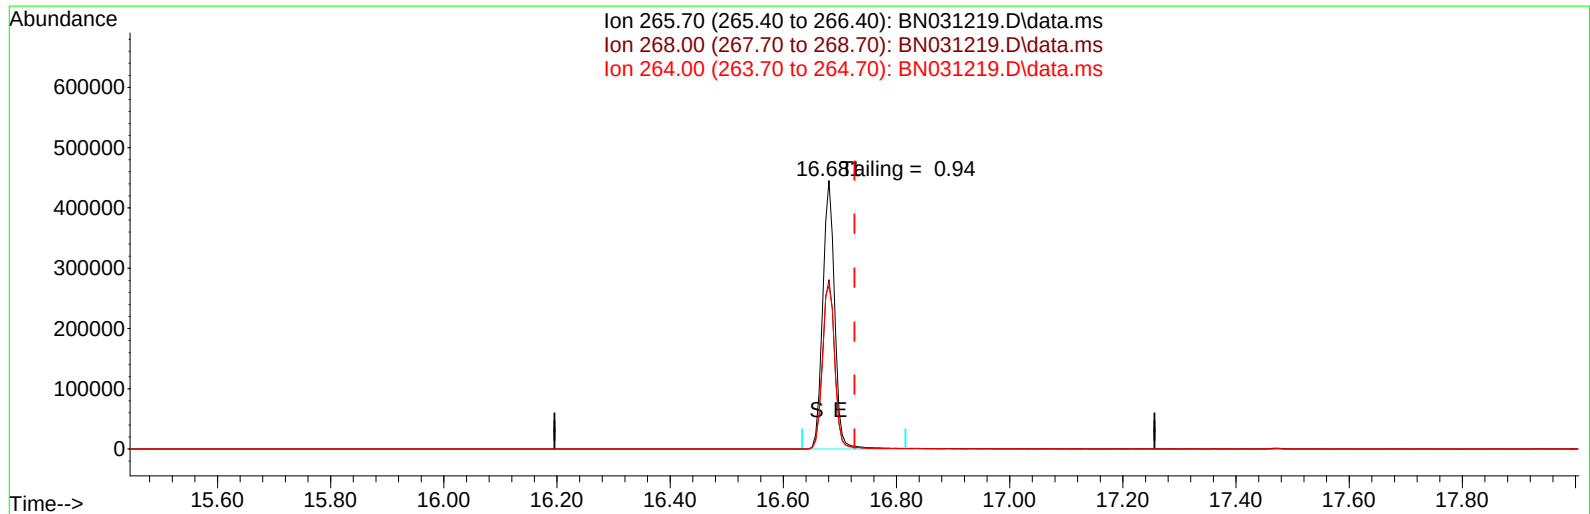

TIC: BN031219.D\data.ms

(70) Pentachlorophenol (C)




16.681min (-0.045) 27841.79 ng

response 655923

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.11
264.00	61.60	60.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042524\
Data File : BN031219.D
Acq On : 25 Apr 2024 13:49
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 25 15:56:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 17 01:56:21 2024
Response via : Initial Calibration

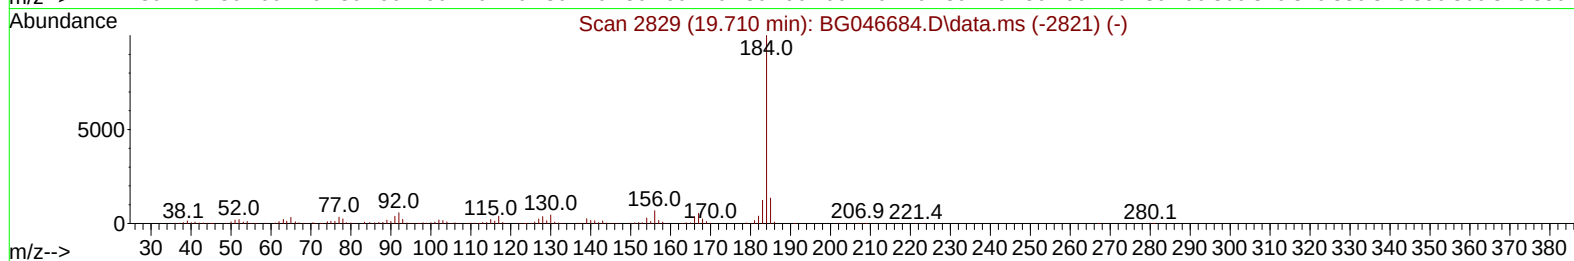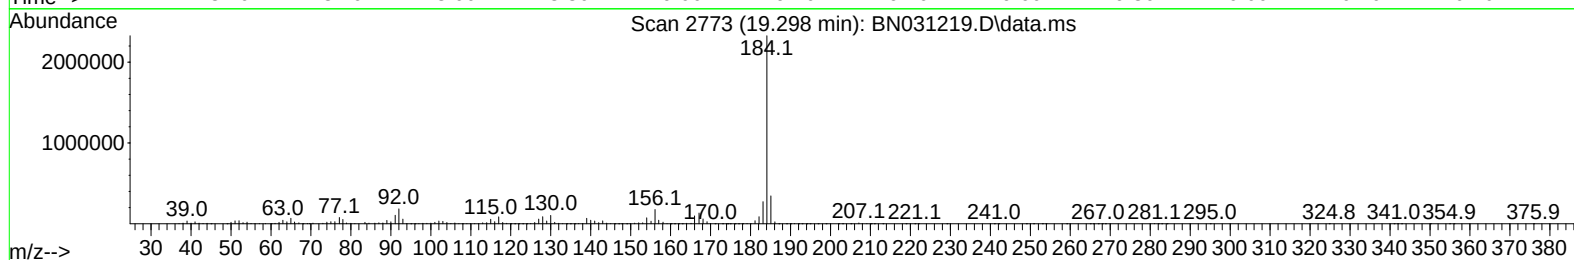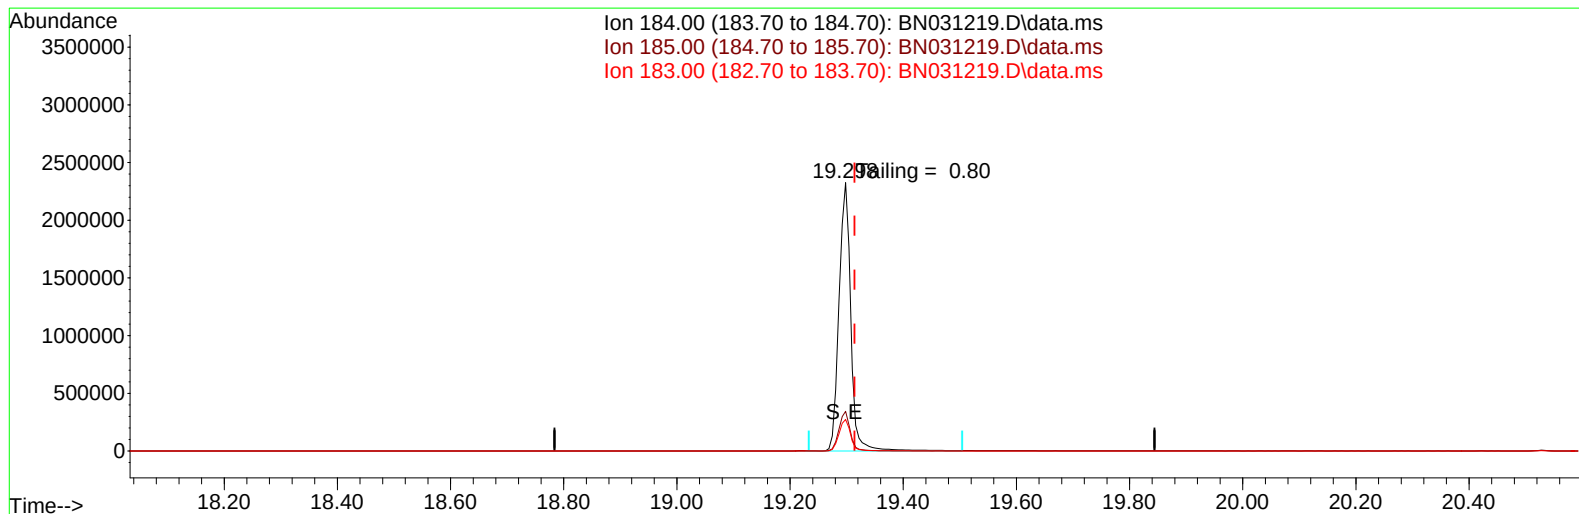

TIC: BN031219.D\data.ms

(77) Benzidine**19.298min (-0.016) 178353.69 ng****response 3370163**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.78
183.00	13.20	11.76
0.00	0.00	0.00