

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042524\
 Data File : BN031235.D
 Acq On : 26 Apr 2024 00:22
 Operator : MA/JU
 Sample : P2248-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RMW-03B-56-042324

Quant Time: Apr 26 00:50:28 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 25 18:00:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.624	152	6452	0.400	ng	0.00
7) Naphthalene-d8	10.400	136	20114	0.400	ng	#-0.01
13) Acenaphthene-d10	14.263	164	12188	0.400	ng	-0.01
19) Phenanthrene-d10	17.016	188	28993	0.400	ng	#-0.01
29) Chrysene-d12	21.220	240	23832	0.400	ng	#-0.02
35) Perylene-d12	23.434	264	22422	0.400	ng	#-0.02
System Monitoring Compounds						
4) 2-Fluorophenol	5.227	112	2416	0.168	ng	0.00
5) Phenol-d6	6.808	99	1817	0.104	ng	0.00
8) Nitrobenzene-d5	8.777	82	4504	0.324	ng	0.00
11) 2-Methylnaphthalene-d10	11.998	152	9470	0.306	ng	0.00
14) 2,4,6-Tribromophenol	15.775	330	2035	0.430	ng	0.00
15) 2-Fluorobiphenyl	12.884	172	14528	0.355	ng	-0.01
27) Fluoranthene-d10	19.058	212	27093	0.347	ng	0.00
31) Terphenyl-d14	19.667	244	20642	0.373	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.175	88	28045	3.536	ng	# 76
9) Naphthalene	10.453	128	3364	0.061	ng	# 90
34) Bis(2-ethylhexyl)phtha...	21.139	149	3347	0.088	ng	# 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042524\
Data File : BN031235.D
Acq On : 26 Apr 2024 00:22
Operator : MA/JU
Sample : P2248-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RMW-03B-56-042324


Quant Time: Apr 26 00:50:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 25 18:00:27 2024
Response via : Initial Calibration

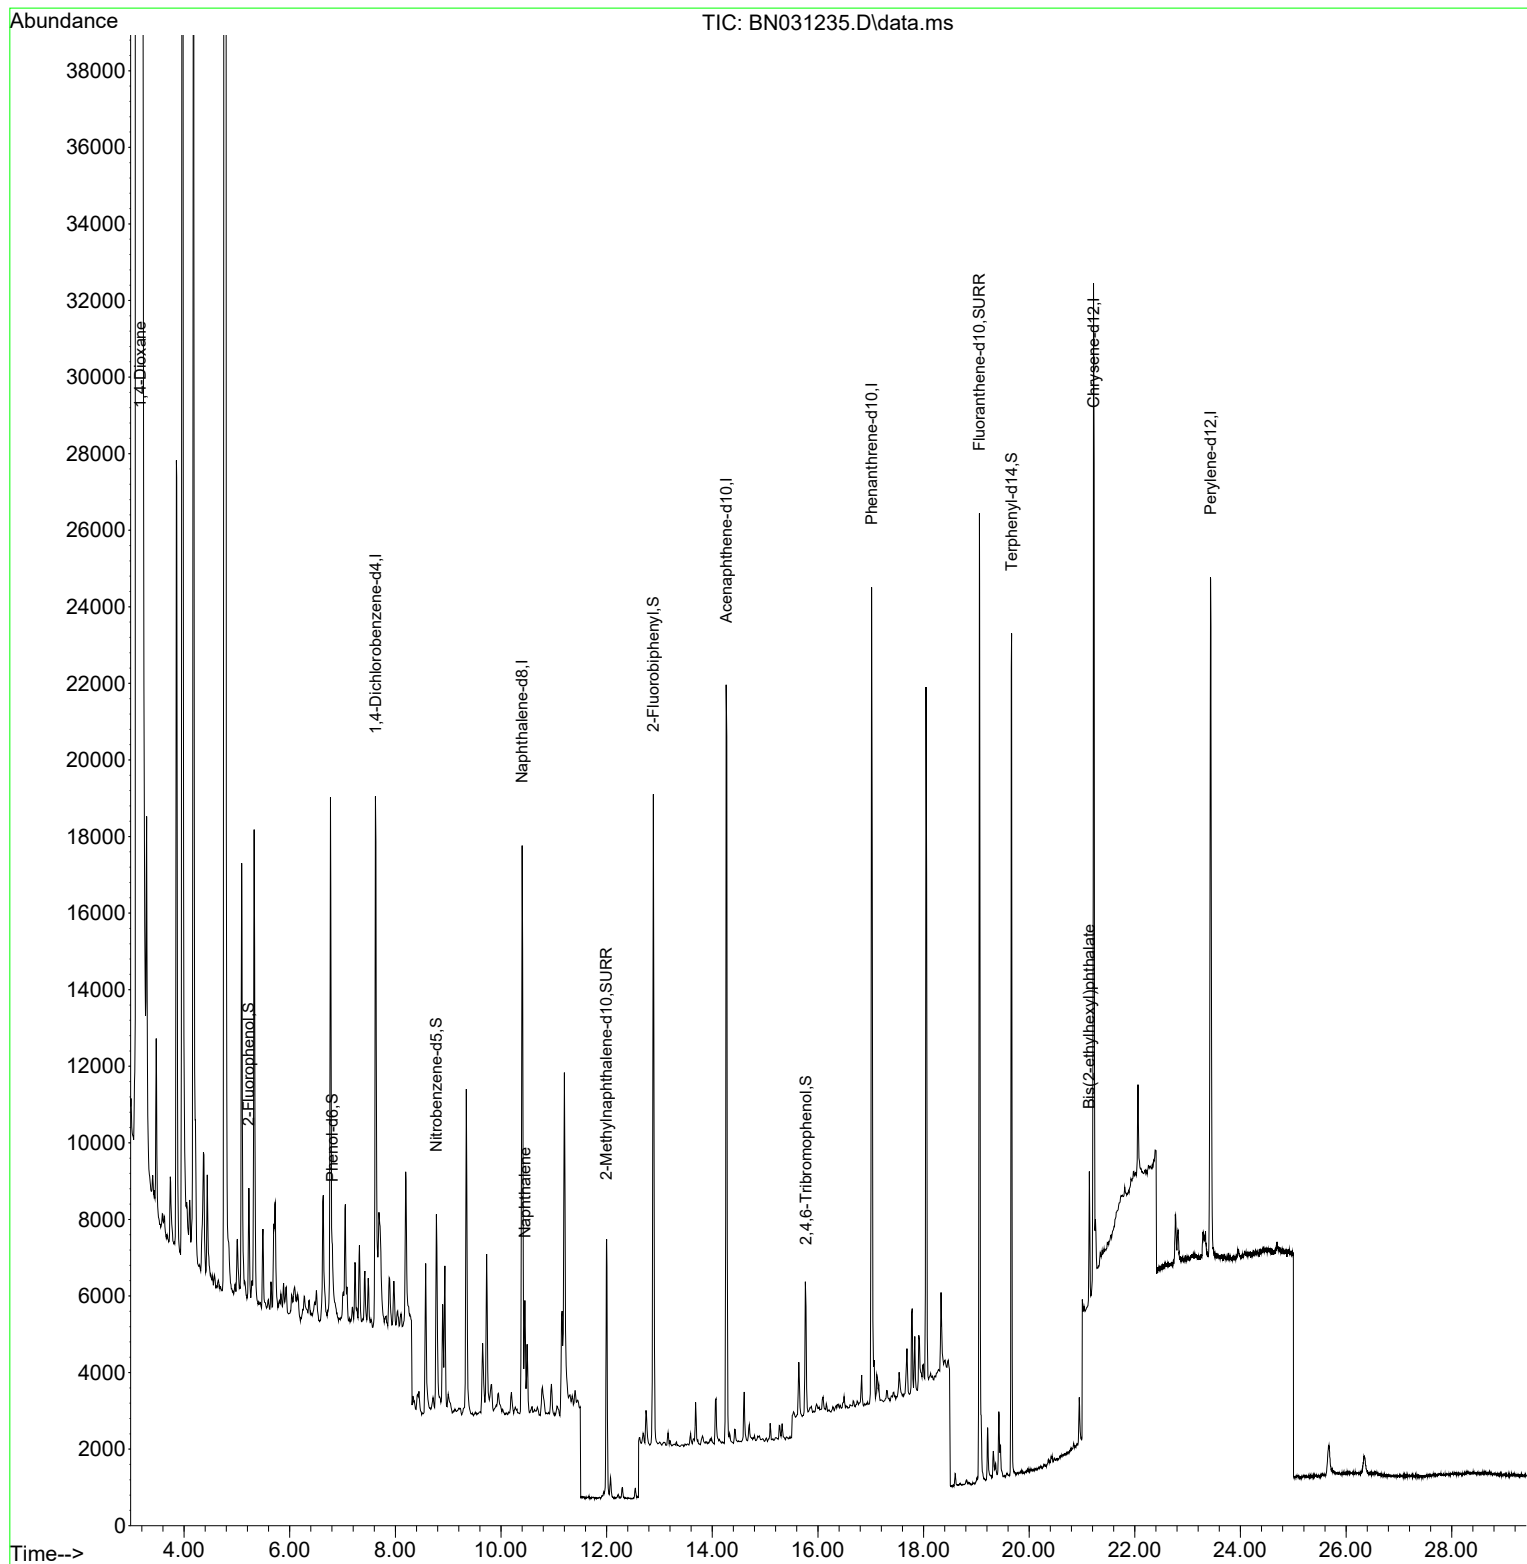






#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.624 min Scan# 64
 Delta R.T. 0.000 min
 Lab File: BN031235.D
 Acq: 26 Apr 2024 00:22

Instrument :
 BNA_N
 ClientSampleId :
 RMW-03B-56-042324







Tgt Ion:152 Resp: 6452
 Ion Ratio Lower Upper
 152 100
 150 155.3 121.7 182.5
 115 62.5 47.8 71.8

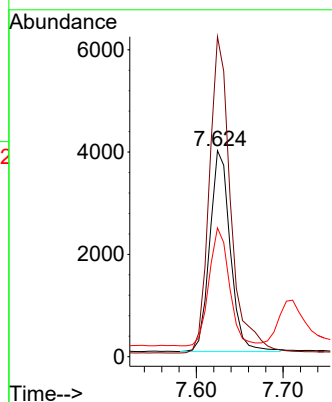

#2
 1,4-Dioxane
 Concen: 3.536 ng
 RT: 3.175 min Scan# 27
 Delta R.T. -0.000 min
 Lab File: BN031235.D
 Acq: 26 Apr 2024 00:22

Tgt Ion: 88 Resp: 28045
 Ion Ratio Lower Upper
 88 100
 43 65.4 23.7 35.5#
 58 64.4 55.7 83.5


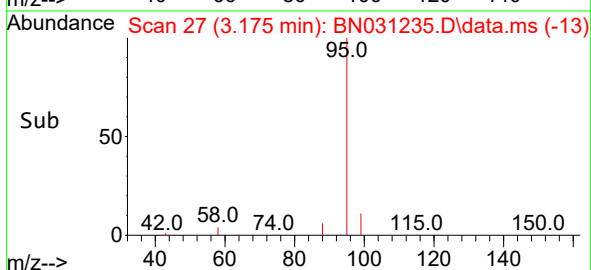
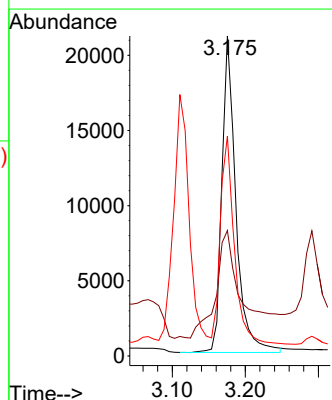





#4
2-Fluorophenol
Concen: 0.168 ng
RT: 5.227 min Scan# 311
Delta R.T. -0.000 min
Lab File: BN031235.D
Acq: 26 Apr 2024 00:22




Instrument :
BNA_N
ClientSampleId :
RMW-03B-56-042324


Tgt Ion:112 Resp: 2416
Ion Ratio Lower Upper
112 100
64 52.2 43.4 65.2
63 25.2 22.2 33.2

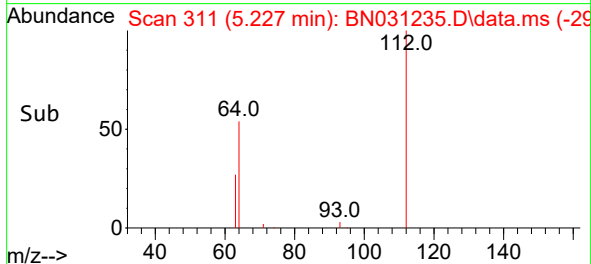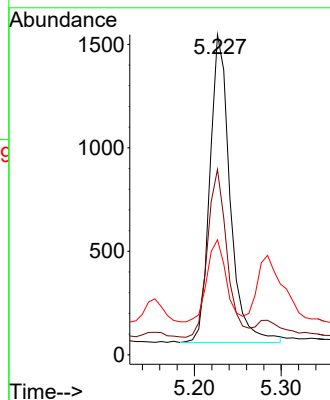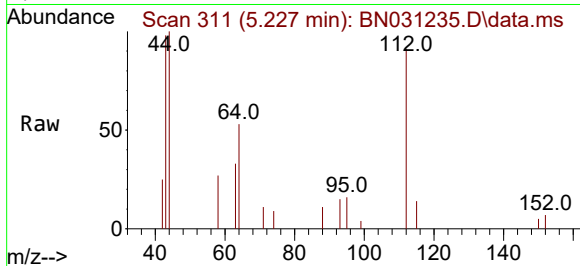

#5
Phenol-d6
Concen: 0.104 ng
RT: 6.808 min Scan# 530
Delta R.T. -0.000 min
Lab File: BN031235.D
Acq: 26 Apr 2024 00:22

Tgt Ion: 99 Resp: 1817
Ion Ratio Lower Upper
99 100
42 0.0 16.4 24.6#
71 31.8 26.3 39.5


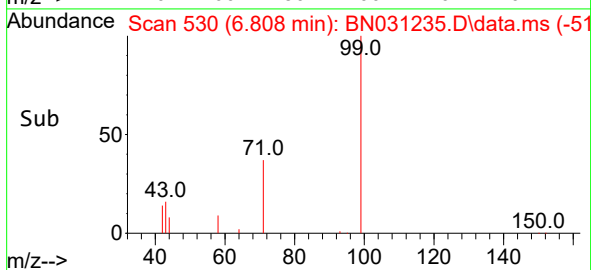
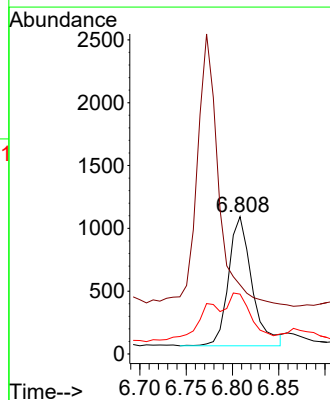
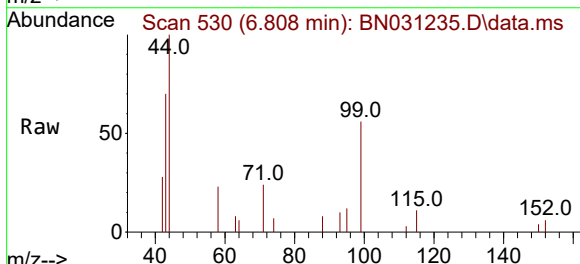




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.400 min Scan# 91
Delta R.T. -0.011 min
Lab File: BN031235.D
Acq: 26 Apr 2024 00:22




Instrument :
BNA_N
ClientSampleId :
RMW-03B-56-042324


Tgt Ion:	136	Resp:	20114
Ion Ratio	Lower	Upper	
136	100		
137	11.1	9.4	14.0
54	8.8	5.3	7.9#
68	7.8	4.7	7.1#

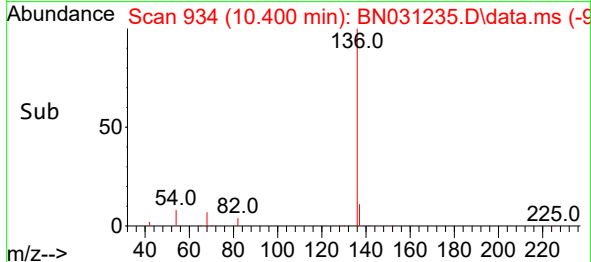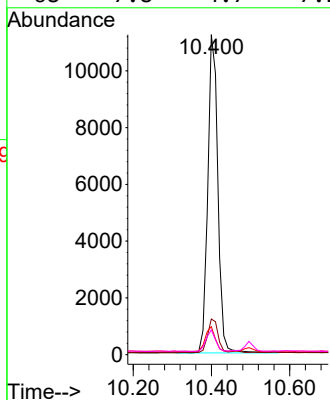

#8
Nitrobenzene-d5
Concen: 0.324 ng
RT: 8.777 min Scan# 782
Delta R.T. -0.000 min
Lab File: BN031235.D
Acq: 26 Apr 2024 00:22

Tgt Ion:	82	Resp:	4504
Ion Ratio	Lower	Upper	
82	100		
128	43.8	33.7	50.5
54	52.8	43.7	65.5

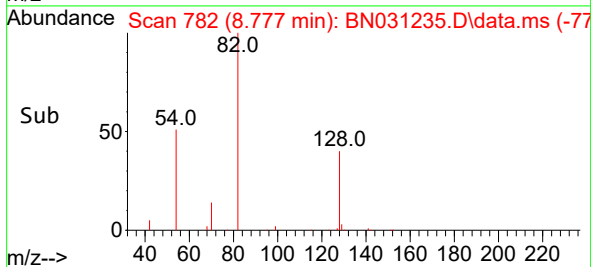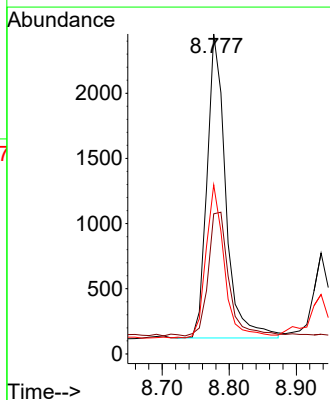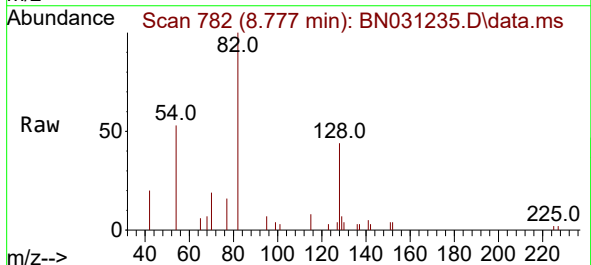



#9

Naphthalene

Concen: 0.061 ng

RT: 10.453 min Scan# 91

Delta R.T. -0.000 min

Lab File: BN031235.D

Acq: 26 Apr 2024 00:22

Instrument :

BNA_N

ClientSampleId :

RMW-03B-56-042324





Tgt Ion:128 Resp: 3364

Ion Ratio Lower Upper

128 100

129 16.3 9.4 14.0#

127 16.9 10.9 16.3#

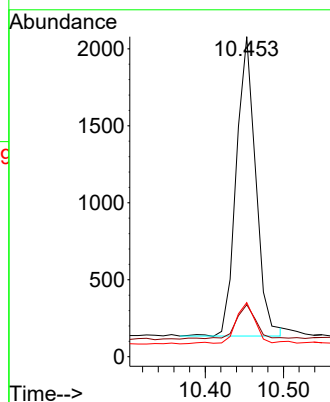

#11

2-Methylnaphthalene-d10

Concen: 0.306 ng

RT: 11.998 min Scan# 1167

Delta R.T. -0.004 min

Lab File: BN031235.D




Acq: 26 Apr 2024 00:22


Tgt Ion:152 Resp: 9470

Ion Ratio Lower Upper

152 100

151 20.3 16.7 25.1

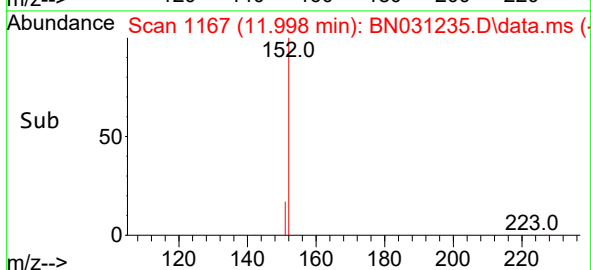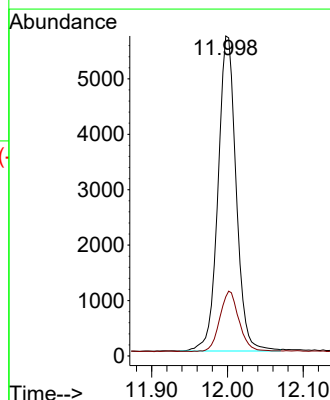



#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.263 min Scan# 14

Delta R.T. -0.011 min

Lab File: BN031235.D

Acq: 26 Apr 2024 00:22

Instrument :

BNA_N

ClientSampleId :

RMW-03B-56-042324





Tgt Ion:164 Resp: 12188

Ion Ratio Lower Upper

164 100

162 105.8 80.6 121.0

160 49.8 40.7 61.1

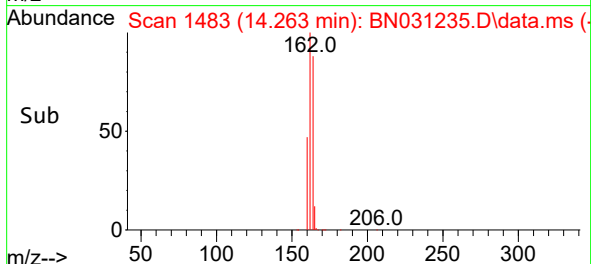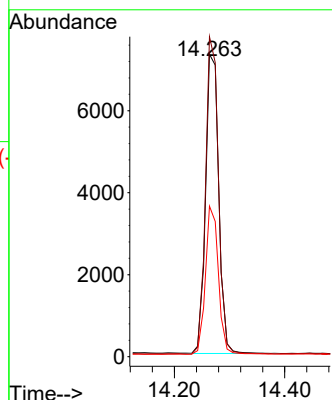

#14

2,4,6-Tribromophenol

Concen: 0.430 ng

RT: 15.775 min Scan# 1621

Delta R.T. -0.000 min

Lab File: BN031235.D

Acq: 26 Apr 2024 00:22




Tgt Ion:330 Resp: 2035


Ion Ratio Lower Upper

330 100

332 98.6 74.2 111.2

141 43.5 37.2 55.8


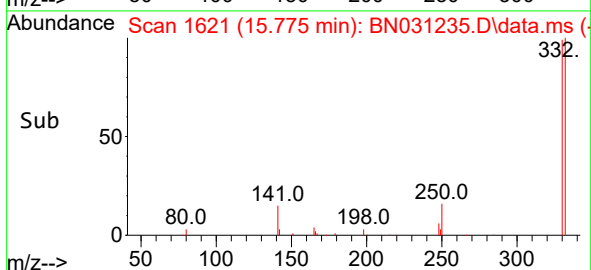
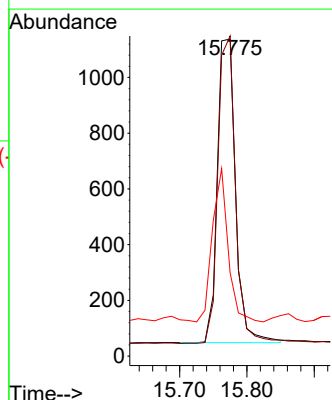



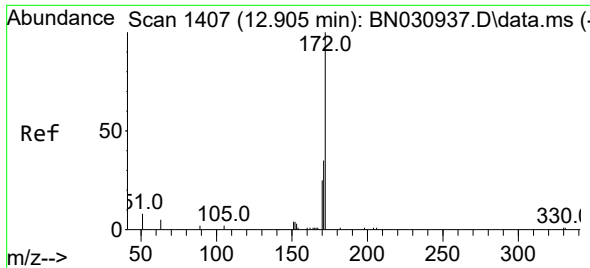

#15
2-Fluorobiphenyl
Concen: 0.355 ng
RT: 12.884 min Scan# 11
Delta R.T. -0.011 min
Lab File: BN031235.D
Acq: 26 Apr 2024 00:22




Instrument :
BNA_N
ClientSampleId :
RMW-03B-56-042324


Tgt Ion:172	Resp:	14528
Ion Ratio	Lower	Upper
172	100	
171	35.6	28.3 42.5
170	24.5	19.8 29.8

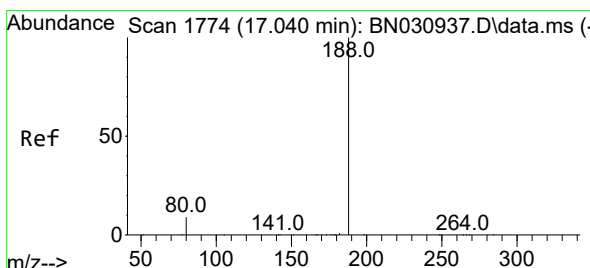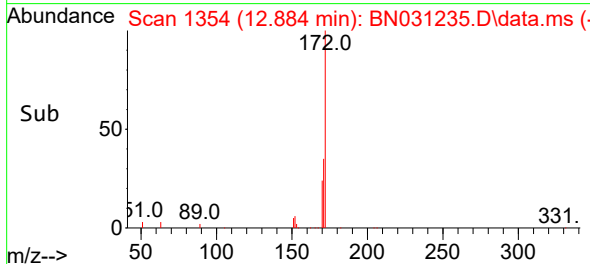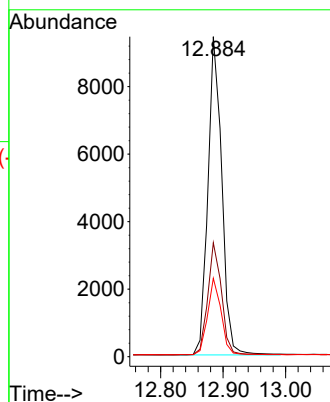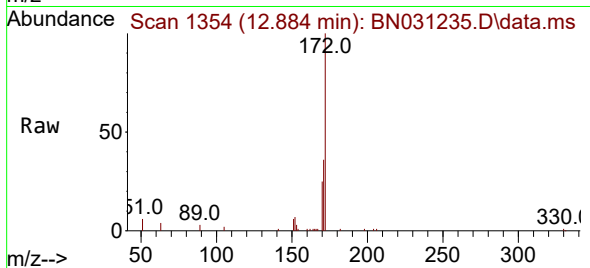

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.016 min Scan# 1721
Delta R.T. -0.013 min
Lab File: BN031235.D
Acq: 26 Apr 2024 00:22

Tgt Ion:188	Resp:	28993
Ion Ratio	Lower	Upper
188	100	
94	0.0	0.0 0.0
80	13.0	7.4 11.2#


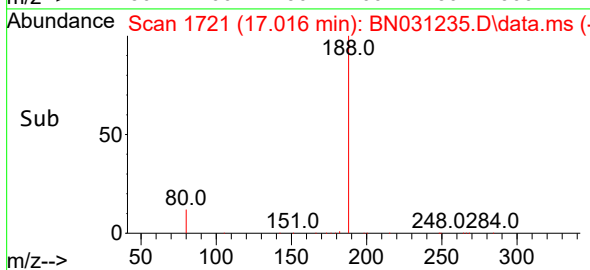
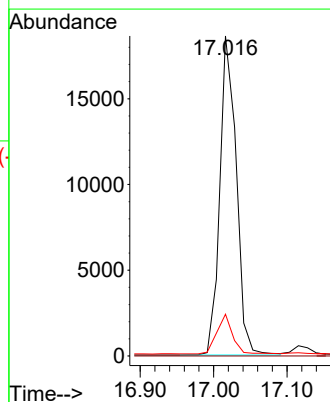
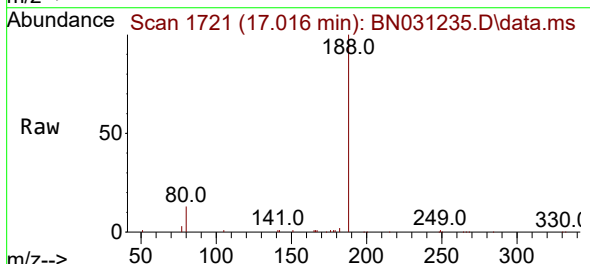


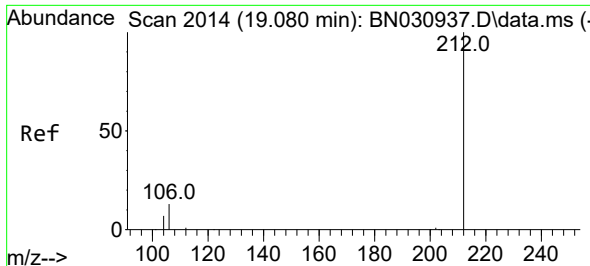

#27
Fluoranthene-d10
Concen: 0.347 ng
RT: 19.058 min Scan# 1906
Delta R.T. -0.009 min
Lab File: BN031235.D
Acq: 26 Apr 2024 00:22




Instrument :
BNA_N
ClientSampleId :
RMW-03B-56-042324


Tgt Ion:212 Resp: 27093
Ion Ratio Lower Upper
212 100
106 15.0 12.0 18.0
104 8.6 6.7 10.1

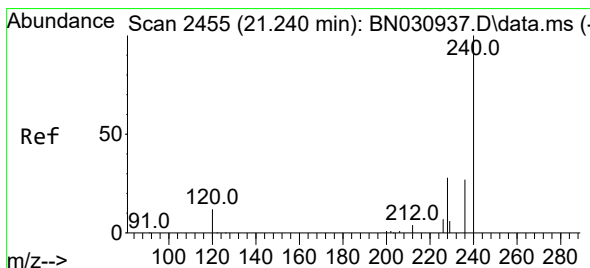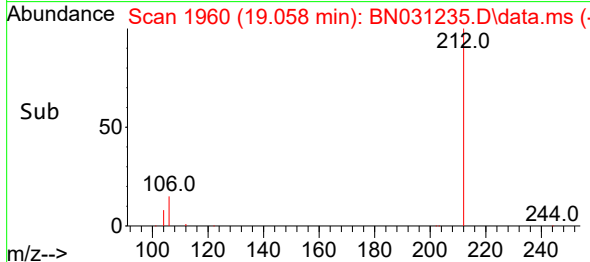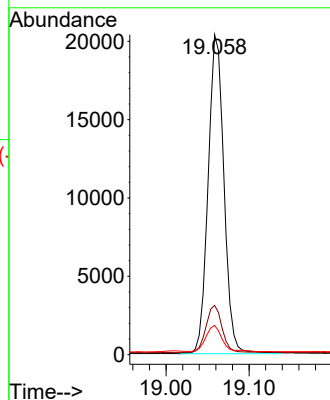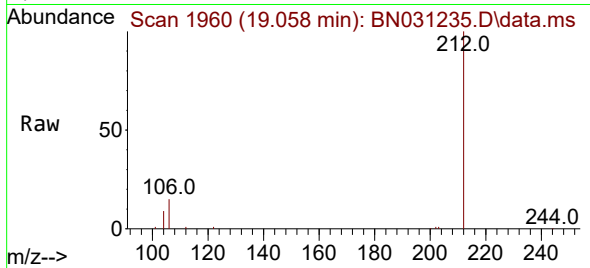

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.220 min Scan# 2403
Delta R.T. -0.018 min
Lab File: BN031235.D
Acq: 26 Apr 2024 00:22

Tgt Ion:240 Resp: 23832
Ion Ratio Lower Upper
240 100
120 17.4 11.0 16.4#
236 28.2 22.3 33.5


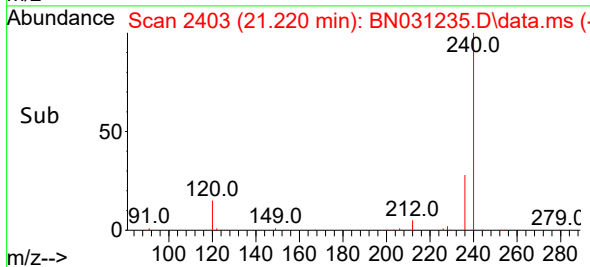
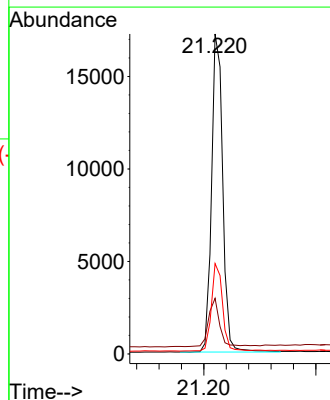
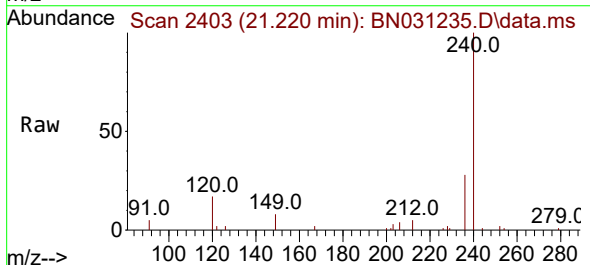




#31
 Terphenyl-d14
 Concen: 0.373 ng
 RT: 19.667 min Scan# 2091
 Delta R.T. -0.005 min
 Lab File: BN031235.D
 Acq: 26 Apr 2024 00:22




Instrument :
 BNA_N
 ClientSampleId :
 RMW-03B-56-042324


Tgt Ion:244 Resp: 20642
 Ion Ratio Lower Upper
 244 100
 212 8.5 7.2 10.8
 122 14.7 12.7 19.1

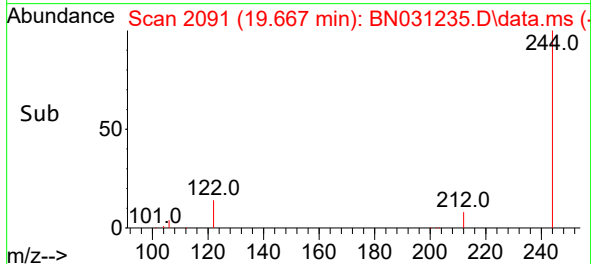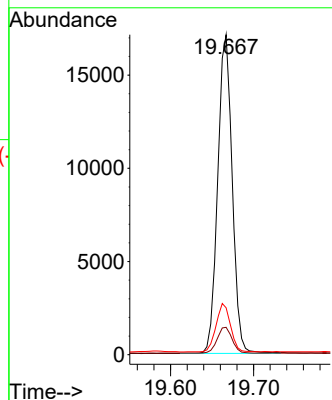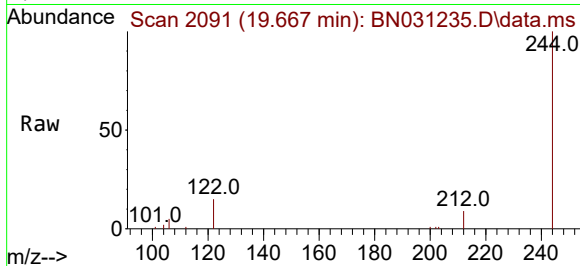

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.088 ng
 RT: 21.139 min Scan# 2394
 Delta R.T. -0.009 min
 Lab File: BN031235.D
 Acq: 26 Apr 2024 00:22


Tgt Ion:149 Resp: 3347
 Ion Ratio Lower Upper
 149 100
 167 27.3 21.0 31.4
 279 4.8 2.9 4.3#

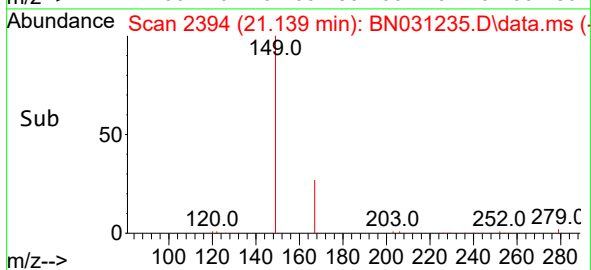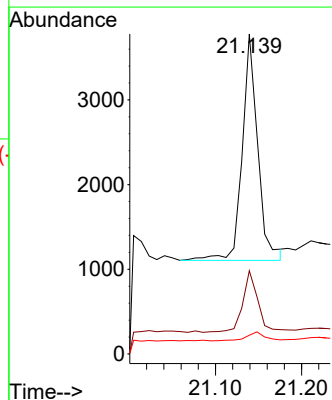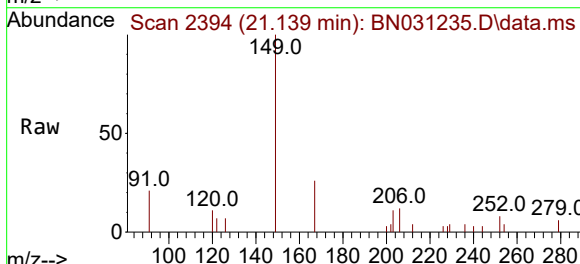

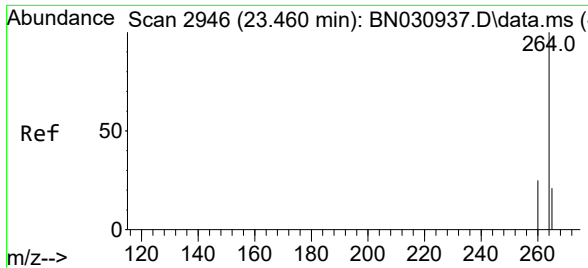

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.434 min Scan# 21
 Delta R.T. -0.021 min
 Lab File: BN031235.D
 Acq: 26 Apr 2024 00:22

Instrument :
 BNA_N
 ClientSampleId :
 RMW-03B-56-042324

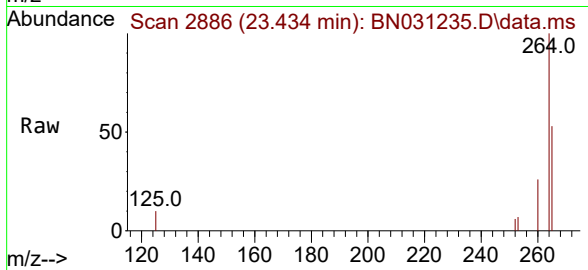

Tgt Ion:264 Resp: 22422
 Ion Ratio Lower Upper
 264 100
 260 26.1 20.6 31.0
 265 53.1 53.3 79.9#

