
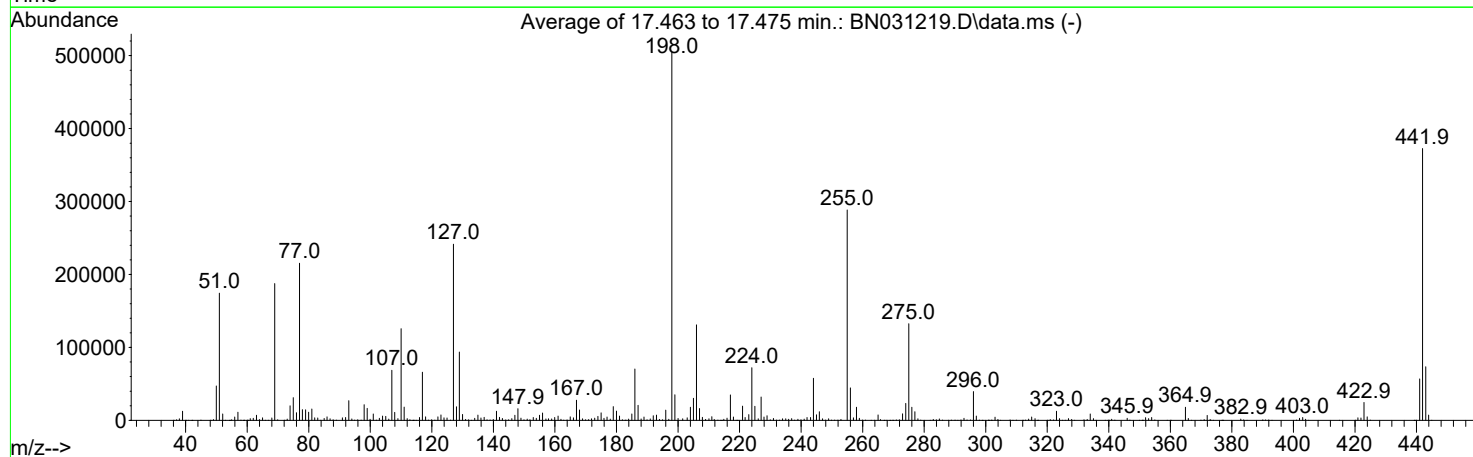


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042524\
Data File : BN031219.D
Acq On : 25 Apr 2024 13:49
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041524.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Apr 25 18:00:27 2024

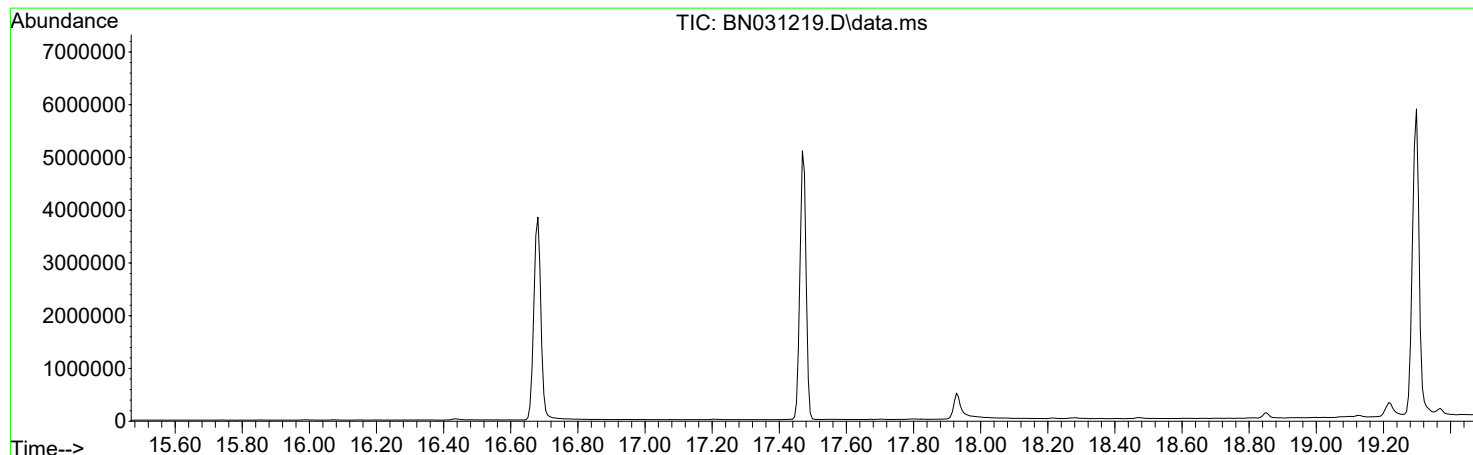

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.6	174443	PASS
68	69	0.00	2	1.8	3317	PASS
69	198	0.00	100	37.2	187503	PASS
70	69	0.00	2	0.5	865	PASS
127	198	10	80	47.9	241493	PASS
197	198	0.00	2	0.3	1472	PASS
198	198	100	100	100.0	504277	PASS
199	198	5	9	6.9	35032	PASS
275	198	10	60	26.3	132389	PASS
365	198	1	100	3.6	18073	PASS
441	198	0.01	100	11.3	56821	PASS
442	442	50	100	100.0	372736	PASS
443	442	15	24	19.7	73469	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/25/2024	BNA_N	<u>BN031219.D</u>
Compound Name	Response	Retention Time
DDT	1666834	20.528
DDD	42243	20.086
DDE	1562	19.575
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
43805	1710639	2.56

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042524\
Data File : BN031219.D
Acq On : 25 Apr 2024 13:49
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 25 15:56:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 17 01:56:21 2024
Response via : Initial Calibration

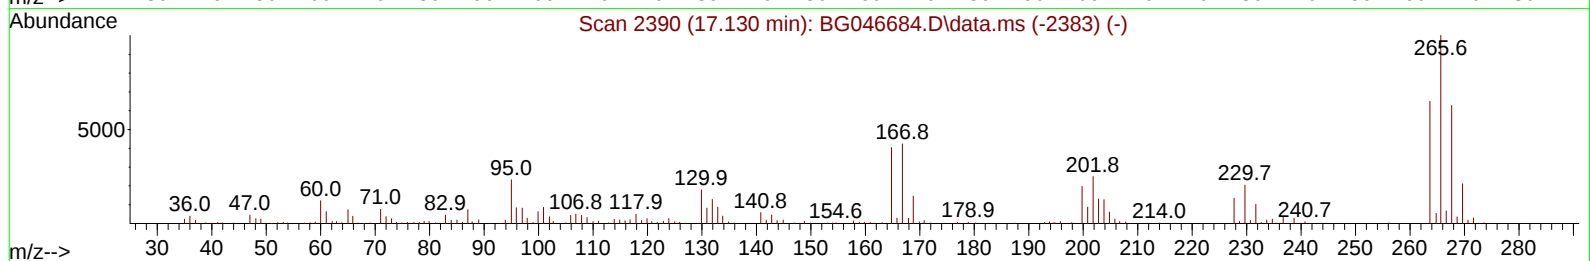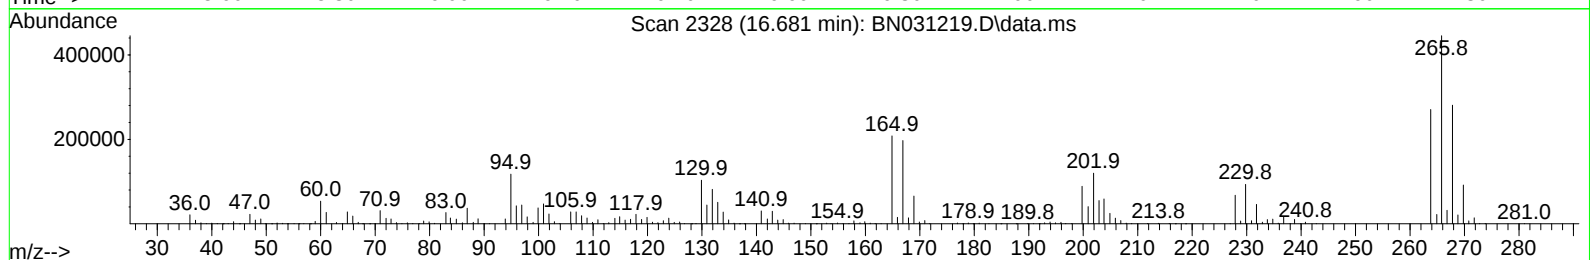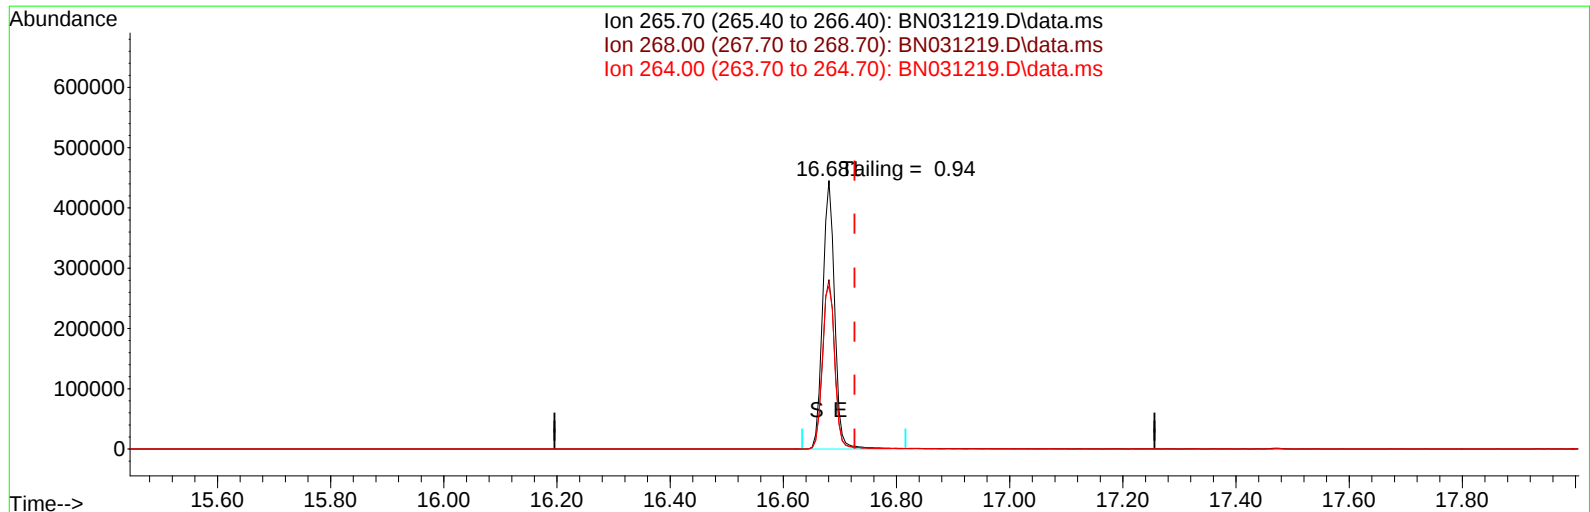

TIC: BN031219.D\data.ms

(70) Pentachlorophenol (C)

16.681min (-0.045) 27841.79 ng




response 655923

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.11
264.00	61.60	60.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042524\
Data File : BN031219.D
Acq On : 25 Apr 2024 13:49
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 25 15:56:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 17 01:56:21 2024
Response via : Initial Calibration

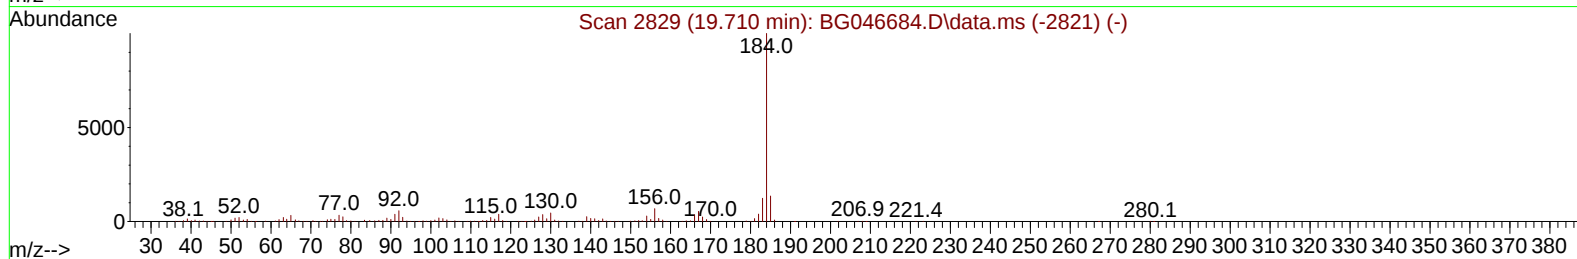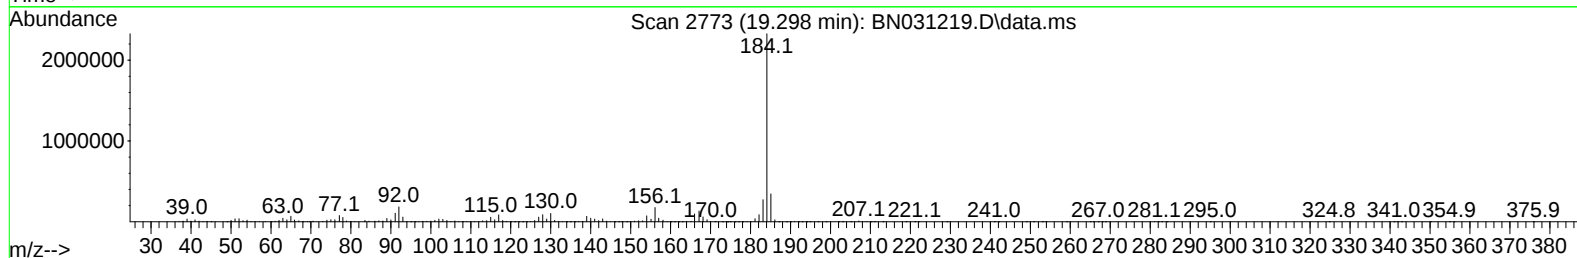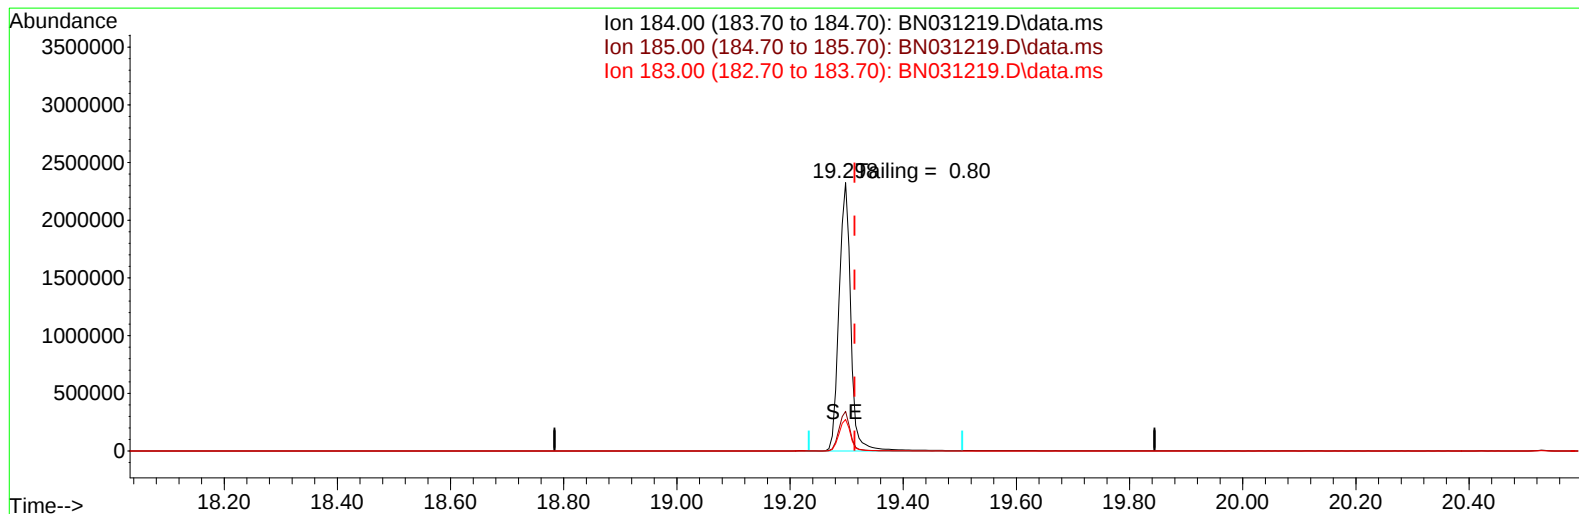

TIC: BN031219.D\data.ms

(77) Benzidine

19.298min (-0.016) 178353.69 ng

response 3370163

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.78
183.00	13.20	11.76
0.00	0.00	0.00