
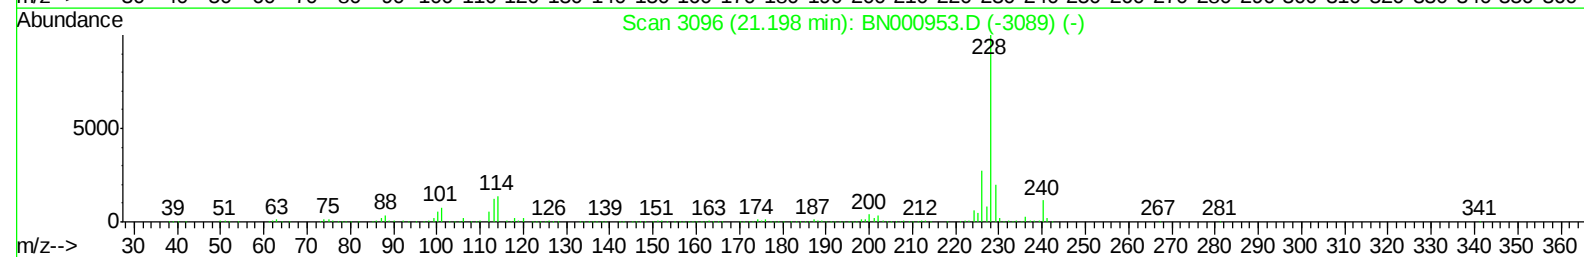
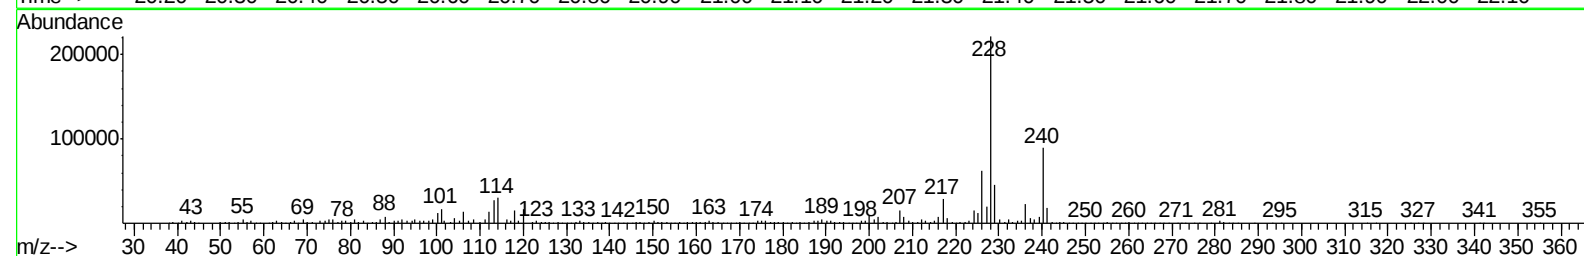


Data Path : Z:\HPCHEM1\BNA N\DATA\BN042618\
Data File : BN000956.D
Acq On : 27 Apr 2018 05:12
Operator : JU/SJ
Sample : J2526-15
Misc :
ALS Vial : 28 Sample Multiplier: 1

Quant Time: Apr 27 09:26:24 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN042418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 27 09:25:35 2018
Response via : Initial Calibration

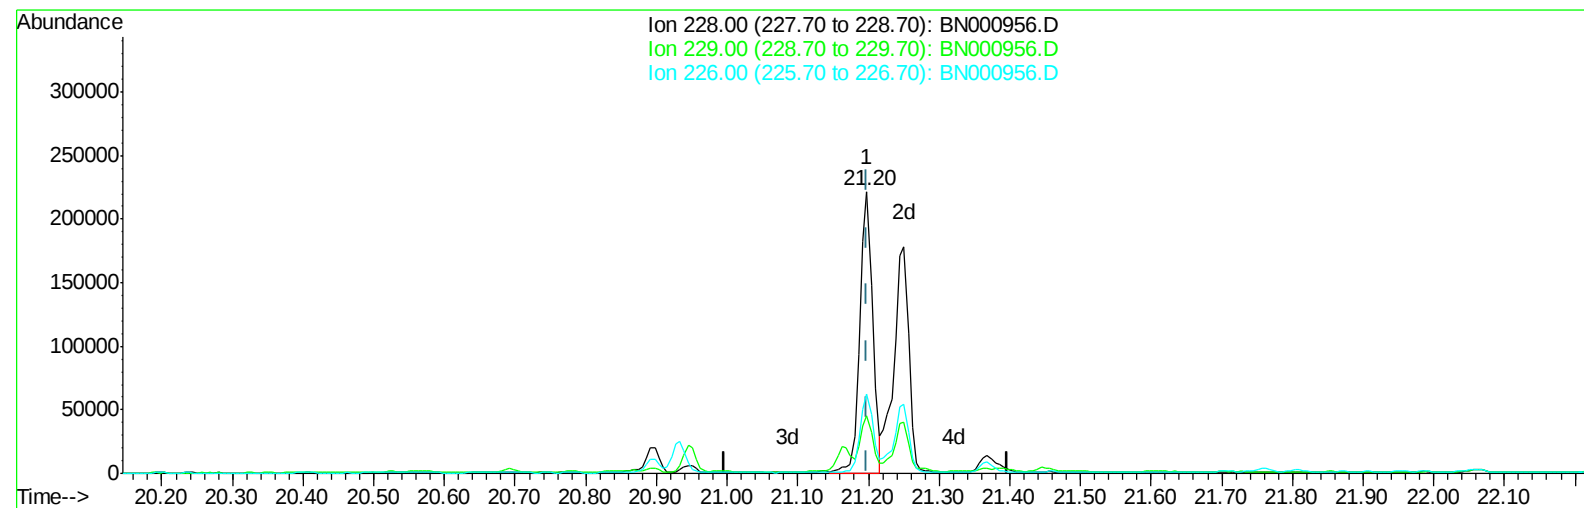

TIC: BN000956.D

(20) Benzo(a)anthracene

21.198min (-0.000) 9.18ng/ul m

response 278331

Ion	Exp%	Act%
228.00	100	100
229.00	19.60	20.61
226.00	26.40	28.08
0.00	0.00	0.00