

Data Path : Z:\HPCHEM1\BNA N\DATA\BN042618\
 Data File : BN000945.D
 Acq On : 26 Apr 2018 22:41
 Operator : JU/SJ
 Sample : J2526-17
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Apr 27 08:24:37 2018
 Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN042418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 27 08:22:19 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	159741	20.00	ng/ul	0.00
2) Naphthalene-d8	10.39	136	652931	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.26	164	304170	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.00	188	554454	20.00	ng/ul	0.00
17) Chrysene-d12	21.21	240	521745	20.00	ng/ul	0.00
22) Perylene-d12	23.41	264	548041	20.00	ng/ul	0.00
System Monitoring Compounds						
7) Acenaphthylene-d8	13.95	160	703302	24.08	ng/ul	0.00
10) Fluorene-d10	15.26	176	464966	23.85	ng/ul	0.00
14) Anthracene-d10	17.10	188	624344	24.62	ng/ul	0.00
18) Pyrene-d10	19.41	212	641024	23.98	ng/ul	0.00
25) Benzo(a)pyrene-d12	23.27	264	703842	27.19	ng/ul	0.00
Target Compounds				Ovalue		
16) Fluoranthene	19.07	202	32178	1.049	ng/ul#	93
24) Benzo(k)fluoranthene	22.76	252	37708	1.237	ng/ul#	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA N\DATA\BN042618\
Data File : BN000945.D
Acq On : 26 Apr 2018 22:41
Operator : JU/SJ
Sample : J2526-17
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Apr 27 08:24:37 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN042418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 27 08:22:19 2018
Response via : Initial Calibration




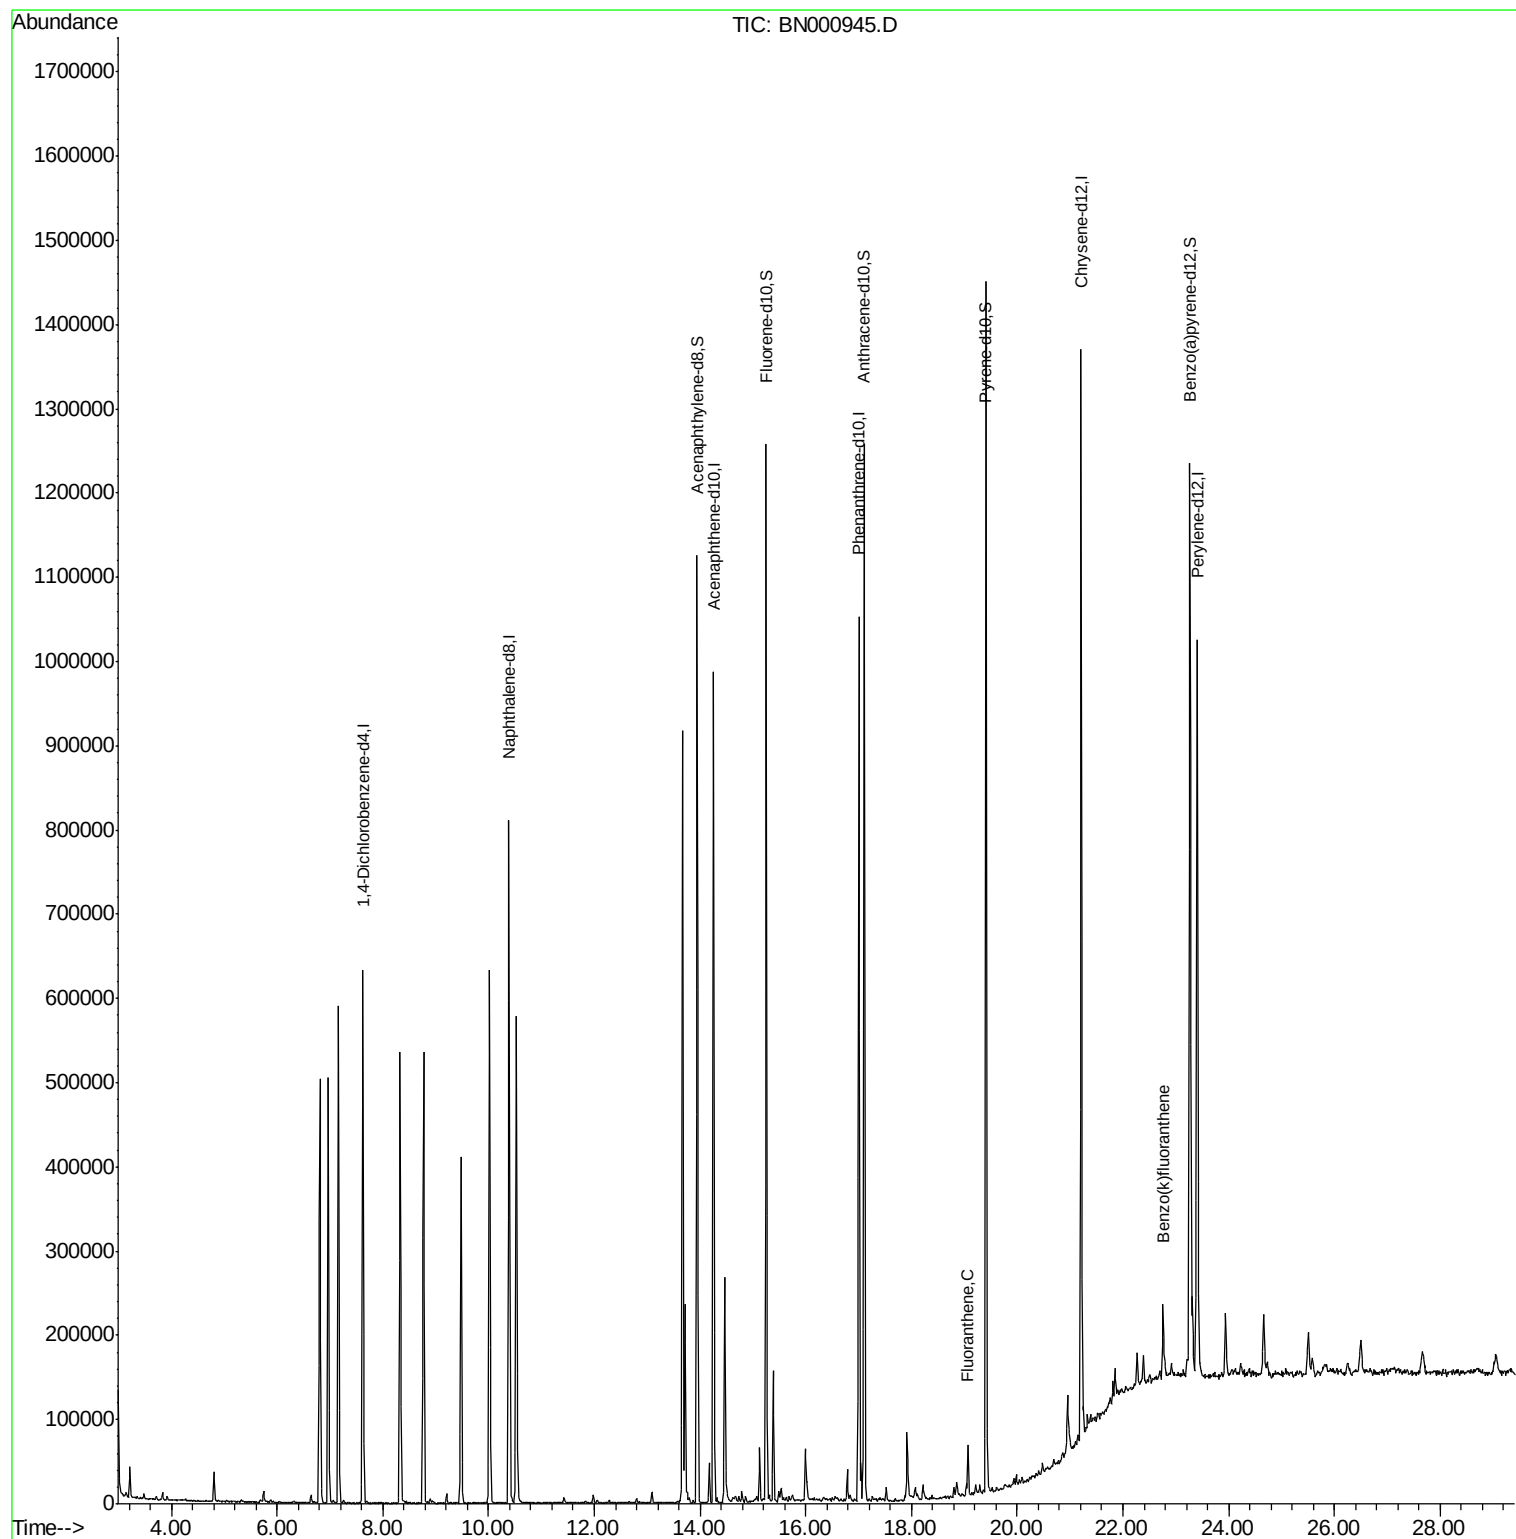


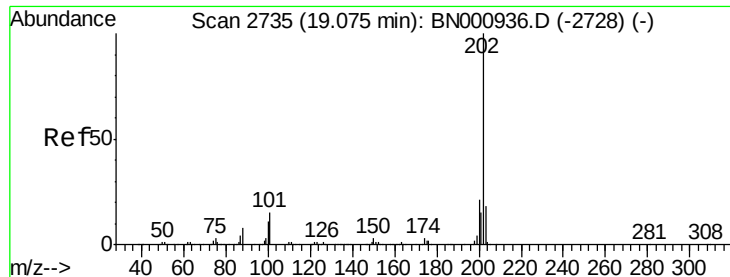

#16
Fluoranthene
Concen: 1.049 ng/ul
RT: 19.07 min Scan# 2734
Delta R.T. -0.01 min
Lab File: BN000945.D
Acq: 26 Apr 2018 22:41

Instrument :
BNA_N
ClientSampleId :

Tot Ion:202 Resp: 32178
Ion Ratio Lower Upper
202 100
101 15.3 9.9 14.9#
100 11.4 7.4 11.0#

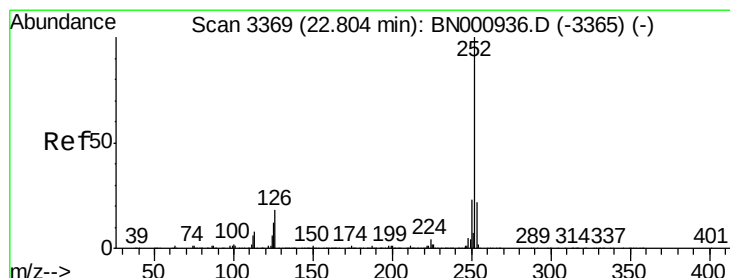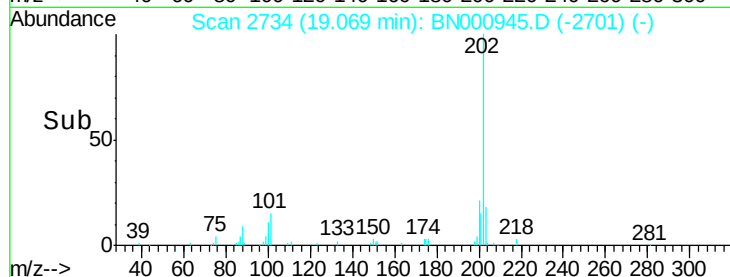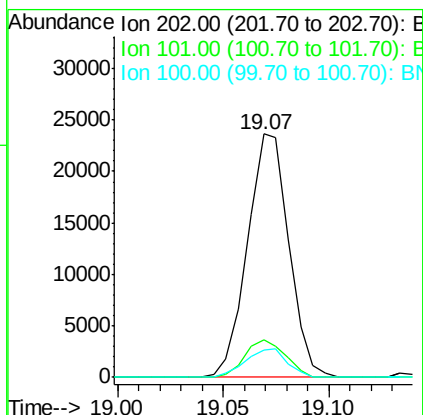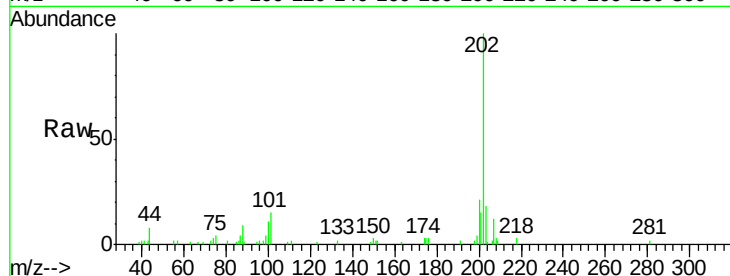

#24
Benzo(k)fluoranthene
Concen: 1.237 ng/ul
RT: 22.76 min Scan# 3361
Delta R.T. -0.05 min
Lab File: BN000945.D
Acq: 26 Apr 2018 22:41

Tgt Ion:252 Resp: 37708
Ion Ratio Lower Upper
252 100
253 23.8 18.0 27.0
125 17.7 8.1 12.1#

