

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042619\
 Data File : BN005324.D
 Acq On : 26 Apr 2019 19:54
 Operator : JU/SJ
 Sample : K2497-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GAHX9

Quant Time: Apr 26 23:32:25 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 26 23:25:31 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	462384	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	1943814	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	1187629	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.98	188	2798560	20.00	ng/ul	0.00
77) Chrysene-d12	21.21	240	2454783	20.00	ng/ul	0.00
85) Perylene-d12	23.40	264	2245365	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	46692	4.88	ng/uL	0.00
5) Phenol-d5	6.78	99	1106153	30.46	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	613788	27.09	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	807495	29.05	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	914002	32.20	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	422571	35.32	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	491881	40.55	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	896350	32.24	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	899676	31.38	ng/ul	0.00
43) Dimethylphthalate-d6	13.65	166	3293380	38.20	ng/ul	0.00
46) Acenaphthylene-d8	13.92	160	3901226	36.84	ng/ul	0.00
51) 4-Nitrophenol-d4	14.43	143	574549	42.21	ng/ul	0.00
57) Fluorene-d10	15.23	176	2835018	39.18	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.35	200	473138	37.59	ng/ul	0.00
70) Anthracene-d10	17.08	188	4702103	40.08	ng/ul	0.00
78) Pyrene-d10	19.39	212	5207564	41.47	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.27	264	4093719	41.72	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	13.69	163	687319	8.001	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042619\
Data File : BN005324.D
Acq On : 26 Apr 2019 19:54
Operator : JU/SJ
Sample : K2497-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GAHX9

Quant Time: Apr 26 23:32:25 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 26 23:25:31 2019
Response via : Initial Calibration

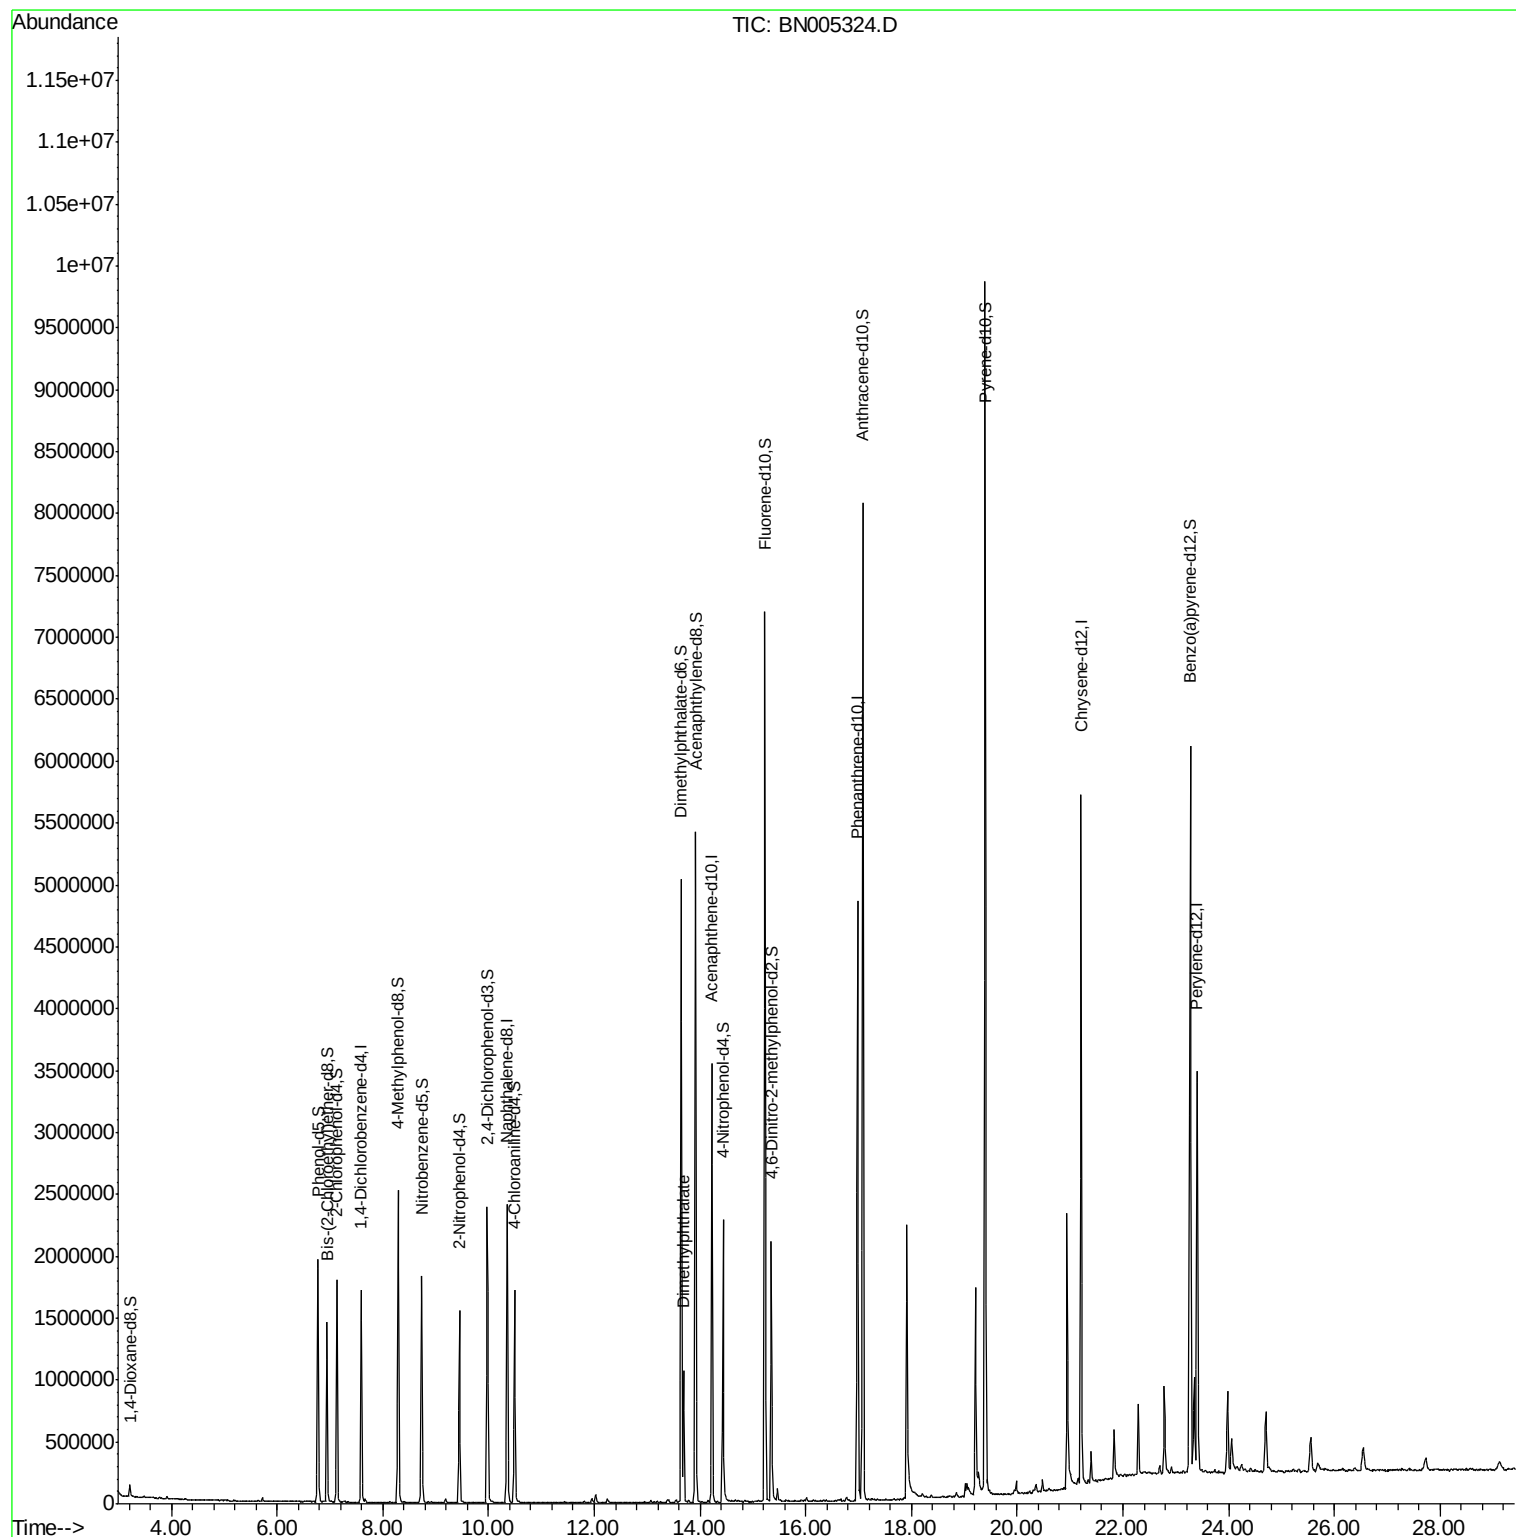

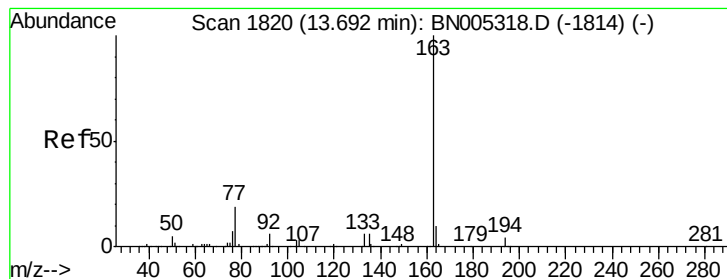

#44

Dimethylphthalate

Concen: 8.001 ng/ul

RT: 13.69 min Scan# 1820

Delta R.T. 0.00 min

Lab File: BN005324.D

Acq: 26 Apr 2019 19:54

Instrument :

BNA_N

ClientSampleId :

GAHX9


Tot Ion:163 Resp: 687319

Ion Ratio Lower Upper

163 100

194 4.5 3.4 5.0

164 9.6 8.1 12.1

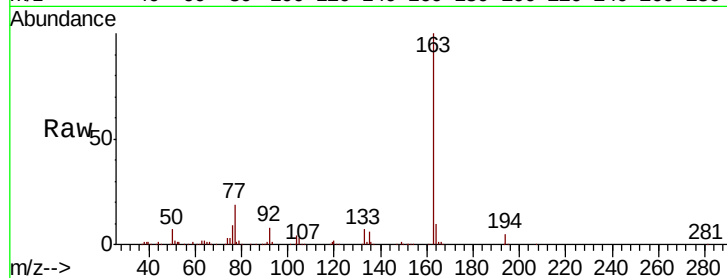

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

