

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042619\
 Data File : BN005345.D
 Acq On : 27 Apr 2019 08:00
 Operator : JU/SJ
 Sample : K2456-12DL 5X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GAHQ0DL

Manual Integrations
 APPROVED

Sohil
 4/29/2019 1:44:21 PM

Quant Time: Apr 29 04:14:51 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 25 03:19:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	531320	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	2200645	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	1262692	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.99	188	2771691	20.00	ng/ul	0.00
77) Chrysene-d12	21.22	240	1948793	20.00	ng/ul	0.00
85) Perylene-d12	23.43	264	2029908	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	6175	0.56	ng/uL	0.00
5) Phenol-d5	6.78	99	134020	3.21	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	82252	3.16	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	112357	3.52	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	110909	3.40	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	57683	4.26	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	60589	4.41	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	112736	3.58	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	49313m	1.52	ng/ul	0.00
43) Dimethylphthalate-d6	13.65	166	345692	3.77	ng/ul	0.00
46) Acenaphthylene-d8	13.92	160	426192	3.79	ng/ul	0.00
51) 4-Nitrophenol-d4	14.44	143	50171	3.47	ng/ul	0.00
57) Fluorene-d10	15.23	176	301250	3.92	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.36	200	16413	1.32	ng/ul	0.00
70) Anthracene-d10	17.08	188	469394	4.04	ng/ul	0.00
78) Pyrene-d10	19.40	212	445109	4.46	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.29	264	338304	3.81	ng/ul	-0.01

Target Compounds

					Qvalue	
34) 2-Methylnaphthalene	12.02	142	115094	1.536	ng/ul	97
44) Dimethylphthalate	13.69	163	98882	1.083	ng/ul#	93
47) Acenaphthylene	13.95	152	3369003	30.451	ng/ul	99
58) Fluorene	15.30	166	303473	3.576	ng/ul#	54
69) Phenanthrene	17.03	178	957547	7.094	ng/ul	98
71) Anthracene	17.12	178	2040732	14.841	ng/ul	99
76) Fluoranthene	19.06	202	2894320	19.331	ng/ul	99
79) Pyrene	19.43	202	7125453	56.787	ng/ul	97
82) Benzo(a)anthracene	21.20	228	3630572m	29.947	ng/ul	
84) Chrysene	21.26	228	3587485	31.884	ng/ul	96
87) Benzo(b)fluoranthene	22.78	252	3663535	32.106	ng/ul	98
88) Benzo(k)fluoranthene	22.82	252	1039393m	9.538	ng/ul	
90) Benzo(a)pyrene	23.34	252	3716818	34.654	ng/ul	98
91) Indeno(1,2,3-cd)pyrene	25.62	276	1751263	14.768	ng/ul	95
92) Dibenzo(a,h)anthracene	25.63	278	638867	6.348	ng/ul	93
93) Benzo(g,h,i)perylene	26.29	276	1449695	14.785	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042619\
Data File : BN005345.D
Acq On : 27 Apr 2019 08:00
Operator : JU/SJ
Sample : K2456-12DL 5X
Misc :
ALS Vial : 28 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleID :
GAHQ0DL

Manual Integrations
APPROVED

Sohil
4/29/2019 1:44:21 PM

Quant Time: Apr 29 04:14:51 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 25 03:19:34 2019
Response via : Initial Calibration

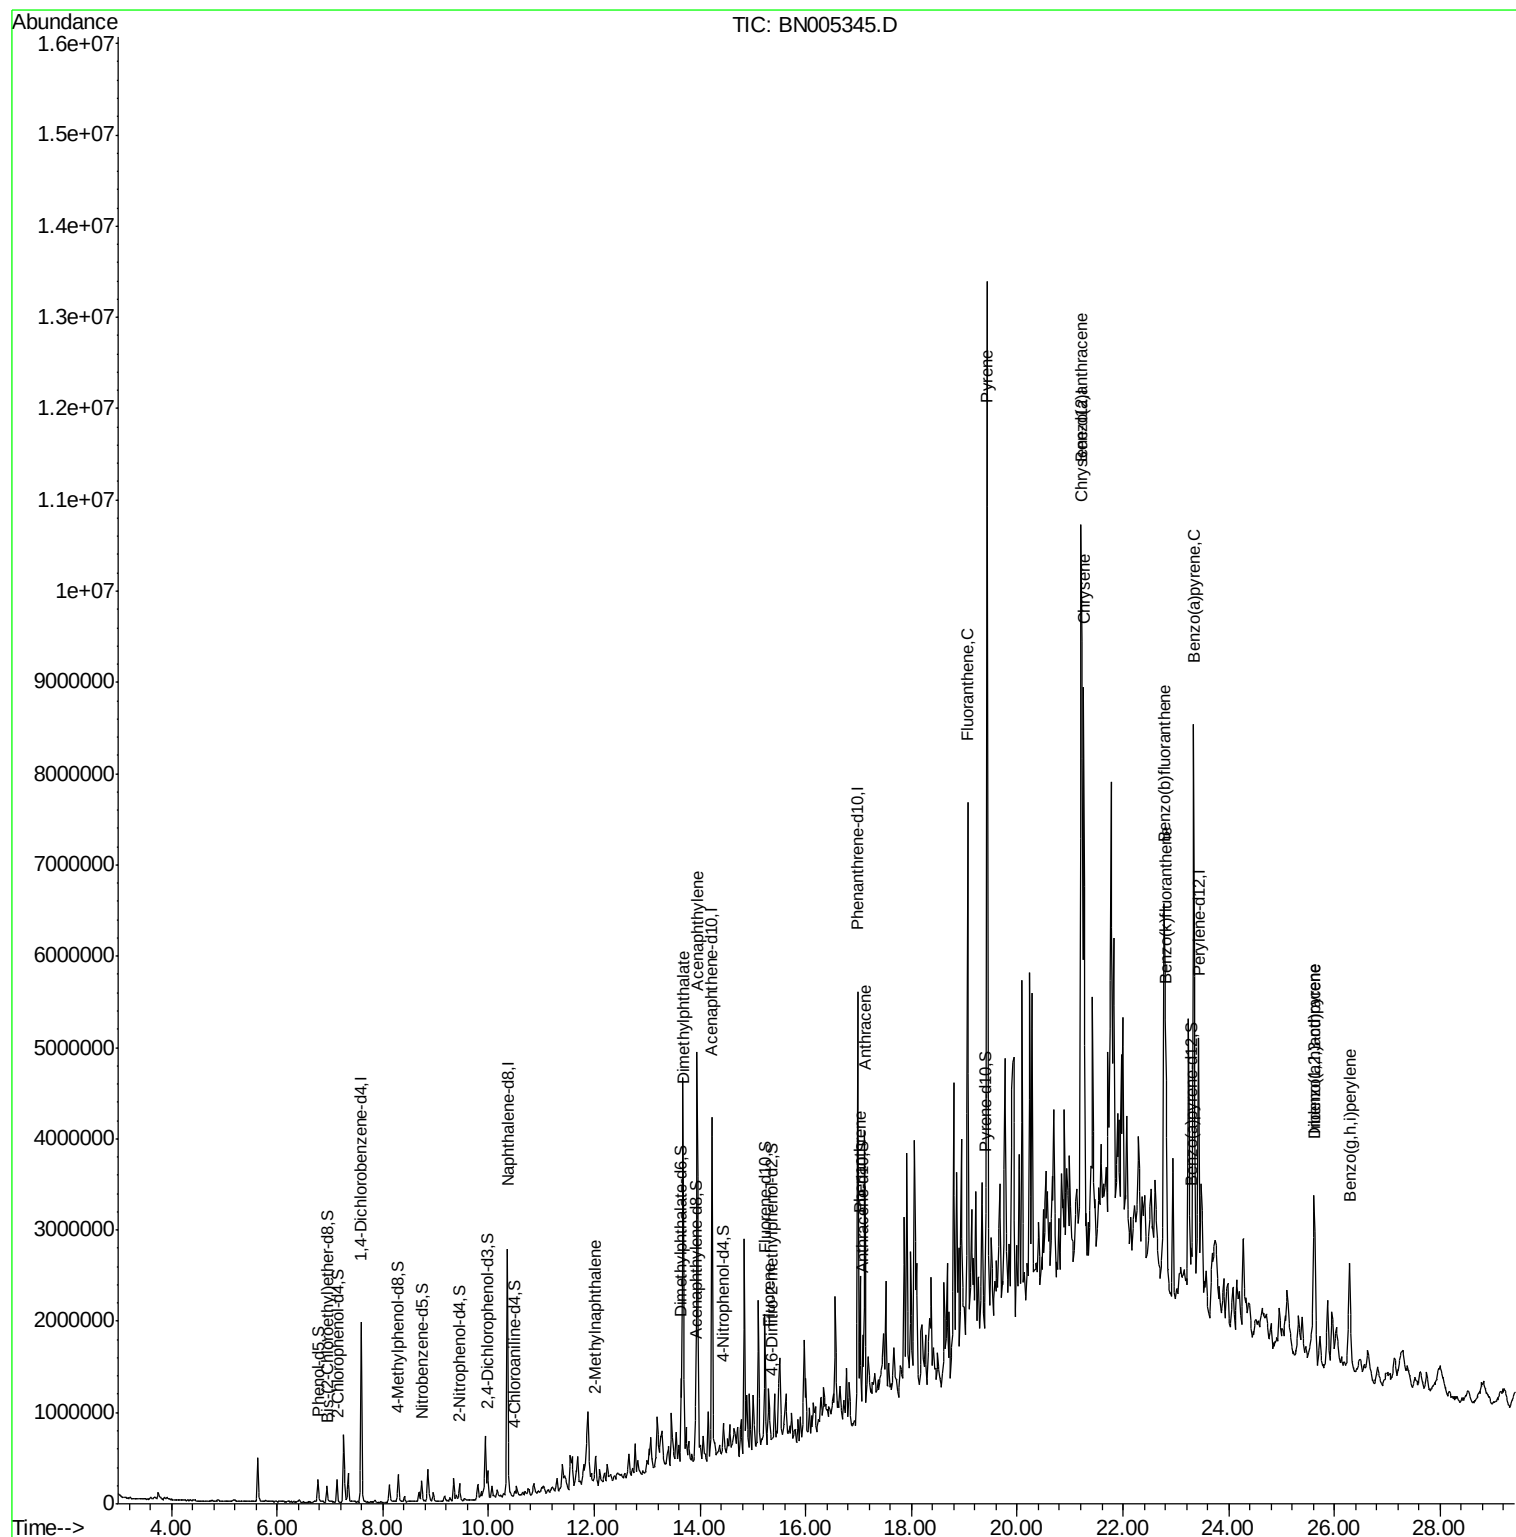

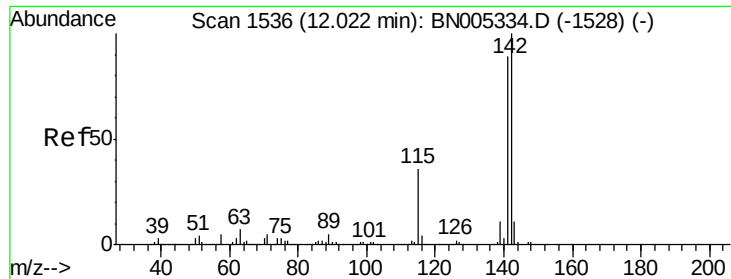





#34
 2-Methylnaphthalene
 Concen: 1.536 ng/ul
 RT: 12.02 min Scan# 1536
 Delta R.T. -0.01 min
 Lab File: BN005345.D
 Acq: 27 Apr 2019 08:00

Instrument :
 BNA_N
 ClientSampleId :
 GAHQ0DL

Tgt Ion:142 Resp: 115094
 Ion Ratio Lower Upper
 142 100
 141 87.2 72.0 108.0




Manual Integrations
 APPROVED


Sohil
 4/29/2019 1:44:21 PM

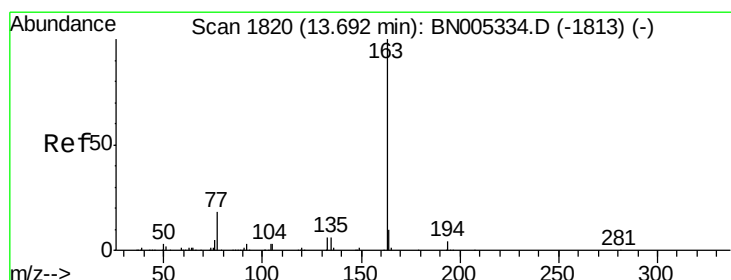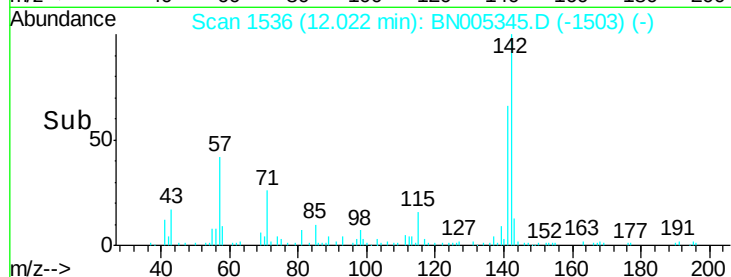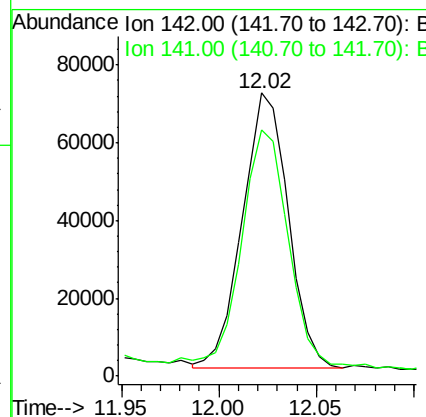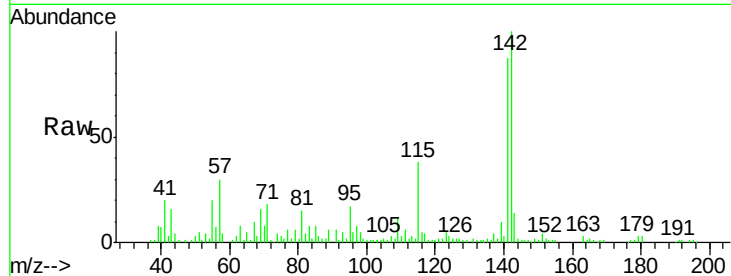

#44
 Dimethylphthalate
 Concen: 1.083 ng/ul
 RT: 13.69 min Scan# 1820
 Delta R.T. -0.01 min
 Lab File: BN005345.D
 Acq: 27 Apr 2019 08:00

Tgt Ion:163 Resp: 98882
 Ion Ratio Lower Upper
 163 100
 194 6.7 3.4 5.0#
 164 12.4 8.1 12.1#

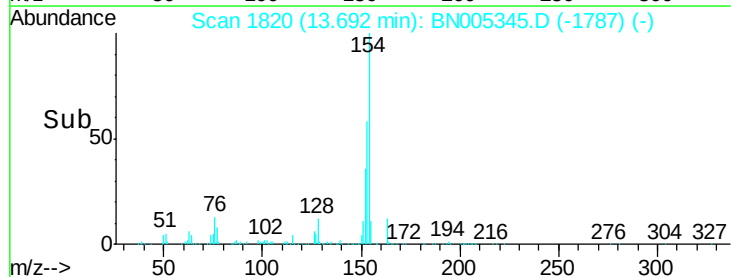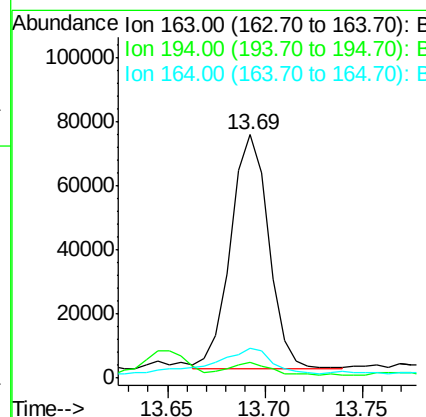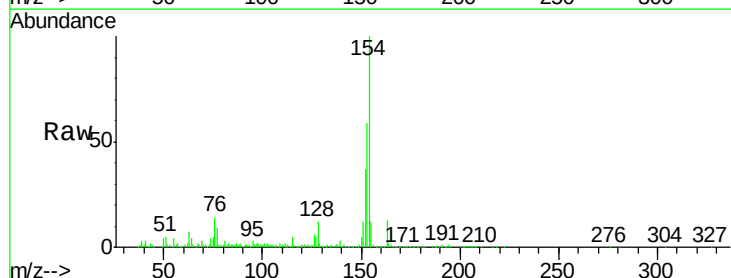

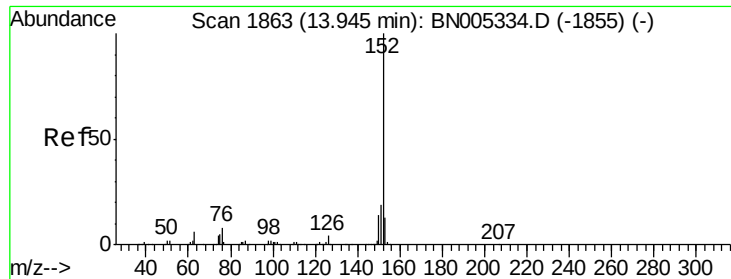





#47
Acenaphthylene
Concen: 30.451 ng/ul
RT: 13.95 min Scan# 1864
Delta R.T. 0.00 min
Lab File: BN005345.D
Acq: 27 Apr 2019 08:00

Instrument :
BNA_N
ClientSampled :
GAHQ0DL

Tgt Ion:152 Resp: 3369003
Ion Ratio Lower Upper
152 100
151 20.0 15.8 23.8
153 13.4 9.8 14.8




Manual Integrations
APPROVED


Sohil
4/29/2019 1:44:21 PM

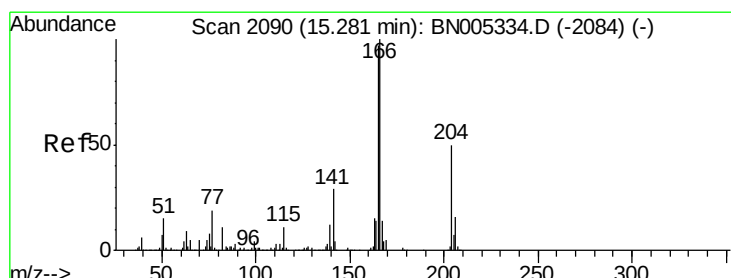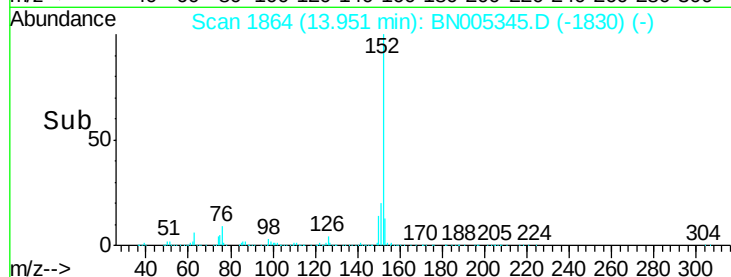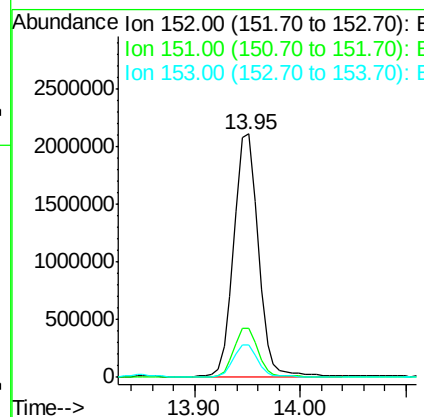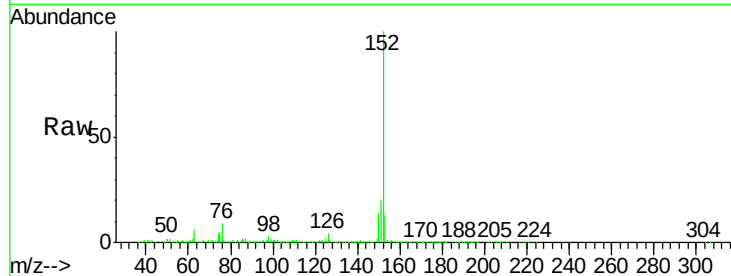

#58
Fluorene
Concen: 3.576 ng/ul
RT: 15.30 min Scan# 2094
Delta R.T. 0.02 min
Lab File: BN005345.D
Acq: 27 Apr 2019 08:00

Tgt Ion:166 Resp: 303473
Ion Ratio Lower Upper
166 100
165 152.2 80.0 120.0#
167 14.5 10.7 16.1

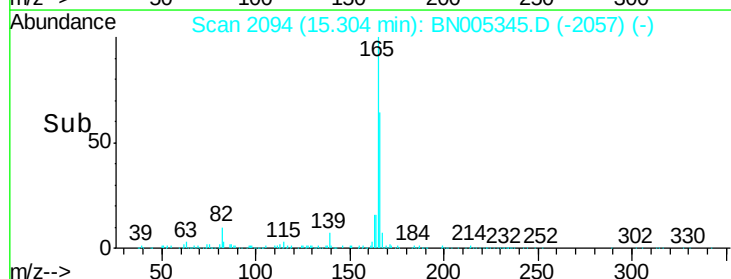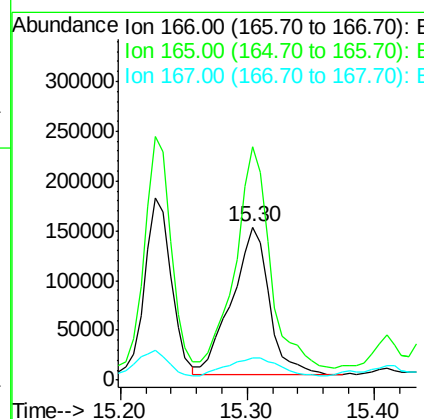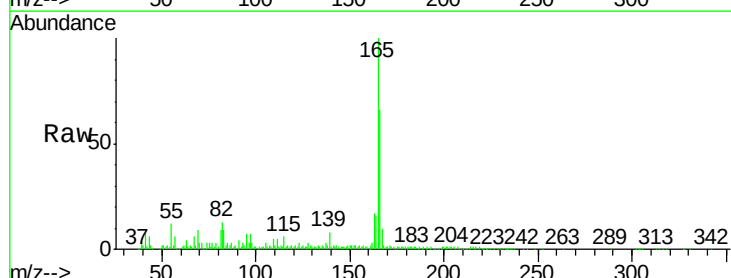

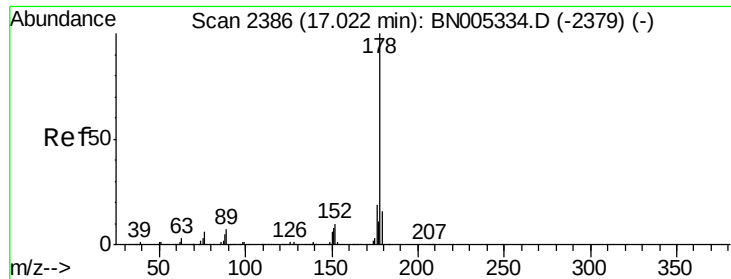

#69

Phenanthrene

Concen: 7.094 ng/ul

RT: 17.03 min Scan# 2387

Delta R.T. 0.00 min

Lab File: BN005345.D

Acq: 27 Apr 2019 08:00

Instrument :

BNA_N


ClientSampled :

GAHQ0DL




Tgt Ion:	178	Resp:	957547
Ion Ratio	Lower	Upper	
178	100		
179	16.9	12.2	18.4
176	19.2	15.1	22.7

Manual Integrations
APPROVED

Sohil
4/29/2019 1:44:21 PM

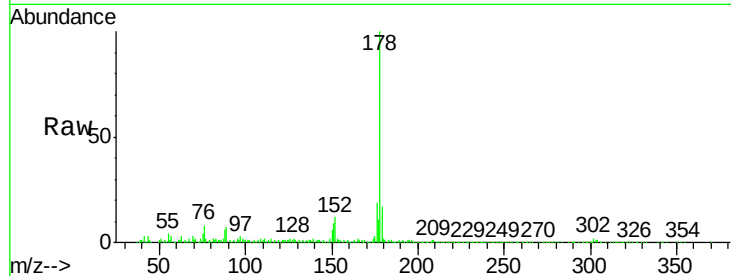

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

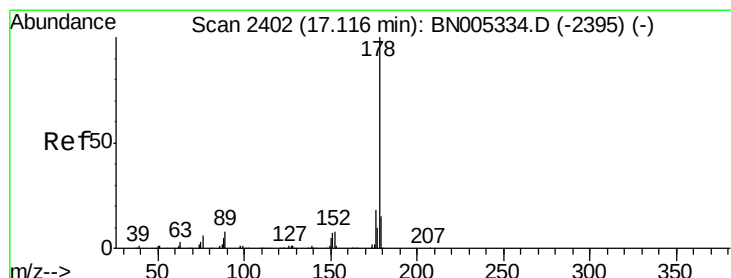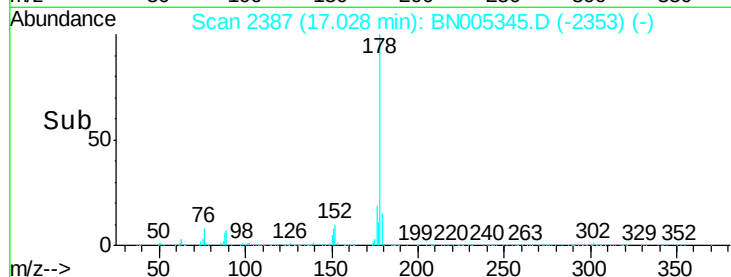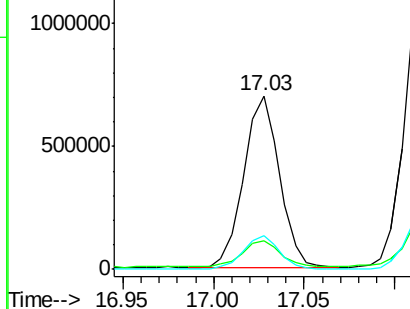

#71

Anthracene

Concen: 14.841 ng/ul


RT: 17.12 min Scan# 2402

Delta R.T. 0.00 min



Lab File: BN005345.D


Acq: 27 Apr 2019 08:00

Tgt Ion:	178	Resp:	2040732
Ion Ratio	Lower	Upper	
178	100		
179	15.6	12.3	18.5
176	18.3	15.1	22.7

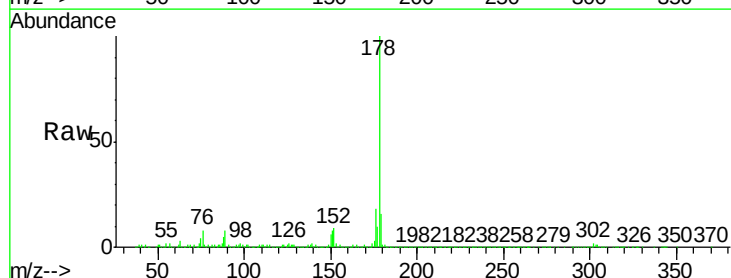

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

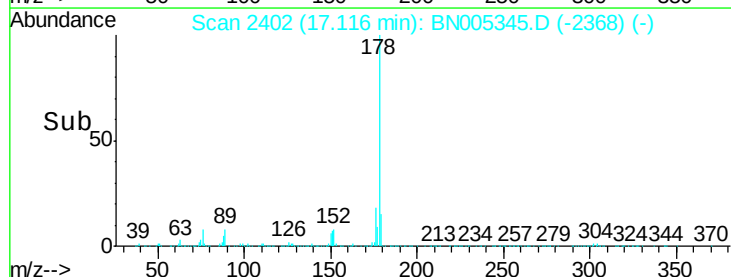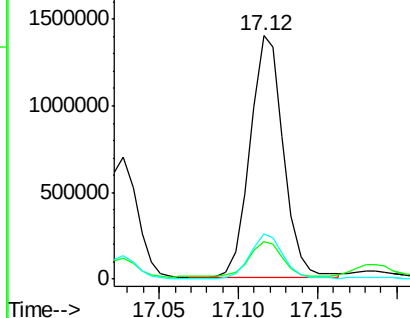

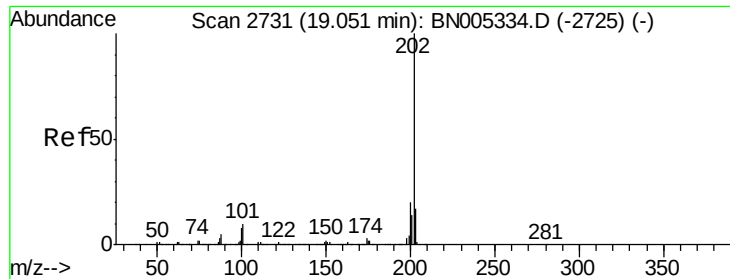


#76
Fluoranthene
Concen: 19.331 ng/ul
RT: 19.06 min Scan# 2733
Delta R.T. 0.00 min
Lab File: BN005345.D
Acq: 27 Apr 2019 08:00

Instrument :
BNA_N
ClientSampled :
GAHQ0DL




Tgt Ion	Ratio	Lower	Upper
202	100		
101	10.3	8.6	12.8
100	7.3	6.3	9.5

Manual Integrations
APPROVED

Sohil
4/29/2019 1:44:21 PM

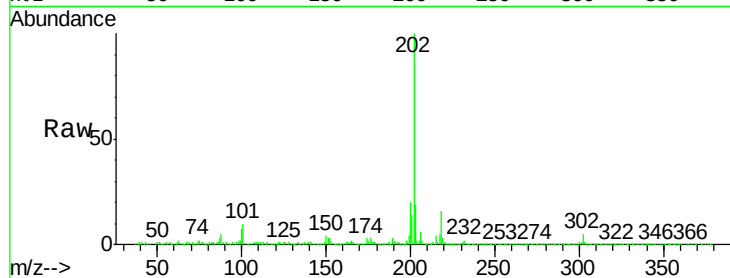




Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

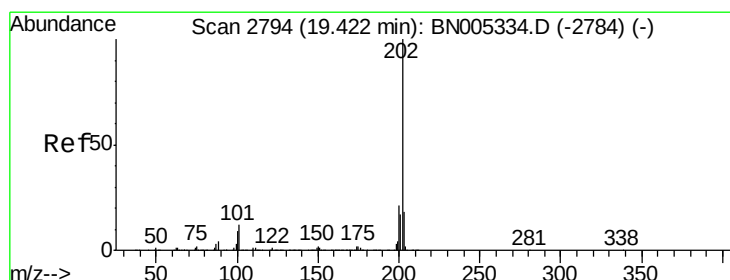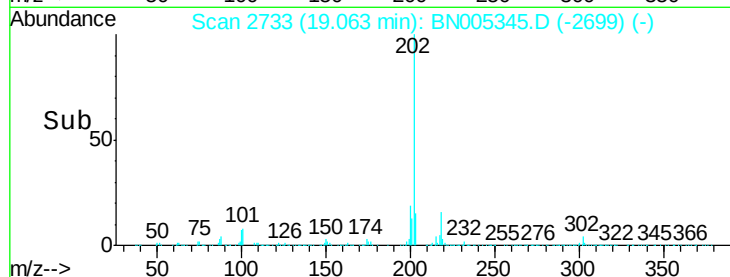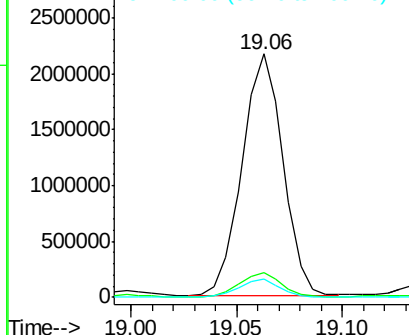


#79
Pyrene
Concen: 56.787 ng/ul
RT: 19.43 min Scan# 2796
Delta R.T. 0.01 min
Lab File: BN005345.D
Acq: 27 Apr 2019 08:00

Tgt Ion	Ratio	Lower	Upper
202	100		
101	11.3	10.3	15.5
100	9.2	7.9	11.9

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

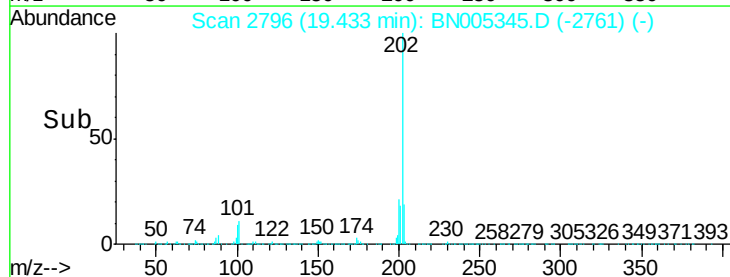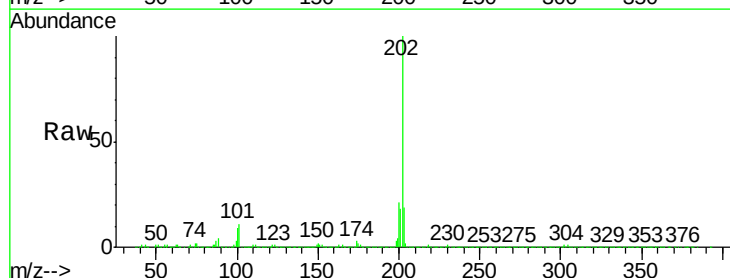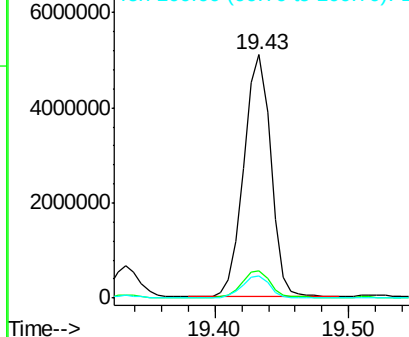

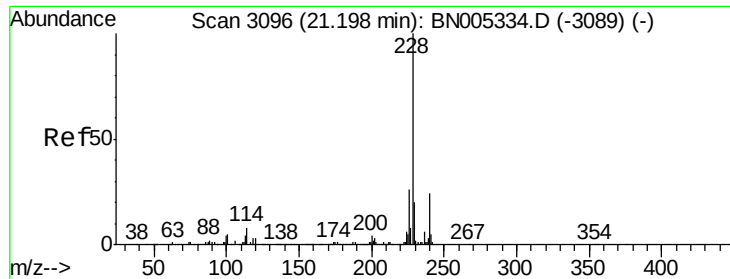

#82

Benzo(a)anthracene

Concen: 29.947 ng/ul m

RT: 21.20 min Scan# 3097

Delta R.T. -0.01 min

Lab File: BN005345.D

Acq: 27 Apr 2019 08:00





Instrument :
BNA_N
ClientSampleId :
GAHQ0DL

Tgt Ion:228 Resp: 3630572

Ion	Ratio	Lower	Upper
228	100		
229	21.8	15.8	23.6
226	33.7	21.4	32.2#

Manual Integrations
APPROVED

Sohil
4/29/2019 1:44:21 PM

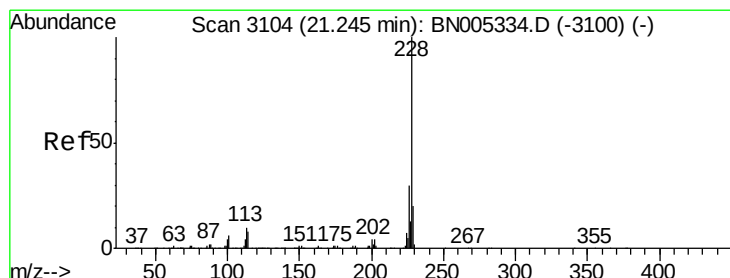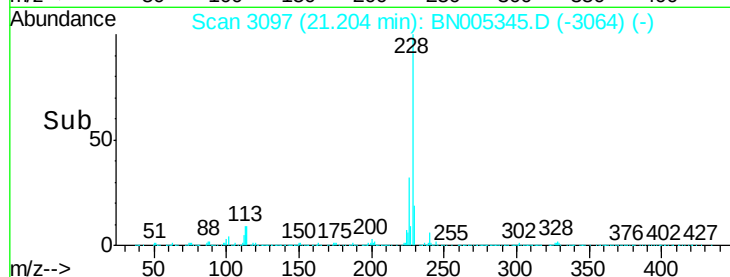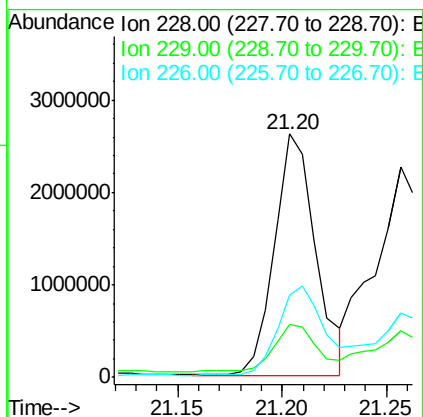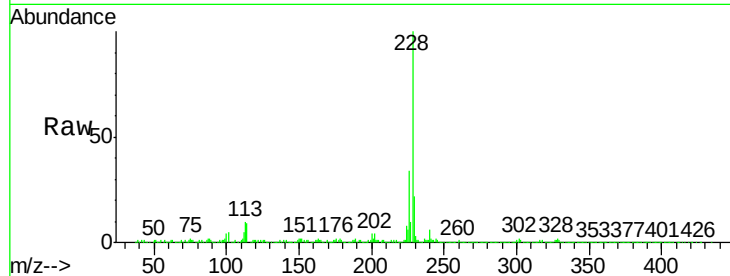

#84

Chrysene

Concen: 31.884 ng/ul

RT: 21.26 min Scan# 3106




Delta R.T. -0.01 min


Lab File: BN005345.D

Acq: 27 Apr 2019 08:00

Tgt Ion:228 Resp: 3587485

Ion	Ratio	Lower	Upper
228	100		
226	30.9	24.0	36.0
229	22.3	15.4	23.0

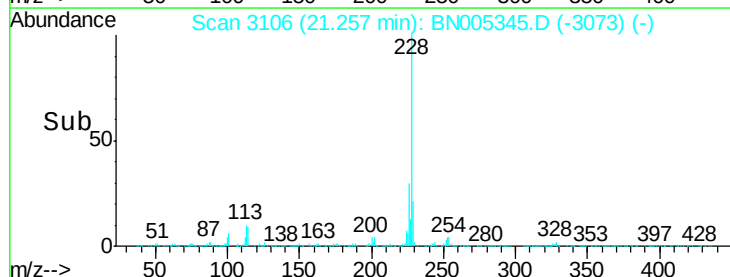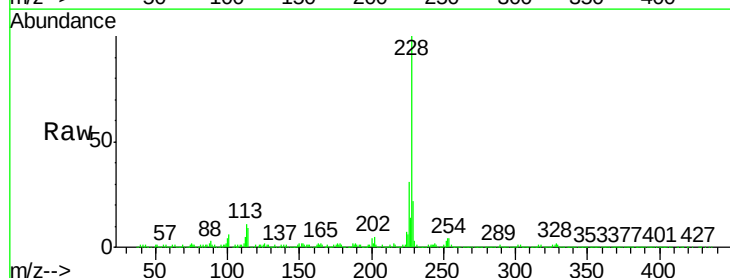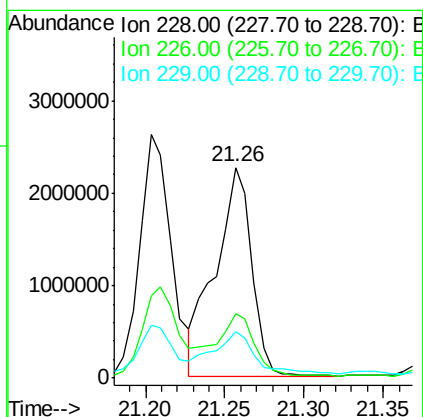

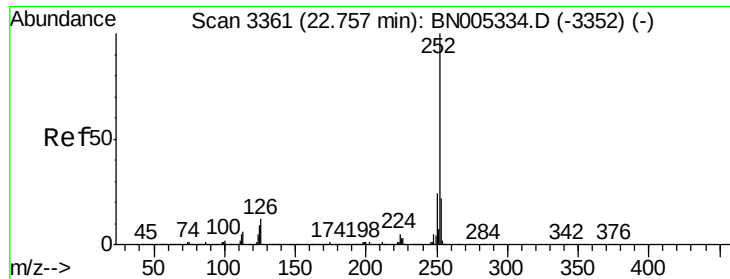





#87
Benzo(b)fluoranthene
Concen: 32.106 ng/ul
RT: 22.78 min Scan# 3365
Delta R.T. -0.01 min
Lab File: BN005345.D
Acq: 27 Apr 2019 08:00

Instrument :
BNA_N
ClientSampleId :
GAHQ0DL

Tgt Ion:252 Resp: 3663535
Ion Ratio Lower Upper
252 100
253 23.1 17.7 26.5
125 9.2 8.4 12.6




Manual Integrations
APPROVED


Sohil
4/29/2019 1:44:21 PM

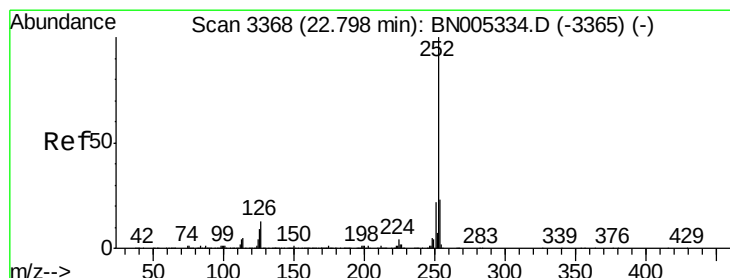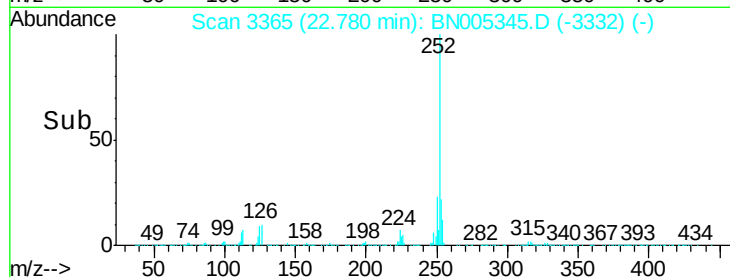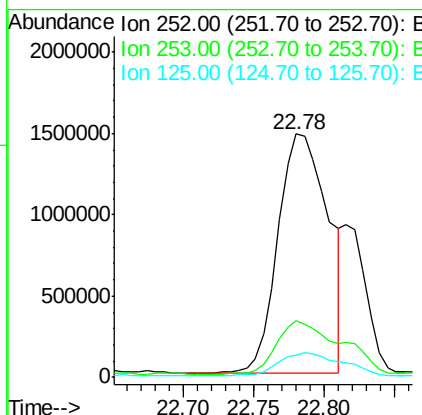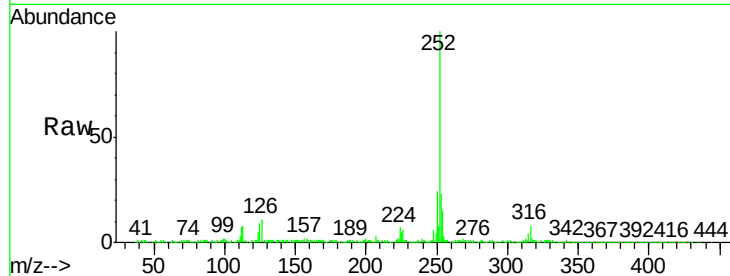

#88
Benzo(k)fluoranthene
Concen: 9.538 ng/ul m
RT: 22.82 min Scan# 3371
Delta R.T. -0.01 min
Lab File: BN005345.D
Acq: 27 Apr 2019 08:00

Tgt Ion:252 Resp: 1039393
Ion Ratio Lower Upper
252 100
253 22.8 17.4 26.0
125 9.3 7.5 11.3

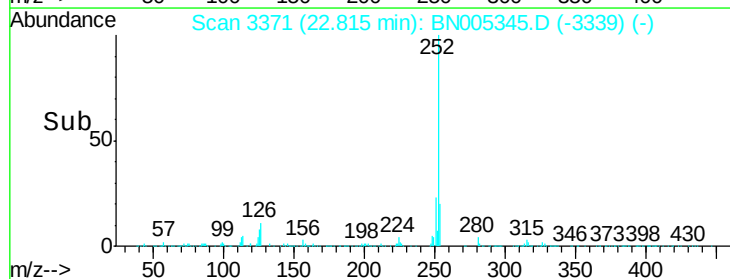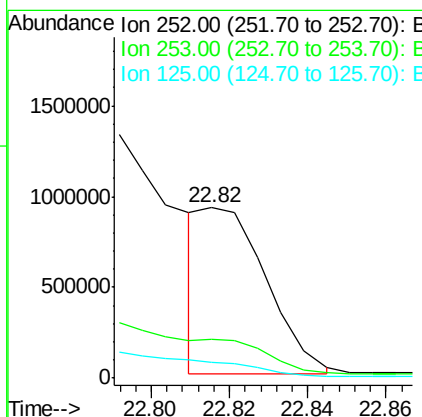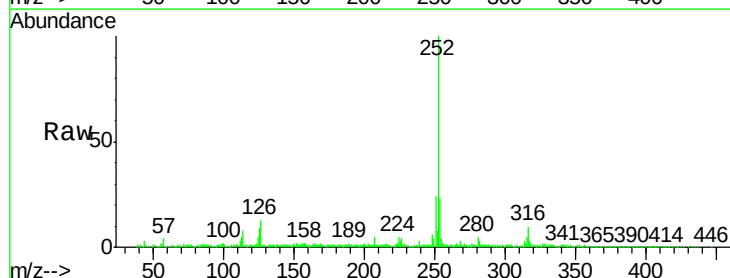

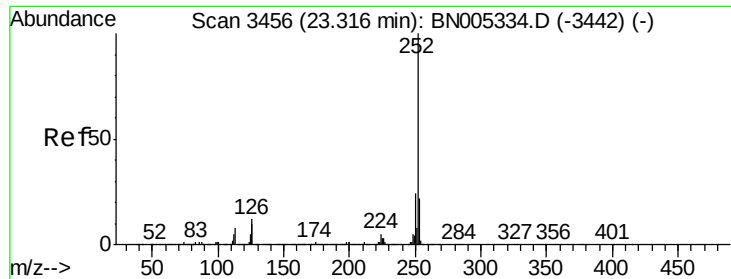

#90

Benzo(a)pyrene

Concen: 34.654 ng/ul

RT: 23.34 min Scan# 3460

Delta R.T. -0.01 min

Lab File: BN005345.D





Acq: 27 Apr 2019 08:00

Instrument :
BNA_N
ClientSampled :
GAHQ0DL

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.1	17.3	25.9
125	9.4	8.6	13.0

Manual Integrations
APPROVED

Sohil
4/29/2019 1:44:21 PM

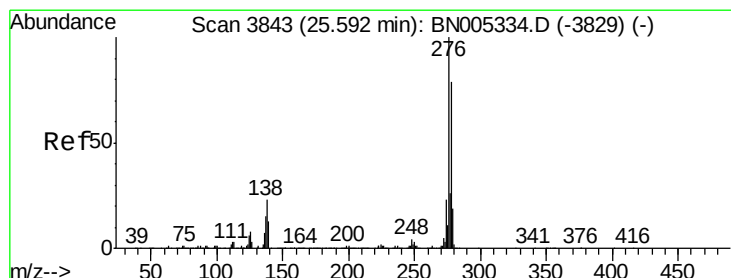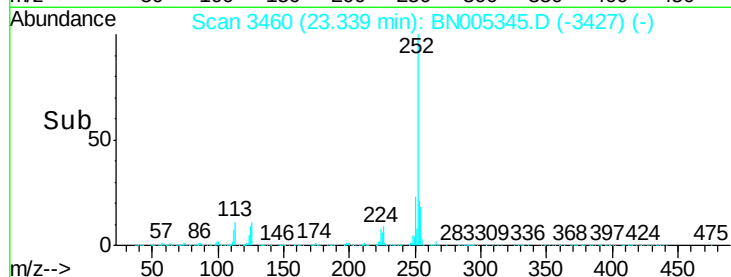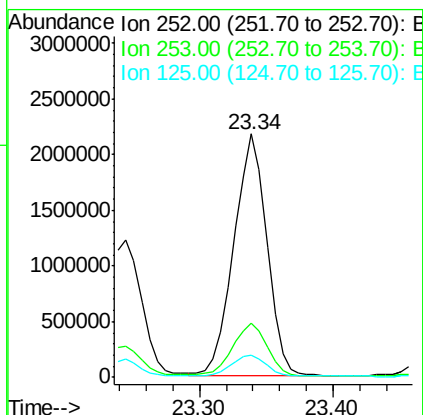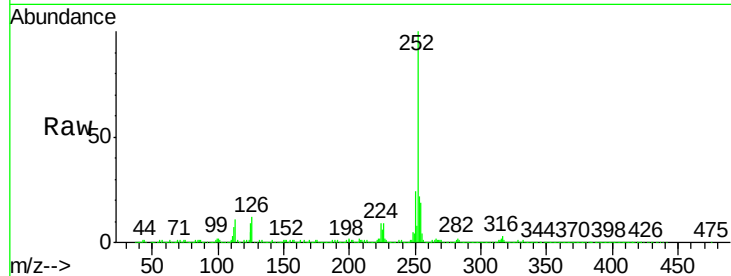

#91

Indeno(1,2,3-cd)pyrene

Concen: 14.768 ng/ul




RT: 25.62 min Scan# 3847


Delta R.T. -0.01 min

Lab File: BN005345.D

Acq: 27 Apr 2019 08:00

Tgt Ion	Ratio	Lower	Upper
276	100		
138	19.1	17.9	26.9
277	26.1	19.7	29.5

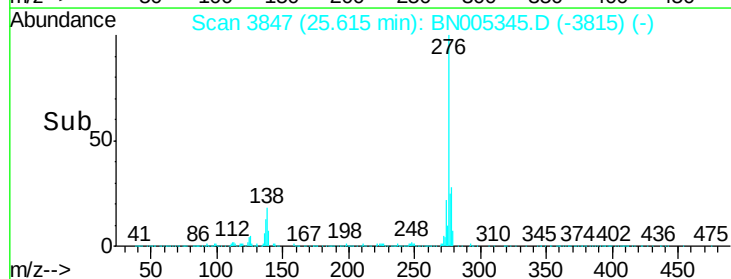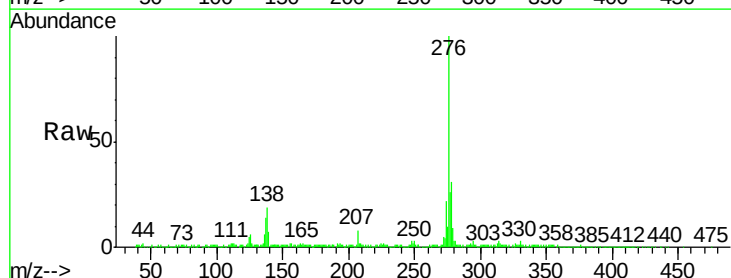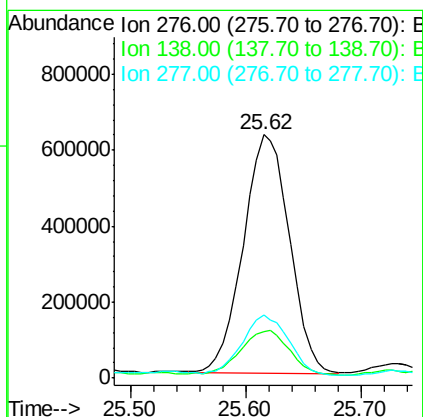

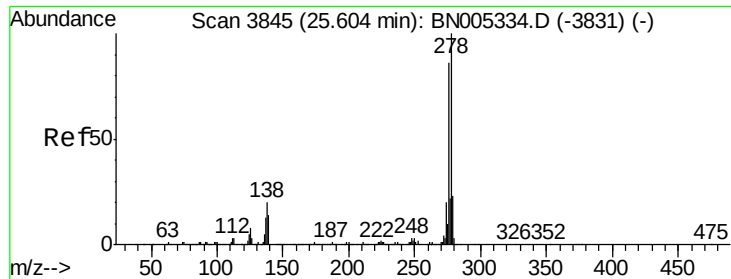

#92

Dibenzo(a,h)anthracene

Concen: 6.348 ng/ul

RT: 25.63 min Scan# 3849

Delta R.T. -0.01 min

Lab File: BN005345.D

Acq: 27 Apr 2019 08:00

Instrument :

BNA_N





ClientSampled :

GAHQ0DL

Tgt Ion:	278	Resp:	638867
Ion Ratio	Lower	Upper	
278	100		
139	18.9	13.1	19.7
279	28.3	19.4	29.0

Manual Integrations
APPROVED

Sohil
4/29/2019 1:44:21 PM

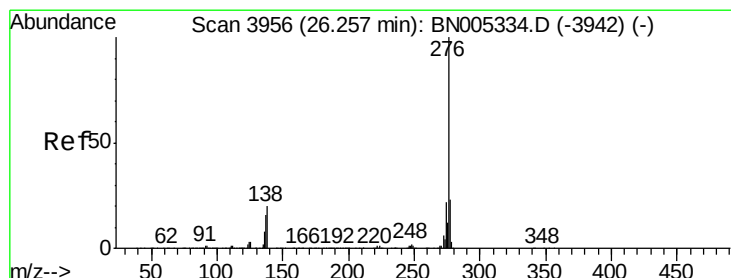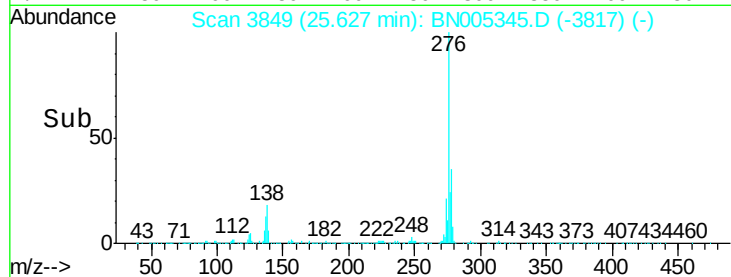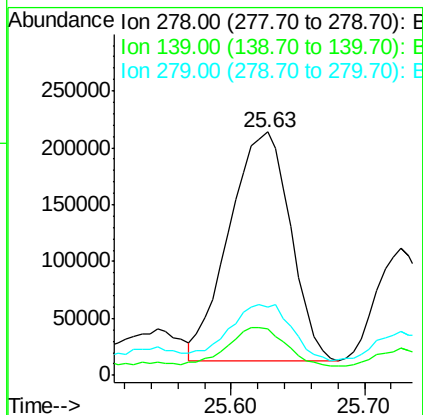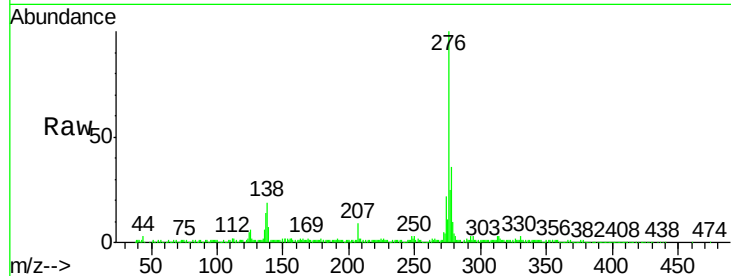

#93

Benzo(g,h,i)perylene

Concen: 14.785 ng/ul

RT: 26.29 min Scan# 3961

Delta R.T. -0.01 min

Lab File: BN005345.D

Acq: 27 Apr 2019 08:00

Tgt Ion:	276	Resp:	1449695
Ion Ratio	Lower	Upper	
276	100		
138	20.2	16.7	25.1
277	25.4	18.2	27.2

