

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042619\
 Data File : BN005320.D
 Acq On : 26 Apr 2019 17:36
 Operator : JU/SJ
 Sample : PB119224BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK24

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	35	39	49	rVB	96679	141103	1.33%	0.128%
2	3.911	154	157	163	rVB4	13055	18449	0.17%	0.017%
3	6.775	635	644	659	rBV	1755719	2819216	26.51%	2.554%
4	6.940	666	672	684	rVB	1396601	2179653	20.50%	1.974%
5	7.134	697	705	720	rVB	1781026	2860815	26.90%	2.591%
6	7.593	776	783	793	rBV	1653499	2592867	24.38%	2.349%
7	8.293	894	902	915	rBV	2225862	3602435	33.88%	3.263%
8	8.734	969	977	986	rBV	1775495	2877221	27.06%	2.606%
9	9.446	1091	1098	1107	rBV	1466882	2393039	22.50%	2.168%
10	9.975	1182	1188	1206	rBV	2162464	3741027	35.18%	3.389%
11	10.352	1245	1252	1259	rBV	2278516	3817911	35.90%	3.458%
12	10.404	1259	1261	1268	rVB	43878	55348	0.52%	0.050%
13	10.493	1268	1276	1293	rBV	2298628	3879988	36.49%	3.515%
14	11.957	1519	1525	1533	rBV2	26915	58362	0.55%	0.053%
15	12.028	1533	1537	1549	rVB3	26065	58584	0.55%	0.053%
16	12.251	1570	1575	1582	rVB3	13158	22798	0.21%	0.021%
17	13.204	1728	1737	1738	rBV3	5631	11177	0.11%	0.010%
18	13.645	1805	1812	1823	rVB	4145154	5694335	53.55%	5.158%
19	13.916	1850	1858	1873	rBV	4566178	6879462	64.69%	6.232%
20	14.228	1904	1911	1918	rBV2	3291078	5093618	47.90%	4.614%
21	14.434	1937	1946	1960	rBV	1754763	2862361	26.92%	2.593%
22	15.228	2074	2081	2089	rBV	5869261	8368249	78.69%	7.580%
23	15.351	2096	2102	2116	rBV	1526529	2247570	21.14%	2.036%
24	15.463	2118	2121	2128	rVB	76644	113660	1.07%	0.103%
25	16.016	2209	2215	2220	rBV5	25617	39857	0.37%	0.036%
26	16.187	2238	2244	2247	rBV4	6623	10789	0.10%	0.010%
27	16.657	2321	2324	2329	rBV5	11091	16430	0.15%	0.015%
28	16.769	2340	2343	2349	rBV3	15125	21909	0.21%	0.020%
29	16.981	2372	2379	2389	rBV2	4557478	6341393	59.63%	5.744%
30	17.081	2389	2396	2409	rVB	6585585	9381709	88.22%	8.498%
31	17.910	2533	2537	2542	rBV6	14351	27316	0.26%	0.025%
32	19.022	2722	2726	2731	rBV	70751	101837	0.96%	0.092%
33	19.204	2754	2757	2762	rBV5	14312	20989	0.20%	0.019%
34	19.280	2766	2770	2776	rVB	69018	85653	0.81%	0.078%

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042619\
Data File : BN005320.D
Acq On : 26 Apr 2019 17:36
Operator : JU/SJ
Sample : PB119224BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK24

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Title : SVOA CALIBRATION

35	19.392	2783	2789	2798	rBV	7711586	10633878	100.00%	9.633%
36	21.157	3087	3089	3092	rVB3	31724	28143	0.26%	0.025%
37	21.216	3093	3099	3109	rVV	4666100	6253746	58.81%	5.665%
38	21.404	3128	3131	3134	rBV5	50477	57193	0.54%	0.052%
39	21.839	3202	3205	3210	rVB	83817	98666	0.93%	0.089%
40	22.298	3279	3283	3290	rBV	175186	224180	2.11%	0.203%
41	22.798	3364	3368	3374	rVB	207202	297330	2.80%	0.269%
42	23.280	3442	3450	3458	rBV2	4305895	8045386	75.66%	7.288%
43	23.351	3458	3462	3466	rVV	256700	420478	3.95%	0.381%
44	23.416	3466	3473	3485	rVB	2649855	5175084	48.67%	4.688%
45	23.986	3566	3570	3576	rVB	225518	347730	3.27%	0.315%
46	24.715	3689	3694	3703	rVB2	180667	376434	3.54%	0.341%


Sum of corrected areas: 110395378

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042619\
Data File : BN005320.D
Acq On : 26 Apr 2019 17:36
Operator : JU/SJ
Sample : PB119224BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK24

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

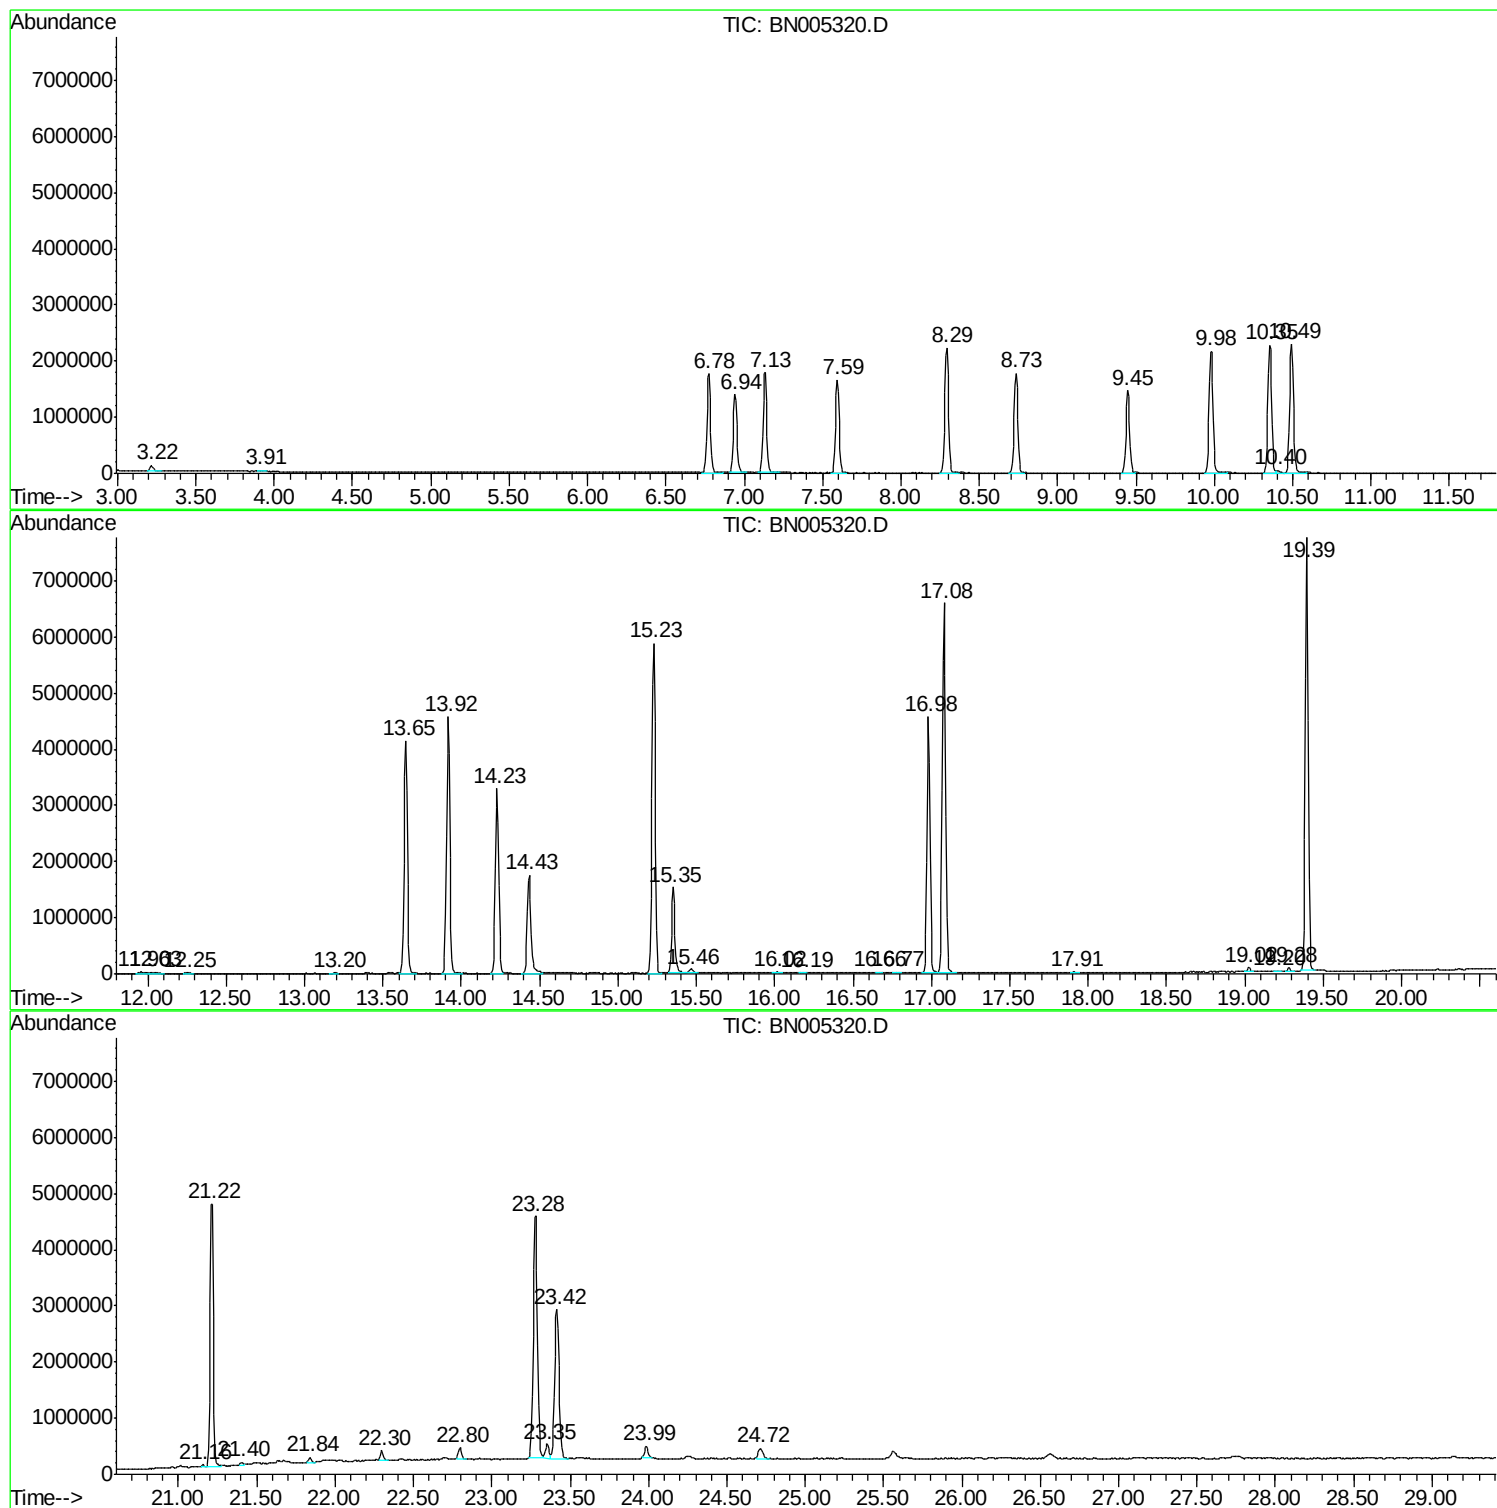

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042619\
Data File : BN005320.D
Acq On : 26 Apr 2019 17:36
Operator : JU/SJ
Sample : PB119224BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK24

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042619\
Data File : BN005320.D
Acq On : 26 Apr 2019 17:36
Operator : JU/SJ
Sample : PB119224BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK24

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc