

Data Path : Z:\HPCHEM1\BNA_N\DATA\BN042718\
 Data File : BN000989.D
 Acq On : 28 Apr 2018 07:03
 Operator : JU/SJ
 Sample : J2274-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0B16

Quant Time: Apr 30 08:30:22 2018
 Quant Method : Z:\HPCHEM1\BNA_N\Methods\SOM-EPA-BN041918-PAH.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 28 03:58:06 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	147804	20.00	ng/ul	0.00
2) Naphthalene-d8	10.39	136	665897	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.25	164	354038	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.00	188	722889	20.00	ng/ul	0.00
18) Chrysene-d12	21.21	240	580427	20.00	ng/ul	0.00
23) Perylene-d12	23.40	264	552577	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 2,4-Dichlorophenol-d3	10.01	165	261730	27.63	ng/ul	0.00
7) Acenaphthylene-d8	13.94	160	910375	26.72	ng/ul	0.00
10) Fluorene-d10	15.25	176	628745	27.54	ng/ul	0.00
15) Anthracene-d10	17.10	188	901687	26.98	ng/ul	0.00
19) Pyrene-d10	19.40	212	885603	30.32	ng/ul	0.00
26) Benzo(a)pyrene-d12	23.26	264	790614	30.34	ng/ul	0.00
Target Compounds				Qvalue		
17) Fluoranthene	19.07	202	48044	1.237	ng/ul#	78
20) Pyrene	19.43	202	70855	1.928	ng/ul#	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_N\DATA\BN042718\
Data File : BN000989.D
Acq On : 28 Apr 2018 07:03
Operator : JU/SJ
Sample : J2274-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B16

Quant Time: Apr 30 08:30:22 2018
Quant Method : Z:\HPCHEM1\BNA_N\Methods\SOM-EPA-BN041918-PAH.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 28 03:58:06 2018
Response via : Initial Calibration




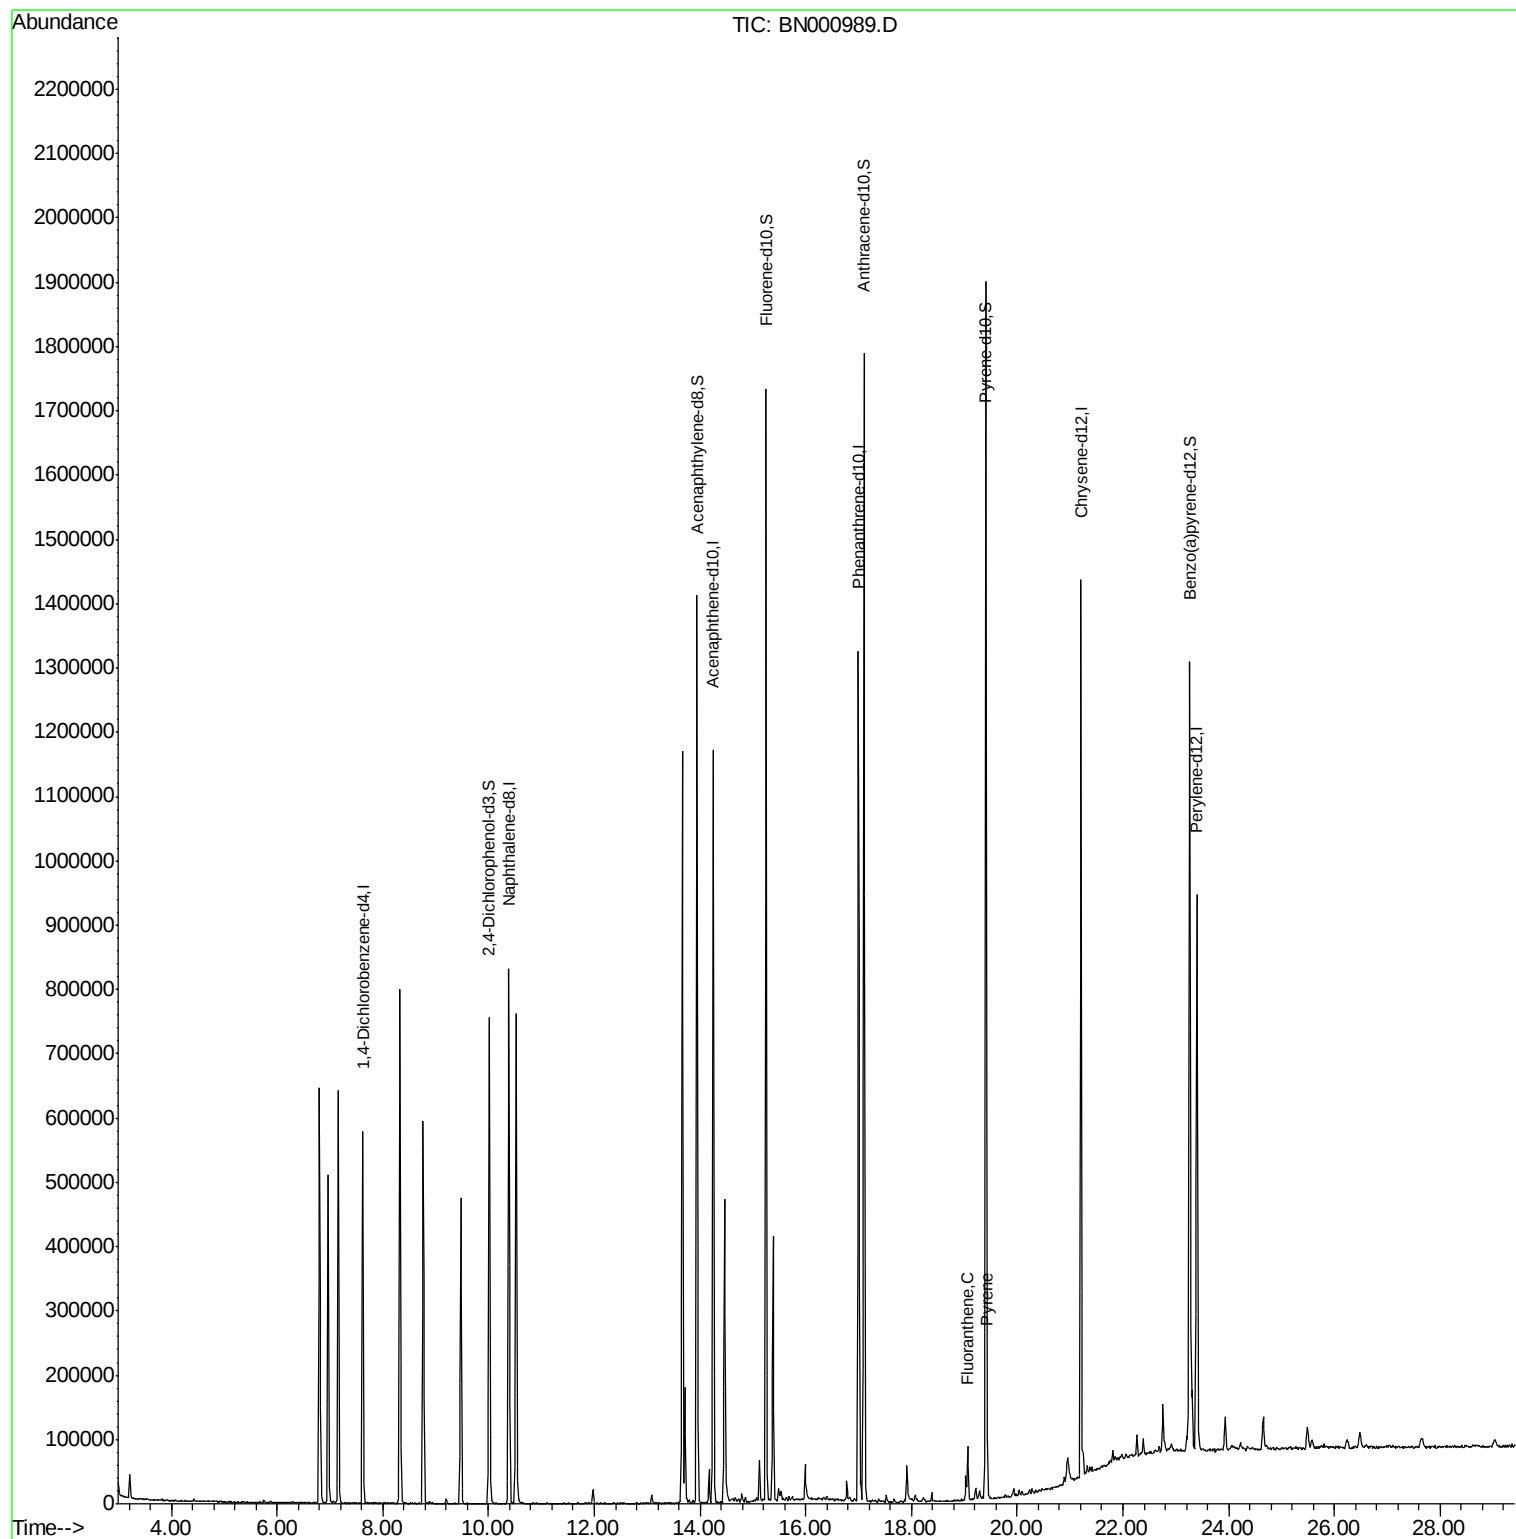


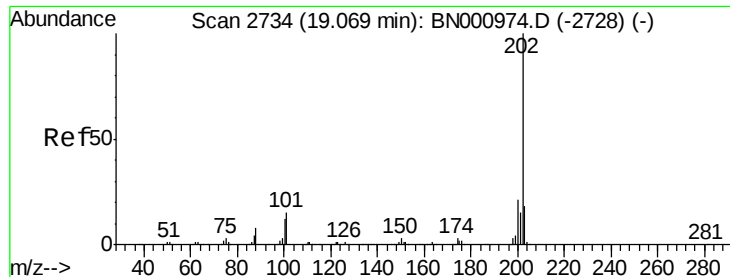

#17
Fluoranthene
 Concen: 1.237 ng/ul
 RT: 19.07 min Scan# 2734
 Delta R.T. 0.00 min
 Lab File: BN000989.D
 Acq: 28 Apr 2018 07:03

Instrument :
 BNA_N
 ClientSampleId :
 C0B16

Tgt Ion:202 Resp: 48044
 Ion Ratio Lower Upper
 202 100
 101 14.5 4.6 7.0#
 100 10.0 3.4 5.2#

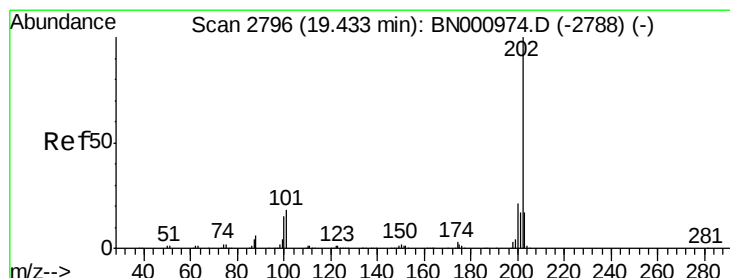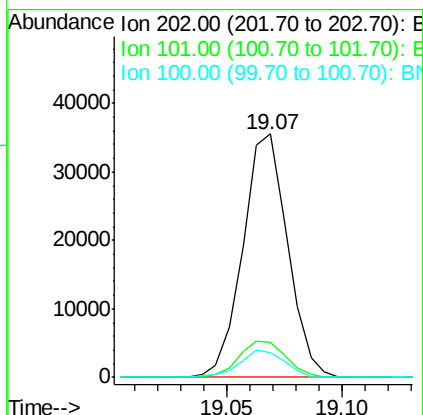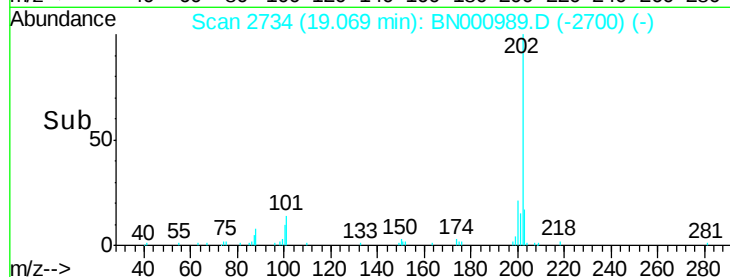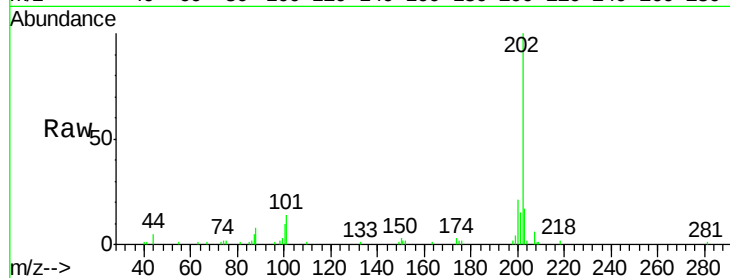

#20
Pyrene
 Concen: 1.928 ng/ul
 RT: 19.43 min Scan# 2796
 Delta R.T. 0.00 min
 Lab File: BN000989.D
 Acq: 28 Apr 2018 07:03

Tgt Ion:202 Resp: 70855
 Ion Ratio Lower Upper
 202 100
 101 17.4 5.1 7.7#
 100 14.6 4.9 7.3#

