
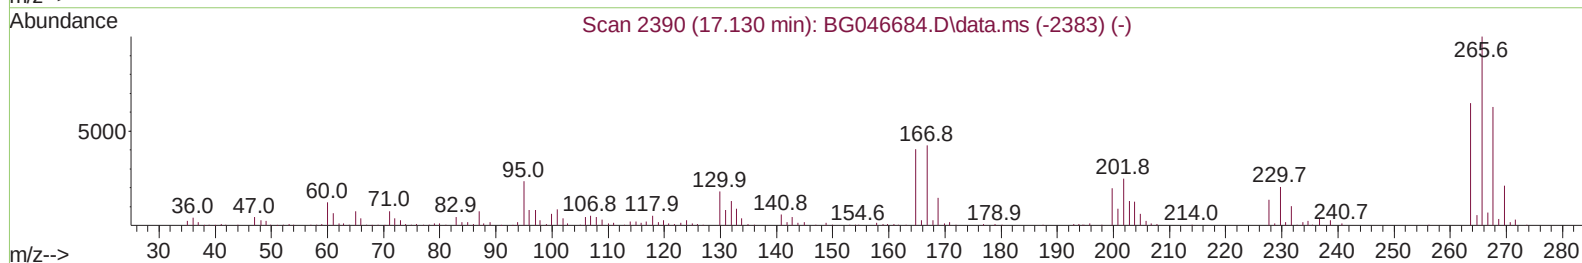
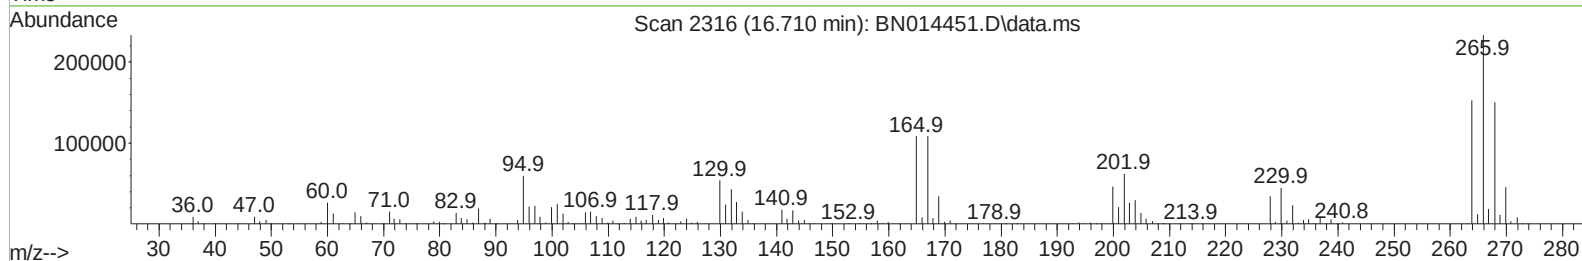


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042721\
Data File : BN014451.D
Acq On : 27 Apr 2021 09:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 27 11:17:25 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 09 09:55:03 2021
Response via : Initial Calibration

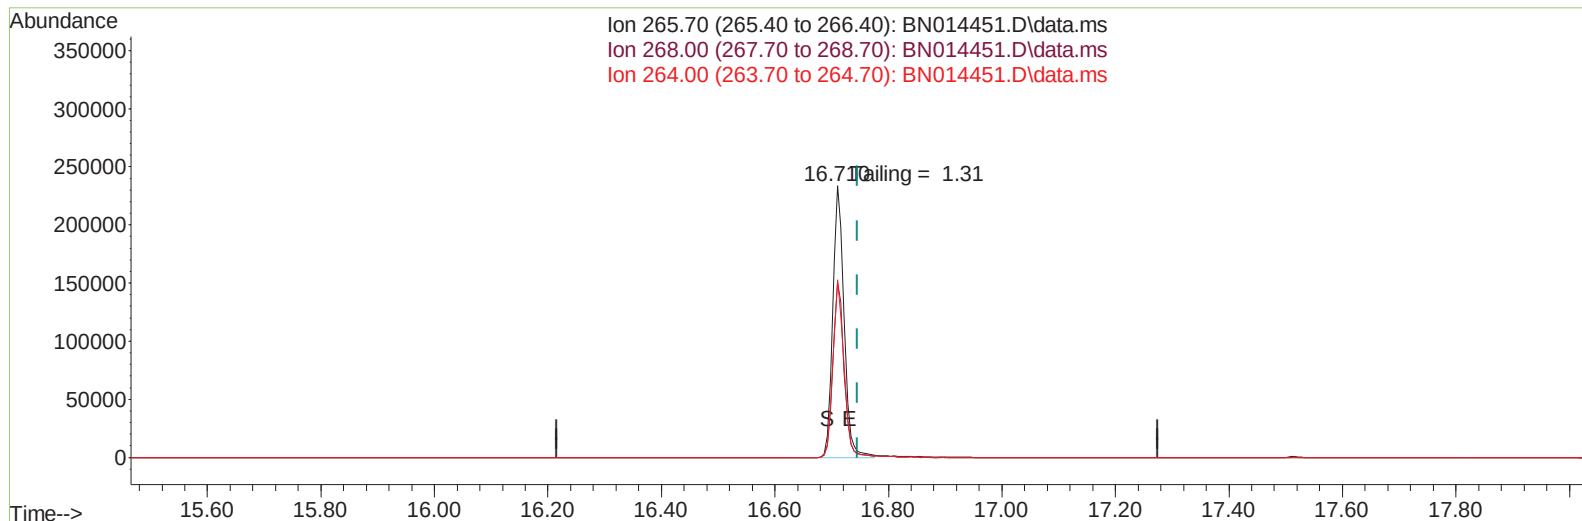




TIC: BN014451.D\data.ms

(70) Pentachlorophenol (C)**16.710min (-0.035) 22130.28 ng****response 325463**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.48
264.00	61.60	65.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042721\
Data File : BN014451.D
Acq On : 27 Apr 2021 09:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 27 11:17:25 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 09 09:55:03 2021
Response via : Initial Calibration

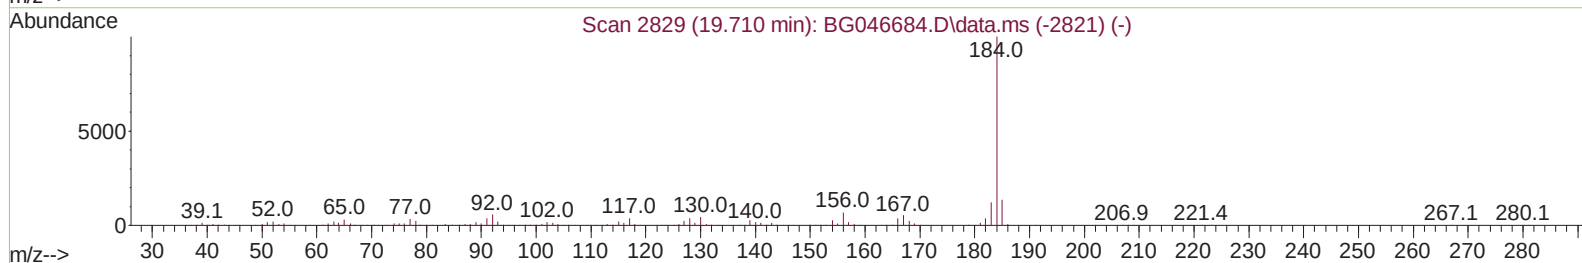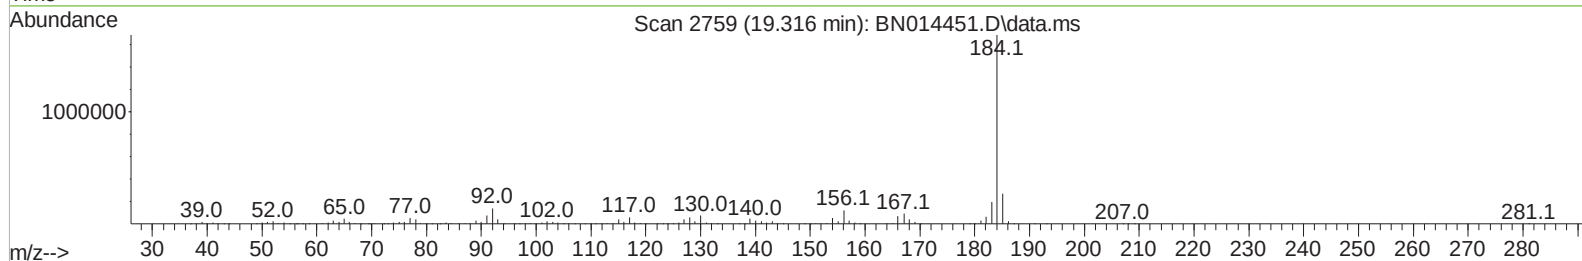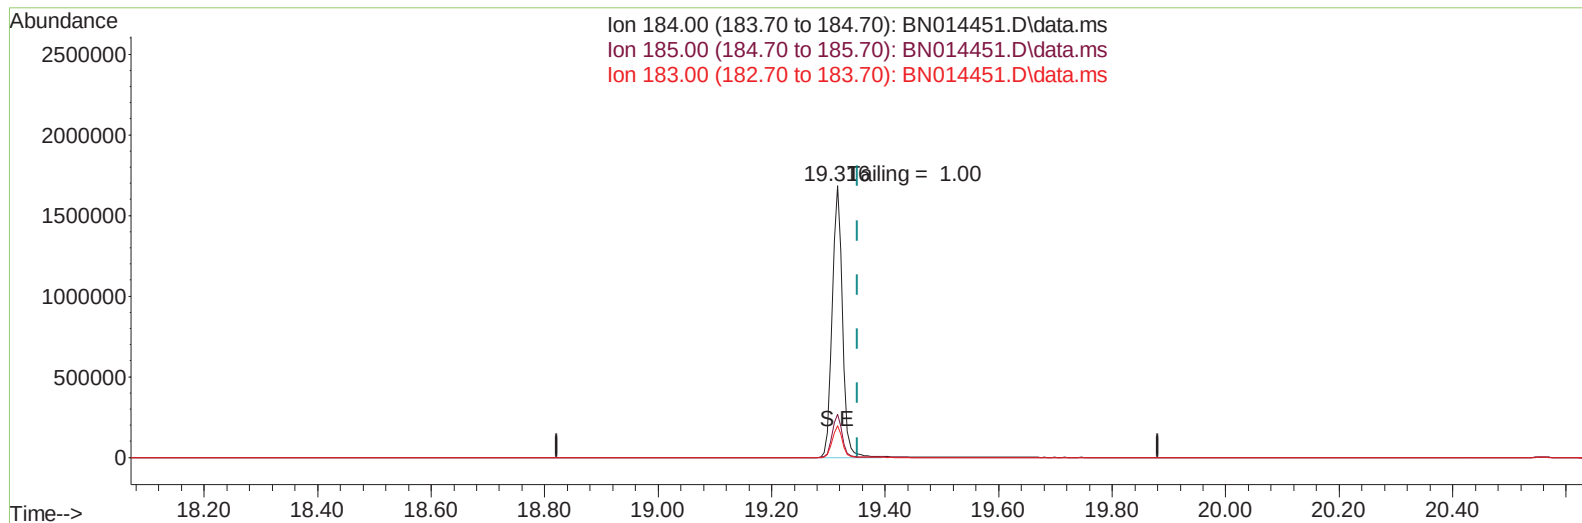

TIC: BN014451.D\data.ms

(77) Benzidine

19.316min (-0.035) 0.00 ng

response 2137484

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	16.04
183.00	13.20	11.67
0.00	0.00	0.00