
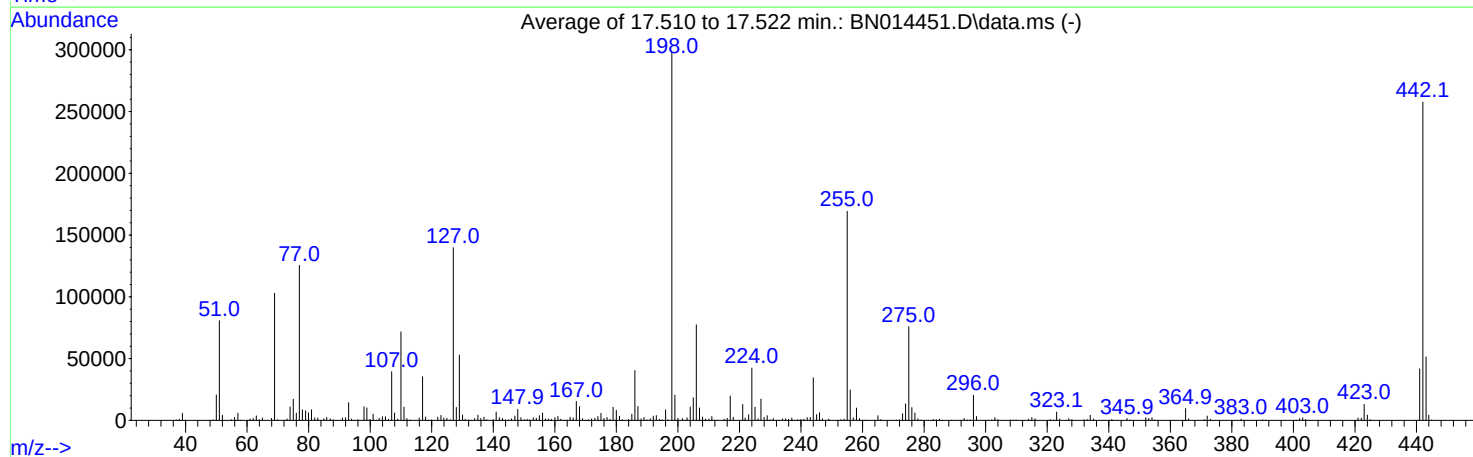


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042721\
 Data File : BN014451.D
 Acq On : 27 Apr 2021 09:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 27 11:43:13 2021

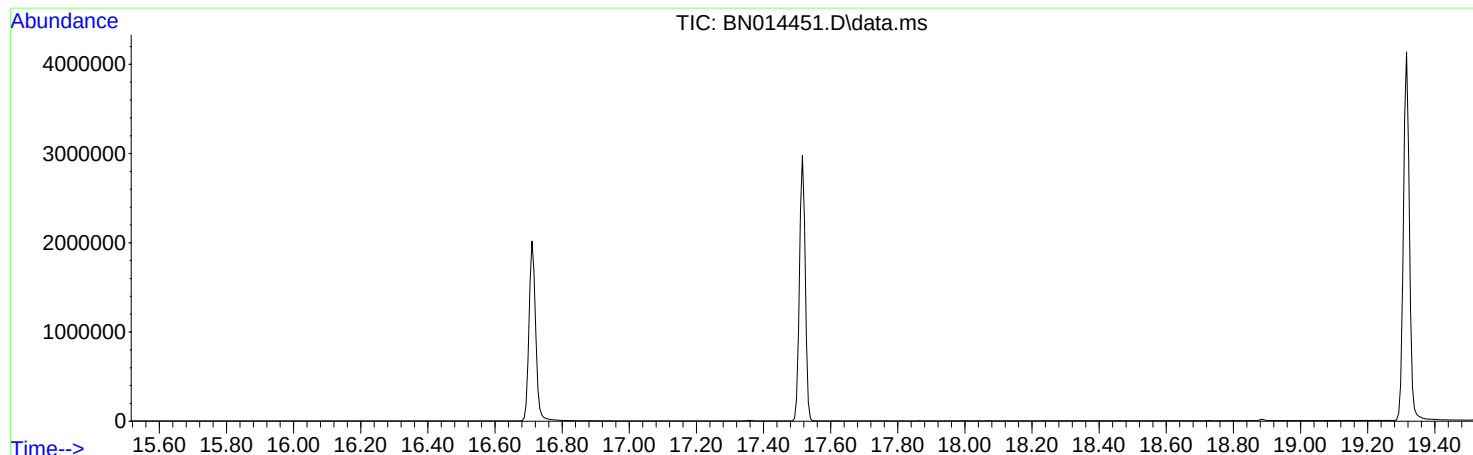




AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.1	80779	PASS
68	69	0.00	2	1.6	1617	PASS
69	198	0.00	100	34.5	102835	PASS
70	69	0.00	2	0.5	530	PASS
127	198	10	80	46.9	139784	PASS
197	198	0.00	2	0.1	355	PASS
198	198	100	100	100.0	297835	PASS
199	198	5	9	6.9	20464	PASS
275	198	10	60	25.5	75808	PASS
365	198	1	100	3.2	9659	PASS
441	198	0.01	100	14.0	41731	PASS
442	442	50	100	100.0	257643	PASS
443	442	15	24	20.0	51464	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042721\
Data File : BN014451.D
Acq On : 27 Apr 2021 09:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 27 11:17:25 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 09 09:55:03 2021
Response via : Initial Calibration

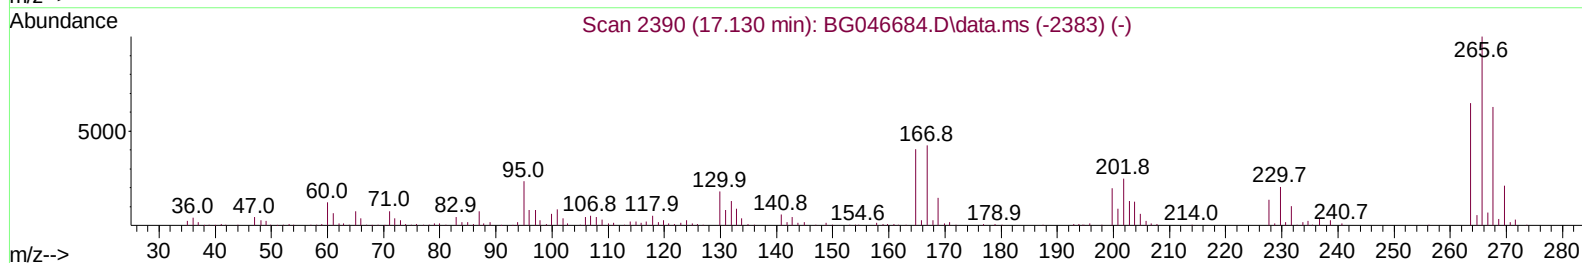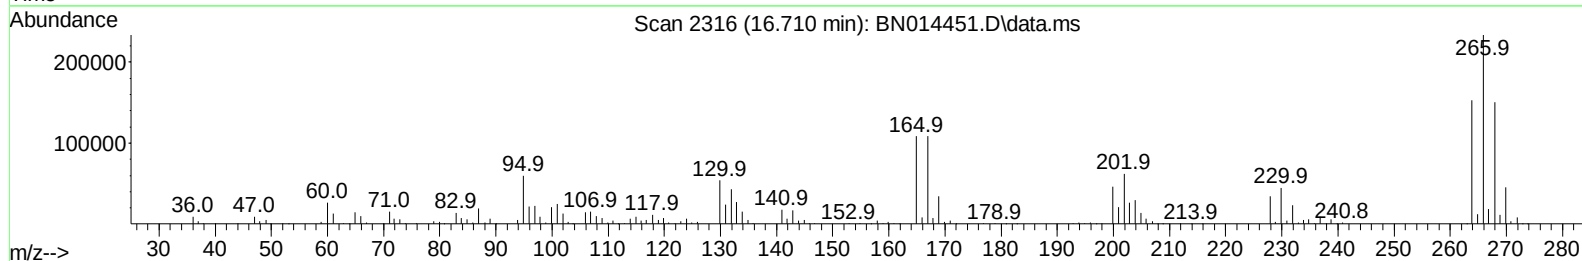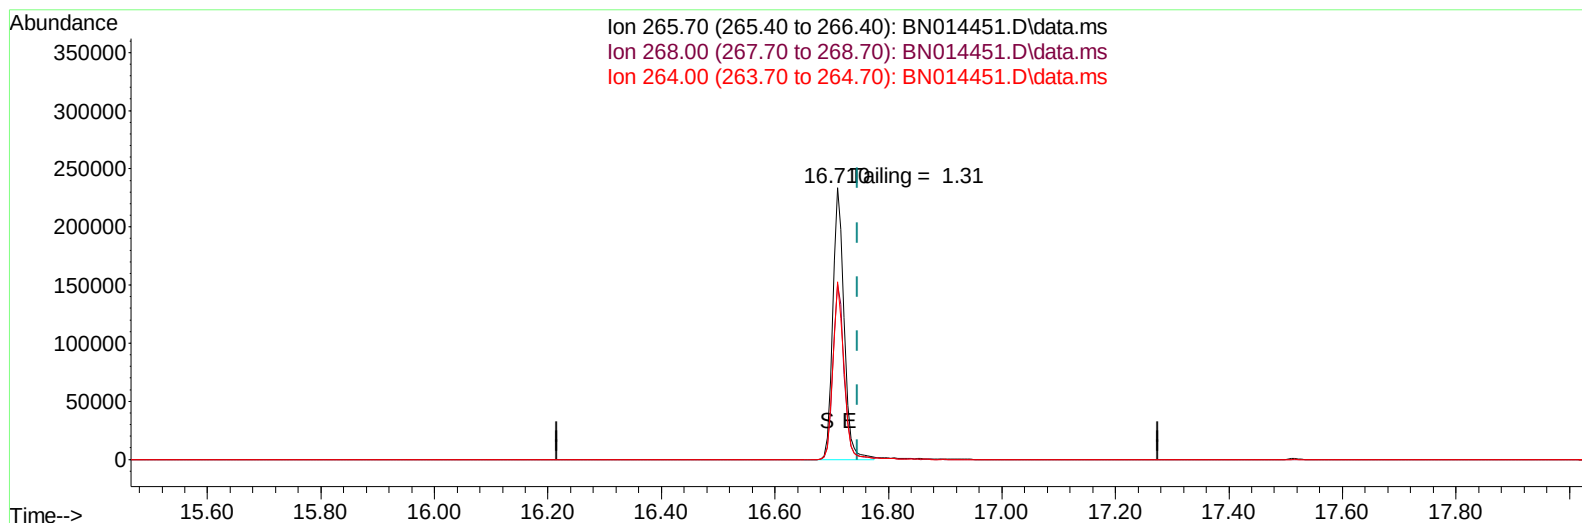

TIC: BN014451.D\data.ms

(70) Pentachlorophenol (C)

16.710min (-0.035) 22130.28 ng




response 325463

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.48
264.00	61.60	65.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042721\
Data File : BN014451.D
Acq On : 27 Apr 2021 09:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 27 11:17:25 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 09 09:55:03 2021
Response via : Initial Calibration

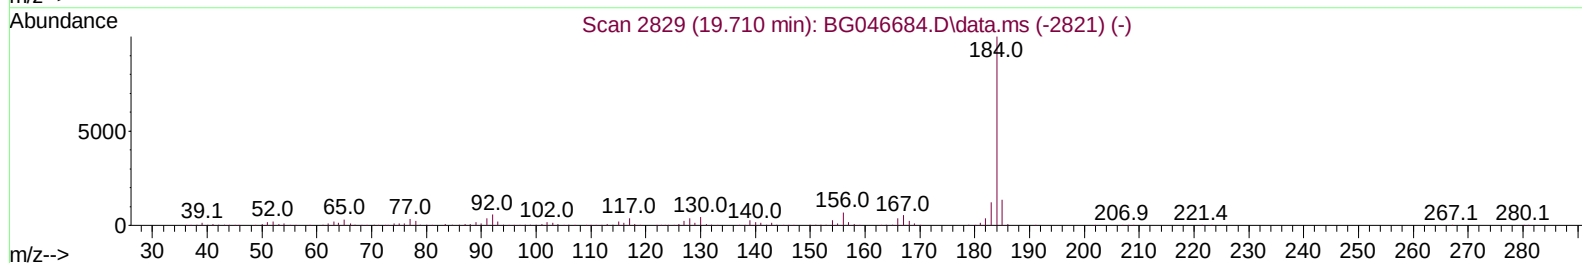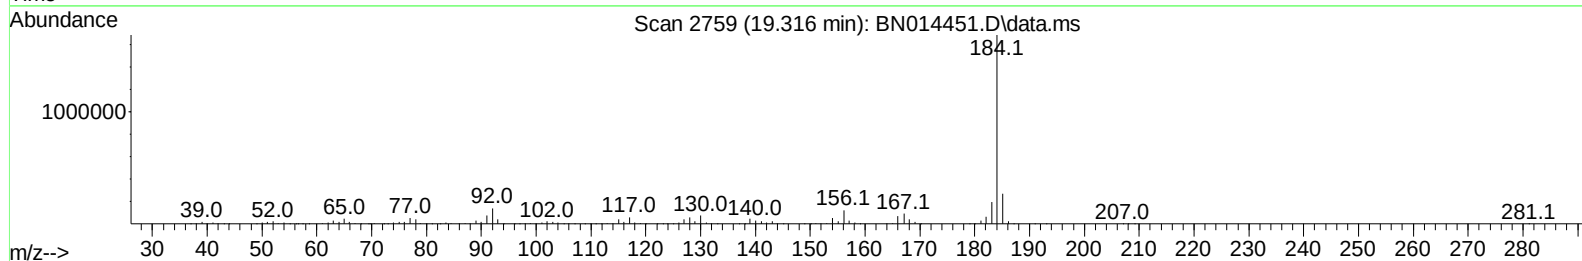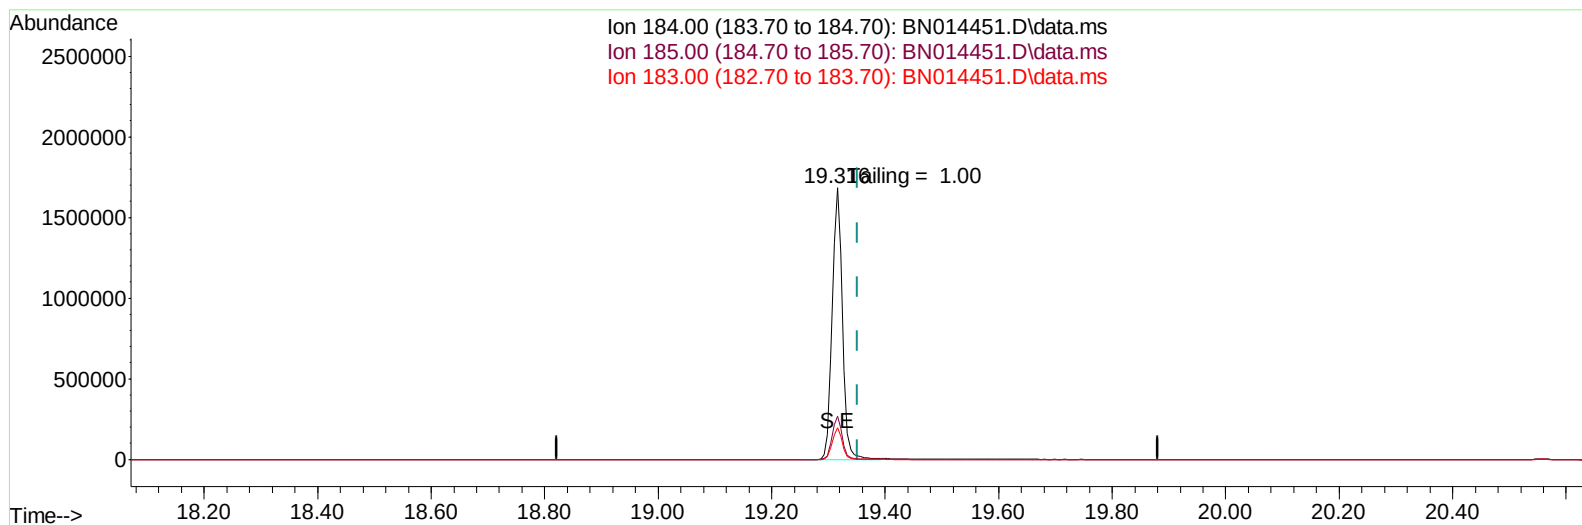

TIC: BN014451.D\data.ms

(77) Benzidine

19.316min (-0.035) 0.00 ng

response 2137484

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	16.04
183.00	13.20	11.67
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/27/2021	BNA_N	<u>BN014451.D</u>
Compound Name	Response	Retention Time
DDT	877074	20.557
DDD	9212	20.116
DDE	979	19.604
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10191	887265	1.15