

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042723\
 Data File : BN025168.D
 Acq On : 27 Apr 2023 09:25
 Operator : CG/JU
 Sample : PB152345BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK345

Quant Time: Apr 28 01:19:29 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 27 15:27:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.917	152	6607	0.400	ng/ul	0.00
4) Naphthalene-d8	10.726	136	21352	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.561	164	13056	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.309	188	27684	0.400	ng/ul	0.00
17) Chrysene-d12	21.502	240	20101	0.400	ng/ul	0.00
23) Perylene-d12	23.926	264	20458	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	40347	5.898	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.321	152	8806	0.321	ng/ul	0.00
18) Fluoranthene-d10	19.335	212	19249	0.363	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.551	166	3219	0.070	ng/ul#	14
20) Pyrene	19.702	202	3079	0.041	ng/ul#	1
26) Benzo(a)pyrene	23.762	252	6041	0.088	ng/ul#	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042723\
Data File : BN025168.D
Acq On : 27 Apr 2023 09:25
Operator : CG/JU
Sample : PB152345BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK345

Quant Time: Apr 28 01:19:29 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 27 15:27:43 2023
Response via : Initial Calibration

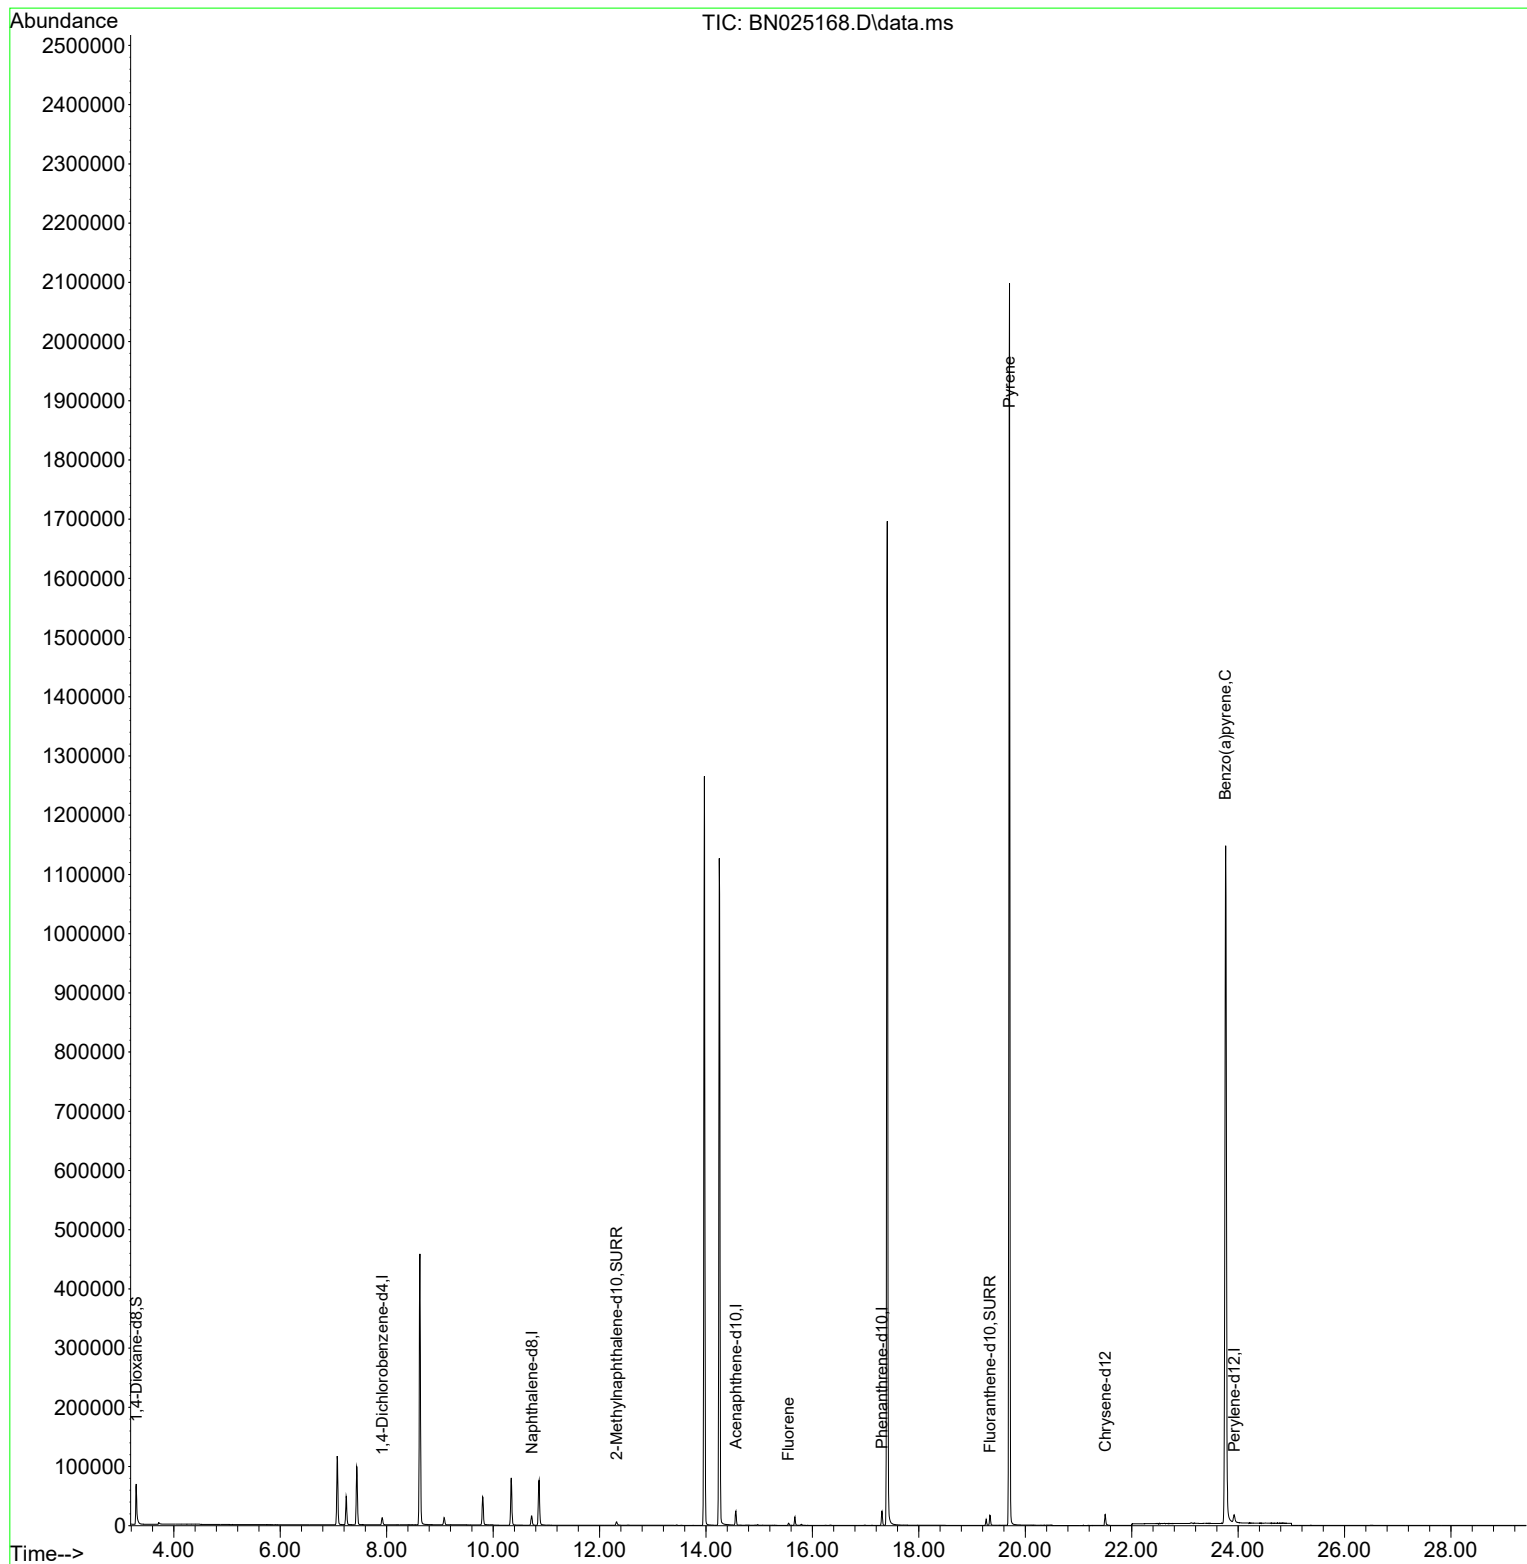

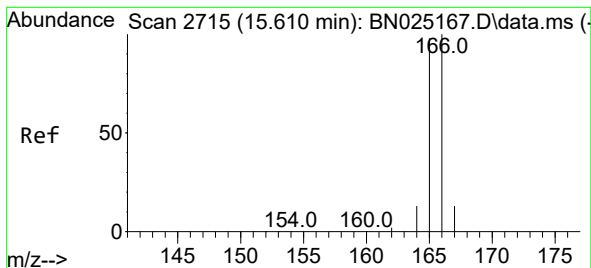

#12

Fluorene

Concen: 0.070 ng/ul

RT: 15.551 min Scan# 21

Delta R.T. -0.060 min

Lab File: BN025168.D

Acq: 27 Apr 2023 09:25

Instrument :

BNA_N

ClientSampleId :

SBLK345





Tgt Ion:166 Resp: 3219

Ion Ratio Lower Upper

166 100

165 7.5 78.1 117.1#

167 32.0 11.0 16.6#

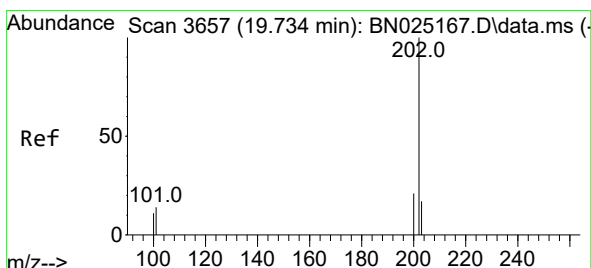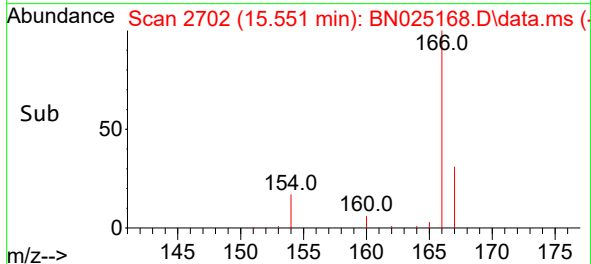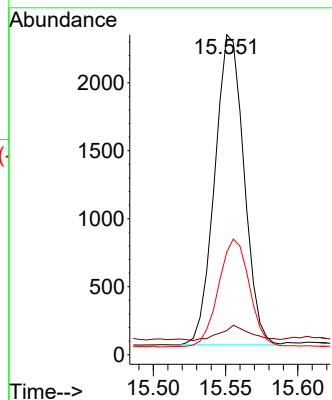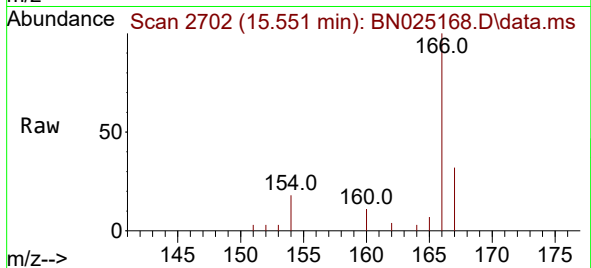

#20

Pyrene

Concen: 0.041 ng/ul

RT: 19.702 min Scan# 3650

Delta R.T. -0.032 min

Lab File: BN025168.D

Acq: 27 Apr 2023 09:25




Tgt Ion:202 Resp: 3079


Ion Ratio Lower Upper

202 100

101 171.3 11.3 16.9#


100 1264.7 9.2 13.8#

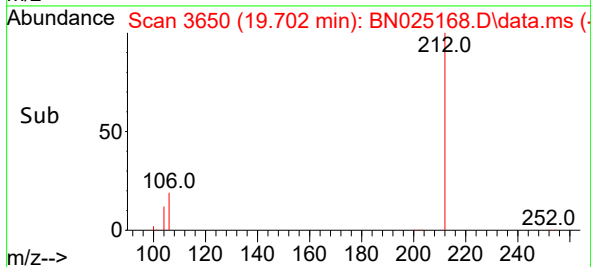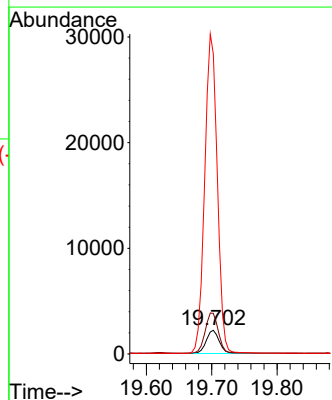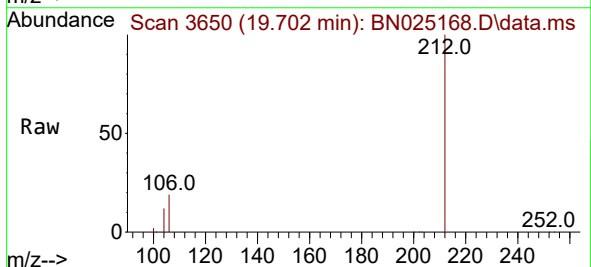

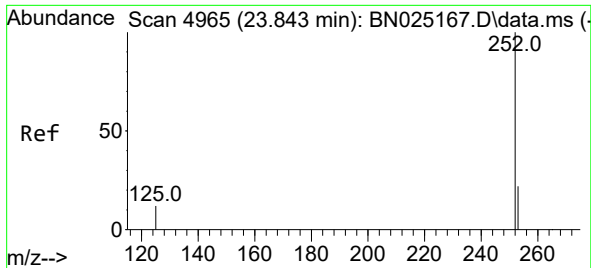

#26
 Benzo(a)pyrene
 Concen: 0.088 ng/ul
 RT: 23.762 min Scan# 4937
 Delta R.T. -0.081 min
 Lab File: BN025168.D
 Acq: 27 Apr 2023 09:25

Instrument :
 BNA_N
 ClientSampleId :
 SBLK345

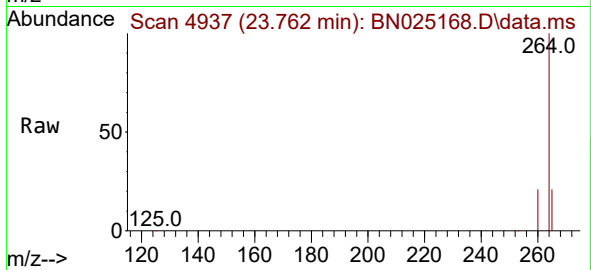

Tgt Ion:252 Resp: 6041
 Ion Ratio Lower Upper
 252 100
 253 44.9 21.4 32.2#
 125 38.5 14.6 22.0#

