

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042723\
 Data File : BN025181.D
 Acq On : 27 Apr 2023 17:09
 Operator : CG/JU
 Sample : PB152345BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Apr 28 01:49:23 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 27 15:27:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.917	152	8608	0.400	ng/ul	0.00
4) Naphthalene-d8	10.726	136	29106	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.561	164	17865	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.309	188	37061	0.400	ng/ul	0.00
17) Chrysene-d12	21.502	240	27781	0.400	ng/ul	0.00
23) Perylene-d12	23.934	264	25376	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	48026	5.388	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.315	152	11885	0.318	ng/ul	0.00
18) Fluoranthene-d10	19.335	212	26075	0.356	ng/ul	0.00
Target Compounds						
					Qvalue	
10) Acenaphthylene	14.283	152	1887	0.028	ng/ul#	74
20) Pyrene	19.703	202	4204	0.041	ng/ul#	1
26) Benzo(a)pyrene	23.777	252	6652	0.078	ng/ul#	38


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042723\
Data File : BN025181.D
Acq On : 27 Apr 2023 17:09
Operator : CG/JU
Sample : PB152345BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 28 01:49:23 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 27 15:27:43 2023
Response via : Initial Calibration




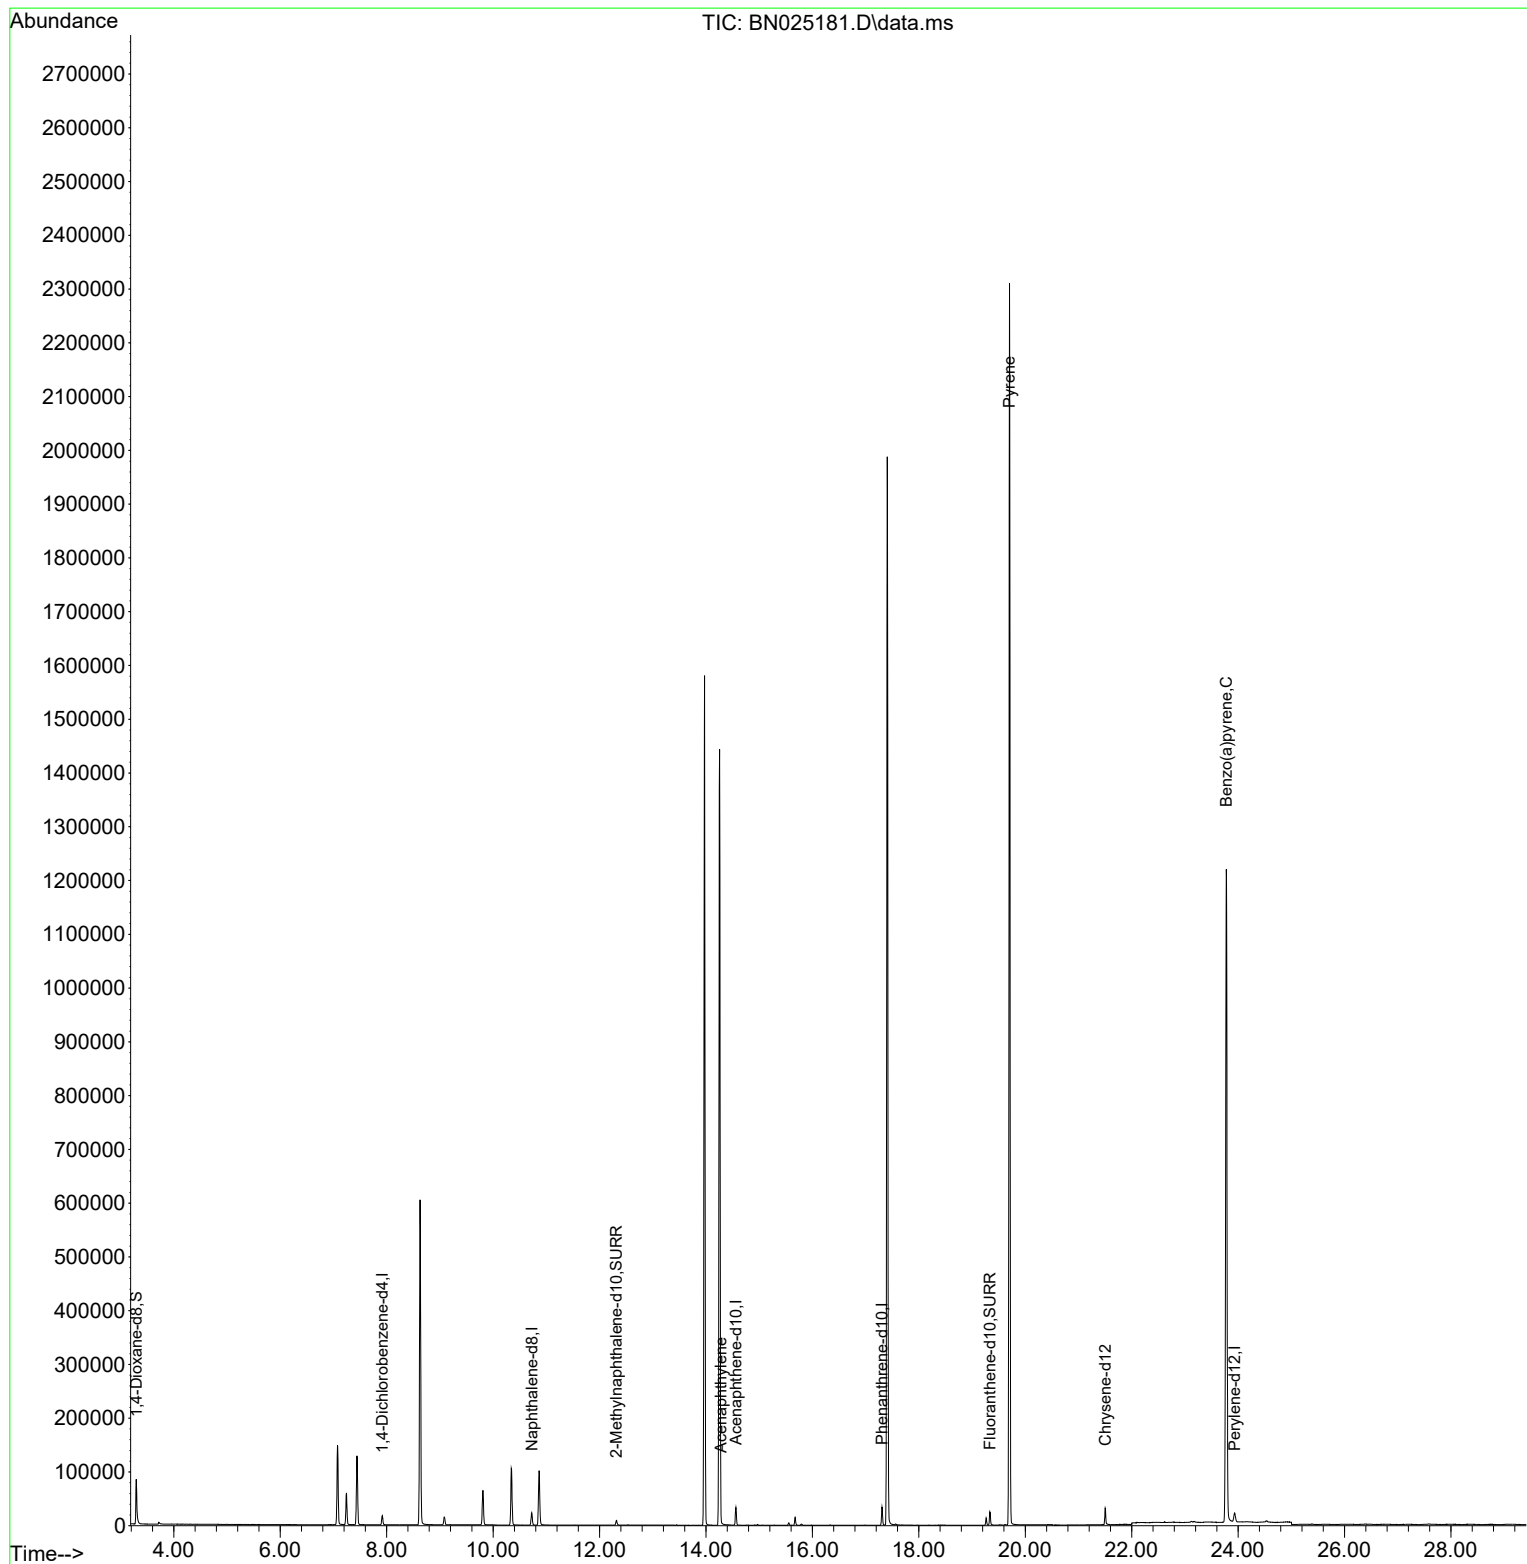


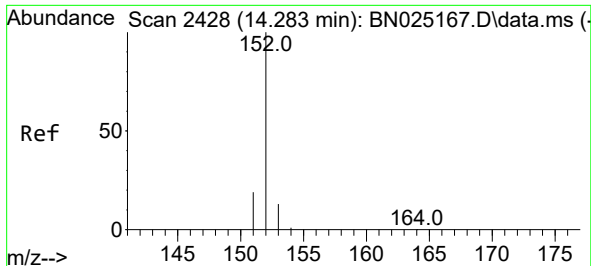

#10
Acenaphthylene
Concen: 0.028 ng/ul
RT: 14.283 min Scan# 2428
Delta R.T. 0.001 min
Lab File: BN025181.D
Acq: 27 Apr 2023 17:09




Instrument :
BNA_N
ClientSampleId :
DFTPP


Tgt Ion:152 Resp: 1887
Ion Ratio Lower Upper
152 100
151 29.9 16.0 24.0#
153 26.8 10.8 16.2#

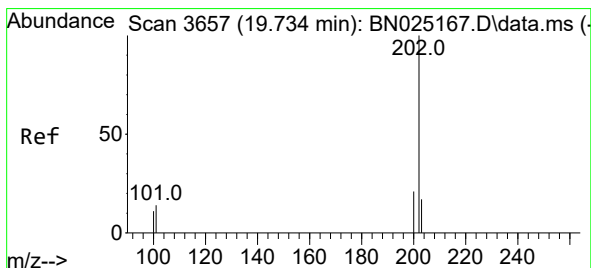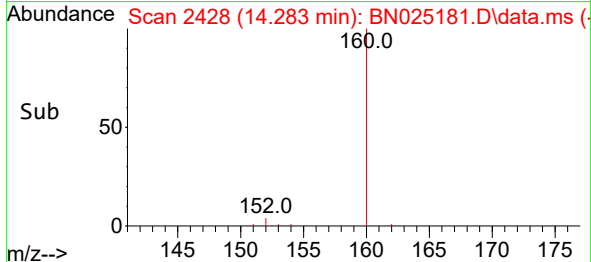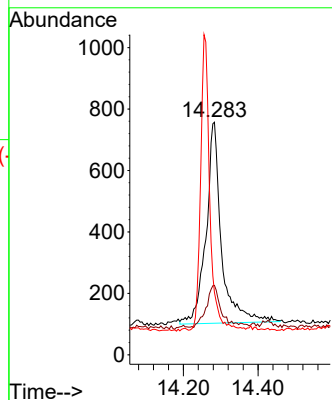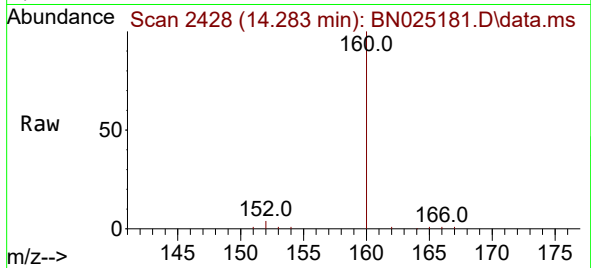

#20
Pyrene
Concen: 0.041 ng/ul
RT: 19.703 min Scan# 3650
Delta R.T. -0.032 min
Lab File: BN025181.D
Acq: 27 Apr 2023 17:09


Tgt Ion:202 Resp: 4204
Ion Ratio Lower Upper
202 100
101 170.3 11.3 16.9#
100 1261.3 9.2 13.8#

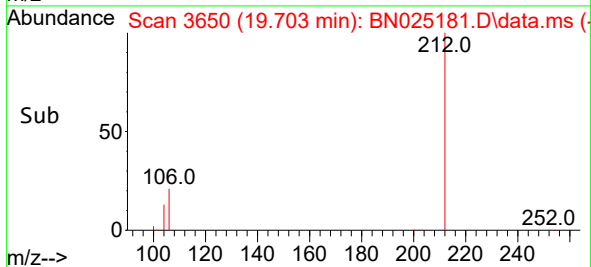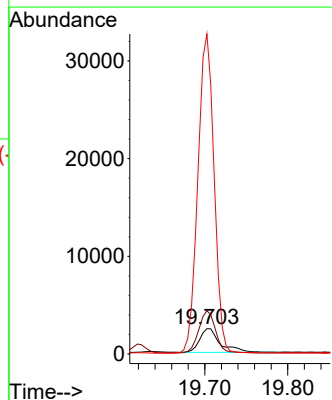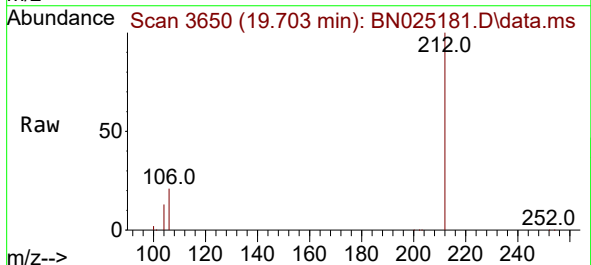

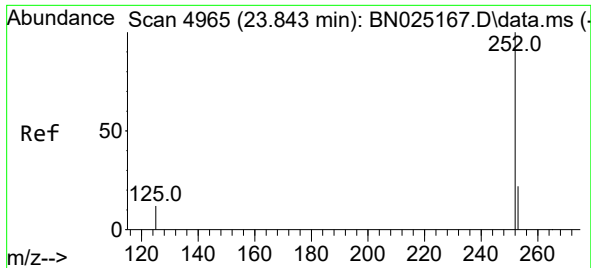

#26
 Benzo(a)pyrene
 Concen: 0.078 ng/ul
 RT: 23.777 min Scan# 4942
 Delta R.T. -0.066 min
 Lab File: BN025181.D
 Acq: 27 Apr 2023 17:09

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

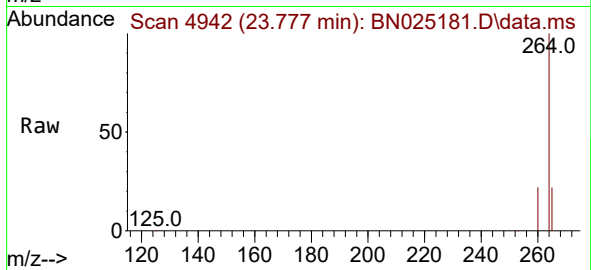

Tgt Ion:252 Resp: 6652
 Ion Ratio Lower Upper
 252 100
 253 50.2 21.4 32.2#
 125 56.5 14.6 22.0#

