

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042723\
 Data File : BN025169.D
 Acq On : 27 Apr 2023 10:01
 Operator : CG/JU
 Sample : 02418-05
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW8Z1

Manual Integrations
 APPROVED

Reviewed By : Christian Giraldo 04/28/2023
 Supervised By : Jagrut Upadhyay 05/01/2023

Quant Time: Apr 28 01:19:35 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 27 15:27:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.917	152	7472	0.400	ng/ul	0.00
4) Naphthalene-d8	10.726	136	23649	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.561	164	14657	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.309	188	31814	0.400	ng/ul	0.00
17) Chrysene-d12	21.506	240	25043	0.400	ng/ul	0.00
23) Perylene-d12	23.926	264	24405	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	34763	4.493	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.315	152	8674	0.286	ng/ul	0.00
18) Fluoranthene-d10	19.335	212	21163	0.320	ng/ul	0.00
Target Compounds						
					Qvalue	
15) Phenanthrene	17.347	178	2652	0.030	ng/ul#	88
19) Fluoranthene	19.368	202	5431	0.060	ng/ul#	93
20) Pyrene	19.731	202	5297	0.057	ng/ul#	89
21) Benzo(a)anthracene	21.488	228	2470	0.033	ng/ul#	91
22) Chrysene	21.541	228	2883	0.035	ng/ul#	93
24) Benzo(b)fluoranthene	23.189	252	3725m	0.038	ng/ul	
26) Benzo(a)pyrene	23.815	252	2308	0.028	ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042723\
Data File : BN025169.D
Acq On : 27 Apr 2023 10:01
Operator : CG/JU
Sample : 02418-05
Misc :
ALS Vial : 4 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
EW8Z1

Manual Integrations
APPROVED

Reviewed By : Christian Giraldo 04/28/2023
Supervised By : Jagrut Upadhyay 05/01/2023


Quant Time: Apr 28 01:19:35 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 27 15:27:43 2023
Response via : Initial Calibration

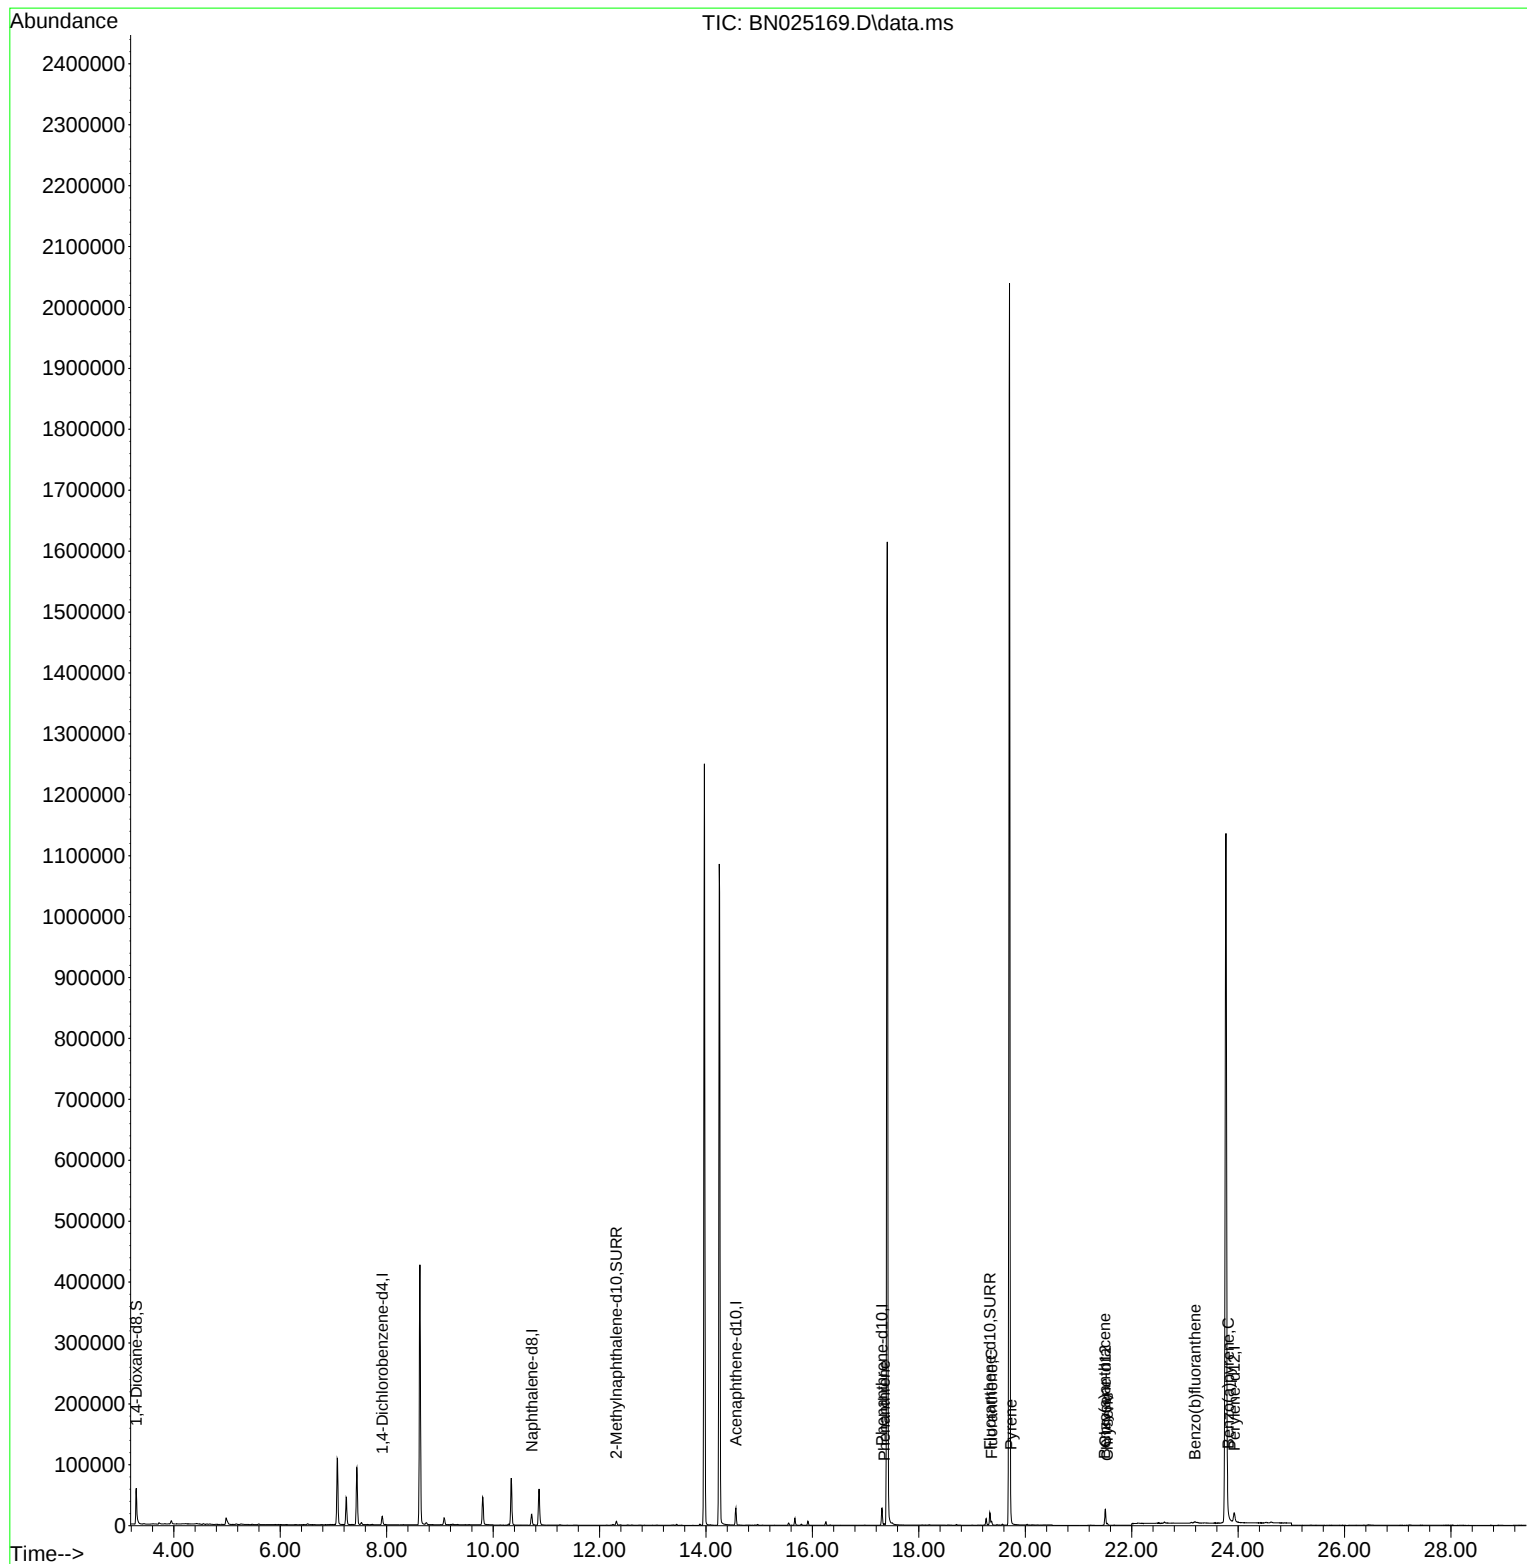

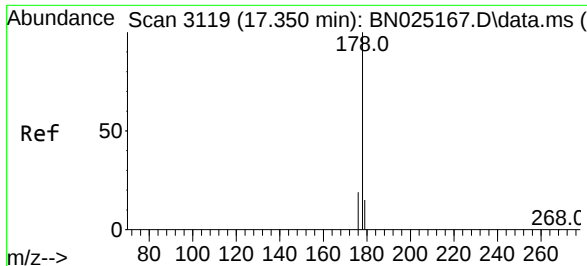

#15
Phenanthrene
Concen: 0.030 ng/ul
RT: 17.347 min Scan# 3118
Delta R.T. -0.004 min
Lab File: BN025169.D
Acq: 27 Apr 2023 10:01




Instrument :
BNA_N
ClientSampleId :
EW8Z1

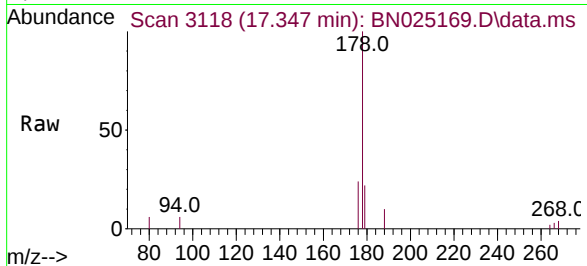

Tgt Ion:178 Resp: 2652
Ion Ratio Lower Upper
178 100
179 22.2 12.5 18.7#
176 23.5 15.6 23.4#




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 04/28/2023
Supervised By :Jagrut Upadhyay 05/01/2023

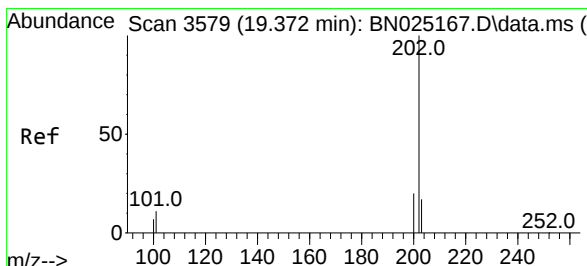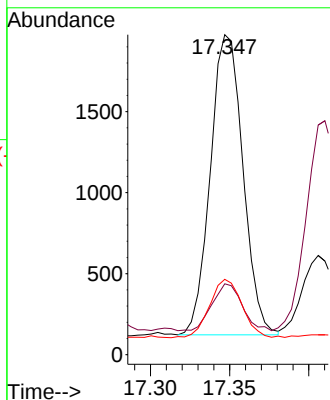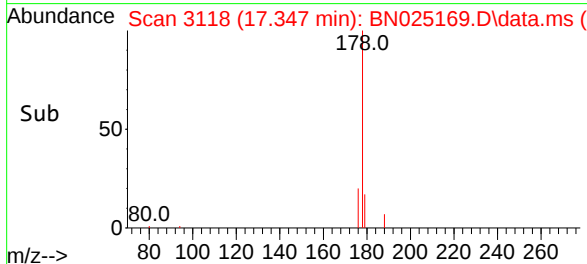

#19
Fluoranthene
Concen: 0.060 ng/ul
RT: 19.368 min Scan# 3578
Delta R.T. -0.004 min
Lab File: BN025169.D
Acq: 27 Apr 2023 10:01

Tgt Ion:202 Resp: 5431
Ion Ratio Lower Upper
202 100
101 15.0 9.7 14.5#
100 11.6 7.3 10.9#

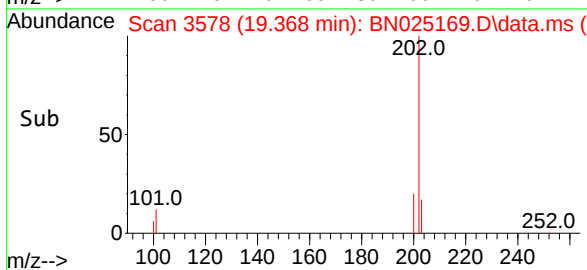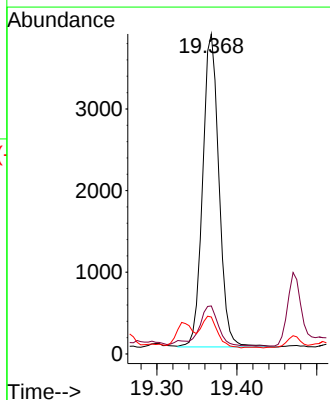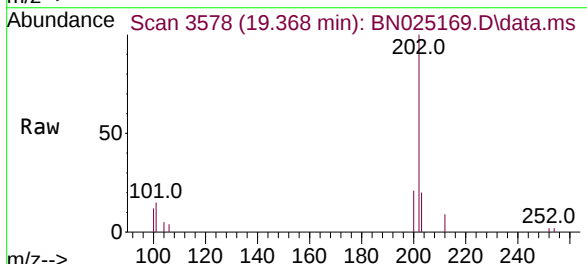

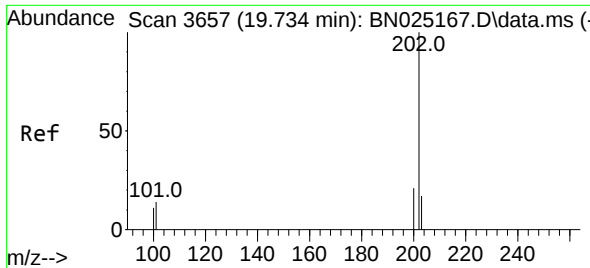





#20
Pyrene
Concen: 0.057 ng/ul
RT: 19.731 min Scan# 3656
Delta R.T. -0.004 min
Lab File: BN025169.D
Acq: 27 Apr 2023 10:01

Instrument :
BNA_N
ClientSampleId :
EW8Z1

Tgt Ion:202 Resp: 5297
Ion Ratio Lower Upper
202 100
101 17.5 11.3 16.9
100 16.9 9.2 13.8




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 04/28/2023
Supervised By :Jagrut Upadhyay 05/01/2023

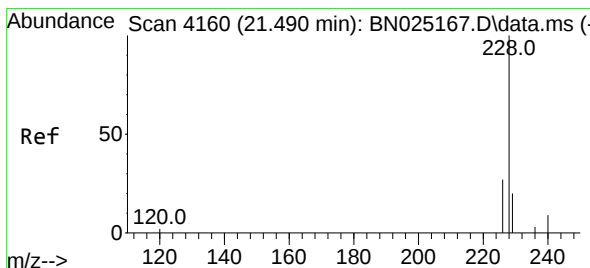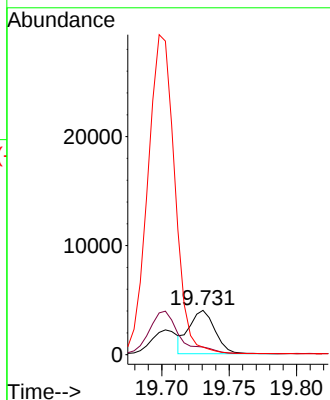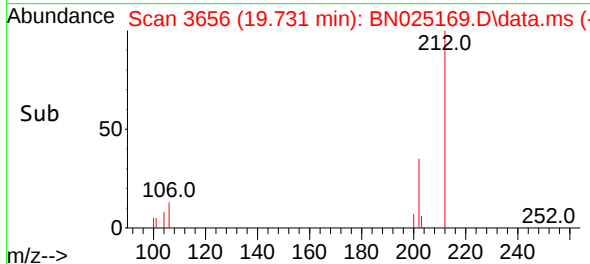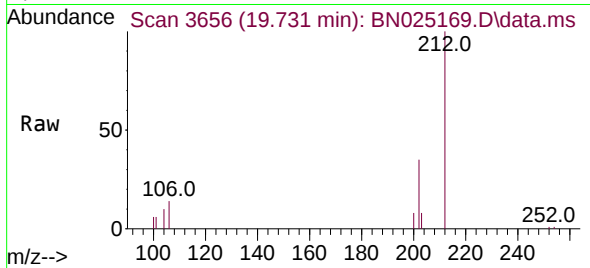

#21
Benzo(a)anthracene
Concen: 0.033 ng/ul
RT: 21.488 min Scan# 4159
Delta R.T. -0.002 min
Lab File: BN025169.D
Acq: 27 Apr 2023 10:01


Tgt Ion:228 Resp: 2470
Ion Ratio Lower Upper
228 100
229 25.2 15.6 23.4
226 31.2 22.1 33.1

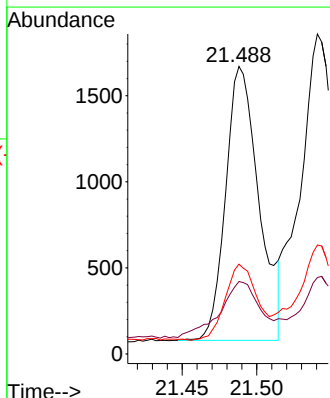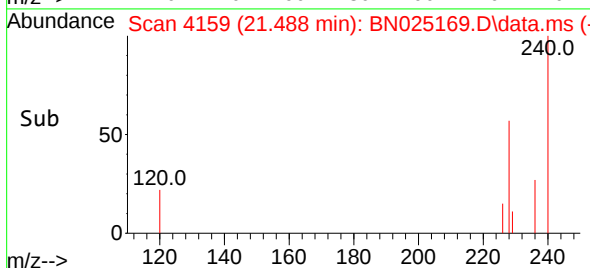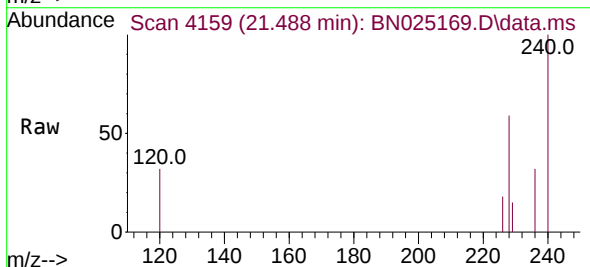

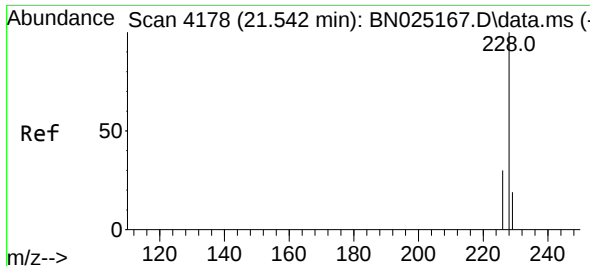

#22
Chrysene
Concen: 0.035 ng/ul
RT: 21.541 min Scan# 4178
Delta R.T. -0.002 min
Lab File: BN025169.D
Acq: 27 Apr 2023 10:01




Instrument :
BNA_N
ClientSampleId :
EW8Z1

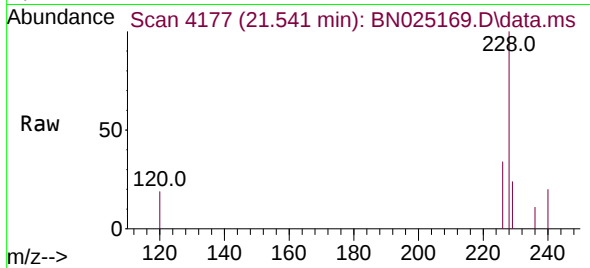


Tgt Ion:228 Resp: 288
Ion Ratio Lower Upper
228 100
226 34.1 24.5 36.7
229 23.9 15.8 23.6

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 04/28/2023
Supervised By :Jagrut Upadhyay 05/01/2023

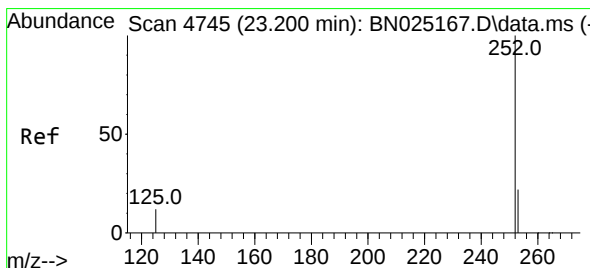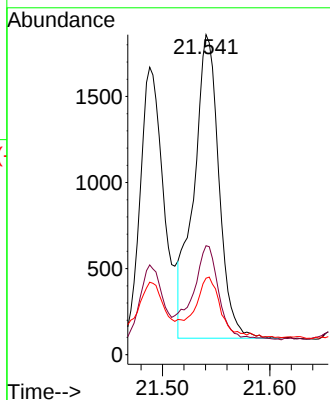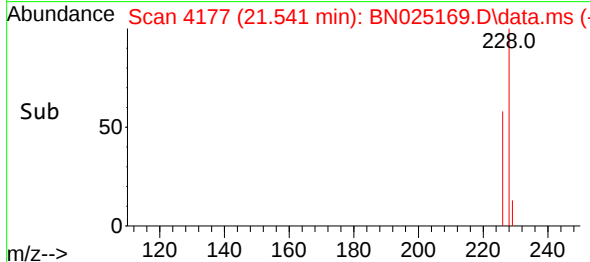


#24
Benzo(b)fluoranthene
Concen: 0.038 ng/ul m
RT: 23.189 min Scan# 4741
Delta R.T. -0.011 min
Lab File: BN025169.D
Acq: 27 Apr 2023 10:01

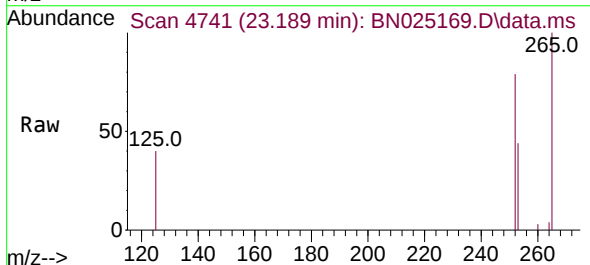


Tgt Ion:252 Resp: 3725
Ion Ratio Lower Upper
252 100
253 55.9 0.0 50.2#
125 50.9 0.0 30.4#

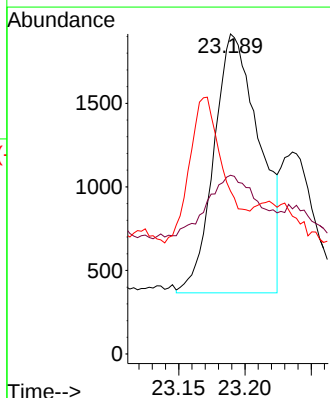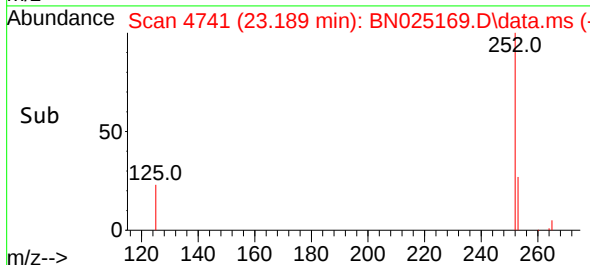

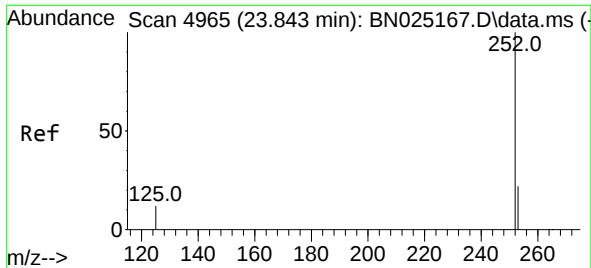

#26
Benzo(a)pyrene
Concen: 0.028 ng/ul
RT: 23.815 min Scan# 4965
Delta R.T. -0.028 min
Lab File: BN025169.D
Acq: 27 Apr 2023 10:01

Instrument :
BNA_N
ClientSampleId :
EW8Z1

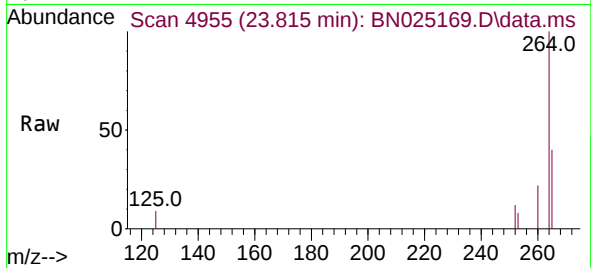

Tgt Ion:252 Resp: 2308
Ion Ratio Lower Upper
252 100
253 67.1 21.4 32.2
125 76.5 14.6 22.0

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 04/28/2023
Supervised By :Jagrut Upadhyay 05/01/2023

