

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042724\
 Data File : BN031282.D
 Acq On : 27 Apr 2024 22:40
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTD020387

Quant Time: Apr 28 21:17:01 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 26 22:57:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.616	152	254743	20.000	ng/ul	0.00
20) Naphthalene-d8	10.398	136	1247610	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.269	164	861011	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.021	188	1869164	20.000	ng/ul	0.00
79) Chrysene-d12	21.257	240	1694905	20.000	ng/ul	0.00
88) Perylene-d12	24.151	264	1809713	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.134	96	38942	7.142	ng/uL	0.00
4) Pyridine-d5	3.546	84	287404	18.303	ng/ul	0.00
7) Phenol-d5	6.798	99	377458	17.565	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.963	67	223346	17.864	ng/ul	0.00
11) 2-Chlorophenol-d4	7.151	132	300731	17.974	ng/ul	0.00
15) 4-Methylphenol-d8	8.328	113	323556	17.904	ng/ul	0.00
21) Nitrobenzene-d5	8.775	128	160682	17.925	ng/ul	0.00
24) 2-Nitrophenol-d4	9.492	143	175364	18.820	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.022	165	321350	17.488	ng/ul	0.00
31) 4-Chloroaniline-d4	10.545	131	491844	17.128	ng/ul	0.00
46) Dimethylphthalate-d6	13.686	166	1025327	17.113	ng/ul	0.00
49) Acenaphthylene-d8	13.957	160	1187320	17.487	ng/ul	0.00
54) 4-Nitrophenol-d4	14.486	143	208913	16.706	ng/ul	0.00
60) Fluorene-d10	15.263	176	885261	16.973	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.392	200	174319	18.485	ng/ul	0.00
73) Anthracene-d10	17.116	188	1378469	17.015	ng/ul	0.00
81) Pyrene-d10	19.421	212	1662152	19.957	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.951	264	1524245	17.761	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.169	88	40066	6.934	ng/uL	95
5) Pyridine	3.563	79	281918	17.791	ng/ul	95
6) Benzaldehyde	6.775	77	226224	21.440	ng/ul	94
8) Phenol	6.822	94	387208	17.477	ng/ul	99
10) Bis(2-Chloroethyl)ether	7.057	93	314704	18.003	ng/ul	100
12) 2-Chlorophenol	7.187	128	313339	18.016	ng/ul	98
13) 2-Methylphenol	8.063	108	306843	17.872	ng/ul	99
14) 2,2'-oxybis(1-Chloropr...	8.140	45	417740	18.329	ng/ul	99
16) Acetophenone	8.440	105	505916	18.068	ng/ul	98
17) N-Nitroso-di-n-propyla...	8.428	70	254769	18.254	ng/ul	98
18) 4-Methylphenol	8.393	108	340858	17.724	ng/ul	97
19) Hexachloroethane	8.681	117	126789	17.568	ng/ul	96
22) Nitrobenzene	8.816	77	371490	17.559	ng/ul	97
23) Isophorone	9.340	82	754919	17.485	ng/ul	100
25) 2-Nitrophenol	9.522	139	191775	18.602	ng/ul	95
26) 2,4-Dimethylphenol	9.587	107	362535	17.243	ng/ul	98
27) Bis(2-Chloroethoxy)met...	9.828	93	458235	17.473	ng/ul	100
29) 2,4-Dichlorophenol	10.051	162	321192	17.501	ng/ul	100
30) Naphthalene	10.451	128	1093668	16.915	ng/ul	99
32) 4-Chloroaniline	10.569	127	467202	16.745	ng/ul	99
33) Hexachlorobutadiene	10.728	225	192170	17.176	ng/ul	99
34) Caprolactam	11.351	113	120454	16.658	ng/ul	96
35) 4-Chloro-3-methylphenol	11.698	107	373605	17.557	ng/ul	96
36) 2-Methylnaphthalene	12.069	142	780389	17.115	ng/ul	96


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042724\
 Data File : BN031282.D
 Acq On : 27 Apr 2024 22:40
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTD020387

Quant Time: Apr 28 21:17:01 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 26 22:57:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.292	142	788624	17.093	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.439	216	394949	17.530	ng/ul	99
40) Hexachlorocyclopentadiene	12.410	237	206685	16.700	ng/ul	95
41) 2,4,6-Trichlorophenol	12.686	196	272705	18.185	ng/ul	93
42) 2,4,5-Trichlorophenol	12.763	196	294774	17.729	ng/ul	98
43) 1,1'-Biphenyl	13.092	154	1042586	17.606	ng/ul	98
44) 2-Chloronaphthalene	13.133	162	811695	17.154	ng/ul	99
45) 2-Nitroaniline	13.351	65	238930	18.290	ng/ul	98
47) Dimethylphthalate	13.733	163	1061902	17.180	ng/ul	100
48) 2,6-Dinitrotoluene	13.857	165	217926	18.782	ng/ul	99
50) Acenaphthylene	13.986	152	1353935	17.071	ng/ul	99
51) 3-Nitroaniline	14.186	138	243518	18.281	ng/ul	97
52) Acenaphthene	14.333	153	896929	17.060	ng/ul	98
53) 2,4-Dinitrophenol	14.392	184	111517	16.995	ng/ul	99
55) 4-Nitrophenol	14.504	109	167229	16.478	ng/ul	98
56) Dibenzofuran	14.669	168	1219693	16.779	ng/ul	99
57) 2,4-Dinitrotoluene	14.645	165	320500	18.179	ng/ul	98
58) 2,3,4,6-Tetrachlorophenol	14.898	232	252136	17.547	ng/ul	93
59) Diethylphthalate	15.104	149	1107549	17.423	ng/ul	100
61) Fluorene	15.322	166	996628	16.660	ng/ul	96
62) 4-Chlorophenyl-phenyle...	15.322	204	486801	17.085	ng/ul	95
63) 4-Nitroaniline	15.357	138	241495	16.815	ng/ul	99
66) 4,6-Dinitro-2-methylph...	15.410	198	183770	18.148	ng/ul#	96
67) N-Nitrosodiphenylamine	15.539	169	874716	17.459	ng/ul	99
68) 4-Bromophenyl-phenylether	16.216	248	317738	17.975	ng/ul	90
69) Hexachlorobenzene	16.322	284	359130	17.623	ng/ul	94
70) Atrazine	16.498	200	313124	17.802	ng/ul	97
71) Pentachlorophenol	16.669	266	227947	17.216	ng/ul	98
72) Phenanthrene	17.063	178	1649554	16.685	ng/ul	99
74) Anthracene	17.151	178	1687075	16.862	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.057	216	401301	18.304	ng/ul	99
76) Pentachlorobenzene	14.580	250	399248	17.635	ng/ul	97
77) Carbazole	17.427	167	1565706	17.132	ng/ul	98
78) Di-n-butylphthalate	17.992	149	1975218	17.732	ng/ul	99
80) Fluoranthene	19.086	202	1977198	20.059	ng/ul	99
82) Pyrene	19.451	202	2070077	19.987	ng/ul	98
83) Butylbenzylphthalate	20.362	149	928077	20.308	ng/ul	98
84) 3,3'-Dichlorobenzidine	21.174	252	633458	17.937	ng/ul	96
85) Benzo(a)anthracene	21.239	228	2034627	17.678	ng/ul	98
86) Bis(2-ethylhexyl)phtha...	21.168	149	1323943	19.295	ng/ul	99
87) Chrysene	21.298	228	1865373	17.074	ng/ul	98
89) Di-n-octyl phthalate	22.262	149	2367625	22.697	ng/ul	100
90) Benzo(b)fluoranthene	23.239	252	1868756	18.353	ng/ul	99
91) Benzo(k)fluoranthene	23.292	252	1944286	18.985	ng/ul	99
93) Benzo(a)pyrene	24.015	252	1787713	17.599	ng/ul	96
94) Indeno(1,2,3-cd)pyrene	27.392	276	1946963	15.446	ng/ul	100
95) Dibenzo(a,h)anthracene	27.450	278	1612745	15.588	ng/ul	96
96) Benzo(g,h,i)perylene	28.403	276	1527209	15.045	ng/ul	99





(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2
1,4-Dioxane
Concen: 6.934 ng/uL
RT: 3.169 min Scan# 31
Delta R.T. -0.006 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40




Instrument :
BNA_N
ClientSampleId :
SSTD020387


Tgt Ion: 88 Resp: 40066
Ion Ratio Lower Upper
88 100
43 27.1 22.2 33.2
58 67.6 50.2 75.2

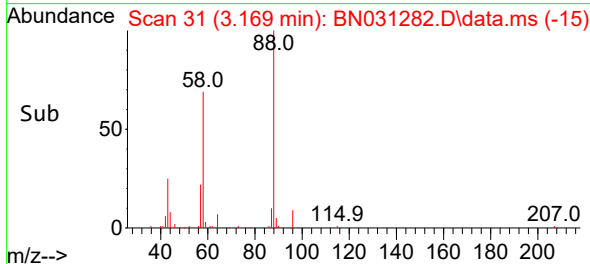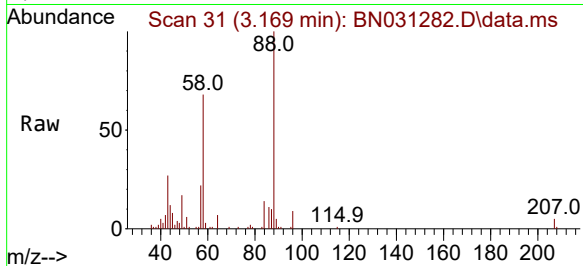

#5
Pyridine
Concen: 17.791 ng/uL
RT: 3.563 min Scan# 98
Delta R.T. -0.000 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40

Tgt Ion: 79 Resp: 281918
Ion Ratio Lower Upper
79 100
52 70.5 59.9 89.9
51 33.3 29.0 43.6




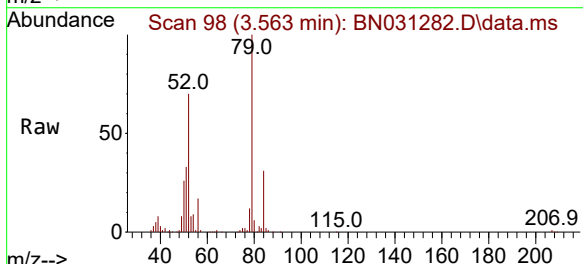




#6
Benzaldehyde
Concen: 21.440 ng/ul
RT: 6.775 min Scan# 644
Delta R.T. -0.000 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40




Instrument :
BNA_N
ClientSampleId :
SSTD020387


Tgt Ion: 77 Resp: 226224
Ion Ratio Lower Upper
77 100
105 103.8 80.0 120.0
106 101.8 75.0 112.6

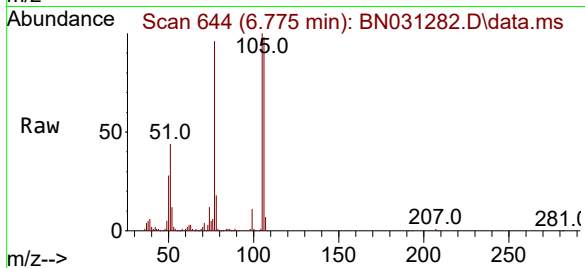

#8
Phenol
Concen: 17.477 ng/ul
RT: 6.822 min Scan# 652
Delta R.T. -0.006 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40

Tgt Ion: 94 Resp: 387208
Ion Ratio Lower Upper
94 100
65 27.0 22.0 33.0
66 38.0 29.8 44.6


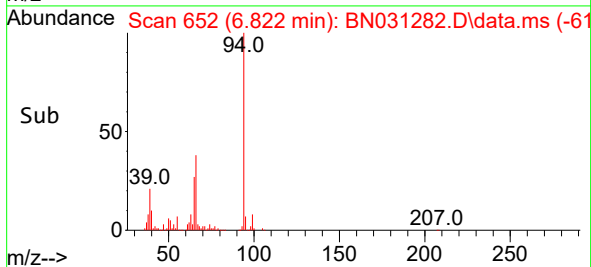

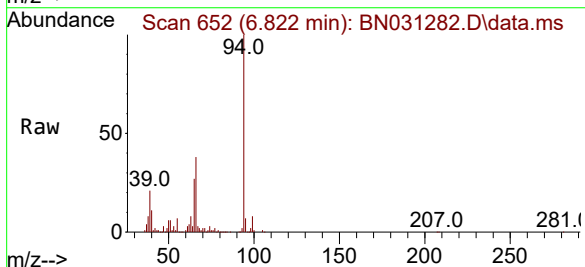




#10
Bis(2-Chloroethyl)ether
Concen: 18.003 ng/ul
RT: 7.057 min Scan# 692
Delta R.T. -0.000 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40




Instrument :
BNA_N
ClientSampleId :
SSTD020387


Tgt Ion: 93 Resp: 314704
Ion Ratio Lower Upper
93 100
63 71.5 57.1 85.7
95 31.6 24.9 37.3

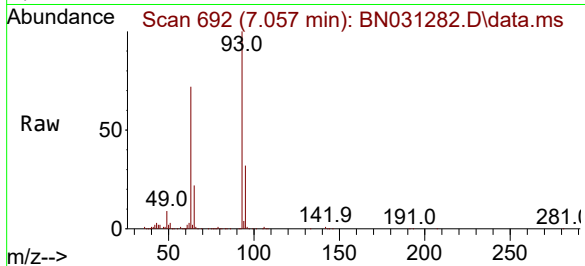

#12
2-Chlorophenol
Concen: 18.016 ng/ul
RT: 7.187 min Scan# 714
Delta R.T. -0.000 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40

Tgt Ion:128 Resp: 313339
Ion Ratio Lower Upper
128 100
64 42.2 34.9 52.3
130 32.7 27.0 40.4

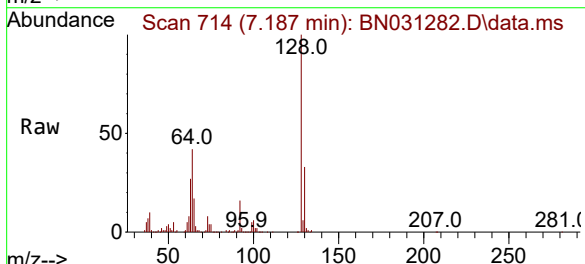



#13

2-Methylphenol

Concen: 17.872 ng/ul

RT: 8.063 min Scan# 8

Delta R.T. -0.006 min

Lab File: BN031282.D

Acq: 27 Apr 2024 22:40

Instrument :

BNA_N

ClientSampleId :





SSTD020387

Tgt Ion:108 Resp: 306843

Ion Ratio Lower Upper

108 100

107 87.0 70.1 105.1

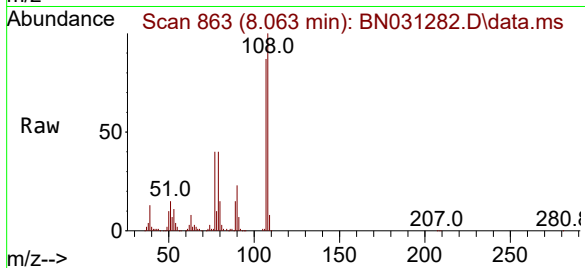

#14

2,2'-oxybis(1-Chloropropane)

Concen: 18.329 ng/ul

RT: 8.140 min Scan# 876

Delta R.T. -0.006 min

Lab File: BN031282.D

Acq: 27 Apr 2024 22:40




Tgt Ion: 45 Resp: 417740


Ion Ratio Lower Upper

45 100

77 15.6 12.5 18.7

79 11.2 9.6 14.4




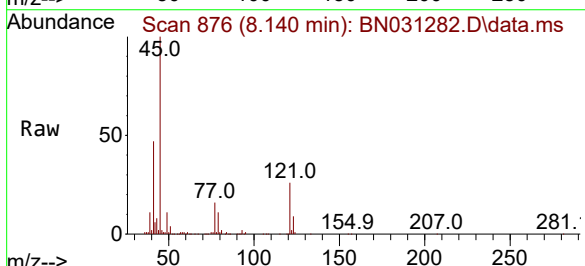




#16
Acetophenone
Concen: 18.068 ng/ul
RT: 8.440 min Scan# 91
Delta R.T. -0.006 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40




Instrument :
BNA_N
ClientSampleId :
SSTD020387


Tgt Ion:105 Resp: 505916
Ion Ratio Lower Upper
105 100
77 74.0 60.2 90.4
51 24.9 20.6 31.0



#17
N-Nitroso-di-n-propylamine
Concen: 18.254 ng/ul
RT: 8.428 min Scan# 925
Delta R.T. -0.006 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40

Tgt Ion: 70 Resp: 254769
Ion Ratio Lower Upper
70 100
42 54.9 45.0 67.6
101 10.4 8.1 12.1
130 23.2 19.2 28.8





#18

4-Methylphenol

Concen: 17.724 ng/ul

RT: 8.393 min Scan# 919

Delta R.T. -0.006 min

Lab File: BN031282.D

Acq: 27 Apr 2024 22:40

Instrument :

BNA_N

ClientSampleId :





SSTD020387

Tgt Ion:108 Resp: 340858

Ion Ratio Lower Upper

108 100

107 108.6 89.8 134.8



#19

Hexachloroethane

Concen: 17.568 ng/ul

RT: 8.681 min Scan# 968

Delta R.T. -0.006 min

Lab File: BN031282.D

Acq: 27 Apr 2024 22:40




Tgt Ion:117 Resp: 126789


Ion Ratio Lower Upper

117 100

201 93.5 77.4 116.0

199 58.6 49.6 74.4









#22
Nitrobenzene
Concen: 17.559 ng/ul
RT: 8.816 min Scan# 991
Delta R.T. -0.006 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40




Instrument :
BNA_N
ClientSampleId :
SSTD020387


Tgt Ion: 77 Resp: 371490
Ion Ratio Lower Upper
77 100
123 45.6 38.2 57.2
65 13.0 10.7 16.1

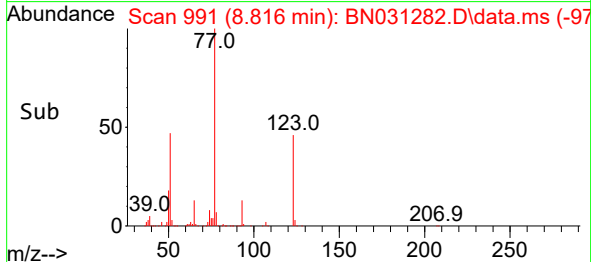

#23
Isophorone
Concen: 17.485 ng/ul
RT: 9.340 min Scan# 1080
Delta R.T. -0.006 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40

Tgt Ion: 82 Resp: 754919
Ion Ratio Lower Upper
82 100
95 7.3 5.9 8.9
138 18.3 14.7 22.1


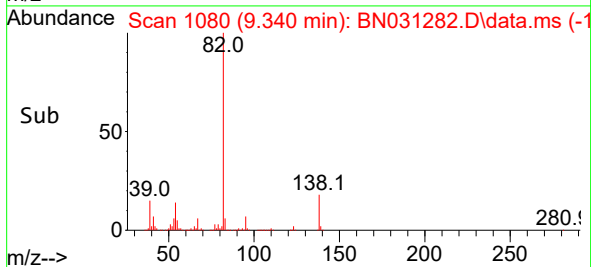

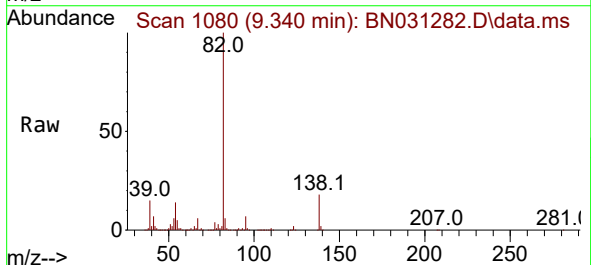




#25
2-Nitrophenol
Concen: 18.602 ng/ul
RT: 9.522 min Scan# 1111
Delta R.T. -0.006 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40




Instrument :
BNA_N
ClientSampleId :
SSTD020387


Tgt Ion:139 Resp: 191775
Ion Ratio Lower Upper
139 100
65 49.3 35.2 52.8
109 32.2 25.4 38.0

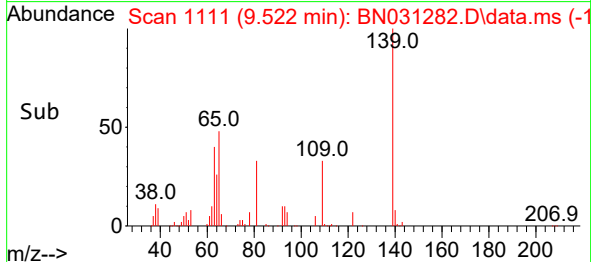

#26
2,4-Dimethylphenol
Concen: 17.243 ng/ul
RT: 9.587 min Scan# 1122
Delta R.T. -0.000 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40

Tgt Ion:107 Resp: 362535
Ion Ratio Lower Upper
107 100
121 50.8 40.3 60.5
122 89.3 69.8 104.8

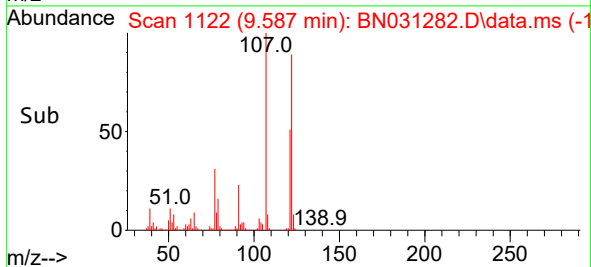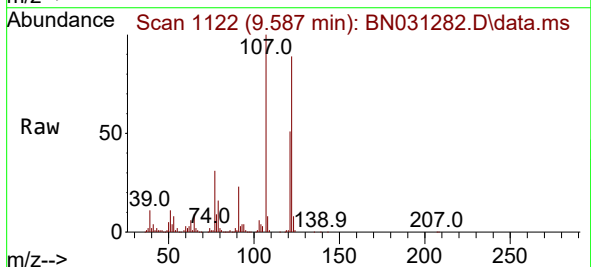



#27

Bis(2-Chloroethoxy)methane

Concen: 17.473 ng/ul

RT: 9.828 min Scan# 1163

Delta R.T. -0.000 min

Lab File: BN031282.D

Acq: 27 Apr 2024 22:40

Instrument :

BNA_N

ClientSampleId :

SSTD020387





Tgt Ion: 93 Resp: 458235

Ion Ratio Lower Upper

93 100

95 32.1 25.8 38.6

123 11.8 9.8 14.6



#29

2,4-Dichlorophenol

Concen: 17.501 ng/ul

RT: 10.051 min Scan# 1201

Delta R.T. -0.006 min

Lab File: BN031282.D

Acq: 27 Apr 2024 22:40




Tgt Ion:162 Resp: 321192


Ion Ratio Lower Upper

162 100

164 63.9 51.0 76.6

98 35.7 28.6 42.8







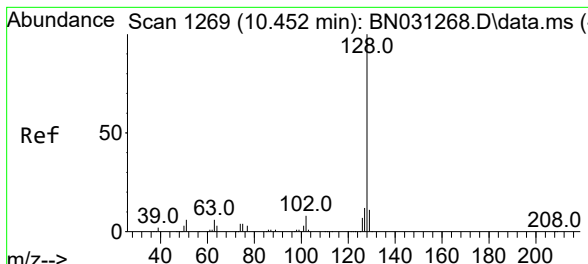

#30
Naphthalene
Concen: 16.915 ng/ul
RT: 10.451 min Scan# 1269
Delta R.T. -0.000 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40




Instrument :
BNA_N
ClientSampleId :
SSTD020387


Tgt Ion:128 Resp: 1093668
Ion Ratio Lower Upper
128 100
129 11.0 9.0 13.4
127 13.3 10.5 15.7

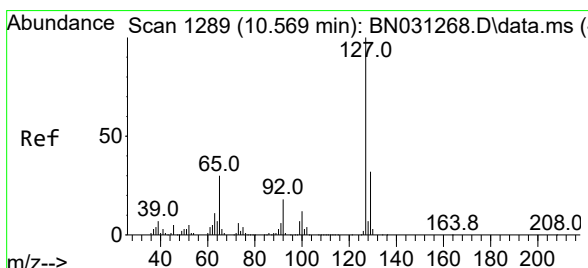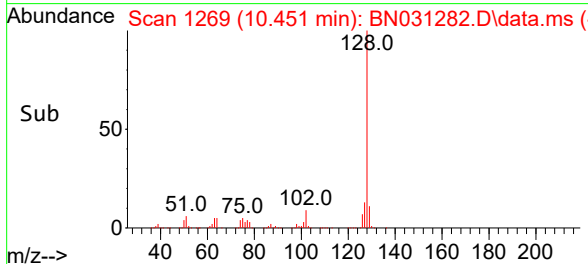

#32
4-Chloroaniline
Concen: 16.745 ng/ul
RT: 10.569 min Scan# 1289
Delta R.T. -0.000 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40

Tgt Ion:127 Resp: 467202
Ion Ratio Lower Upper
127 100
129 32.6 25.4 38.2


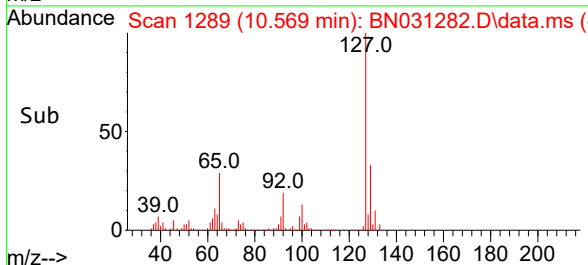

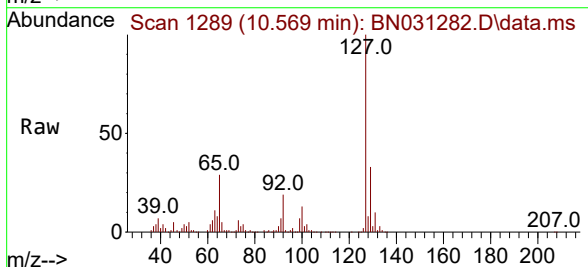




#33
Hexachlorobutadiene
Concen: 17.176 ng/ul
RT: 10.728 min Scan# 1316
Delta R.T. -0.000 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40




Instrument :
BNA_N
ClientSampleId :
SSTD020387


Tgt Ion:225 Resp: 192170
Ion Ratio Lower Upper
225 100
223 62.1 49.8 74.6
227 62.2 48.8 73.2

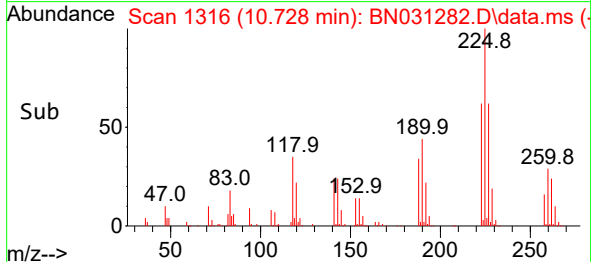

#34
Caprolactam
Concen: 16.658 ng/ul
RT: 11.351 min Scan# 1422
Delta R.T. -0.000 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40

Tgt Ion:113 Resp: 120454
Ion Ratio Lower Upper
113 100
55 145.8 112.4 168.6
56 105.5 88.0 132.0


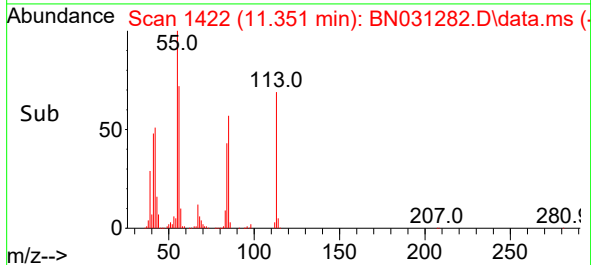

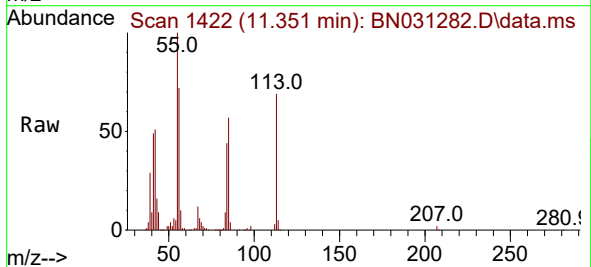




#35
4-Chloro-3-methylphenol
Concen: 17.557 ng/ul
RT: 11.698 min Scan# 1481
Delta R.T. -0.006 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40




Instrument :
BNA_N
ClientSampleId :
SSTD020387


Tgt Ion:107 Resp: 373605
Ion Ratio Lower Upper
107 100
144 27.2 20.6 31.0
142 80.4 67.4 101.2



#36
2-Methylnaphthalene
Concen: 17.115 ng/ul
RT: 12.069 min Scan# 1544
Delta R.T. -0.000 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40

Tgt Ion:142 Resp: 780389
Ion Ratio Lower Upper
142 100
141 90.2 69.6 104.4







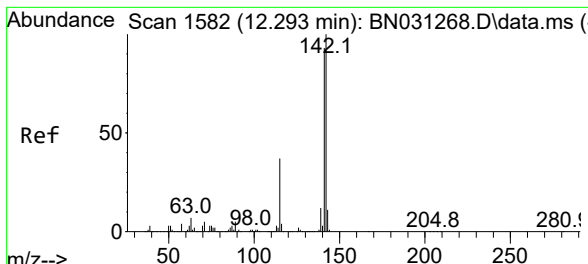

#37
1-Methylnaphthalene
Concen: 17.093 ng/ul
RT: 12.292 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40




Instrument :
BNA_N
ClientSampleId :
SSTD020387


Tgt Ion:142 Resp: 788624
Ion Ratio Lower Upper
142 100
141 88.8 70.2 105.4
116 3.7 3.1 4.7

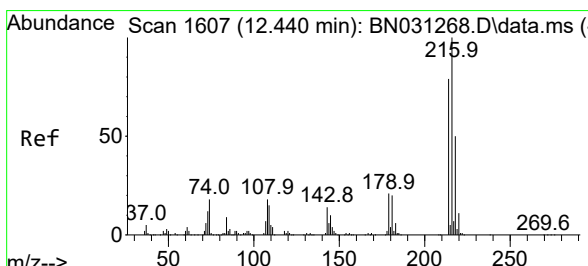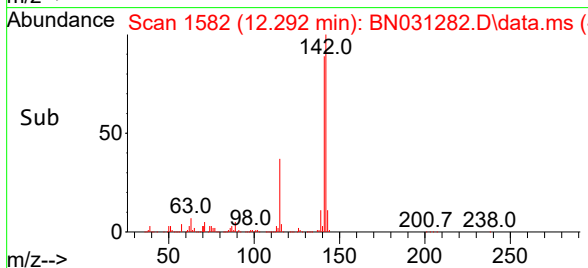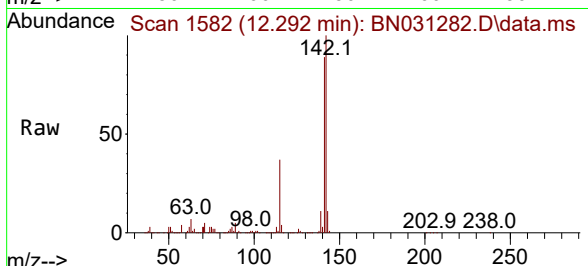

#39
1,2,4,5-Tetrachlorobenzene
Concen: 17.530 ng/ul
RT: 12.439 min Scan# 1607
Delta R.T. -0.000 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40

Tgt Ion:216 Resp: 394949
Ion Ratio Lower Upper
216 100
214 79.7 63.1 94.7
179 23.4 17.0 25.6
108 17.7 14.2 21.4


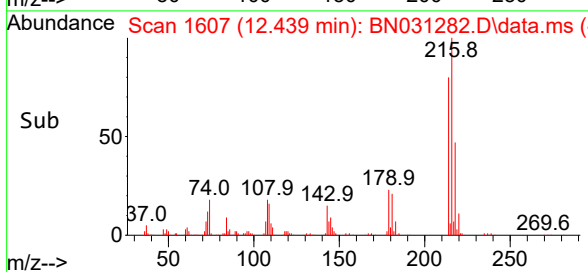

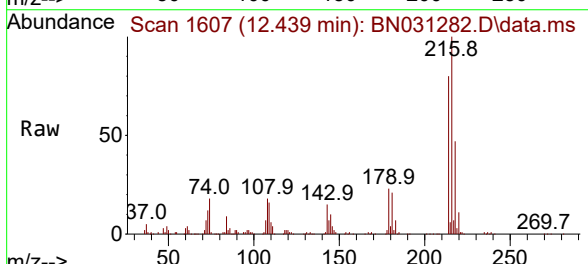




#40
Hexachlorocyclopentadiene
Concen: 16.700 ng/ul
RT: 12.410 min Scan# 1602
Delta R.T. -0.006 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40




Instrument :
BNA_N
ClientSampleId :
SSTD020387


Tgt Ion:237 Resp: 206685
Ion Ratio Lower Upper
237 100
235 64.2 47.6 71.4
272 12.9 10.8 16.2



#41
2,4,6-Trichlorophenol
Concen: 18.185 ng/ul
RT: 12.686 min Scan# 1649
Delta R.T. -0.006 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40


Tgt Ion:196 Resp: 272705
Ion Ratio Lower Upper
196 100
198 95.1 69.9 104.9
200 30.4 23.4 35.2








#42
2,4,5-Trichlorophenol
Concen: 17.729 ng/ul
RT: 12.763 min Scan# 1662
Delta R.T. -0.000 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40

Instrument :
BNA_N
ClientSampleId :
SSTD020387



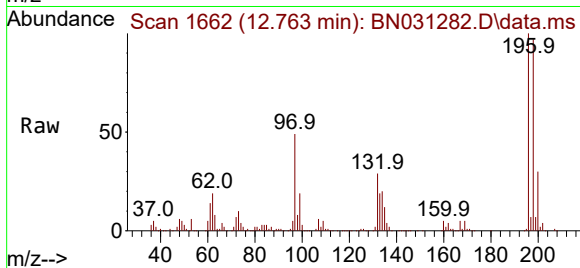



Tgt Ion:196 Resp: 294774
Ion Ratio Lower Upper
196 100
198 97.1 75.9 113.9
200 30.4 24.7 37.1



#43
1,1'-Biphenyl
Concen: 17.606 ng/ul
RT: 13.092 min Scan# 1718
Delta R.T. -0.006 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40

Tgt Ion:154 Resp: 1042586
Ion Ratio Lower Upper
154 100
153 40.7 31.8 47.8
76 12.6 10.6 15.8

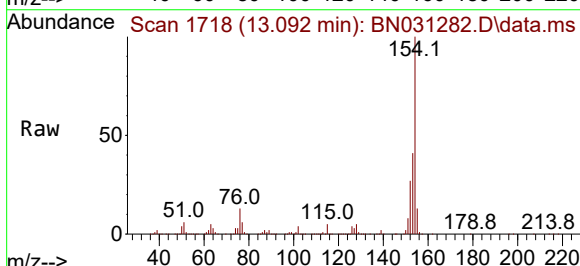

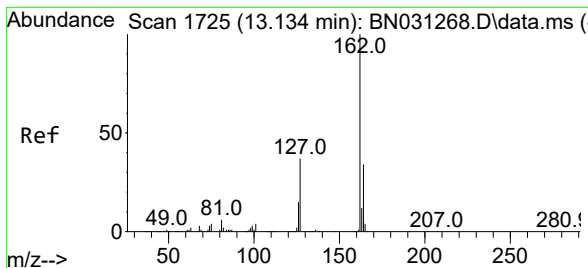

#44

2-Chloronaphthalene

Concen: 17.154 ng/ul

RT: 13.133 min Scan# 1725

Delta R.T. -0.006 min

Lab File: BN031282.D

Acq: 27 Apr 2024 22:40

Instrument :

BNA_N

ClientSampleId :

SSTD020387





Tgt Ion:162 Resp: 811695

Ion Ratio Lower Upper

162 100

164 33.4 25.8 38.8

127 41.4 33.7 50.5

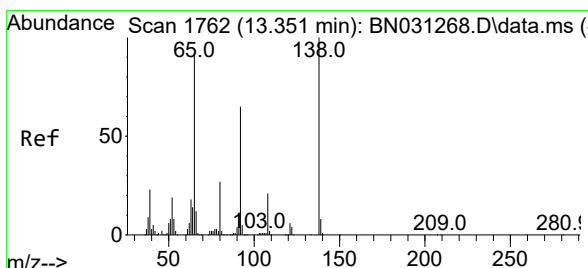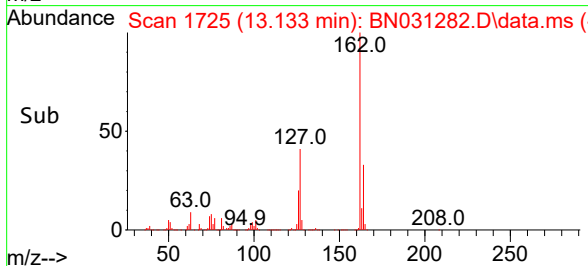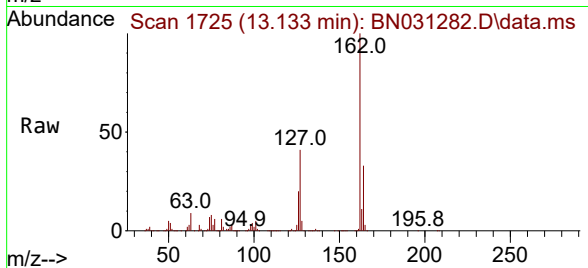

#45

2-Nitroaniline

Concen: 18.290 ng/ul

RT: 13.351 min Scan# 1762

Delta R.T. -0.006 min

Lab File: BN031282.D

Acq: 27 Apr 2024 22:40




Tgt Ion: 65 Resp: 238930


Ion Ratio Lower Upper

65 100

92 73.3 57.4 86.2

138 111.6 91.6 137.4




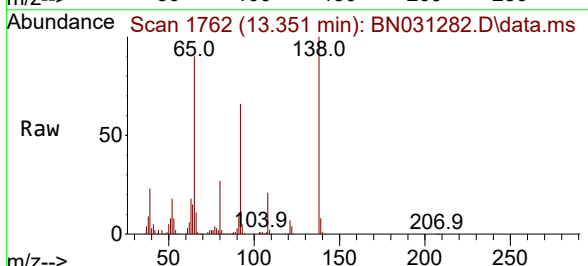




#47
Dimethylphthalate
Concen: 17.180 ng/ul
RT: 13.733 min Scan# 1827
Delta R.T. -0.000 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40




Instrument :
BNA_N
ClientSampleId :
SSTD020387


Tgt Ion:163 Resp: 1061902
Ion Ratio Lower Upper
163 100
194 4.1 3.0 4.6
164 10.0 8.0 12.0

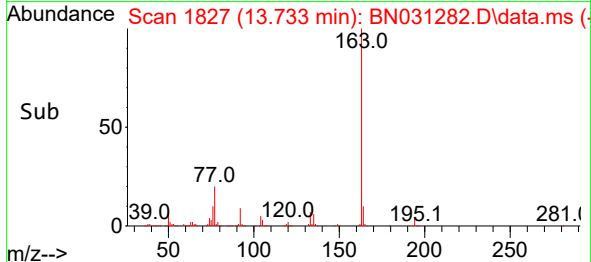

#48
2,6-Dinitrotoluene
Concen: 18.782 ng/ul
RT: 13.857 min Scan# 1848
Delta R.T. -0.000 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40

Tgt Ion:165 Resp: 217926
Ion Ratio Lower Upper
165 100
89 56.3 44.7 67.1
121 21.7 17.0 25.4


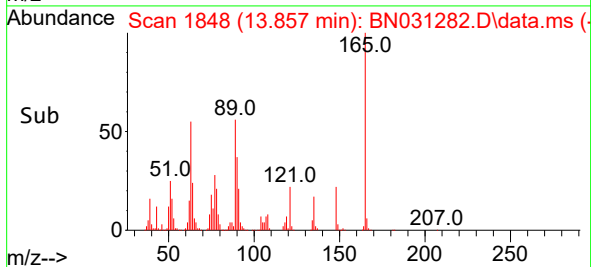

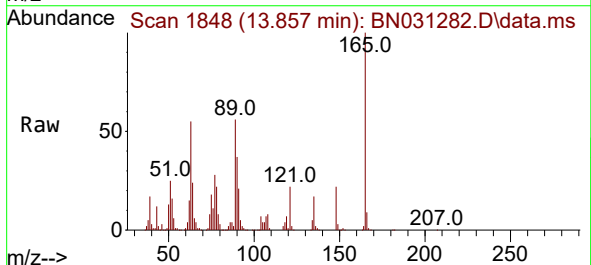


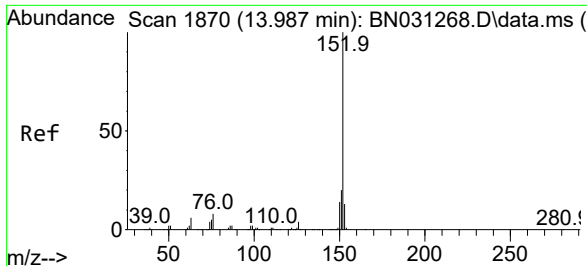

#50
Acenaphthylene
Concen: 17.071 ng/ul
RT: 13.986 min Scan# 1870
Delta R.T. -0.006 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40




Instrument :
BNA_N
ClientSampleId :
SSTD020387


Tgt Ion:152 Resp: 1353935
Ion Ratio Lower Upper
152 100
151 20.2 15.8 23.8
153 13.6 10.5 15.7

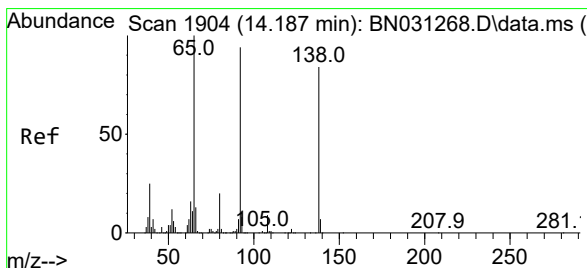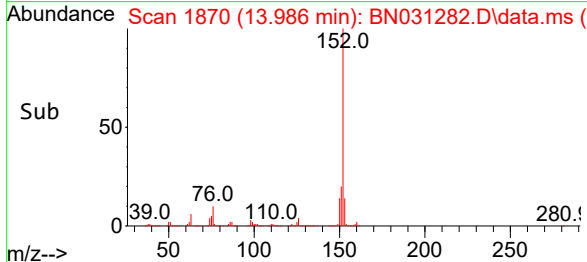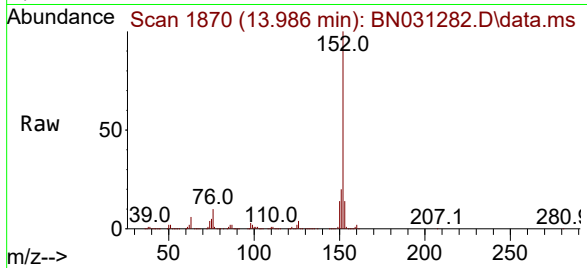

#51
3-Nitroaniline
Concen: 18.281 ng/ul
RT: 14.186 min Scan# 1904
Delta R.T. -0.006 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40

Tgt Ion:138 Resp: 243518
Ion Ratio Lower Upper
138 100
108 11.9 11.1 16.7
92 114.9 93.9 140.9

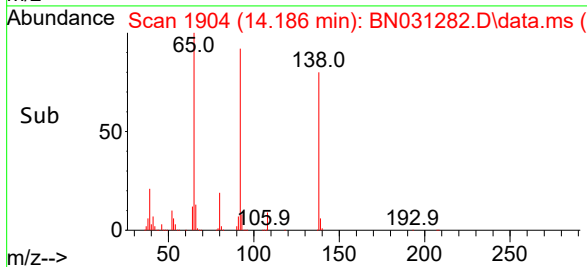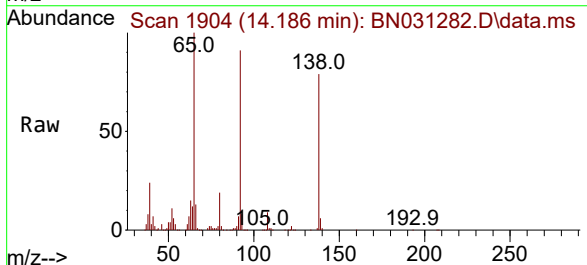




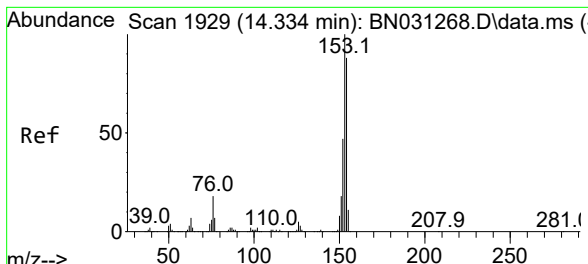


#52
 Acenaphthene
 Concen: 17.060 ng/ul
 RT: 14.333 min Scan# 1929
 Delta R.T. -0.000 min
 Lab File: BN031282.D
 Acq: 27 Apr 2024 22:40

Instrument :
 BNA_N
 ClientSampleId :
 SSTD020387

Tgt Ion:153 Resp: 896929




Ion	Ratio	Lower	Upper
153	100		
152	46.9	36.3	54.5
154	88.1	72.4	108.6

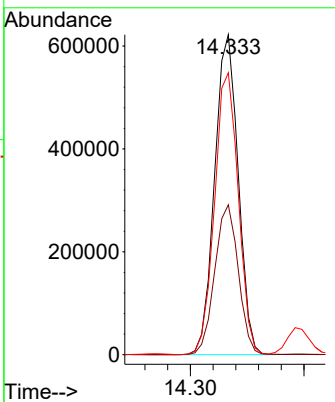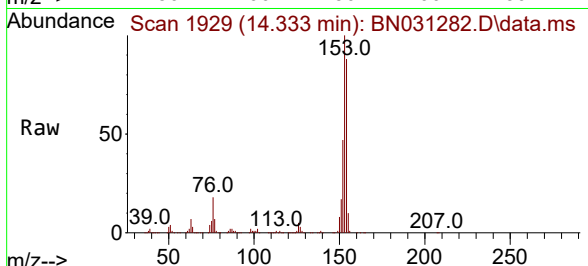


#53
 2,4-Dinitrophenol
 Concen: 16.995 ng/ul
 RT: 14.392 min Scan# 1939
 Delta R.T. -0.006 min
 Lab File: BN031282.D
 Acq: 27 Apr 2024 22:40

Tgt Ion:184 Resp: 111517

Ion	Ratio	Lower	Upper
184	100		
63	64.2	50.4	75.6
154	67.0	53.0	79.6


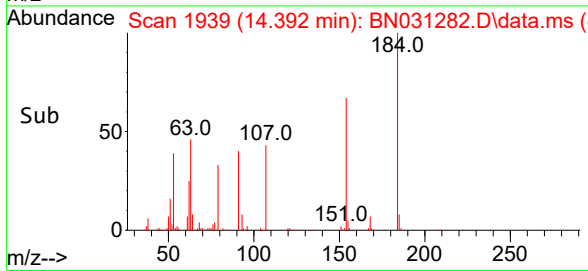
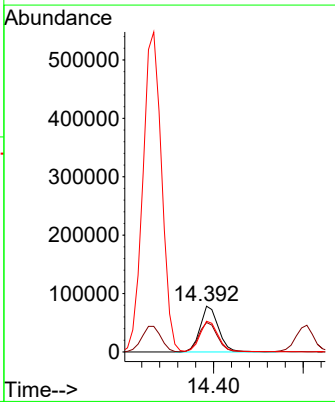
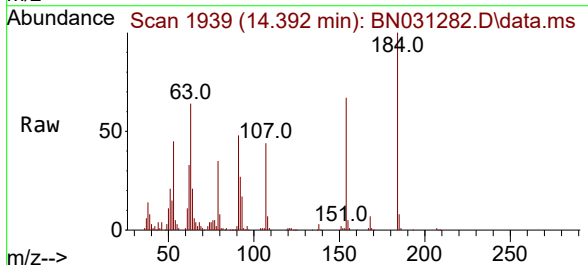


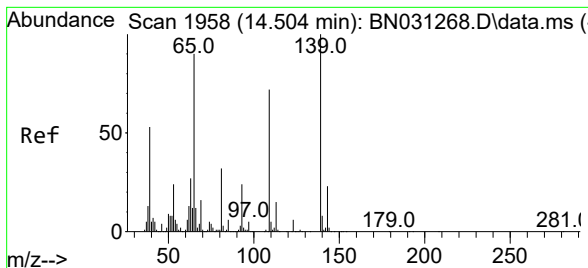

#55
4-Nitrophenol
Concen: 16.478 ng/ul
RT: 14.504 min Scan# 1958
Delta R.T. -0.000 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40




Instrument :
BNA_N
ClientSampleId :
SSTD020387


Tgt Ion:109 Resp: 167229
Ion Ratio Lower Upper
109 100
139 134.3 105.6 158.4
65 120.2 98.2 147.2

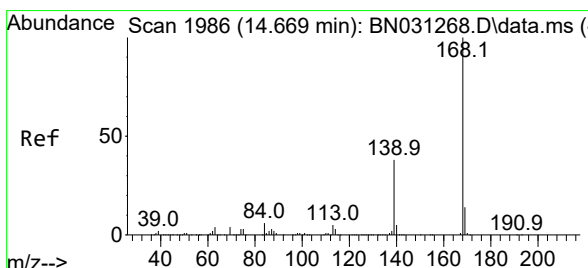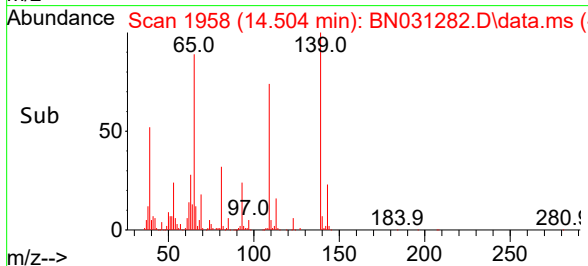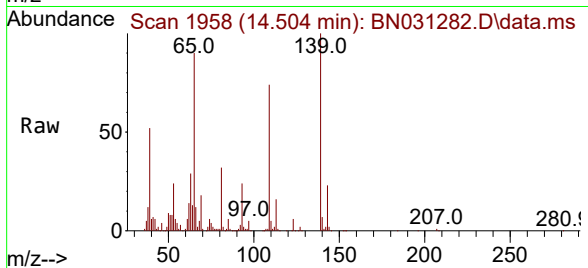

#56
Dibenzofuran
Concen: 16.779 ng/ul
RT: 14.669 min Scan# 1986
Delta R.T. -0.006 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40

Tgt Ion:168 Resp: 1219693
Ion Ratio Lower Upper
168 100
139 39.2 31.0 46.6


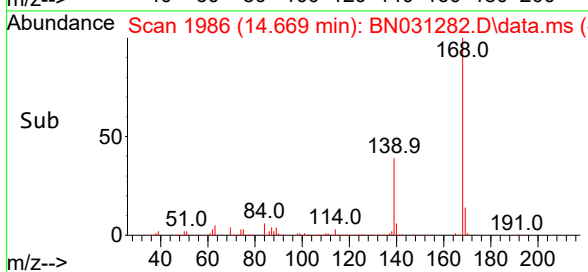

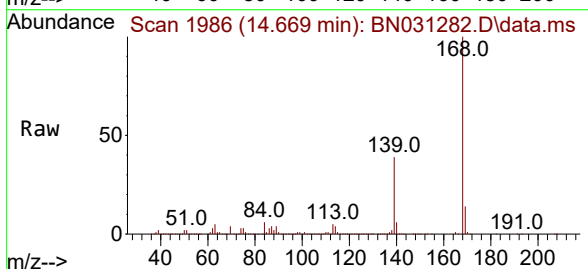




#57
2,4-Dinitrotoluene
Concen: 18.179 ng/ul
RT: 14.645 min Scan# 1982
Delta R.T. -0.006 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40




Instrument :
BNA_N
ClientSampleId :
SSTD020387


Tgt Ion:165 Resp: 320500
Ion Ratio Lower Upper
165 100
63 43.8 33.9 50.9
182 3.1 2.6 4.0

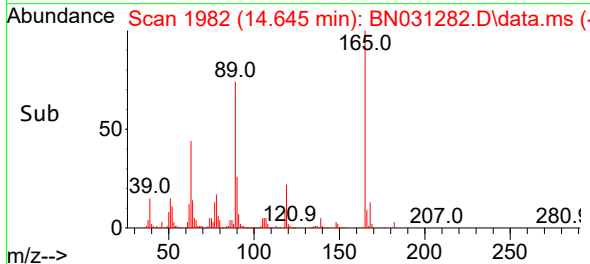

#58
2,3,4,6-Tetrachlorophenol
Concen: 17.547 ng/ul
RT: 14.898 min Scan# 2025
Delta R.T. -0.000 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40

Tgt Ion:232 Resp: 252136
Ion Ratio Lower Upper
232 100
131 46.0 41.2 61.8
130 2.5 2.2 3.2
166 30.9 27.3 40.9

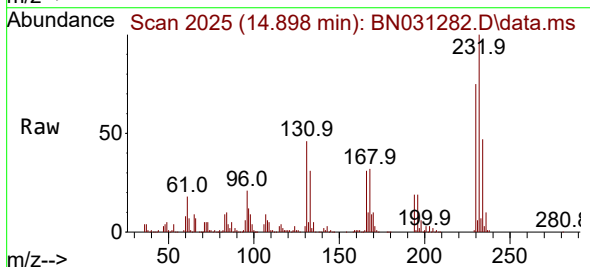




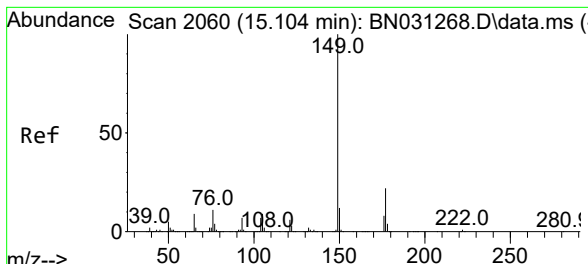


#59
 Diethylphthalate
 Concen: 17.423 ng/ul
 RT: 15.104 min Scan# 2060
 Delta R.T. -0.006 min
 Lab File: BN031282.D
 Acq: 27 Apr 2024 22:40

Instrument :
 BNA_N
 ClientSampleId :
 SSTD020387

Tgt Ion:149 Resp: 1107549




Ion	Ratio	Lower	Upper
149	100		
177	21.0	16.8	25.2
150	12.1	10.1	15.1

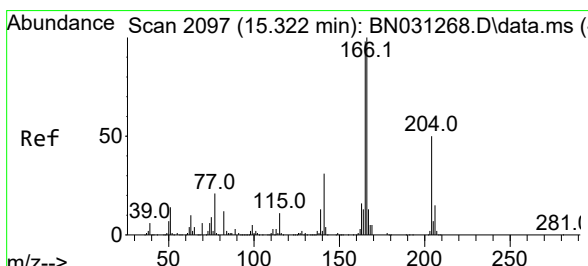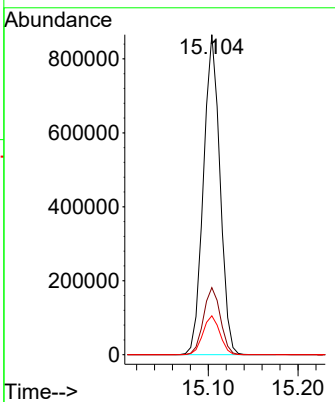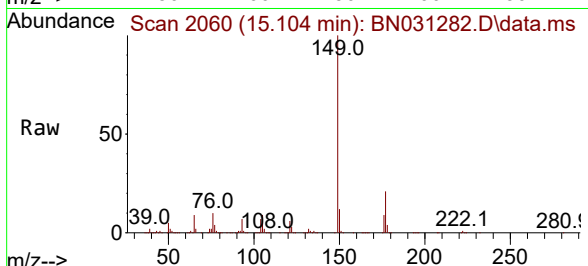


#61
 Fluorene
 Concen: 16.660 ng/ul
 RT: 15.322 min Scan# 2097
 Delta R.T. -0.000 min
 Lab File: BN031282.D
 Acq: 27 Apr 2024 22:40

Tgt Ion:166 Resp: 996628

Ion	Ratio	Lower	Upper
166	100		
165	97.1	74.6	112.0
167	12.9	10.6	16.0


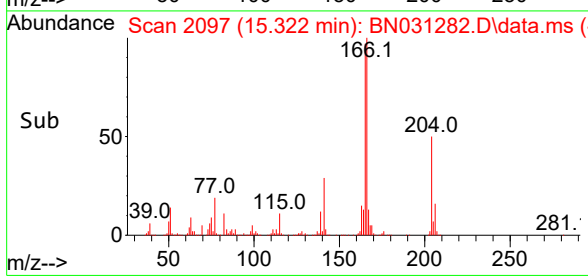
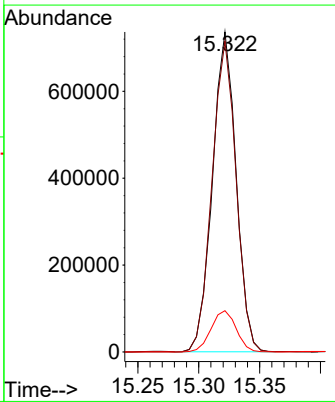
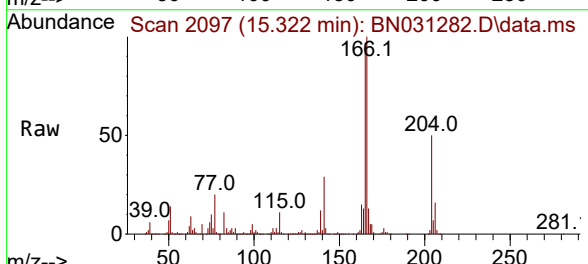


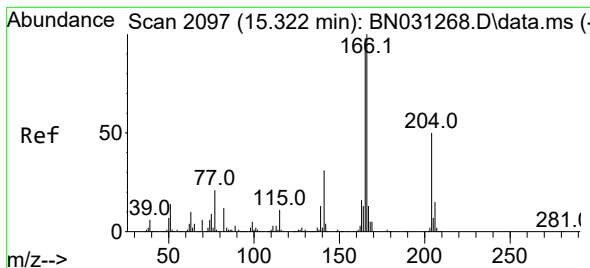

#62
4-Chlorophenyl-phenylether
Concen: 17.085 ng/ul
RT: 15.322 min Scan# 2097
Delta R.T. -0.000 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40




Instrument :
BNA_N
ClientSampleId :
SSTD020387


Tgt Ion:204 Resp: 486801
Ion Ratio Lower Upper
204 100
206 32.1 26.4 39.6
141 57.9 50.7 76.1

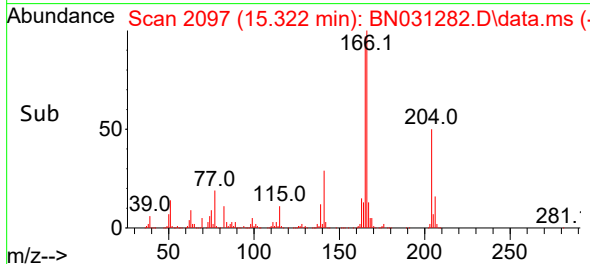

#63
4-Nitroaniline
Concen: 16.815 ng/ul
RT: 15.357 min Scan# 2103
Delta R.T. -0.000 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40

Tgt Ion:138 Resp: 241495
Ion Ratio Lower Upper
138 100
92 48.9 38.4 57.6
108 79.1 63.8 95.8


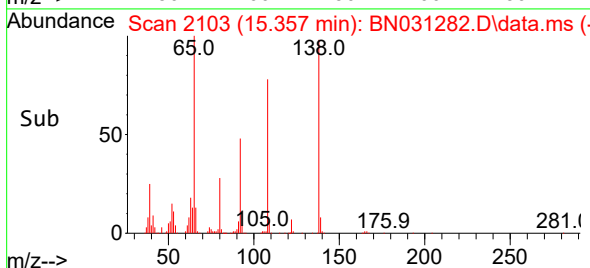

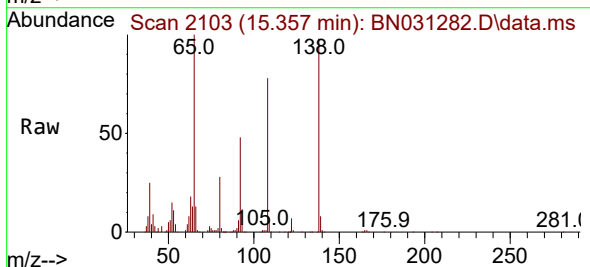




#66
4,6-Dinitro-2-methylphenol
Concen: 18.148 ng/ul
RT: 15.410 min Scan# 2112
Delta R.T. -0.000 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40




Instrument :
BNA_N
ClientSampleId :
SSTD020387


Tgt Ion:198 Resp: 183770
Ion Ratio Lower Upper
198 100
182 3.9 4.0 6.0#
77 25.6 22.2 33.4

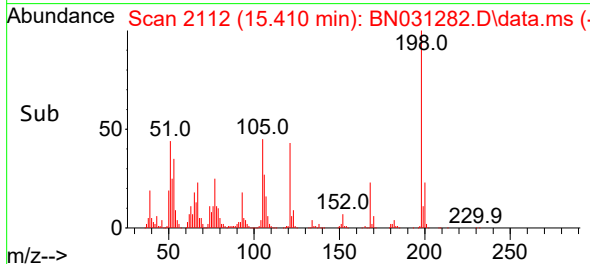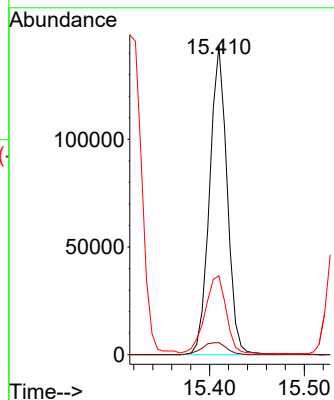

#67
N-Nitrosodiphenylamine
Concen: 17.459 ng/ul
RT: 15.539 min Scan# 2134
Delta R.T. -0.000 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40

Tgt Ion:169 Resp: 874716
Ion Ratio Lower Upper
169 100
168 66.6 52.6 79.0
167 35.7 27.8 41.6



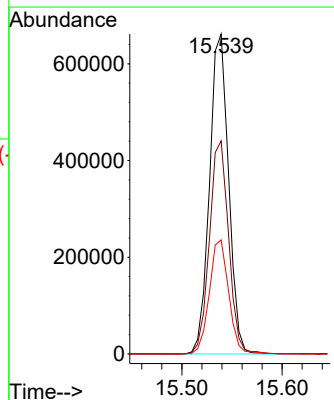
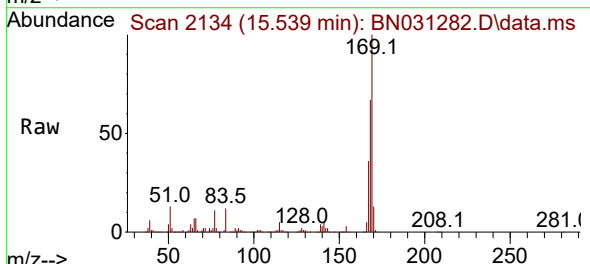




#68
4-Bromophenyl-phenylether
Concen: 17.975 ng/ul
RT: 16.216 min Scan# 21
Delta R.T. -0.000 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40




Instrument :
BNA_N
ClientSampleId :
SSTD020387


Tgt Ion:248 Resp: 317738
Ion Ratio Lower Upper
248 100
250 91.1 78.2 117.2
141 77.3 71.4 107.0

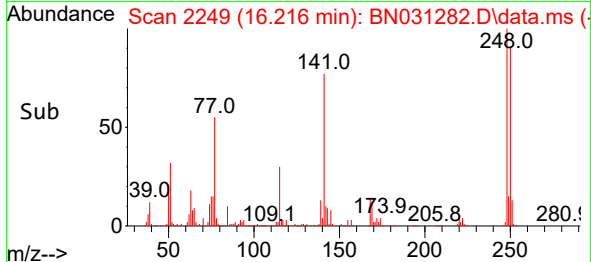

#69
Hexachlorobenzene
Concen: 17.623 ng/ul
RT: 16.322 min Scan# 2267
Delta R.T. -0.000 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40

Tgt Ion:284 Resp: 359130
Ion Ratio Lower Upper
284 100
142 33.4 30.0 45.0
249 29.2 25.5 38.3






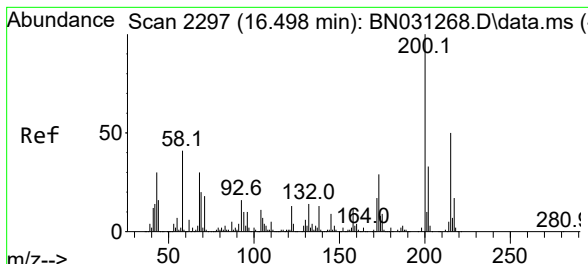


#70
 Atrazine
 Concen: 17.802 ng/ul
 RT: 16.498 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BN031282.D
 Acq: 27 Apr 2024 22:40

Instrument :
 BNA_N
 ClientSampleId :
 SST020387

Tgt Ion: 200 Resp: 313124




Ion	Ratio	Lower	Upper
200	100		
173	26.5	20.6	31.0
215	49.3	37.6	56.4

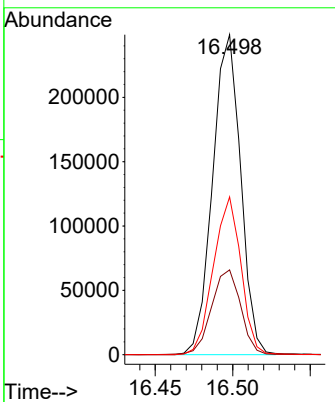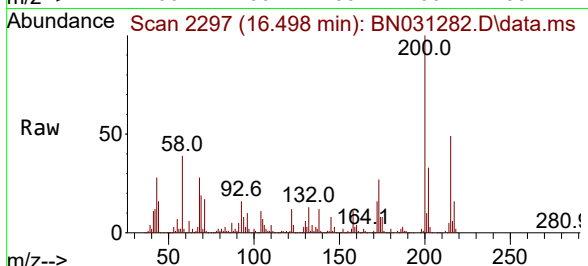


#71
 Pentachlorophenol
 Concen: 17.216 ng/ul
 RT: 16.669 min Scan# 2326
 Delta R.T. -0.006 min
 Lab File: BN031282.D
 Acq: 27 Apr 2024 22:40

Tgt Ion: 266 Resp: 227947

Ion	Ratio	Lower	Upper
266	100		
264	61.5	49.1	73.7
268	64.5	49.2	73.8


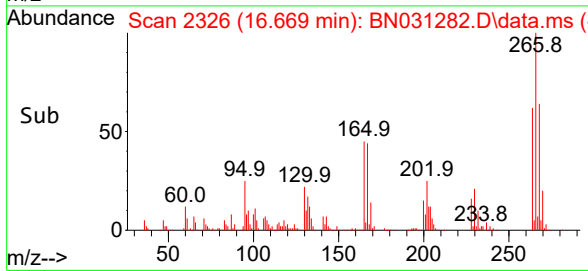
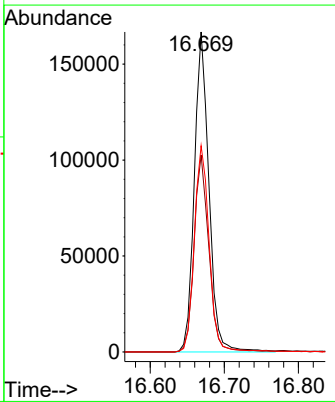
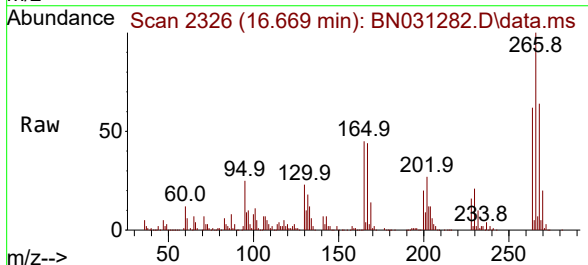




#72
Phenanthrene
Concen: 16.685 ng/ul
RT: 17.063 min Scan# 21
Delta R.T. -0.000 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40




Instrument :
BNA_N
ClientSampleId :
SSTD020387


Tgt Ion:178 Resp: 1649554
Ion Ratio Lower Upper
178 100
179 14.9 12.4 18.6
176 18.5 14.6 21.8

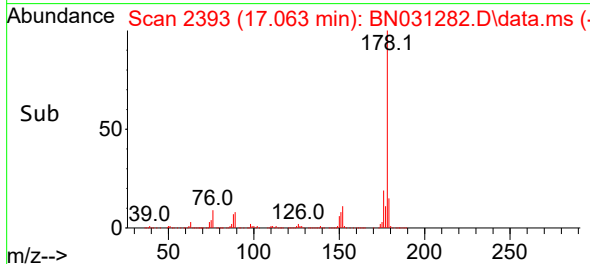

#74
Anthracene
Concen: 16.862 ng/ul
RT: 17.151 min Scan# 2408
Delta R.T. -0.006 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40

Tgt Ion:178 Resp: 1687075
Ion Ratio Lower Upper
178 100
179 15.1 12.2 18.4
176 18.3 14.4 21.6




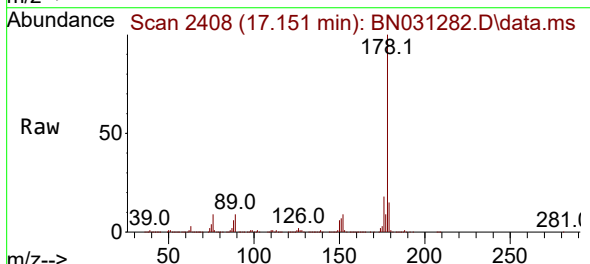


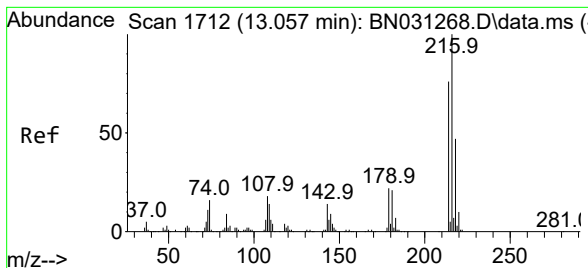

#75
1,2,3,4-Tetrachlorobenzene
Concen: 18.304 ng/uL
RT: 13.057 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40




Instrument :
BNA_N
ClientSampleId :
SSTD020387


Tgt Ion:216 Resp: 401301
Ion Ratio Lower Upper
216 100
214 77.8 63.0 94.6
218 48.6 38.3 57.5

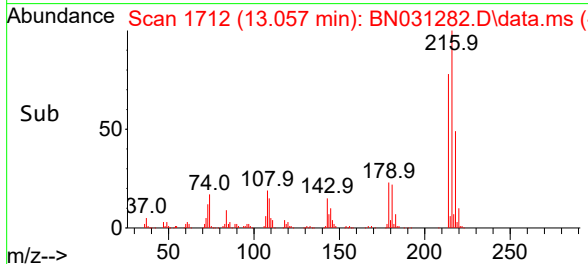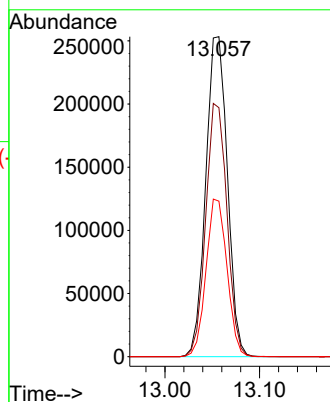

#76
Pentachlorobenzene
Concen: 17.635 ng/uL
RT: 14.580 min Scan# 1971
Delta R.T. -0.006 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40

Tgt Ion:250 Resp: 399248
Ion Ratio Lower Upper
250 100
248 59.9 49.3 73.9
252 62.6 52.9 79.3



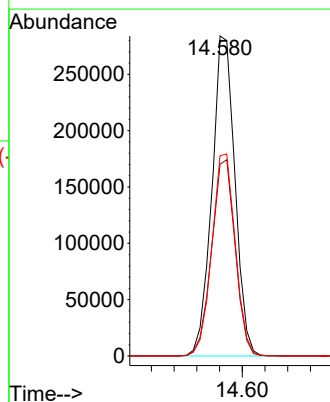
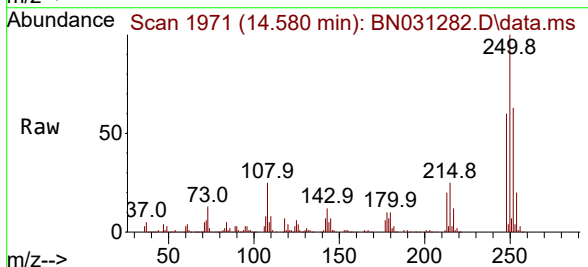




#77
Carbazole
Concen: 17.132 ng/ul
RT: 17.427 min Scan# 2455
Delta R.T. -0.006 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40




Instrument :
BNA_N
ClientSampleId :
SSTD020387


Tgt Ion:167 Resp: 1565706
Ion Ratio Lower Upper
167 100
166 22.0 16.2 24.2
139 13.4 10.6 15.8



#78
Di-n-butylphthalate
Concen: 17.732 ng/ul
RT: 17.992 min Scan# 2551
Delta R.T. -0.006 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40

Tgt Ion:149 Resp: 1975218
Ion Ratio Lower Upper
149 100
150 9.3 7.1 10.7
104 5.0 3.9 5.9









#80
Fluoranthene
Concen: 20.059 ng/ul
RT: 19.086 min Scan# 2737
Delta R.T. -0.000 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40




Instrument :
BNA_N
ClientSampleId :
SSTD020387


Tgt Ion:202 Resp: 1977198
Ion Ratio Lower Upper
202 100
101 11.8 9.0 13.6
100 8.8 6.9 10.3



#82
Pyrene
Concen: 19.987 ng/ul
RT: 19.451 min Scan# 2799
Delta R.T. -0.000 min
Lab File: BN031282.D
Acq: 27 Apr 2024 22:40

Tgt Ion:202 Resp: 2070077
Ion Ratio Lower Upper
202 100
101 13.0 11.1 16.7
100 10.7 9.3 13.9





#83

Butylbenzylphthalate

Concen: 20.308 ng/ul

RT: 20.362 min Scan# 2954

Delta R.T. -0.000 min

Lab File: BN031282.D

Acq: 27 Apr 2024 22:40

Instrument :

BNA_N

ClientSampleId :

SSTD020387





Tgt Ion:149 Resp: 928077

Ion Ratio Lower Upper

149 100

91 69.7 57.3 85.9

206 20.9 16.2 24.4

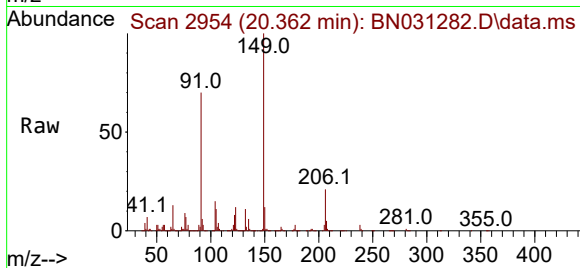

#84

3,3'-Dichlorobenzidine

Concen: 17.937 ng/ul

RT: 21.174 min Scan# 3092

Delta R.T. -0.000 min

Lab File: BN031282.D

Acq: 27 Apr 2024 22:40




Tgt Ion:252 Resp: 633458


Ion Ratio Lower Upper

252 100

254 64.9 54.5 81.7

126 11.7 9.8 14.6

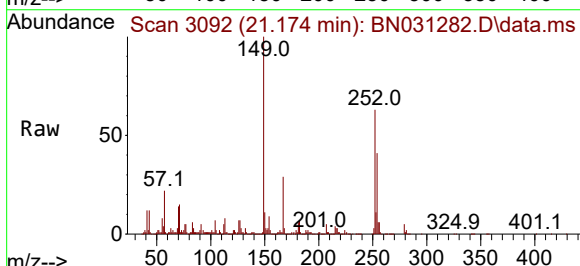



#85

Benzo(a)anthracene

Concen: 17.678 ng/ul

RT: 21.239 min Scan# 3103

Delta R.T. -0.000 min

Lab File: BN031282.D

Acq: 27 Apr 2024 22:40

Instrument :

BNA_N

ClientSampleId :

SSTD020387





Tgt Ion:228 Resp: 2034627

Ion Ratio Lower Upper

228 100

229 19.5 16.7 25.1

226 26.1 21.2 31.8

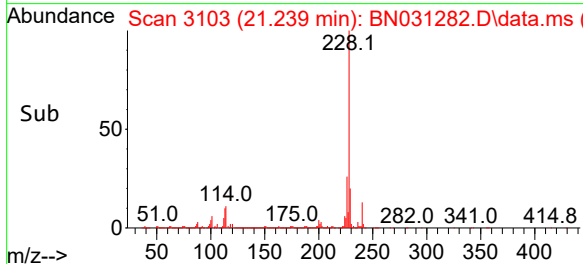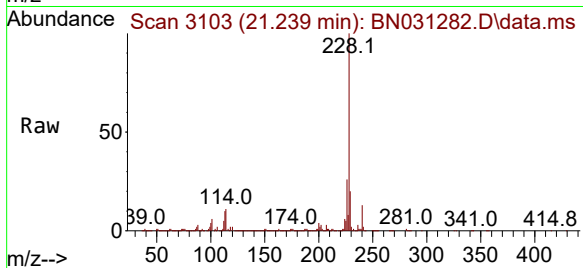

#86

Bis(2-ethylhexyl)phthalate

Concen: 19.295 ng/ul

RT: 21.168 min Scan# 3091

Delta R.T. -0.000 min

Lab File: BN031282.D

Acq: 27 Apr 2024 22:40




Tgt Ion:149 Resp: 1323943


Ion Ratio Lower Upper

149 100

167 28.3 22.3 33.5

279 4.4 3.0 4.6

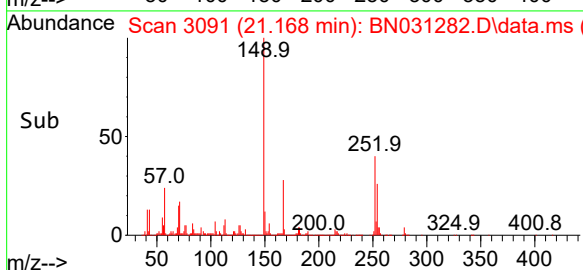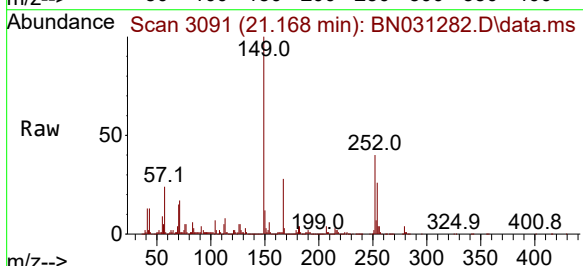



#87

Chrysene

Concen: 17.074 ng/ul

RT: 21.298 min Scan# 3114

Delta R.T. -0.000 min

Lab File: BN031282.D

Acq: 27 Apr 2024 22:40

Instrument :

BNA_N

ClientSampleId :

SSTD020387





Tgt Ion:228 Resp: 1865373

Ion Ratio Lower Upper

228 100

226 29.7 22.6 34.0

229 20.1 15.8 23.8

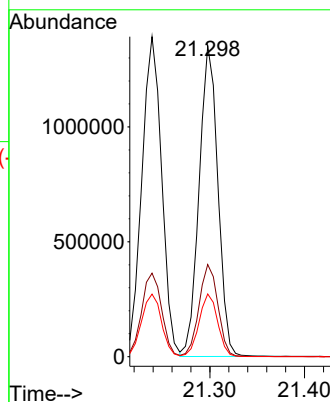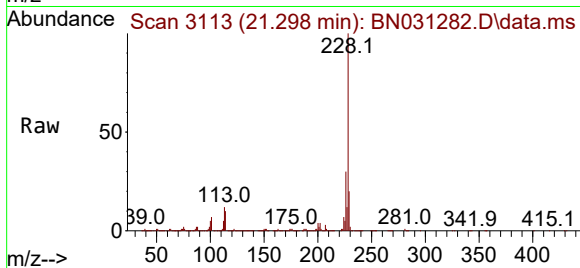

#89

Di-n-octyl phthalate

Concen: 22.697 ng/ul




RT: 22.262 min Scan# 3277


Delta R.T. -0.000 min

Lab File: BN031282.D

Acq: 27 Apr 2024 22:40

Tgt Ion:149 Resp: 2367625

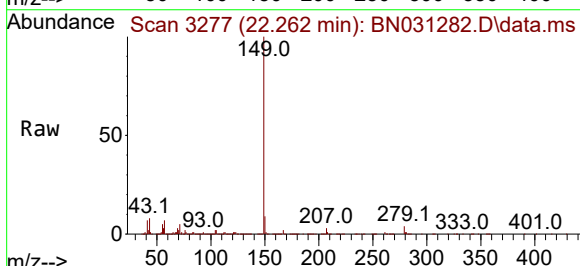

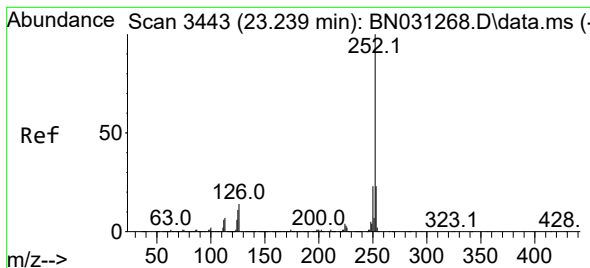

#90

Benzo(b)fluoranthene

Concen: 18.353 ng/ul

RT: 23.239 min Scan# 3443

Delta R.T. 0.006 min

Lab File: BN031282.D

Acq: 27 Apr 2024 22:40

Instrument :

BNA_N

ClientSampleId :

SSTD020387





Tgt Ion:252 Resp: 1868756

Ion Ratio Lower Upper

252 100

253 22.5 17.6 26.4

125 10.6 8.6 12.8

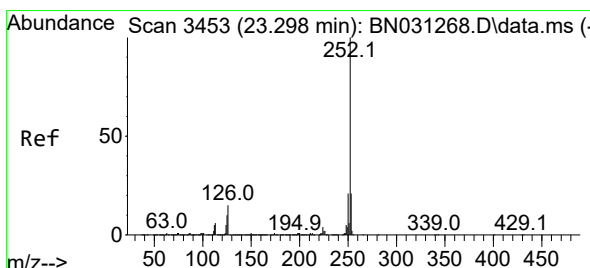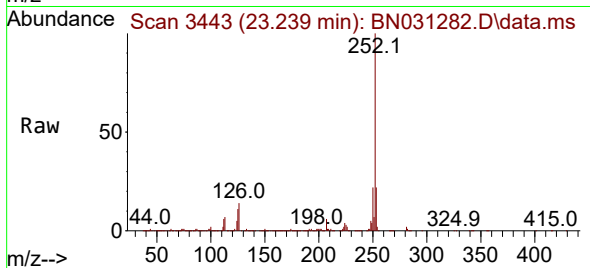

#91

Benzo(k)fluoranthene

Concen: 18.985 ng/ul

RT: 23.292 min Scan# 3452

Delta R.T. -0.006 min

Lab File: BN031282.D

Acq: 27 Apr 2024 22:40




Tgt Ion:252 Resp: 1944286


Ion Ratio Lower Upper

252 100

253 21.5 17.4 26.0

125 11.4 9.4 14.2





#93

Benzo(a)pyrene

Concen: 17.599 ng/ul

RT: 24.015 min Scan# 31

Delta R.T. -0.006 min

Lab File: BN031282.D

Acq: 27 Apr 2024 22:40

Instrument :

BNA_N

ClientSampleId :

SSTD020387





Tgt Ion:252 Resp: 1787713

Ion Ratio Lower Upper

252 100

253 20.2 17.7 26.5

125 11.2 9.9 14.9

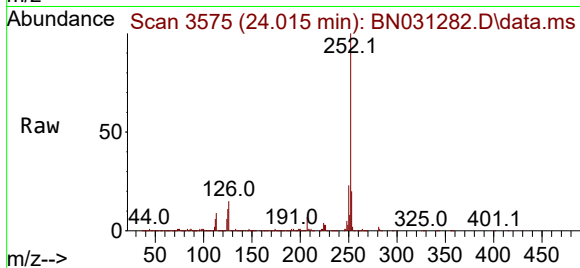

#94

Indeno(1,2,3-cd)pyrene

Concen: 15.446 ng/ul

RT: 27.392 min Scan# 4149

Delta R.T. -0.006 min

Lab File: BN031282.D

Acq: 27 Apr 2024 22:40




Tgt Ion:276 Resp: 1946963


Ion Ratio Lower Upper

276 100

138 21.6 17.4 26.2

277 22.8 18.3 27.5

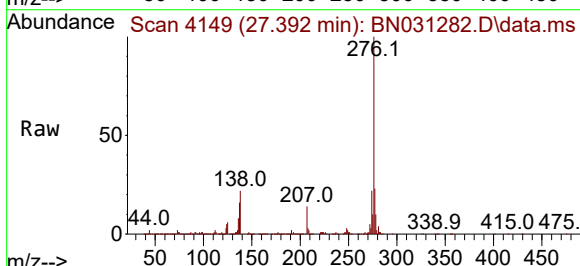



#95

Dibenzo(a,h)anthracene

Concen: 15.588 ng/ul

RT: 27.450 min Scan# 4159

Delta R.T. -0.006 min

Lab File: BN031282.D

Acq: 27 Apr 2024 22:40

Instrument :

BNA_N

ClientSampleId :

SSTD020387





Tgt Ion:278 Resp: 1612745

Ion Ratio Lower Upper

278 100

139 16.9 13.3 19.9

279 24.5 17.0 25.6



#96

Benzo(g,h,i)perylene

Concen: 15.045 ng/ul

RT: 28.403 min Scan# 4321

Delta R.T. -0.006 min

Lab File: BN031282.D

Acq: 27 Apr 2024 22:40

Tgt Ion:276 Resp: 1527209

Ion Ratio Lower Upper

276 100

138 24.0 19.0 28.6

277 23.8 19.3 28.9

