

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042724\
 Data File : BN031286.D
 Acq On : 28 Apr 2024 01:18
 Operator : MA/JU
 Sample : P2203-04
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1CZ0

Quant Time: Apr 28 21:18:04 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 26 22:57:25 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.622	152	219771	20.000	ng/ul	0.00
20) Naphthalene-d8	10.399	136	1053596	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.269	164	767305	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.016	188	1666221	20.000	ng/ul	0.00
79) Chrysene-d12	21.251	240	1533832	20.000	ng/ul	0.00
88) Perylene-d12	24.145	264	1625301	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.134	96	17571	3.735	ng/uL	0.00
4) Pyridine-d5	3.552	84	60697	4.480	ng/ul	0.00
7) Phenol-d5	6.799	99	113384	6.116	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.963	67	328412	30.447	ng/ul	0.00
11) 2-Chlorophenol-d4	7.152	132	336215	23.292	ng/ul	0.00
15) 4-Methylphenol-d8	8.328	113	231627	14.856	ng/ul	0.00
21) Nitrobenzene-d5	8.775	128	233816	30.887	ng/ul	0.00
24) 2-Nitrophenol-d4	9.493	143	252441	32.081	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.022	165	409610	26.396	ng/ul	0.00
31) 4-Chloroaniline-d4	10.546	131	554209	22.854	ng/ul	0.00
46) Dimethylphthalate-d6	13.687	166	1668051	31.240	ng/ul	0.00
49) Acenaphthylene-d8	13.957	160	1844126	30.478	ng/ul	0.00
54) 4-Nitrophenol-d4	14.487	143	57406	5.151	ng/ul	0.00
60) Fluorene-d10	15.263	176	1399637	30.111	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.392	200	242158	28.806	ng/ul	0.00
73) Anthracene-d10	17.116	188	2290066	31.710	ng/ul	0.00
81) Pyrene-d10	19.422	212	2650533	35.166	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.951	264	2448081	31.763	ng/ul	0.00
Target Compounds						
16) Acetophenone	8.446	105	25174	1.042	ng/ul	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042724\
Data File : BN031286.D
Acq On : 28 Apr 2024 01:18
Operator : MA/JU
Sample : P2203-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1CZ0

Quant Time: Apr 28 21:18:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 26 22:57:25 2024
Response via : Initial Calibration

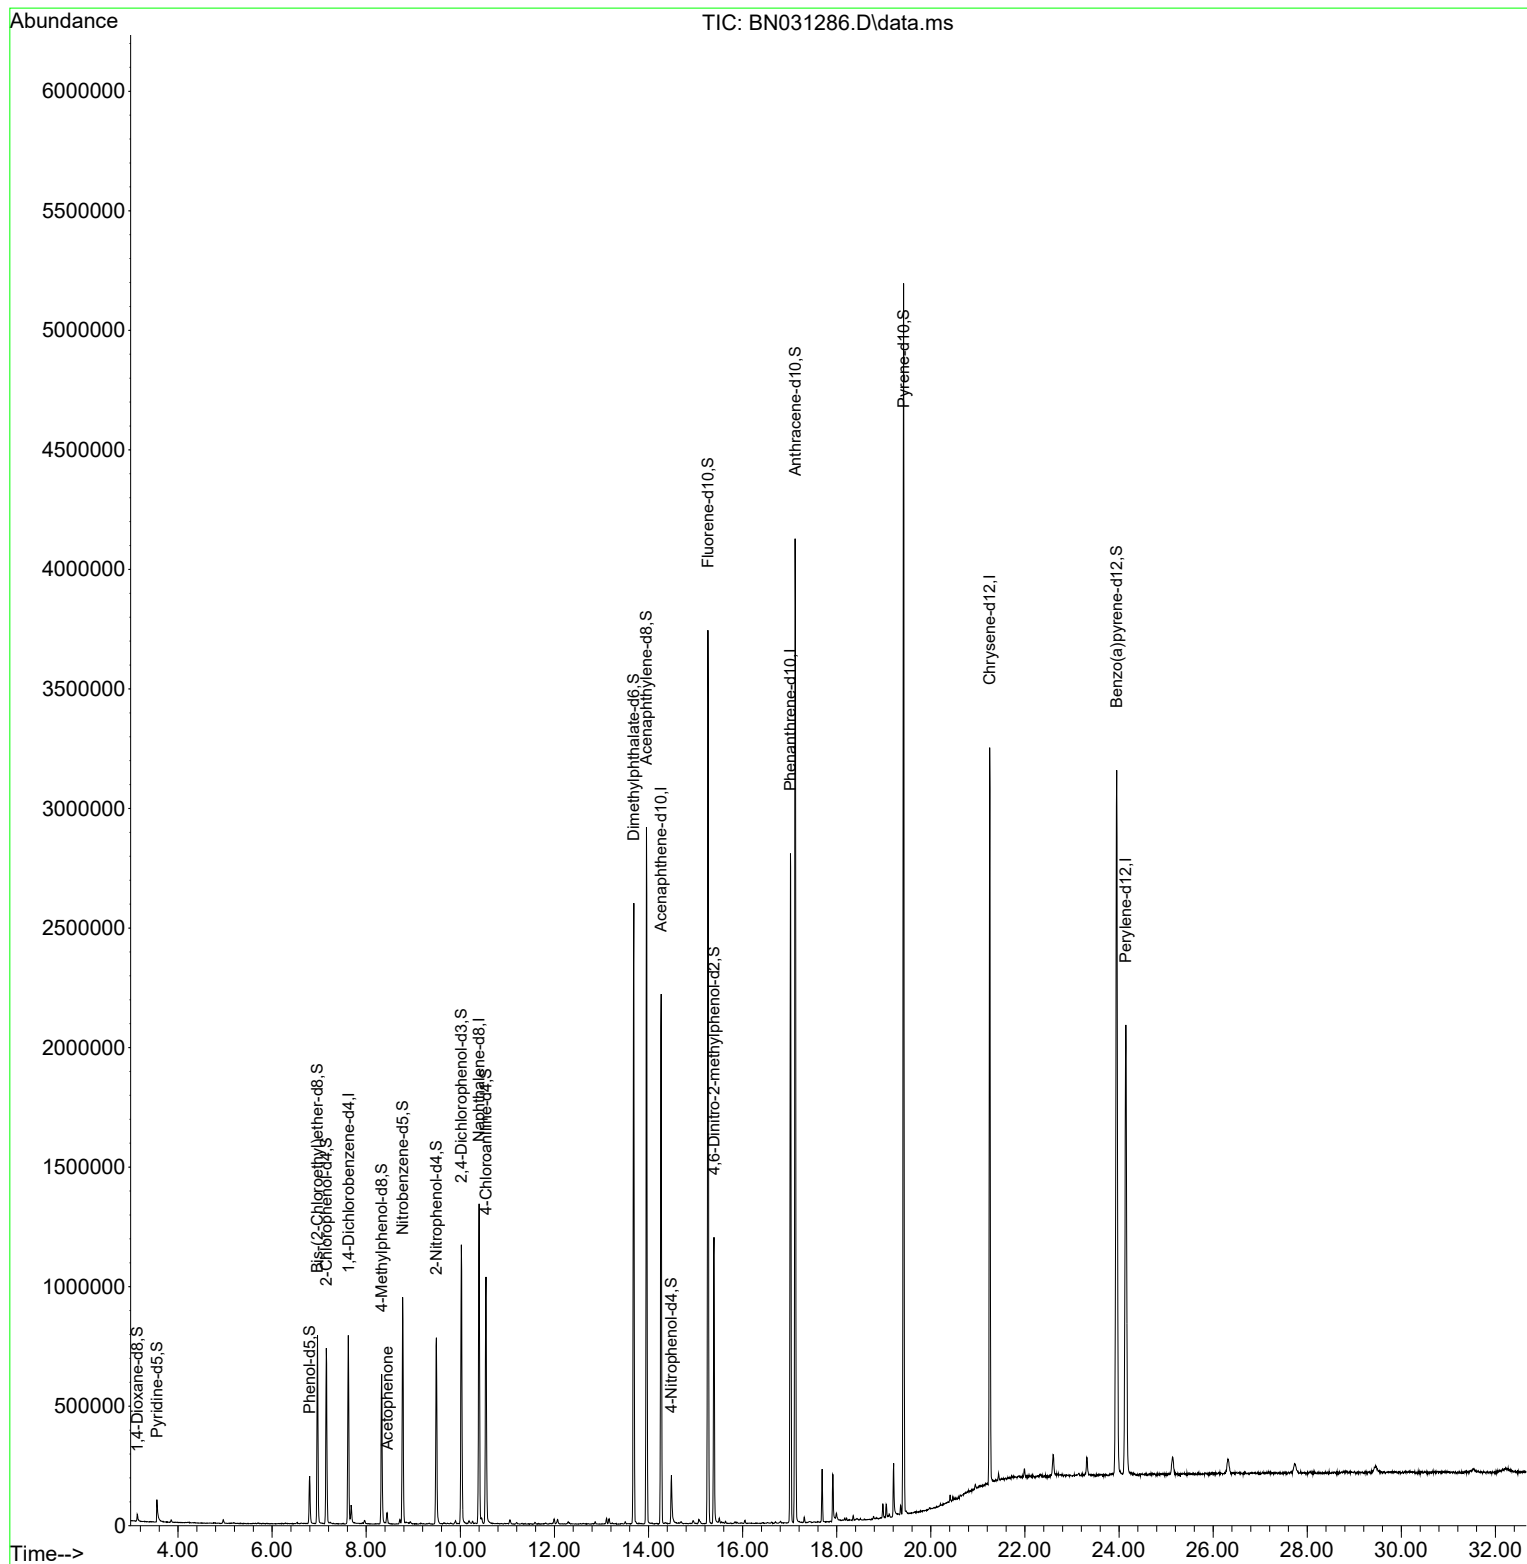

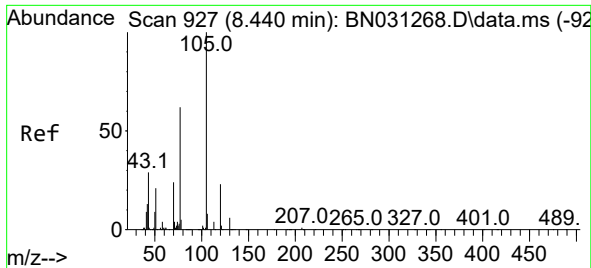

#16
 Acetophenone
 Concen: 1.042 ng/ul
 RT: 8.446 min Scan# 91
 Delta R.T. 0.000 min
 Lab File: BN031286.D
 Acq: 28 Apr 2024 01:18

Instrument :
 BNA_N
 ClientSampleId :
 E1CZ0

Tgt Ion:105 Resp: 25174
 Ion Ratio Lower Upper
 105 100
 77 79.3 60.2 90.4
 51 28.0 20.6 31.0

