

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042724\
 Data File : BN031277.D
 Acq On : 27 Apr 2024 18:43
 Operator : MA/JU
 Sample : P2269-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0RP9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031277.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	21	25	36	rVB	24192	43382	0.59%	0.068%
2	3.546	92	95	110	rBV	139850	245438	3.31%	0.383%
3	3.852	144	147	152	rBV3	9503	13548	0.18%	0.021%
4	4.958	331	335	342	rVB5	5665	9650	0.13%	0.015%
5	6.746	635	639	642	rBV	10663	15639	0.21%	0.024%
6	6.799	642	648	660	rVB	146774	240002	3.24%	0.374%
7	6.964	669	676	687	rBV	722001	1106503	14.94%	1.726%
8	7.152	700	708	717	rBV	629451	989009	13.35%	1.543%
9	7.616	779	787	803	rBV	862137	1368829	18.48%	2.135%
10	7.964	840	846	852	rBV	14764	25722	0.35%	0.040%
11	8.328	899	908	917	rBV	506468	817927	11.04%	1.276%
12	8.775	976	984	1000	rBV	907359	1463070	19.75%	2.282%
13	8.940	1007	1012	1016	rVB6	6397	10749	0.15%	0.017%
14	9.169	1045	1051	1056	rBV	35480	55255	0.75%	0.086%
15	9.228	1056	1061	1067	rVB5	5130	9362	0.13%	0.015%
16	9.346	1077	1081	1087	rVB4	5328	8948	0.12%	0.014%
17	9.493	1098	1106	1119	rBV	448186	751864	10.15%	1.173%
18	10.022	1189	1196	1205	rBV	955441	1575170	21.27%	2.457%
19	10.263	1232	1237	1243	rVB	10701	17782	0.24%	0.028%
20	10.399	1253	1260	1270	rBV	1383616	2272653	30.68%	3.545%
21	10.546	1278	1285	1297	rVB	577037	992576	13.40%	1.548%
22	10.775	1319	1324	1331	rVB3	7593	13090	0.18%	0.020%
23	11.005	1358	1363	1369	rBV6	6064	11687	0.16%	0.018%
24	11.152	1381	1388	1393	rBV3	14913	33709	0.46%	0.053%
25	11.657	1469	1474	1480	rVB2	9503	15839	0.21%	0.025%
26	11.993	1526	1531	1539	rVB2	19690	34418	0.46%	0.054%
27	13.081	1706	1716	1720	rBV5	21176	36305	0.49%	0.057%
28	13.163	1725	1730	1734	rBV2	25217	40628	0.55%	0.063%
29	13.275	1745	1749	1753	rVB4	8487	12449	0.17%	0.019%
30	13.687	1812	1819	1828	rBV	2425980	3362479	45.40%	5.245%
31	13.957	1858	1865	1873	rBV2	2596592	3906533	52.74%	6.094%
32	14.269	1911	1918	1925	rBV	2281885	3432329	46.34%	5.354%
33	14.493	1949	1956	1966	rBV	76600	160549	2.17%	0.250%
34	15.263	2080	2087	2093	rBV	3595684	5149732	69.53%	8.033%
35	15.316	2093	2096	2103	rVV2	37577	54638	0.74%	0.085%
36	15.393	2103	2109	2122	rVV2	93797	171601	2.32%	0.268%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042724\
Data File : BN031277.D
Acq On : 27 Apr 2024 18:43
Operator : MA/JU
Sample : P2269-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RP9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Title : SVOA CALIBRATION

37	15.504	2122	2128	2133	rVB3	19361	31477	0.42%	0.049%
38	16.051	2217	2221	2224	rBV5	8129	10770	0.15%	0.017%
39	16.692	2327	2330	2334	rVB5	5201	7600	0.10%	0.012%
40	16.804	2342	2349	2356	rBV4	6897	16240	0.22%	0.025%
41	16.945	2369	2373	2376	rBV3	12246	14409	0.19%	0.022%
42	17.016	2379	2385	2395	rVV	2974181	4351847	58.75%	6.788%
43	17.116	2395	2402	2417	rBV2	4492292	6304161	85.11%	9.834%
44	17.416	2446	2453	2460	rBV8	6877	20166	0.27%	0.031%
45	17.916	2533	2538	2545	rBV3	36697	56781	0.77%	0.089%
46	18.351	2608	2612	2616	rBV5	11018	15223	0.21%	0.024%
47	18.398	2616	2620	2624	rVB5	28783	36209	0.49%	0.056%
48	18.981	2715	2719	2727	rBV	61258	81649	1.10%	0.127%
49	19.051	2727	2731	2735	rBV	55348	76438	1.03%	0.119%
50	19.122	2740	2743	2745	rVV4	6896	7638	0.10%	0.012%
51	19.210	2754	2758	2763	rBV5	27681	42068	0.57%	0.066%
52	19.363	2780	2784	2787	rBV	29764	36053	0.49%	0.056%
53	19.422	2788	2794	2801	rBV	5275996	7406933	100.00%	11.554%
54	19.686	2837	2839	2844	rVB2	16364	17978	0.24%	0.028%
55	20.416	2960	2963	2967	rBV3	20622	28506	0.38%	0.044%
56	20.951	3051	3054	3062	rBV4	44104	95414	1.29%	0.149%
57	21.257	3100	3106	3117	rBV	3295661	4783844	64.59%	7.462%
58	23.957	3555	3565	3581	rVB2	3098472	7372887	99.54%	11.501%
59	24.151	3589	3598	3609	rBV	2022064	4824353	65.13%	7.525%




Sum of corrected areas: 64107708

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042724\
Data File : BN031277.D
Acq On : 27 Apr 2024 18:43
Operator : MA/JU
Sample : P2269-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RP9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

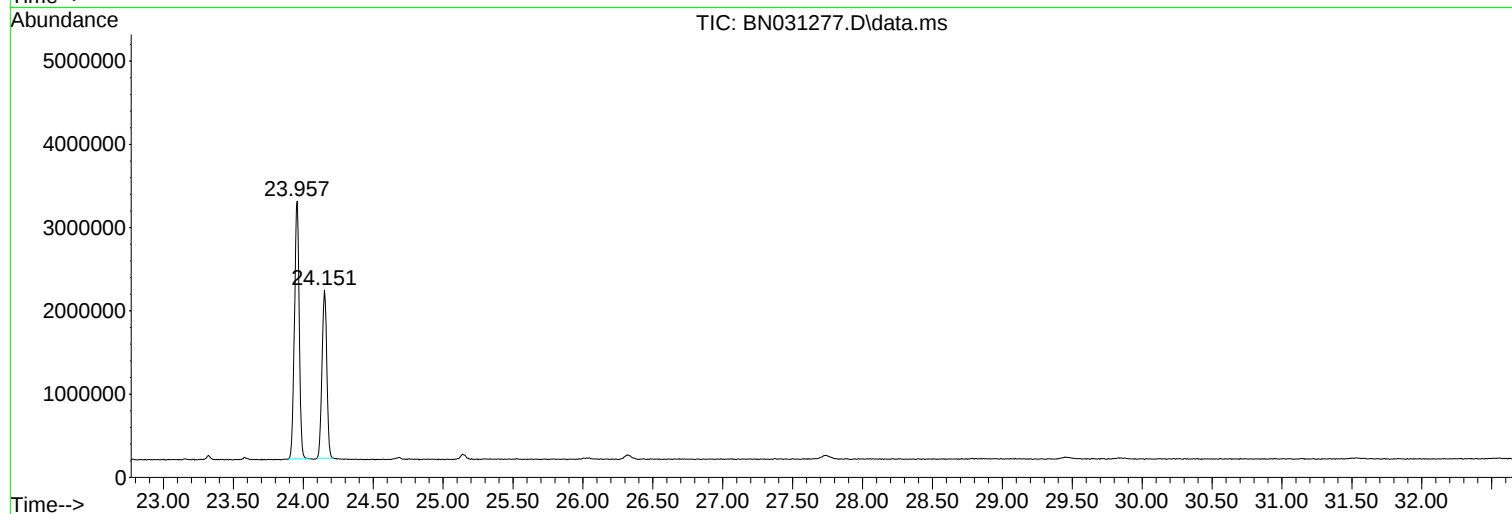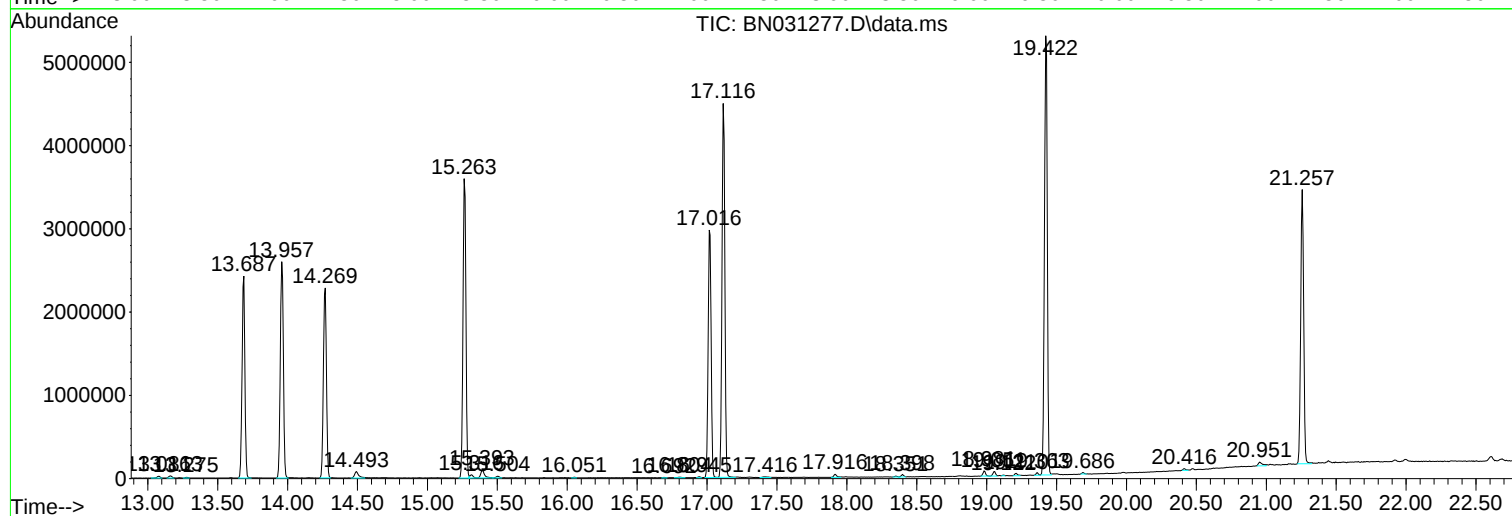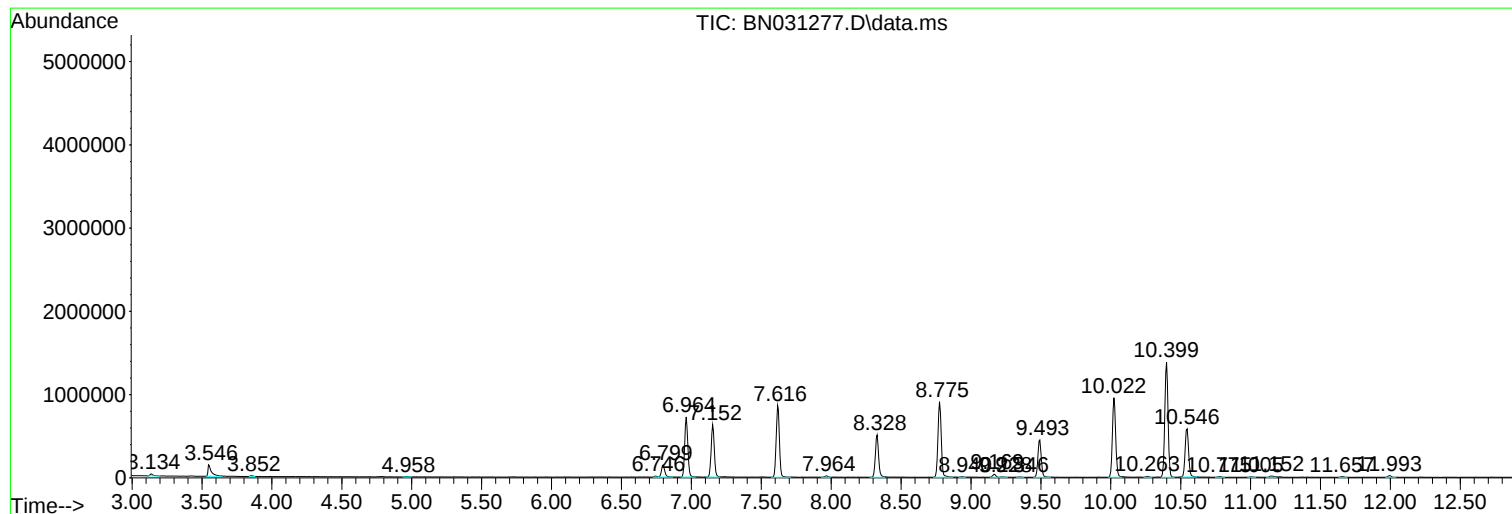

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042724\
Data File : BN031277.D
Acq On : 27 Apr 2024 18:43
Operator : MA/JU
Sample : P2269-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RP9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042724\
Data File : BN031277.D
Acq On : 27 Apr 2024 18:43
Operator : MA/JU
Sample : P2269-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RP9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------