

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042724\
 Data File : BN031278.D
 Acq On : 27 Apr 2024 19:22
 Operator : MA/JU
 Sample : P2269-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0RQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031278.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	22	25	38	rVB	31582	55431	0.63%	0.076%
2	3.564	96	98	115	rBV	31012	66382	0.75%	0.091%
3	3.858	144	148	152	rVB	9383	13971	0.16%	0.019%
4	6.746	631	639	642	rBV	27549	40991	0.47%	0.056%
5	6.799	642	648	657	rVB	237321	377856	4.29%	0.519%
6	6.963	669	676	688	rBV	827033	1270444	14.44%	1.744%
7	7.152	701	708	719	rBV	808625	1281631	14.56%	1.759%
8	7.234	719	722	727	rVB6	5111	8975	0.10%	0.012%
9	7.616	779	787	798	rBV	801841	1255474	14.27%	1.723%
10	8.328	901	908	925	rBV	710399	1151297	13.08%	1.580%
11	8.775	977	984	998	rBV	1032185	1650427	18.75%	2.265%
12	9.169	1044	1051	1055	rBV	58068	86146	0.98%	0.118%
13	9.493	1098	1106	1117	rBV	826785	1369749	15.57%	1.880%
14	10.022	1189	1196	1211	rBV	1216675	2040760	23.19%	2.801%
15	10.399	1252	1260	1272	rVB	1270366	2107196	23.95%	2.892%
16	10.546	1276	1285	1296	rBV	467466	808489	9.19%	1.110%
17	11.657	1468	1474	1479	rVB	17308	27903	0.32%	0.038%
18	11.993	1525	1531	1538	rBV	23442	38451	0.44%	0.053%
19	13.163	1724	1730	1737	rBV2	30657	48569	0.55%	0.067%
20	13.687	1812	1819	1829	rBV	2881565	4086079	46.43%	5.609%
21	13.957	1858	1865	1884	rBV2	3151068	4678427	53.16%	6.422%
22	14.269	1911	1918	1924	rBV	2200537	3210471	36.48%	4.407%
23	14.322	1924	1927	1934	rVB	26820	46183	0.52%	0.063%
24	14.487	1949	1955	1969	rBV	326465	562806	6.40%	0.773%
25	14.681	1985	1988	1994	rVB8	5145	8888	0.10%	0.012%
26	15.263	2080	2087	2100	rBV	4143906	6045654	68.70%	8.298%
27	15.392	2103	2109	2120	rBV	1587039	2141946	24.34%	2.940%
28	15.504	2125	2128	2134	rVB2	20660	31164	0.35%	0.043%
29	16.051	2215	2221	2225	rBV3	9931	13936	0.16%	0.019%
30	17.016	2377	2385	2395	rBV	2780312	4074575	46.30%	5.593%
31	17.116	2395	2402	2416	rVV	4995400	7426017	84.39%	10.193%
32	17.686	2495	2499	2505	rBV8	5085	9498	0.11%	0.013%
33	17.916	2533	2538	2545	rBV2	48114	71922	0.82%	0.099%
34	18.986	2715	2720	2726	rVB	69502	97122	1.10%	0.133%
35	19.057	2726	2732	2736	rBV	65898	96698	1.10%	0.133%
36	19.210	2754	2758	2762	rBV4	43464	58368	0.66%	0.080%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042724\
Data File : BN031278.D
Acq On : 27 Apr 2024 19:22
Operator : MA/JU
Sample : P2269-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Title : SVOA CALIBRATION

37	19.363	2780	2784	2788	rBV3	29660	38266	0.43%	0.053%
38	19.422	2788	2794	2802	rBV	6289983	8799963	100.00%	12.079%
39	20.416	2960	2963	2968	rBV5	20923	28463	0.32%	0.039%
40	21.257	3100	3106	3115	rBV2	3183932	4443555	50.50%	6.099%
41	23.957	3555	3565	3580	rVB2	3560282	8666966	98.49%	11.896%
42	24.151	3589	3598	3609	rVB	1917679	4516214	51.32%	6.199%




Sum of corrected areas: 72853323

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042724\
Data File : BN031278.D
Acq On : 27 Apr 2024 19:22
Operator : MA/JU
Sample : P2269-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RQ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

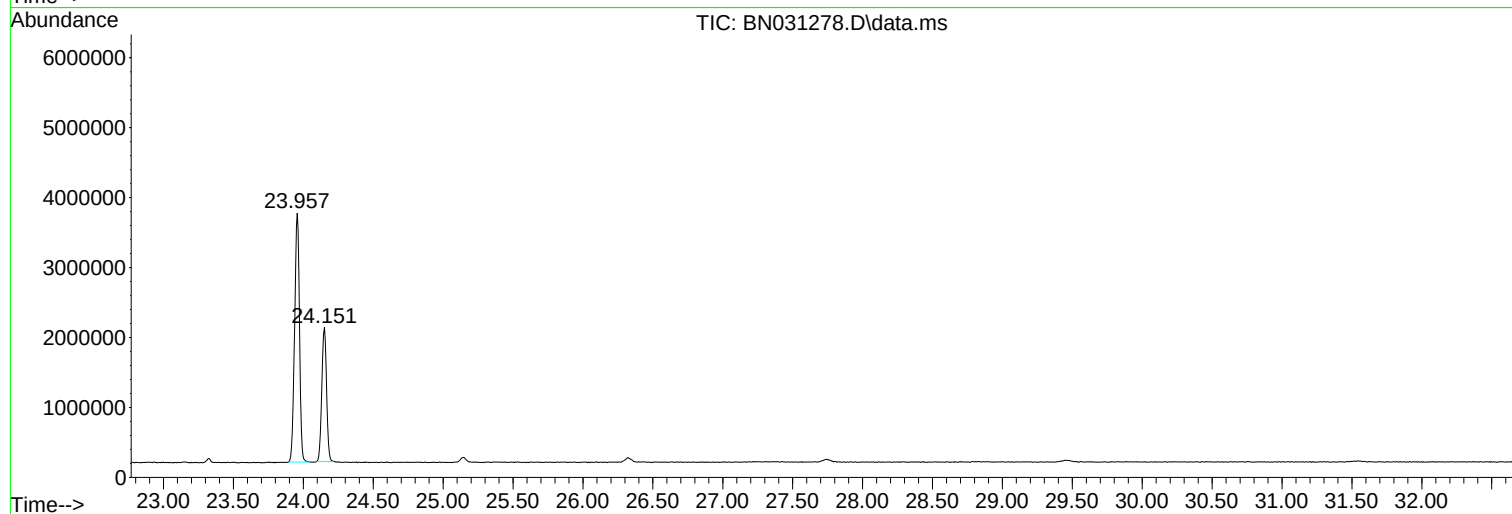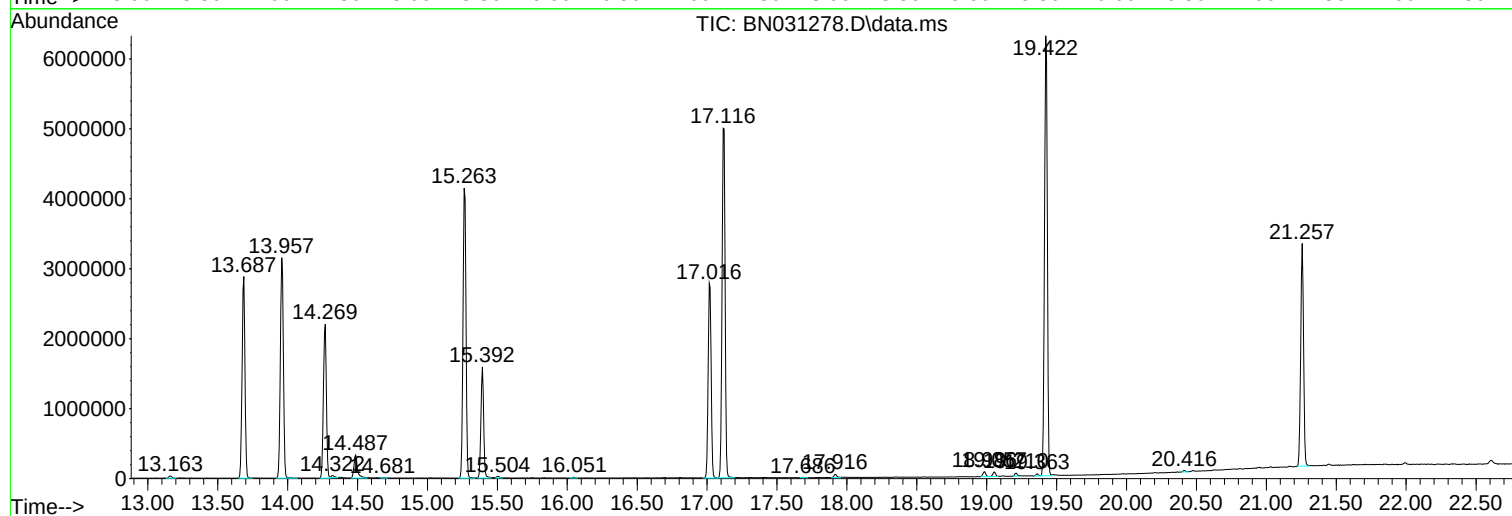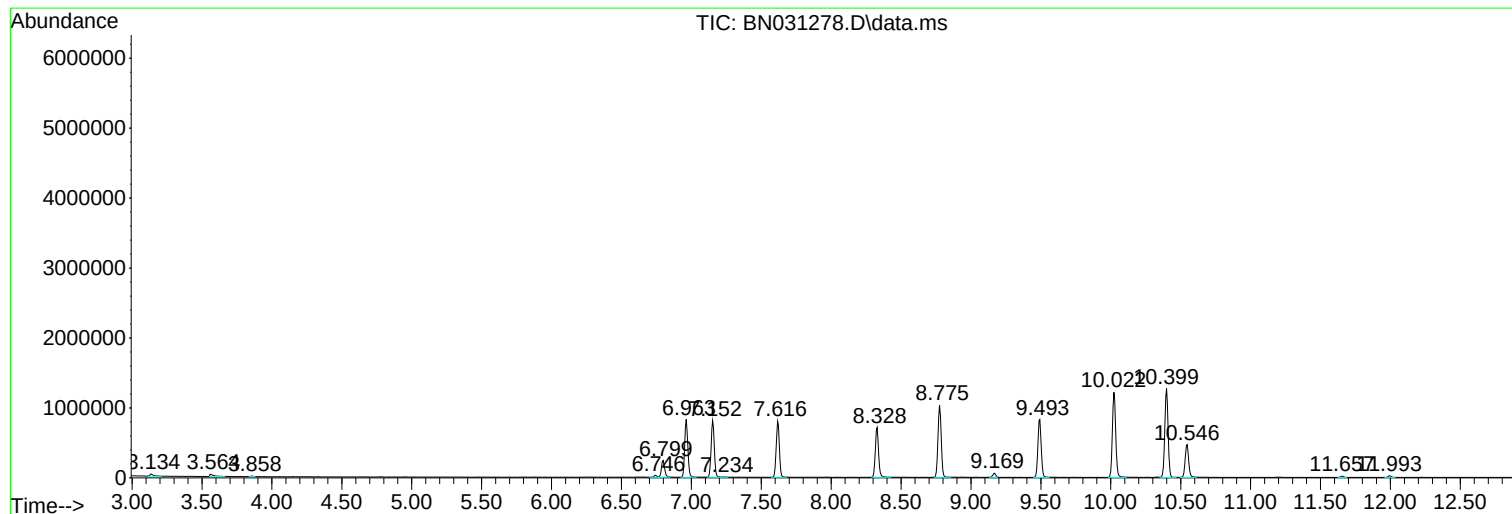

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042724\
Data File : BN031278.D
Acq On : 27 Apr 2024 19:22
Operator : MA/JU
Sample : P2269-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RQ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042724\
Data File : BN031278.D
Acq On : 27 Apr 2024 19:22
Operator : MA/JU
Sample : P2269-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RQ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------