

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042724\
 Data File : BN031279.D
 Acq On : 27 Apr 2024 20:02
 Operator : MA/JU
 Sample : P2269-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0RQ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031279.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	21	25	35	rVB	29791	45259	0.62%	0.071%
2	3.546	94	95	111	rBV	124474	212747	2.91%	0.332%
3	3.852	143	147	154	rVB2	7685	12953	0.18%	0.020%
4	6.740	634	638	642	rBV3	6039	9148	0.13%	0.014%
5	6.799	642	648	659	rVB	182960	294021	4.02%	0.459%
6	6.964	669	676	686	rBV	758291	1171212	16.01%	1.827%
7	7.152	701	708	718	rBV	722644	1116301	15.26%	1.741%
8	7.616	780	787	798	rBV	727568	1154329	15.78%	1.800%
9	8.328	901	908	921	rBV	558464	899209	12.30%	1.403%
10	8.775	976	984	1000	rBV	938864	1526515	20.87%	2.381%
11	9.163	1046	1050	1058	rVB	17021	26147	0.36%	0.041%
12	9.487	1098	1105	1119	rBV	741586	1211020	16.56%	1.889%
13	10.022	1189	1196	1213	rBV	1101622	1823563	24.94%	2.844%
14	10.399	1252	1260	1272	rVB	1205474	1962365	26.83%	3.061%
15	10.546	1277	1285	1303	rBV	837050	1444465	19.75%	2.253%
16	11.210	1394	1398	1407	rVB7	6847	13890	0.19%	0.022%
17	11.651	1469	1473	1477	rVB2	6155	9228	0.13%	0.014%
18	11.993	1526	1531	1539	rVB	19954	34857	0.48%	0.054%
19	13.157	1723	1729	1734	rBV	31455	50370	0.69%	0.079%
20	13.687	1812	1819	1829	rBV	2562608	3632424	49.67%	5.666%
21	13.957	1858	1865	1877	rBV2	2850032	4189645	57.29%	6.535%
22	14.269	1911	1918	1924	rBV	2077931	2991347	40.90%	4.666%
23	14.328	1924	1928	1934	rVB6	7403	14453	0.20%	0.023%
24	14.487	1949	1955	1972	rBV	199801	361673	4.95%	0.564%
25	15.263	2080	2087	2094	rBV	3804122	5398725	73.82%	8.421%
26	15.316	2094	2096	2099	rVV3	7928	8395	0.11%	0.013%
27	15.392	2103	2109	2123	rVV	1206801	1629798	22.29%	2.542%
28	15.504	2123	2128	2133	rVB	17717	27724	0.38%	0.043%
29	15.828	2180	2183	2188	rBV4	4463	7570	0.10%	0.012%
30	16.051	2217	2221	2225	rVB2	8949	10568	0.14%	0.016%
31	16.563	2304	2308	2314	rVB5	5310	8624	0.12%	0.013%
32	17.016	2379	2385	2395	rBV	2686135	3766299	51.50%	5.875%
33	17.116	2396	2402	2418	rVV2	4302916	6280576	85.88%	9.796%
34	17.381	2441	2447	2448	rBV5	7777	10701	0.15%	0.017%
35	17.404	2448	2451	2458	rVB5	5522	9813	0.13%	0.015%
36	17.916	2533	2538	2545	rBV2	45155	66029	0.90%	0.103%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042724\
Data File : BN031279.D
Acq On : 27 Apr 2024 20:02
Operator : MA/JU
Sample : P2269-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RQ1

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Title : SVOA CALIBRATION

37	18.351	2608	2612	2615	rVB6	7814	9749	0.13%	0.015%
38	18.980	2715	2719	2724	rBV2	58874	83964	1.15%	0.131%
39	19.051	2727	2731	2736	rBV	52300	76396	1.04%	0.119%
40	19.210	2754	2758	2763	rBV2	40914	55518	0.76%	0.087%
41	19.363	2780	2784	2787	rBV	27541	31247	0.43%	0.049%
42	19.422	2788	2794	2802	rBV	5378199	7313264	100.00%	11.407%
43	20.410	2960	2962	2966	rBV4	19970	20441	0.28%	0.032%
44	21.257	3100	3106	3112	rBV	2838743	3993572	54.61%	6.229%
45	23.957	3555	3565	3581	rVB2	2953010	7047915	96.37%	10.993%
46	24.151	3589	3598	3611	rVB	1702086	4047955	55.35%	6.314%




Sum of corrected areas: 64111984

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042724\
Data File : BN031279.D
Acq On : 27 Apr 2024 20:02
Operator : MA/JU
Sample : P2269-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RQ1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

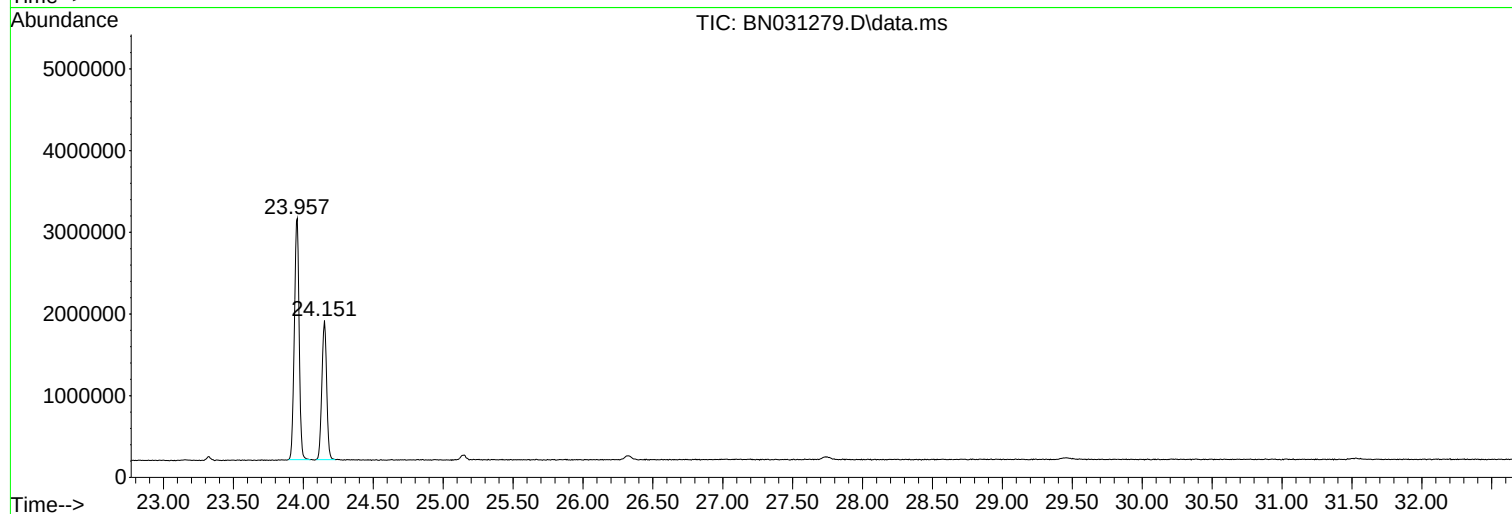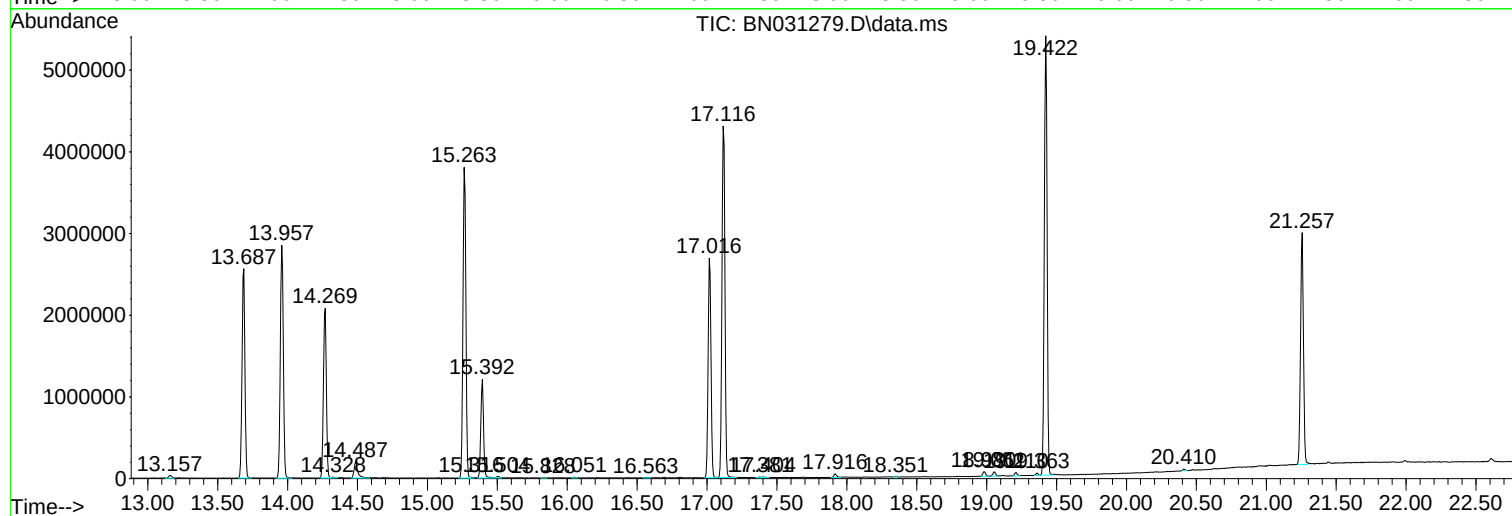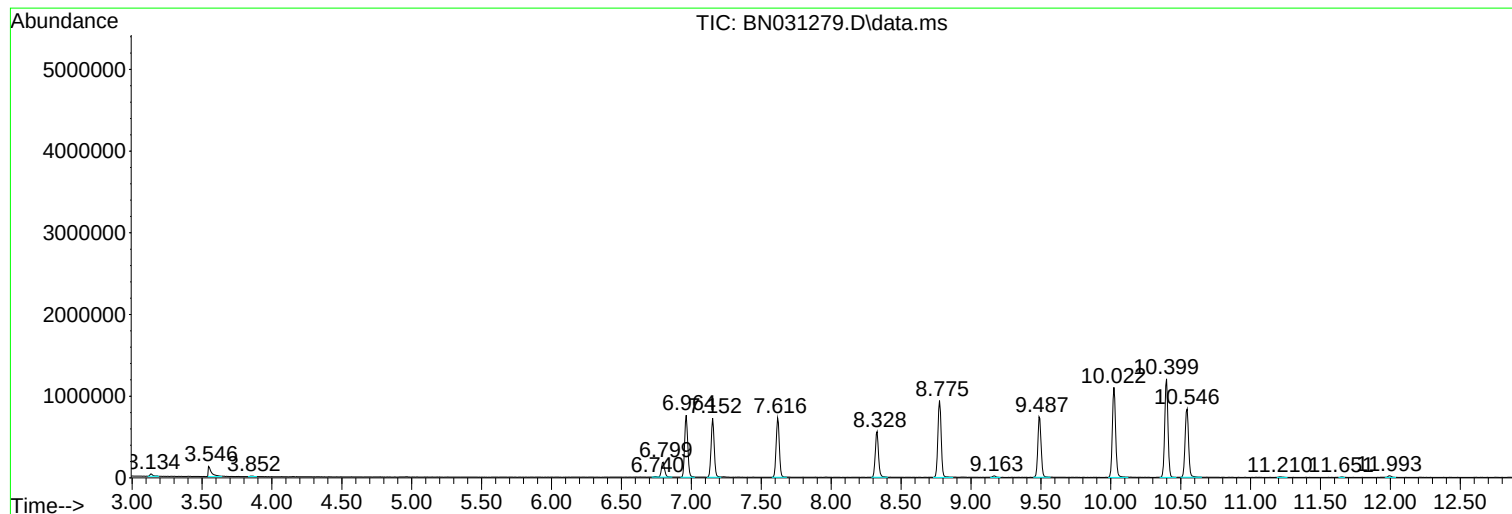

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042724\
Data File : BN031279.D
Acq On : 27 Apr 2024 20:02
Operator : MA/JU
Sample : P2269-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RQ1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042724\
Data File : BN031279.D
Acq On : 27 Apr 2024 20:02
Operator : MA/JU
Sample : P2269-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RQ1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------