

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042724\
 Data File : BN031283.D
 Acq On : 27 Apr 2024 23:19
 Operator : MA/JU
 Sample : PB160538BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK538

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031283.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	21	25	38	rVB	40085	64373	1.14%	0.104%
2	3.540	91	94	119	rBV	538491	938746	16.61%	1.522%
3	3.852	144	147	153	rVB3	9397	14765	0.26%	0.024%
4	6.799	641	648	663	rVB	764691	1214773	21.50%	1.969%
5	6.963	669	676	688	rBV	643949	1002862	17.75%	1.626%
6	7.152	700	708	720	rBV	802631	1262029	22.33%	2.046%
7	7.616	781	787	797	rBV	780704	1259123	22.28%	2.041%
8	8.328	900	908	919	rBV	1025605	1631642	28.87%	2.645%
9	8.775	977	984	996	rBV	799598	1279891	22.65%	2.075%
10	9.493	1098	1106	1121	rBV	661880	1108201	19.61%	1.797%
11	10.022	1189	1196	1217	rBV	1033175	1720415	30.44%	2.789%
12	10.399	1252	1260	1270	rVB	1310721	2126012	37.62%	3.446%
13	10.546	1276	1285	1301	rBV	1106915	1860754	32.93%	3.016%
14	11.998	1525	1532	1539	rBV2	16952	31363	0.55%	0.051%
15	13.157	1725	1729	1735	rVB	26024	39067	0.69%	0.063%
16	13.687	1812	1819	1830	rBV	2079634	2924828	51.76%	4.741%
17	13.957	1857	1865	1878	rBV	2348020	3464169	61.30%	5.616%
18	14.269	1910	1918	1931	rBV	2224764	3269455	57.85%	5.300%
19	14.481	1948	1954	1972	rBV	919487	1476812	26.13%	2.394%
20	15.263	2080	2087	2100	rBV	2988212	4323591	76.51%	7.009%
21	15.392	2103	2109	2123	rVV	986686	1335172	23.63%	2.164%
22	15.504	2123	2128	2133	rVB2	14688	22495	0.40%	0.036%
23	16.051	2216	2221	2224	rBV3	6505	8473	0.15%	0.014%
24	16.804	2344	2349	2352	rBV2	6422	8857	0.16%	0.014%
25	17.016	2379	2385	2394	rBV	2891464	4142538	73.30%	6.715%
26	17.116	2396	2402	2415	rVB2	3533272	4796127	84.87%	7.775%
27	17.916	2535	2538	2542	rBV4	8051	12634	0.22%	0.020%
28	18.986	2715	2720	2724	rVB2	43526	66113	1.17%	0.107%
29	19.051	2727	2731	2736	rVV	38434	56591	1.00%	0.092%
30	19.116	2740	2742	2747	rVB5	6868	10497	0.19%	0.017%
31	19.210	2755	2758	2762	rBV4	8850	11539	0.20%	0.019%
32	19.357	2780	2783	2788	rBV2	19673	24631	0.44%	0.040%
33	19.422	2788	2794	2801	rBV2	4174548	5651258	100.00%	9.161%
34	21.251	3099	3105	3114	rBV	3066822	4486440	79.39%	7.273%
35	23.951	3555	3564	3580	rVB2	2281277	5468476	96.77%	8.865%
36	24.145	3588	3597	3614	rVB	1836529	4571888	80.90%	7.411%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042724\
Data File : BN031283.D
Acq On : 27 Apr 2024 23:19
Operator : MA/JU
Sample : PB160538BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK538

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 61686600

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042724\
Data File : BN031283.D
Acq On : 27 Apr 2024 23:19
Operator : MA/JU
Sample : PB160538BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK538

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

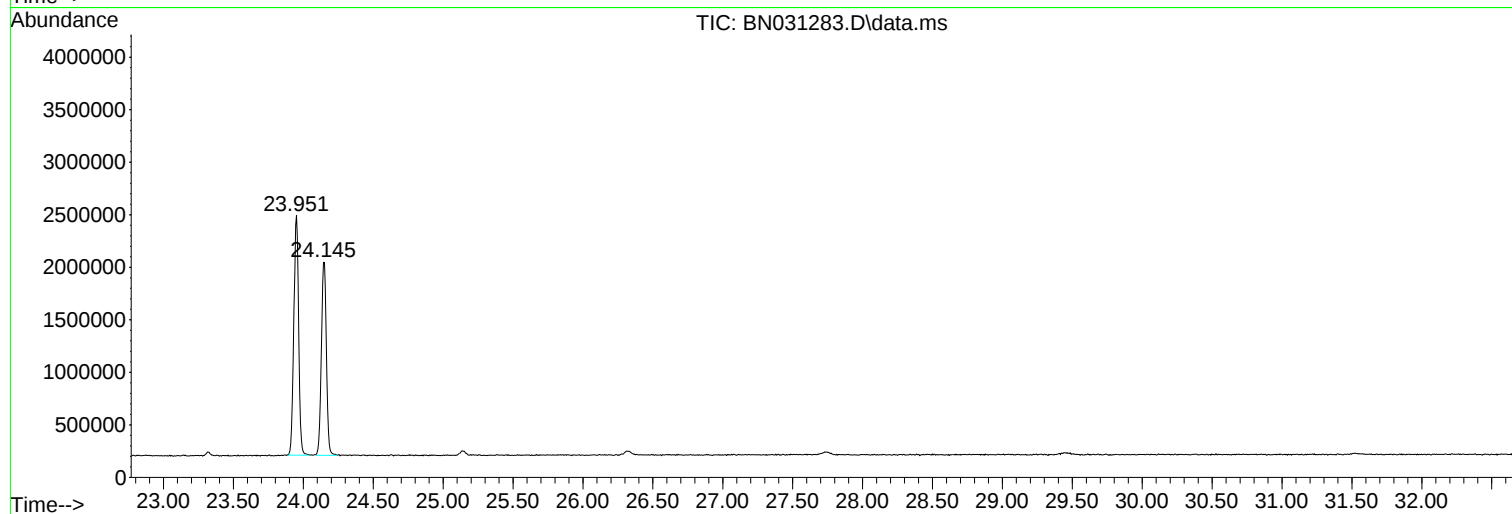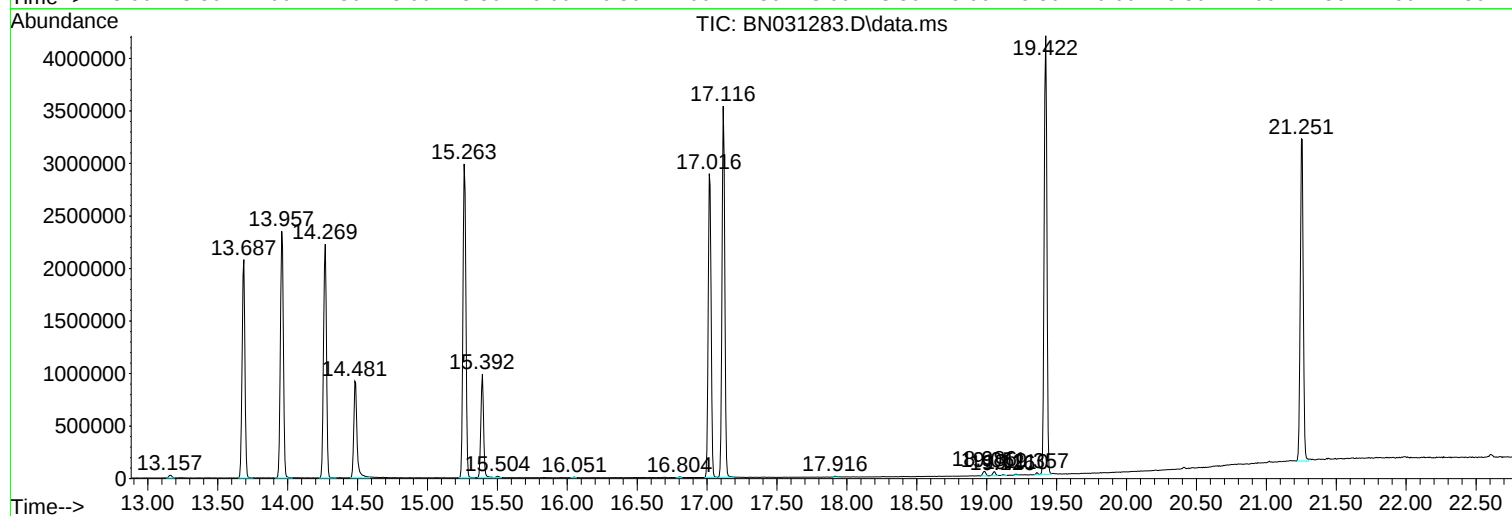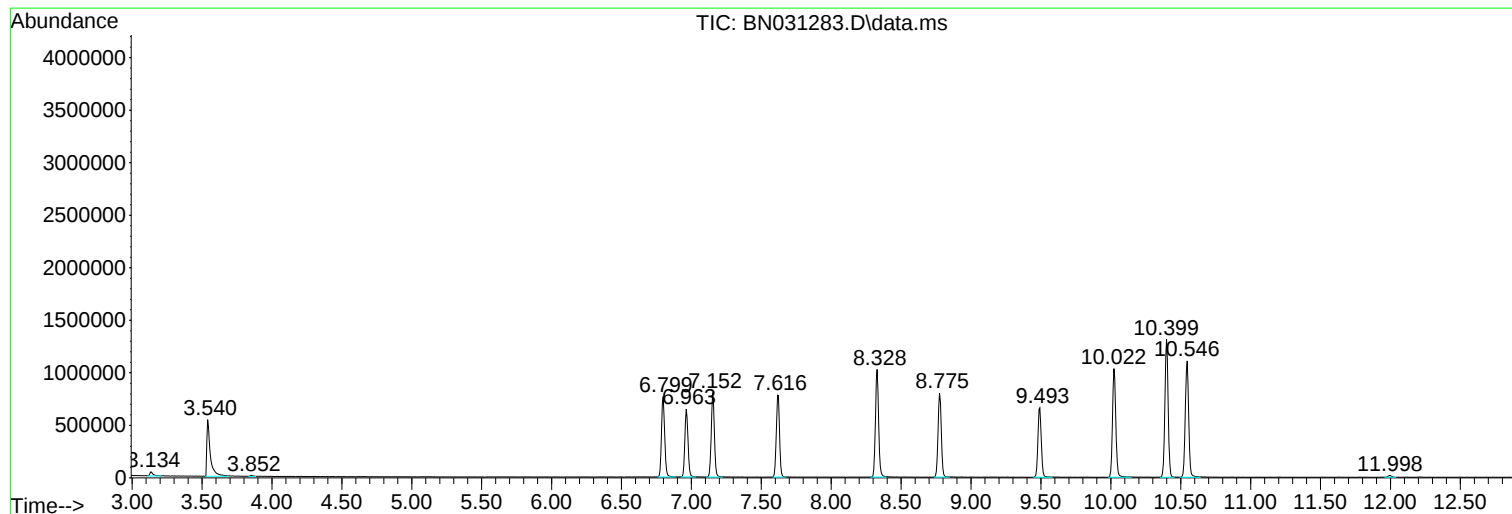

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042724\
Data File : BN031283.D
Acq On : 27 Apr 2024 23:19
Operator : MA/JU
Sample : PB160538BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK538

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042724\
Data File : BN031283.D
Acq On : 27 Apr 2024 23:19
Operator : MA/JU
Sample : PB160538BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK538

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------