

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042724\
 Data File : BN031284.D
 Acq On : 27 Apr 2024 23:59
 Operator : MA/JU
 Sample : PB160492BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK492

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031284.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	22	26	33	rBV	48123	71558	1.06%	0.103%
2	3.540	92	94	115	rBV	717169	1175983	17.43%	1.695%
3	3.858	144	148	155	rVB2	10618	17700	0.26%	0.026%
4	6.799	641	648	662	rBV	954948	1512367	22.41%	2.180%
5	6.964	670	676	686	rVB	816465	1242476	18.41%	1.791%
6	7.152	701	708	721	rBV	1002017	1565709	23.20%	2.257%
7	7.617	779	787	796	rBV	793113	1253392	18.58%	1.806%
8	8.328	899	908	921	rBV	1278984	2027940	30.05%	2.923%
9	8.775	976	984	997	rBV	1001319	1601325	23.73%	2.308%
10	9.493	1097	1106	1116	rBV	829636	1370535	20.31%	1.975%
11	10.022	1187	1196	1215	rBV	1276212	2129239	31.56%	3.069%
12	10.399	1251	1260	1268	rBV	1282643	2096059	31.06%	3.021%
13	10.546	1276	1285	1302	rBV	1358041	2293027	33.98%	3.305%
14	11.993	1525	1531	1536	rBV	20771	35098	0.52%	0.051%
15	13.157	1725	1729	1737	rVB2	24371	40259	0.60%	0.058%
16	13.228	1737	1741	1750	rVB9	3005	7148	0.11%	0.010%
17	13.687	1812	1819	1830	rBV	2539992	3510917	52.03%	5.060%
18	13.957	1858	1865	1879	rBV2	2869310	4168015	61.77%	6.007%
19	14.269	1911	1918	1927	rBV	2113192	3157308	46.79%	4.550%
20	14.487	1948	1955	1971	rBV	1159864	1846186	27.36%	2.661%
21	15.263	2080	2087	2097	rBV	3501102	5119578	75.87%	7.378%
22	15.393	2102	2109	2122	rVV	1196337	1669132	24.74%	2.406%
23	15.504	2124	2128	2135	rVB2	18739	27446	0.41%	0.040%
24	16.051	2218	2221	2224	rBV4	8323	10282	0.15%	0.015%
25	16.693	2327	2330	2334	rBV4	5426	6780	0.10%	0.010%
26	16.810	2345	2350	2356	rBV3	6792	13139	0.19%	0.019%
27	17.022	2379	2386	2392	rBV	2759074	3968008	58.81%	5.719%
28	17.116	2396	2402	2416	rVV2	3860671	5751460	85.24%	8.289%
29	17.922	2533	2539	2544	rBV7	11281	19438	0.29%	0.028%
30	18.981	2714	2719	2725	rBV2	55499	79521	1.18%	0.115%
31	19.051	2727	2731	2738	rVV	46702	68495	1.02%	0.099%
32	19.210	2754	2758	2761	rBV5	13229	19829	0.29%	0.029%
33	19.357	2780	2783	2787	rBV3	16666	19919	0.30%	0.029%
34	19.422	2788	2794	2801	rBV	5018969	6747502	100.00%	9.725%
35	21.251	3100	3105	3117	rBV	2946238	4229139	62.68%	6.095%
36	23.951	3555	3564	3579	rVB2	2709123	6363001	94.30%	9.170%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042724\
Data File : BN031284.D
Acq On : 27 Apr 2024 23:59
Operator : MA/JU
Sample : PB160492BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK492

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Title : SVOA CALIBRATION

37	24.145	3589	3597	3613	rVB	1712082	4150800	61.52%	5.982%
----	--------	------	------	------	-----	---------	---------	--------	--------


Sum of corrected areas: 69385710

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042724\
Data File : BN031284.D
Acq On : 27 Apr 2024 23:59
Operator : MA/JU
Sample : PB160492BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK492

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

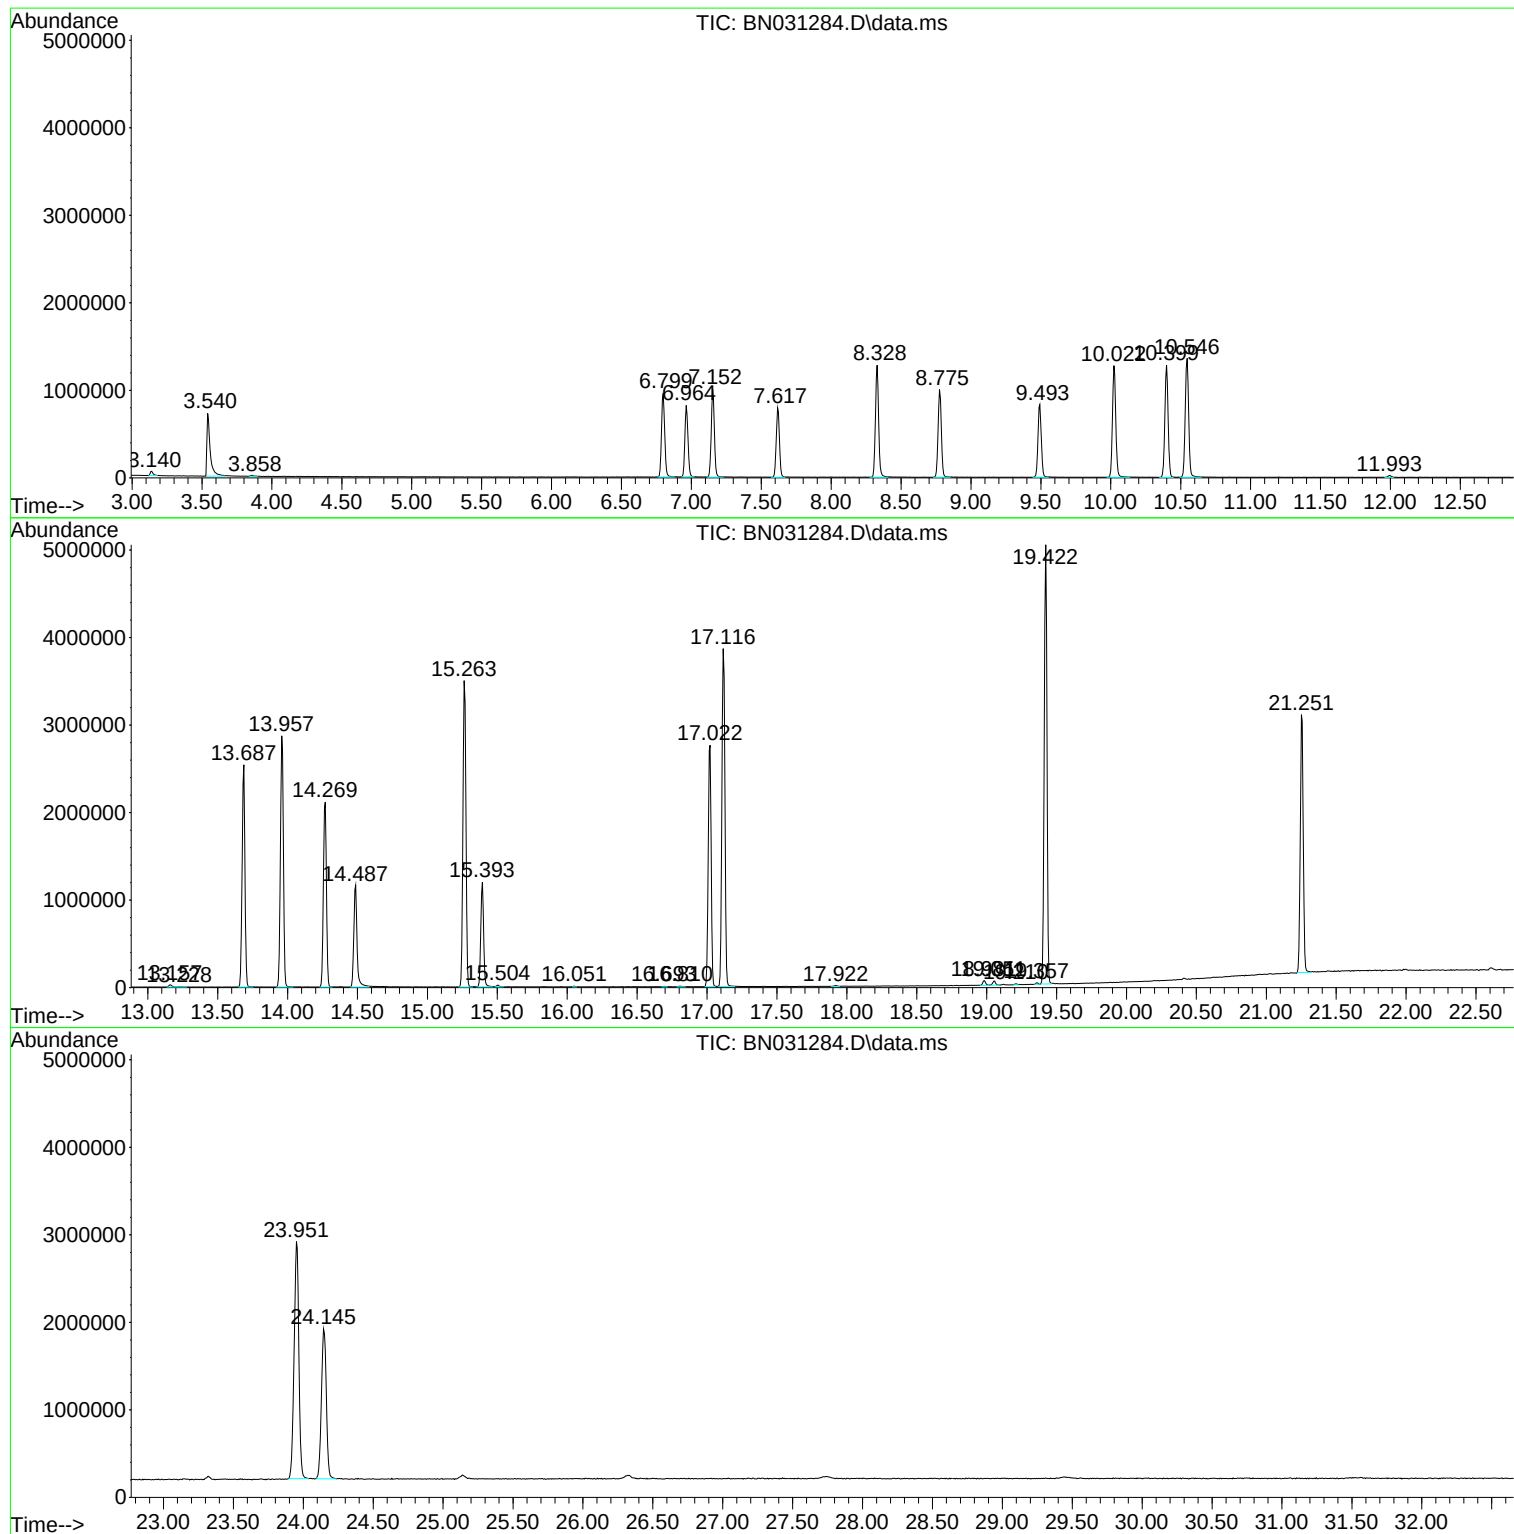

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042724\
Data File : BN031284.D
Acq On : 27 Apr 2024 23:59
Operator : MA/JU
Sample : PB160492BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK492

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042724\
Data File : BN031284.D
Acq On : 27 Apr 2024 23:59
Operator : MA/JU
Sample : PB160492BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK492

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------