

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042724\
 Data File : BN031286.D
 Acq On : 28 Apr 2024 01:18
 Operator : MA/JU
 Sample : P2203-04
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1CZ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031286.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	22	25	33	rVB	28488	41487	0.59%	0.062%
2	3.552	93	96	114	rBV	92983	174664	2.48%	0.260%
3	3.852	144	147	154	rVB	10604	14927	0.21%	0.022%
4	4.964	330	336	341	rBV	15976	26926	0.38%	0.040%
5	5.699	455	461	465	rBV7	4236	7378	0.10%	0.011%
6	6.534	596	603	606	rBV6	5206	7335	0.10%	0.011%
7	6.799	642	648	660	rVB	198276	313489	4.46%	0.466%
8	6.963	669	676	688	rBV	786932	1204428	17.13%	1.791%
9	7.152	702	708	719	rBV	733811	1150964	16.37%	1.712%
10	7.616	776	787	794	rBV	788005	1286905	18.31%	1.914%
11	7.681	794	798	809	rVB	75624	127131	1.81%	0.189%
12	7.963	842	846	853	rVB	13746	24047	0.34%	0.036%
13	8.328	901	908	919	rBV	626629	1000264	14.23%	1.488%
14	8.446	923	928	932	rVB	44020	69631	0.99%	0.104%
15	8.716	969	974	977	rBV4	18574	27670	0.39%	0.041%
16	8.775	977	984	992	rVV	944766	1514277	21.54%	2.252%
17	8.940	1006	1012	1019	rVB8	8861	17509	0.25%	0.026%
18	9.493	1097	1106	1122	rBV	778844	1296601	18.45%	1.928%
19	9.652	1129	1133	1142	rVB	4711	9418	0.13%	0.014%
20	9.793	1154	1157	1166	rVB8	4186	8557	0.12%	0.013%
21	9.899	1166	1175	1180	rBV	13450	25398	0.36%	0.038%
22	10.022	1189	1196	1206	rBV	1166969	1894664	26.95%	2.818%
23	10.187	1219	1224	1233	rBV7	11212	18596	0.26%	0.028%
24	10.263	1233	1237	1241	rVB4	10091	14896	0.21%	0.022%
25	10.399	1251	1260	1267	rBV	1338281	2150463	30.59%	3.198%
26	10.451	1267	1269	1277	rVB5	23557	35988	0.51%	0.054%
27	10.546	1277	1285	1303	rBV	1031509	1745431	24.83%	2.596%
28	11.057	1366	1372	1379	rVB2	17476	32312	0.46%	0.048%
29	11.199	1390	1396	1399	rBV7	7091	12749	0.18%	0.019%
30	11.587	1458	1462	1468	rBV6	8113	13522	0.19%	0.020%
31	11.816	1497	1501	1506	rVB7	4332	8146	0.12%	0.012%
32	11.993	1526	1531	1536	rVB2	20809	33085	0.47%	0.049%
33	12.069	1536	1544	1551	rVB3	19060	36296	0.52%	0.054%
34	12.293	1577	1582	1586	rBV3	8779	12558	0.18%	0.019%
35	12.869	1675	1680	1683	rBV3	9394	12225	0.17%	0.018%
36	13.110	1715	1721	1725	rBV	23354	32160	0.46%	0.048%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042724\
Data File : BN031286.D
Acq On : 28 Apr 2024 01:18
Operator : MA/JU
Sample : P2203-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1CZ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Title : SVOA CALIBRATION

37	13.163	1725	1730	1734	rVV	20989	33283	0.47%	0.050%
38	13.504	1783	1788	1793	rVV6	9296	13925	0.20%	0.021%
39	13.687	1812	1819	1825	rBV	2594596	3547146	50.46%	5.276%
40	13.728	1825	1826	1833	rVB3	9206	10103	0.14%	0.015%
41	13.957	1856	1865	1878	rBV	2914936	4217694	60.00%	6.273%
42	14.269	1910	1918	1927	rBV	2216153	3283654	46.71%	4.884%
43	14.487	1950	1955	1969	rBV	202720	360808	5.13%	0.537%
44	14.687	1984	1989	1994	rVB9	6713	12421	0.18%	0.018%
45	14.945	2029	2033	2040	rBV2	12909	23772	0.34%	0.035%
46	15.069	2050	2054	2064	rBV3	17827	39397	0.56%	0.059%
47	15.263	2081	2087	2096	rBV	3735718	5301678	75.42%	7.885%
48	15.392	2101	2109	2123	rBV	1197815	1694049	24.10%	2.519%
49	15.504	2124	2128	2132	rVB2	20818	28147	0.40%	0.042%
50	15.634	2146	2150	2154	rBV3	8240	10034	0.14%	0.015%
51	15.839	2181	2185	2189	rBV6	7055	10517	0.15%	0.016%
52	15.875	2189	2191	2197	rVB6	5725	7652	0.11%	0.011%
53	16.051	2216	2221	2227	rVB	13320	18320	0.26%	0.027%
54	16.616	2314	2317	2321	rVB5	6426	9688	0.14%	0.014%
55	16.698	2328	2331	2336	rBV5	5568	7554	0.11%	0.011%
56	16.804	2341	2349	2352	rBV4	7791	13837	0.20%	0.021%
57	17.016	2379	2385	2395	rVB	2798464	4079348	58.03%	6.067%
58	17.116	2395	2402	2413	rBV2	4115559	5957635	84.75%	8.861%
59	17.310	2430	2435	2440	rBV	23042	29098	0.41%	0.043%
60	17.692	2494	2500	2506	rBV	222140	277051	3.94%	0.412%
61	17.863	2525	2529	2534	rBV7	4426	9135	0.13%	0.014%
62	17.916	2534	2538	2547	rBV	199385	309949	4.41%	0.461%
63	17.992	2547	2551	2562	rVB	30188	63481	0.90%	0.094%
64	18.169	2578	2581	2585	rVV3	10755	12395	0.18%	0.018%
65	18.210	2585	2588	2593	rVB6	10228	12143	0.17%	0.018%
66	18.351	2608	2612	2617	rBV3	20555	26869	0.38%	0.040%
67	18.786	2682	2686	2689	rBV2	12045	15246	0.22%	0.023%
68	18.980	2715	2719	2725	rBV2	60121	81715	1.16%	0.122%
69	19.051	2727	2731	2735	rBV	56558	78067	1.11%	0.116%
70	19.116	2740	2742	2746	rVB4	13765	14673	0.21%	0.022%
71	19.210	2753	2758	2770	rBV	223704	347260	4.94%	0.516%
72	19.357	2779	2783	2787	rBV4	40100	51418	0.73%	0.076%
73	19.422	2788	2794	2801	rBV	5146492	7029482	100.00%	10.455%
74	20.410	2960	2962	2965	rBV2	24507	20740	0.30%	0.031%
75	21.251	3099	3105	3116	rBV	3083205	4444869	63.23%	6.611%
76	23.951	3555	3564	3576	rVB2	2934983	6769944	96.31%	10.069%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042724\
Data File : BN031286.D
Acq On : 28 Apr 2024 01:18
Operator : MA/JU
Sample : P2203-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1CZ0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Title : SVOA CALIBRATION

77	24.145	3588	3597	3610	rVB	1873933	4561762	64.89%	6.784%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 67238056

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042724\
Data File : BN031286.D
Acq On : 28 Apr 2024 01:18
Operator : MA/JU
Sample : P2203-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1CZ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

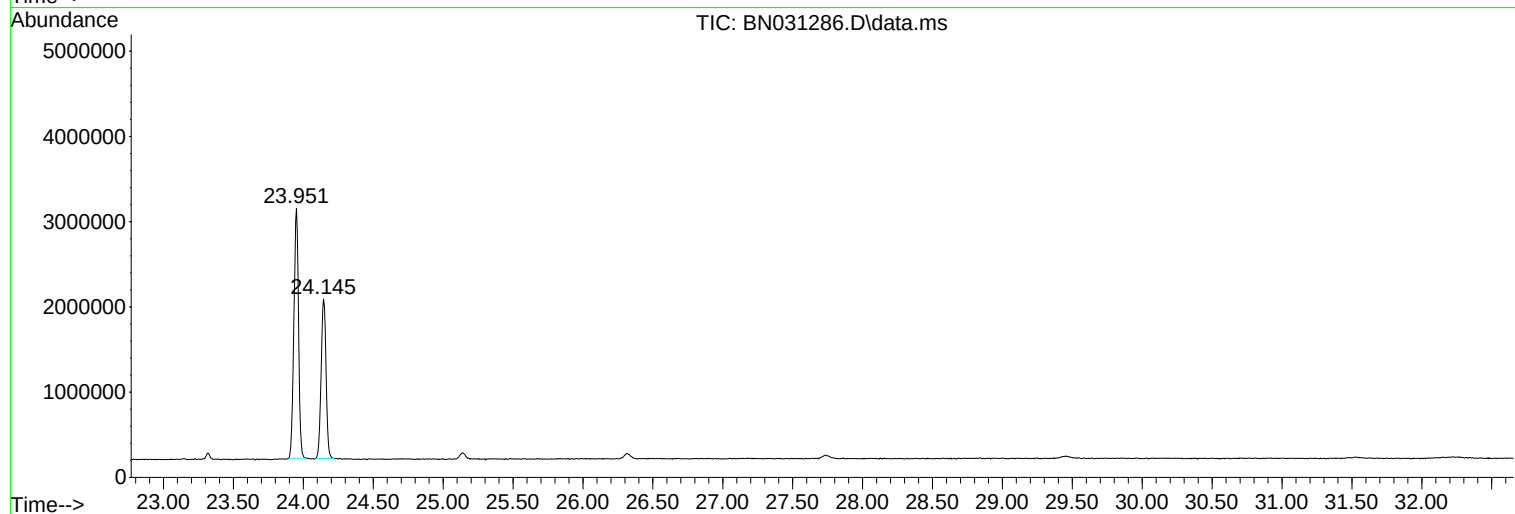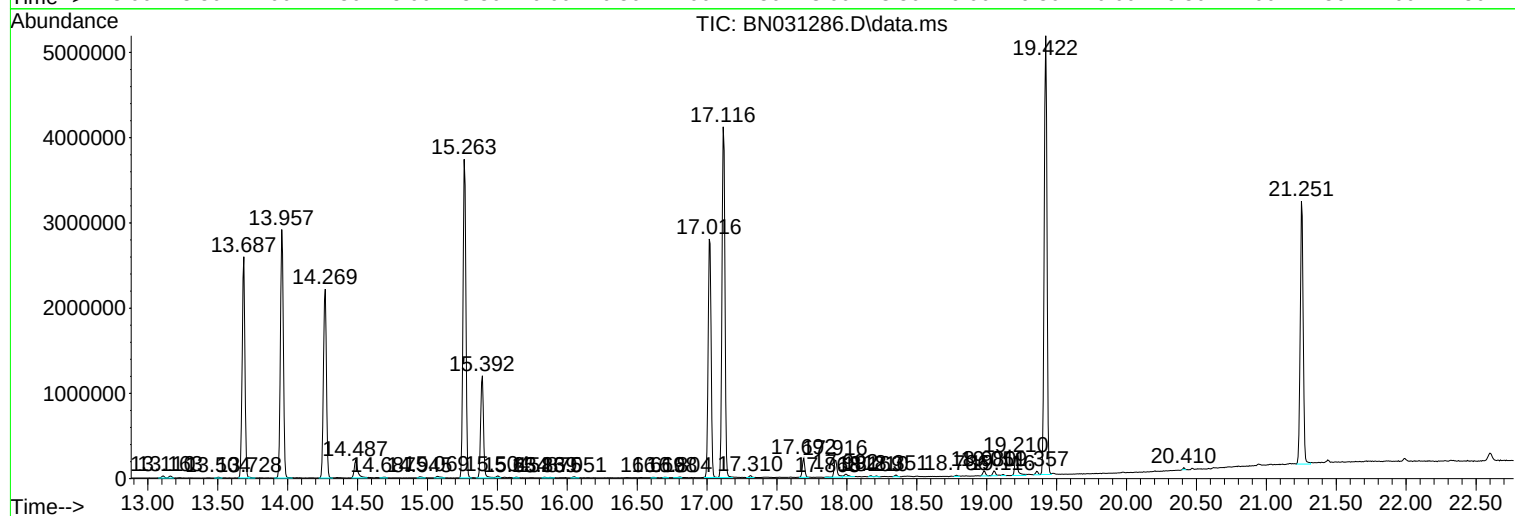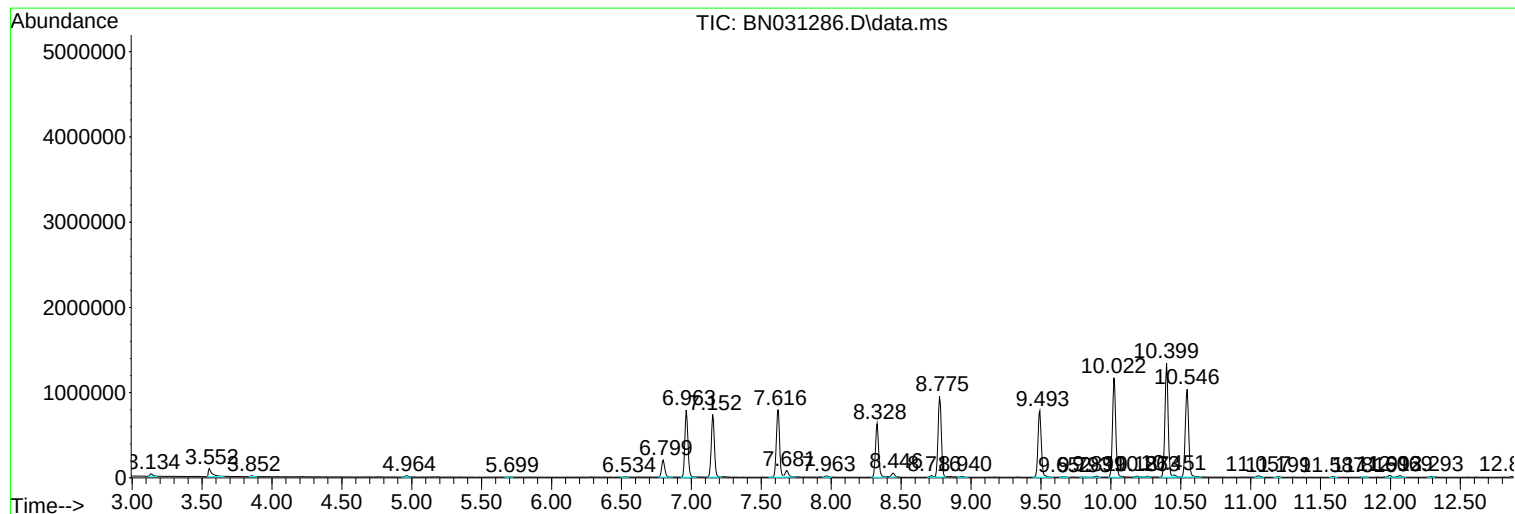

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042724\
Data File : BN031286.D
Acq On : 28 Apr 2024 01:18
Operator : MA/JU
Sample : P2203-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1CZ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042724\
Data File : BN031286.D
Acq On : 28 Apr 2024 01:18
Operator : MA/JU
Sample : P2203-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1CZ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------