

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042821\
 Data File : BN014462.D
 Acq On : 27 Apr 2021 18:13
 Operator : CG/JU
 Sample : SSTDICC3.2
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2

Quant Time: Apr 27 18:59:04 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 27 18:52:25 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.668	152	10313	0.40	ng	0.00
7) Naphthalene-d8	10.442	136	36025	0.40	ng	0.00
13) Acenaphthene-d10	14.308	164	19073	0.40	ng	0.00
19) Phenanthrene-d10	17.055	188	38536	0.40	ng	0.00
29) Chrysene-d12	21.250	240	41905	0.40	ng	0.00
35) Perylene-d12	23.469	264	33078	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.276	112	61673	2.91	ng	0.00
5) Phenol-d6	6.839	99	81211	3.12	ng	0.00
8) Nitrobenzene-d5	8.807	82	82267	2.72	ng	-0.01
11) 2-Methylnaphthalene-d10	12.040	152	175922	3.25	ng	0.00
14) 2,4,6-Tribromophenol	15.793	330	23885	3.90	ng	0.00
15) 2-Fluorobiphenyl	12.925	172	226344	3.00	ng	0.00
27) Fluoranthene-d10	19.089	212	354511	3.47	ng	0.00
31) Terphenyl-d14	19.695	244	270096	3.04	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.231	88	32872	2.61	ng	98
3) n-Nitrosodimethylamine	3.553	42	20288	3.09	ng	# 100
6) bis(2-Chloroethyl)ether	7.104	93	76111	2.98	ng	99
9) Naphthalene	10.492	128	282438	3.16	ng	99
10) Hexachlorobutadiene	10.784	225	53771	2.75	ng	# 99
12) 2-Methylnaphthalene	12.111	142	188661	3.23	ng	99
16) Acenaphthylene	14.016	152	263616	3.26	ng	100
17) Acenaphthene	14.371	154	174644	3.27	ng	96
18) Fluorene	15.361	166	217874	3.31	ng	99
20) 4,6-Dinitro-2-methylph...	15.437	198	16268	3.78	ng	# 18
21) 4-Bromophenyl-phenylether	16.252	248	67344	3.10	ng	96
22) Hexachlorobenzene	16.362	284	84747	2.84	ng	99
23) Atrazine	16.520	200	46219	3.68	ng	98
24) Pentachlorophenol	16.702	266	21778	3.95	ng	99
25) Phenanthrene	17.092	178	351071	3.24	ng	100
26) Anthracene	17.177	178	300200	3.54	ng	100
28) Fluoranthene	19.119	202	400101	3.46	ng	99
30) Pyrene	19.481	202	394427	3.16	ng	100
32) Benzo(a)anthracene	21.239	228	388967	3.51	ng	100
33) Chrysene	21.282	228	402427	3.08	ng	100
34) Bis(2-ethylhexyl)phtha...	21.176	149	151848	3.87	ng	95
36) Indeno(1,2,3-cd)pyrene	25.693	276	434407	3.15	ng	98
37) Benzo(b)fluoranthene	22.805	252	387035	3.18	ng	# 92
38) Benzo(k)fluoranthene	22.805	252	387035	3.13	ng	95
39) Benzo(a)pyrene	23.373	252	355983	3.45	ng	# 83
40) Dibenzo(a,h)anthracene	25.707	278	363056	3.17	ng	96
41) Benzo(g,h,i)perylene	26.371	276	370179	3.06	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042821\
Data File : BN014462.D
Acq On : 27 Apr 2021 18:13
Operator : CG/JU
Sample : SSTDICC3.2
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Quant Time: Apr 27 18:59:04 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 27 18:52:25 2021
Response via : Initial Calibration




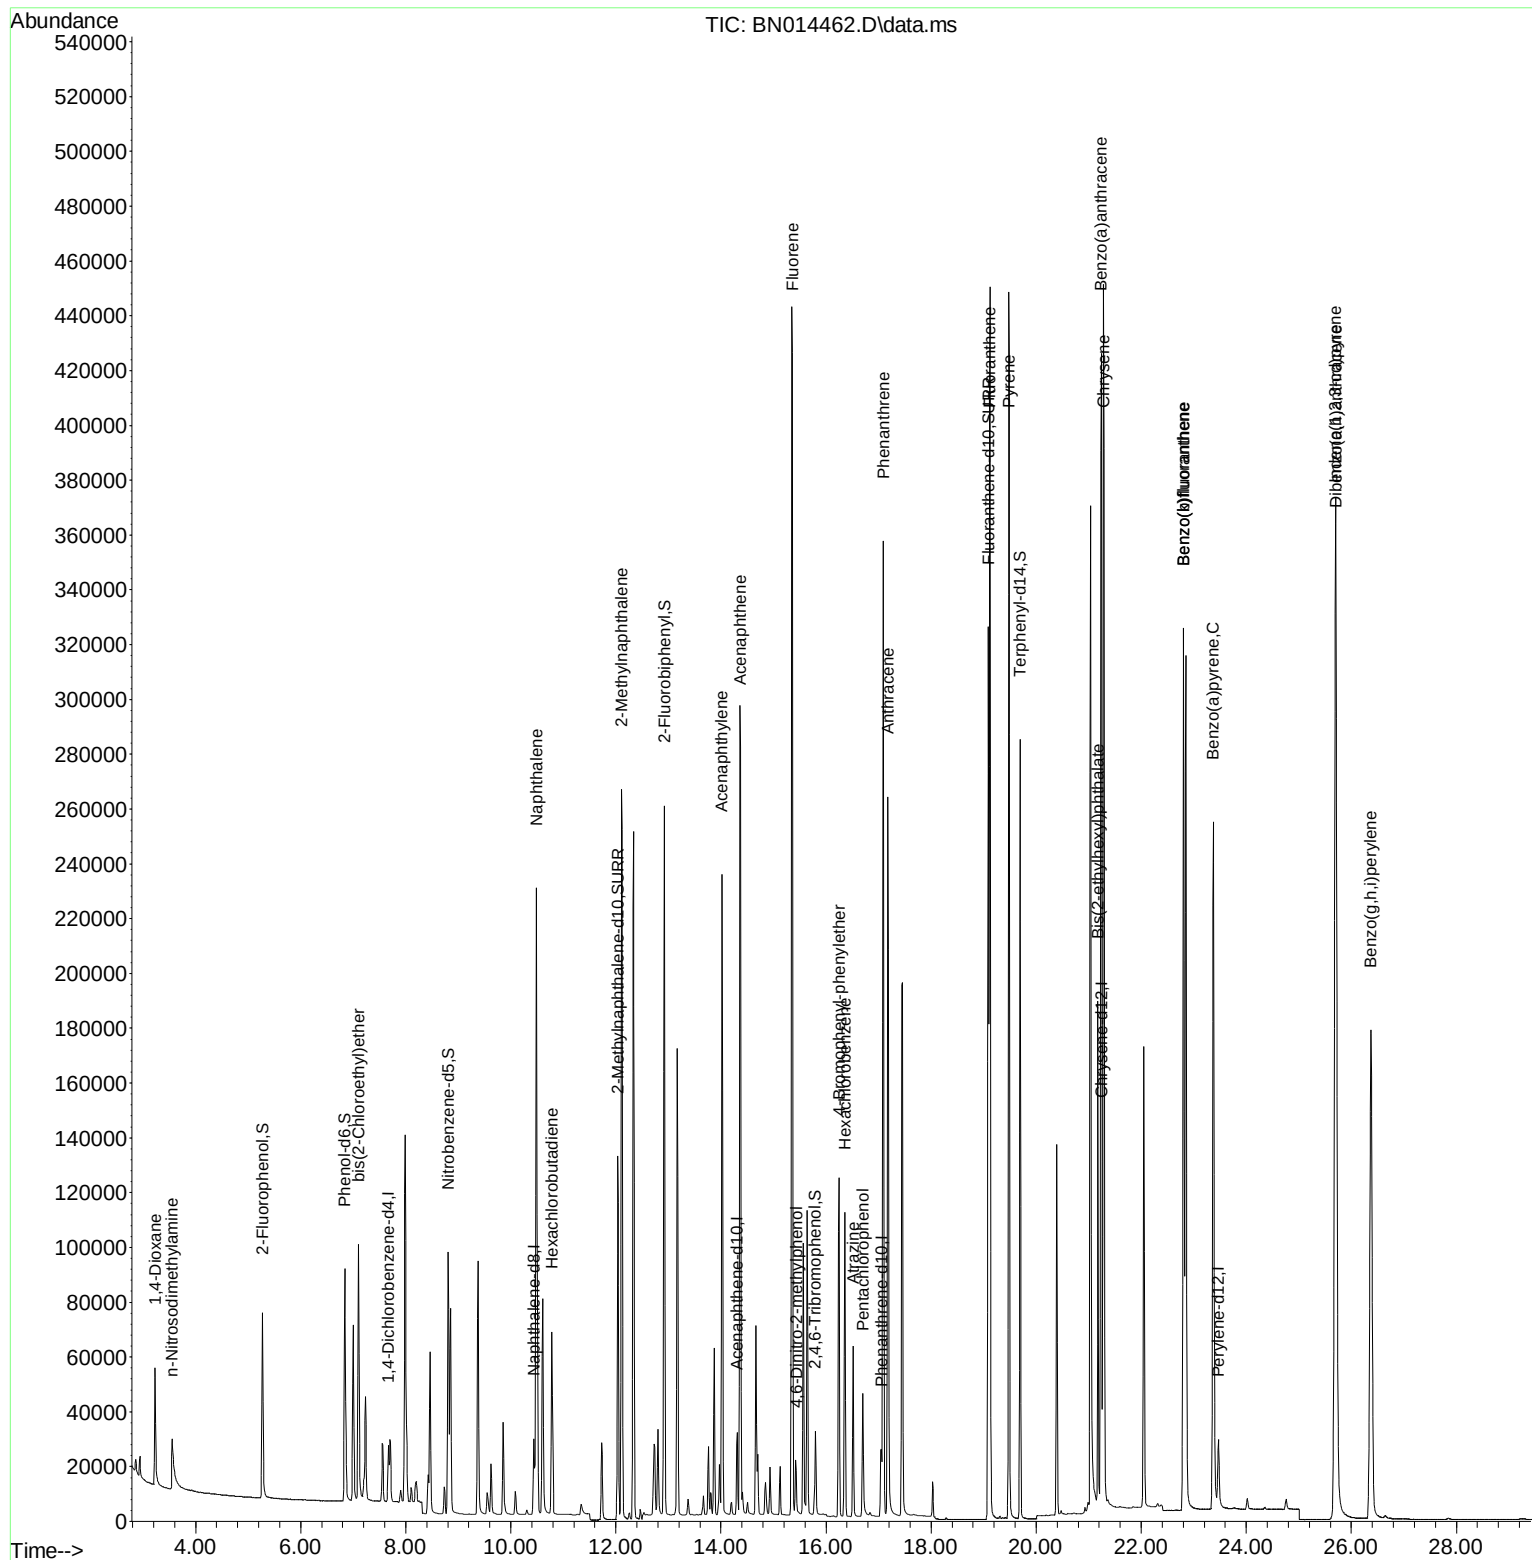


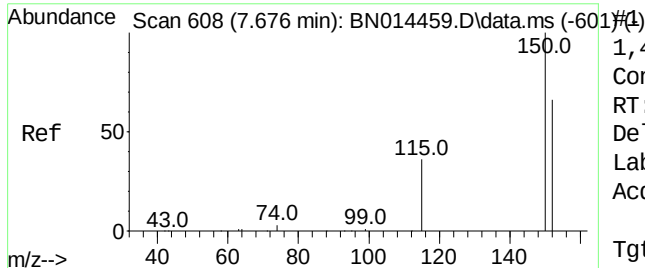

1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.668 min Scan# 607
Delta R.T. -0.008 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:	152	Resp:	10313
Ion	Ratio	Lower	Upper
152	100		
150	160.4	121.2	181.8
115	60.8	46.0	69.0

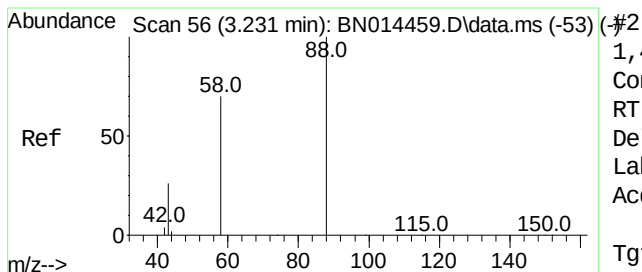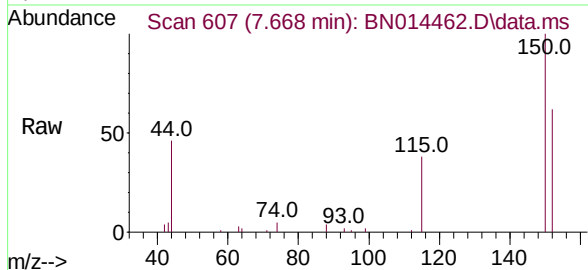

1,4-Dioxane
Concen: 2.61 ng
RT: 3.231 min Scan# 56
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

Tgt Ion:	88	Resp:	32872
Ion	Ratio	Lower	Upper
88	100		
58	65.2	53.1	79.7
43	23.8	20.3	30.5







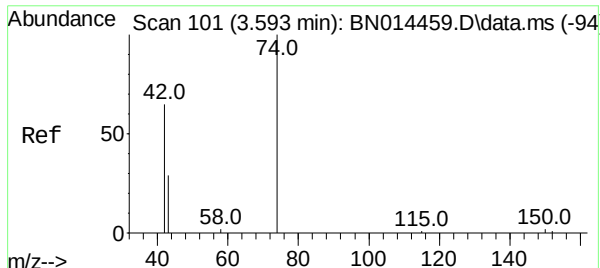

Scan 101 (3.593 min): BN014459.D\data.ms (-94) #3
 n-Nitrosodimethylamine
 Concen: 3.09 ng
 RT: 3.553 min Scan# 96
 Delta R.T. -0.040 min
 Lab File: BN014462.D
 Acq: 27 Apr 2021 18:13




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2


Tgt Ion:	42	Resp:	20288
Ion	Ratio	Lower	Upper
42	100		
74	155.9	124.7	187.1
44	6.4	0.0	0.0#

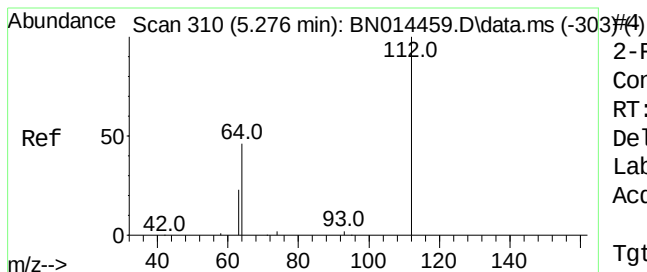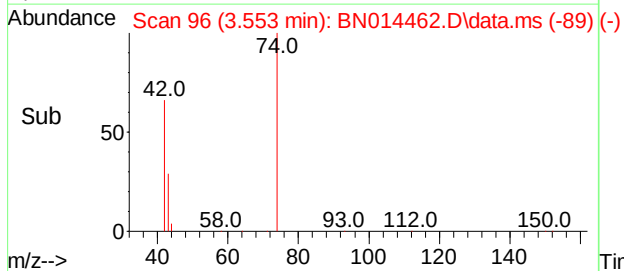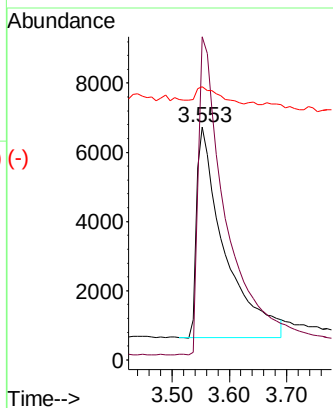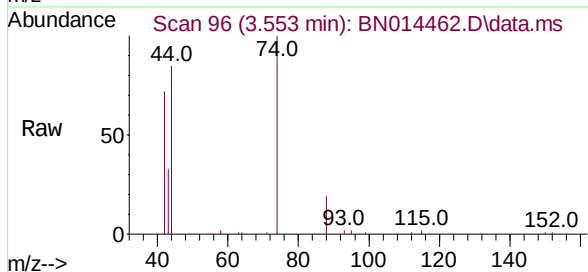

Scan 310 (5.276 min): BN014459.D\data.ms (-303) #4
 2-Fluorophenol
 Concen: 2.91 ng
 RT: 5.276 min Scan# 310
 Delta R.T. -0.000 min
 Lab File: BN014462.D
 Acq: 27 Apr 2021 18:13

Tgt Ion:	112	Resp:	61673
Ion	Ratio	Lower	Upper
112	100		
64	51.9	41.4	62.2
63	27.0	21.8	32.8


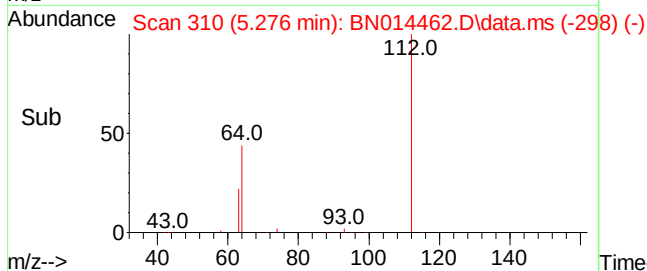




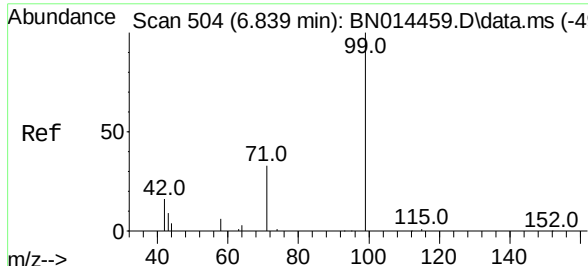

Phenol-d6
 Concen: 3.12 ng
 RT: 6.839 min Scan# 504
 Delta R.T. -0.000 min
 Lab File: BN014462.D
 Acq: 27 Apr 2021 18:13




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2

Tgt Ion:	99	Resp:	81211
Ion	Ratio	Lower	Upper
99	100		
42	16.9	13.8	20.6
71	31.9	25.5	38.3

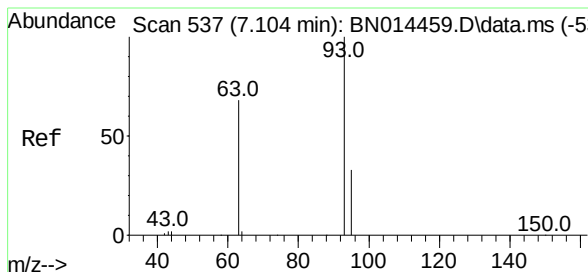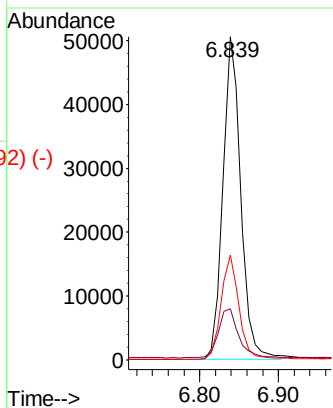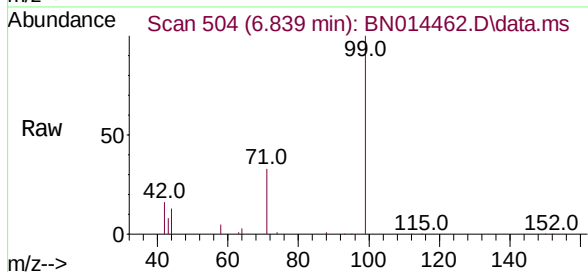

bis(2-Chloroethyl)ether
 Concen: 2.98 ng
 RT: 7.104 min Scan# 537
 Delta R.T. -0.000 min
 Lab File: BN014462.D
 Acq: 27 Apr 2021 18:13


Tgt Ion:	93	Resp:	76111
Ion	Ratio	Lower	Upper
93	100		
63	71.4	56.7	85.1
95	33.5	26.3	39.5






Abundance Scan 855 (10.442 min): BN014459.D\data.ms (-8507-)

Naphthalene-d8
Concen: 0.40 ng
RT: 10.442 min Scan# 855
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

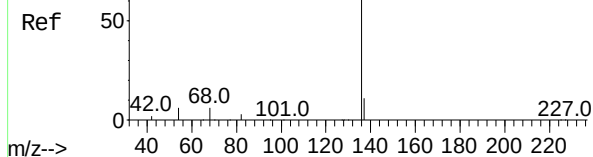


Tgt Ion:	136	Resp:	36025
Ion Ratio	Lower	Upper	
136	100		
137	11.1	9.0	13.4
54	6.3	5.7	8.5
68	6.0	5.2	7.8

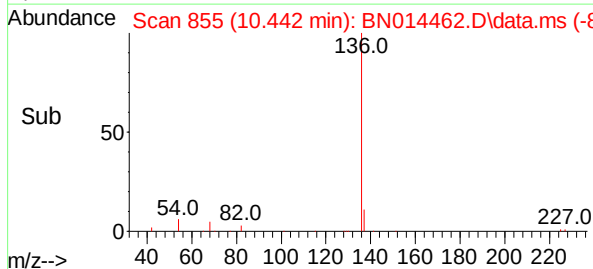
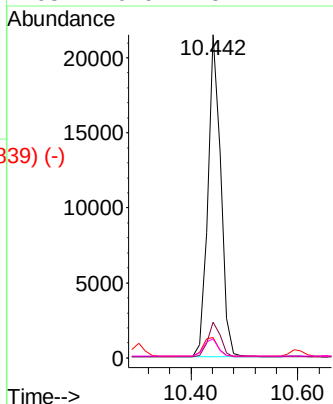
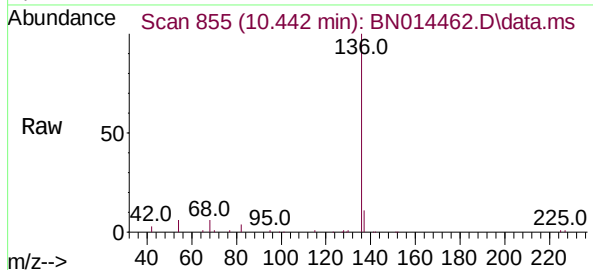



Abundance Scan 727 (8.819 min): BN014459.D\data.ms (-7237-)

Nitrobenzene-d5
Concen: 2.72 ng
RT: 8.807 min Scan# 726
Delta R.T. -0.013 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

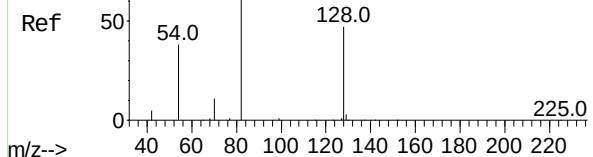

Tgt Ion:	82	Resp:	82267
Ion Ratio	Lower	Upper	
82	100		
128	34.7	38.5	57.7#
54	46.0	32.1	48.1


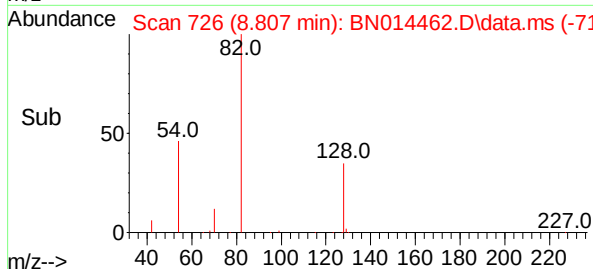
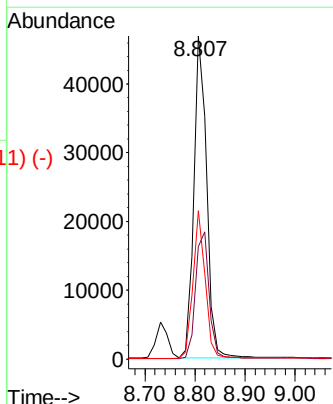
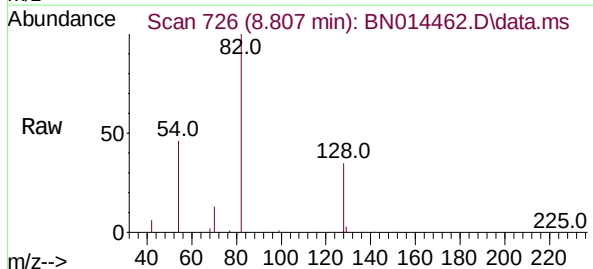


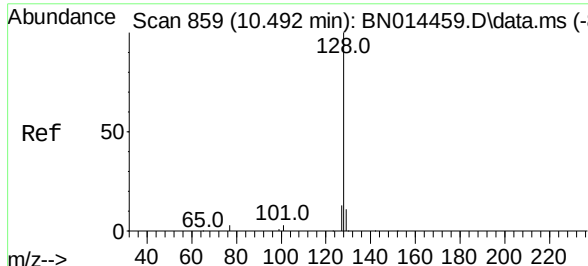

Naphthalene
 Concen: 3.16 ng
 RT: 10.492 min Scan# 859
 Delta R.T. -0.000 min
 Lab File: BN014462.D
 Acq: 27 Apr 2021 18:13




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2

Tgt Ion:	128	Resp:	282438
Ion	Ratio	Lower	Upper
128	100		
129	10.9	9.0	13.4
127	12.8	10.5	15.7

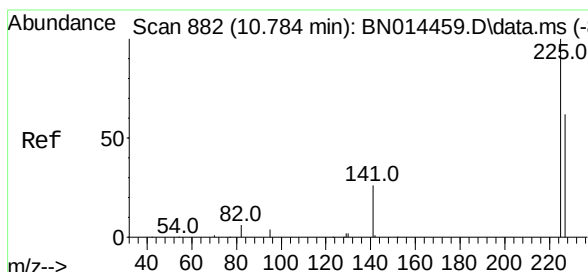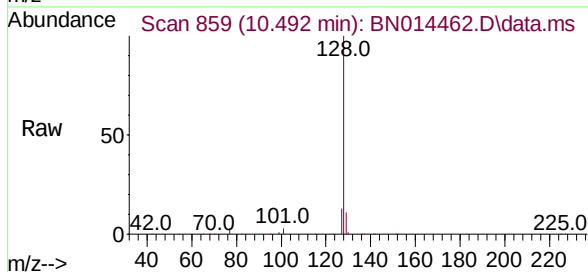


Hexachlorobutadiene
 Concen: 2.75 ng
 RT: 10.784 min Scan# 882
 Delta R.T. -0.000 min
 Lab File: BN014462.D
 Acq: 27 Apr 2021 18:13

Tgt Ion:	225	Resp:	53771
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.9	51.5	77.3

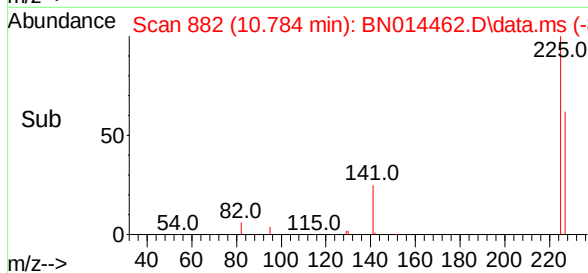




Abundance Scan 1059 (12.040 min): BN014459.D\data.ms (-1014) (-)




2-Methylnaphthalene-d10
Concen: 3.25 ng
RT: 12.040 min Scan# 1059
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Tgt Ion:152 Resp: 175922
Ion Ratio Lower Upper
152 100
151 20.0 16.2 24.4


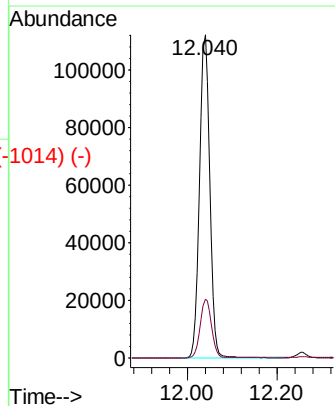
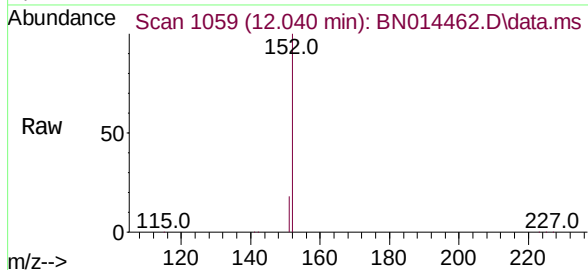


Abundance Scan 1076 (12.115 min): BN014459.D\data.ms (-1014) (-)



2-Methylnaphthalene
Concen: 3.23 ng
RT: 12.111 min Scan# 1075
Delta R.T. -0.005 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13


Tgt Ion:142 Resp: 188661
Ion Ratio Lower Upper
142 100
141 88.1 69.6 104.4
115 33.9 27.0 40.6

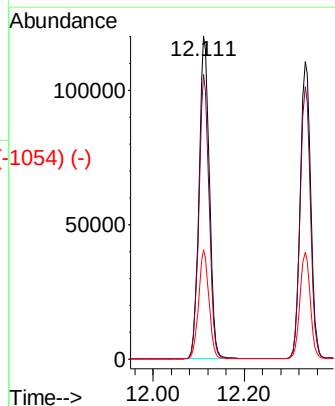



Abundance Scan 1306 (14.308 min): BN014459.D\data.ms (-1290) (-)

Acenaphthene-d10
Concen: 0.40 ng
RT: 14.308 min Scan# 1306
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13


Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

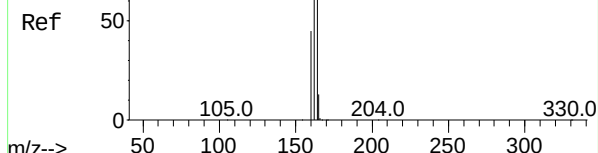

Tgt Ion:	164	Resp:	19073
Ion Ratio	Lower	Upper	
164	100		
162	98.5	78.3	117.5
160	45.7	36.6	54.8

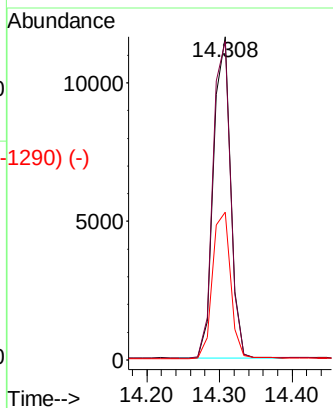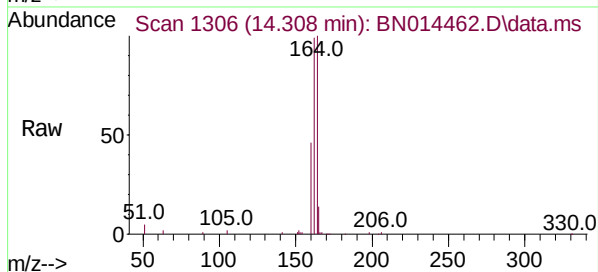



Abundance Scan 1306 (14.308 min): BN014462.D\data.ms (-1290) (-)

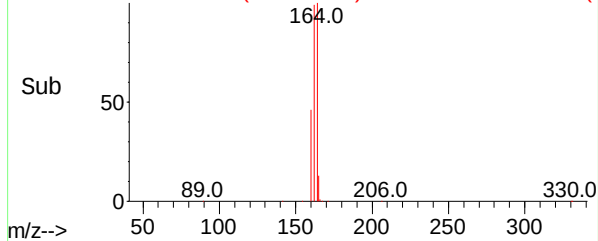


Abundance Scan 1423 (15.793 min): BN014459.D\data.ms (-1415) (-)

2,4,6-Tribromophenol
Concen: 3.90 ng
RT: 15.793 min Scan# 1423
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13


Tgt Ion:	330	Resp:	23885
Ion Ratio	Lower	Upper	
330	100		
332	0.0	0.0	0.0
141	33.8	29.3	43.9

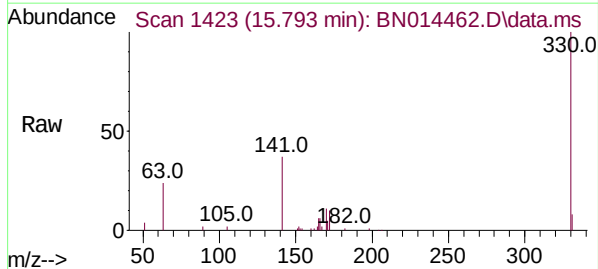

Abundance Scan 1423 (15.793 min): BN014462.D\data.ms (-1415) (-)

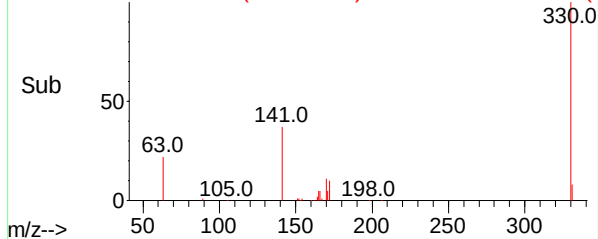



Abundance Scan 1197 (12.925 min): BN014459.D\data.ms (-1197) (-)

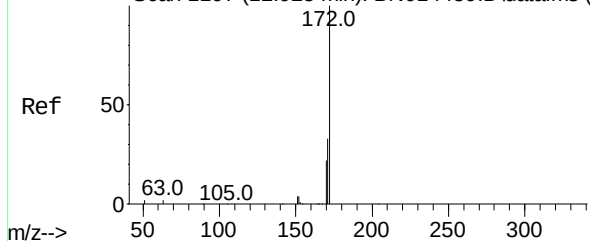


2-Fluorobiphenyl
Concen: 3.00 ng
RT: 12.925 min Scan# 1197
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:	172	Resp:	226344
Ion	Ratio	Lower	Upper
172	100		
171	33.7	27.0	40.4
170	22.3	18.2	27.4

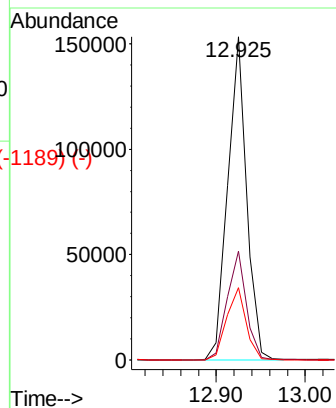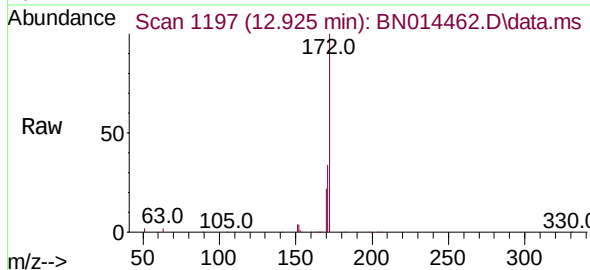

Abundance Scan 1197 (12.925 min): BN014462.D\data.ms (-1189) (-)


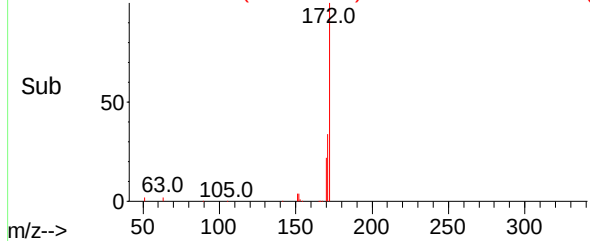


Abundance Scan 1283 (14.016 min): BN014459.D\data.ms (-1276) (-)

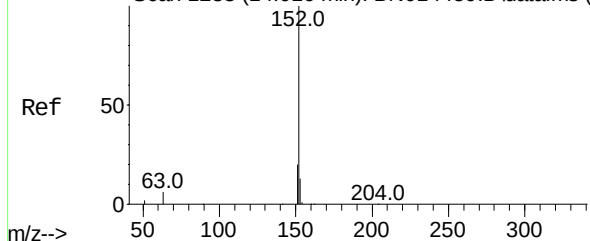


Acenaphthylene
Concen: 3.26 ng
RT: 14.016 min Scan# 1283
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

Tgt Ion:	152	Resp:	263616
Ion	Ratio	Lower	Upper
152	100		
151	19.3	15.4	23.2
153	13.1	10.4	15.6

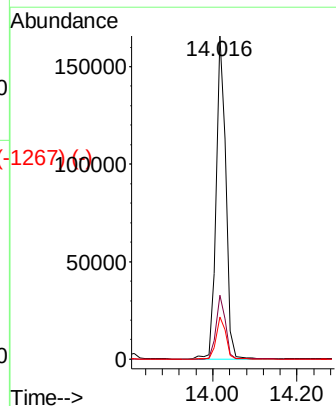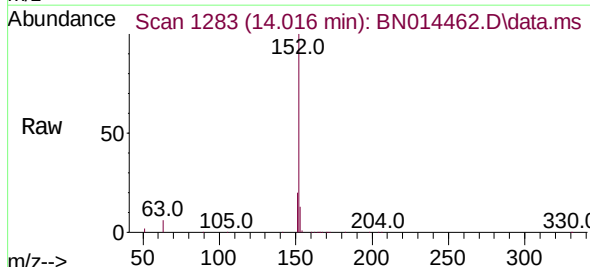


Abundance Scan 1283 (14.016 min): BN014462.D\data.ms (-1267) (-)

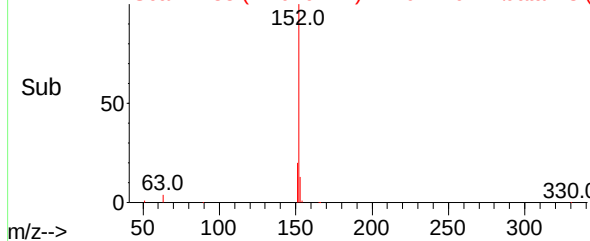




Abundance Scan 1311 (14.372 min): BN014459.D\data.ms (-1307) (-)

Acenaphthene
Concen: 3.27 ng
RT: 14.371 min Scan# 1311
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

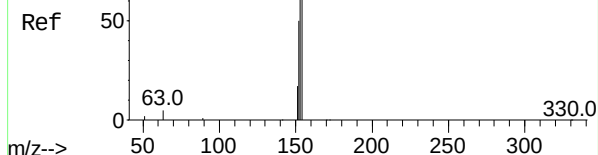


Tgt Ion:	154	Resp:	174644
Ion	Ratio	Lower	Upper
154	100		
153	109.6	90.5	135.7
152	55.3	47.2	70.8

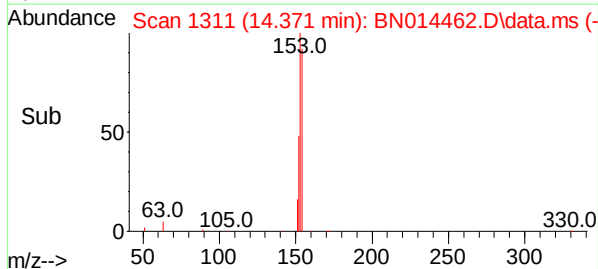

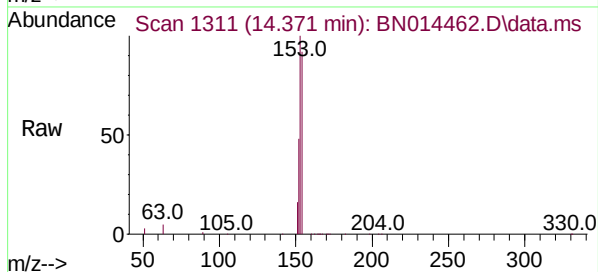



Abundance Scan 1389 (15.361 min): BN014459.D\data.ms (-1373) (-)

Fluorene
Concen: 3.31 ng
RT: 15.361 min Scan# 1389
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

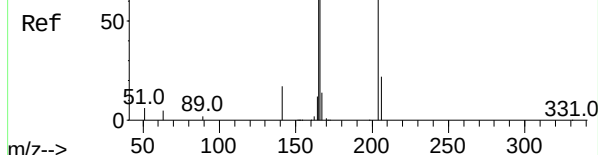

Tgt Ion:	166	Resp:	217874
Ion	Ratio	Lower	Upper
166	100		
165	97.1	78.1	117.1
167	13.5	11.0	16.6


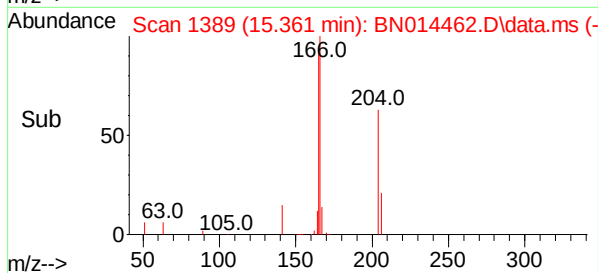

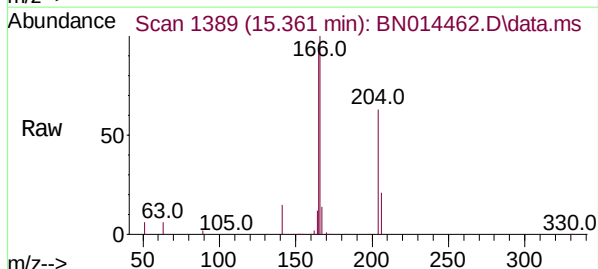


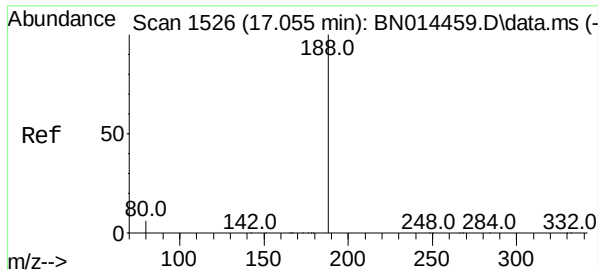

Phenanthrene-d10
Concen: 0.40 ng
RT: 17.055 min Scan# 1526
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Tgt Ion:	188	Resp:	38536
Ion Ratio	Lower	Upper	
188	100		
94	0.0	0.0	0.0
80	6.3	5.4	8.2

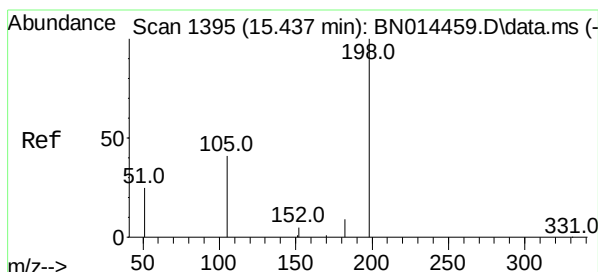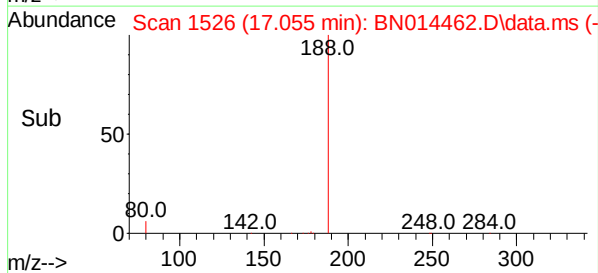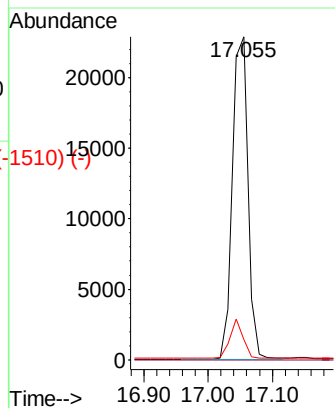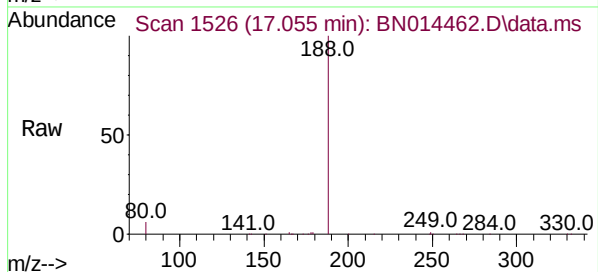

4,6-Dinitro-2-methylphenol
Concen: 3.78 ng
RT: 15.437 min Scan# 1395
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13


Tgt Ion:	198	Resp:	16268
Ion Ratio	Lower	Upper	
198	100		
51	21.0	104.5	156.7#
105	23.8	62.2	93.2#

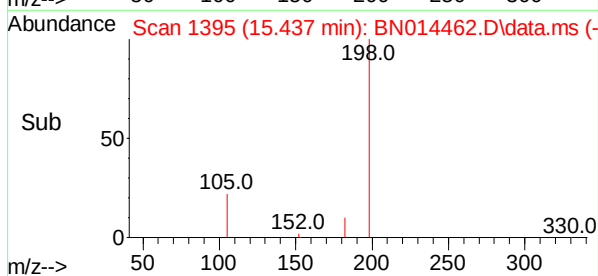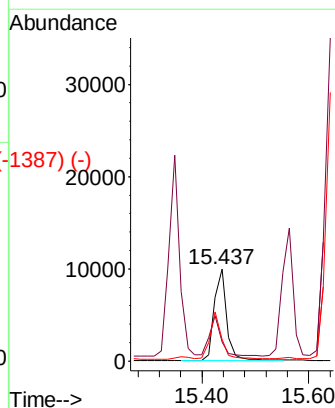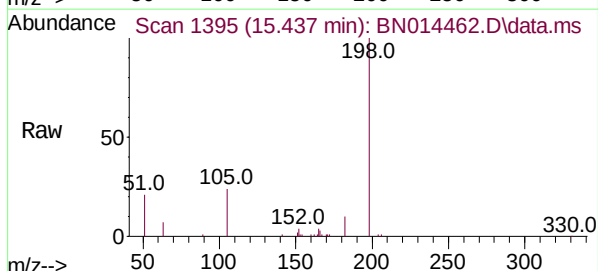




Abundance Scan 1460 (16.252 min): BN014459.D\data.ms (-1452) (-)

4-Bromophenyl-phenylether
Concen: 3.10 ng
RT: 16.252 min Scan# 1460
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

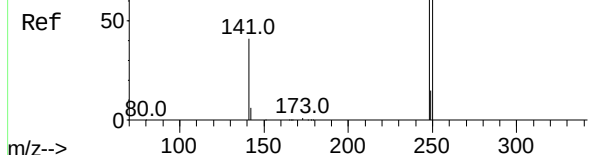




Tgt Ion:	248	Resp:	67344
Ion	Ratio	Lower	Upper
248	100		
250	103.6	81.8	122.6
141	36.0	34.2	51.2

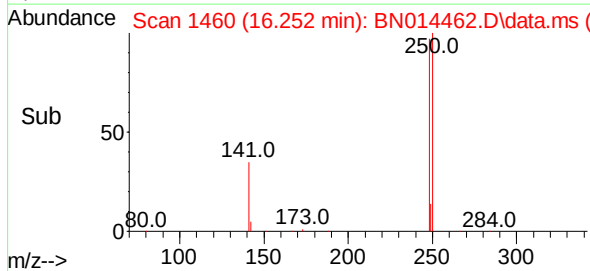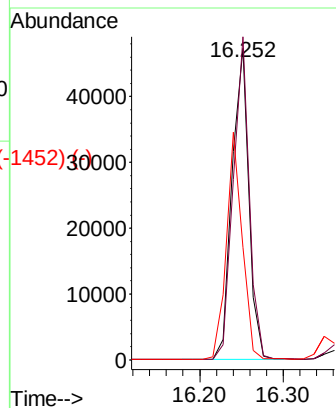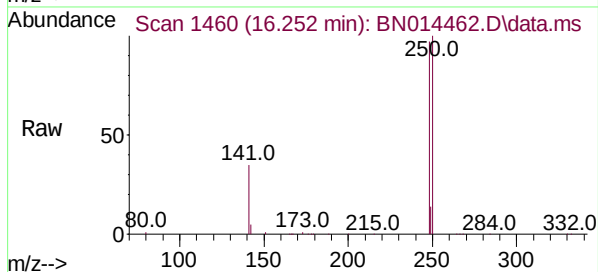

Abundance Scan 1469 (16.362 min): BN014459.D\data.ms (-1461) (-)

Hexachlorobenzene
Concen: 2.84 ng
RT: 16.362 min Scan# 1469
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13


Tgt Ion:	284	Resp:	84747
Ion	Ratio	Lower	Upper
284	100		
142	33.4	27.2	40.8
249	29.0	23.4	35.2

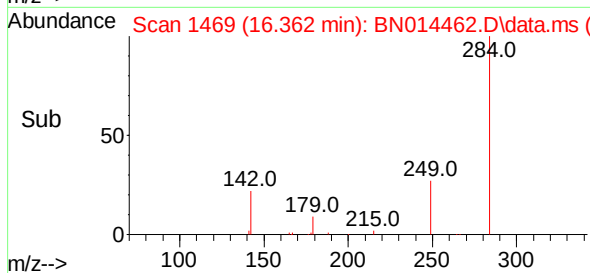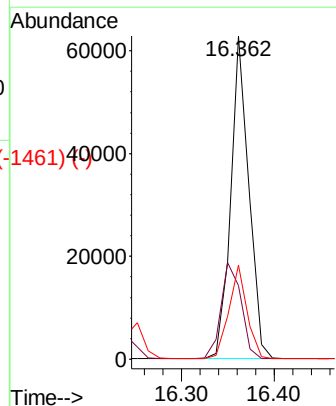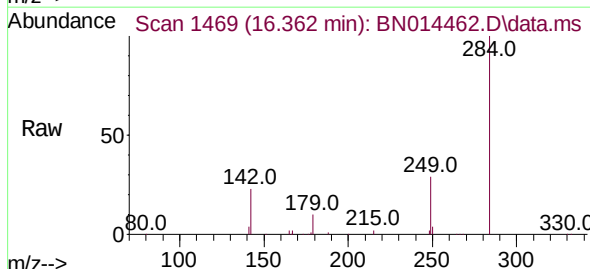




Abundance Scan 1482 (16.520 min): BN014459.D\data.ms (-1428) (-)

Atrazine
Concen: 3.68 ng
RT: 16.520 min Scan# 1482
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

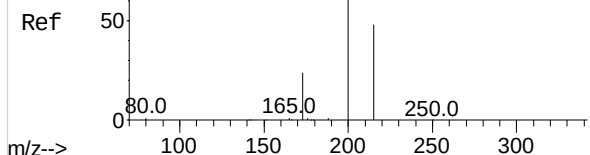


Tgt Ion	Ratio	Lower	Upper
200	100		
173	23.9	20.8	31.2
215	48.7	39.3	58.9

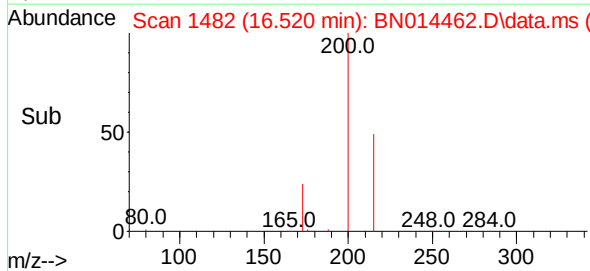
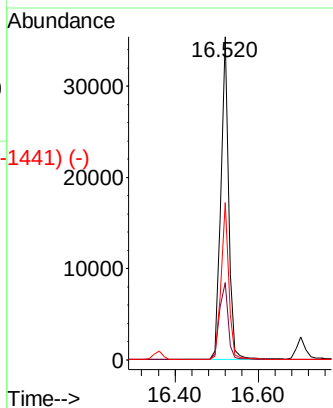
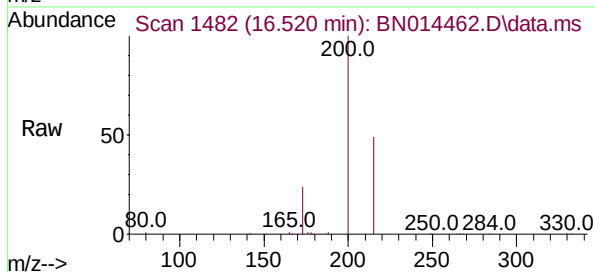


Abundance Scan 1498 (16.715 min): BN014459.D\data.ms (-1424) (-)


Pentachlorophenol
Concen: 3.95 ng
RT: 16.702 min Scan# 1497
Delta R.T. -0.012 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

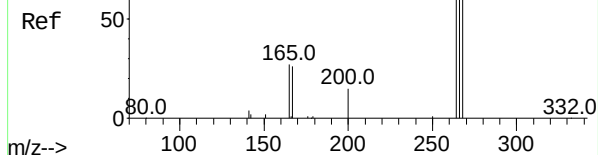

Tgt Ion	Ratio	Lower	Upper
266	100		
264	62.7	49.9	74.9
268	63.6	51.6	77.4

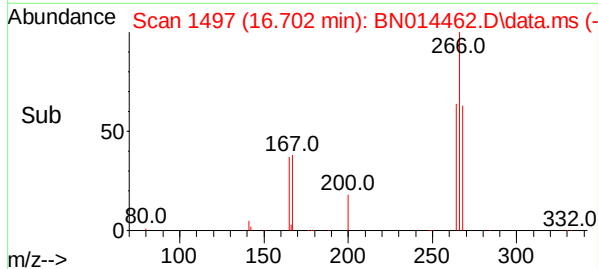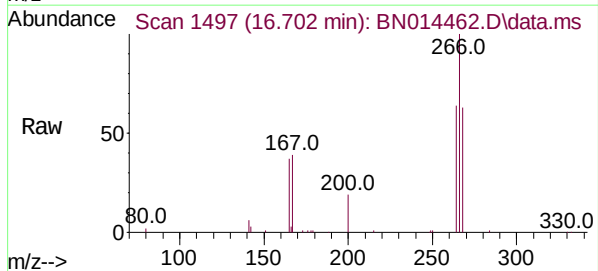




Abundance Scan 1529 (17.092 min): BN014459.D\data.ms (-1525) (-)




Phenanthrene
Concen: 3.24 ng
RT: 17.092 min Scan# 1529
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Tgt Ion:	178	Resp:	351071
Ion	Ratio	Lower	Upper
178	100		
176	18.9	15.1	22.7
179	15.3	12.2	18.4


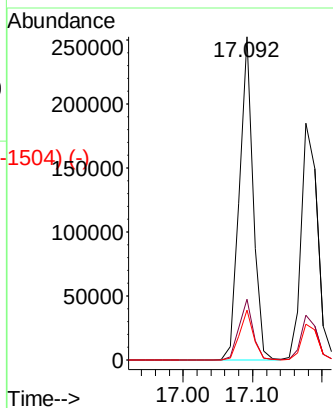
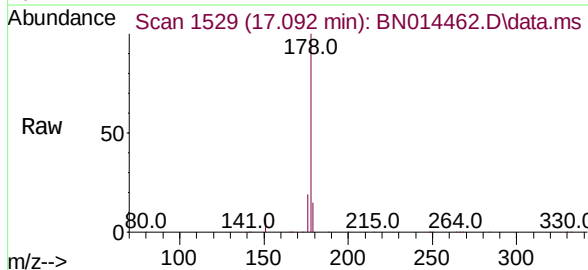


Abundance Scan 1536 (17.177 min): BN014459.D\data.ms (-1526) (-)




Anthracene
Concen: 3.54 ng
RT: 17.177 min Scan# 1536
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

Tgt Ion:	178	Resp:	300200
Ion	Ratio	Lower	Upper
178	100		
176	18.4	14.6	22.0
179	15.3	12.0	18.0






Abundance Scan 1821 (19.089 min): BN014459.D\data.ms (-1821) (-)

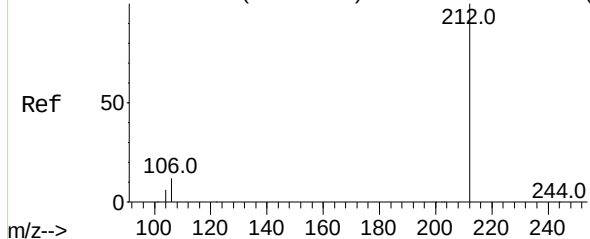


Fluoranthene-d10
Concen: 3.47 ng
RT: 19.089 min Scan# 1821
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Tgt Ion:212 Resp: 354511
Ion Ratio Lower Upper
212 100
106 12.7 10.2 15.4
104 7.0 5.6 8.4

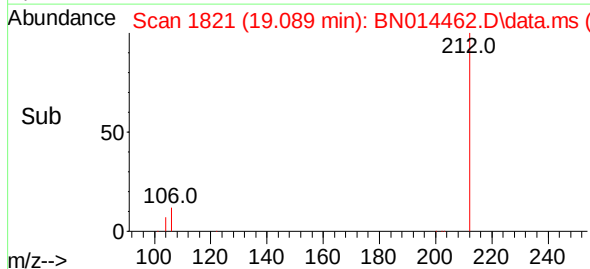
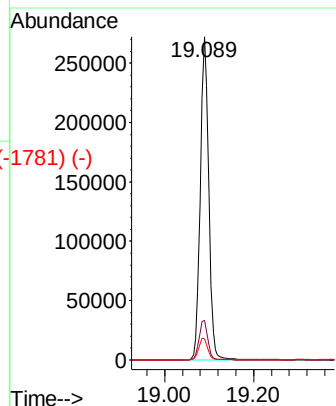
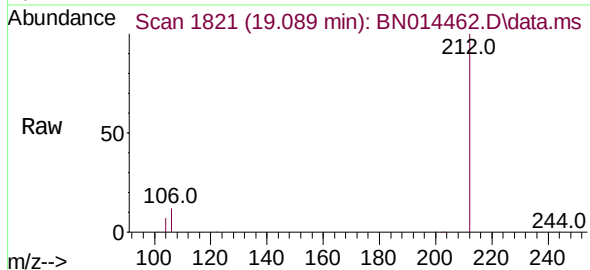


Abundance Scan 1827 (19.119 min): BN014459.D\data.ms (-1827) (-)

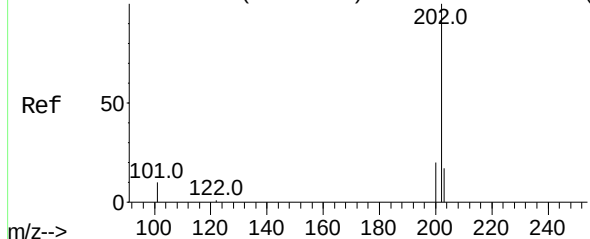


Fluoranthene
Concen: 3.46 ng
RT: 19.119 min Scan# 1827
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

Tgt Ion:202 Resp: 400101
Ion Ratio Lower Upper
202 100
101 10.7 8.5 12.7
203 17.4 13.7 20.5

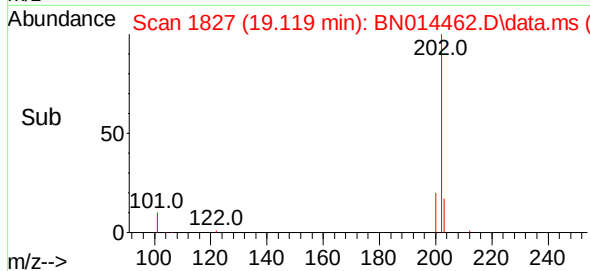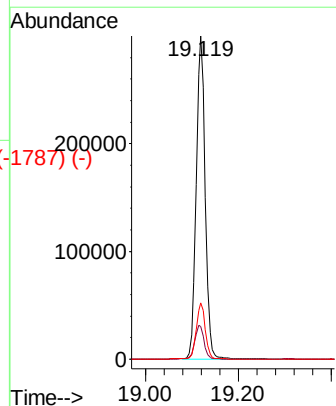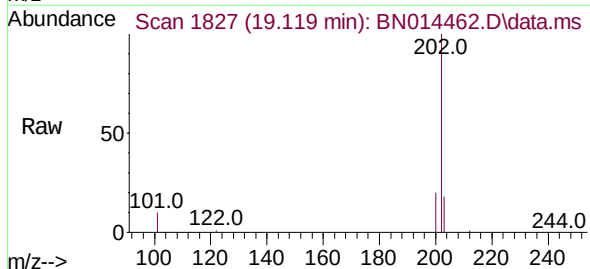




Abundance Scan 2123 (21.250 min): BN014459.D\data.ms (-2123) (-)

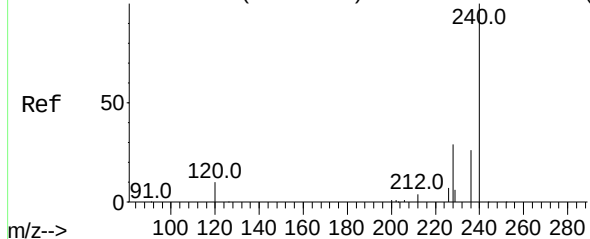


Chrysene-d12
Concen: 0.40 ng
RT: 21.250 min Scan# 2123
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Tgt Ion:	240	Resp:	41905
Ion	Ratio	Lower	Upper
240	100		
120	9.5	9.0	13.6
236	26.4	21.4	32.0

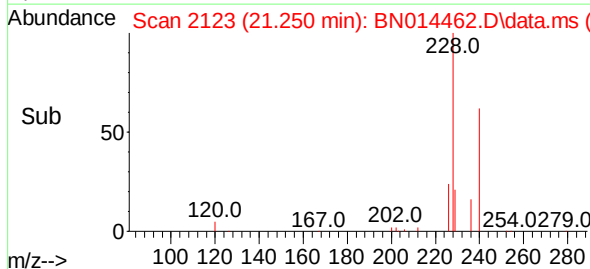
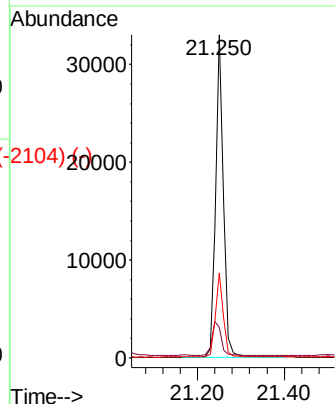
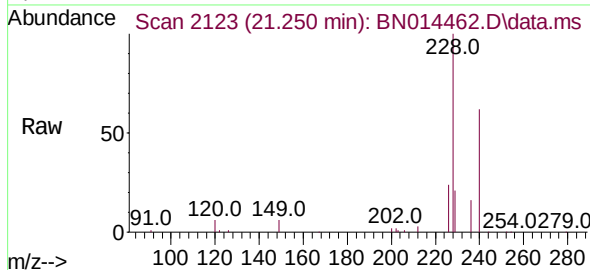


Abundance Scan 1901 (19.486 min): BN014459.D\data.ms (-1901) (-)

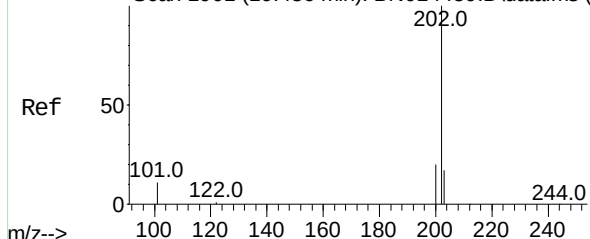

Pyrene
Concen: 3.16 ng
RT: 19.481 min Scan# 1900
Delta R.T. -0.005 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13


Tgt Ion:	202	Resp:	394427
Ion	Ratio	Lower	Upper
202	100		
200	20.5	16.4	24.6
203	17.4	13.9	20.9

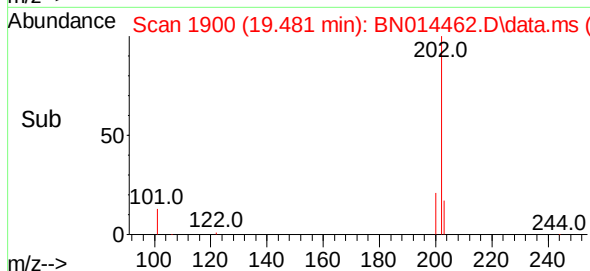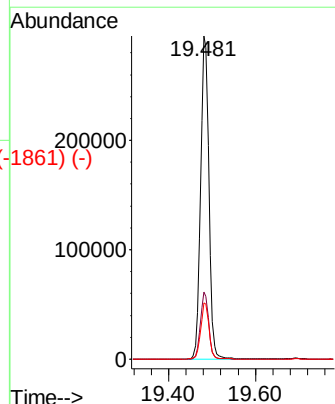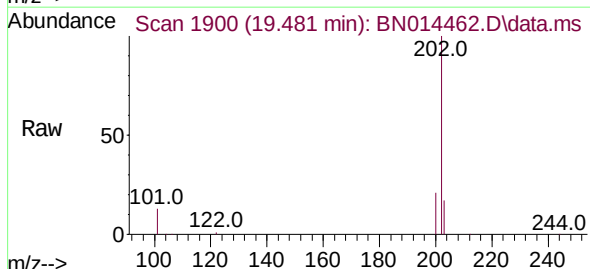



Abundance Scan 1943 (19.695 min): BN014459.D\data.ms (-1932) (-)

Terphenyl-d14
Concen: 3.04 ng
RT: 19.695 min Scan# 1943
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13


Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

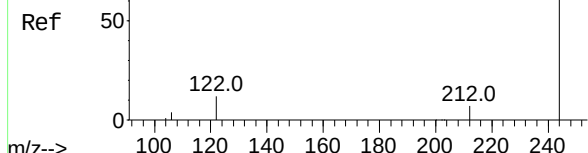

Tgt Ion	Ratio	Lower	Upper
244	100		
212	7.4	6.2	9.2
122	11.5	9.8	14.8

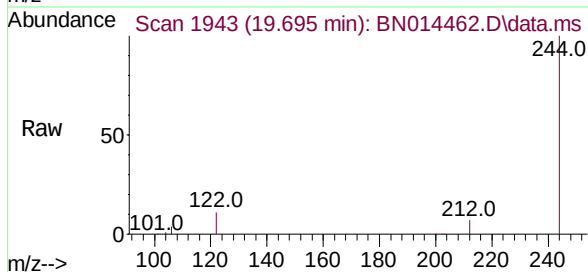



Abundance Scan 1943 (19.695 min): BN014462.D\data.ms (-1913) (-)




Abundance Scan 2122 (21.239 min): BN014459.D\data.ms (-2132) (-)

Benzo(a)anthracene
Concen: 3.51 ng
RT: 21.239 min Scan# 2122
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13


Tgt Ion	Ratio	Lower	Upper
228	100		
226	25.6	20.8	31.2
229	20.1	16.1	24.1

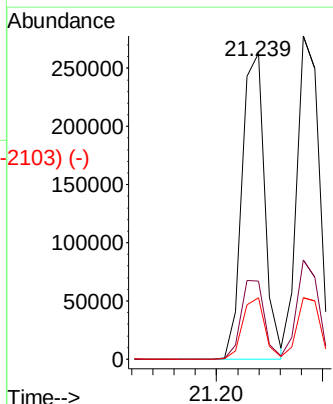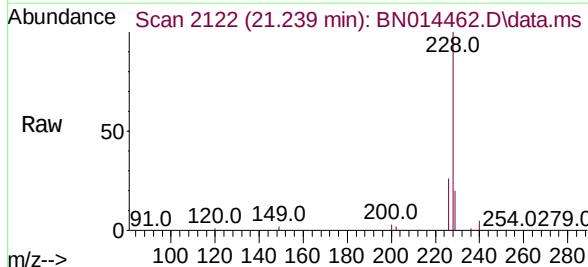

Abundance Scan 2122 (21.239 min): BN014462.D\data.ms (-2103) (-)






Abundance Scan 2126 (21.282 min): BN014459.D\data.ms (-2126) (-)

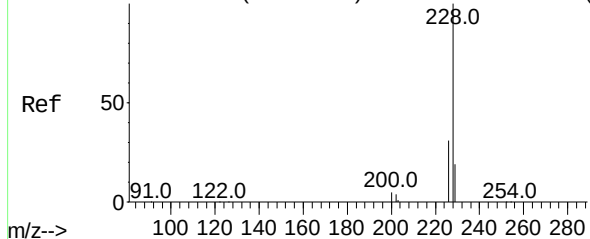


Chrysene
Concen: 3.08 ng
RT: 21.282 min Scan# 2126
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Tgt Ion:	228	Resp:	402427
Ion	Ratio	Lower	Upper
228	100		
226	30.7	24.8	37.2
229	19.0	15.3	22.9

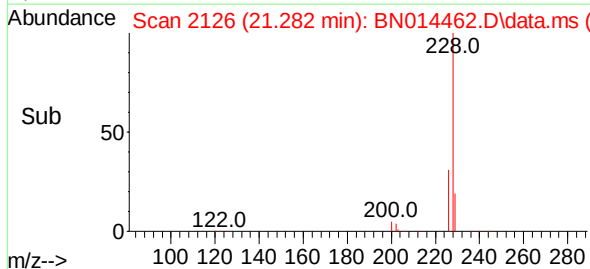
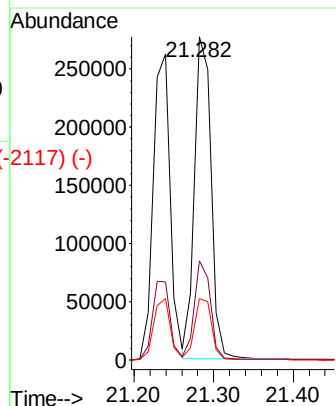
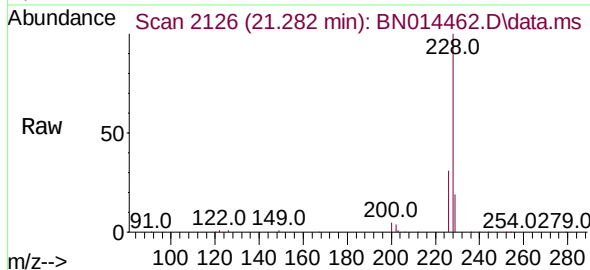


Abundance Scan 2116 (21.176 min): BN014459.D\data.ms (-2116) (-)

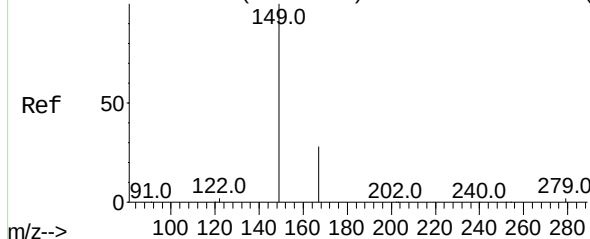

Bis(2-ethylhexyl)phthalate
Concen: 3.87 ng
RT: 21.176 min Scan# 2116
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13


Tgt Ion:	149	Resp:	151848
Ion	Ratio	Lower	Upper
149	100		
167	27.1	19.4	29.2
279	3.6	2.9	4.3

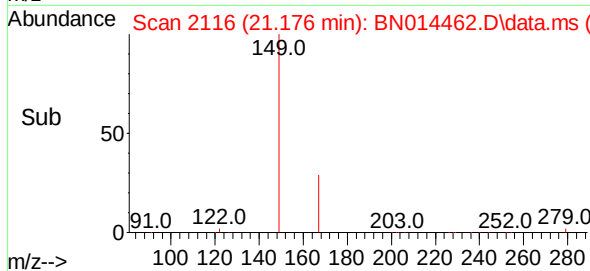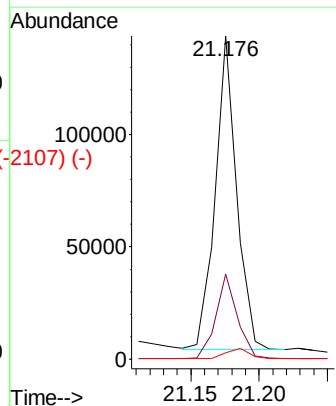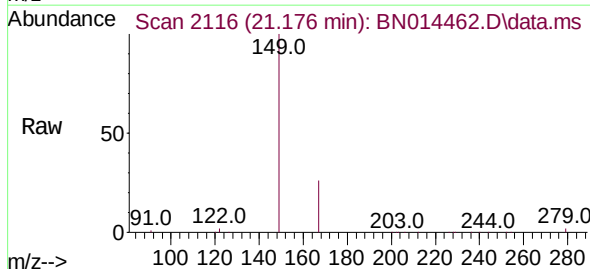




Abundance Scan 2543 (23.472 min): BN014459.D\data.ms (-2525) (-)

Perylene-d12
Concen: 0.40 ng
RT: 23.469 min Scan# 2542
Delta R.T. -0.004 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

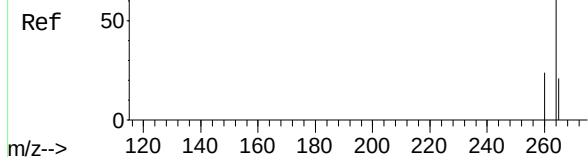





Tgt Ion:	264	Resp:	33078
Ion	Ratio	Lower	Upper
264	100		
260	24.9	19.8	29.6
265	36.3	31.6	47.4

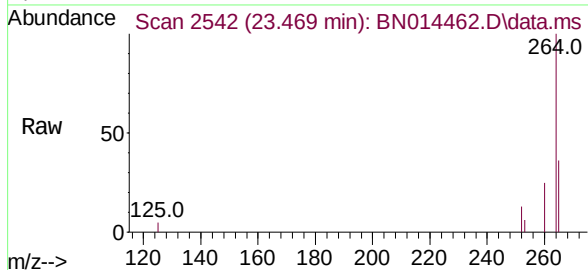


Abundance Scan 3193 (25.697 min): BN014459.D\data.ms (-3180) (-)

Indeno(1,2,3-cd)pyrene
Concen: 3.15 ng
RT: 25.693 min Scan# 3192
Delta R.T. -0.004 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

Tgt Ion:	276	Resp:	434407
Ion	Ratio	Lower	Upper
276	100		
138	25.2	18.5	27.7
277	24.9	19.9	29.9

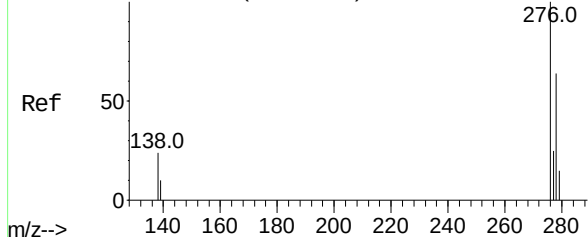




Abundance Scan 2349 (22.808 min): BN014459.D\data.ms (-2349) (-)




Benzo(b)fluoranthene
Concen: 3.18 ng
RT: 22.805 min Scan# 2348
Delta R.T. -0.004 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Tgt Ion:252 Resp: 387035
Ion Ratio Lower Upper
252 100
253 21.9 19.3 28.9
125 10.4 12.8 19.2#


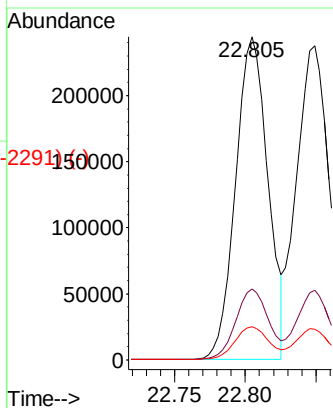
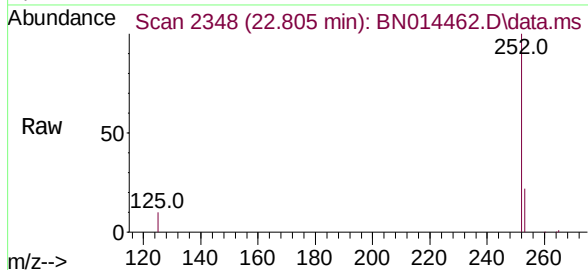


Abundance Scan 2361 (22.849 min): BN014459.D\data.ms (-2338) (-)




Benzo(k)fluoranthene
Concen: 3.13 ng
RT: 22.805 min Scan# 2348
Delta R.T. -0.045 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

Tgt Ion:252 Resp: 387035
Ion Ratio Lower Upper
252 100
253 21.9 19.3 28.9
125 10.4 10.0 15.0





Abundance Scan 2515 (23.376 min): BN014459.D\data.ms (-2457) (-)

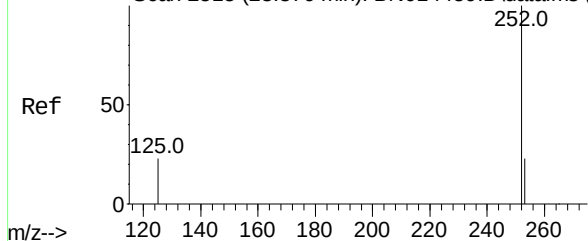


Benzo(a)pyrene
Concen: 3.45 ng
RT: 23.373 min Scan# 2514
Delta R.T. -0.004 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:252 Resp: 355983
Ion Ratio Lower Upper
252 100
253 22.3 21.0 31.6
125 12.5 20.8 31.2#

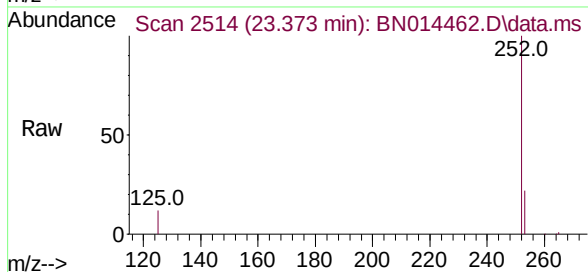

Abundance Scan 2514 (23.373 min): BN014462.D\data.ms (-2457) (-)





Abundance Scan 3197 (25.711 min): BN014459.D\data.ms (-3174) (-)

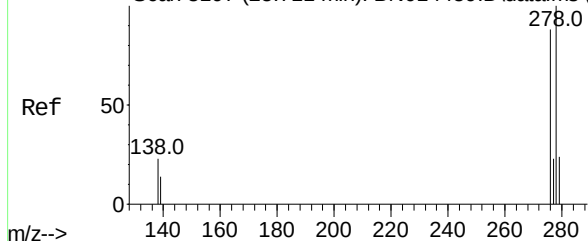


Dibenzo(a,h)anthracene
Concen: 3.17 ng
RT: 25.707 min Scan# 3196
Delta R.T. -0.004 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13


Tgt Ion:278 Resp: 363056
Ion Ratio Lower Upper
278 100
139 16.5 14.3 21.5
279 23.3 20.3 30.5



Abundance Scan 3196 (25.707 min): BN014462.D\data.ms (-3174) (-)

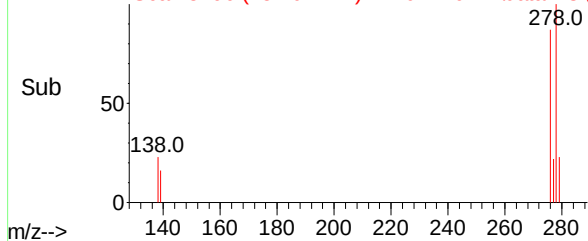


Abundance Scan 3391 (26.375 min): BN014459.D\data.ms (-3333) (-)



Benzo(g,h,i)perylene
Concen: 3.06 ng
RT: 26.371 min Scan# 3390
Delta R.T. -0.004 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Abundance Scan 3390 (26.371 min): BN014462.D\data.ms

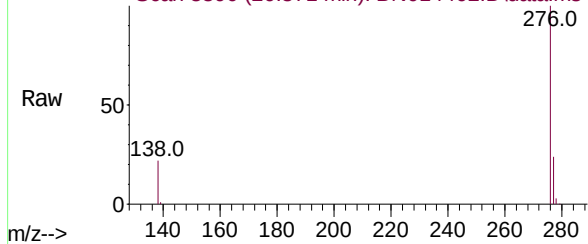

Tgt Ion:276 Resp: 370179
Ion Ratio Lower Upper
276 100
277 23.7 19.5 29.3
138 21.8 18.3 27.5

Abundance Scan 3390 (26.371 min): BN014462.D\data.ms (-3333) (-)

