

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042821\
 Data File : BN014463.D
 Acq On : 27 Apr 2021 18:49
 Operator : CG/JU
 Sample : SSTDICC5.0
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Quant Time: Apr 27 19:17:53 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 27 18:52:25 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.668	152	9773	0.40	ng	0.00
7) Naphthalene-d8	10.441	136	33124	0.40	ng	0.00
13) Acenaphthene-d10	14.308	164	17936	0.40	ng	0.00
19) Phenanthrene-d10	17.043	188	36669	0.40	ng	#-0.01
29) Chrysene-d12	21.250	240	40595	0.40	ng	0.00
35) Perylene-d12	23.469	264	31460	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.276	112	89352	4.45	ng	0.00
5) Phenol-d6	6.839	99	120222	4.88	ng	0.00
8) Nitrobenzene-d5	8.807	82	118297	4.26	ng	-0.01
11) 2-Methylnaphthalene-d10	12.040	152	250081	5.02	ng	0.00
14) 2,4,6-Tribromophenol	15.793	330	37674	6.54	ng	0.00
15) 2-Fluorobiphenyl	12.925	172	322355	4.55	ng	0.00
27) Fluoranthene-d10	19.089	212	521967	5.37	ng	0.00
31) Terphenyl-d14	19.695	244	396278	4.60	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.231	88	47205	3.96	ng	97
3) n-Nitrosodimethylamine	3.545	42	29783	4.79	ng	# 99
6) bis(2-Chloroethyl)ether	7.104	93	106627	4.41	ng	99
9) Naphthalene	10.492	128	396607	4.82	ng	99
10) Hexachlorobutadiene	10.784	225	74901	4.16	ng	# 99
12) 2-Methylnaphthalene	12.111	142	265619	4.95	ng	99
16) Acenaphthylene	14.016	152	391684	5.15	ng	100
17) Acenaphthene	14.359	154	254376	5.06	ng	95
18) Fluorene	15.348	166	314239	5.07	ng	100
20) 4,6-Dinitro-2-methylph...	15.437	198	26925	6.58	ng	# 15
21) 4-Bromophenyl-phenylether	16.252	248	97916	4.74	ng	# 95
22) Hexachlorobenzene	16.362	284	121855	4.29	ng	99
23) Atrazine	16.520	200	71654	6.00	ng	98
24) Pentachlorophenol	16.702	266	34823	6.64	ng	99
25) Phenanthrene	17.092	178	506302	4.92	ng	100
26) Anthracene	17.177	178	447277	5.54	ng	100
28) Fluoranthene	19.119	202	578854	5.27	ng	99
30) Pyrene	19.481	202	585567	4.84	ng	100
32) Benzo(a)anthracene	21.239	228	580641	5.41	ng	99
33) Chrysene	21.282	228	580526	4.59	ng	100
34) Bis(2-ethylhexyl)phtha...	21.176	149	239595	6.31	ng	95
36) Indeno(1,2,3-cd)pyrene	25.693	276	639032	4.87	ng	98
37) Benzo(b)fluoranthene	22.805	252	573437	4.95	ng	# 92
38) Benzo(k)fluoranthene	22.805	252	573437	4.87	ng	95
39) Benzo(a)pyrene	23.373	252	523492	5.34	ng	# 82
40) Dibenzo(a,h)anthracene	25.707	278	534227	4.91	ng	97
41) Benzo(g,h,i)perylene	26.375	276	547016	4.75	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042821\
Data File : BN014463.D
Acq On : 27 Apr 2021 18:49
Operator : CG/JU
Sample : SSTDIC5.0
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Quant Time: Apr 27 19:17:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 27 18:52:25 2021
Response via : Initial Calibration









1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.668 min Scan# 607
Delta R.T. -0.008 min
Lab File: BN014463.D
Acq: 27 Apr 2021 18:49




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:152 Resp: 9773
Ion Ratio Lower Upper
152 100
150 159.3 121.2 181.8
115 59.9 46.0 69.0



1,4-Dioxane
Concen: 3.96 ng
RT: 3.231 min Scan# 56
Delta R.T. -0.000 min
Lab File: BN014463.D
Acq: 27 Apr 2021 18:49

Tgt Ion: 88 Resp: 47205
Ion Ratio Lower Upper
88 100
58 63.7 53.1 79.7
43 23.4 20.3 30.5









n-Nitrosodimethylamine
Concen: 4.79 ng
RT: 3.545 min Scan# 95
Delta R.T. -0.048 min
Lab File: BN014463.D
Acq: 27 Apr 2021 18:49




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion: 42 Resp: 29783
Ion Ratio Lower Upper
42 100
74 154.8 124.7 187.1
44 9.2 0.0 0.0#



2-Fluorophenol
Concen: 4.45 ng
RT: 5.276 min Scan# 310
Delta R.T. -0.000 min
Lab File: BN014463.D
Acq: 27 Apr 2021 18:49

Tgt Ion: 112 Resp: 89352
Ion Ratio Lower Upper
112 100
64 51.9 41.4 62.2
63 27.0 21.8 32.8









Phenol-d6
 Concen: 4.88 ng
 RT: 6.839 min Scan# 504
 Delta R.T. -0.000 min
 Lab File: BN014463.D
 Acq: 27 Apr 2021 18:49




Instrument :
 BNA_N
 ClientSampled :
 SSTDICC5.0

Tgt Ion:	99	Resp:	120222
Ion	Ratio	Lower	Upper
99	100		
42	16.7	13.8	20.6
71	31.8	25.5	38.3



bis(2-Chloroethyl)ether
 Concen: 4.41 ng
 RT: 7.104 min Scan# 537
 Delta R.T. -0.000 min
 Lab File: BN014463.D
 Acq: 27 Apr 2021 18:49


Tgt Ion:	93	Resp:	106627
Ion	Ratio	Lower	Upper
93	100		
63	71.5	56.7	85.1
95	33.4	26.3	39.5






Abundance Scan 855 (10.442 min): BN014459.D\data.ms (-8507-)

Naphthalene-d8
Concen: 0.40 ng
RT: 10.441 min Scan# 855
Delta R.T. -0.000 min
Lab File: BN014463.D
Acq: 27 Apr 2021 18:49

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

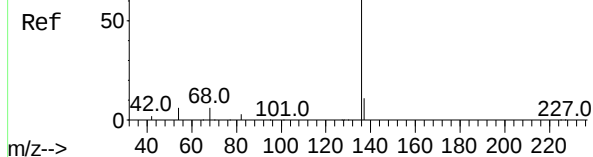




Tgt Ion:	136	Resp:	33124
Ion	Ratio	Lower	Upper
136	100		
137	11.2	9.0	13.4
54	6.3	5.7	8.5
68	5.8	5.2	7.8




Abundance Scan 727 (8.819 min): BN014459.D\data.ms (-723#8)

Nitrobenzene-d5
Concen: 4.26 ng
RT: 8.807 min Scan# 726
Delta R.T. -0.013 min
Lab File: BN014463.D
Acq: 27 Apr 2021 18:49

Tgt Ion:	82	Resp:	118297
Ion	Ratio	Lower	Upper
82	100		
128	35.8	38.5	57.7#
54	45.7	32.1	48.1









Scan 859 (10.492 min): BN014459.D\data.ms (-854) (-)
 Naphthalene
 Concen: 4.82 ng
 RT: 10.492 min Scan# 859
 Delta R.T. -0.000 min
 Lab File: BN014463.D
 Acq: 27 Apr 2021 18:49




Instrument :
 BNA_N
 ClientSampled :
 SSTDICC5.0

Tgt Ion:	128	Resp:	396607
Ion	Ratio	Lower	Upper
128	100		
129	10.9	9.0	13.4
127	12.7	10.5	15.7



Scan 882 (10.784 min): BN014459.D\data.ms (-876) (-)
 Hexachlorobutadiene
 Concen: 4.16 ng
 RT: 10.784 min Scan# 882
 Delta R.T. -0.000 min
 Lab File: BN014463.D
 Acq: 27 Apr 2021 18:49


Tgt Ion:	225	Resp:	74901
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.7	51.5	77.3






Abundance Scan 1059 (12.040 min): BN014459.D\data.ms (-1045) (-)

2-Methylnaphthalene-d10
Concen: 5.02 ng
RT: 12.040 min Scan# 1059
Delta R.T. -0.000 min
Lab File: BN014463.D
Acq: 27 Apr 2021 18:49

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0




Tgt Ion:152 Resp: 250081
Ion Ratio Lower Upper
152 100
151 20.0 16.2 24.4






Abundance Scan 1076 (12.115 min): BN014459.D\data.ms (-1045) (-)

2-Methylnaphthalene
Concen: 4.95 ng
RT: 12.111 min Scan# 1075
Delta R.T. -0.005 min
Lab File: BN014463.D
Acq: 27 Apr 2021 18:49




Tgt Ion:142 Resp: 265619
Ion Ratio Lower Upper
142 100
141 88.3 69.6 104.4
115 34.1 27.0 40.6






Abundance Scan 1306 (14.308 min): BN014459.D\data.ms (-1290) (-)

Acenaphthene-d10
Concen: 0.40 ng
RT: 14.308 min Scan# 1306
Delta R.T. -0.000 min
Lab File: BN014463.D
Acq: 27 Apr 2021 18:49

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

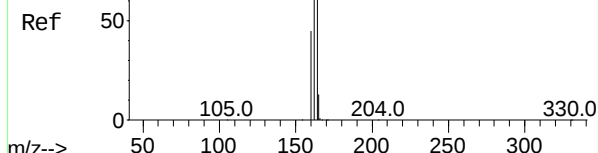





Tgt Ion:	164	Resp:	17936
Ion Ratio	Lower	Upper	
164	100		
162	98.9	78.3	117.5
160	45.8	36.6	54.8




Abundance Scan 1423 (15.793 min): BN014459.D\data.ms (-1415) (-)

2,4,6-Tribromophenol
Concen: 6.54 ng
RT: 15.793 min Scan# 1423
Delta R.T. -0.000 min
Lab File: BN014463.D
Acq: 27 Apr 2021 18:49

Tgt Ion:	330	Resp:	37674
Ion Ratio	Lower	Upper	
330	100		
332	0.0	0.0	0.0
141	34.1	29.3	43.9

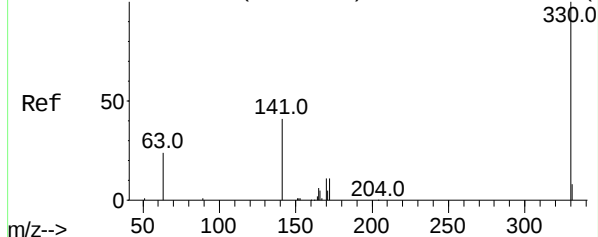



Abundance Scan 1197 (12.925 min): BN014459.D\data.ms (-1189) (-)

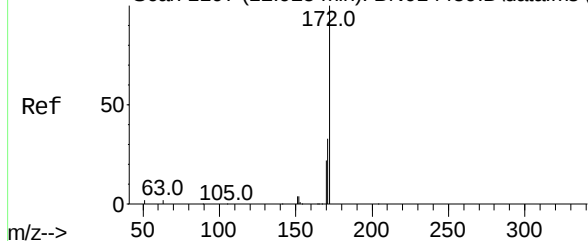


2-Fluorobiphenyl
Concen: 4.55 ng
RT: 12.925 min Scan# 1197
Delta R.T. -0.000 min
Lab File: BN014463.D
Acq: 27 Apr 2021 18:49

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:	172	Resp:	322355
Ion	Ratio	Lower	Upper
172	100		
171	33.4	27.0	40.4
170	22.1	18.2	27.4



Abundance Scan 1197 (12.925 min): BN014463.D\data.ms (-1189) (-)





Abundance Scan 1283 (14.016 min): BN014459.D\data.ms (-1267) (-)

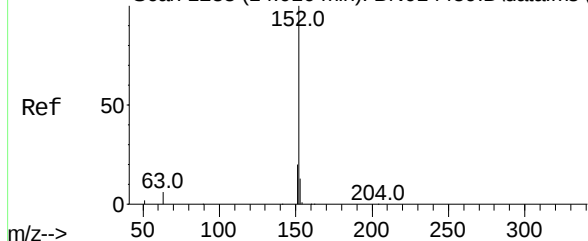


Acenaphthylene
Concen: 5.15 ng
RT: 14.016 min Scan# 1283
Delta R.T. -0.000 min
Lab File: BN014463.D
Acq: 27 Apr 2021 18:49

Tgt Ion:	152	Resp:	391684
Ion	Ratio	Lower	Upper
152	100		
151	19.1	15.4	23.2
153	13.0	10.4	15.6




Abundance Scan 1283 (14.016 min): BN014463.D\data.ms (-1267) (-)






Abundance Scan 1311 (14.372 min): BN014459.D\data.ms (-1307) (-)

Acenaphthene
Concen: 5.06 ng
RT: 14.359 min Scan# 1310
Delta R.T. -0.013 min
Lab File: BN014463.D
Acq: 27 Apr 2021 18:49

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

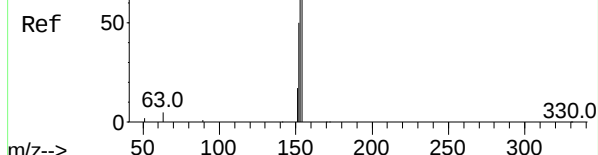


Tgt Ion:	154	Resp:	254376
Ion Ratio	Lower	Upper	
154	100		
153	108.7	90.5	135.7
152	54.3	47.2	70.8







Abundance Scan 1389 (15.361 min): BN014459.D\data.ms (-1373) (-)

Fluorene
Concen: 5.07 ng
RT: 15.348 min Scan# 1388
Delta R.T. -0.013 min
Lab File: BN014463.D
Acq: 27 Apr 2021 18:49

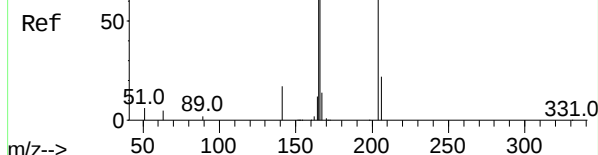

Tgt Ion:	166	Resp:	314239
Ion Ratio	Lower	Upper	
166	100		
165	97.5	78.1	117.1
167	13.4	11.0	16.6







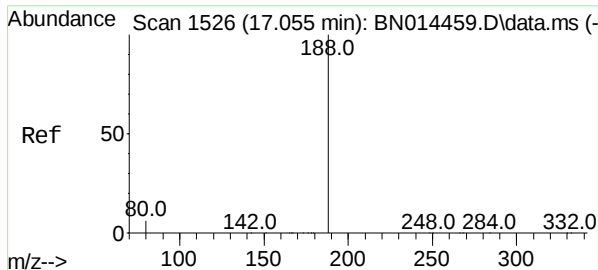

Phenanthrene-d10
Concen: 0.40 ng
RT: 17.043 min Scan# 1525
Delta R.T. -0.012 min
Lab File: BN014463.D
Acq: 27 Apr 2021 18:49




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:	188	Resp:	36669
Ion Ratio	Lower	Upper	
188	100		
94	0.0	0.0	0.0
80	12.9	5.4	8.2#




4,6-Dinitro-2-methylphenol
Concen: 6.58 ng
RT: 15.437 min Scan# 1395
Delta R.T. -0.000 min
Lab File: BN014463.D
Acq: 27 Apr 2021 18:49

Tgt Ion:	198	Resp:	26925
Ion Ratio	Lower	Upper	
198	100		
51	17.8	104.5	156.7#
105	21.8	62.2	93.2#






Abundance Scan 1460 (16.252 min): BN014459.D\data.ms (-1452) (-)




4-Bromophenyl-phenylether
Concen: 4.74 ng
RT: 16.252 min Scan# 1460
Delta R.T. -0.000 min
Lab File: BN014463.D
Acq: 27 Apr 2021 18:49

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:	248	Resp:	97916
Ion	Ratio	Lower	Upper
248	100		
250	103.5	81.8	122.6
141	33.6	34.2	51.2#






Abundance Scan 1469 (16.362 min): BN014459.D\data.ms (-1461) (-)



Hexachlorobenzene
Concen: 4.29 ng
RT: 16.362 min Scan# 1469
Delta R.T. -0.000 min
Lab File: BN014463.D
Acq: 27 Apr 2021 18:49


Tgt Ion:	284	Resp:	121855
Ion	Ratio	Lower	Upper
284	100		
142	33.2	27.2	40.8
249	28.9	23.4	35.2





Abundance Scan 1482 (16.520 min): BN014459.D\data.ms (-1428) (-)

Atrazine
Concen: 6.00 ng
RT: 16.520 min Scan# 1482
Delta R.T. -0.000 min
Lab File: BN014463.D
Acq: 27 Apr 2021 18:49


Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

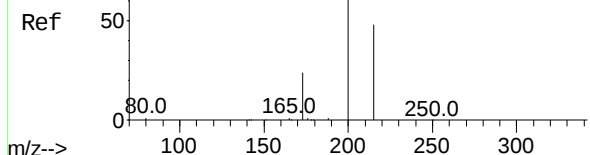

Tgt Ion:	200	Resp:	71654
Ion Ratio	Lower	Upper	
200	100		
173	23.5	20.8	31.2
215	49.0	39.3	58.9






Abundance Scan 1482 (16.520 min): BN014463.D\data.ms (-1441) (-)




Abundance Scan 1498 (16.715 min): BN014459.D\data.ms (-1424) (-)

Pentachlorophenol
Concen: 6.64 ng
RT: 16.702 min Scan# 1497
Delta R.T. -0.012 min
Lab File: BN014463.D
Acq: 27 Apr 2021 18:49


Tgt Ion:	266	Resp:	34823
Ion Ratio	Lower	Upper	
266	100		
264	62.7	49.9	74.9
268	63.5	51.6	77.4



Abundance Scan 1497 (16.702 min): BN014463.D\data.ms (-1490) (-)






Abundance Scan 1529 (17.092 min): BN014459.D\data.ms (-1525) (-)




Phenanthrene
Concen: 4.92 ng
RT: 17.092 min Scan# 1529
Delta R.T. -0.000 min
Lab File: BN014463.D
Acq: 27 Apr 2021 18:49

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:	178	Resp:	506302
Ion Ratio	Lower	Upper	
178	100		
176	18.9	15.1	22.7
179	15.3	12.2	18.4






Abundance Scan 1536 (17.177 min): BN014459.D\data.ms (-1528) (-)




Anthracene
Concen: 5.54 ng
RT: 17.177 min Scan# 1536
Delta R.T. -0.000 min
Lab File: BN014463.D
Acq: 27 Apr 2021 18:49

Tgt Ion:	178	Resp:	447277
Ion Ratio	Lower	Upper	
178	100		
176	18.3	14.6	22.0
179	15.4	12.0	18.0





Abundance Scan 1821 (19.089 min): BN014459.D\data.ms (-1821) (-)




Fluoranthene-d10
Concen: 5.37 ng
RT: 19.089 min Scan# 1821
Delta R.T. -0.000 min
Lab File: BN014463.D
Acq: 27 Apr 2021 18:49

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:	212	Resp:	521967
Ion Ratio	Lower	Upper	
212	100		
106	12.8	10.2	15.4
104	7.0	5.6	8.4



Abundance Scan 1821 (19.089 min): BN014463.D\data.ms (-1781) (-)





Abundance Scan 1827 (19.119 min): BN014459.D\data.ms (-1827) (-)




Fluoranthene
Concen: 5.27 ng
RT: 19.119 min Scan# 1827
Delta R.T. -0.000 min
Lab File: BN014463.D
Acq: 27 Apr 2021 18:49

Tgt Ion:	202	Resp:	578854
Ion Ratio	Lower	Upper	
202	100		
101	10.8	8.5	12.7
203	17.4	13.7	20.5



Abundance Scan 1827 (19.119 min): BN014463.D\data.ms (-1787) (-)



Abundance Scan 2123 (21.250 min): BN014459.D\data.ms (-129) (-)

Chrysene-d12

Concen: 0.40 ng

RT: 21.250 min Scan# 2123

Delta R.T. -0.000 min

Lab File: BN014463.D


Acq: 27 Apr 2021 18:49

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0






Tgt Ion:240 Resp: 40595

Ion Ratio Lower Upper

240 100

120 9.1 9.0 13.6

236 26.4 21.4 32.0



Abundance Scan 1901 (19.486 min): BN014459.D\data.ms (-186) (-)

Pyrene


Concen: 4.84 ng

RT: 19.481 min Scan# 1900

Delta R.T. -0.005 min

Lab File: BN014463.D

Acq: 27 Apr 2021 18:49






Tgt Ion:202 Resp: 585567

Ion Ratio Lower Upper

202 100

200 20.5 16.4 24.6


203 17.5 13.9 20.9






Abundance Scan 1943 (19.695 min): BN014459.D\data.ms (-1932) (-)

Terphenyl-d14
Concen: 4.60 ng
RT: 19.695 min Scan# 1943
Delta R.T. -0.000 min
Lab File: BN014463.D
Acq: 27 Apr 2021 18:49

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0




Tgt Ion	Ratio	Lower	Upper
244	100		
212	7.3	6.2	9.2
122	10.8	9.8	14.8






Abundance Scan 2122 (21.239 min): BN014459.D\data.ms (-2132) (-)


Benzo(a)anthracene
Concen: 5.41 ng
RT: 21.239 min Scan# 2122
Delta R.T. -0.000 min
Lab File: BN014463.D
Acq: 27 Apr 2021 18:49



Tgt Ion	Ratio	Lower	Upper
228	100		
226	25.5	20.8	31.2
229	20.3	16.1	24.1






Abundance Scan 2126 (21.282 min): BN014459.D\data.ms (-2126) (-)

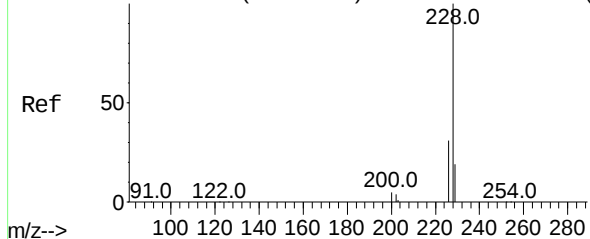


Chrysene
Concen: 4.59 ng
RT: 21.282 min Scan# 2126
Delta R.T. -0.000 min
Lab File: BN014463.D
Acq: 27 Apr 2021 18:49

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:	228	Resp:	580526
Ion	Ratio	Lower	Upper
228	100		
226	30.7	24.8	37.2
229	19.3	15.3	22.9






Abundance Scan 2116 (21.176 min): BN014459.D\data.ms (-2116) (-)

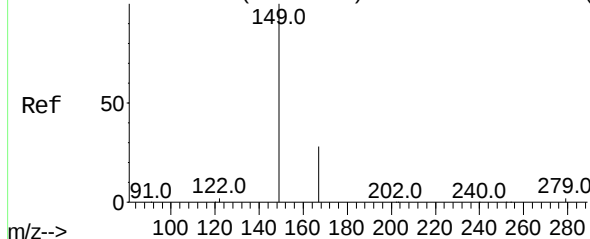

Bis(2-ethylhexyl)phthalate
Concen: 6.31 ng
RT: 21.176 min Scan# 2116
Delta R.T. -0.000 min
Lab File: BN014463.D
Acq: 27 Apr 2021 18:49


Tgt Ion:	149	Resp:	239595
Ion	Ratio	Lower	Upper
149	100		
167	27.3	19.4	29.2
279	3.6	2.9	4.3






Abundance Scan 2543 (23.472 min): BN014459.D\data.ms (-2525) (-)

Perylene-d12
Concen: 0.40 ng
RT: 23.469 min Scan# 2542
Delta R.T. -0.004 min
Lab File: BN014463.D
Acq: 27 Apr 2021 18:49

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

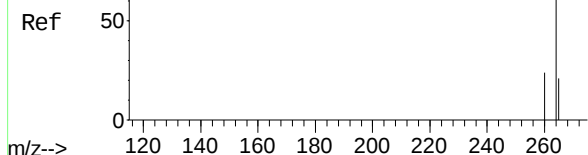


Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.8	19.8	29.6
265	36.4	31.6	47.4






Abundance Scan 3193 (25.697 min): BN014459.D\data.ms (-3130) (-)


Indeno(1,2,3-cd)pyrene
Concen: 4.87 ng
RT: 25.693 min Scan# 3192
Delta R.T. -0.004 min
Lab File: BN014463.D
Acq: 27 Apr 2021 18:49



Tgt Ion	Ratio	Lower	Upper
276	100		
138	25.2	18.5	27.7
277	24.9	19.9	29.9






Abundance Scan 2349 (22.808 min): BN014459.D\data.ms (-2349) (-)




Benzo(b)fluoranthene
Concen: 4.95 ng
RT: 22.805 min Scan# 2348
Delta R.T. -0.004 min
Lab File: BN014463.D
Acq: 27 Apr 2021 18:49

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:252 Resp: 573437
Ion Ratio Lower Upper
252 100
253 22.0 19.3 28.9
125 10.1 12.8 19.2#






Abundance Scan 2361 (22.849 min): BN014459.D\data.ms (-2338) (-)




Benzo(k)fluoranthene
Concen: 4.87 ng
RT: 22.805 min Scan# 2348
Delta R.T. -0.045 min
Lab File: BN014463.D
Acq: 27 Apr 2021 18:49

Tgt Ion:252 Resp: 573437
Ion Ratio Lower Upper
252 100
253 22.0 19.3 28.9
125 10.1 10.0 15.0





Abundance Scan 2515 (23.376 min): BN014459.D\data.ms (-2459) (-)




Benzo(a)pyrene
Concen: 5.34 ng
RT: 23.373 min Scan# 2514
Delta R.T. -0.004 min
Lab File: BN014463.D
Acq: 27 Apr 2021 18:49

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:252 Resp: 523492
Ion Ratio Lower Upper
252 100
253 21.9 21.0 31.6
125 11.6 20.8 31.2#



Abundance Scan 2514 (23.373 min): BN014463.D\data.ms (-2457) (-)





Abundance Scan 3197 (25.711 min): BN014459.D\data.ms (-3176) (-)




Dibenzo(a,h)anthracene
Concen: 4.91 ng
RT: 25.707 min Scan# 3196
Delta R.T. -0.004 min
Lab File: BN014463.D
Acq: 27 Apr 2021 18:49


Tgt Ion:278 Resp: 534227
Ion Ratio Lower Upper
278 100
139 16.6 14.3 21.5
279 23.5 20.3 30.5



Abundance Scan 3196 (25.707 min): BN014463.D\data.ms (-3174) (-)




Abundance Scan 3391 (26.375 min): BN014459.D\data.ms (-3333) (-)



Benzo(g,h,i)perylene
Concen: 4.75 ng
RT: 26.375 min Scan# 3391
Delta R.T. -0.000 min
Lab File: BN014463.D
Acq: 27 Apr 2021 18:49

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Abundance Scan 3391 (26.375 min): BN014463.D\data.ms



Tgt Ion:276 Resp: 547016
Ion Ratio Lower Upper
276 100
277 23.7 19.5 29.3
138 21.7 18.3 27.5

Abundance Scan 3391 (26.375 min): BN014463.D\data.ms (-3333) (-)

