

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042821\
 Data File : BN014467.D
 Acq On : 28 Apr 2021 10:32
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Quant Time: Apr 28 12:30:35 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 27 19:23:29 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.668	152	7630	0.40	ng	0.00
7) Naphthalene-d8	10.442	136	27822	0.40	ng	0.00
13) Acenaphthene-d10	14.308	164	14273	0.40	ng	0.00
19) Phenanthrene-d10	17.043	188	29139	0.40	ng	#-0.01
29) Chrysene-d12	21.247	240	27939	0.40	ng	0.00
35) Perylene-d12	23.466	264	22521	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.276	112	6213	0.43	ng	0.00
5) Phenol-d6	6.839	99	7501	0.42	ng	0.00
8) Nitrobenzene-d5	8.807	82	8260	0.44	ng	-0.01
11) 2-Methylnaphthalene-d10	12.040	152	17763	0.42	ng	0.00
14) 2,4,6-Tribromophenol	15.793	330	1718	0.37	ng	0.00
15) 2-Fluorobiphenyl	12.925	172	23395	0.44	ng	0.00
27) Fluoranthene-d10	19.086	212	32221	0.40	ng	0.00
31) Terphenyl-d14	19.692	244	24758	0.44	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.231	88	3453	0.41	ng	95
3) n-Nitrosodimethylamine	3.609	42	1348	0.33	ng	# 95
6) bis(2-Chloroethyl)ether	7.104	93	7841	0.43	ng	99
9) Naphthalene	10.492	128	29659	0.43	ng	100
10) Hexachlorobutadiene	10.784	225	5898	0.44	ng	# 100
12) 2-Methylnaphthalene	12.111	142	19094	0.42	ng	98
16) Acenaphthylene	14.016	152	23640	0.42	ng	100
17) Acenaphthene	14.359	154	16302	0.41	ng	98
18) Fluorene	15.349	166	20295	0.41	ng	100
20) 4,6-Dinitro-2-methylph...	15.437	198	897	0.40	ng	# 90
21) 4-Bromophenyl-phenylether	16.252	248	6525	0.43	ng	97
22) Hexachlorobenzene	16.361	284	9319	0.47	ng	100
23) Atrazine	16.519	200	3401	0.35	ng	98
24) Pentachlorophenol	16.702	266	1146	0.45	ng	99
25) Phenanthrene	17.091	178	34793	0.43	ng	100
26) Anthracene	17.177	178	25650	0.40	ng	100
28) Fluoranthene	19.116	202	36265	0.40	ng	100
30) Pyrene	19.483	202	35223	0.43	ng	100
32) Benzo(a)anthracene	21.237	228	30580	0.40	ng	99
33) Chrysene	21.279	228	38078	0.45	ng	100
34) Bis(2-ethylhexyl)phtha...	21.173	149	9653	0.30	ng	96
36) Indeno(1,2,3-cd)pyrene	25.691	276	35496	0.41	ng	98
37) Benzo(b)fluoranthene	22.802	252	34994	0.44	ng	# 96
38) Benzo(k)fluoranthene	22.846	252	35836	0.43	ng	99
39) Benzo(a)pyrene	23.370	252	29394	0.41	ng	# 89
40) Dibenzo(a,h)anthracene	25.708	278	29782	0.41	ng	99
41) Benzo(g,h,i)perylene	26.369	276	34122	0.45	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042821\
Data File : BN014467.D
Acq On : 28 Apr 2021 10:32
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Quant Time: Apr 28 12:30:35 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 27 19:23:29 2021
Response via : Initial Calibration




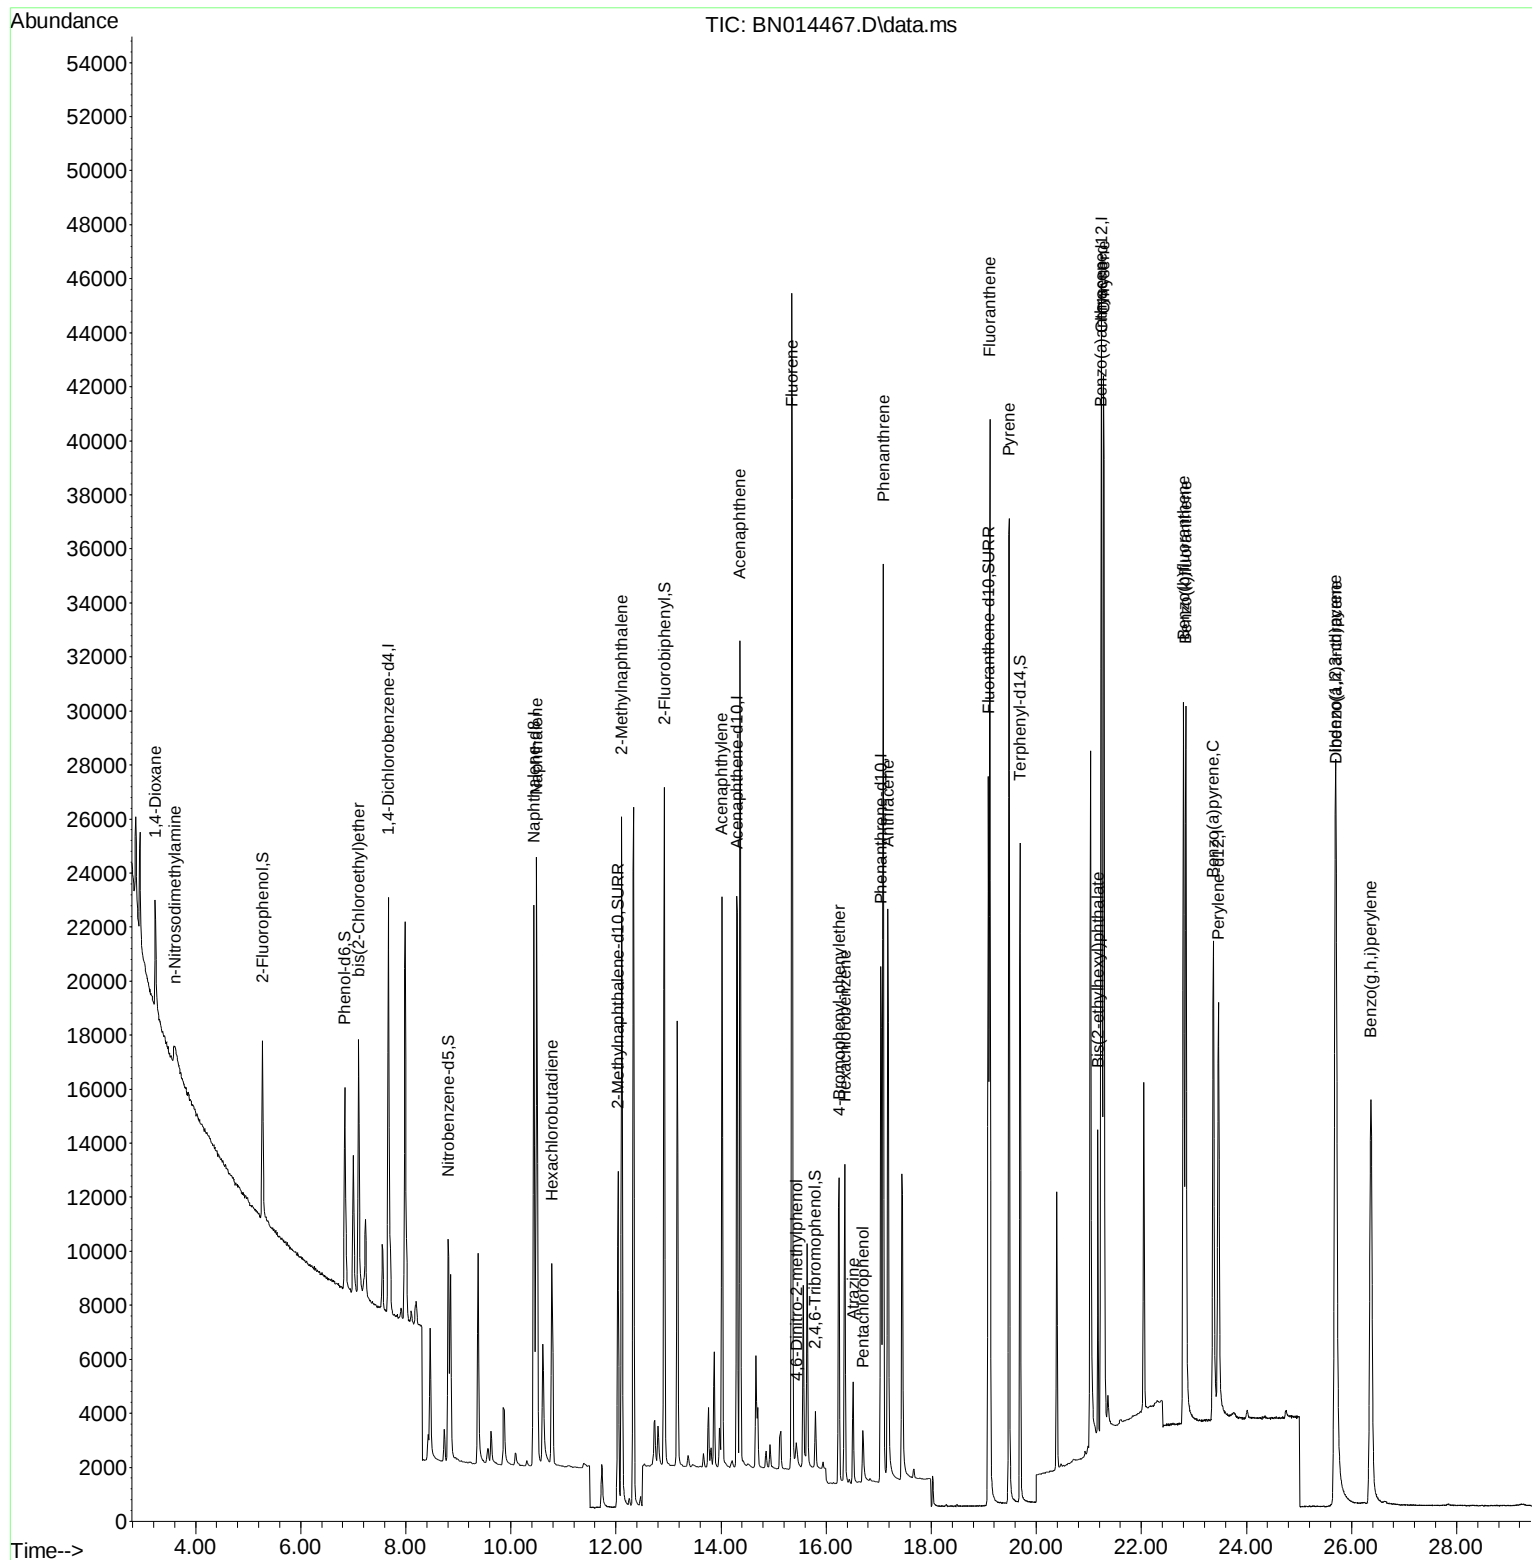


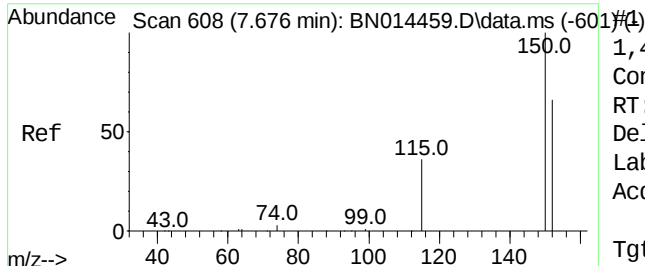

1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.668 min Scan# 607
 Delta R.T. -0.008 min
 Lab File: BN014467.D
 Acq: 28 Apr 2021 10:32




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4


Tgt Ion:	152	Resp:	7630
Ion	Ratio	Lower	Upper
152	100		
150	157.2	121.2	181.8
115	60.1	46.0	69.0

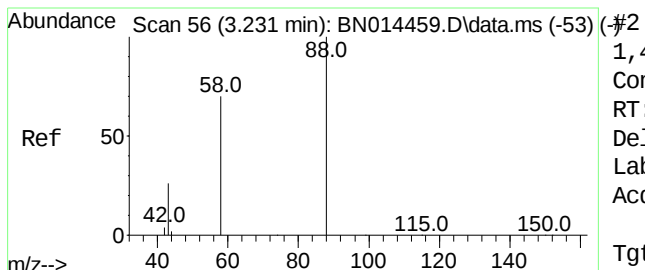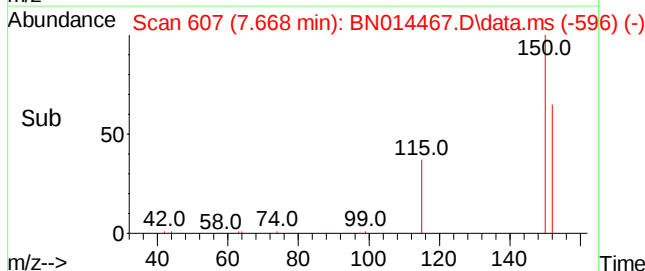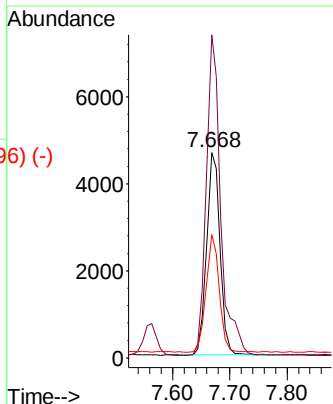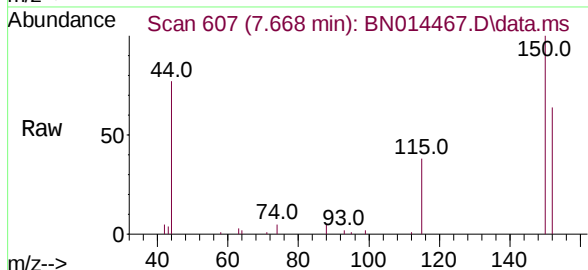

1,4-Dioxane
 Concen: 0.41 ng
 RT: 3.231 min Scan# 56
 Delta R.T. -0.000 min
 Lab File: BN014467.D
 Acq: 28 Apr 2021 10:32

Tgt Ion:	88	Resp:	3453
Ion	Ratio	Lower	Upper
88	100		
58	62.9	53.1	79.7
43	23.0	20.3	30.5


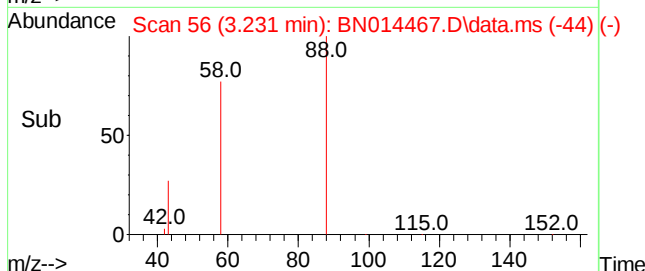
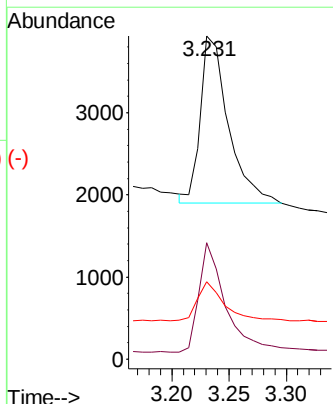



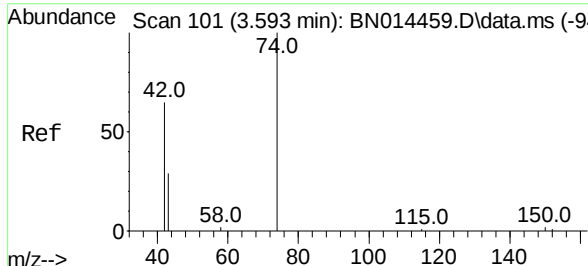

Scan 101 (3.593 min): BN014459.D\data.ms (-94) #3
 n-Nitrosodimethylamine
 Concen: 0.33 ng
 RT: 3.609 min Scan# 103
 Delta R.T. 0.016 min
 Lab File: BN014467.D
 Acq: 28 Apr 2021 10:32




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4


Tgt Ion:	42	Resp:	1348
Ion	Ratio	Lower	Upper
42	100		
74	149.8	124.7	187.1
44	0.0	0.0	0.0

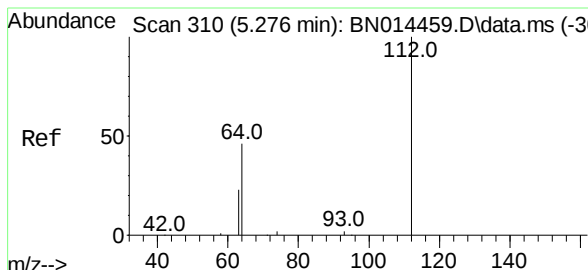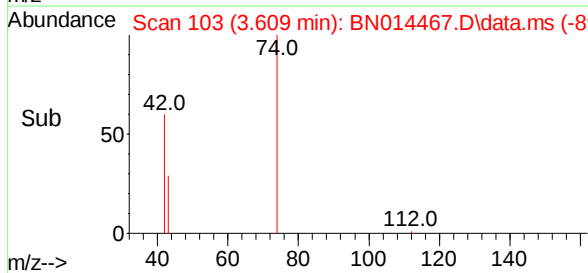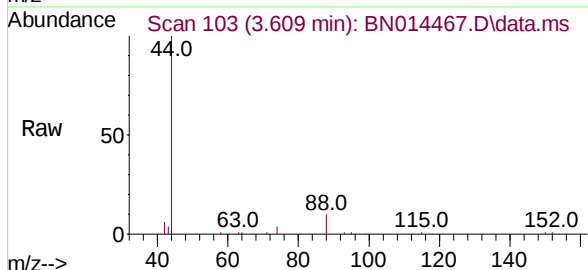

Scan 310 (5.276 min): BN014459.D\data.ms (-303) #4
 2-Fluorophenol
 Concen: 0.43 ng
 RT: 5.276 min Scan# 310
 Delta R.T. -0.000 min
 Lab File: BN014467.D
 Acq: 28 Apr 2021 10:32

Tgt Ion:	112	Resp:	6213
Ion	Ratio	Lower	Upper
112	100		
64	52.3	41.4	62.2
63	27.7	21.8	32.8


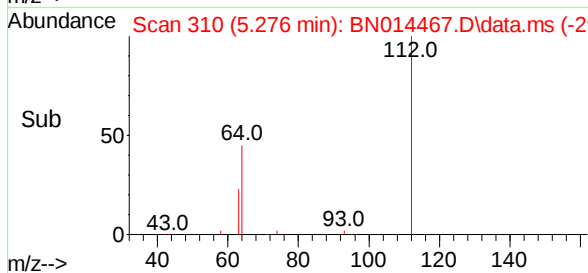




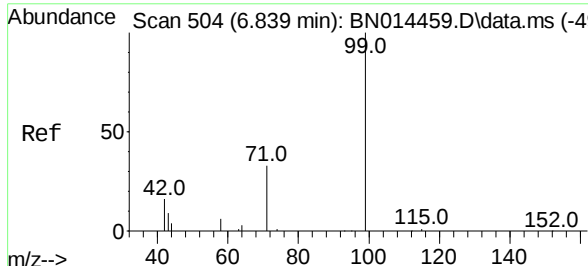

Phenol-d6
 Concen: 0.42 ng
 RT: 6.839 min Scan# 504
 Delta R.T. -0.000 min
 Lab File: BN014467.D
 Acq: 28 Apr 2021 10:32




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Tgt Ion:	99	Resp:	7501
Ion	Ratio	Lower	Upper
99	100		
42	17.9	13.8	20.6
71	32.3	25.5	38.3

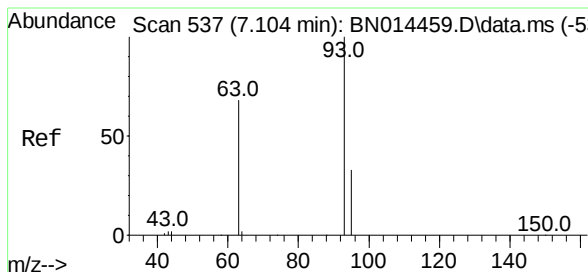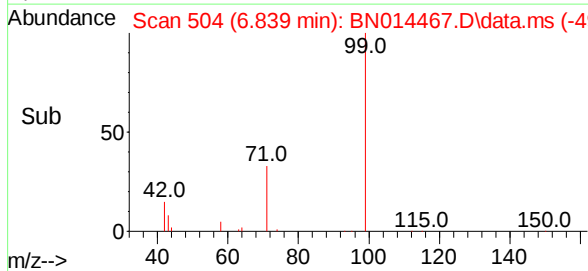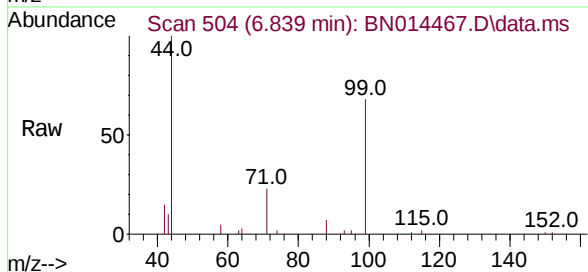

bis(2-Chloroethyl)ether
 Concen: 0.43 ng
 RT: 7.104 min Scan# 537
 Delta R.T. -0.000 min
 Lab File: BN014467.D
 Acq: 28 Apr 2021 10:32


Tgt Ion:	93	Resp:	7841
Ion	Ratio	Lower	Upper
93	100		
63	71.7	56.7	85.1
95	34.1	26.3	39.5

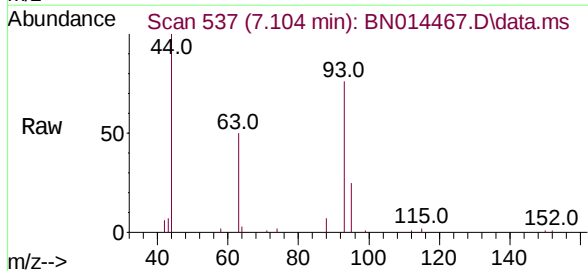




Abundance Scan 855 (10.442 min): BN014459.D\data.ms (-8507-)

Naphthalene-d8
Concen: 0.40 ng
RT: 10.442 min Scan# 855
Delta R.T. -0.000 min
Lab File: BN014467.D
Acq: 28 Apr 2021 10:32

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

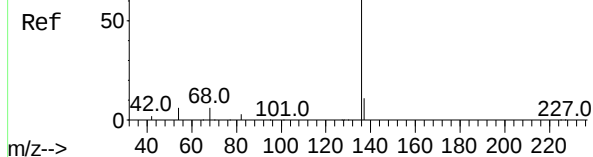



Tgt Ion	Ratio	Lower	Upper
136	100		
137	11.1	9.0	13.4
54	6.3	5.7	8.5
68	5.7	5.2	7.8

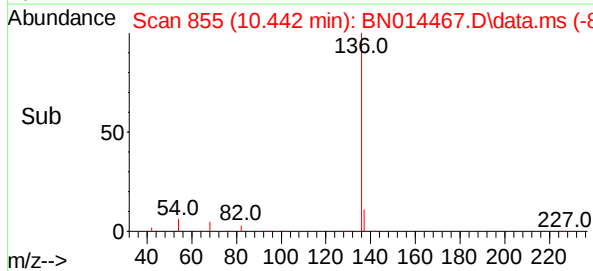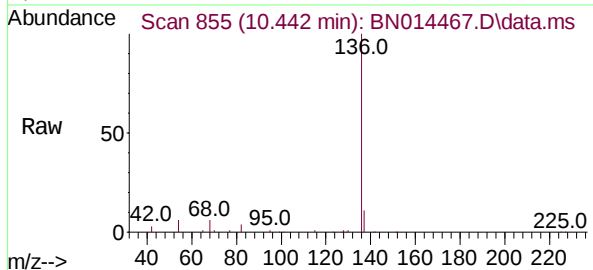


Abundance Scan 727 (8.819 min): BN014459.D\data.ms (-7237-)

Nitrobenzene-d5
Concen: 0.44 ng
RT: 8.807 min Scan# 726
Delta R.T. -0.013 min
Lab File: BN014467.D
Acq: 28 Apr 2021 10:32


Tgt Ion	Ratio	Lower	Upper
82	100		
128	34.2	38.5	57.7#
54	50.0	32.1	48.1#

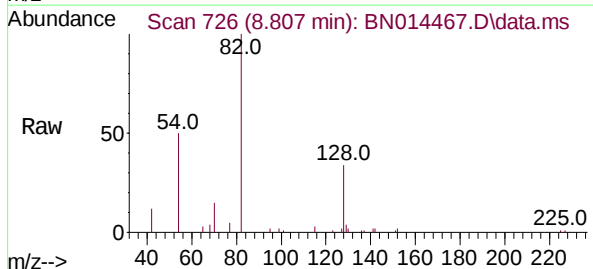

Abundance Scan 726 (8.807 min): BN014467.D\data.ms (-711-)

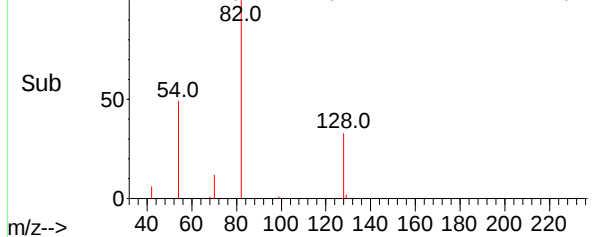




Abundance Scan 859 (10.492 min): BN014459.D\data.ms (-854) (-)




Naphthalene
Concen: 0.43 ng
RT: 10.492 min Scan# 859
Delta R.T. -0.000 min
Lab File: BN014467.D
Acq: 28 Apr 2021 10:32

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:	128	Resp:	29659
Ion	Ratio	Lower	Upper
128	100		
129	11.4	9.0	13.4
127	13.1	10.5	15.7



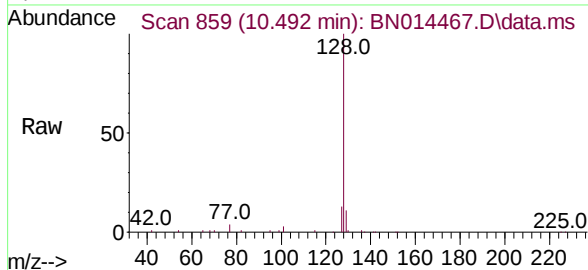


Abundance Scan 882 (10.784 min): BN014459.D\data.ms (-876) (-)




Hexachlorobutadiene
Concen: 0.44 ng
RT: 10.784 min Scan# 882
Delta R.T. -0.000 min
Lab File: BN014467.D
Acq: 28 Apr 2021 10:32

Tgt Ion:	225	Resp:	5898
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	64.3	51.5	77.3

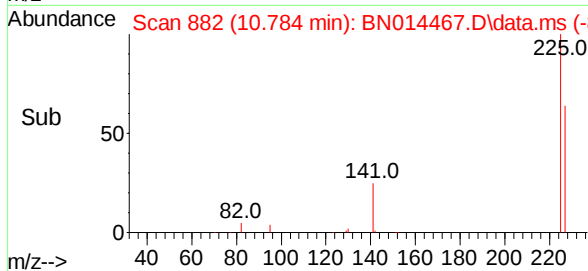




Abundance Scan 1059 (12.040 min): BN014459.D\data.ms (-1014) (-)




2-Methylnaphthalene-d10
Concen: 0.42 ng
RT: 12.040 min Scan# 1059
Delta R.T. -0.000 min
Lab File: BN014467.D
Acq: 28 Apr 2021 10:32

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:152 Resp: 17763
Ion Ratio Lower Upper
152 100
151 20.3 16.2 24.4

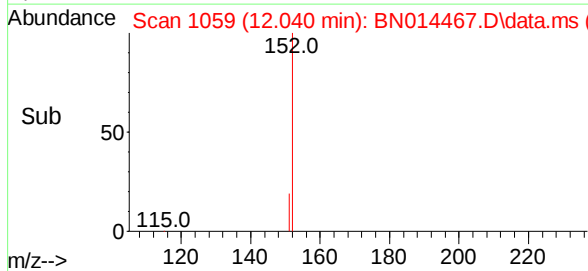
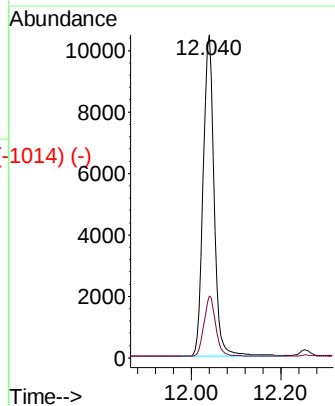
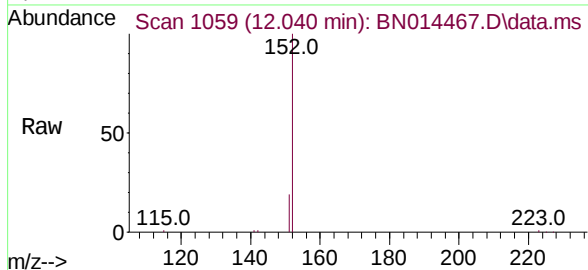


Abundance Scan 1076 (12.115 min): BN014459.D\data.ms (-1014) (-)



2-Methylnaphthalene
Concen: 0.42 ng
RT: 12.111 min Scan# 1075
Delta R.T. -0.005 min
Lab File: BN014467.D
Acq: 28 Apr 2021 10:32


Tgt Ion:142 Resp: 19094
Ion Ratio Lower Upper
142 100
141 88.6 69.6 104.4
115 35.5 27.0 40.6

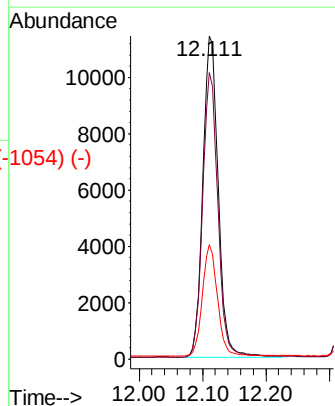




Abundance Scan 1306 (14.308 min): BN014459.D\data.ms (-1290) (-)

Acenaphthene-d10
Concen: 0.40 ng
RT: 14.308 min Scan# 1306
Delta R.T. -0.000 min
Lab File: BN014467.D
Acq: 28 Apr 2021 10:32

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

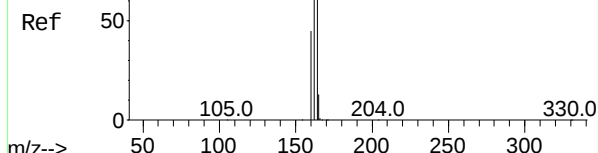





Tgt Ion	Ratio	Lower	Upper
164	100		
162	97.8	78.3	117.5
160	46.8	36.6	54.8

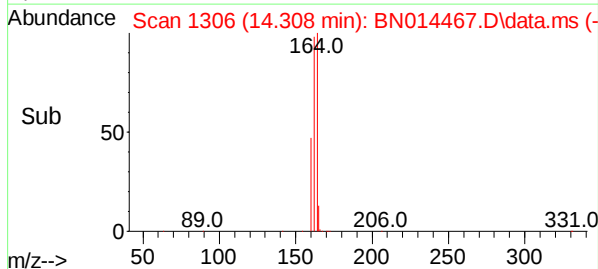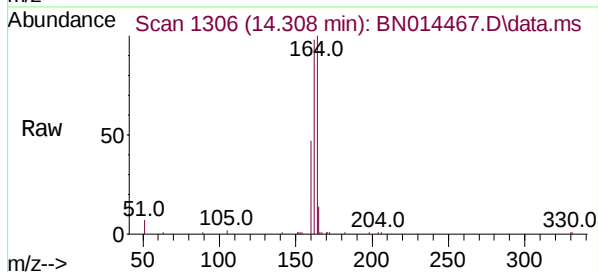


Abundance Scan 1423 (15.793 min): BN014459.D\data.ms (-1415) (-)

2,4,6-Tribromophenol
Concen: 0.37 ng
RT: 15.793 min Scan# 1423
Delta R.T. -0.000 min
Lab File: BN014467.D
Acq: 28 Apr 2021 10:32

Tgt Ion	Ratio	Lower	Upper
330	100		
332	0.0	0.0	0.0
141	35.0	29.3	43.9

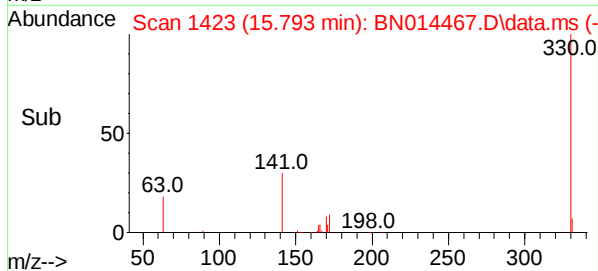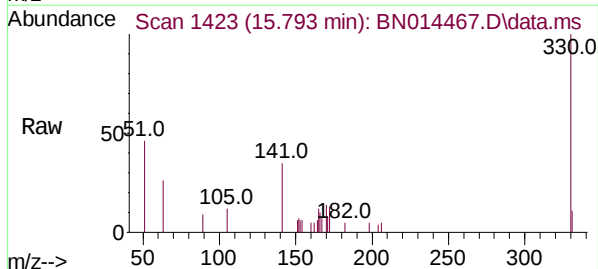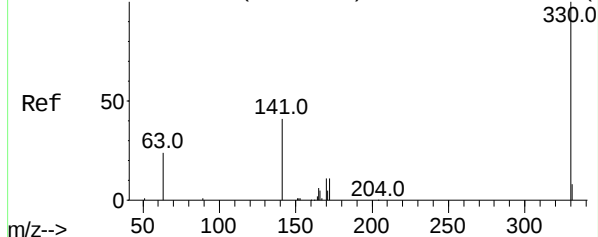



Abundance Scan 1197 (12.925 min): BN014459.D\data.ms (-1189) (-)

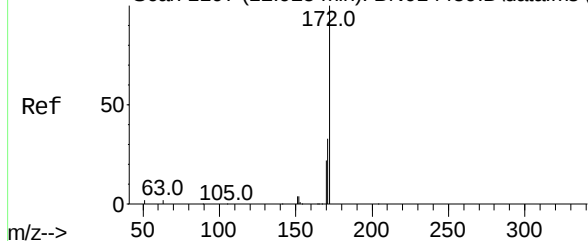


2-Fluorobiphenyl
Concen: 0.44 ng
RT: 12.925 min Scan# 1197
Delta R.T. -0.000 min
Lab File: BN014467.D
Acq: 28 Apr 2021 10:32

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	172	Resp:	23395
Ion Ratio	Lower	Upper	
172	100		
171	34.0	27.0	40.4
170	22.7	18.2	27.4

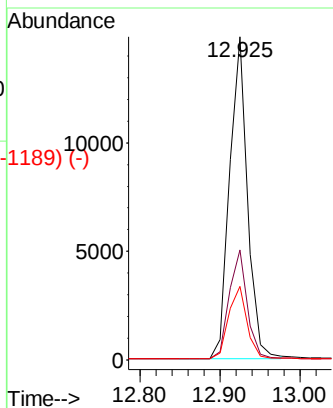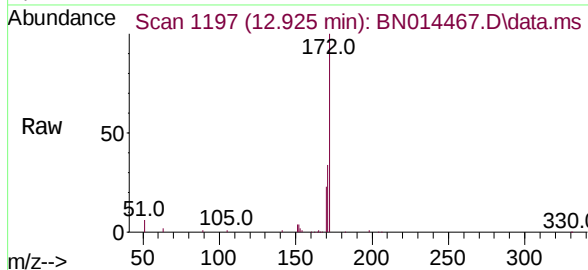

Abundance Scan 1197 (12.925 min): BN014467.D\data.ms (-1189) (-)


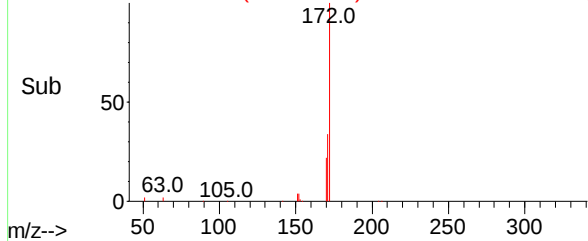


Abundance Scan 1283 (14.016 min): BN014459.D\data.ms (-1267) (-)

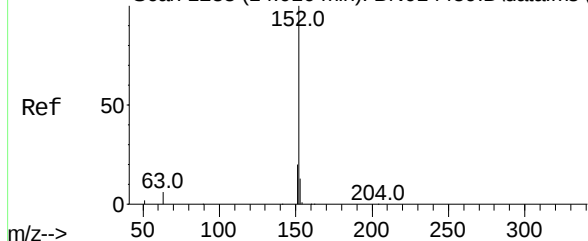


Acenaphthylene
Concen: 0.42 ng
RT: 14.016 min Scan# 1283
Delta R.T. -0.000 min
Lab File: BN014467.D
Acq: 28 Apr 2021 10:32

Tgt Ion:	152	Resp:	23640
Ion Ratio	Lower	Upper	
152	100		
151	19.4	15.4	23.2
153	13.0	10.4	15.6




Abundance Scan 1283 (14.016 min): BN014467.D\data.ms (-1267) (-)

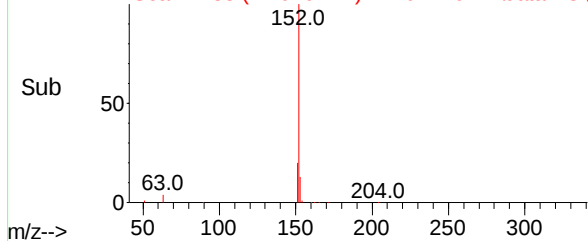




Abundance Scan 1311 (14.372 min): BN014459.D\data.ms (-1307) (-)

Acenaphthene
Concen: 0.41 ng
RT: 14.359 min Scan# 1310
Delta R.T. -0.013 min
Lab File: BN014467.D
Acq: 28 Apr 2021 10:32

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

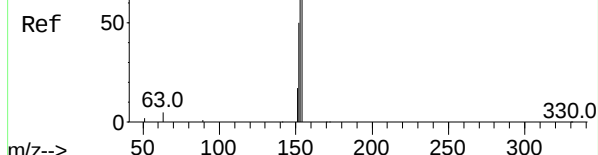


Tgt Ion:	154	Resp:	16302
Ion Ratio	Lower	Upper	
154	100		
153	114.2	90.5	135.7
152	61.5	47.2	70.8

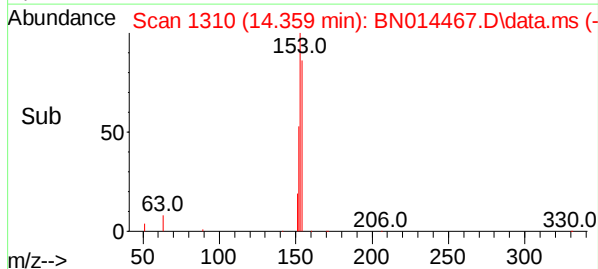

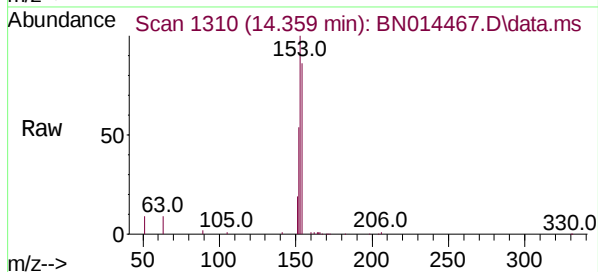



Abundance Scan 1389 (15.361 min): BN014459.D\data.ms (-1373) (-)

Fluorene
Concen: 0.41 ng
RT: 15.349 min Scan# 1388
Delta R.T. -0.013 min
Lab File: BN014467.D
Acq: 28 Apr 2021 10:32

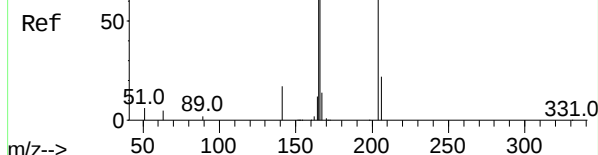

Tgt Ion:	166	Resp:	20295
Ion Ratio	Lower	Upper	
166	100		
165	98.0	78.1	117.1
167	13.5	11.0	16.6


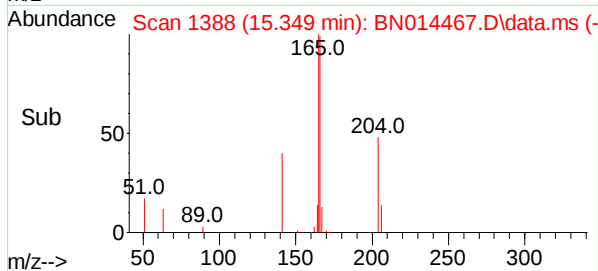

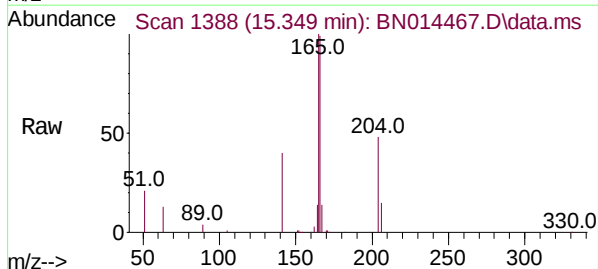


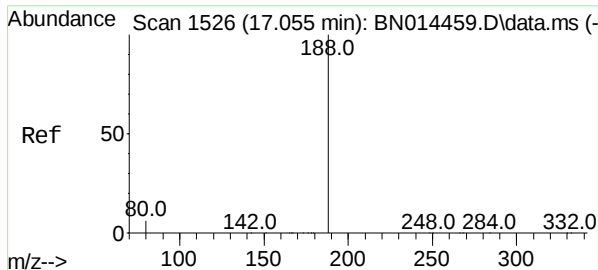

Phenanthrene-d10
Concen: 0.40 ng
RT: 17.043 min Scan# 1525
Delta R.T. -0.013 min
Lab File: BN014467.D
Acq: 28 Apr 2021 10:32




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:	188	Resp:	29139
Ion Ratio	Lower	Upper	
188	100		
94	0.0	0.0	0.0
80	12.9	5.4	8.2#

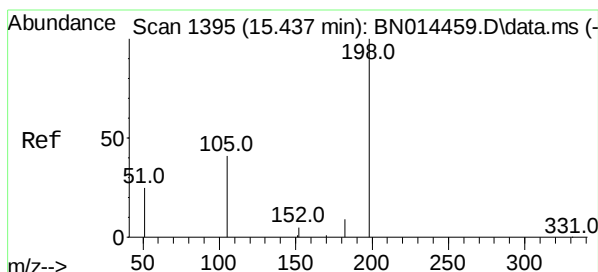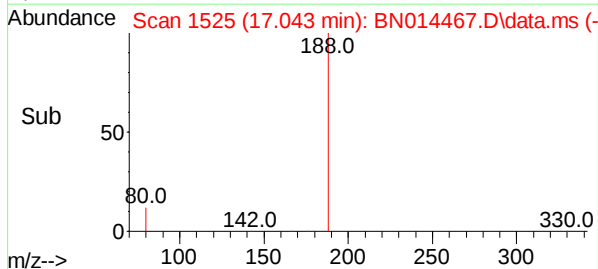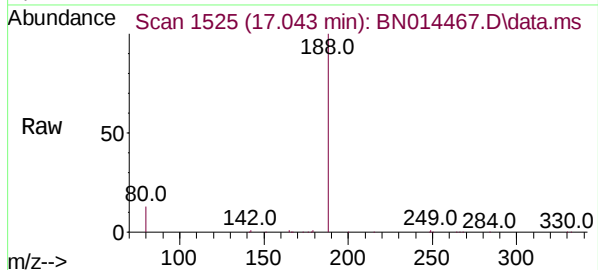


4,6-Dinitro-2-methylphenol
Concen: 0.40 ng
RT: 15.437 min Scan# 1395
Delta R.T. 0.000 min
Lab File: BN014467.D
Acq: 28 Apr 2021 10:32

Tgt Ion:	198	Resp:	897
Ion Ratio	Lower	Upper	
198	100		
51	131.3	104.5	156.7
105	56.5	62.2	93.2#

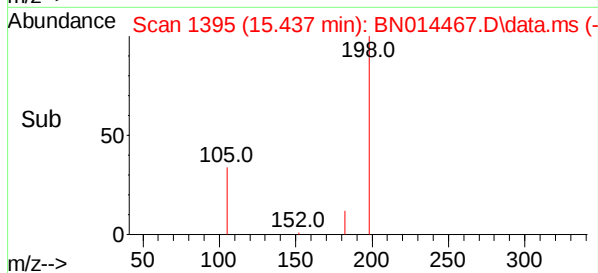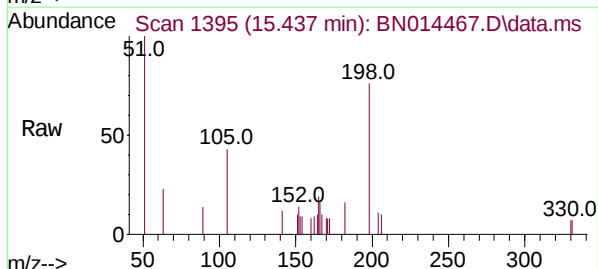



Abundance Scan 1460 (16.252 min): BN014459.D\data.ms (-1452) (-)

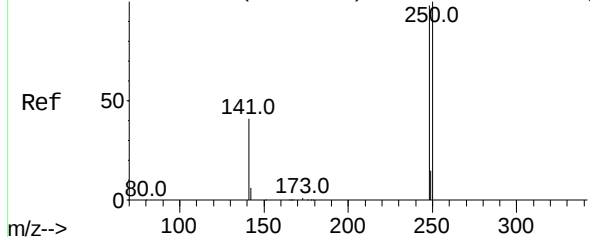


4-Bromophenyl-phenylether
Concen: 0.43 ng
RT: 16.252 min Scan# 1460
Delta R.T. -0.001 min
Lab File: BN014467.D
Acq: 28 Apr 2021 10:32

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	248	Resp:	6525
Ion	Ratio	Lower	Upper
248	100		
250	103.2	81.8	122.6
141	37.1	34.2	51.2

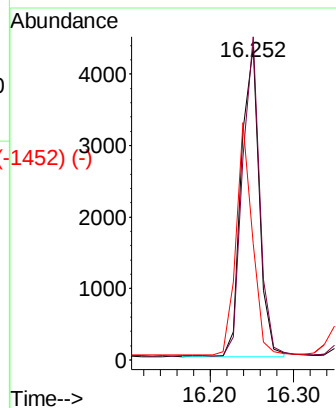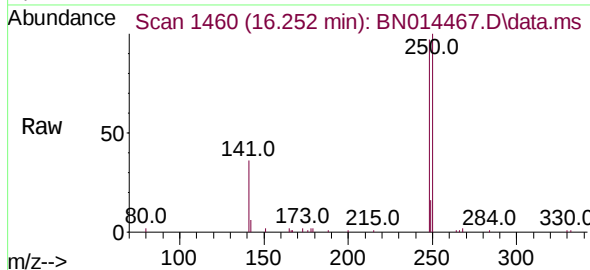

Abundance Scan 1460 (16.252 min): BN014467.D\data.ms (-1452) (-)


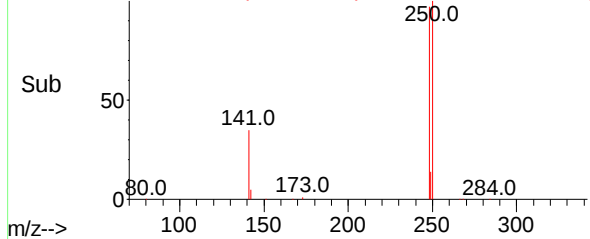


Abundance Scan 1469 (16.361 min): BN014459.D\data.ms (-1461) (-)

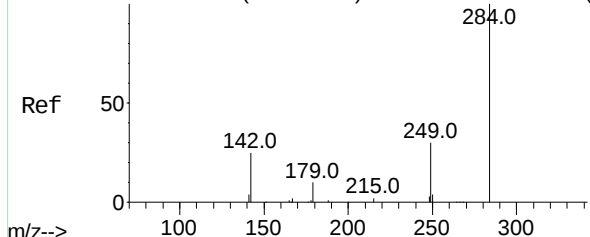


Hexachlorobenzene
Concen: 0.47 ng
RT: 16.361 min Scan# 1469
Delta R.T. -0.001 min
Lab File: BN014467.D
Acq: 28 Apr 2021 10:32

Tgt Ion:	284	Resp:	9319
Ion	Ratio	Lower	Upper
284	100		
142	34.0	27.2	40.8
249	29.2	23.4	35.2

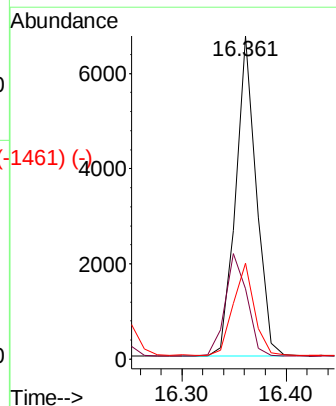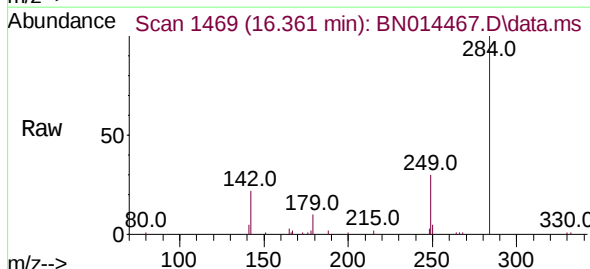


Abundance Scan 1469 (16.361 min): BN014467.D\data.ms (-1461) (-)

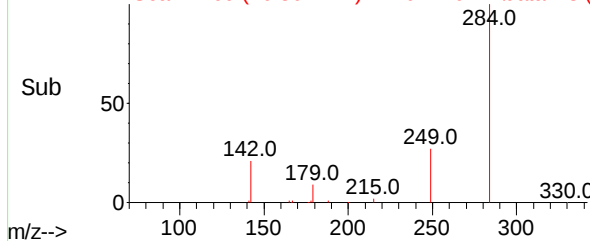



Abundance Scan 1482 (16.520 min): BN014459.D\data.ms (-1428) (-)

Atrazine
Concen: 0.35 ng
RT: 16.519 min Scan# 1482
Delta R.T. -0.001 min
Lab File: BN014467.D
Acq: 28 Apr 2021 10:32


Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

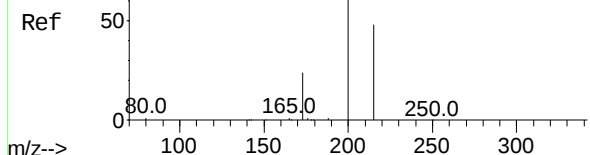

Tgt Ion	Ratio	Lower	Upper
200	100		
173	24.6	20.8	31.2
215	49.8	39.3	58.9

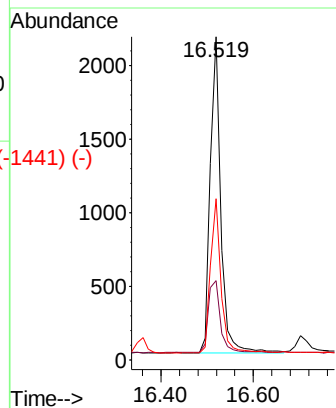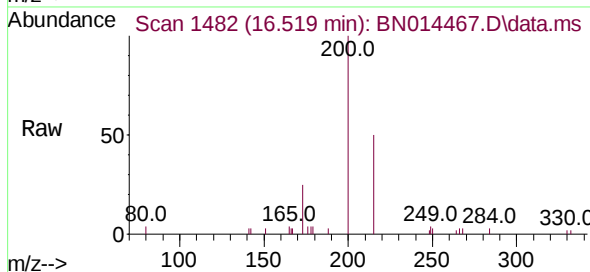




Abundance Scan 1482 (16.519 min): BN014467.D\data.ms (-1441) (-)

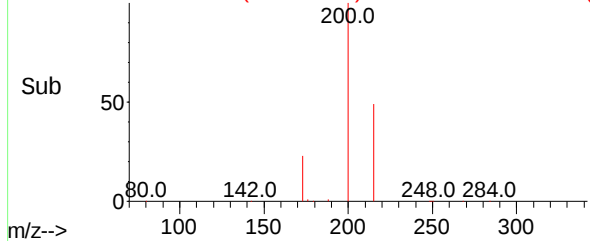


Abundance Scan 1498 (16.715 min): BN014459.D\data.ms (-1424) (-)

Pentachlorophenol
Concen: 0.45 ng
RT: 16.702 min Scan# 1497
Delta R.T. -0.013 min
Lab File: BN014467.D
Acq: 28 Apr 2021 10:32

Tgt Ion	Ratio	Lower	Upper
266	100		
264	63.8	49.9	74.9
268	64.6	51.6	77.4

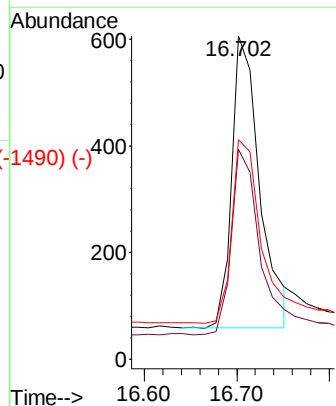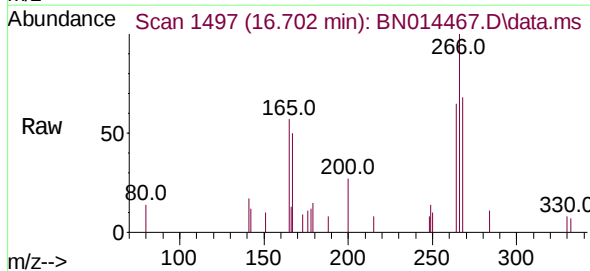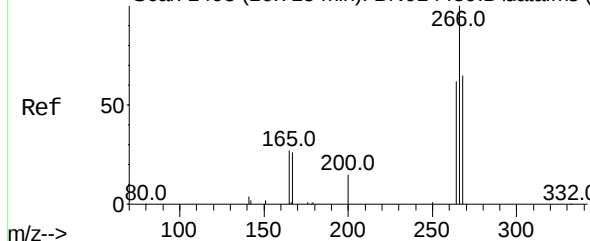


Abundance Scan 1497 (16.702 min): BN014467.D\data.ms (-1490) (-)

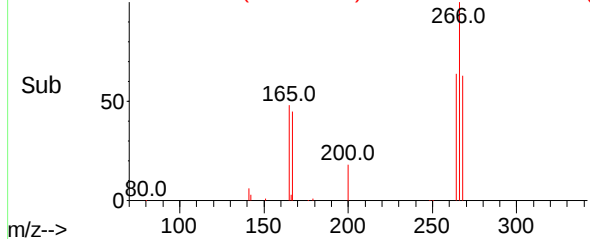




Abundance Scan 1529 (17.092 min): BN014459.D\data.ms (-1525) (-)

Phenanthrene
Concen: 0.43 ng
RT: 17.091 min Scan# 1529
Delta R.T. -0.001 min
Lab File: BN014467.D
Acq: 28 Apr 2021 10:32

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

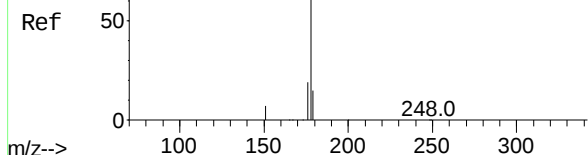





Tgt Ion:	178	Resp:	34793
Ion Ratio	Lower	Upper	
178	100		
176	18.9	15.1	22.7
179	15.3	12.2	18.4

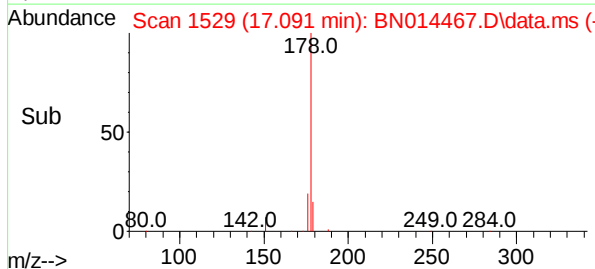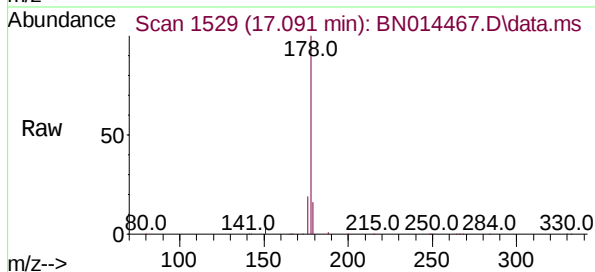


Abundance Scan 1536 (17.177 min): BN014459.D\data.ms (-1526) (-)

Anthracene
Concen: 0.40 ng
RT: 17.177 min Scan# 1536
Delta R.T. -0.001 min
Lab File: BN014467.D
Acq: 28 Apr 2021 10:32

Tgt Ion:	178	Resp:	25650
Ion Ratio	Lower	Upper	
178	100		
176	18.3	14.6	22.0
179	15.3	12.0	18.0

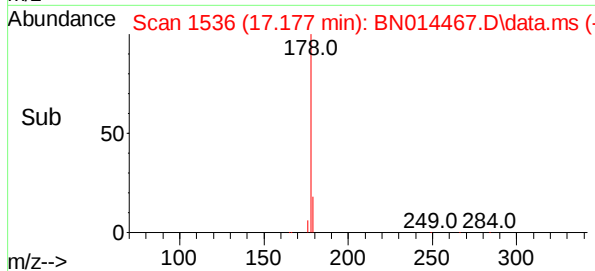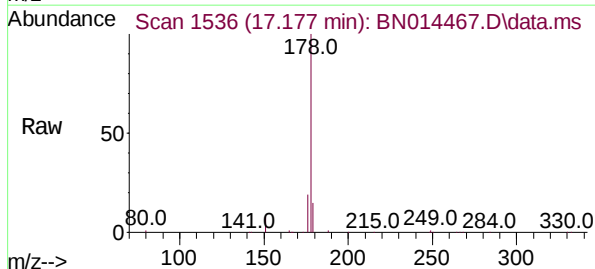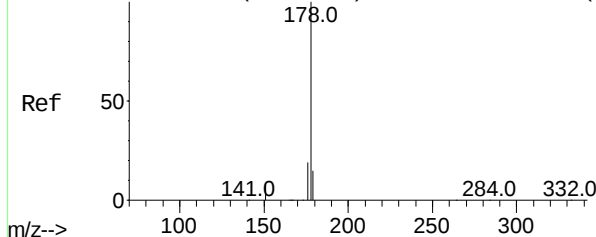



Abundance Scan 1821 (19.089 min): BN014459.D\data.ms (-1821) (-)

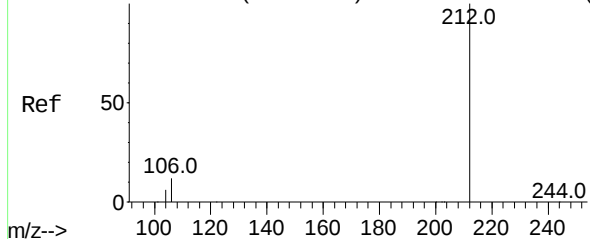


Fluoranthene-d10
Concen: 0.40 ng
RT: 19.086 min Scan# 1822
Delta R.T. -0.003 min
Lab File: BN014467.D
Acq: 28 Apr 2021 10:32

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	212	Resp:	32221
Ion Ratio	Lower	Upper	
212	100		
106	12.5	10.2	15.4
104	7.0	5.6	8.4

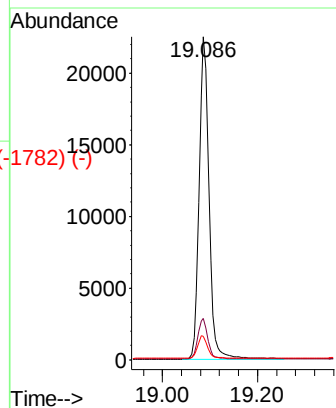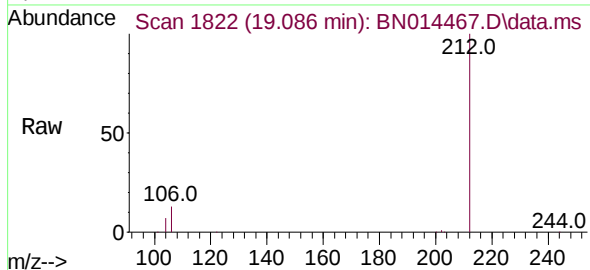

Abundance Scan 1822 (19.086 min): BN014467.D\data.ms (-1782) (-)


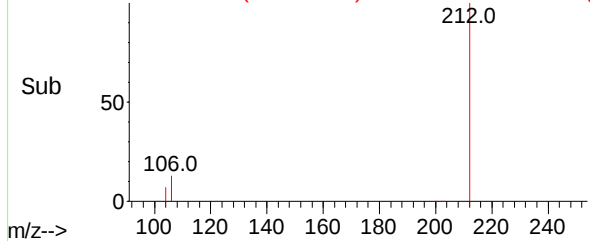


Abundance Scan 1827 (19.119 min): BN014459.D\data.ms (-1827) (-)

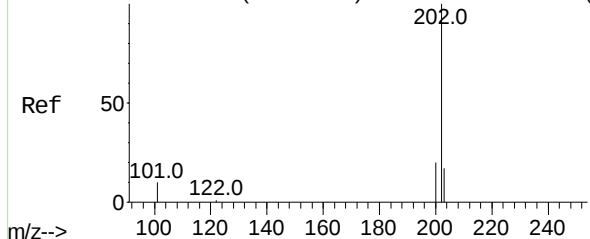


Fluoranthene
Concen: 0.40 ng
RT: 19.116 min Scan# 1828
Delta R.T. -0.003 min
Lab File: BN014467.D
Acq: 28 Apr 2021 10:32


Tgt Ion:	202	Resp:	36265
Ion Ratio	Lower	Upper	
202	100		
101	10.8	8.5	12.7
203	17.2	13.7	20.5

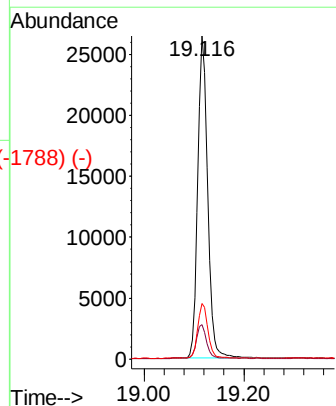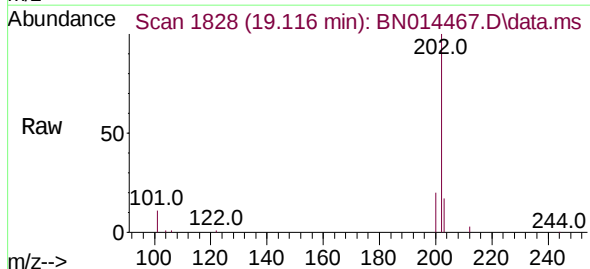

Abundance Scan 1828 (19.116 min): BN014467.D\data.ms (-1788) (-)

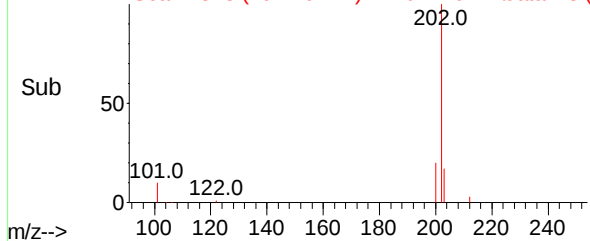



Abundance Scan 2123 (21.250 min): BN014459.D\data.ms (-2123) (-)

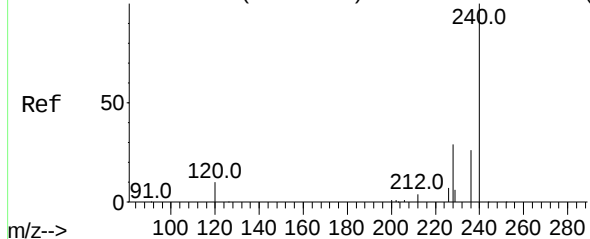


Chrysene-d12
Concen: 0.40 ng
RT: 21.247 min Scan# 2124
Delta R.T. -0.003 min
Lab File: BN014467.D
Acq: 28 Apr 2021 10:32

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	240	Resp:	27939
Ion	Ratio	Lower	Upper
240	100		
120	9.5	9.0	13.6
236	26.4	21.4	32.0

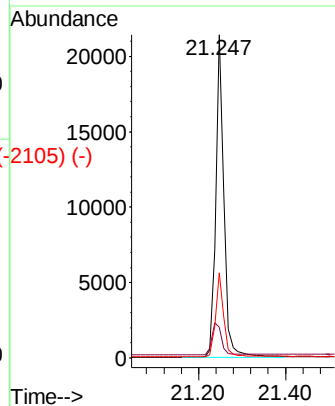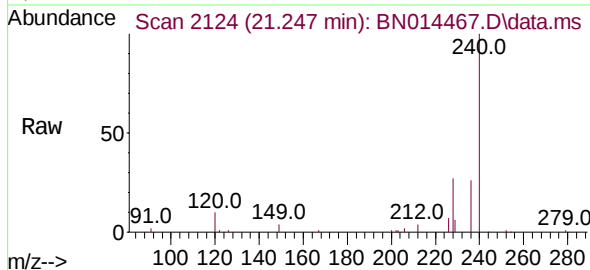

Abundance Scan 2124 (21.247 min): BN014467.D\data.ms (-2105) (-)


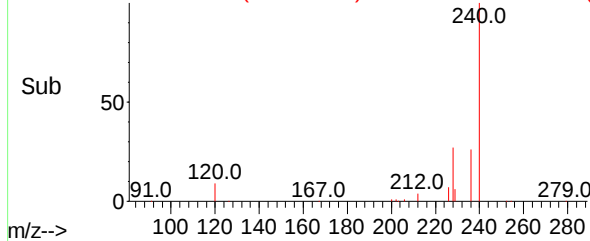


Abundance Scan 1901 (19.486 min): BN014459.D\data.ms (-1898) (-)

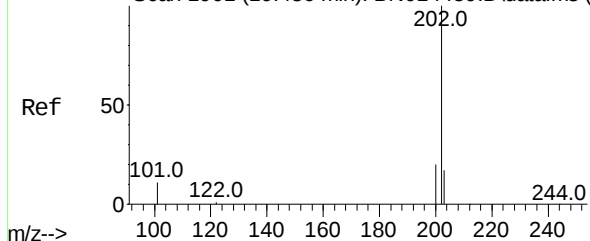


Pyrene
Concen: 0.43 ng
RT: 19.483 min Scan# 1902
Delta R.T. -0.003 min
Lab File: BN014467.D
Acq: 28 Apr 2021 10:32


Tgt Ion:	202	Resp:	35223
Ion	Ratio	Lower	Upper
202	100		
200	20.5	16.4	24.6
203	17.4	13.9	20.9

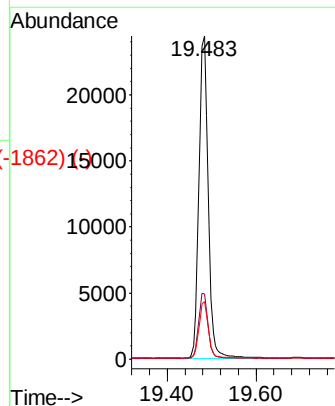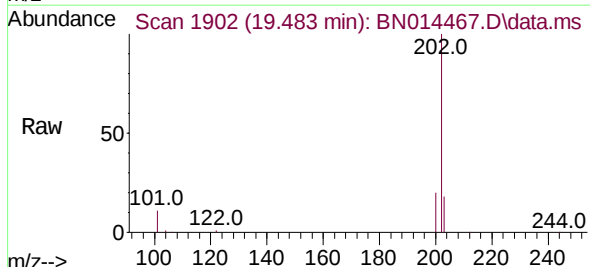

Abundance Scan 1902 (19.483 min): BN014467.D\data.ms (-1862) (-)

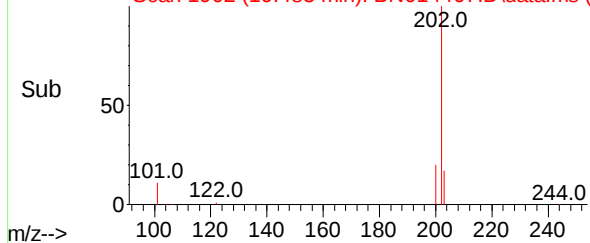



Abundance Scan 1943 (19.695 min): BN014459.D\data.ms (-1932) (-)




Terphenyl-d14
Concen: 0.44 ng
RT: 19.692 min Scan# 1944
Delta R.T. -0.003 min
Lab File: BN014467.D
Acq: 28 Apr 2021 10:32

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion	Ratio	Lower	Upper
244	100		
212	7.7	6.2	9.2
122	12.2	9.8	14.8

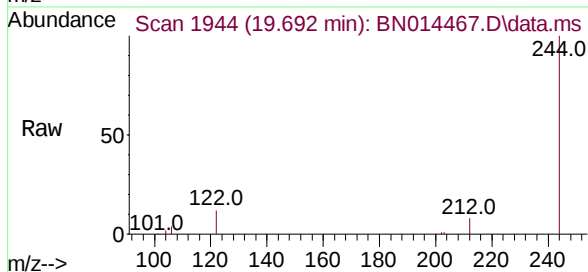

Abundance Scan 1944 (19.692 min): BN014467.D\data.ms (-1914) (-)





Abundance Scan 2122 (21.239 min): BN014459.D\data.ms (-2132) (-)




Benzo(a)anthracene
Concen: 0.40 ng
RT: 21.237 min Scan# 2123
Delta R.T. -0.003 min
Lab File: BN014467.D
Acq: 28 Apr 2021 10:32


Tgt Ion	Ratio	Lower	Upper
228	100		
226	26.3	20.8	31.2
229	19.8	16.1	24.1



Abundance Scan 2123 (21.237 min): BN014467.D\data.ms (-2104) (-)

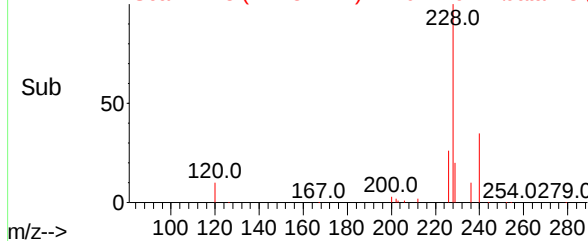




Abundance Scan 2126 (21.282 min): BN014459.D\data.ms (-2126) (-)

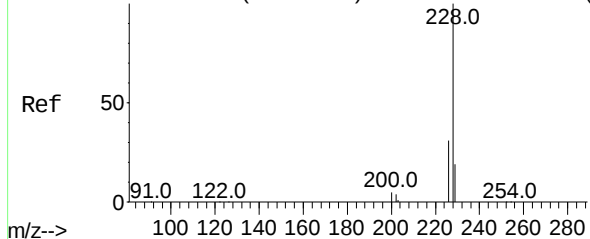


Chrysene
Concen: 0.45 ng
RT: 21.279 min Scan# 2127
Delta R.T. -0.003 min
Lab File: BN014467.D
Acq: 28 Apr 2021 10:32

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:	228	Resp:	38078
Ion	Ratio	Lower	Upper
228	100		
226	30.8	24.8	37.2
229	19.2	15.3	22.9

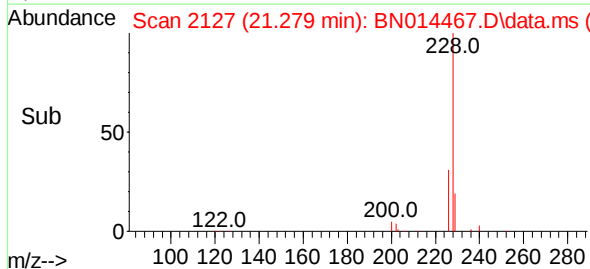
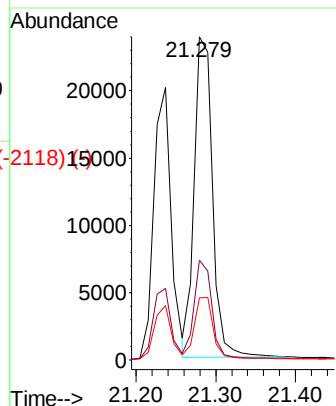
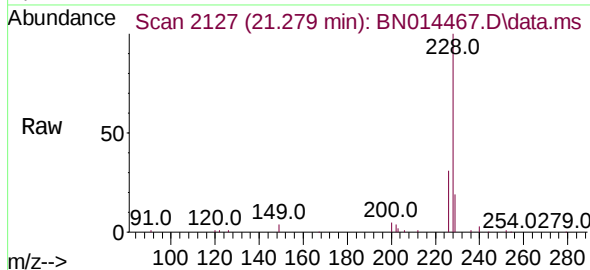


Abundance Scan 2116 (21.176 min): BN014459.D\data.ms (-2116) (-)

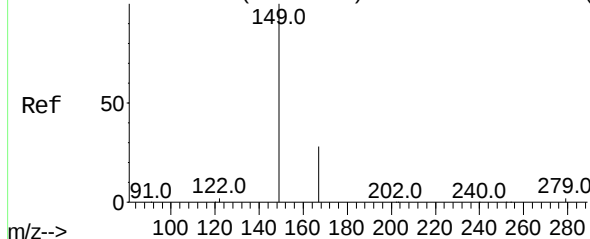

Bis(2-ethylhexyl)phthalate
Concen: 0.30 ng
RT: 21.173 min Scan# 2117
Delta R.T. -0.003 min
Lab File: BN014467.D
Acq: 28 Apr 2021 10:32


Tgt Ion:	149	Resp:	9653
Ion	Ratio	Lower	Upper
149	100		
167	26.4	19.4	29.2
279	3.7	2.9	4.3

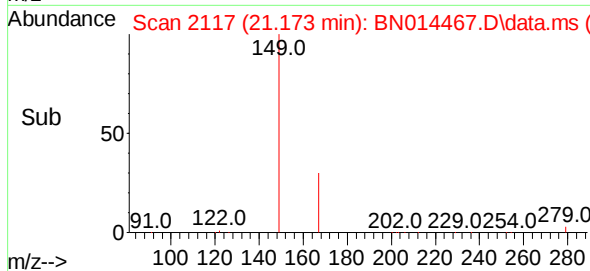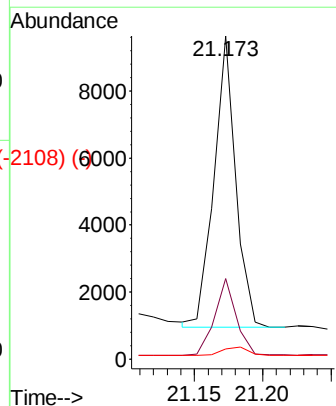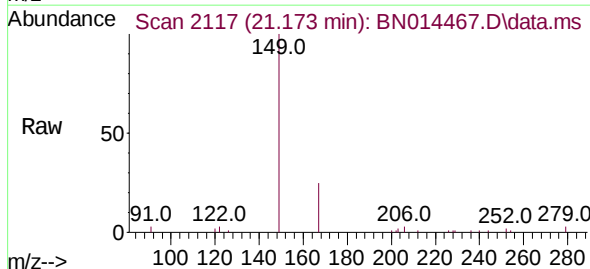




Abundance Scan 2543 (23.472 min): BN014459.D\data.ms (-2525) (-)

Perylene-d12
Concen: 0.40 ng
RT: 23.466 min Scan# 2543
Delta R.T. -0.006 min
Lab File: BN014467.D
Acq: 28 Apr 2021 10:32

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

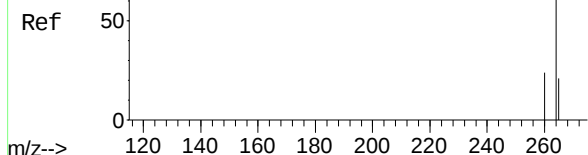





Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.6	19.8	29.6
265	41.9	31.6	47.4

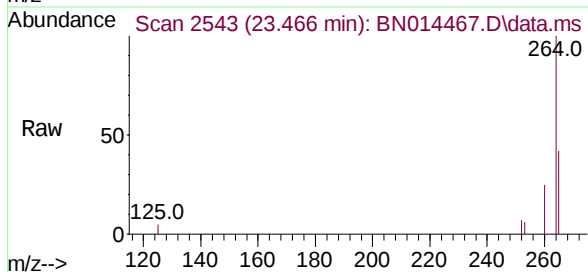


Abundance Scan 3193 (25.697 min): BN014459.D\data.ms (-3180) (-)

Indeno(1,2,3-cd)pyrene
Concen: 0.41 ng
RT: 25.691 min Scan# 3193
Delta R.T. -0.006 min
Lab File: BN014467.D
Acq: 28 Apr 2021 10:32

Tgt Ion	Ratio	Lower	Upper
276	100		
138	24.9	18.5	27.7
277	24.8	19.9	29.9

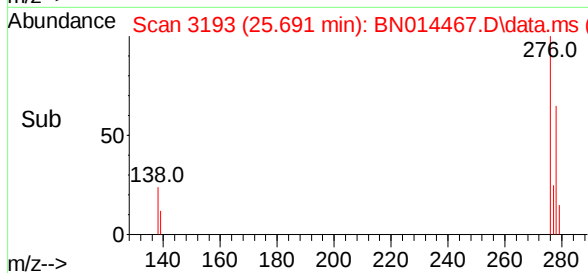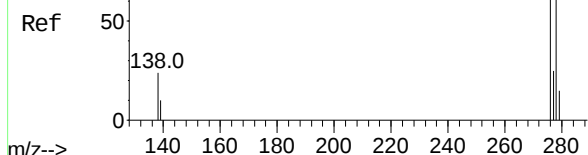



Abundance Scan 2349 (22.802 min): BN014459.D\data.ms (-2349) (-)




Benzo(b)fluoranthene
Concen: 0.44 ng
RT: 22.802 min Scan# 2349
Delta R.T. -0.006 min
Lab File: BN014467.D
Acq: 28 Apr 2021 10:32

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:252 Resp: 34994
Ion Ratio Lower Upper
252 100
253 23.9 19.3 28.9
125 12.5 12.8 19.2#

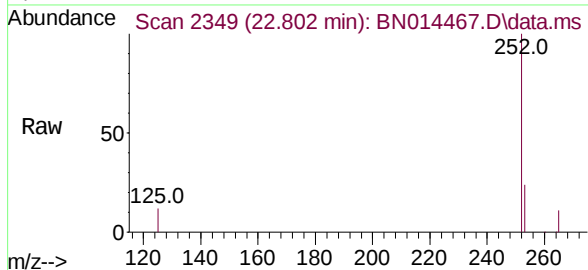

Abundance Scan 2349 (22.802 min): BN014467.D\data.ms (-2292) (-)


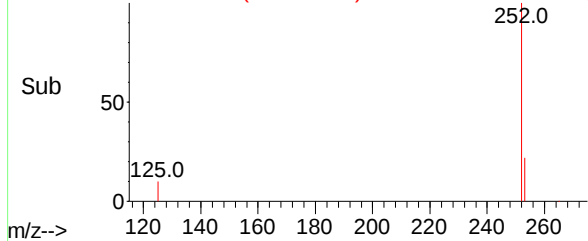


Abundance Scan 2361 (22.849 min): BN014459.D\data.ms (-2338) (-)

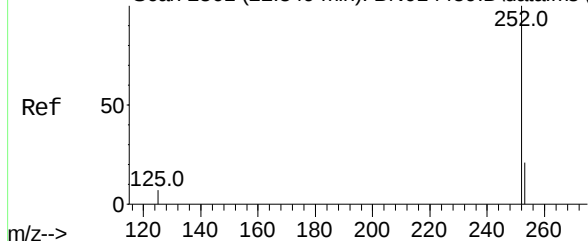


Benzo(k)fluoranthene
Concen: 0.43 ng
RT: 22.846 min Scan# 2362
Delta R.T. -0.003 min
Lab File: BN014467.D
Acq: 28 Apr 2021 10:32


Tgt Ion:252 Resp: 35836
Ion Ratio Lower Upper
252 100
253 23.7 19.3 28.9
125 11.8 10.0 15.0

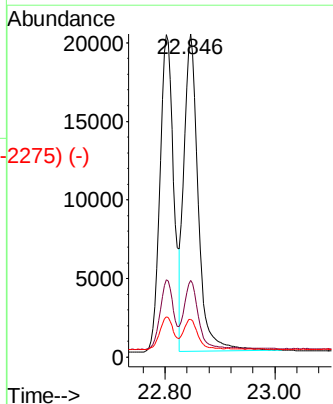

Abundance Scan 2362 (22.846 min): BN014467.D\data.ms (-2275) (-)

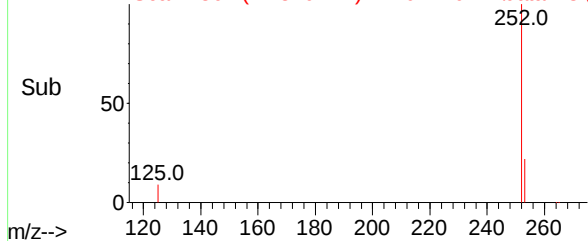



Abundance Scan 2515 (23.376 min): BN014459.D\data.ms (-2458) (-)




Benzo(a)pyrene
Concen: 0.41 ng
RT: 23.370 min Scan# 2515
Delta R.T. -0.006 min
Lab File: BN014467.D
Acq: 28 Apr 2021 10:32

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	252	Resp:	29394
Ion Ratio	Lower	Upper	
252	100		
253	25.2	21.0	31.6
125	15.6	20.8	31.2#

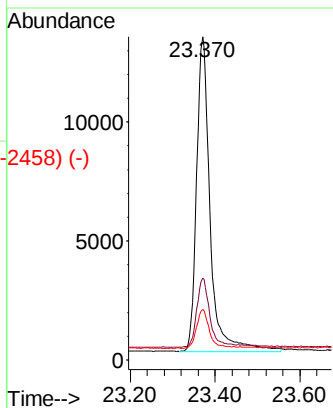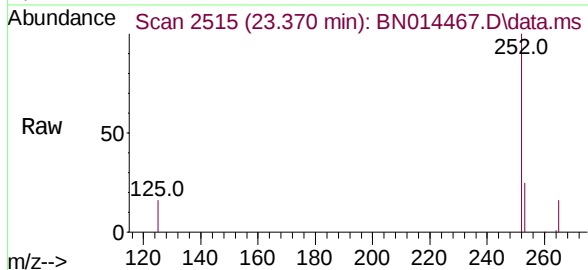

Abundance Scan 2515 (23.370 min): BN014467.D\data.ms (-2458) (-)





Abundance Scan 3197 (25.711 min): BN014459.D\data.ms (-3176) (-)




Dibenzo(a,h)anthracene
Concen: 0.41 ng
RT: 25.708 min Scan# 3198
Delta R.T. -0.003 min
Lab File: BN014467.D
Acq: 28 Apr 2021 10:32


Tgt Ion:	278	Resp:	29782
Ion Ratio	Lower	Upper	
278	100		
139	17.2	14.3	21.5
279	25.2	20.3	30.5



Abundance Scan 3198 (25.708 min): BN014467.D\data.ms (-3175) (-)



Abundance Scan 3391 (26.375 min): BN014459.D\data.ms (-3334) (-)



Benzo(g,h,i)perylene
Concen: 0.45 ng
RT: 26.369 min Scan# 3391
Delta R.T. -0.006 min
Lab File: BN014467.D
Acq: 28 Apr 2021 10:32

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:	276	Resp:	34122
Ion	Ratio	Lower	Upper
276	100		
277	24.4	19.5	29.3
138	22.4	18.3	27.5

