

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042821\
 Data File : BN014478.D
 Acq On : 28 Apr 2021 19:30
 Operator : CG/JU
 Sample : M1458-08
 Misc : LOQ--WTR-0.1PPM
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 LOQ-WATER-02-QT1-2021

Quant Time: Apr 29 02:07:31 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 27 19:23:29 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.668	152	4979	0.40	ng	0.00
7) Naphthalene-d8	10.442	136	16449	0.40	ng	0.00
13) Acenaphthene-d10	14.308	164	7378	0.40	ng	# 0.00
19) Phenanthrene-d10	17.043	188	14291	0.40	ng	#-0.01
29) Chrysene-d12	21.250	240	11685	0.40	ng	0.00
35) Perylene-d12	23.465	264	10947	0.40	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.276	112	3871	0.41	ng	0.00
5) Phenol-d6	6.839	99	4563	0.39	ng	0.00
8) Nitrobenzene-d5	8.819	82	5121	0.47	ng	0.00
11) 2-Methylnaphthalene-d10	12.040	152	9391	0.38	ng	0.00
14) 2,4,6-Tribromophenol	15.793	330	721	0.30	ng	0.00
15) 2-Fluorobiphenyl	12.925	172	12295	0.44	ng	0.00
27) Fluoranthene-d10	19.089	212	14156	0.36	ng	0.00
31) Terphenyl-d14	19.690	244	10580	0.45	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.239	88	493	0.09	ng	# 78
3) n-Nitrosodimethylamine	3.601	42	39	0.01	ng	# 1
6) bis(2-Chloroethyl)ether	7.104	93	1421	0.12	ng	94
9) Naphthalene	10.492	128	4901	0.12	ng	97
10) Hexachlorobutadiene	10.784	225	1060	0.13	ng	# 98
12) 2-Methylnaphthalene	12.115	142	2919	0.11	ng	95
16) Acenaphthylene	14.016	152	3751	0.13	ng	99
17) Acenaphthene	14.359	154	2269	0.11	ng	# 91
18) Fluorene	15.361	166	2808	0.11	ng	99
20) 4,6-Dinitro-2-methylph...	15.437	198	82	0.21	ng	# 1
21) 4-Bromophenyl-phenylether	16.252	248	889	0.12	ng	98
22) Hexachlorobenzene	16.362	284	1491	0.15	ng	97
23) Atrazine	16.520	200	415	0.09	ng	# 88
24) Pentachlorophenol	16.715	266	125	0.29	ng	92
25) Phenanthrene	17.092	178	4563	0.12	ng	100
26) Anthracene	17.177	178	3276	0.10	ng	98
28) Fluoranthene	19.114	202	4532	0.10	ng	98
30) Pyrene	19.481	202	4241	0.12	ng	100
32) Benzo(a)anthracene	21.229	228	3527	0.11	ng	96
33) Chrysene	21.282	228	4374	0.12	ng	98
34) Bis(2-ethylhexyl)phtha...	21.176	149	1802	0.13	ng	100
36) Indeno(1,2,3-cd)pyrene	25.693	276	4988	0.12	ng	100
37) Benzo(b)fluoranthene	22.801	252	4463	0.11	ng	# 81
38) Benzo(k)fluoranthene	22.846	252	4635	0.12	ng	# 78
39) Benzo(a)pyrene	23.369	252	3881	0.11	ng	# 75
40) Dibenzo(a,h)anthracene	25.704	278	3975	0.11	ng	# 85
41) Benzo(g,h,i)perylene	26.368	276	4969	0.13	ng	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042821\
 Data File : BN014478.D
 Acq On : 28 Apr 2021 19:30
 Operator : CG/JU
 Sample : M1458-08
 Misc : LOQ--WTR-0.1PPM
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 LOQ-WATER-02-QT1-2021

Quant Time: Apr 29 02:07:31 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 27 19:23:29 2021
 Response via : Initial Calibration




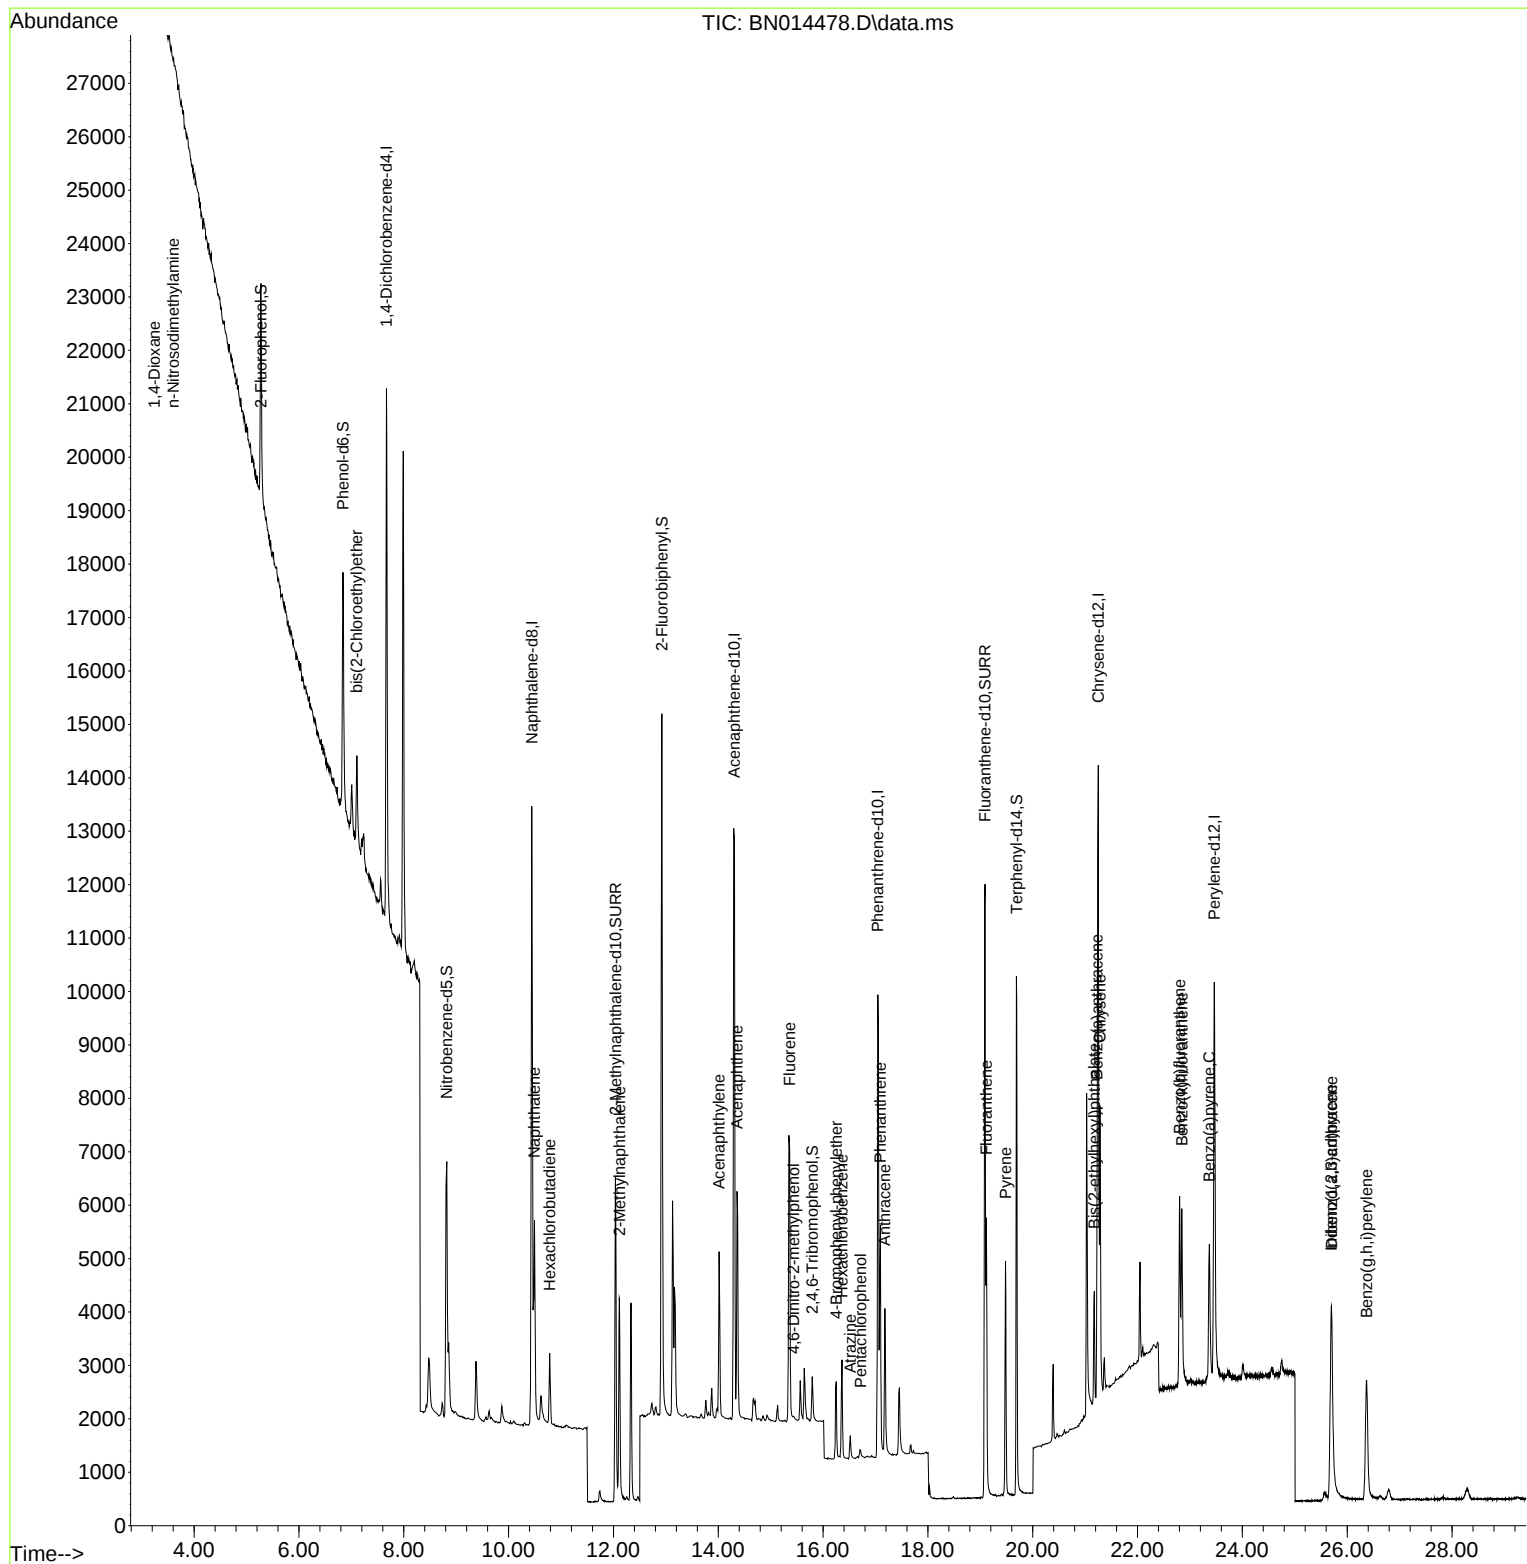




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.668 min Scan# 607
 Delta R.T. -0.008 min
 Lab File: BN014478.D
 Acq: 28 Apr 2021 19:30




Instrument :
 BNA_N
 ClientSampleId :
 LOQ-WATER-02-QT1-2021


Tgt Ion:152 Resp: 4979
 Ion Ratio Lower Upper
 152 100
 150 157.5 121.2 181.8
 115 61.6 46.0 69.0

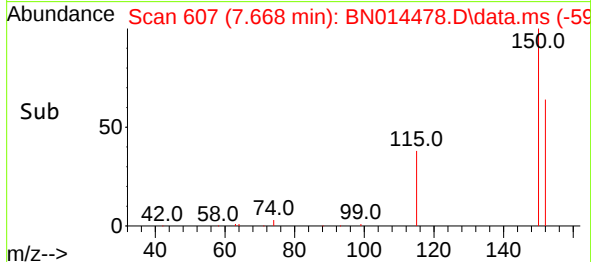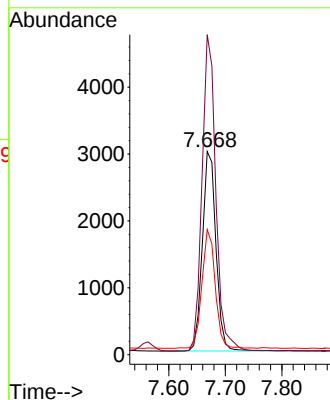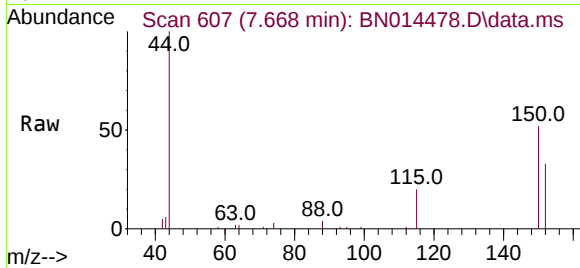

#2
 1,4-Dioxane
 Concen: 0.09 ng
 RT: 3.239 min Scan# 57
 Delta R.T. 0.008 min
 Lab File: BN014478.D
 Acq: 28 Apr 2021 19:30

Tgt Ion: 88 Resp: 493
 Ion Ratio Lower Upper
 88 100
 58 58.8 53.1 79.7
 43 52.5 20.3 30.5#



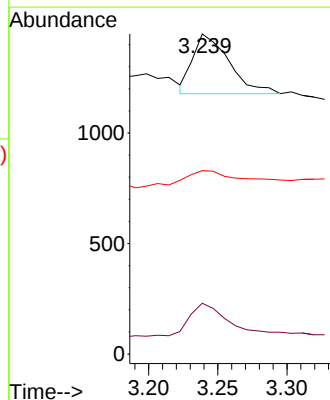
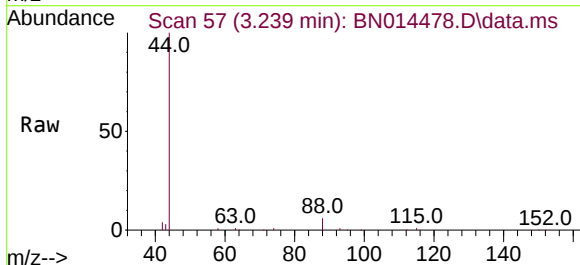




#3
n-Nitrosodimethylamine
Concen: 0.01 ng
RT: 3.601 min Scan# 102
Delta R.T. 0.008 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021


Tgt Ion: 42 Resp: 39
Ion Ratio Lower Upper
42 100
74 0.0 124.7 187.1#
44 0.0 0.0 0.0

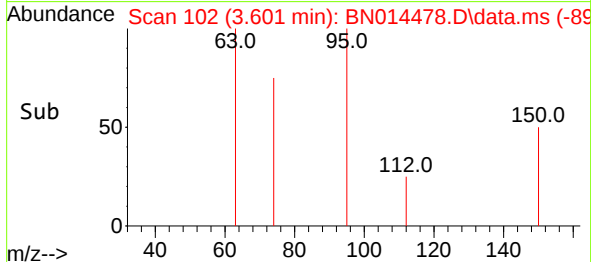

#4
2-Fluorophenol
Concen: 0.41 ng
RT: 5.276 min Scan# 310
Delta R.T. -0.000 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30

Tgt Ion: 112 Resp: 3871
Ion Ratio Lower Upper
112 100
64 53.7 41.4 62.2
63 29.3 21.8 32.8


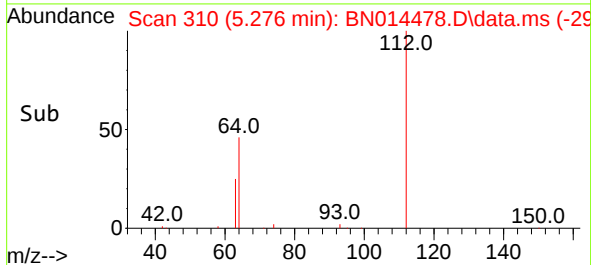




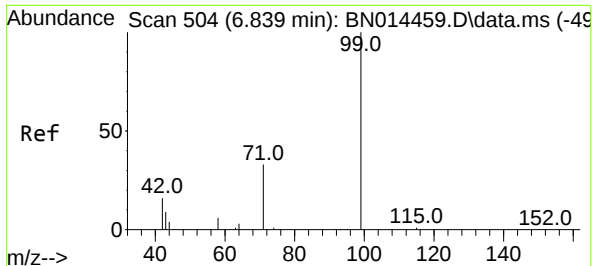

#5
Phenol-d6
Concen: 0.39 ng
RT: 6.839 min Scan# 504
Delta R.T. -0.000 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021


Tgt Ion: 99	Resp: 4563
Ion Ratio	Lower Upper
99 100	
42 18.3	13.8 20.6
71 33.6	25.5 38.3

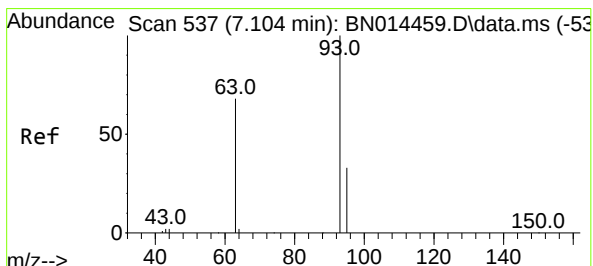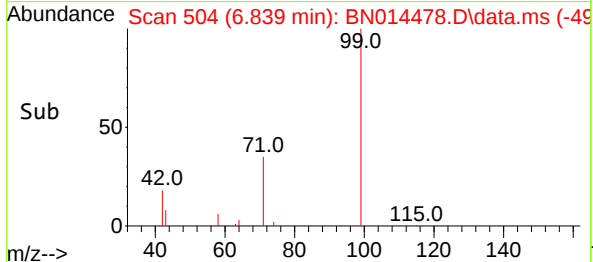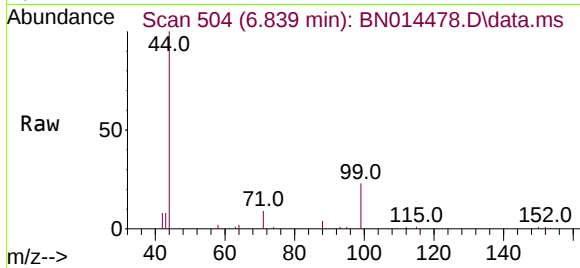

#6
bis(2-Chloroethyl)ether
Concen: 0.12 ng
RT: 7.104 min Scan# 537
Delta R.T. -0.000 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30

Tgt Ion: 93	Resp: 1421
Ion Ratio	Lower Upper
93 100	
63 75.9	56.7 85.1
95 35.4	26.3 39.5


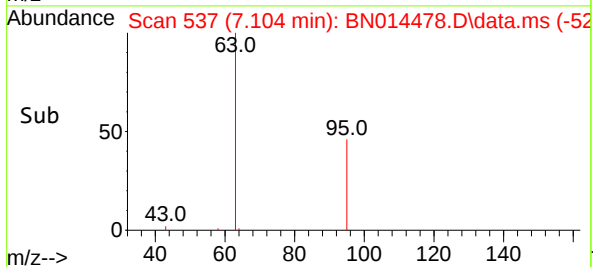

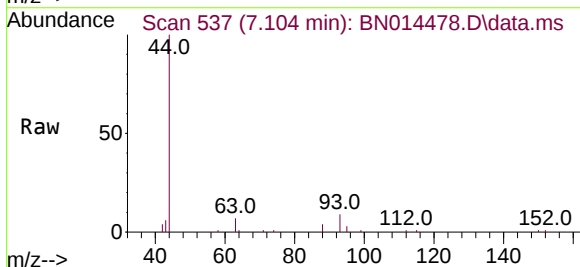




#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.442 min Scan# 855
Delta R.T. -0.000 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021


Tgt Ion:	136	Resp:	16449
Ion Ratio	Lower	Upper	
136	100		
137	11.5	9.0	13.4
54	7.7	5.7	8.5
68	6.9	5.2	7.8

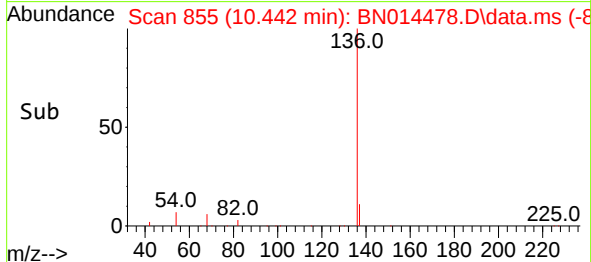

#8
Nitrobenzene-d5
Concen: 0.47 ng
RT: 8.819 min Scan# 727
Delta R.T. -0.000 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30

Tgt Ion:	82	Resp:	5121
Ion Ratio	Lower	Upper	
82	100		
128	41.9	38.5	57.7
54	44.0	32.1	48.1




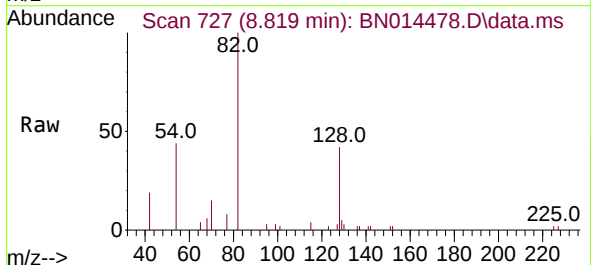




#9
Naphthalene
Concen: 0.12 ng
RT: 10.492 min Scan# 859
Delta R.T. -0.000 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021


Tgt Ion:128	Resp:	4901
Ion Ratio	Lower	Upper
128	100	
129	12.6	9.0 13.4
127	14.3	10.5 15.7

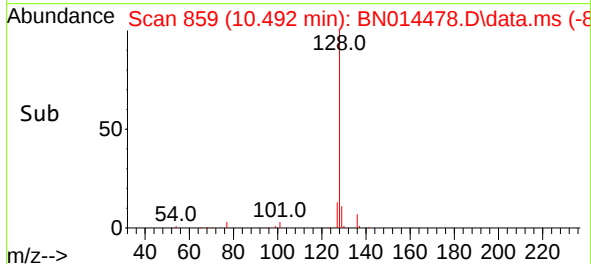

#10
Hexachlorobutadiene
Concen: 0.13 ng
RT: 10.784 min Scan# 882
Delta R.T. -0.000 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30

Tgt Ion:225	Resp:	1060
Ion Ratio	Lower	Upper
225	100	
223	0.0	0.0 0.0
227	65.9	51.5 77.3


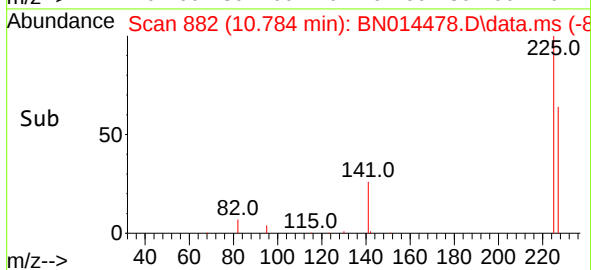

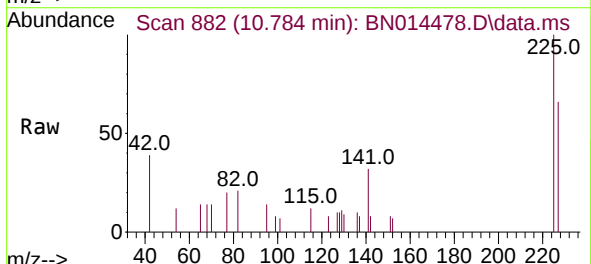




#11
2-Methylnaphthalene-d10
Concen: 0.38 ng
RT: 12.040 min Scan# 1059
Delta R.T. -0.000 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021


Tgt Ion:152 Resp: 9391
Ion Ratio Lower Upper
152 100
151 18.9 16.2 24.4

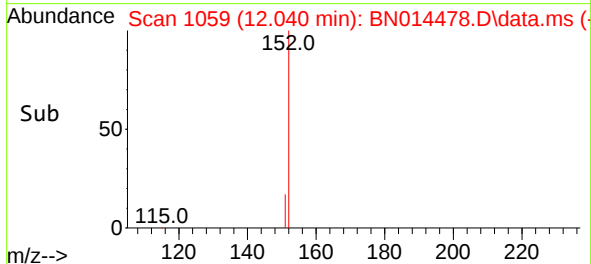

#12
2-Methylnaphthalene
Concen: 0.11 ng
RT: 12.115 min Scan# 1076
Delta R.T. -0.000 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30

Tgt Ion:142 Resp: 2919
Ion Ratio Lower Upper
142 100
141 89.9 69.6 104.4
115 38.9 27.0 40.6







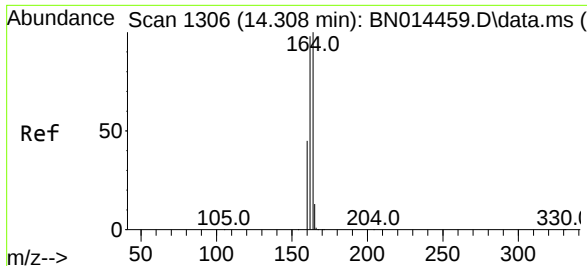

#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.308 min Scan# 1306
Delta R.T. -0.000 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021


Tgt Ion:164 Resp: 7378
Ion Ratio Lower Upper
164 100
162 97.7 78.3 117.5
160 55.8 36.6 54.8#

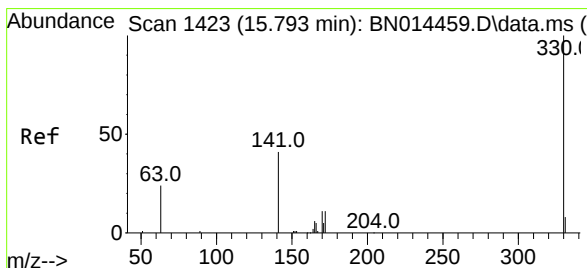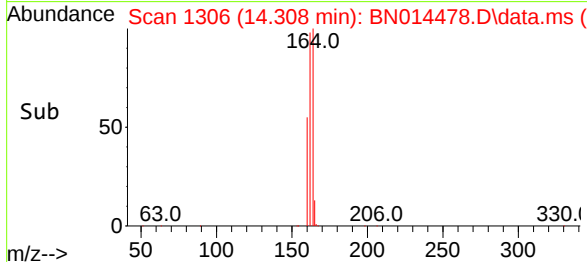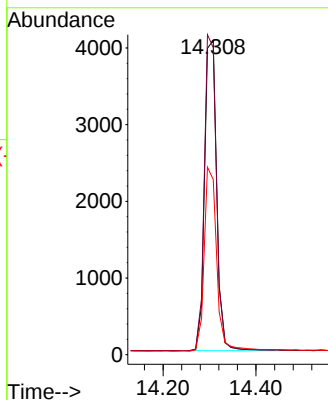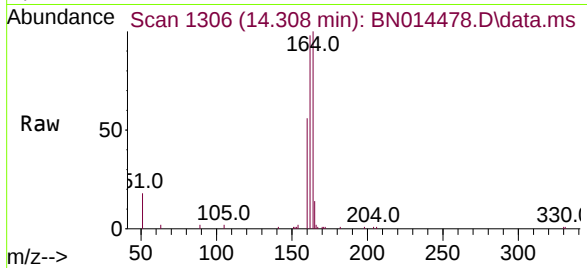

#14
2,4,6-Tribromophenol
Concen: 0.30 ng
RT: 15.793 min Scan# 1423
Delta R.T. -0.000 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30

Tgt Ion:330 Resp: 721
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 39.1 29.3 43.9


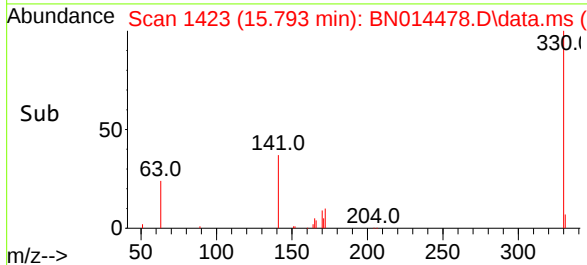
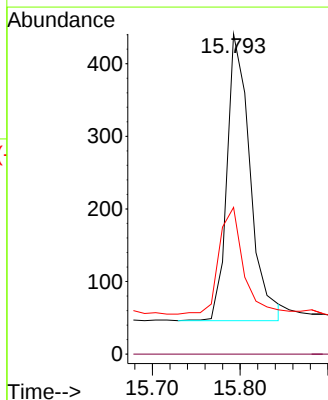
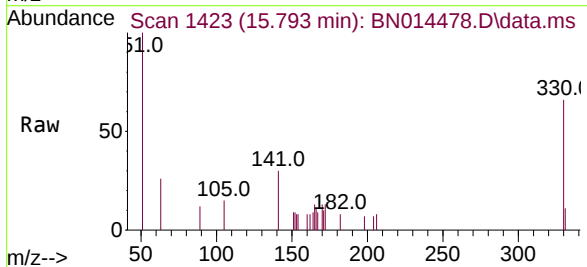




#15
2-Fluorobiphenyl
Concen: 0.44 ng
RT: 12.925 min Scan# 1197
Delta R.T. -0.000 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021


Tgt Ion:	172	Resp:	12295
Ion Ratio	Lower	Upper	
172	100		
171	34.0	27.0	40.4
170	23.3	18.2	27.4

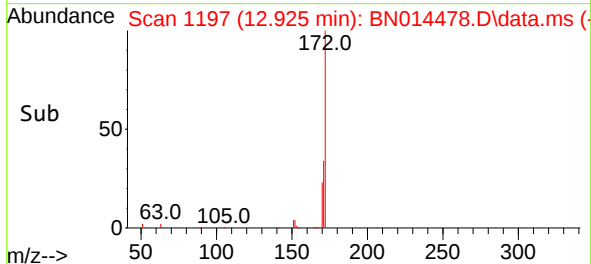

#16
Acenaphthylene
Concen: 0.13 ng
RT: 14.016 min Scan# 1283
Delta R.T. -0.000 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30

Tgt Ion:	152	Resp:	3751
Ion Ratio	Lower	Upper	
152	100		
151	19.0	15.4	23.2
153	12.8	10.4	15.6


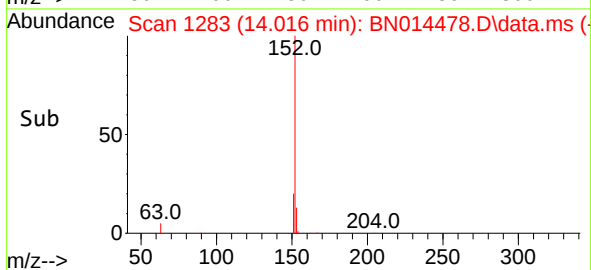




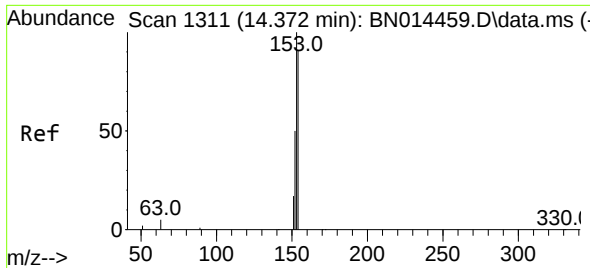

#17
Acenaphthene
Concen: 0.11 ng
RT: 14.359 min Scan# 1310
Delta R.T. -0.013 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021


Tgt Ion:154 Resp: 2269
Ion Ratio Lower Upper
154 100
153 116.4 90.5 135.7
152 74.0 47.2 70.8#

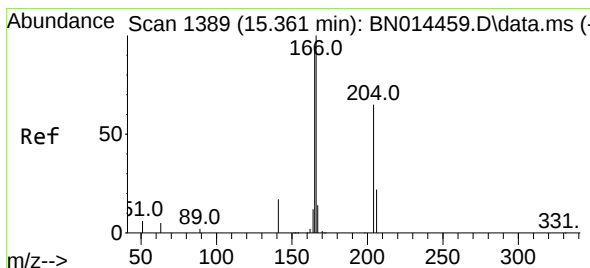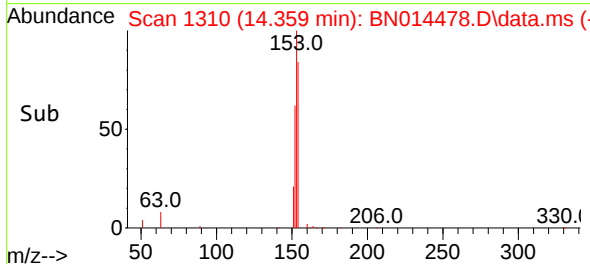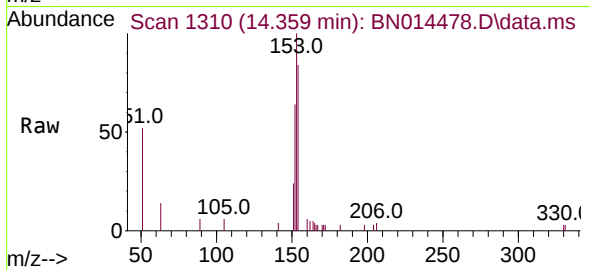

#18
Fluorene
Concen: 0.11 ng
RT: 15.361 min Scan# 1389
Delta R.T. -0.000 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30

Tgt Ion:166 Resp: 2808
Ion Ratio Lower Upper
166 100
165 98.5 78.1 117.1
167 14.1 11.0 16.6


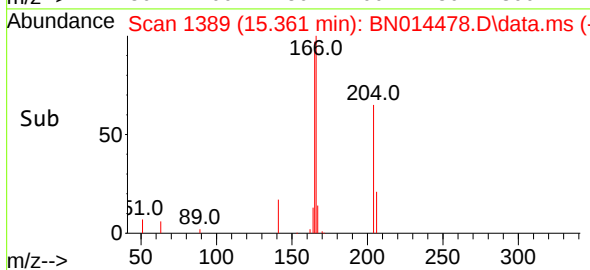

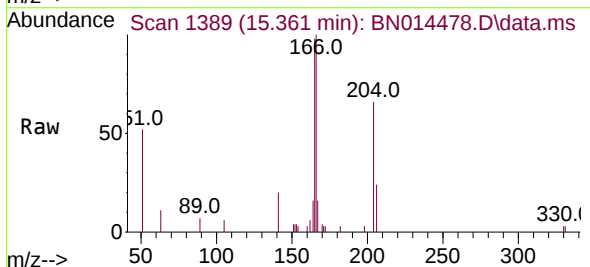


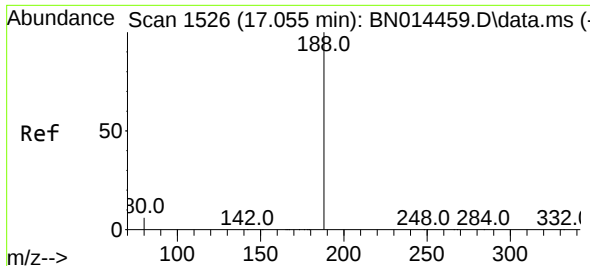

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.043 min Scan# 1525
Delta R.T. -0.012 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021


Tgt Ion:188 Resp: 14291
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 14.0 5.4 8.2#

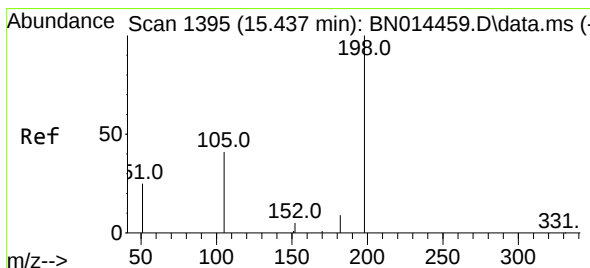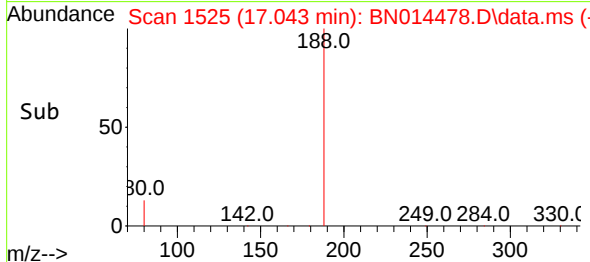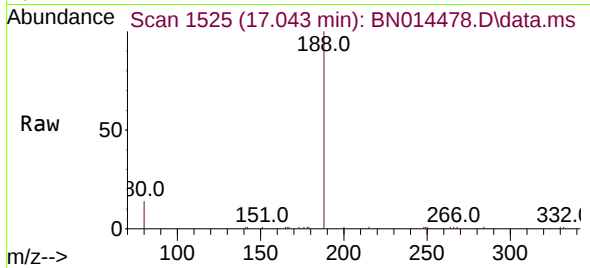

#20
4,6-Dinitro-2-methylphenol
Concen: 0.21 ng
RT: 15.437 min Scan# 1395
Delta R.T. 0.000 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30

Tgt Ion:198 Resp: 82
Ion Ratio Lower Upper
198 100
51 946.6 104.5 156.7#
105 146.6 62.2 93.2#


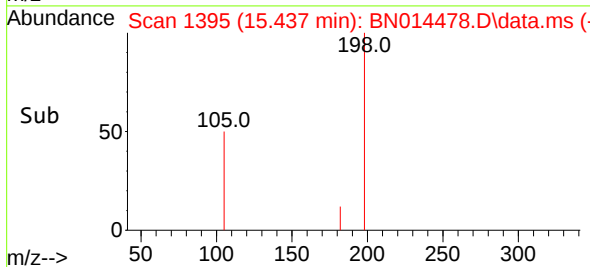

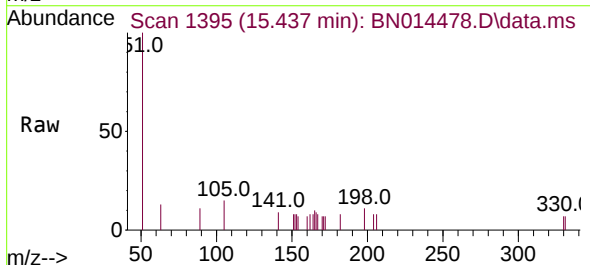


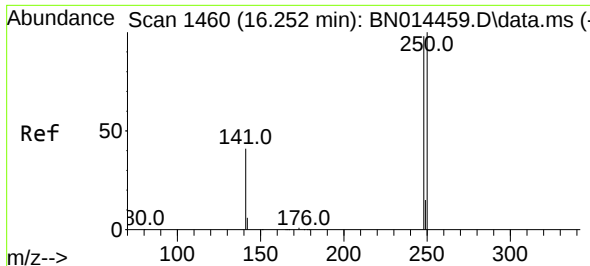

#21
4-Bromophenyl-phenylether
Concen: 0.12 ng
RT: 16.252 min Scan# 1460
Delta R.T. -0.000 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021


Tgt Ion:	248	Resp:	889
Ion	Ratio	Lower	Upper
248	100		
250	103.2	81.8	122.6
141	44.5	34.2	51.2

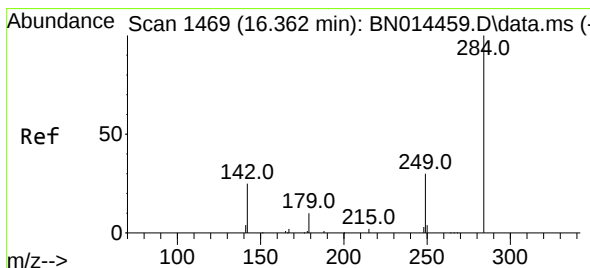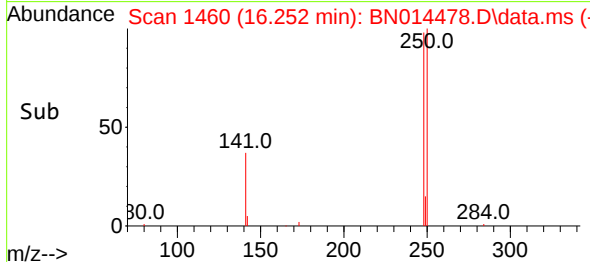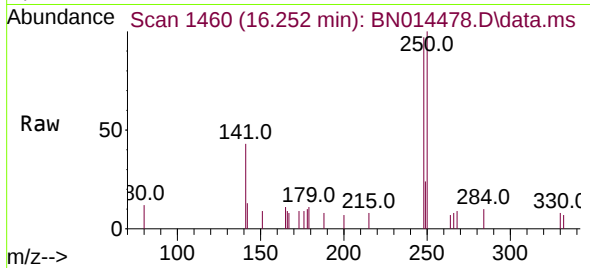

#22
Hexachlorobenzene
Concen: 0.15 ng
RT: 16.362 min Scan# 1469
Delta R.T. -0.000 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30

Tgt Ion:	284	Resp:	1491
Ion	Ratio	Lower	Upper
284	100		
142	34.5	27.2	40.8
249	31.7	23.4	35.2


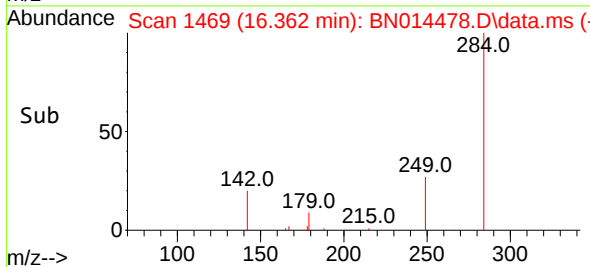

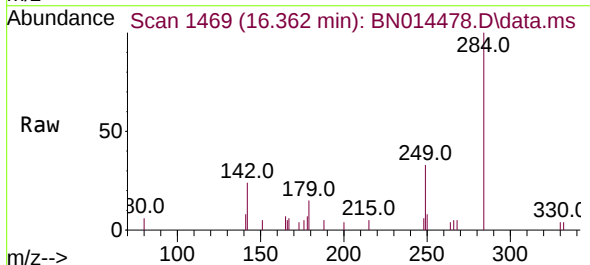




#23
Atrazine
Concen: 0.09 ng
RT: 16.520 min Scan# 1482
Delta R.T. -0.000 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021


Tgt Ion:200 Resp: 415
Ion Ratio Lower Upper
200 100
173 36.9 20.8 31.2#
215 54.2 39.3 58.9

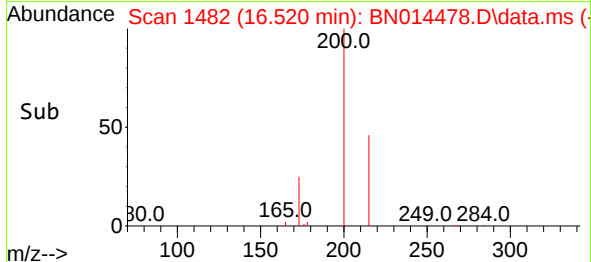

#24
Pentachlorophenol
Concen: 0.29 ng
RT: 16.715 min Scan# 1498
Delta R.T. -0.000 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30

Tgt Ion:266 Resp: 125
Ion Ratio Lower Upper
266 100
264 60.0 49.9 74.9
268 74.4 51.6 77.4




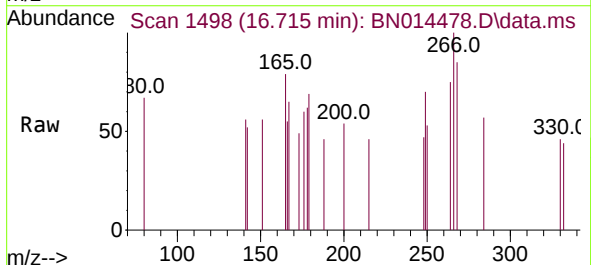




#25
Phenanthrene
Concen: 0.12 ng
RT: 17.092 min Scan# 1529
Delta R.T. -0.000 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021


Tgt Ion:178 Resp: 4563
Ion Ratio Lower Upper
178 100
176 19.0 15.1 22.7
179 15.6 12.2 18.4

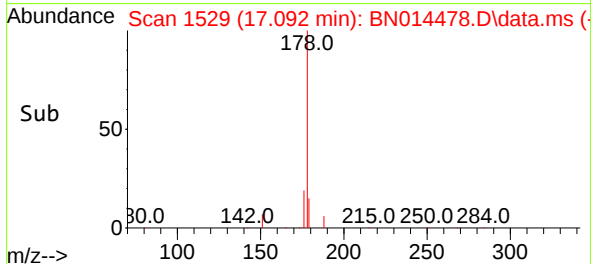

#26
Anthracene
Concen: 0.10 ng
RT: 17.177 min Scan# 1536
Delta R.T. -0.000 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30

Tgt Ion:178 Resp: 3276
Ion Ratio Lower Upper
178 100
176 19.0 14.6 22.0
179 15.8 12.0 18.0


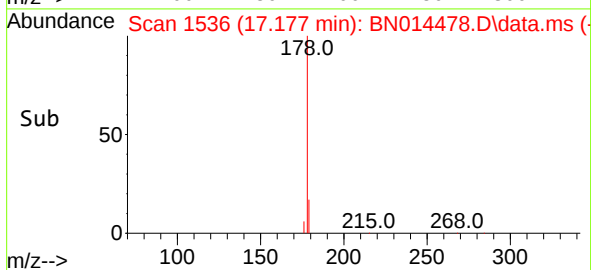

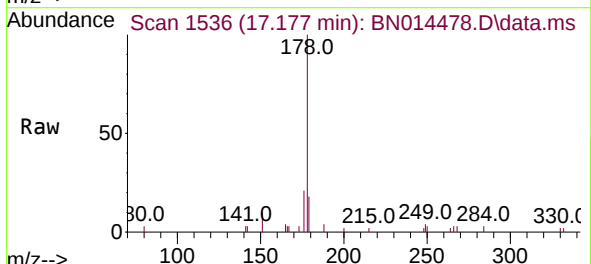




#27
Fluoranthene-d10
Concen: 0.36 ng
RT: 19.089 min Scan# 1821
Delta R.T. -0.000 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021


Tgt Ion:212 Resp: 14156
Ion Ratio Lower Upper
212 100
106 13.0 10.2 15.4
104 7.3 5.6 8.4

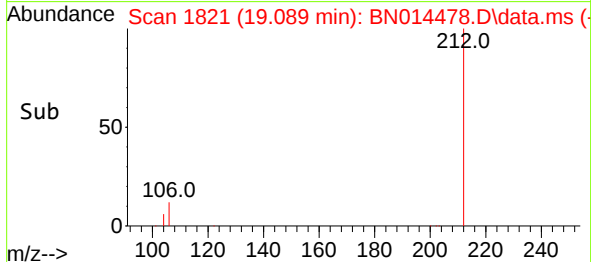

#28
Fluoranthene
Concen: 0.10 ng
RT: 19.114 min Scan# 1826
Delta R.T. -0.005 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30

Tgt Ion:202 Resp: 4532
Ion Ratio Lower Upper
202 100
101 11.8 8.5 12.7
203 17.8 13.7 20.5




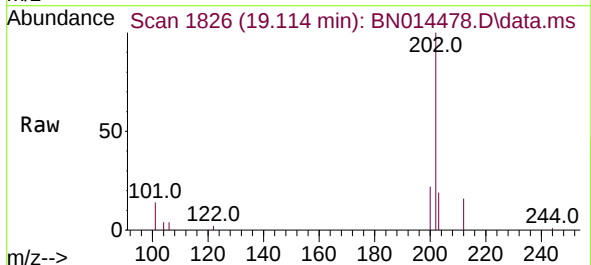


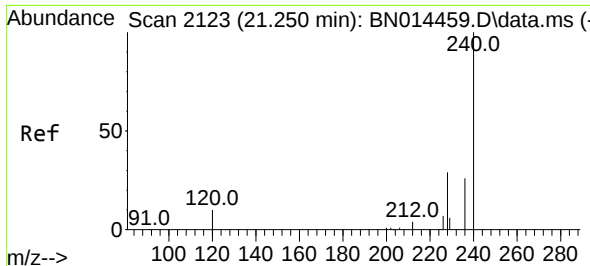

#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.250 min Scan# 2123
Delta R.T. -0.000 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021


Tgt Ion:240 Resp: 11685
Ion Ratio Lower Upper
240 100
120 9.1 9.0 13.6
236 26.4 21.4 32.0

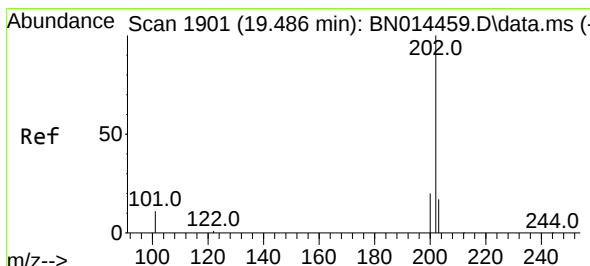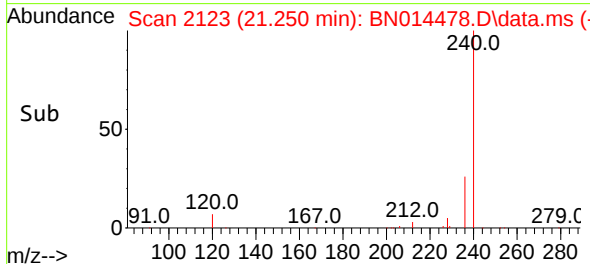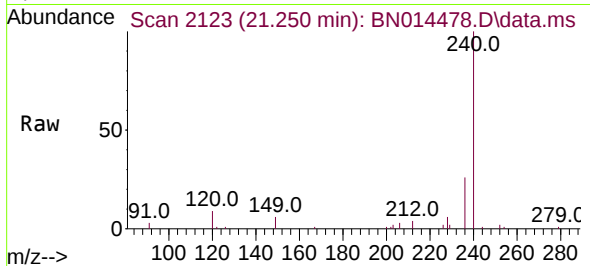

#30
Pyrene
Concen: 0.12 ng
RT: 19.481 min Scan# 1900
Delta R.T. -0.005 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30

Tgt Ion:202 Resp: 4241
Ion Ratio Lower Upper
202 100
200 20.5 16.4 24.6
203 17.8 13.9 20.9


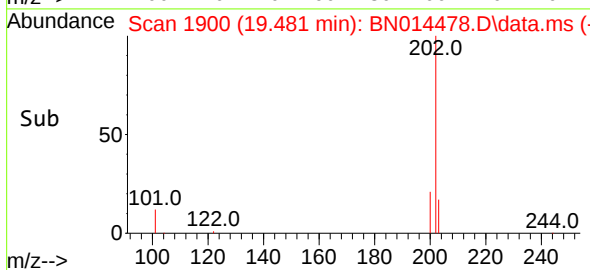

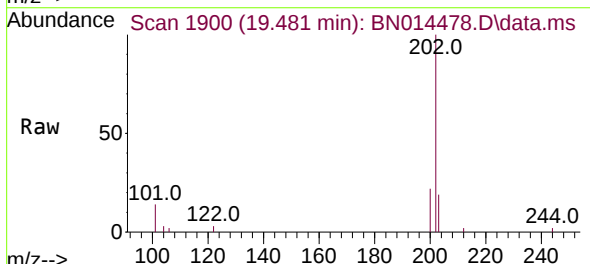




#31
Terphenyl-d14
Concen: 0.45 ng
RT: 19.690 min Scan# 1942
Delta R.T. -0.005 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021


Tgt Ion:244 Resp: 10580
Ion Ratio Lower Upper
244 100
212 8.2 6.2 9.2
122 13.9 9.8 14.8

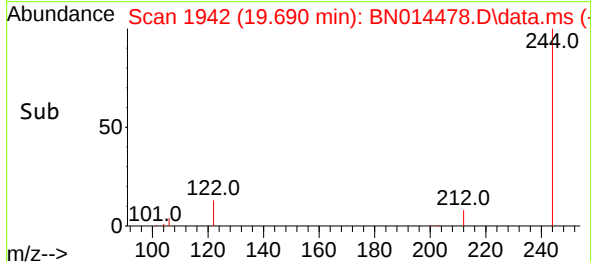

#32
Benzo(a)anthracene
Concen: 0.11 ng
RT: 21.229 min Scan# 2121
Delta R.T. -0.011 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30

Tgt Ion:228 Resp: 3527
Ion Ratio Lower Upper
228 100
226 28.6 20.8 31.2
229 20.9 16.1 24.1



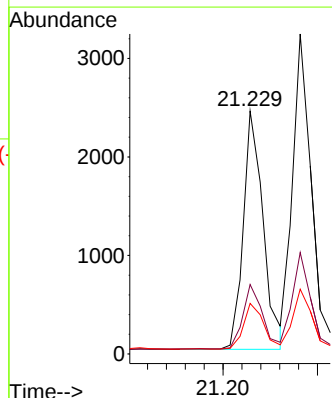
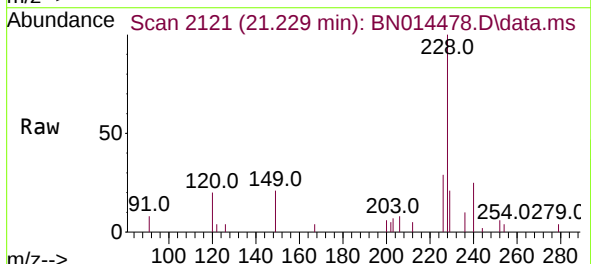




#33
Chrysene
Concen: 0.12 ng
RT: 21.282 min Scan# 2126
Delta R.T. -0.000 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021


Tgt Ion:228	Resp:	4374
Ion Ratio	Lower	Upper
228	100	
226	31.7	24.8 37.2
229	20.3	15.3 22.9

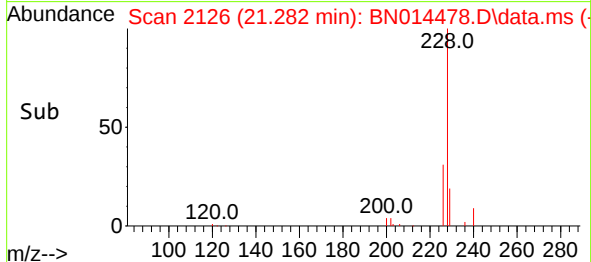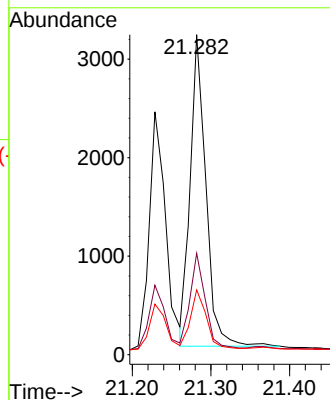

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.13 ng
RT: 21.176 min Scan# 2116
Delta R.T. -0.000 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30

Tgt Ion:149	Resp:	1802
Ion Ratio	Lower	Upper
149	100	
167	24.3	19.4 29.2
279	3.7	2.9 4.3


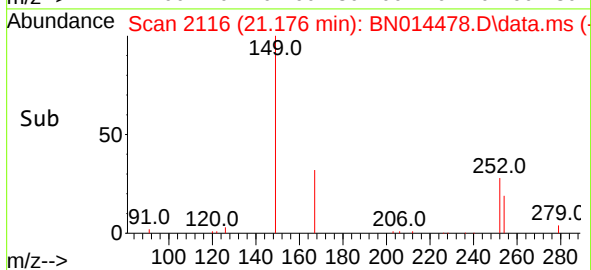
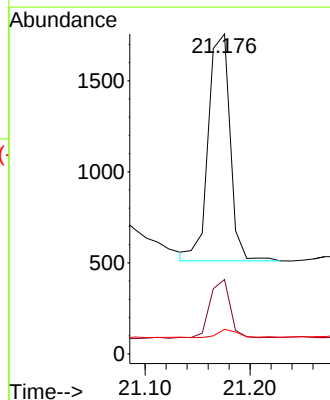
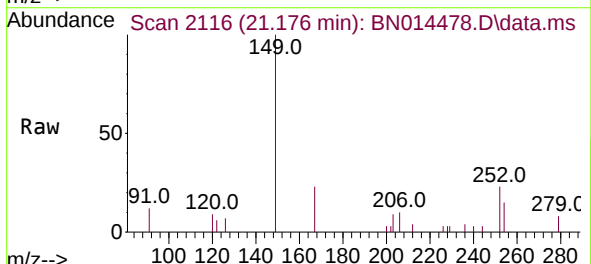




#35
 Perylene-d12
 Concen: 0.40 ng
 RT: 23.465 min Scan# 2541
 Delta R.T. -0.007 min
 Lab File: BN014478.D
 Acq: 28 Apr 2021 19:30




Instrument :
 BNA_N
 ClientSampleId :
 LOQ-WATER-02-QT1-2021


Tgt Ion:264	Resp:	10947
Ion Ratio	Lower	Upper
264	100	
260	24.7	19.8 29.6
265	51.2	31.6 47.4#

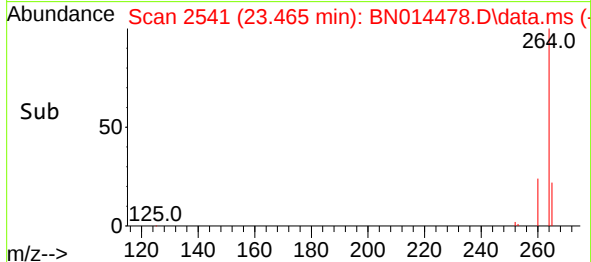

#36
 Indeno(1,2,3-cd)pyrene
 Concen: 0.12 ng
 RT: 25.693 min Scan# 3192
 Delta R.T. -0.004 min
 Lab File: BN014478.D
 Acq: 28 Apr 2021 19:30

Tgt Ion:276	Resp:	4988
Ion Ratio	Lower	Upper
276	100	
138	23.4	18.5 27.7
277	25.0	19.9 29.9




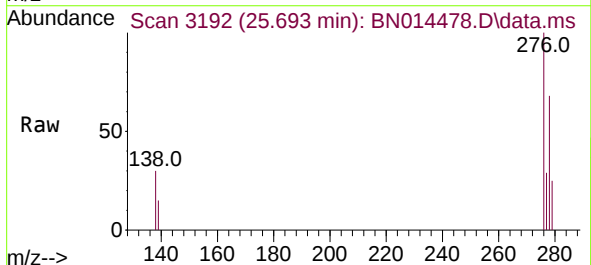




#37
Benzo(b)fluoranthene
Concen: 0.11 ng
RT: 22.801 min Scan# 2347
Delta R.T. -0.007 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021


Tgt Ion:252 Resp: 4463
Ion Ratio Lower Upper
252 100
253 32.6 19.3 28.9#
125 25.2 12.8 19.2#

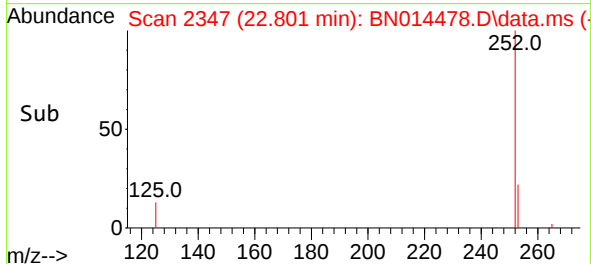

#38
Benzo(k)fluoranthene
Concen: 0.12 ng
RT: 22.846 min Scan# 2360
Delta R.T. -0.004 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30

Tgt Ion:252 Resp: 4635
Ion Ratio Lower Upper
252 100
253 33.6 19.3 28.9#
125 22.8 10.0 15.0#


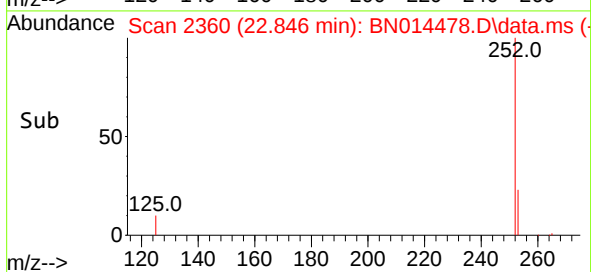






#39
Benzo(a)pyrene
Concen: 0.11 ng
RT: 23.369 min Scan# 2513
Delta R.T. -0.007 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021


Tgt Ion:252 Resp: 3881
Ion Ratio Lower Upper
252 100
253 39.5 21.0 31.6#
125 38.4 20.8 31.2#

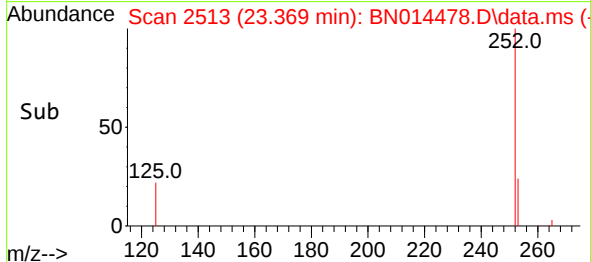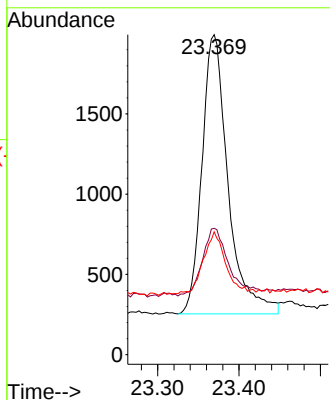

#40
Dibenzo(a,h)anthracene
Concen: 0.11 ng
RT: 25.704 min Scan# 3195
Delta R.T. -0.007 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30

Tgt Ion:278 Resp: 3975
Ion Ratio Lower Upper
278 100
139 22.5 14.3 21.5#
279 34.5 20.3 30.5#

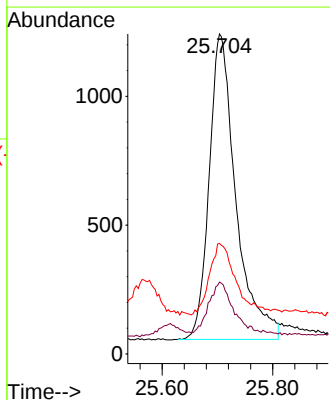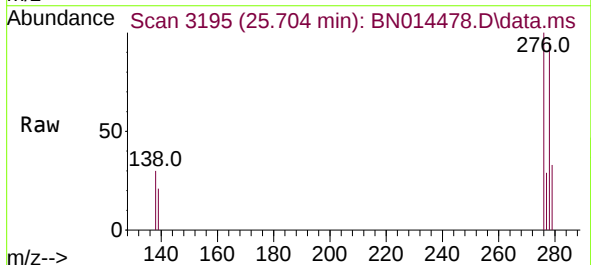

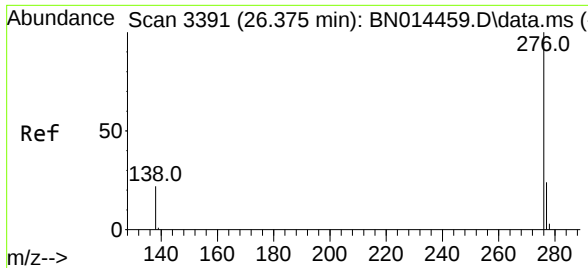

#41
Benzo(g,h,i)perylene
Concen: 0.13 ng
RT: 26.368 min Scan# 3389
Delta R.T. -0.007 min
Lab File: BN014478.D
Acq: 28 Apr 2021 19:30

Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT1-2021

Tgt Ion:	276	Resp:	4969
Ion Ratio	Lower	Upper	
276	100		
277	27.4	19.5	29.3
138	26.5	18.3	27.5

