
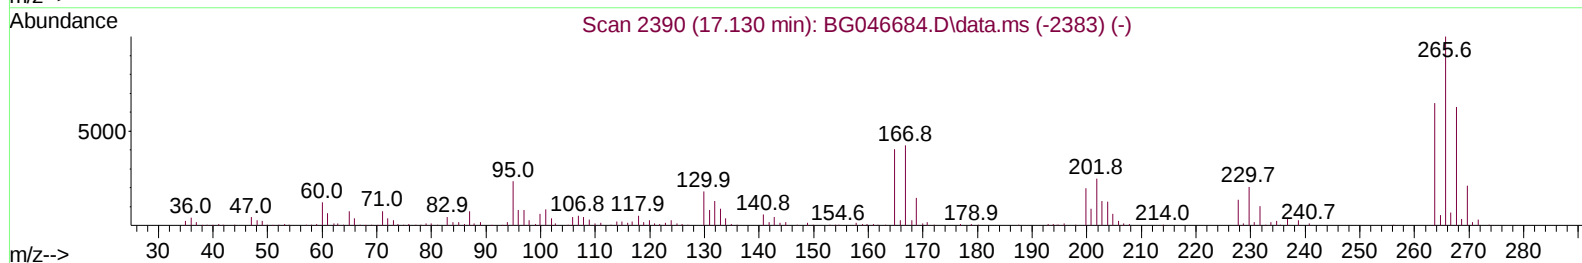
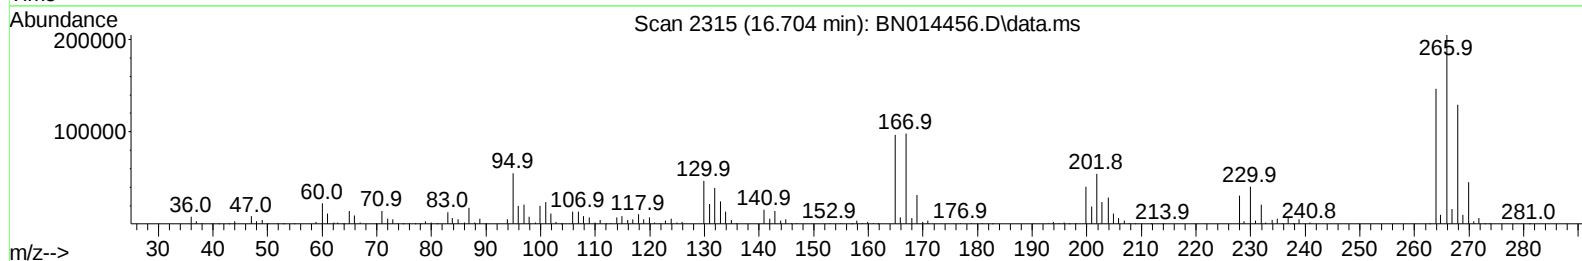


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042821\
Data File : BN014456.D
Acq On : 27 Apr 2021 14:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 27 15:22:48 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 09 09:55:03 2021
Response via : Initial Calibration

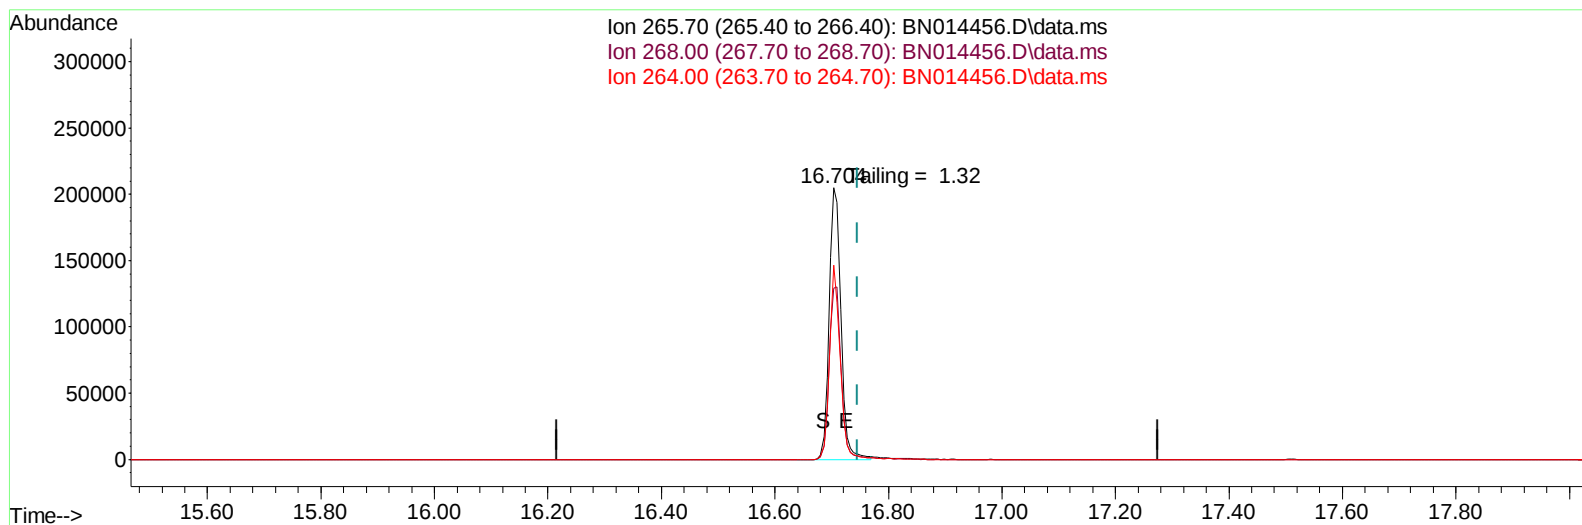




TIC: BN014456.D\data.ms

(70) Pentachlorophenol (C)**16.704min (-0.041) 23494.39 ng****response 300905**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.10
264.00	61.60	71.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042821\
Data File : BN014456.D
Acq On : 27 Apr 2021 14:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 27 15:22:48 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 09 09:55:03 2021
Response via : Initial Calibration

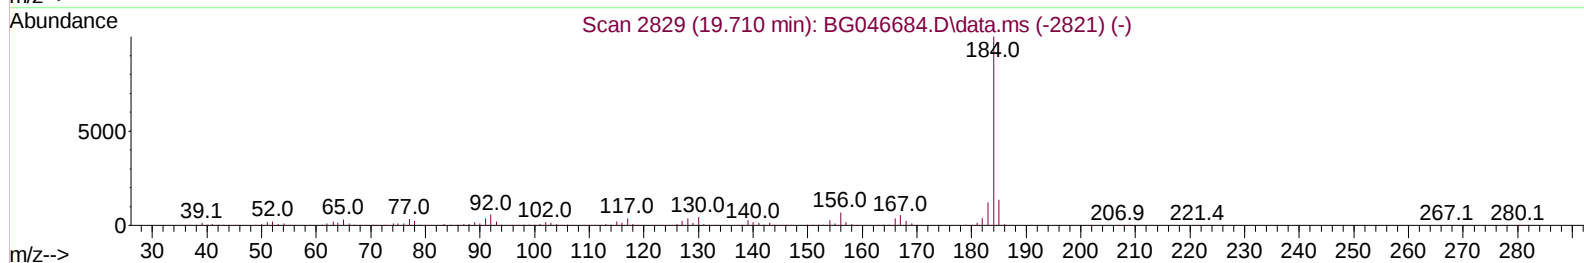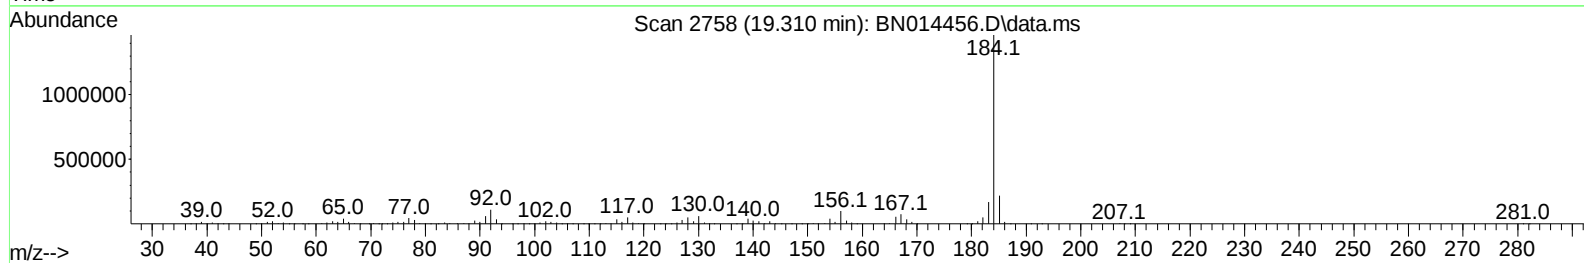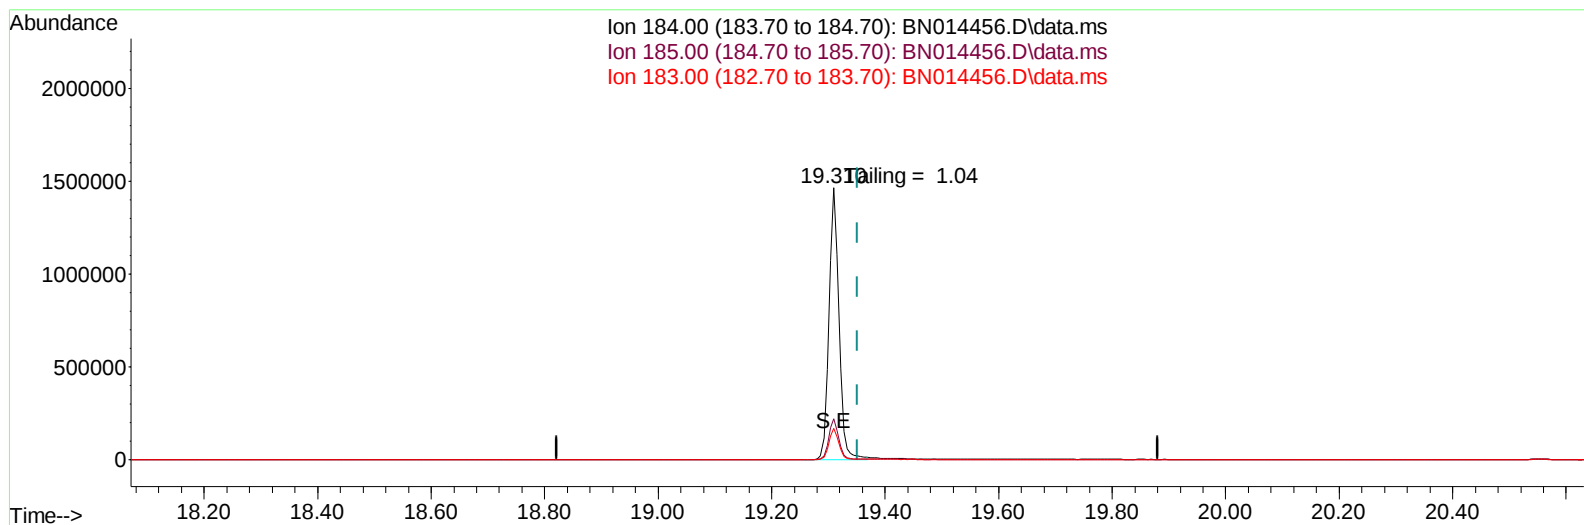

TIC: BN014456.D\data.ms

(77) Benzidine**19.310min (-0.041) 93822.41 ng****response 1804677**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.05
183.00	13.20	11.43
0.00	0.00	0.00