

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042821\
 Data File : BN014462.D
 Acq On : 27 Apr 2021 18:13
 Operator : CG/JU
 Sample : SSTDICC3.2
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2

Manual Integrations
 APPROVED

mohammad
 4/28/2021 11:03:14 AM

Quant Time: Apr 27 18:59:04 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 27 18:52:25 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.668	152	10313	0.40	ng	0.00
7) Naphthalene-d8	10.442	136	36025	0.40	ng	0.00
13) Acenaphthene-d10	14.308	164	19073	0.40	ng	0.00
19) Phenanthrene-d10	17.055	188	38536	0.40	ng	0.00
29) Chrysene-d12	21.250	240	41905	0.40	ng	0.00
35) Perylene-d12	23.469	264	33078	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.276	112	61673	2.91	ng	0.00
5) Phenol-d6	6.839	99	81211	3.12	ng	0.00
8) Nitrobenzene-d5	8.807	82	82267	2.72	ng	-0.01
11) 2-Methylnaphthalene-d10	12.040	152	175922	3.25	ng	0.00
14) 2,4,6-Tribromophenol	15.793	330	23885	3.90	ng	0.00
15) 2-Fluorobiphenyl	12.925	172	226344	3.00	ng	0.00
27) Fluoranthene-d10	19.089	212	354511	3.47	ng	0.00
31) Terphenyl-d14	19.695	244	270096	3.04	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.231	88	32872	2.61	ng	98
3) n-Nitrosodimethylamine	3.553	42	20288	3.09	ng	# 100
6) bis(2-Chloroethyl)ether	7.104	93	76111	2.98	ng	99
9) Naphthalene	10.492	128	282438	3.16	ng	99
10) Hexachlorobutadiene	10.784	225	53771	2.75	ng	# 99
12) 2-Methylnaphthalene	12.111	142	188661	3.23	ng	99
16) Acenaphthylene	14.016	152	263616	3.26	ng	100
17) Acenaphthene	14.371	154	174644	3.27	ng	96
18) Fluorene	15.361	166	217874	3.31	ng	99
20) 4,6-Dinitro-2-methylph...	15.437	198	16268	3.78	ng	# 18
21) 4-Bromophenyl-phenylether	16.252	248	67344	3.10	ng	96
22) Hexachlorobenzene	16.362	284	84747	2.84	ng	99
23) Atrazine	16.520	200	46219	3.68	ng	98
24) Pentachlorophenol	16.702	266	21778	3.95	ng	99
25) Phenanthrene	17.092	178	351071	3.24	ng	100
26) Anthracene	17.177	178	300200	3.54	ng	100
28) Fluoranthene	19.119	202	400101	3.46	ng	99
30) Pyrene	19.481	202	394427	3.16	ng	100
32) Benzo(a)anthracene	21.239	228	388967	3.51	ng	100
33) Chrysene	21.282	228	402427	3.08	ng	100
34) Bis(2-ethylhexyl)phtha...	21.176	149	151848	3.87	ng	95
36) Indeno(1,2,3-cd)pyrene	25.693	276	434407	3.15	ng	98
37) Benzo(b)fluoranthene	22.805	252	387035	3.18	ng	# 92
38) Benzo(k)fluoranthene	22.849	252	393851m	3.18	ng	
39) Benzo(a)pyrene	23.373	252	355983	3.45	ng	# 83
40) Dibenzo(a,h)anthracene	25.707	278	363056	3.17	ng	96
41) Benzo(g,h,i)perylene	26.371	276	370179	3.06	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042821\
Data File : BN014462.D
Acq On : 27 Apr 2021 18:13
Operator : CG/JU
Sample : SSTDICC3.2
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Manual Integrations
APPROVED

mohammad
4/28/2021 11:03:14 AM

Quant Time: Apr 27 18:59:04 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 27 18:52:25 2021
Response via : Initial Calibration

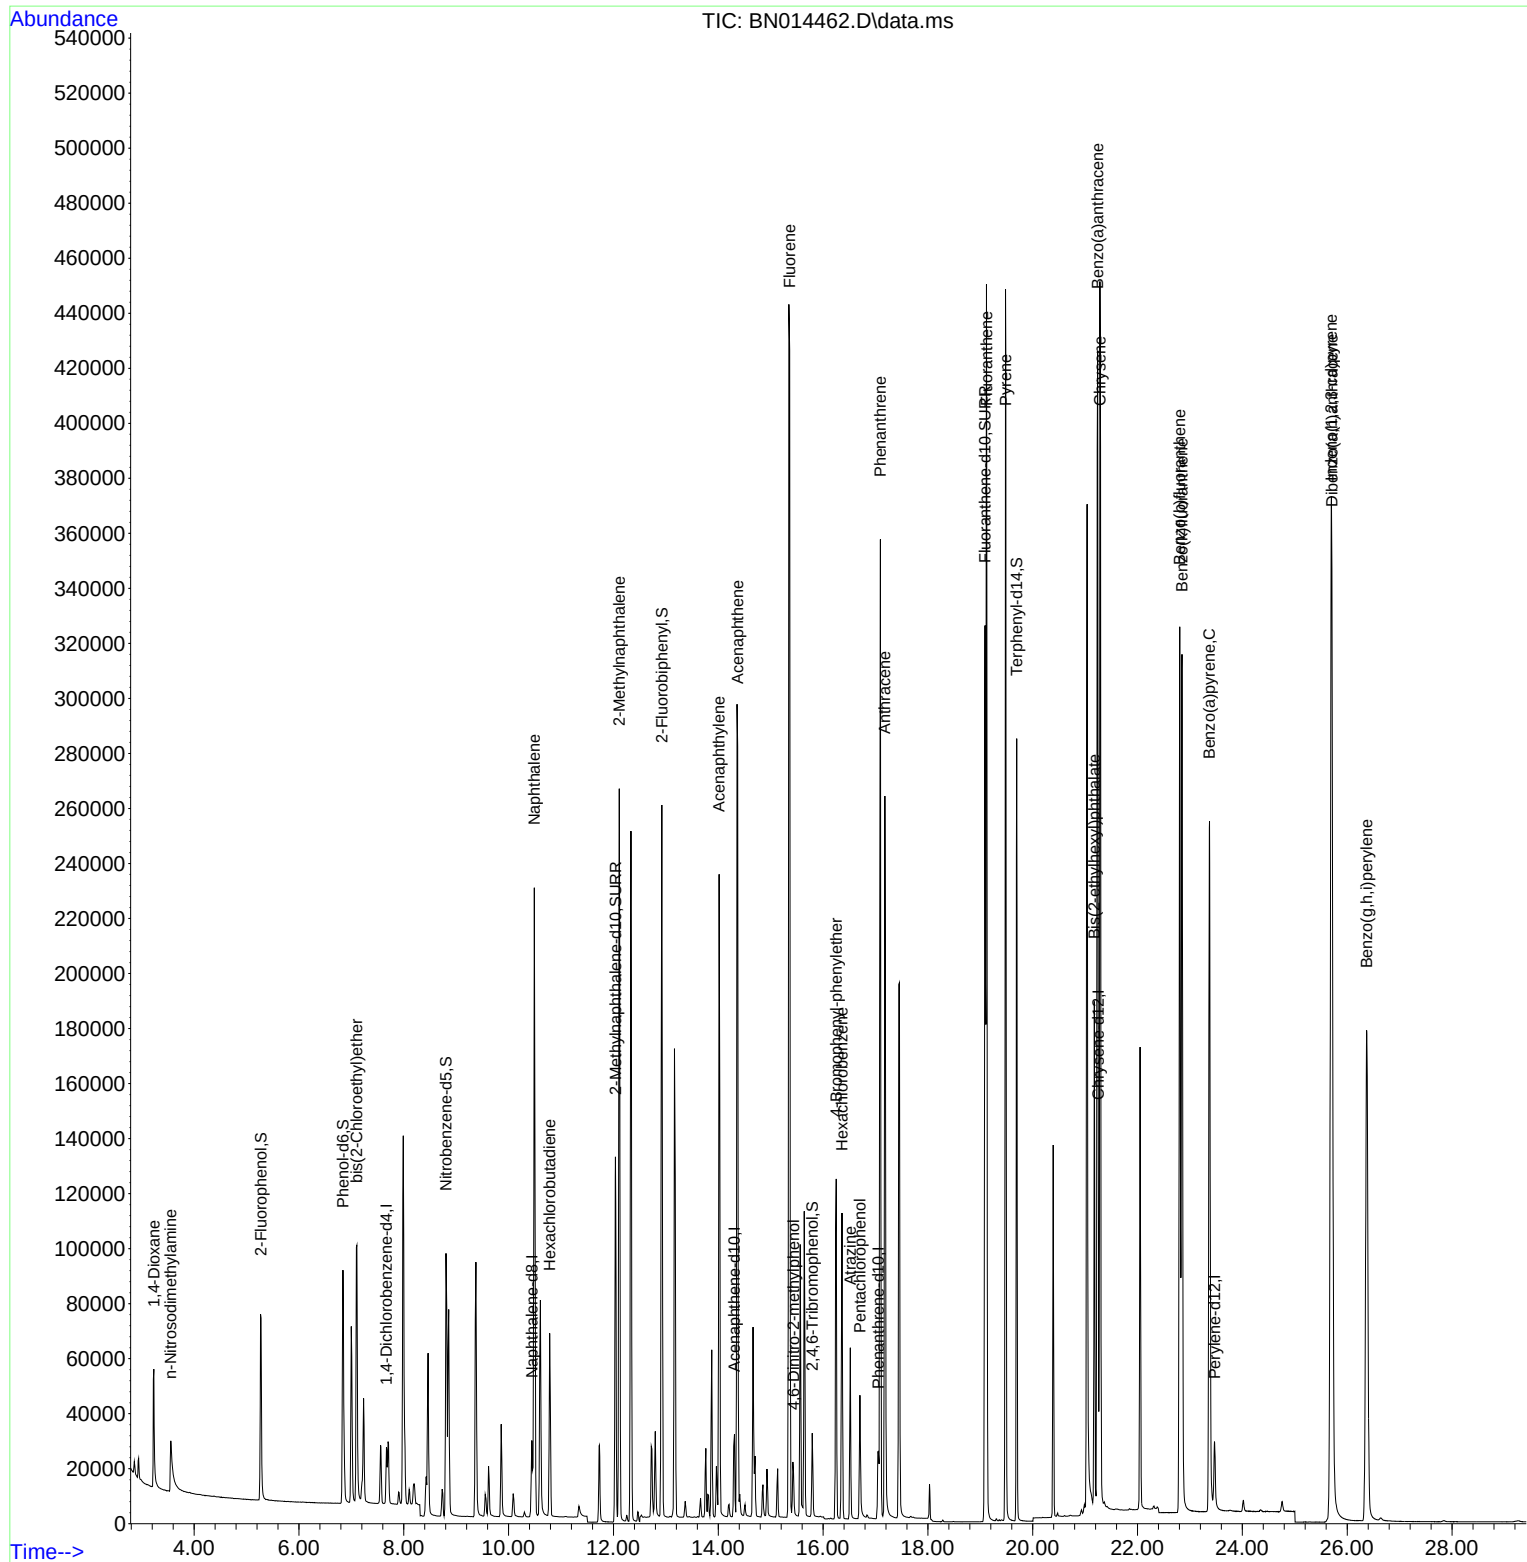







#1
1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.668 min Scan# 607
Delta R.T. -0.008 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

Tgt Ion: 152 Resp: 10313
Ion Ratio Lower Upper
152 100
150 160.4 121.2 181.8
115 60.8 46.0 69.0

Instrument :
BNA_N
ClientSampled :
SSTDICC3.2




Manual Integrations
APPROVED


mohammad
4/28/2021 11:03:14 AM

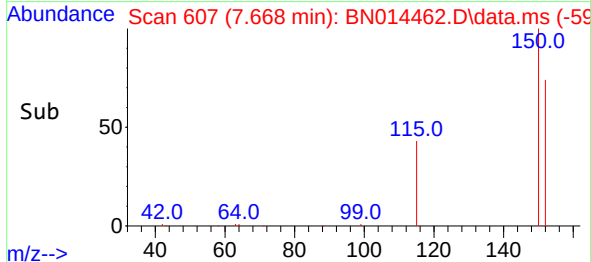

#2
1,4-Dioxane
Concen: 2.61 ng
RT: 3.231 min Scan# 56
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

Tgt Ion: 88 Resp: 32872
Ion Ratio Lower Upper
88 100
58 65.2 53.1 79.7
43 23.8 20.3 30.5

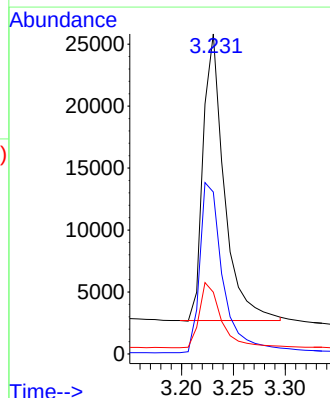



#3
n-Nitrosodimethylamine
Concen: 3.09 ng
RT: 3.553 min Scan# 96
Delta R.T. -0.040 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13





Tgt Ion: 42 Resp: 20288

Ion	Ratio	Lower	Upper
42	100		
74	155.9	124.7	187.1
44	6.4	0.0	0.0#

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Manual Integrations
APPROVED




mohammad
4/28/2021 11:03:14 AM

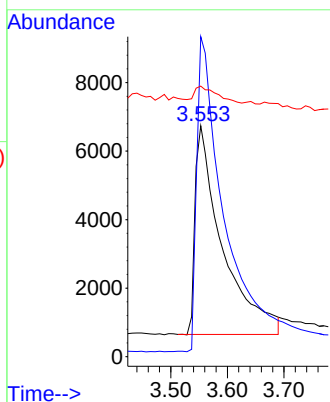


#4
2-Fluorophenol
Concen: 2.91 ng
RT: 5.276 min Scan# 310
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

Tgt Ion: 112 Resp: 61673

Ion	Ratio	Lower	Upper
112	100		
64	51.9	41.4	62.2
63	27.0	21.8	32.8









#5
Phenol-d6
Concen: 3.12 ng
RT: 6.839 min Scan# 504
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

Tgt Ion: 99 Resp: 81211
Ion Ratio Lower Upper
99 100
42 16.9 13.8 20.6
71 31.9 25.5 38.3

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2




Manual Integrations
APPROVED


mohammad
4/28/2021 11:03:14 AM

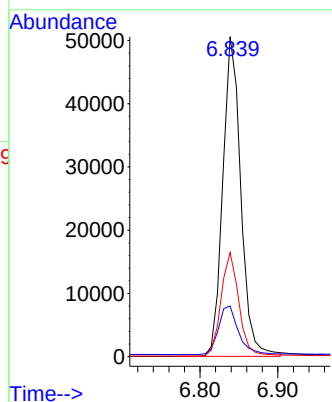

#6
bis(2-Chloroethyl)ether
Concen: 2.98 ng
RT: 7.104 min Scan# 537
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13


Tgt Ion: 93 Resp: 76111
Ion Ratio Lower Upper
93 100
63 71.4 56.7 85.1
95 33.5 26.3 39.5

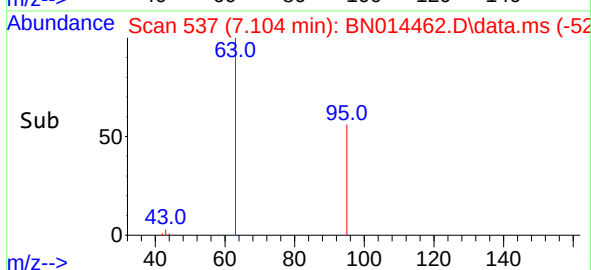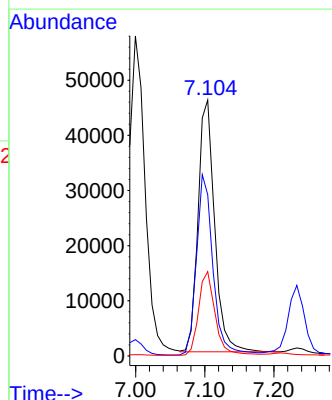



#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.442 min Scan# 855
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13



Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2




Tgt Ion:	136	Resp:	36025
Ion	Ratio	Lower	Upper
136	100		
137	11.1	9.0	13.4
54	6.3	5.7	8.5
68	6.0	5.2	7.8

Manual Integrations
APPROVED



mohammad
4/28/2021 11:03:14 AM




#8
Nitrobenzene-d5
Concen: 2.72 ng
RT: 8.807 min Scan# 726
Delta R.T. -0.013 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13




Tgt Ion:	82	Resp:	82267
Ion	Ratio	Lower	Upper
82	100		
128	34.7	38.5	57.7#
54	46.0	32.1	48.1

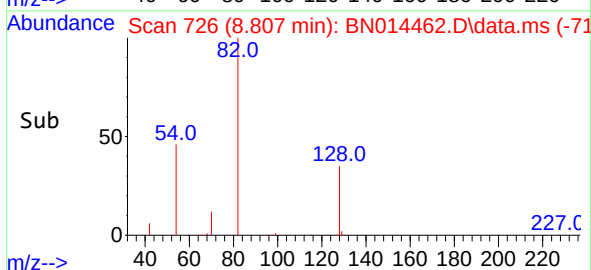

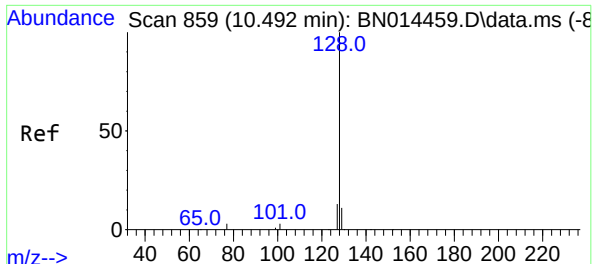

#9
Naphthalene
Concen: 3.16 ng
RT: 10.492 min Scan# 859
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

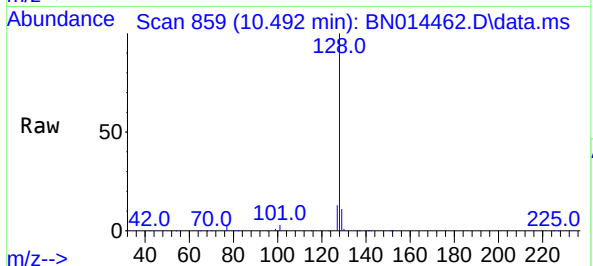


Tgt Ion:128 Resp: 282438
Ion Ratio Lower Upper
128 100
129 10.9 9.0 13.4
127 12.8 10.5 15.7

Manual Integrations
APPROVED



mohammad
4/28/2021 11:03:14 AM

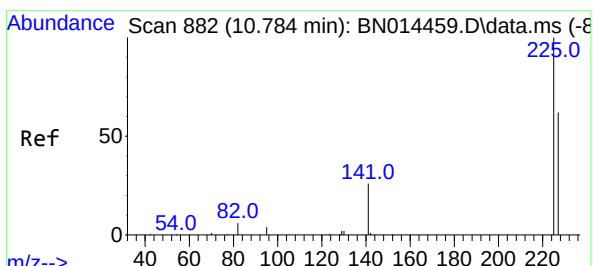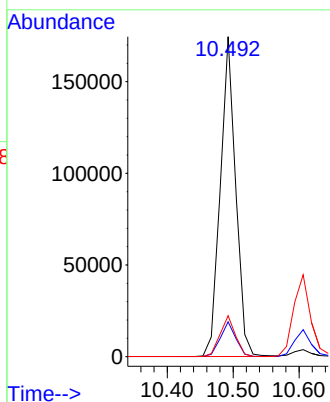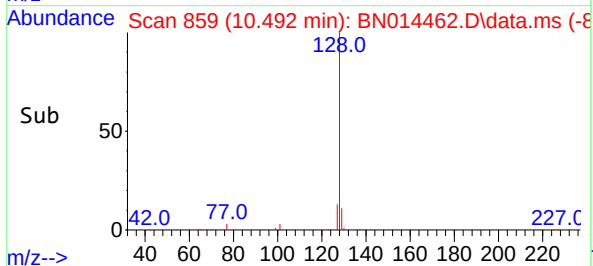


#10
Hexachlorobutadiene
Concen: 2.75 ng
RT: 10.784 min Scan# 882
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

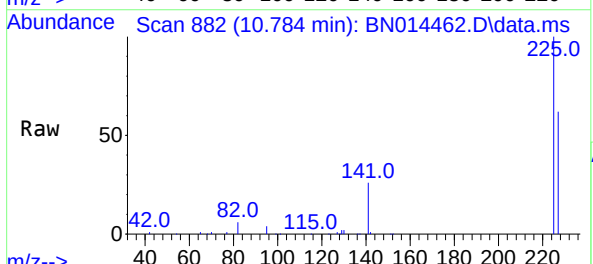

Tgt Ion:225 Resp: 53771
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.9 51.5 77.3

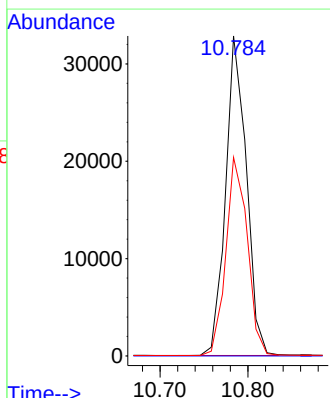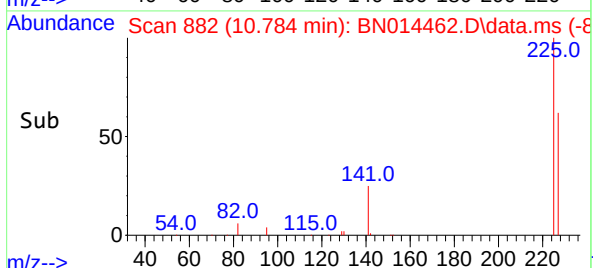







#11
2-Methylnaphthalene-d10
Concen: 3.25 ng
RT: 12.040 min Scan# 1059
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

Tgt Ion:152 Resp: 175922
Ion Ratio Lower Upper
152 100
151 20.0 16.2 24.4

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2




Manual Integrations
APPROVED


mohammad
4/28/2021 11:03:14 AM

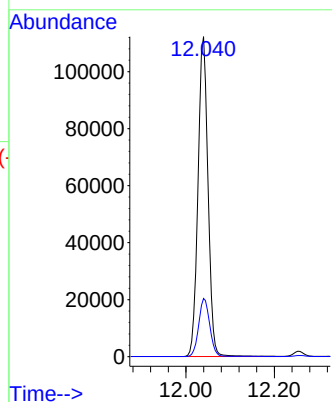

#12
2-Methylnaphthalene
Concen: 3.23 ng
RT: 12.111 min Scan# 1075
Delta R.T. -0.005 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13


Tgt Ion:142 Resp: 188661
Ion Ratio Lower Upper
142 100
141 88.1 69.6 104.4
115 33.9 27.0 40.6

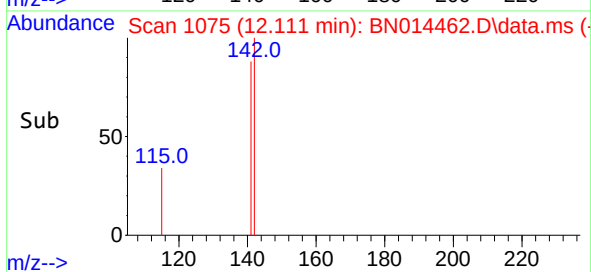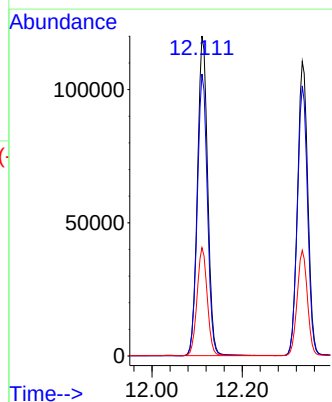

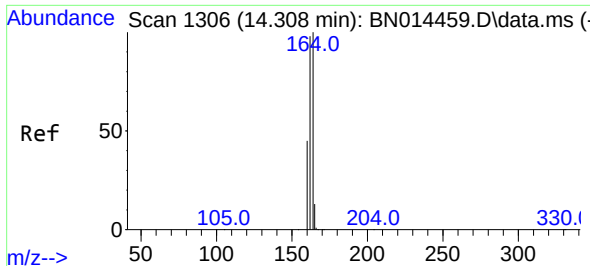

#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.308 min Scan# 1306
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

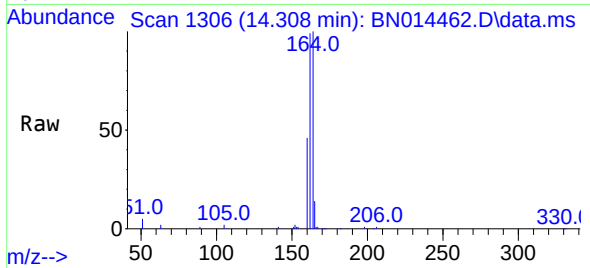


Tgt Ion:164 Resp: 19073
Ion Ratio Lower Upper
164 100
162 98.5 78.3 117.5
160 45.7 36.6 54.8

Manual Integrations
APPROVED



mohammad
4/28/2021 11:03:14 AM

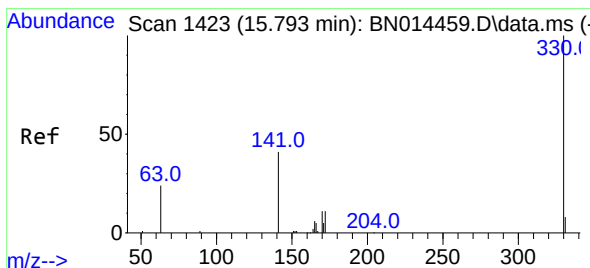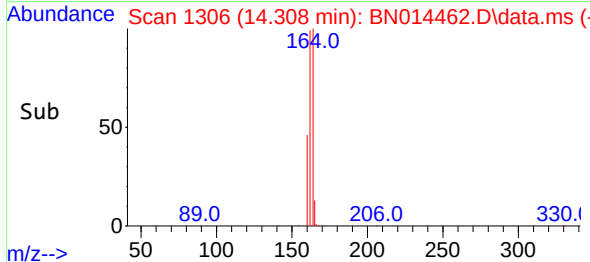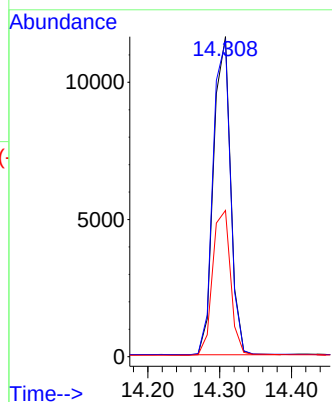


#14
2,4,6-Tribromophenol
Concen: 3.90 ng
RT: 15.793 min Scan# 1423
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

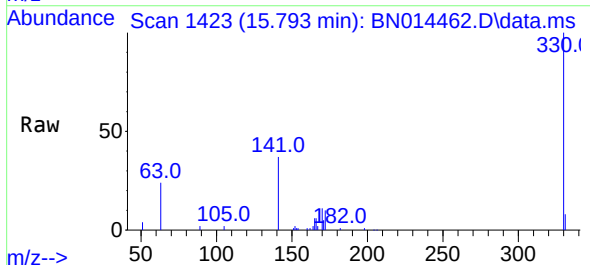

Tgt Ion:330 Resp: 23885
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 33.8 29.3 43.9

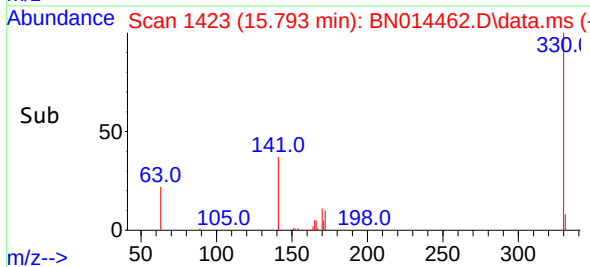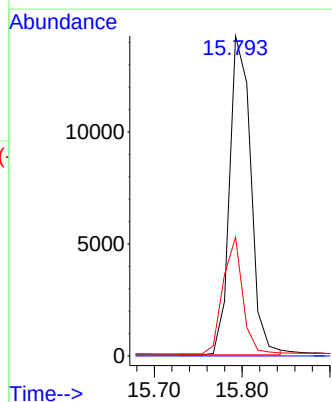



#15
2-Fluorobiphenyl
Concen: 3.00 ng
RT: 12.925 min Scan# 1197
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13





Tgt Ion:172 Resp: 226344

Ion	Ratio	Lower	Upper
172	100		
171	33.7	27.0	40.4
170	22.3	18.2	27.4

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Manual Integrations
APPROVED




mohammad
4/28/2021 11:03:14 AM




#16
Acenaphthylene
Concen: 3.26 ng
RT: 14.016 min Scan# 1283
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

Tgt Ion:152 Resp: 263616


Ion	Ratio	Lower	Upper
152	100		
151	19.3	15.4	23.2
153	13.1	10.4	15.6

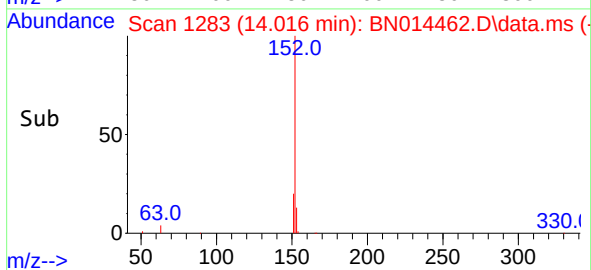



#17
Acenaphthene
Concen: 3.27 ng
RT: 14.371 min Scan# 1311
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2




Tgt Ion:154 Resp: 174644
Ion Ratio Lower Upper
154 100
153 109.6 90.5 135.7
152 55.3 47.2 70.8

Manual Integrations
APPROVED



mohammad
4/28/2021 11:03:14 AM

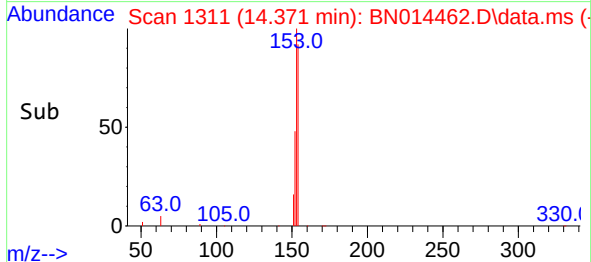


#18
Fluorene
Concen: 3.31 ng
RT: 15.361 min Scan# 1389
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13




Tgt Ion:166 Resp: 217874
Ion Ratio Lower Upper
166 100
165 97.1 78.1 117.1
167 13.5 11.0 16.6

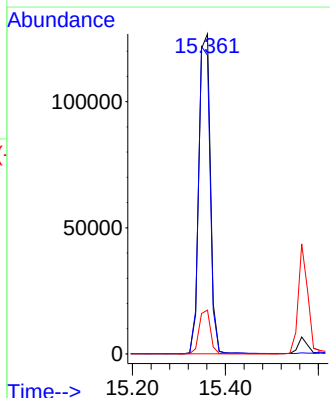

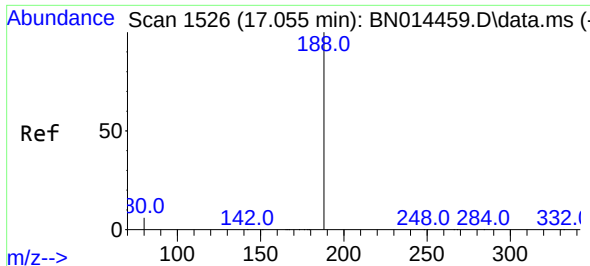

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.055 min Scan# 1526
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13



Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

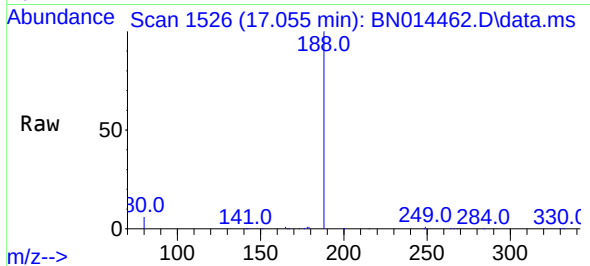


Tgt Ion:188 Resp: 38536
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 6.3 5.4 8.2

Manual Integrations
APPROVED



mohammad
4/28/2021 11:03:14 AM

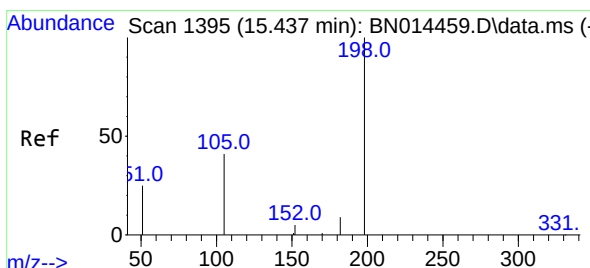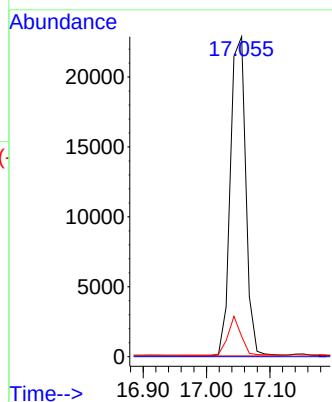


#20
4,6-Dinitro-2-methylphenol
Concen: 3.78 ng
RT: 15.437 min Scan# 1395
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

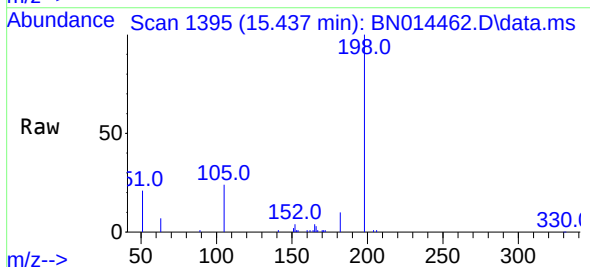


Tgt Ion:198 Resp: 16268
Ion Ratio Lower Upper
198 100
51 21.0 104.5 156.7#
105 23.8 62.2 93.2#


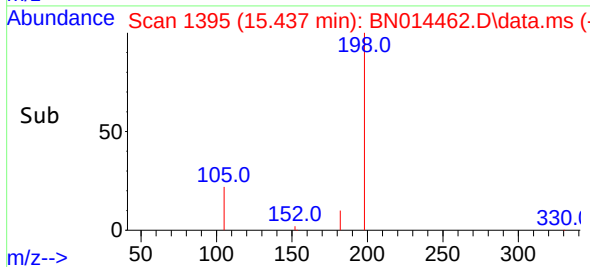
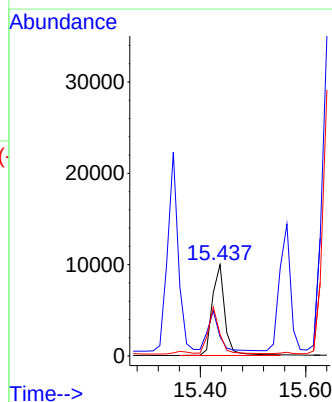





#21
4-Bromophenyl-phenylether
Concen: 3.10 ng
RT: 16.252 min Scan# 1460
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13





Tgt Ion:248 Resp: 67344
Ion Ratio Lower Upper
248 100
250 103.6 81.8 122.6
141 36.0 34.2 51.2



#22
Hexachlorobenzene
Concen: 2.84 ng
RT: 16.362 min Scan# 1469
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13




Tgt Ion:284 Resp: 84747
Ion Ratio Lower Upper
284 100
142 33.4 27.2 40.8
249 29.0 23.4 35.2

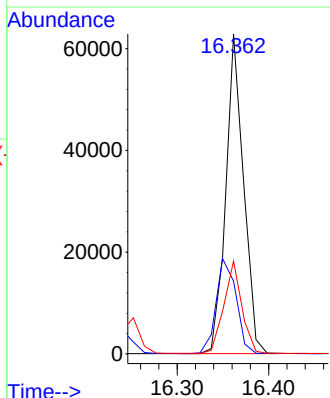


Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Manual Integrations
APPROVED




mohammad
4/28/2021 11:03:14 AM




#23
Atrazine
Concen: 3.68 ng
RT: 16.520 min Scan# 1482
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13





Tgt Ion:200 Resp: 46219
Ion Ratio Lower Upper
200 100
173 23.9 20.8 31.2
215 48.7 39.3 58.9



#24
Pentachlorophenol
Concen: 3.95 ng
RT: 16.702 min Scan# 1497
Delta R.T. -0.012 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13




Tgt Ion:266 Resp: 21778
Ion Ratio Lower Upper
266 100
264 62.7 49.9 74.9
268 63.6 51.6 77.4

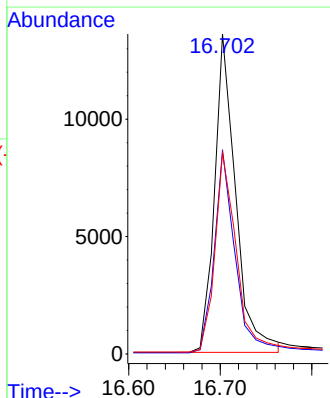

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Manual Integrations
APPROVED

mohammad
4/28/2021 11:03:14 AM







#25
Phenanthrene
Concen: 3.24 ng
RT: 17.092 min Scan# 1529
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

Tgt Ion:178 Resp: 351071
Ion Ratio Lower Upper
178 100
176 18.9 15.1 22.7
179 15.3 12.2 18.4

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2




Manual Integrations
APPROVED


mohammad
4/28/2021 11:03:14 AM

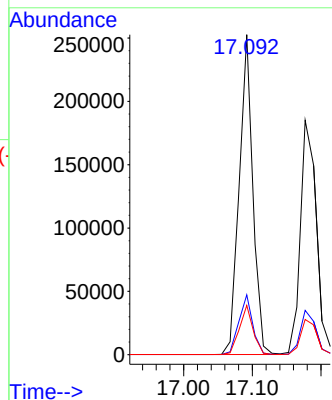

#26
Anthracene
Concen: 3.54 ng
RT: 17.177 min Scan# 1536
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

Tgt Ion:178 Resp: 300200
Ion Ratio Lower Upper
178 100
176 18.4 14.6 22.0
179 15.3 12.0 18.0

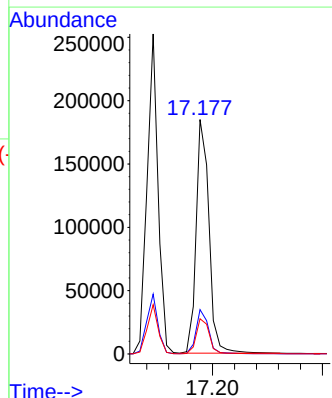







#27
Fluoranthene-d10
Concen: 3.47 ng
RT: 19.089 min Scan# 1821
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

Tgt Ion:212 Resp: 354511
Ion Ratio Lower Upper
212 100
106 12.7 10.2 15.4
104 7.0 5.6 8.4

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2




Manual Integrations
APPROVED


mohammad
4/28/2021 11:03:14 AM

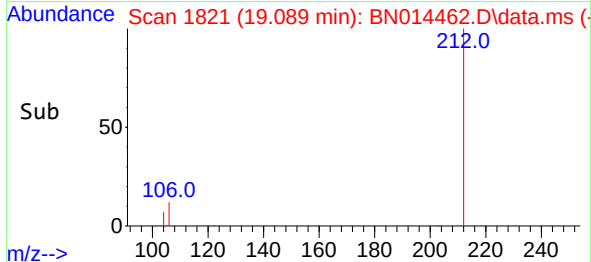


#28
Fluoranthene
Concen: 3.46 ng
RT: 19.119 min Scan# 1827
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

Tgt Ion:202 Resp: 400101
Ion Ratio Lower Upper
202 100
101 10.7 8.5 12.7
203 17.4 13.7 20.5

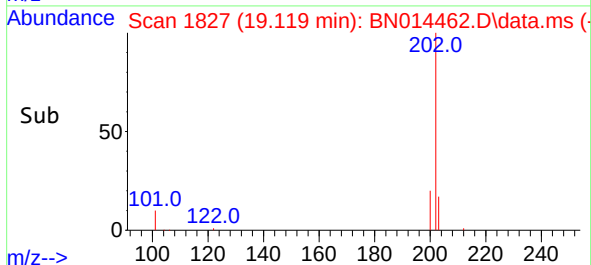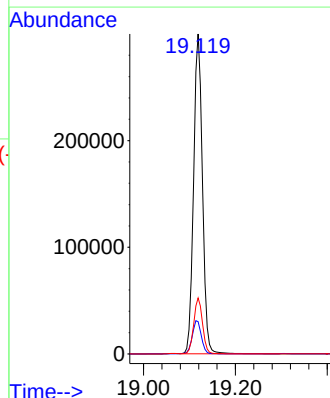
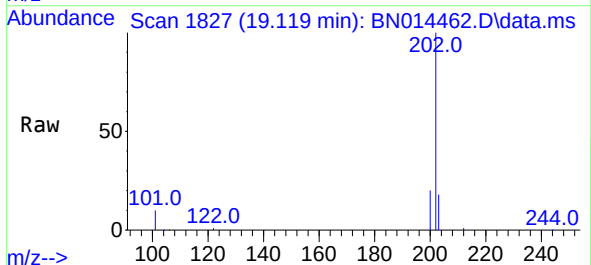


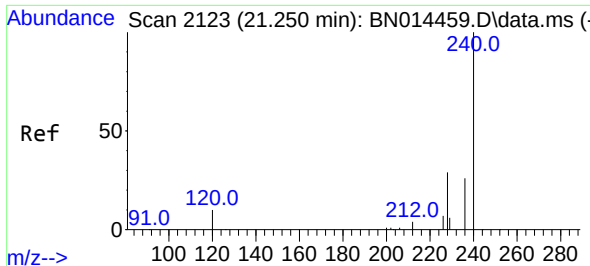

#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.250 min Scan# 2123
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

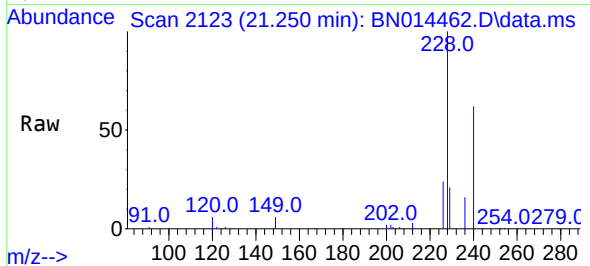


Tgt Ion:240 Resp: 41905
Ion Ratio Lower Upper
240 100
120 9.5 9.0 13.6
236 26.4 21.4 32.0

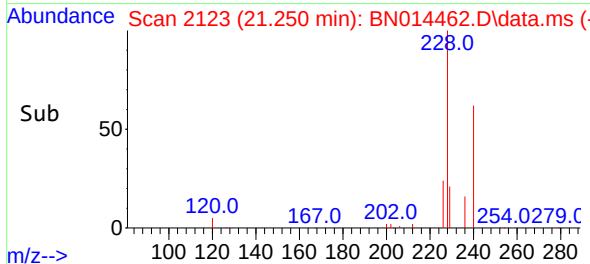


Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Manual Integrations
APPROVED



mohammad
4/28/2021 11:03:14 AM

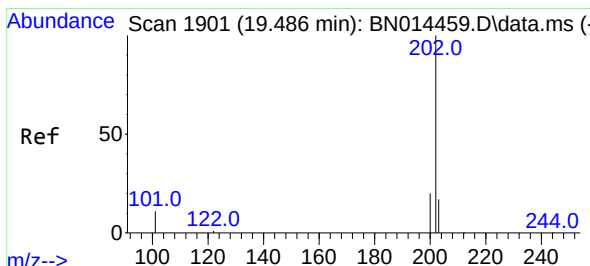


#30
Pyrene
Concen: 3.16 ng
RT: 19.481 min Scan# 1900
Delta R.T. -0.005 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

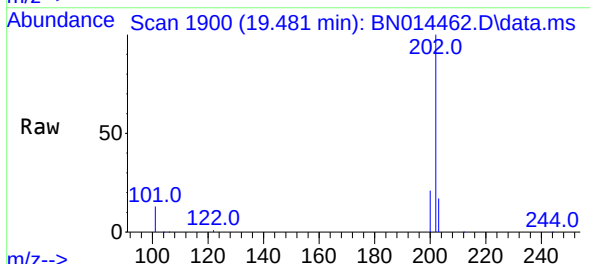


Tgt Ion:202 Resp: 394427
Ion Ratio Lower Upper
202 100
200 20.5 16.4 24.6
203 17.4 13.9 20.9


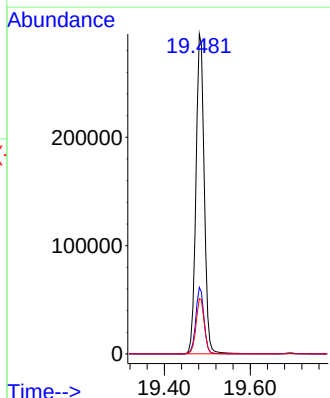
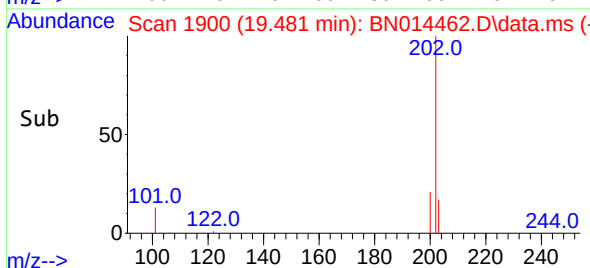


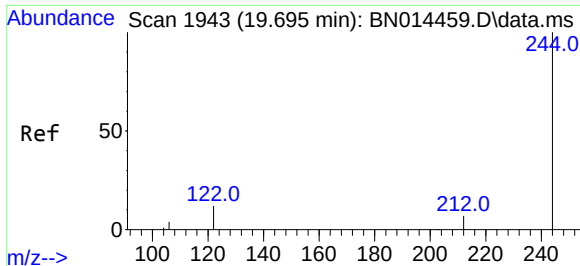


#31
Terphenyl-d14
Concen: 3.04 ng
RT: 19.695 min Scan# 1943
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

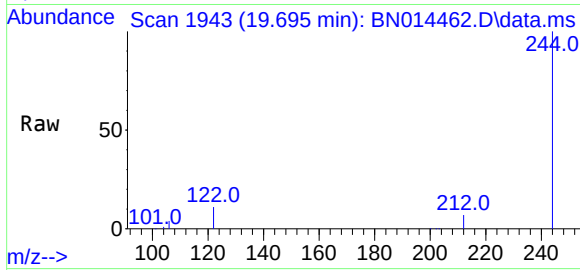



Tgt Ion:244 Resp: 270096
Ion Ratio Lower Upper
244 100
212 7.4 6.2 9.2
122 11.5 9.8 14.8

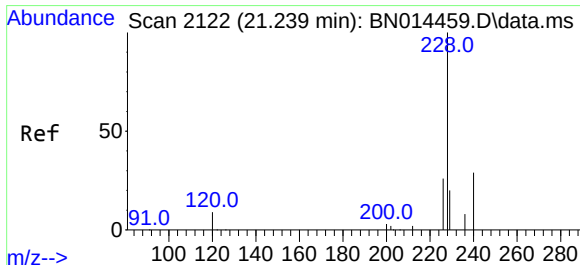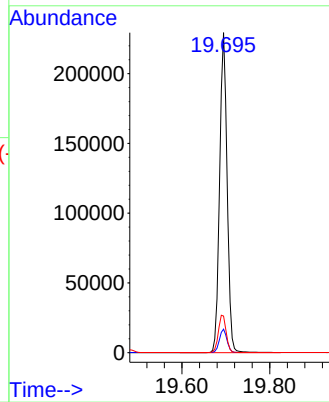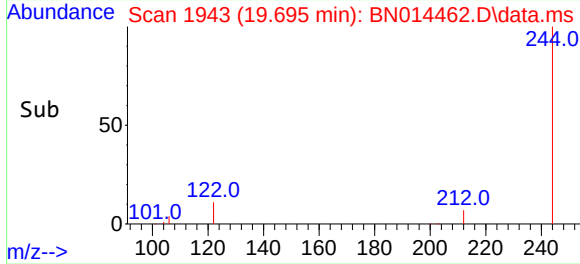

#32
Benzo(a)anthracene
Concen: 3.51 ng
RT: 21.239 min Scan# 2122
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

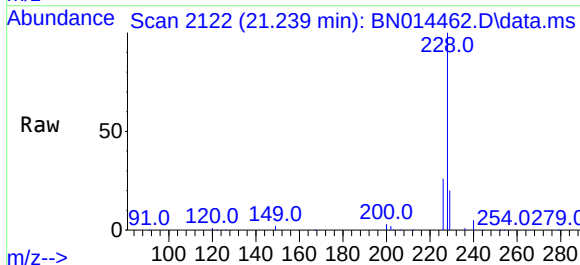


Tgt Ion:228 Resp: 388967
Ion Ratio Lower Upper
228 100
226 25.6 20.8 31.2
229 20.1 16.1 24.1

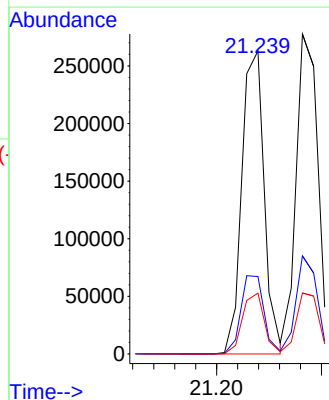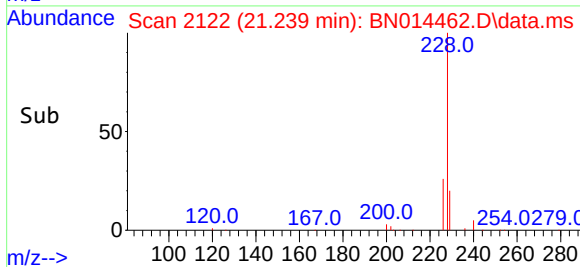

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Manual Integrations
APPROVED

mohammad
4/28/2021 11:03:14 AM

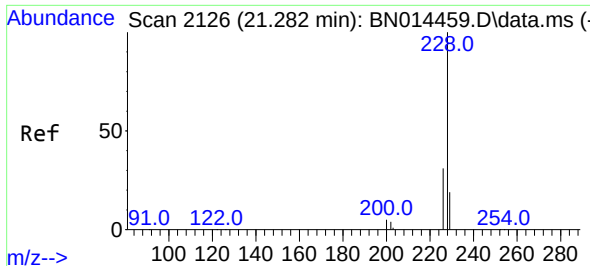





#33
Chrysene
Concen: 3.08 ng
RT: 21.282 min Scan# 2126
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

Tgt Ion:228 Resp: 402427
Ion Ratio Lower Upper
228 100
226 30.7 24.8 37.2
229 19.0 15.3 22.9

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2




Manual Integrations
APPROVED


mohammad
4/28/2021 11:03:14 AM

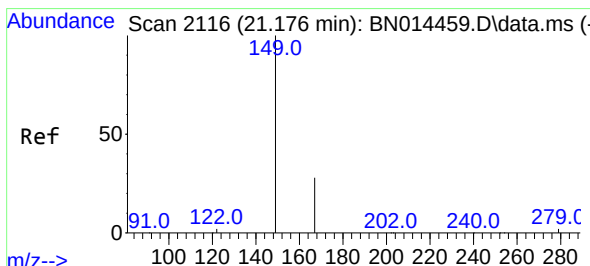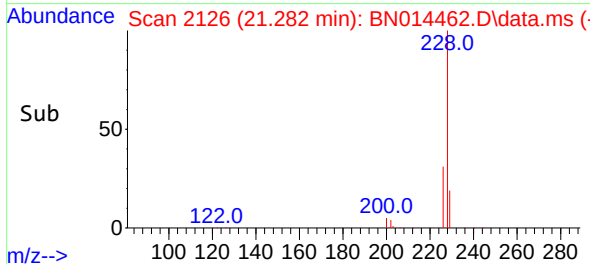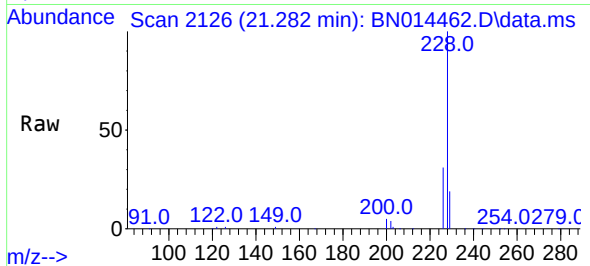


#34
Bis(2-ethylhexyl)phthalate
Concen: 3.87 ng
RT: 21.176 min Scan# 2116
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

Tgt Ion:149 Resp: 151848
Ion Ratio Lower Upper
149 100
167 27.1 19.4 29.2
279 3.6 2.9 4.3

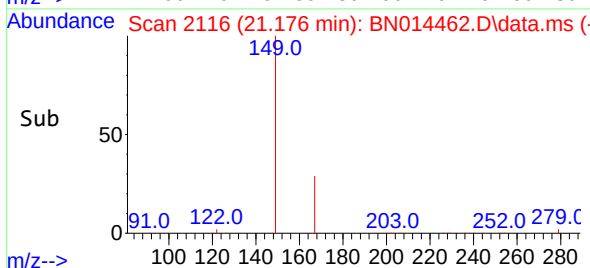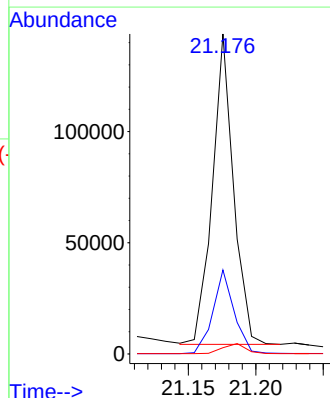
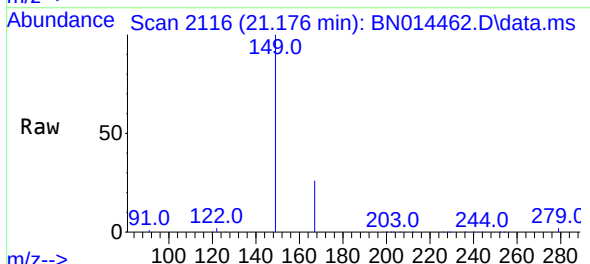


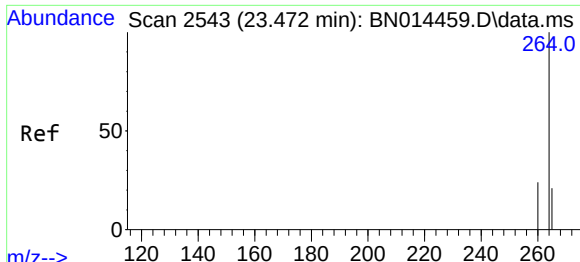

#35
Perylene-d12
Concen: 0.40 ng
RT: 23.469 min Scan# 2542
Delta R.T. -0.004 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

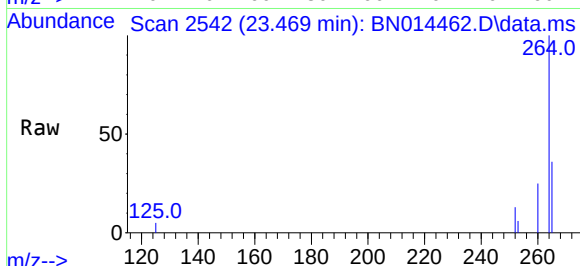


Tgt Ion:264 Resp: 33078
Ion Ratio Lower Upper
264 100
260 24.9 19.8 29.6
265 36.3 31.6 47.4

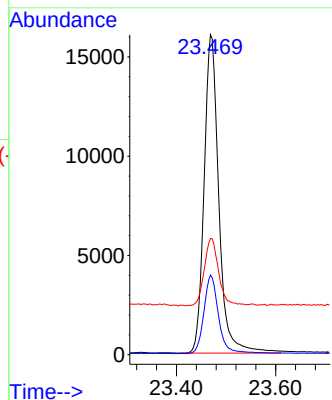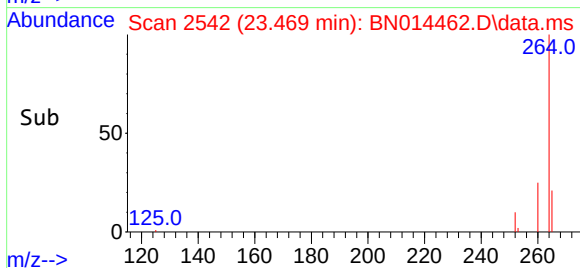


Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Manual Integrations
APPROVED



mohammad
4/28/2021 11:03:14 AM

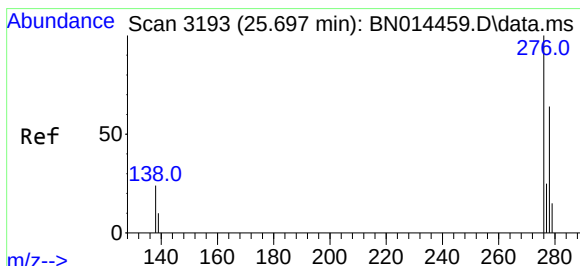


#36
Indeno(1,2,3-cd)pyrene
Concen: 3.15 ng
RT: 25.693 min Scan# 3192
Delta R.T. -0.004 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

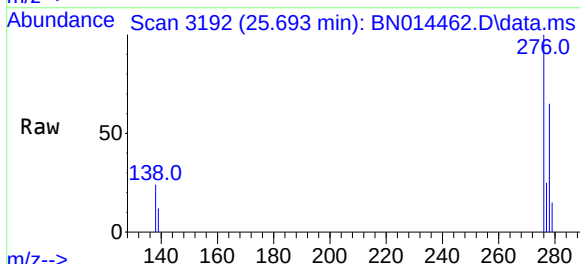


Tgt Ion:276 Resp: 434407
Ion Ratio Lower Upper
276 100
138 25.2 18.5 27.7
277 24.9 19.9 29.9


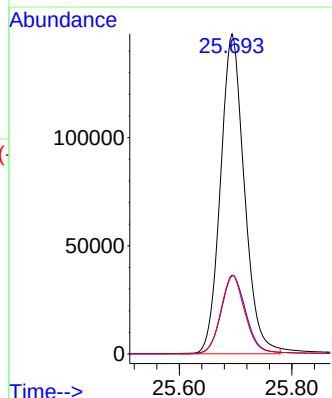
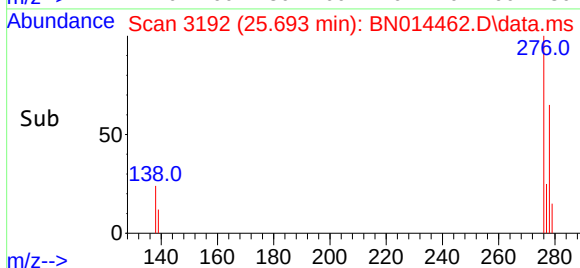





#37
Benzo(b)fluoranthene
Concen: 3.18 ng
RT: 22.805 min Scan# 2348
Delta R.T. -0.004 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13





Tgt Ion:252 Resp: 387035
Ion Ratio Lower Upper
252 100
253 21.9 19.3 28.9
125 10.4 12.8 19.2#

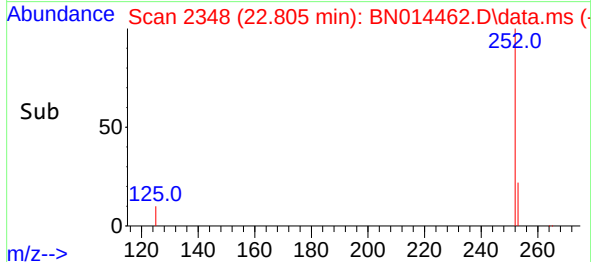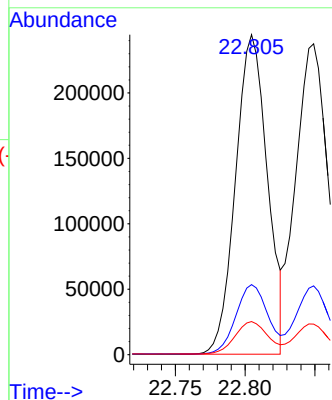

#38
Benzo(k)fluoranthene
Concen: 3.18 ng m
RT: 22.849 min Scan# 2361
Delta R.T. -0.000 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

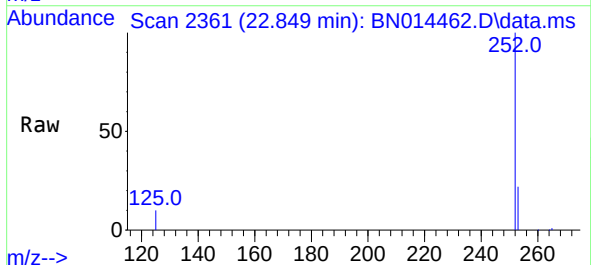


Tgt Ion:252 Resp: 393851
Ion Ratio Lower Upper
252 100
253 22.1 19.3 28.9
125 9.8 10.0 15.0#

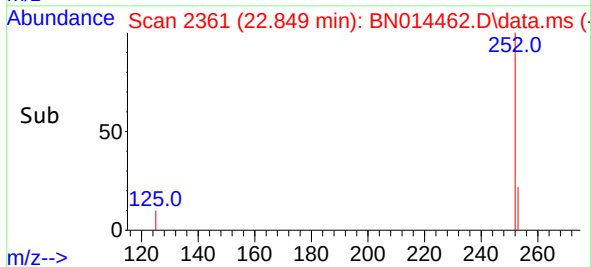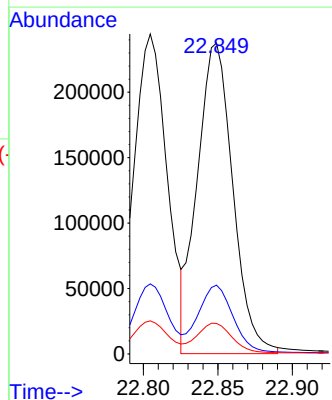


Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Manual Integrations
APPROVED




mohammad
4/28/2021 11:03:14 AM




#39
Benzo(a)pyrene
Concen: 3.45 ng
RT: 23.373 min Scan# 2514
Delta R.T. -0.004 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13





Tgt Ion:252 Resp: 355983
Ion Ratio Lower Upper
252 100
253 22.3 21.0 31.6
125 12.5 20.8 31.2#

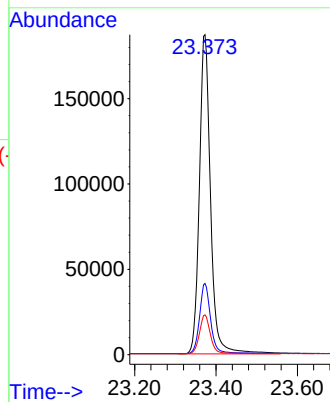

#40
Dibenzo(a,h)anthracene
Concen: 3.17 ng
RT: 25.707 min Scan# 3196
Delta R.T. -0.004 min
Lab File: BN014462.D
Acq: 27 Apr 2021 18:13

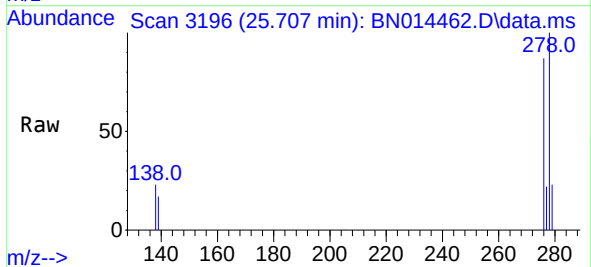


Tgt Ion:278 Resp: 363056
Ion Ratio Lower Upper
278 100
139 16.5 14.3 21.5
279 23.3 20.3 30.5

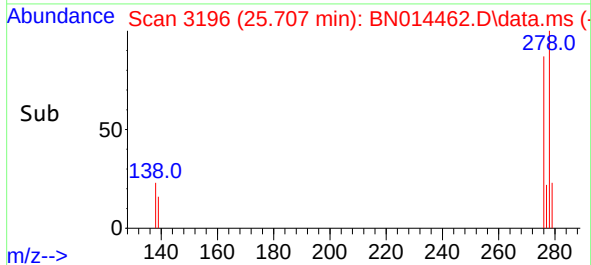

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Manual Integrations
APPROVED

mohammad
4/28/2021 11:03:14 AM

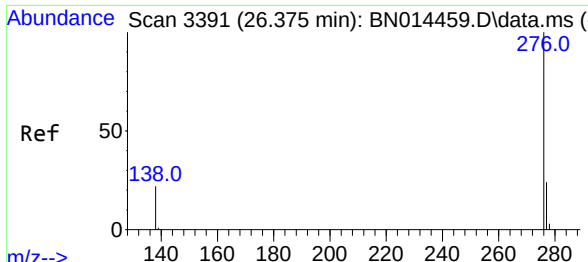

#41
 Benzo(g,h,i)perylene
 Concen: 3.06 ng
 RT: 26.371 min Scan# 3390
 Delta R.T. -0.004 min
 Lab File: BN014462.D
 Acq: 27 Apr 2021 18:13

Tgt Ion:	276	Resp:	370179
Ion Ratio	Lower	Upper	
276	100		
277	23.7	19.5	29.3
138	21.8	18.3	27.5

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2

Manual Integrations
 APPROVED

mohammad
 4/28/2021 11:03:14 AM

