

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042821\
 Data File : BN014476.D
 Acq On : 28 Apr 2021 18:18
 Operator : CG/JU
 Sample : M1458-07
 Misc : LOD-MDL-WTR-0.1PPM
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2021

Quant Time: Apr 29 02:07:09 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 27 19:23:29 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.668	152	4807	0.40	ng	0.00
7) Naphthalene-d8	10.442	136	16275	0.40	ng	0.00
13) Acenaphthene-d10	14.308	164	7383	0.40	ng	0.00
19) Phenanthrene-d10	17.055	188	14582	0.40	ng	0.00
29) Chrysene-d12	21.247	240	11555	0.40	ng	0.00
35) Perylene-d12	23.466	264	10523	0.40	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.276	112	3542	0.39	ng	0.00
5) Phenol-d6	6.839	99	4048	0.36	ng	0.00
8) Nitrobenzene-d5	8.819	82	4663	0.43	ng	0.00
11) 2-Methylnaphthalene-d10	12.040	152	9034	0.37	ng	0.00
14) 2,4,6-Tribromophenol	15.805	330	668	0.27	ng	0.01
15) 2-Fluorobiphenyl	12.925	172	11660	0.42	ng	0.00
27) Fluoranthene-d10	19.086	212	13747	0.34	ng	0.00
31) Terphenyl-d14	19.692	244	10153	0.44	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.239	88	579	0.11	ng	# 84
3) n-Nitrosodimethylamine	3.601	42	76	0.03	ng	# 1
6) bis(2-Chloroethyl)ether	7.104	93	1372	0.12	ng	100
9) Naphthalene	10.492	128	4685	0.12	ng	96
10) Hexachlorobutadiene	10.784	225	1010	0.13	ng	# 100
12) 2-Methylnaphthalene	12.115	142	2816	0.11	ng	95
16) Acenaphthylene	14.016	152	3618	0.12	ng	99
17) Acenaphthene	14.359	154	2236	0.11	ng	# 93
18) Fluorene	15.361	166	2695	0.11	ng	98
20) 4,6-Dinitro-2-methylph...	15.450	198	72	0.21	ng	# 1
21) 4-Bromophenyl-phenylether	16.252	248	876	0.11	ng	97
22) Hexachlorobenzene	16.361	284	1400	0.14	ng	98
23) Atrazine	16.519	200	395	0.08	ng	# 85
24) Pentachlorophenol	16.714	266	97	0.28	ng	# 83
25) Phenanthrene	17.091	178	4457	0.11	ng	99
26) Anthracene	17.177	178	3255	0.10	ng	99
28) Fluoranthene	19.116	202	4382	0.10	ng	98
30) Pyrene	19.483	202	4053	0.12	ng	99
32) Benzo(a)anthracene	21.237	228	3199	0.10	ng	96
33) Chrysene	21.279	228	4227	0.12	ng	98
34) Bis(2-ethylhexyl)phtha...	21.173	149	1383	0.10	ng	# 97
36) Indeno(1,2,3-cd)pyrene	25.694	276	4361	0.11	ng	100
37) Benzo(b)fluoranthene	22.802	252	4222	0.11	ng	# 77
38) Benzo(k)fluoranthene	22.846	252	4260	0.11	ng	# 75
39) Benzo(a)pyrene	23.370	252	3599	0.11	ng	# 69
40) Dibenzo(a,h)anthracene	25.708	278	3463	0.10	ng	# 82
41) Benzo(g,h,i)perylene	26.369	276	4417	0.12	ng	# 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042821\
Data File : BN014476.D
Acq On : 28 Apr 2021 18:18
Operator : CG/JU
Sample : M1458-07
Misc : LOD-MDL-WTR-0.1PPM
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

Quant Time: Apr 29 02:07:09 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 27 19:23:29 2021
Response via : Initial Calibration




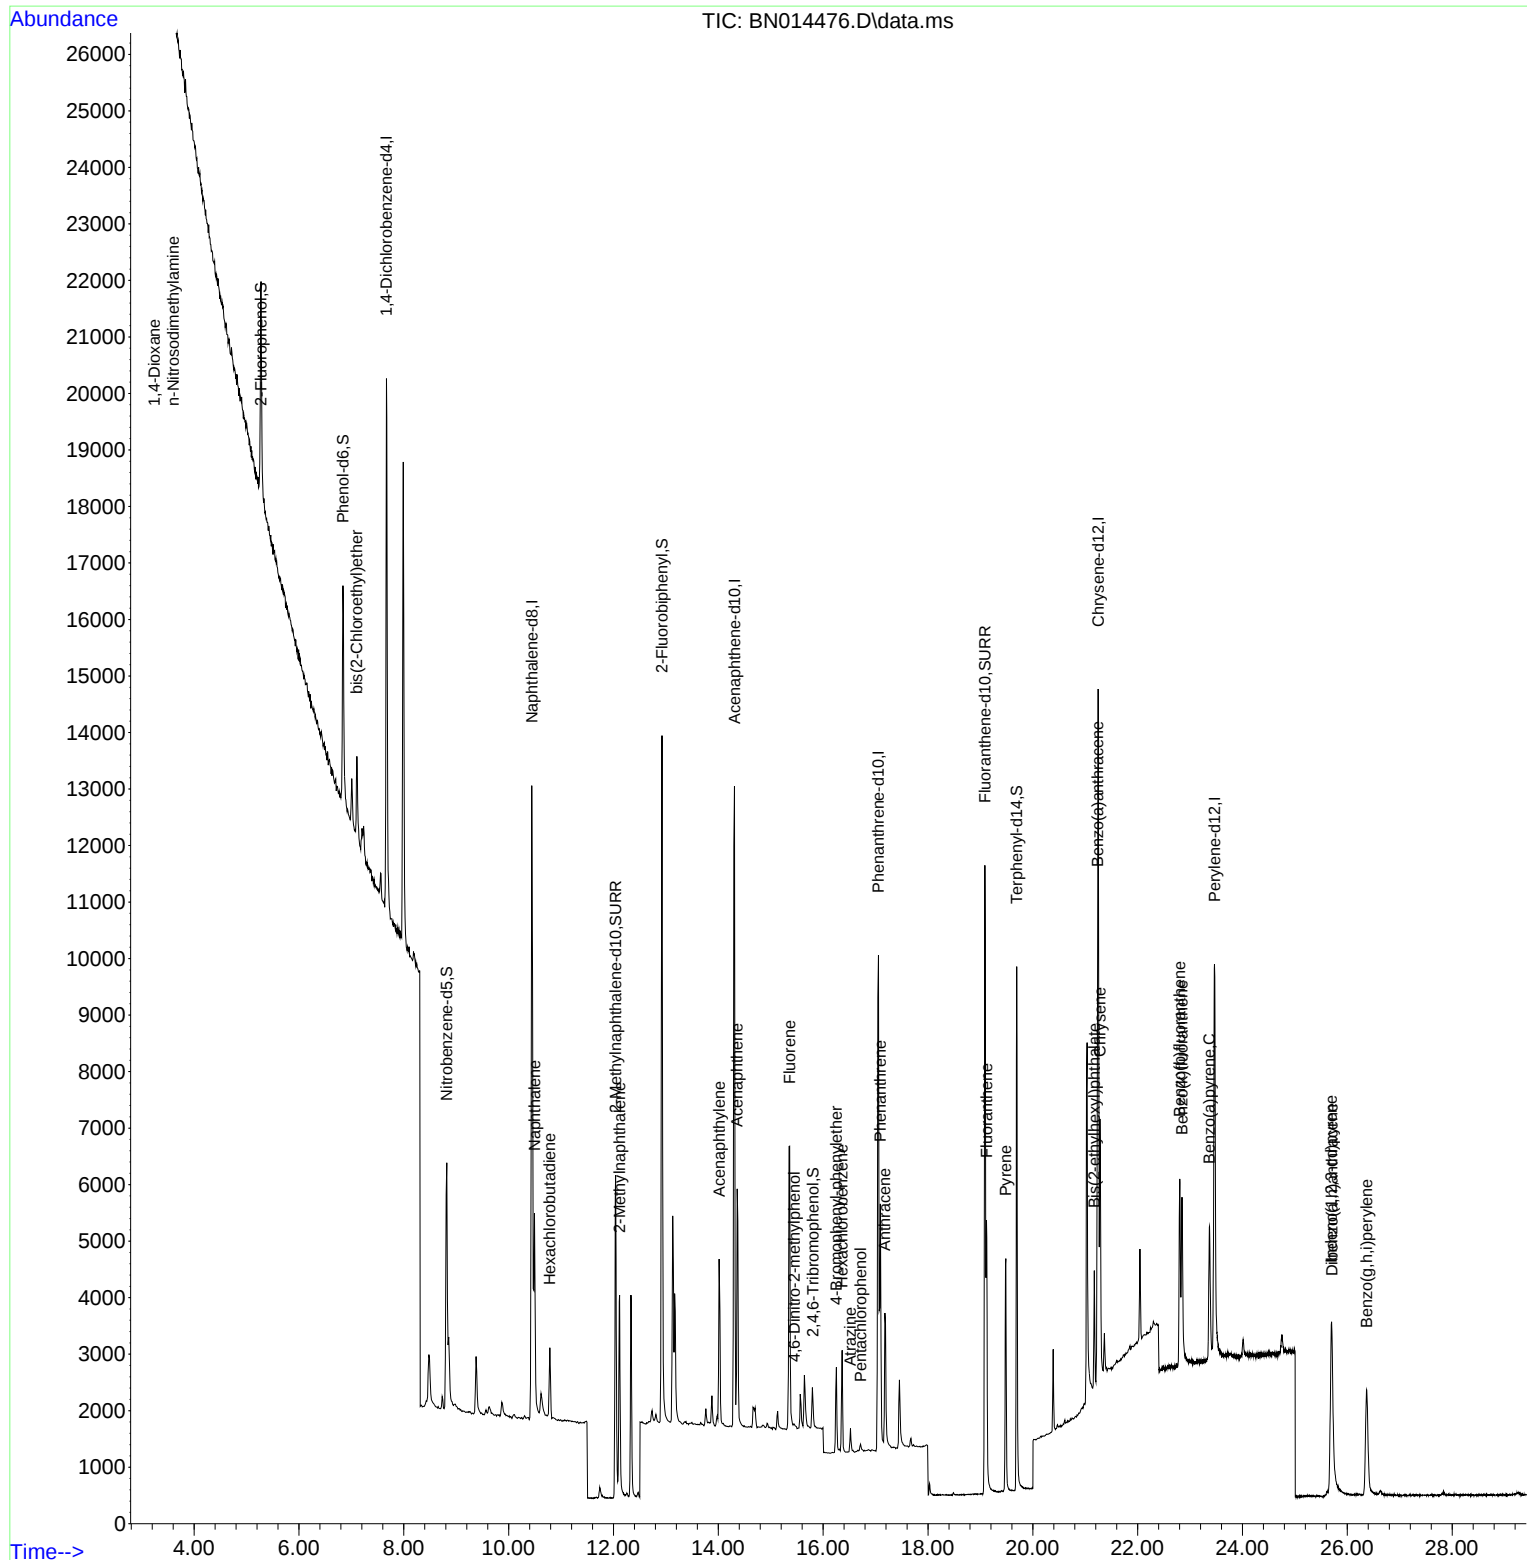




#1
1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.668 min Scan# 607
Delta R.T. -0.008 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18




Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021


Tgt Ion:152 Resp: 4807
Ion Ratio Lower Upper
152 100
150 157.5 121.2 181.8
115 61.7 46.0 69.0



#2
1,4-Dioxane
Concen: 0.11 ng
RT: 3.239 min Scan# 57
Delta R.T. 0.008 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18

Tgt Ion: 88 Resp: 579
Ion Ratio Lower Upper
88 100
58 50.3 53.1 79.7#
43 27.6 20.3 30.5


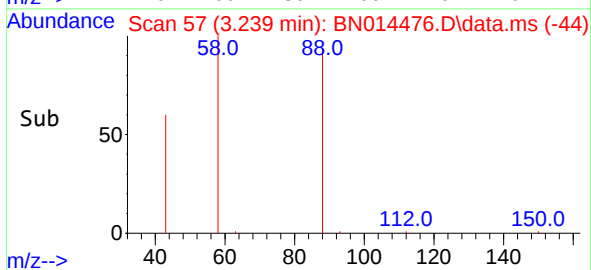






#3
n-Nitrosodimethylamine
Concen: 0.03 ng
RT: 3.601 min Scan# 102
Delta R.T. 0.008 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18




Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021


Tgt Ion: 42 Resp: 76
Ion Ratio Lower Upper
42 100
74 0.0 124.7 187.1#
44 0.0 0.0 0.0

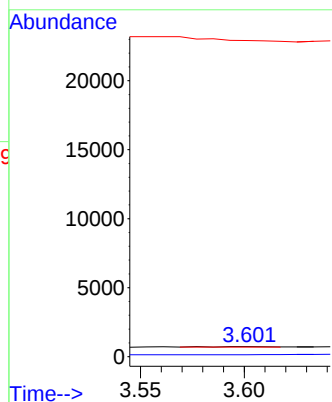

#4
2-Fluorophenol
Concen: 0.39 ng
RT: 5.276 min Scan# 310
Delta R.T. -0.000 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18

Tgt Ion: 112 Resp: 3542
Ion Ratio Lower Upper
112 100
64 53.0 41.4 62.2
63 28.3 21.8 32.8


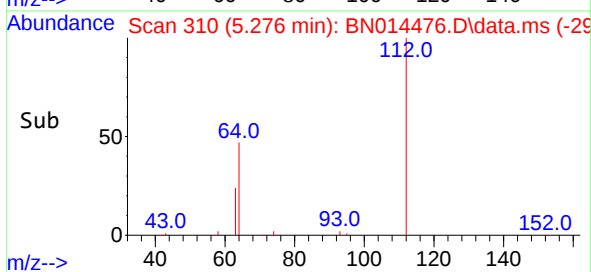
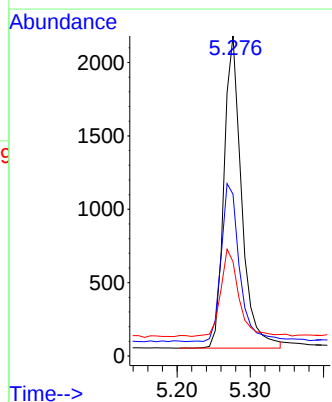



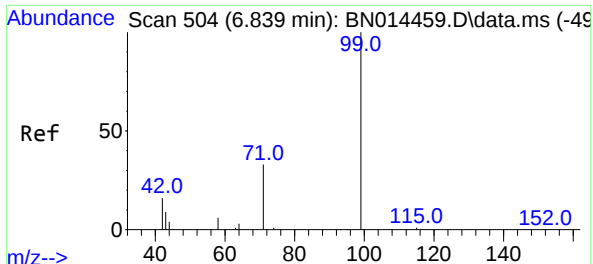

#5
Phenol-d6
Concen: 0.36 ng
RT: 6.839 min Scan# 504
Delta R.T. -0.000 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18




Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021


Tgt Ion: 99 Resp: 4048
Ion Ratio Lower Upper
99 100
42 19.9 13.8 20.6
71 33.5 25.5 38.3

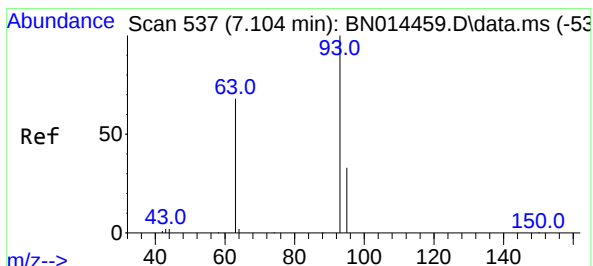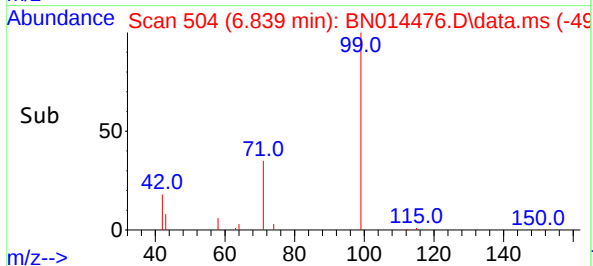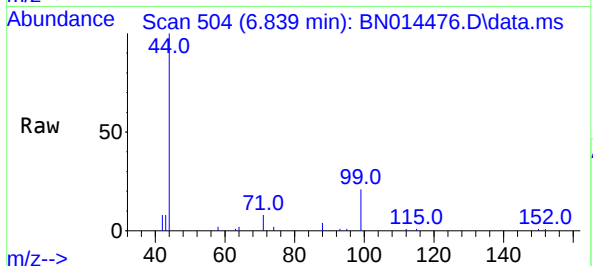

#6
bis(2-Chloroethyl)ether
Concen: 0.12 ng
RT: 7.104 min Scan# 537
Delta R.T. -0.000 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18

Tgt Ion: 93 Resp: 1372
Ion Ratio Lower Upper
93 100
63 70.7 56.7 85.1
95 33.5 26.3 39.5


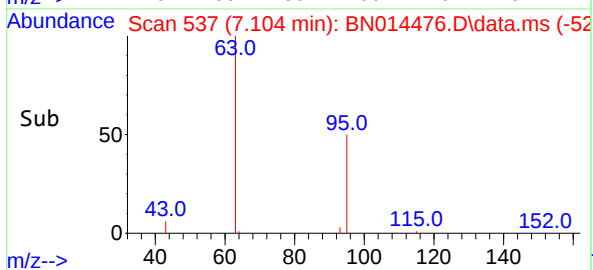

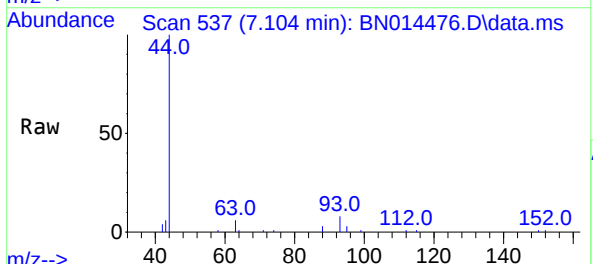




#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.442 min Scan# 855
Delta R.T. -0.000 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18




Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021


Tgt Ion:	136	Resp:	16275
Ion	Ratio	Lower	Upper
136	100		
137	11.5	9.0	13.4
54	7.9	5.7	8.5
68	6.9	5.2	7.8

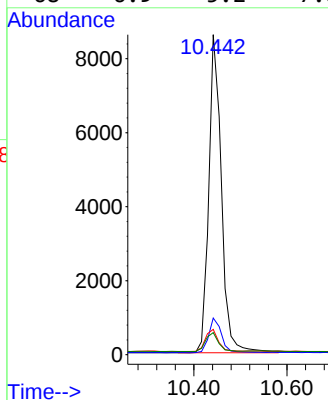

#8
Nitrobenzene-d5
Concen: 0.43 ng
RT: 8.819 min Scan# 727
Delta R.T. -0.000 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18

Tgt Ion:	82	Resp:	4663
Ion	Ratio	Lower	Upper
82	100		
128	41.5	38.5	57.7
54	42.9	32.1	48.1



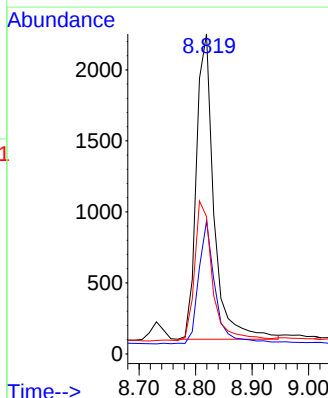



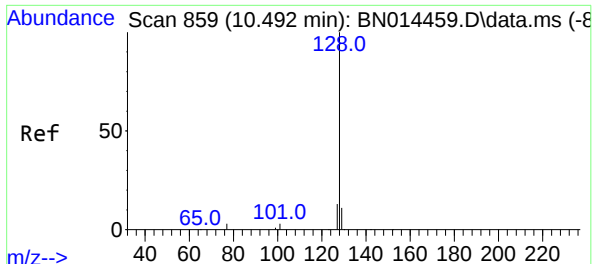

#9
Naphthalene
Concen: 0.12 ng
RT: 10.492 min Scan# 859
Delta R.T. -0.000 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18




Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021


Tgt Ion:	128	Resp:	4685
Ion	Ratio	Lower	Upper
128	100		
129	12.9	9.0	13.4
127	14.4	10.5	15.7

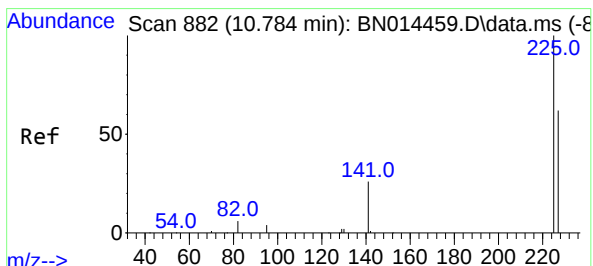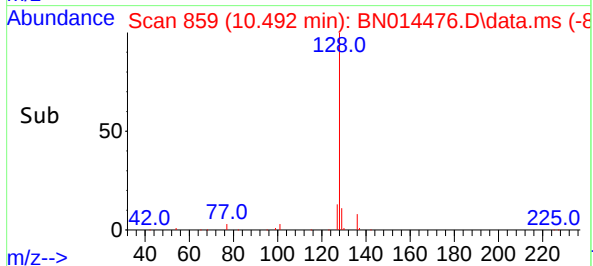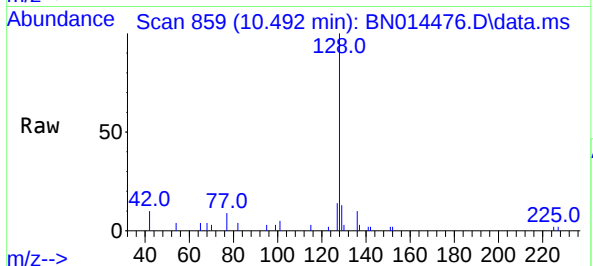

#10
Hexachlorobutadiene
Concen: 0.13 ng
RT: 10.784 min Scan# 882
Delta R.T. -0.000 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18

Tgt Ion:	225	Resp:	1010
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	64.2	51.5	77.3


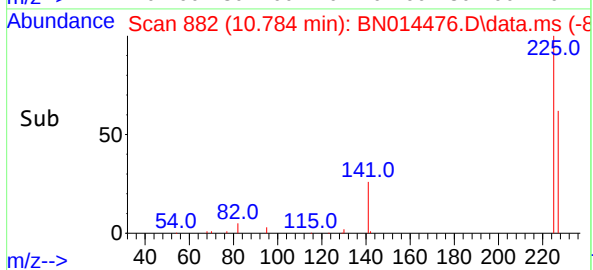

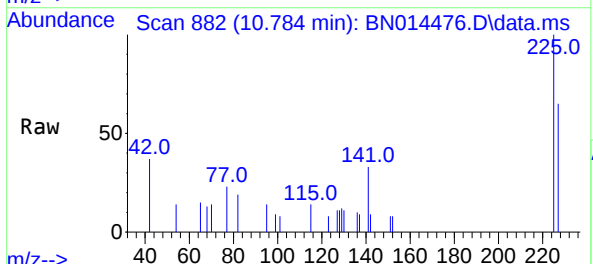




#11
2-Methylnaphthalene-d10
Concen: 0.37 ng
RT: 12.040 min Scan# 1059
Delta R.T. -0.000 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18




Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021


Tgt Ion:152 Resp: 9034
Ion Ratio Lower Upper
152 100
151 18.9 16.2 24.4

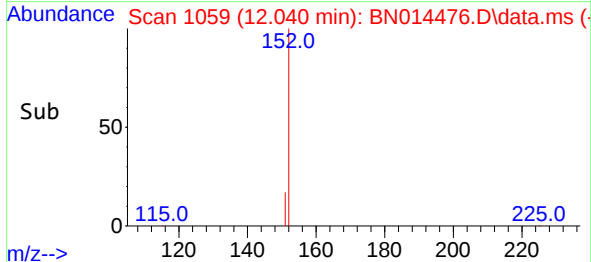

#12
2-Methylnaphthalene
Concen: 0.11 ng
RT: 12.115 min Scan# 1076
Delta R.T. -0.000 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18

Tgt Ion:142 Resp: 2816
Ion Ratio Lower Upper
142 100
141 89.9 69.6 104.4
115 38.9 27.0 40.6


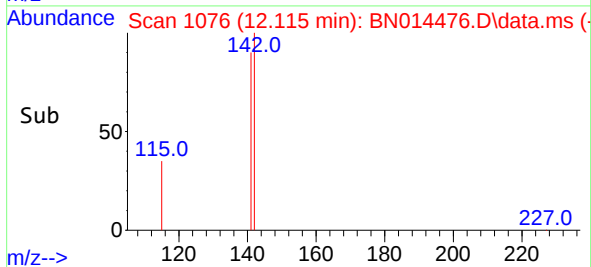

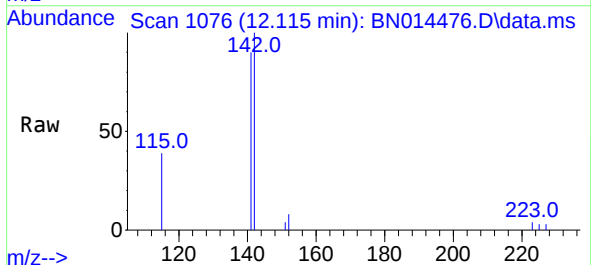




#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.308 min Scan# 1306
Delta R.T. -0.000 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18




Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021


Tgt Ion:164 Resp: 7383
Ion Ratio Lower Upper
164 100
162 98.0 78.3 117.5
160 54.4 36.6 54.8



#14
2,4,6-Tribromophenol
Concen: 0.27 ng
RT: 15.805 min Scan# 1424
Delta R.T. 0.013 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18

Tgt Ion:330 Resp: 668
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 37.7 29.3 43.9


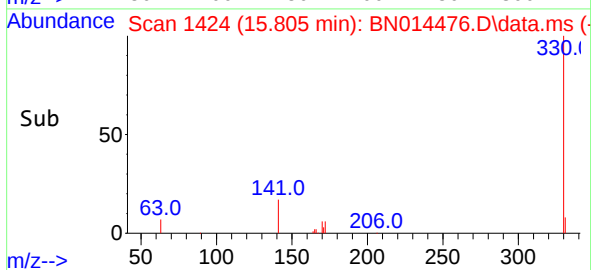






#15
2-Fluorobiphenyl
Concen: 0.42 ng
RT: 12.925 min Scan# 1197
Delta R.T. -0.000 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18




Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021


Tgt Ion:	172	Resp:	11660
Ion	Ratio	Lower	Upper
172	100		
171	34.1	27.0	40.4
170	23.2	18.2	27.4



#16
Acenaphthylene
Concen: 0.12 ng
RT: 14.016 min Scan# 1283
Delta R.T. -0.000 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18

Tgt Ion:	152	Resp:	3618
Ion	Ratio	Lower	Upper
152	100		
151	19.1	15.4	23.2
153	13.6	10.4	15.6


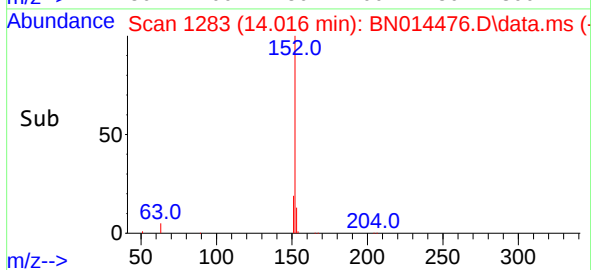






#17
Acenaphthene
Concen: 0.11 ng
RT: 14.359 min Scan# 1310
Delta R.T. -0.013 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18




Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021


Tgt Ion:154 Resp: 2236
Ion Ratio Lower Upper
154 100
153 115.3 90.5 135.7
152 70.9 47.2 70.8#

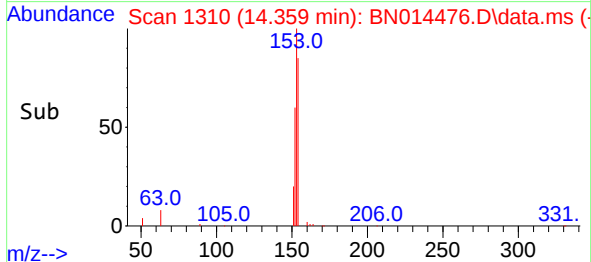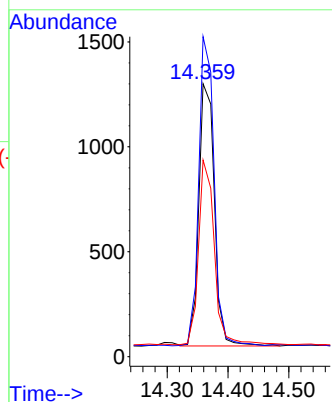

#18
Fluorene
Concen: 0.11 ng
RT: 15.361 min Scan# 1389
Delta R.T. -0.000 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18

Tgt Ion:166 Resp: 2695
Ion Ratio Lower Upper
166 100
165 100.0 78.1 117.1
167 14.0 11.0 16.6


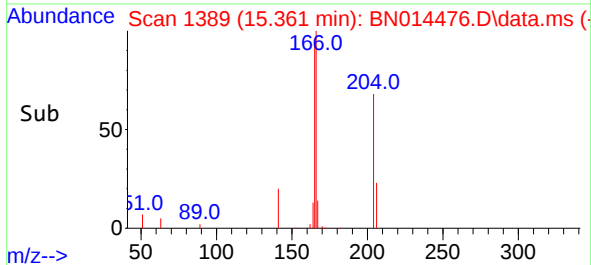
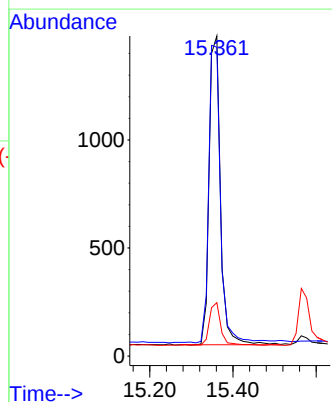
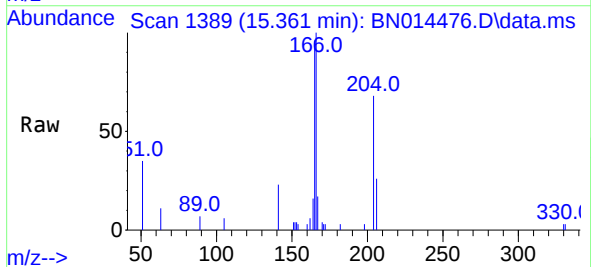


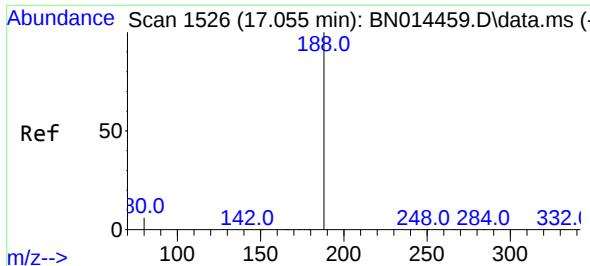

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.055 min Scan# 1526
Delta R.T. -0.001 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18




Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021


Tgt Ion:188	Resp:	14582
Ion Ratio	Lower	Upper
188	100	
94	0.0	0.0
80	7.5	5.4

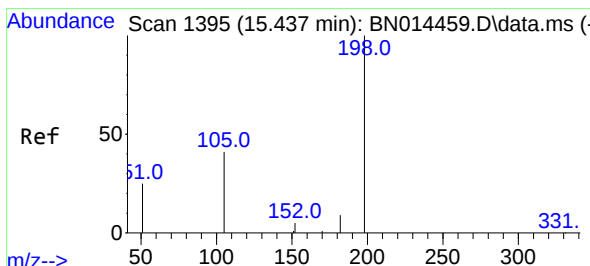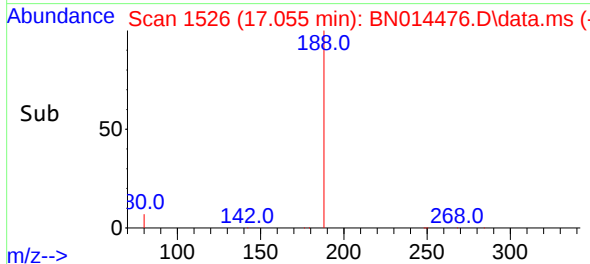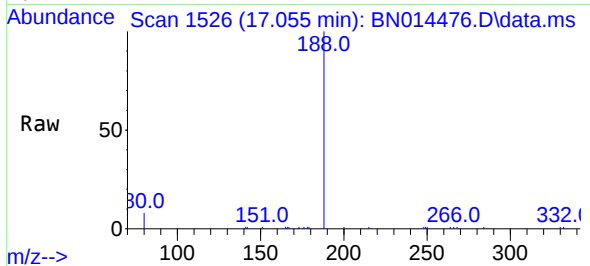

#20
4,6-Dinitro-2-methylphenol
Concen: 0.21 ng
RT: 15.450 min Scan# 1396
Delta R.T. 0.013 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18

Tgt Ion:198	Resp:	72
Ion Ratio	Lower	Upper
198	100	
51	640.9	104.5
105	151.5	62.2


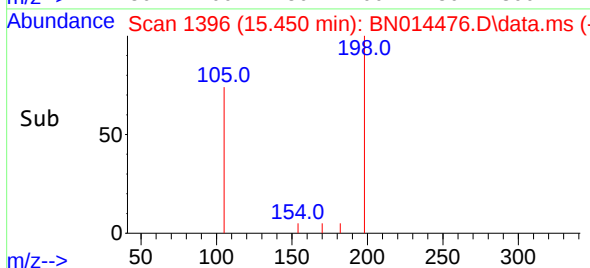
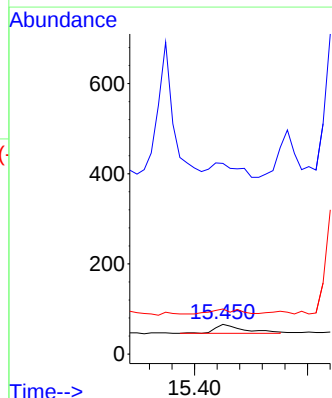
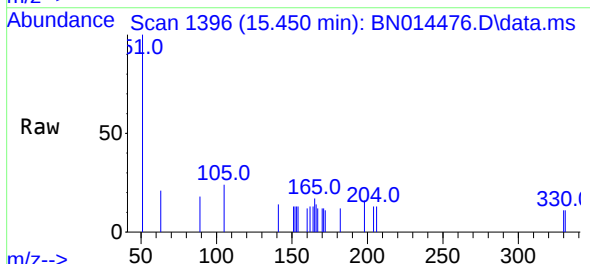




#21
4-Bromophenyl-phenylether
Concen: 0.11 ng
RT: 16.252 min Scan# 1460
Delta R.T. -0.001 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18




Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021


Tgt Ion:	248	Resp:	876
Ion	Ratio	Lower	Upper
248	100		
250	101.0	81.8	122.6
141	48.0	34.2	51.2

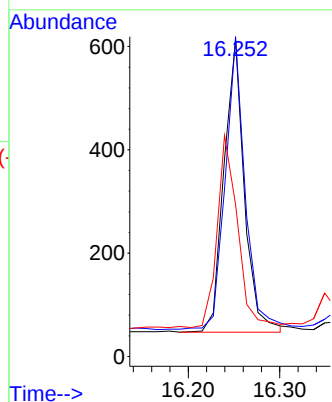

#22
Hexachlorobenzene
Concen: 0.14 ng
RT: 16.361 min Scan# 1469
Delta R.T. -0.001 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18

Tgt Ion:	284	Resp:	1400
Ion	Ratio	Lower	Upper
284	100		
142	35.0	27.2	40.8
249	30.2	23.4	35.2


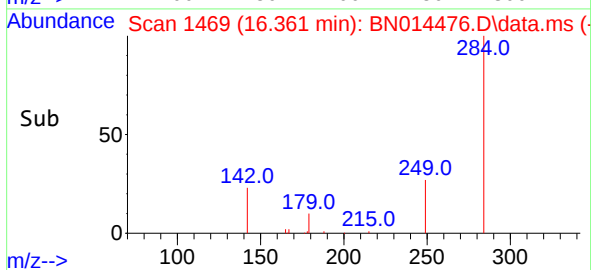






#23
Atrazine
Concen: 0.08 ng
RT: 16.519 min Scan# 1482
Delta R.T. -0.001 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18




Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021


Tgt Ion:200 Resp: 395
Ion Ratio Lower Upper
200 100
173 37.2 20.8 31.2#
215 57.1 39.3 58.9

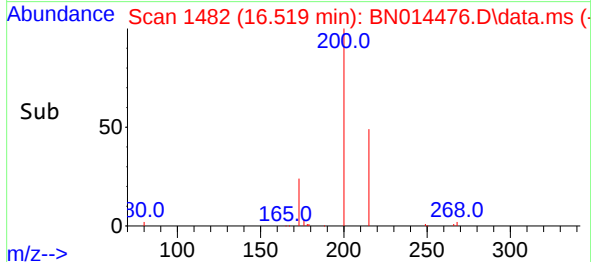

#24
Pentachlorophenol
Concen: 0.28 ng
RT: 16.714 min Scan# 1498
Delta R.T. -0.001 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18

Tgt Ion:266 Resp: 97
Ion Ratio Lower Upper
266 100
264 49.5 49.9 74.9#
268 78.4 51.6 77.4#


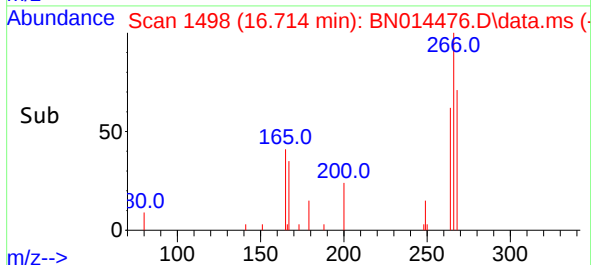
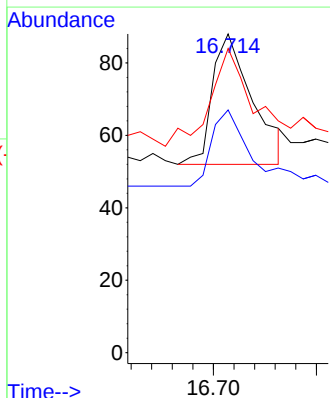
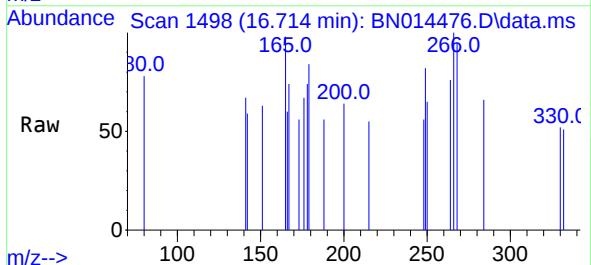




#25
Phenanthrene
Concen: 0.11 ng
RT: 17.091 min Scan# 1529
Delta R.T. -0.001 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18




Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021


Tgt Ion:	178	Resp:	4457
Ion	Ratio	Lower	Upper
178	100		
176	19.3	15.1	22.7
179	16.2	12.2	18.4

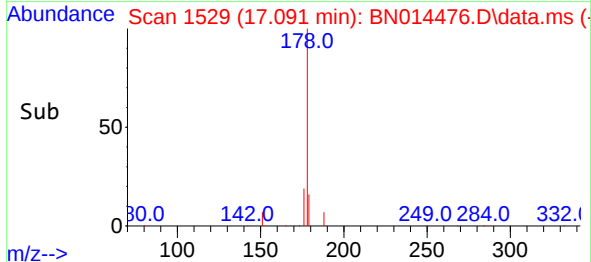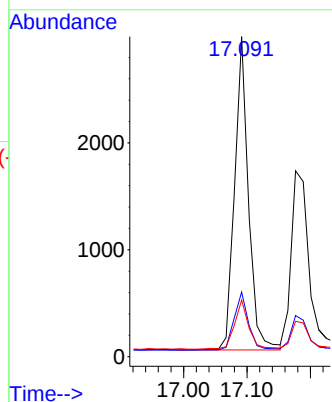

#26
Anthracene
Concen: 0.10 ng
RT: 17.177 min Scan# 1536
Delta R.T. -0.001 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18

Tgt Ion:	178	Resp:	3255
Ion	Ratio	Lower	Upper
178	100		
176	18.1	14.6	22.0
179	14.7	12.0	18.0


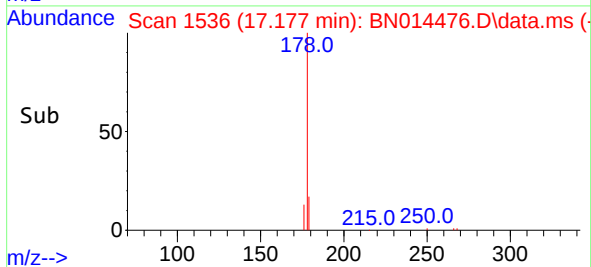

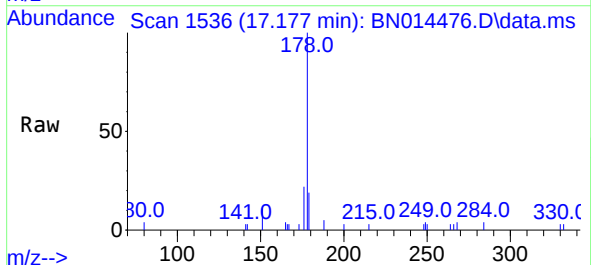




#27
Fluoranthene-d10
Concen: 0.34 ng
RT: 19.086 min Scan# 1822
Delta R.T. -0.003 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18




Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021


Tgt Ion:212 Resp: 13747
Ion Ratio Lower Upper
212 100
106 12.9 10.2 15.4
104 7.7 5.6 8.4



#28
Fluoranthene
Concen: 0.10 ng
RT: 19.116 min Scan# 1828
Delta R.T. -0.003 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18

Tgt Ion:202 Resp: 4382
Ion Ratio Lower Upper
202 100
101 11.2 8.5 12.7
203 18.1 13.7 20.5


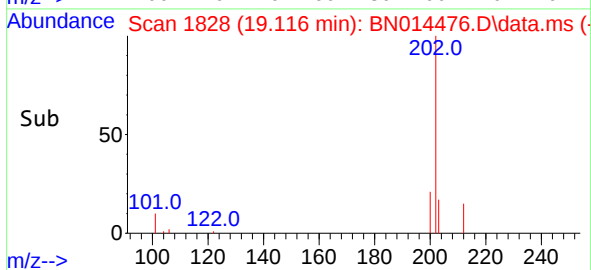






#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.247 min Scan# 2124
Delta R.T. -0.003 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18




Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021


Tgt Ion:240	Resp:	11555
Ion Ratio	Lower	Upper
240	100	
120	10.8	9.0 13.6
236	26.8	21.4 32.0

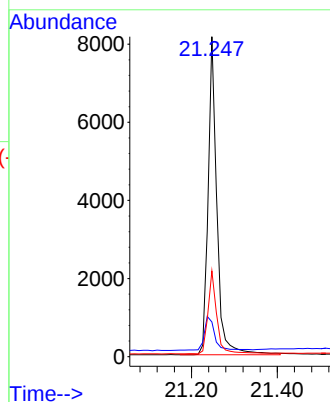

#30
Pyrene
Concen: 0.12 ng
RT: 19.483 min Scan# 1902
Delta R.T. -0.003 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18

Tgt Ion:202	Resp:	4053
Ion Ratio	Lower	Upper
202	100	
200	20.5	16.4 24.6
203	18.3	13.9 20.9


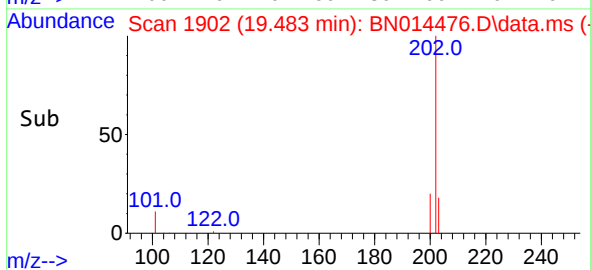






#31
Terphenyl-d14
Concen: 0.44 ng
RT: 19.692 min Scan# 1944
Delta R.T. -0.003 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18




Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021


Tgt Ion:244 Resp: 10153
Ion Ratio Lower Upper
244 100
212 8.0 6.2 9.2
122 13.3 9.8 14.8

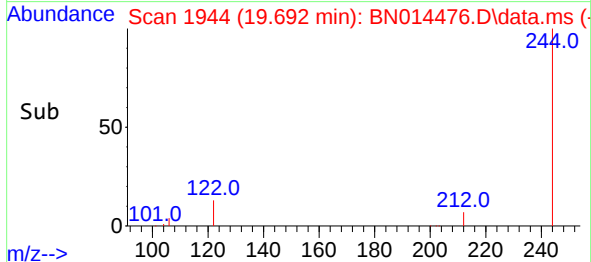

#32
Benzo(a)anthracene
Concen: 0.10 ng
RT: 21.237 min Scan# 2123
Delta R.T. -0.003 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18

Tgt Ion:228 Resp: 3199
Ion Ratio Lower Upper
228 100
226 27.4 20.8 31.2
229 22.3 16.1 24.1


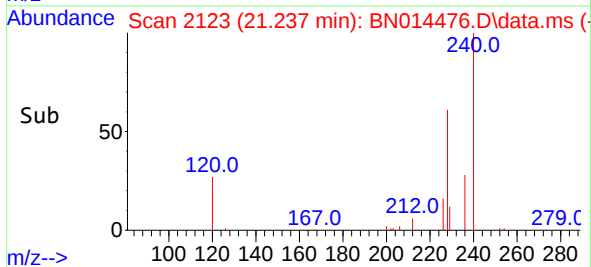

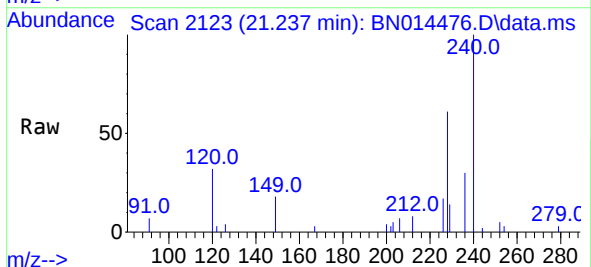




#33
Chrysene
Concen: 0.12 ng
RT: 21.279 min Scan# 2127
Delta R.T. -0.003 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18




Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021


Tgt Ion:228 Resp: 4227
Ion Ratio Lower Upper
228 100
226 32.0 24.8 37.2
229 20.7 15.3 22.9



#34
Bis(2-ethylhexyl)phthalate
Concen: 0.10 ng
RT: 21.173 min Scan# 2117
Delta R.T. -0.003 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18

Tgt Ion:149 Resp: 1383
Ion Ratio Lower Upper
149 100
167 25.7 19.4 29.2
279 5.4 2.9 4.3#


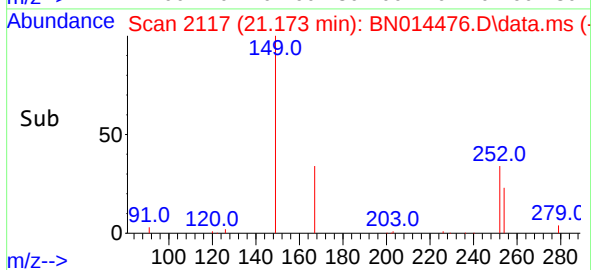






#35
 Perylene-d12
 Concen: 0.40 ng
 RT: 23.466 min Scan# 2543
 Delta R.T. -0.006 min
 Lab File: BN014476.D
 Acq: 28 Apr 2021 18:18




Instrument :
 BNA_N
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2021


Tgt Ion:264	Resp:	10523
Ion Ratio	Lower	Upper
264	100	
260	25.4	19.8 29.6
265	55.5	31.6 47.4#

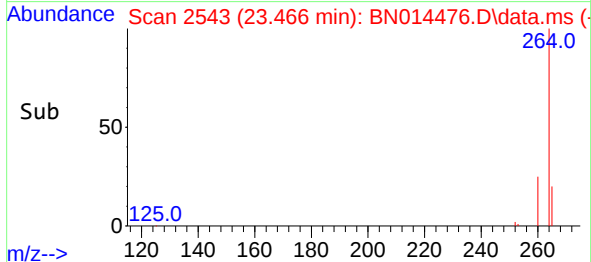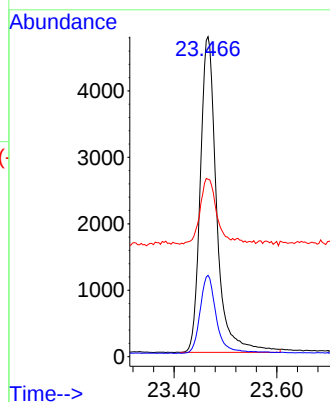

#36
 Indeno(1,2,3-cd)pyrene
 Concen: 0.11 ng
 RT: 25.694 min Scan# 3194
 Delta R.T. -0.003 min
 Lab File: BN014476.D
 Acq: 28 Apr 2021 18:18

Tgt Ion:276	Resp:	4361
Ion Ratio	Lower	Upper
276	100	
138	23.3	18.5 27.7
277	24.9	19.9 29.9


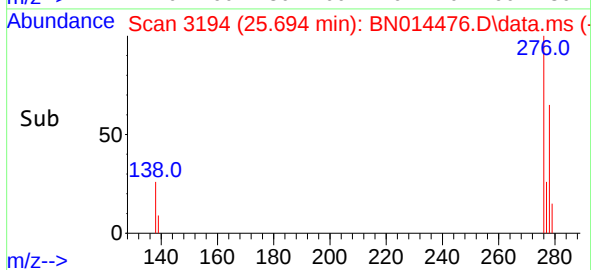






#37
Benzo(b)fluoranthene
Concen: 0.11 ng
RT: 22.802 min Scan# 2349
Delta R.T. -0.006 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18




Tgt Ion:252 Resp: 4222
Ion Ratio Lower Upper
252 100
253 33.6 19.3 28.9#
125 27.9 12.8 19.2#


Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

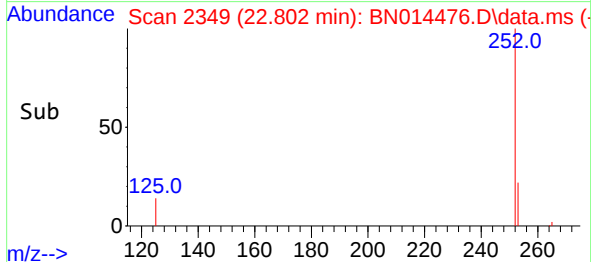

#38
Benzo(k)fluoranthene
Concen: 0.11 ng
RT: 22.846 min Scan# 2362
Delta R.T. -0.003 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18

Tgt Ion:252 Resp: 4260
Ion Ratio Lower Upper
252 100
253 35.1 19.3 28.9#
125 24.9 10.0 15.0#


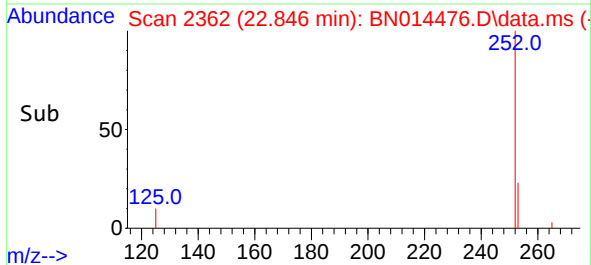

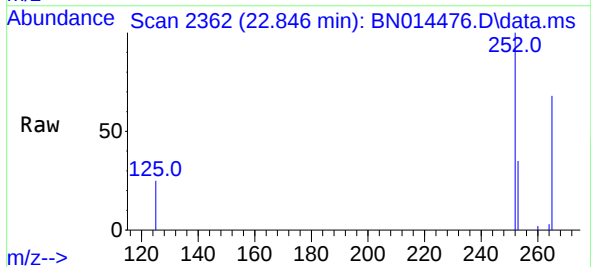




#39
Benzo(a)pyrene
Concen: 0.11 ng
RT: 23.370 min Scan# 2515
Delta R.T. -0.006 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18




Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021


Tgt Ion:252	Resp:	3599
Ion Ratio	Lower	Upper
252	100	
253	41.4	21.0 31.6#
125	42.3	20.8 31.2#

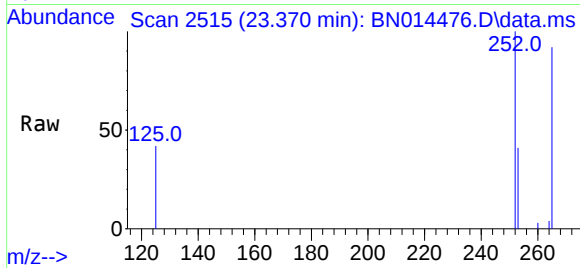

#40
Dibenzo(a,h)anthracene
Concen: 0.10 ng
RT: 25.708 min Scan# 3198
Delta R.T. -0.003 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18

Tgt Ion:278	Resp:	3463
Ion Ratio	Lower	Upper
278	100	
139	22.6	14.3 21.5#
279	37.4	20.3 30.5#

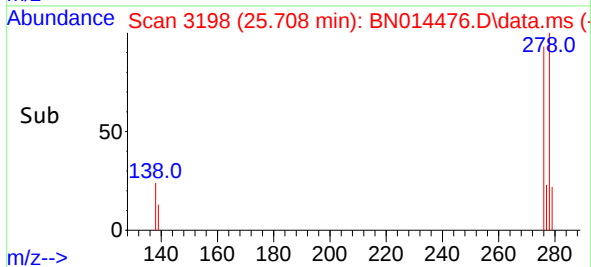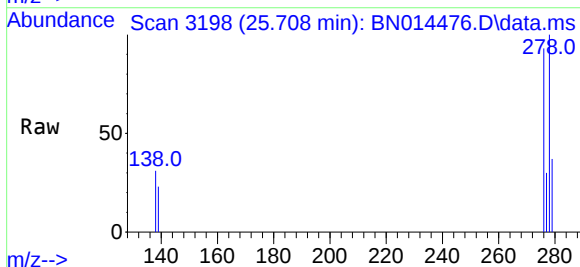

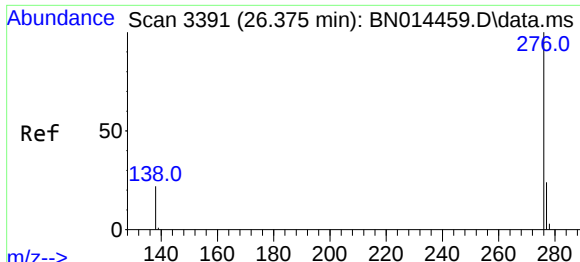

#41
Benzo(g,h,i)perylene
Concen: 0.12 ng
RT: 26.369 min Scan# 3391
Delta R.T. -0.006 min
Lab File: BN014476.D
Acq: 28 Apr 2021 18:18

Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

Tgt Ion:	276	Resp:	4417
Ion	Ratio	Lower	Upper
276	100		
277	29.0	19.5	29.3
138	27.9	18.3	27.5#

