
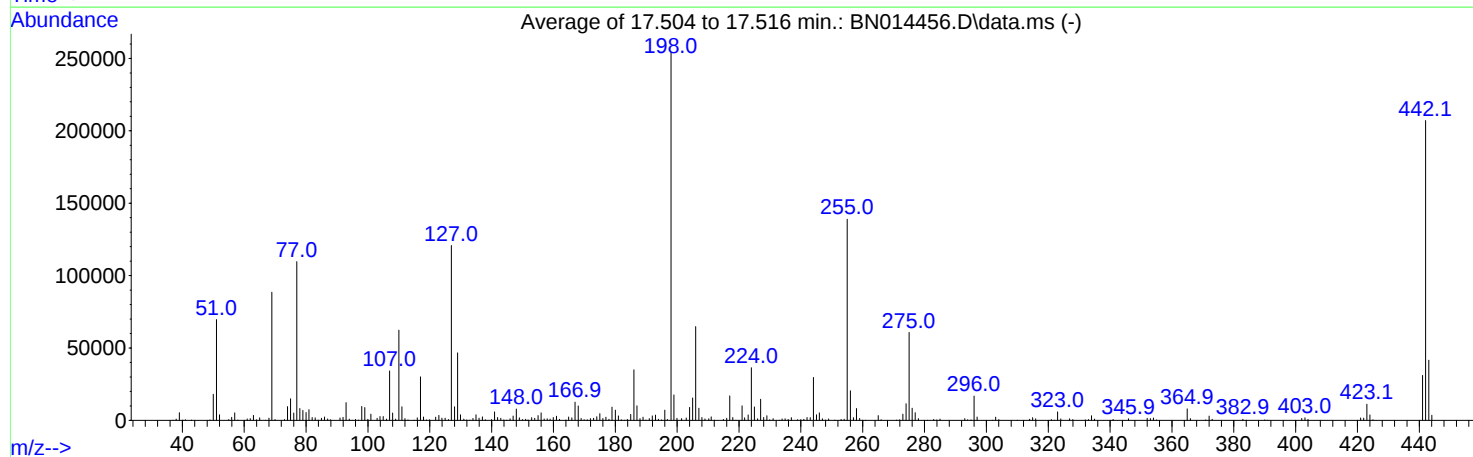


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042821\
 Data File : BN014456.D
 Acq On : 27 Apr 2021 14:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 27 19:23:29 2021

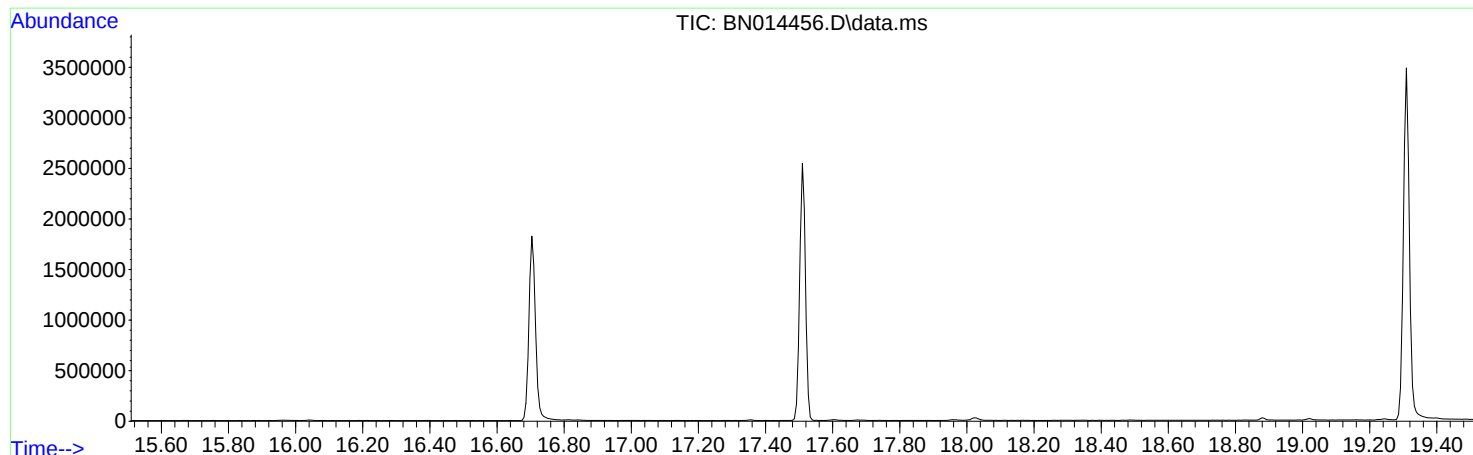




AutoFind: Scans 2451, 2452, 2453; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.4	69691	PASS
68	69	0.00	2	1.7	1511	PASS
69	198	0.00	100	34.9	88557	PASS
70	69	0.00	2	0.6	553	PASS
127	198	10	80	47.6	120840	PASS
197	198	0.00	2	0.3	664	PASS
198	198	100	100	100.0	254101	PASS
199	198	5	9	6.9	17544	PASS
275	198	10	60	23.9	60744	PASS
365	198	1	100	3.1	7928	PASS
441	198	0.01	100	12.2	31096	PASS
442	442	50	100	100.0	207163	PASS
443	442	15	24	20.1	41584	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042821\
Data File : BN014456.D
Acq On : 27 Apr 2021 14:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 27 15:22:48 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 09 09:55:03 2021
Response via : Initial Calibration

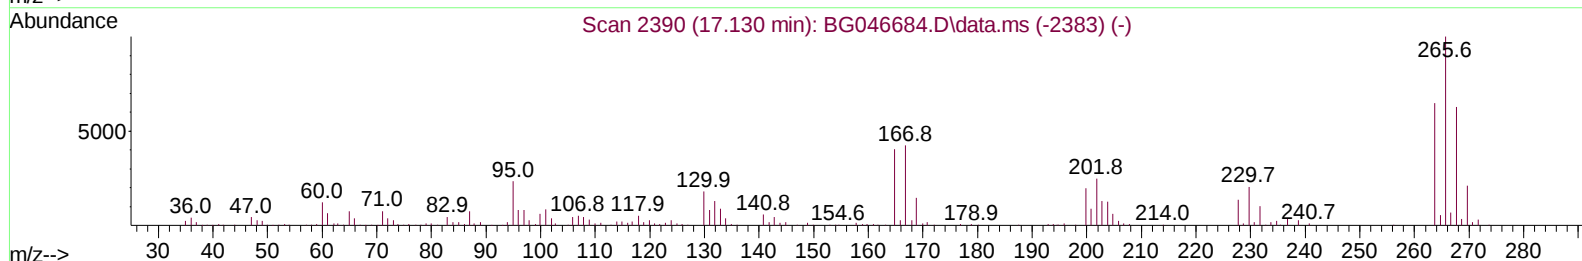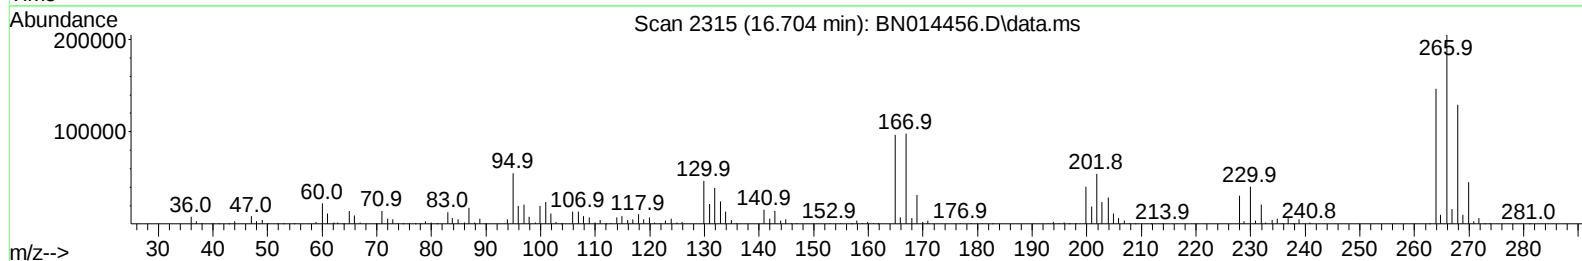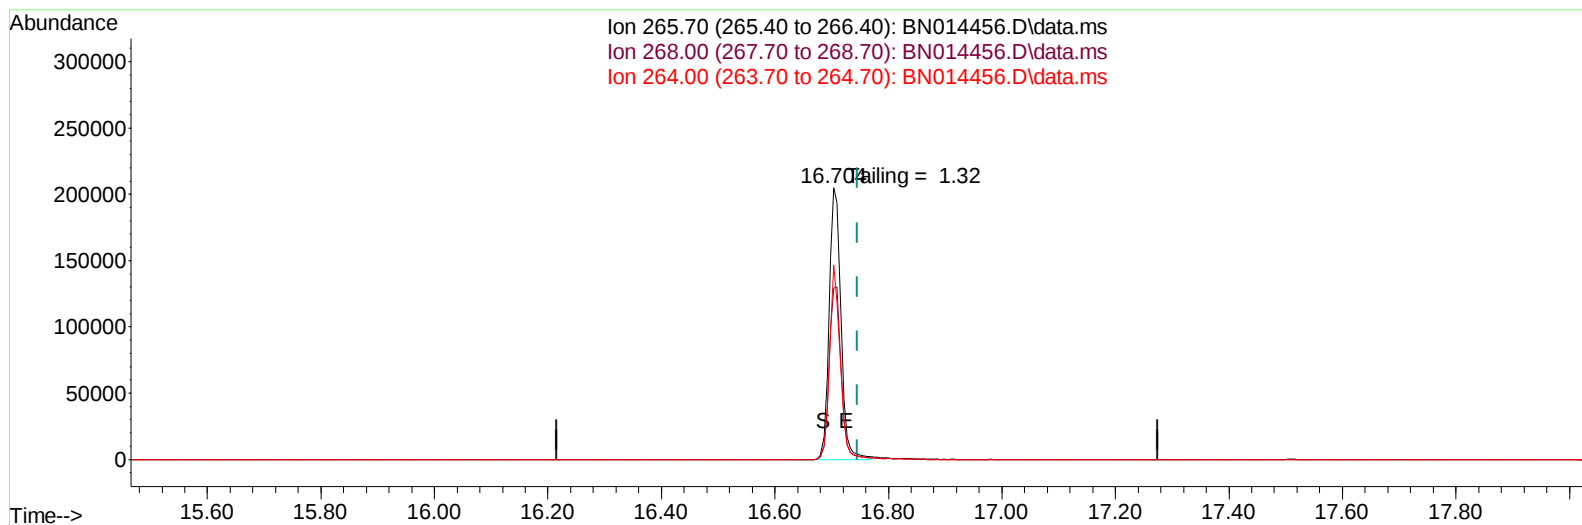

TIC: BN014456.D\data.ms

(70) Pentachloropheno1 (C)

16.704min (-0.041) 23494.39 ng




response 300905

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.10
264.00	61.60	71.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042821\
 Data File : BN014456.D
 Acq On : 27 Apr 2021 14:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Apr 27 15:22:48 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 09 09:55:03 2021
 Response via : Initial Calibration

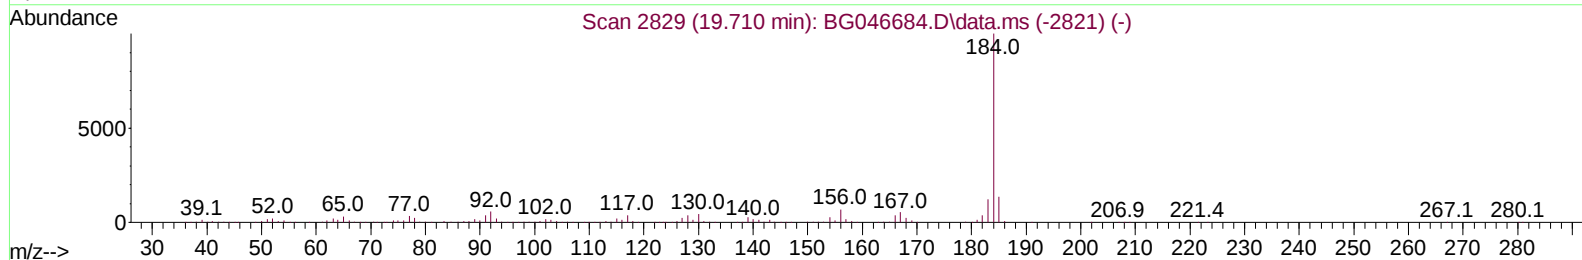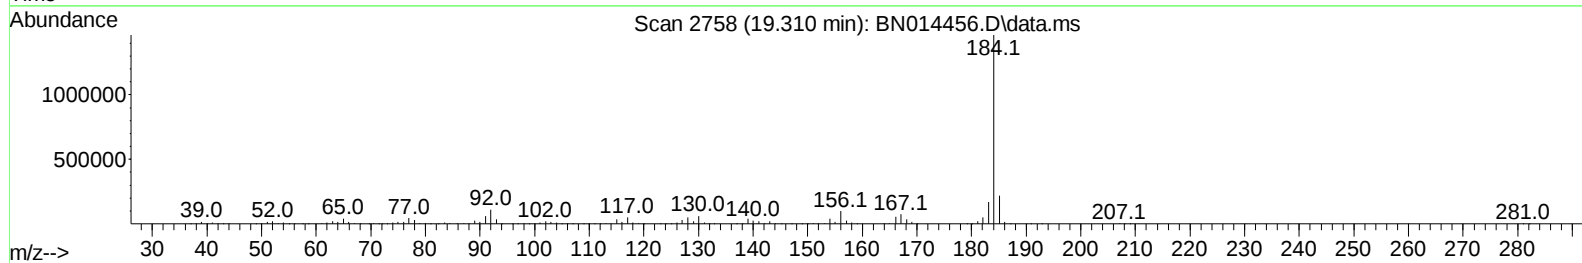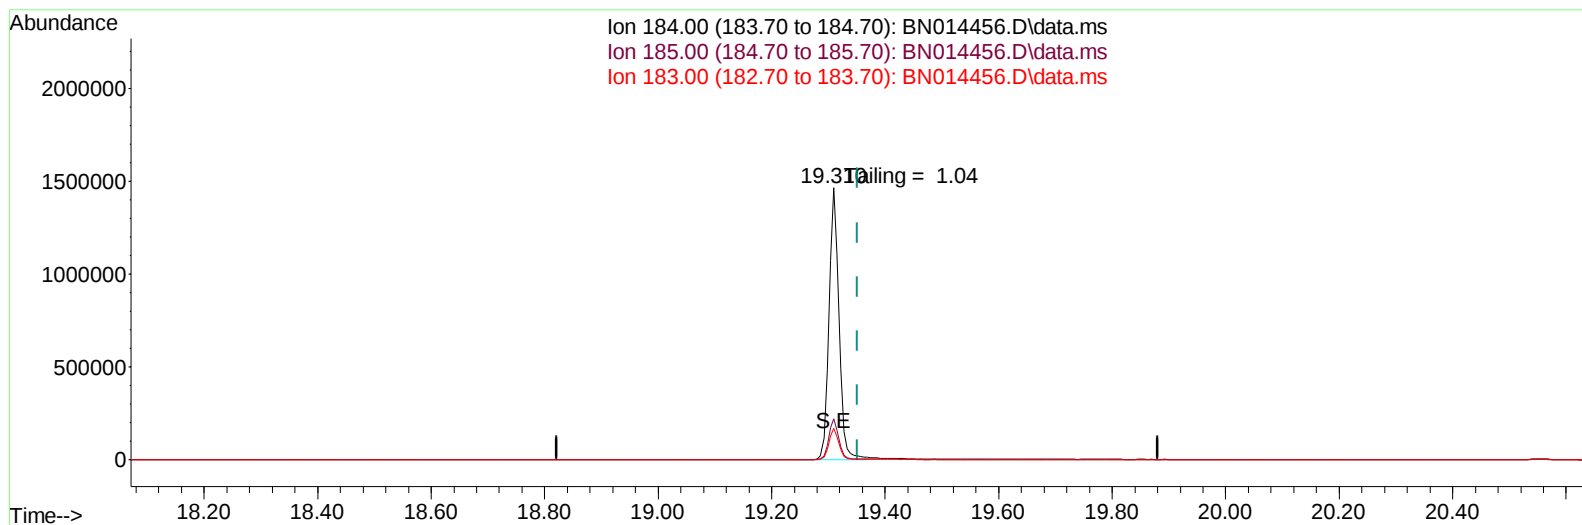

TIC: BN014456.D\data.ms

(77) Benzidine**19.310min (-0.041) 93822.41 ng****response 1804677**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.05
183.00	13.20	11.43
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/28/2021	BNA_N	<u>BN014456.D</u>
Compound Name	Response	Retention Time
DDT	862639	20.557
DDD	2025	20.11
DDE	749	19.604
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2774	865413	0.32

Instrument :
BNA_N
ClientSampleId :
DFTPP