
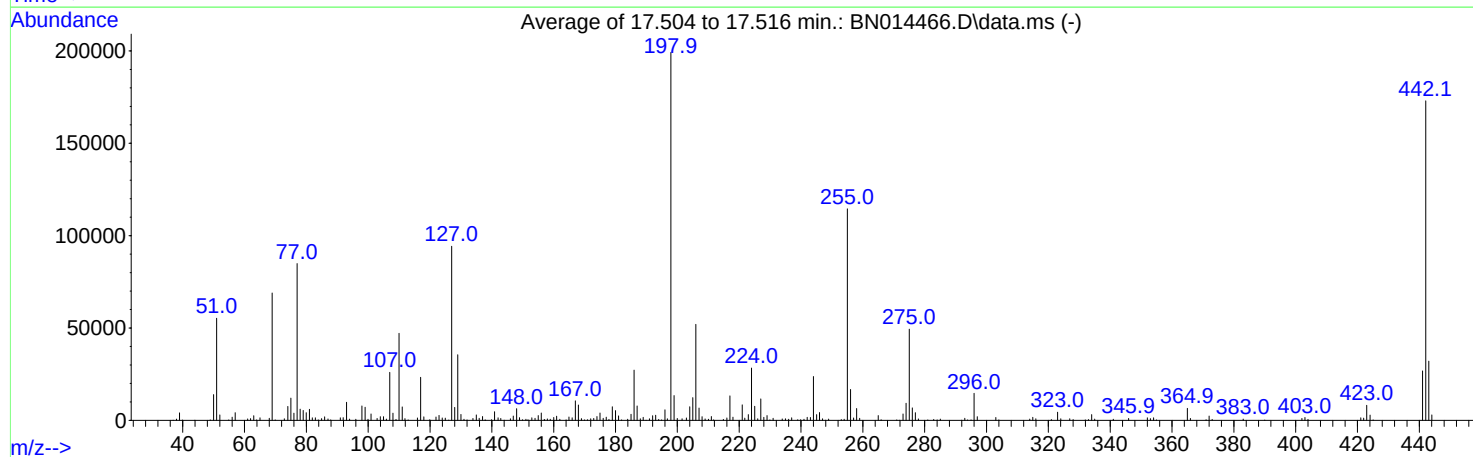


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042821\
 Data File : BN014466.D
 Acq On : 28 Apr 2021 09:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 27 19:23:29 2021

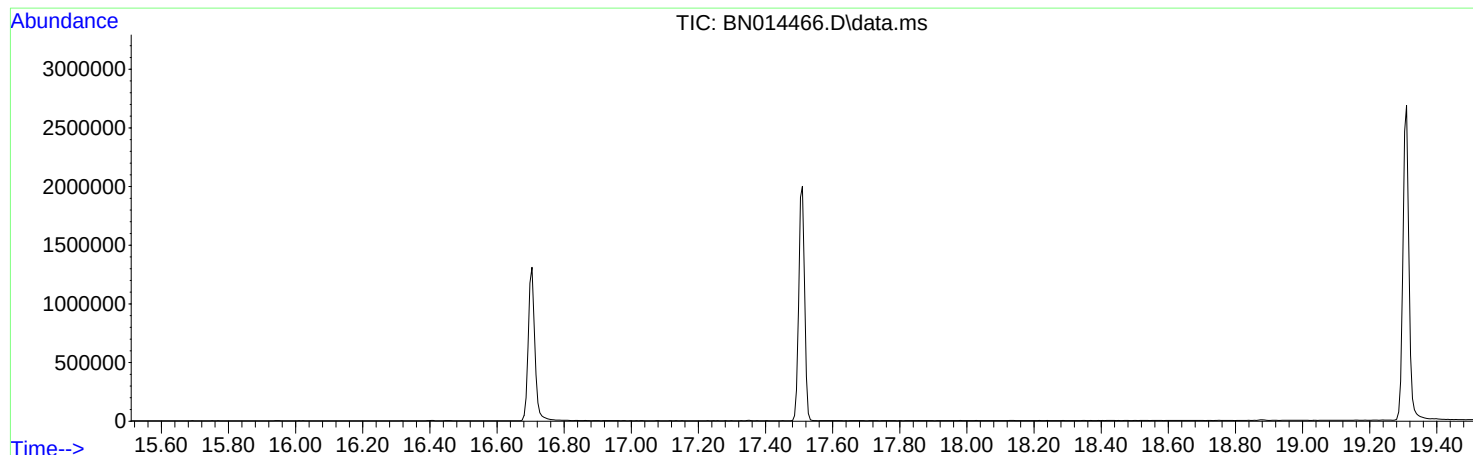




AutoFind: Scans 2451, 2452, 2453; Background Corrected with Scan 2444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.8	55315	PASS
68	69	0.00	2	1.7	1166	PASS
69	198	0.00	100	34.6	68920	PASS
70	69	0.00	2	0.4	278	PASS
127	198	10	80	47.3	94248	PASS
197	198	0.00	2	0.4	883	PASS
198	198	100	100	100.0	199168	PASS
199	198	5	9	6.7	13430	PASS
275	198	10	60	24.8	49397	PASS
365	198	1	100	3.3	6512	PASS
441	198	0.01	100	13.4	26760	PASS
442	442	50	100	100.0	172971	PASS
443	442	15	24	18.5	32064	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042821\
Data File : BN014466.D
Acq On : 28 Apr 2021 09:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 28 10:50:29 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 09 09:55:03 2021
Response via : Initial Calibration

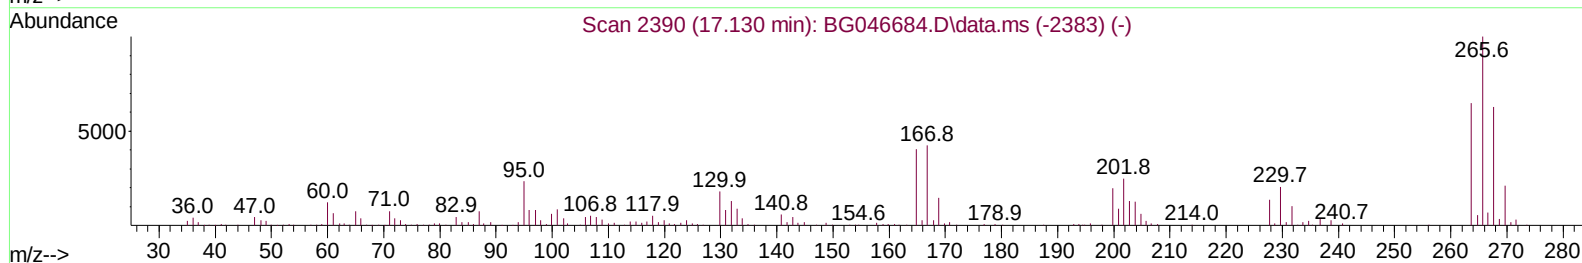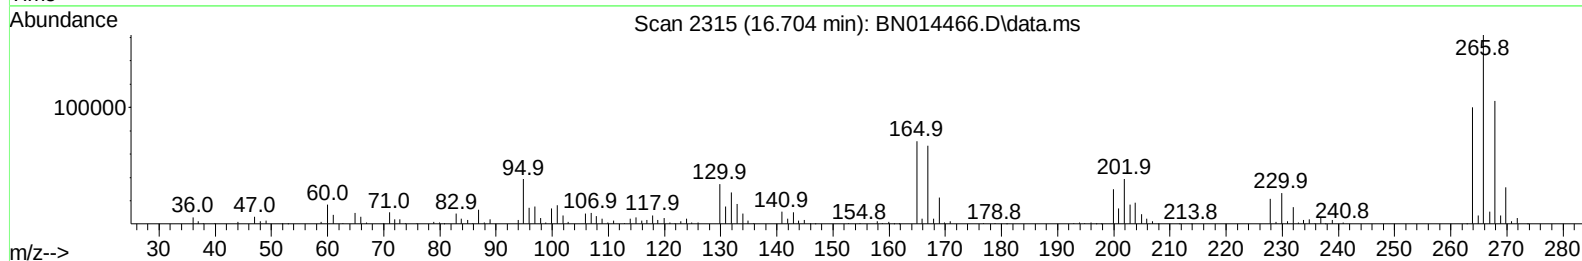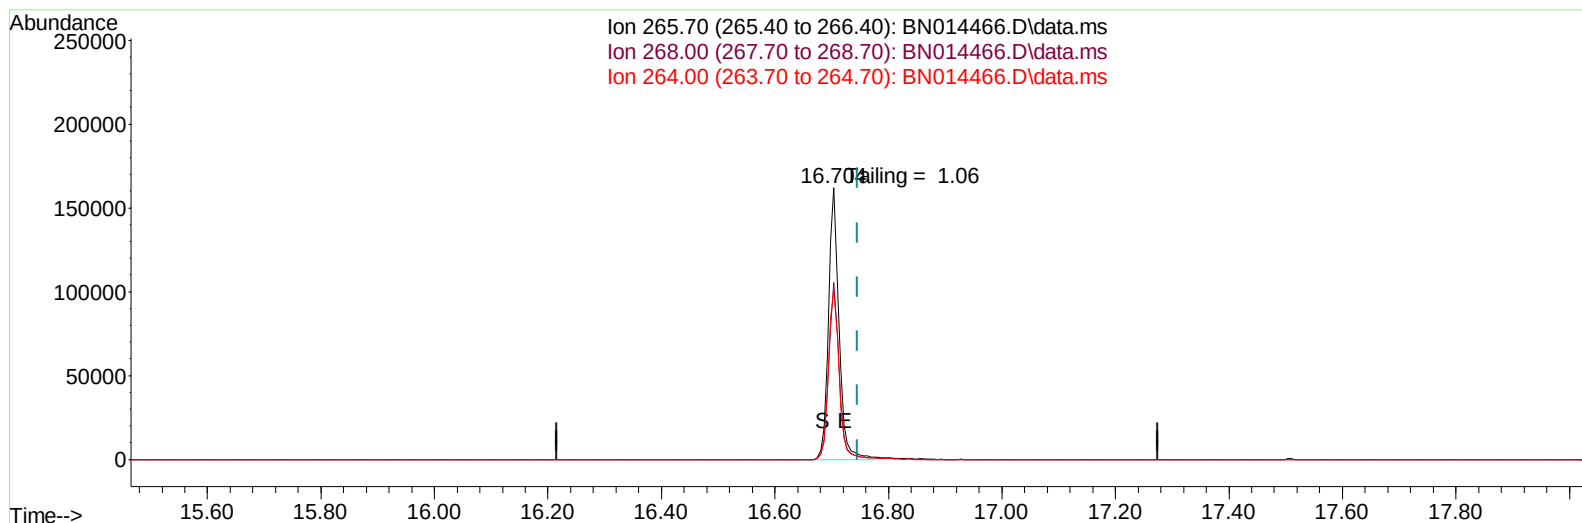

TIC: BN014466.D\data.ms

(70) Pentachlorophenol (C)

16.704min (-0.041) 23282.10 ng




response 210667

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.16
264.00	61.60	61.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042821\
Data File : BN014466.D
Acq On : 28 Apr 2021 09:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 28 10:50:29 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 09 09:55:03 2021
Response via : Initial Calibration

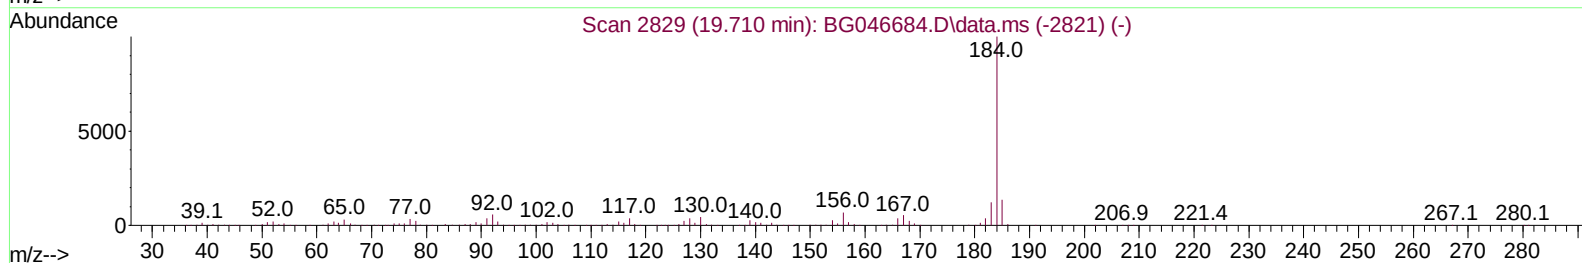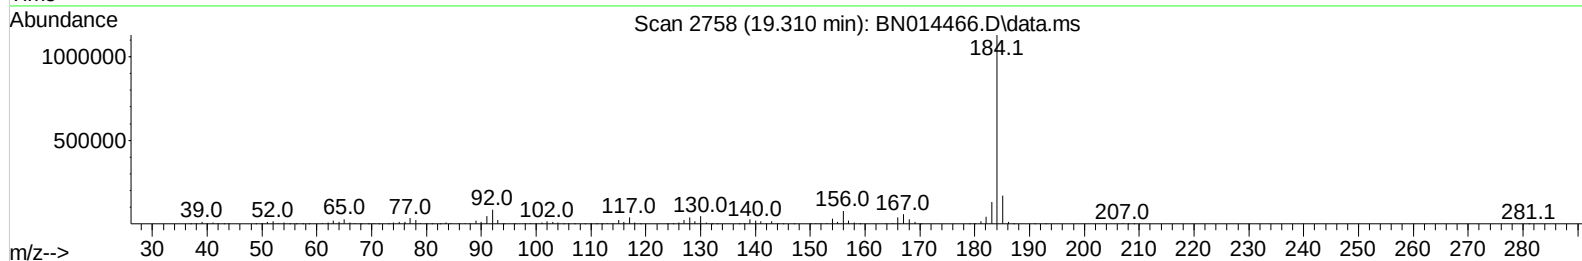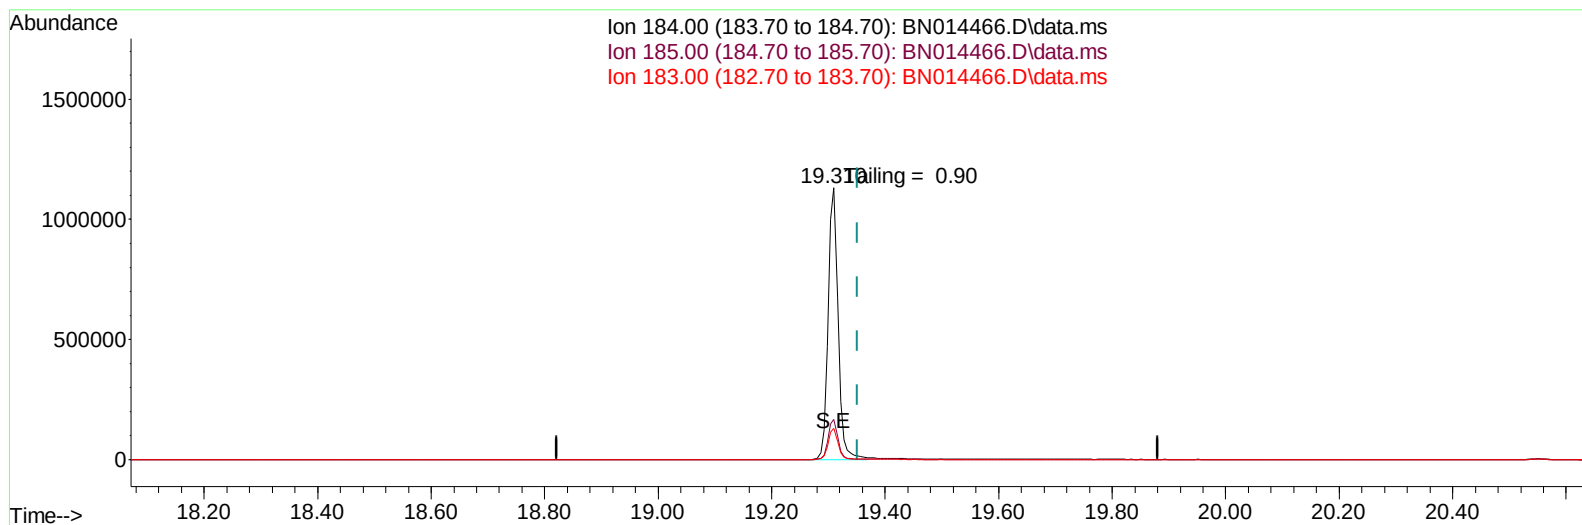

TIC: BN014466.D\data.ms

(77) Benzidine

19.310min (-0.041) 0.00 ng

response 1398049

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.87
183.00	13.20	11.48
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/28/2021	BNA_N	<u>BN014466.D</u>
Compound Name	Response	Retention Time
DDT	668197	20.551
DDD	1250	20.11
DDE	685	19.598
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1935	670132	0.29

Instrument :
BNA_N
ClientSampleId :
DFTPP