
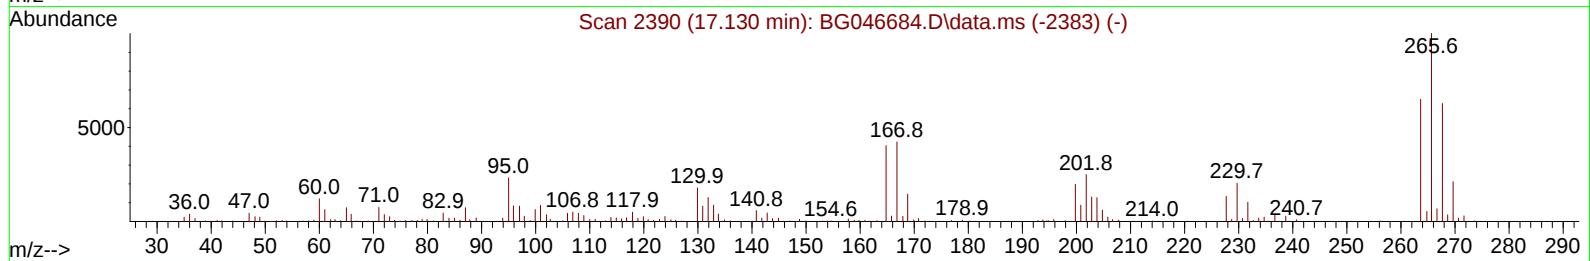
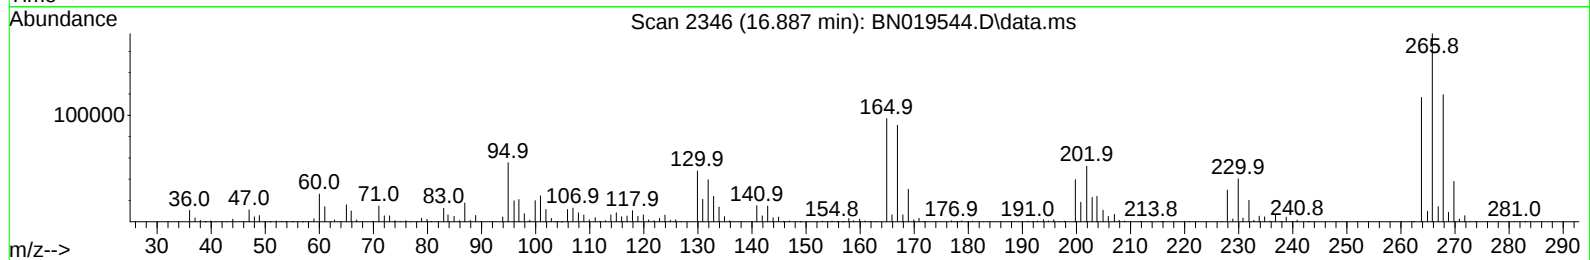


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042822\
Data File : BN019544.D
Acq On : 27 Apr 2022 14:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 08:26:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

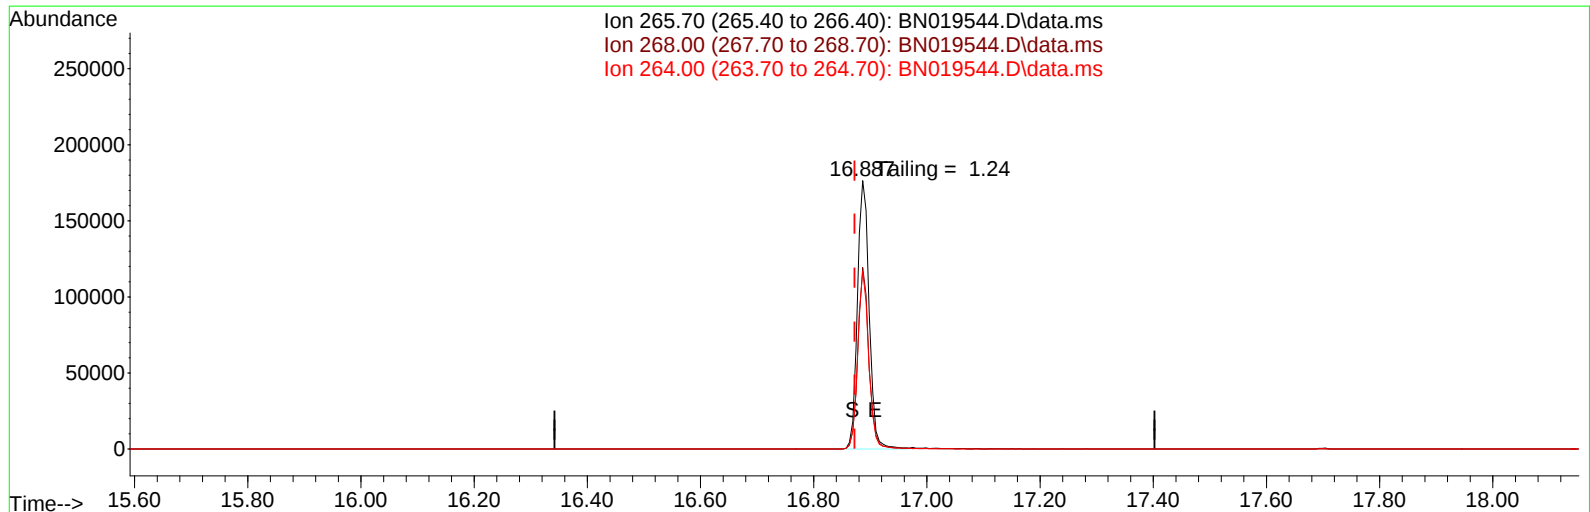

TIC: BN019544.D\data.ms

(70) Pentachlorophenol (C)




16.887min (+ 0.015) 21592.16 ng

response 253497

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.63
264.00	61.60	66.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042822\
Data File : BN019544.D
Acq On : 27 Apr 2022 14:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 08:26:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

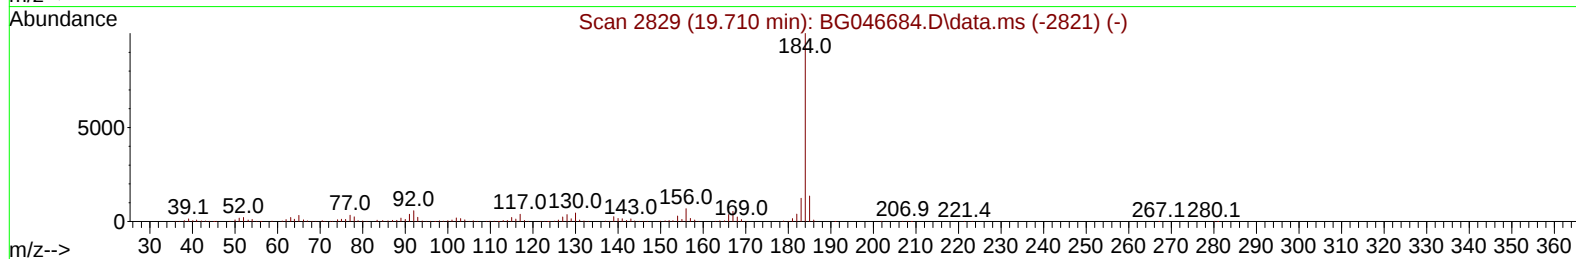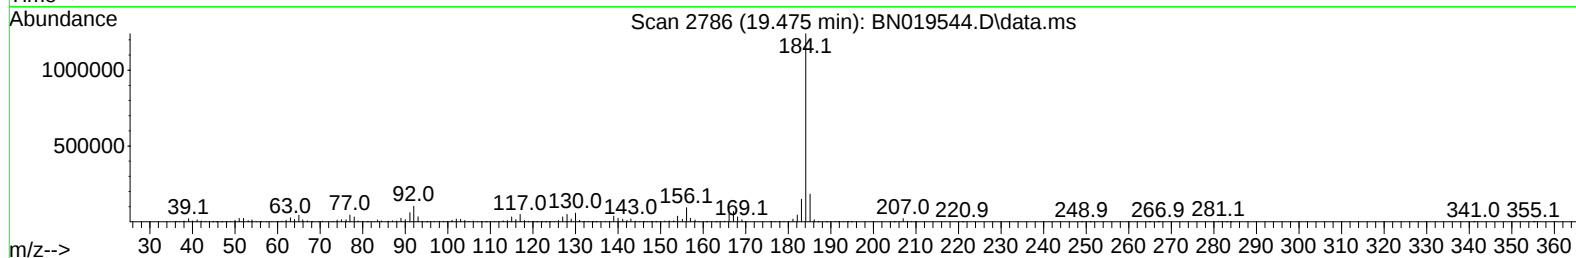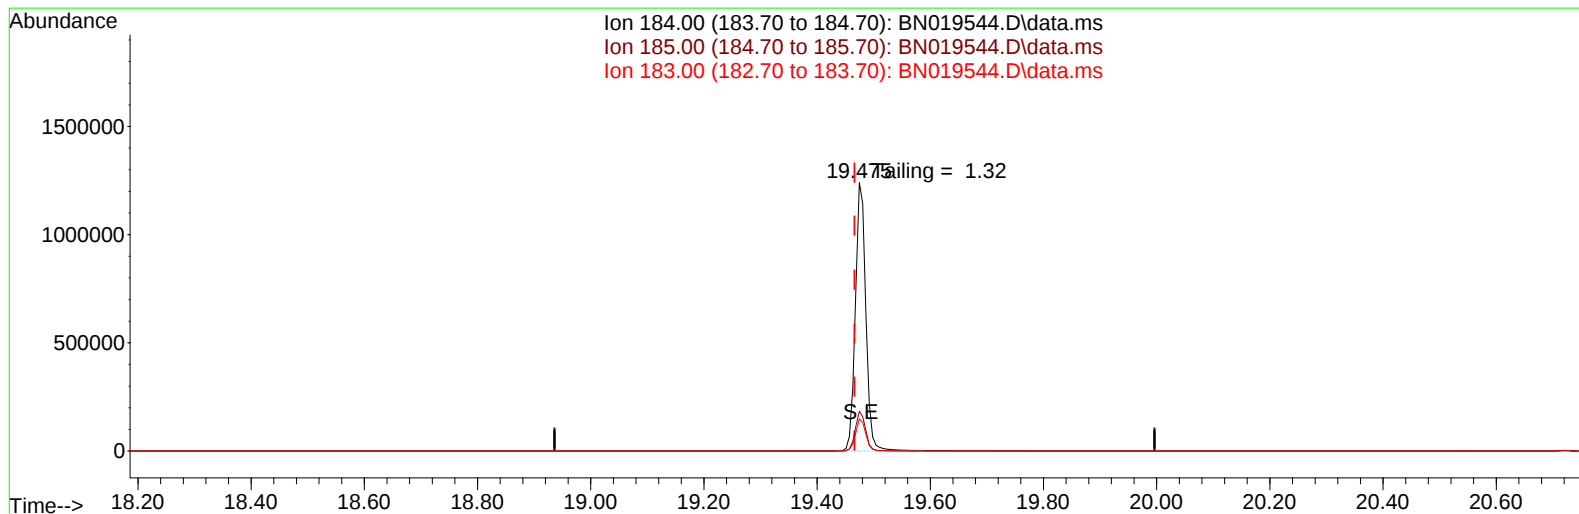

TIC: BN019544.D\data.ms

(77) Benzidine**19.475min (+ 0.009) 0.00 ng****response 1603037**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.78
183.00	13.20	12.02
0.00	0.00	0.00