
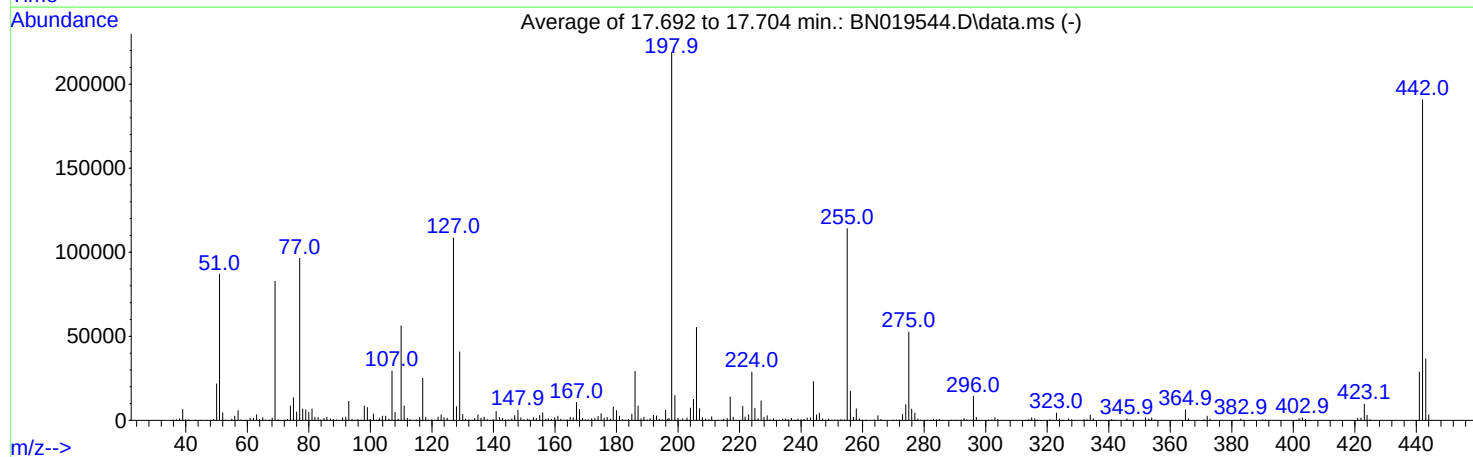


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042822\
 Data File : BN019544.D
 Acq On : 27 Apr 2022 14:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 28 02:56:24 2022

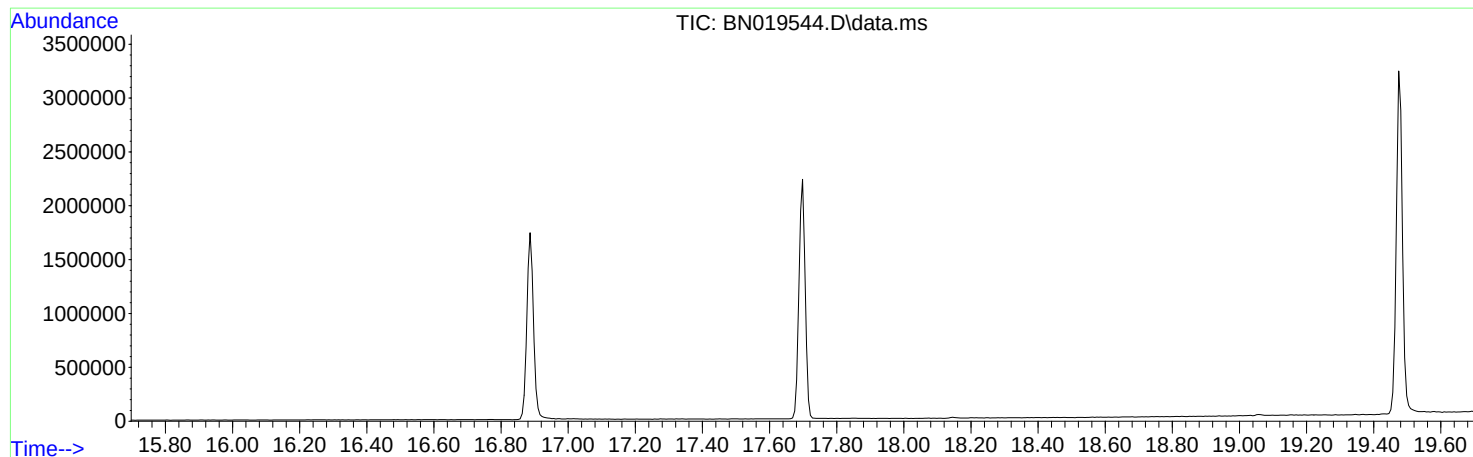




AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.7	86790	PASS
68	69	0.00	2	1.8	1455	PASS
69	198	0.00	100	37.8	82707	PASS
70	69	0.00	2	0.5	414	PASS
127	198	10	80	49.6	108485	PASS
197	198	0.00	2	0.5	1053	PASS
198	198	100	100	100.0	218816	PASS
199	198	5	9	6.7	14719	PASS
275	198	10	60	24.0	52557	PASS
365	198	1	100	2.9	6328	PASS
441	198	0.01	100	13.1	28712	PASS
442	442	50	100	100.0	190720	PASS
443	442	15	24	19.2	36523	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042822\
Data File : BN019544.D
Acq On : 27 Apr 2022 14:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 28 08:26:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

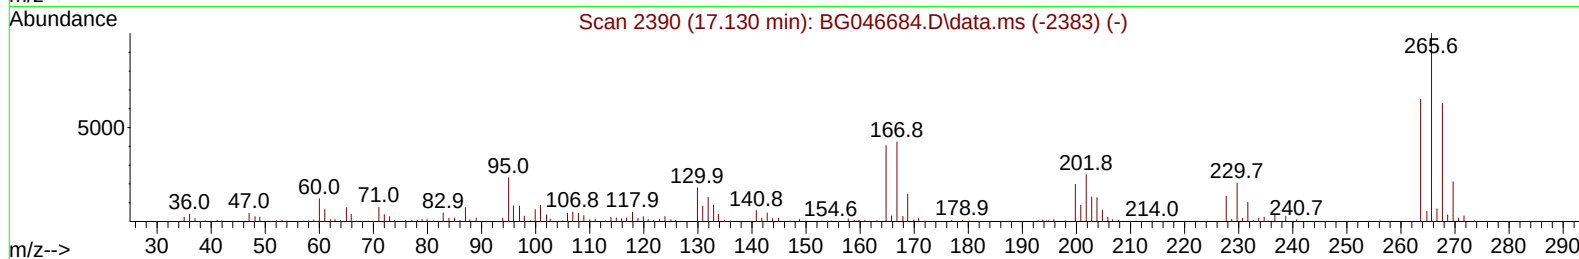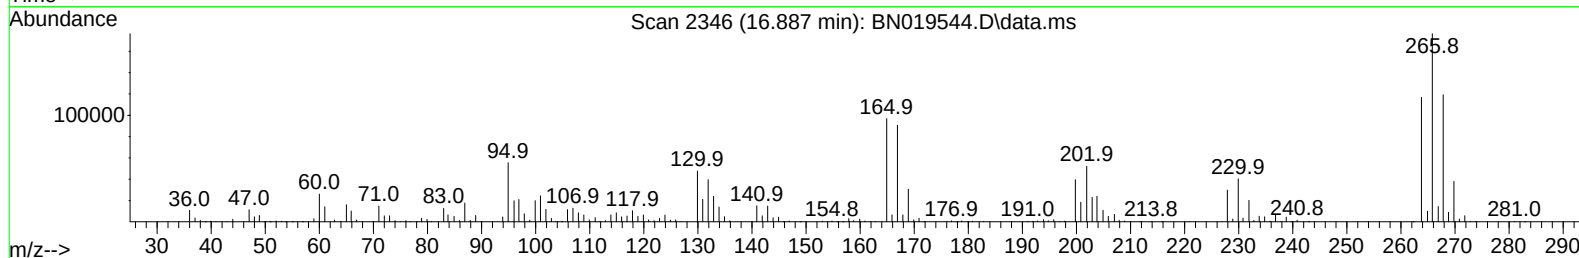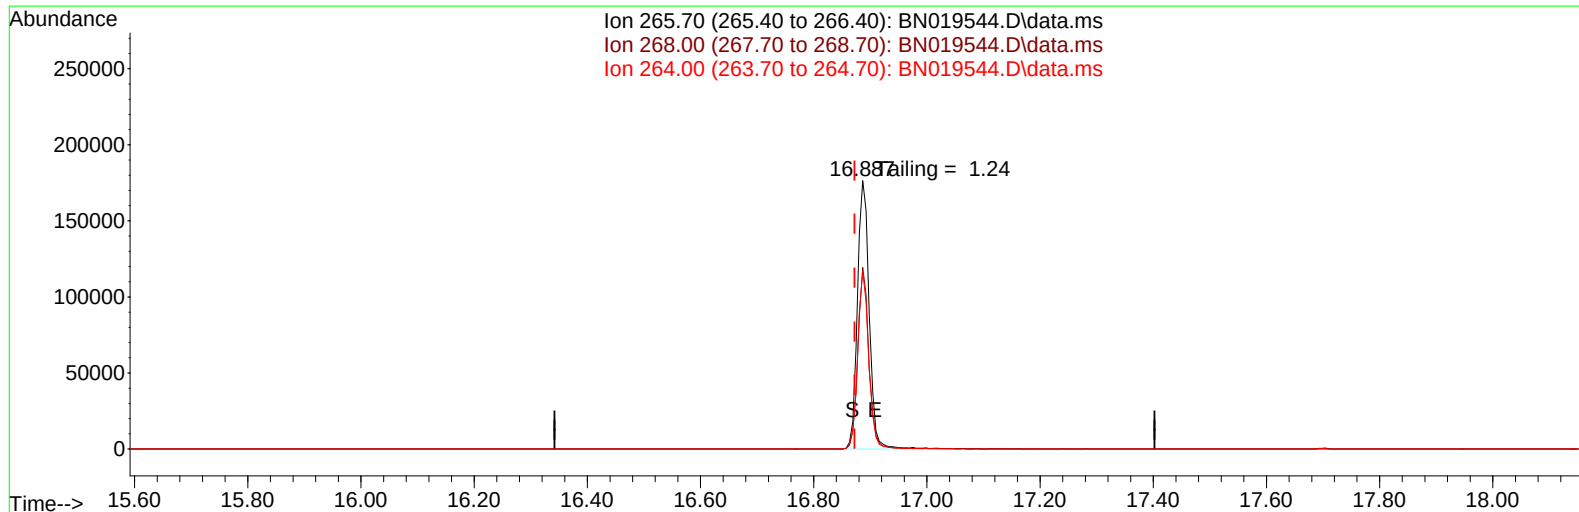

TIC: BN019544.D\data.ms

(70) Pentachlorophenol (C)

16.887min (+ 0.015) 21592.16 ng




response 253497

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.63
264.00	61.60	66.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042822\
Data File : BN019544.D
Acq On : 27 Apr 2022 14:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 28 08:26:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

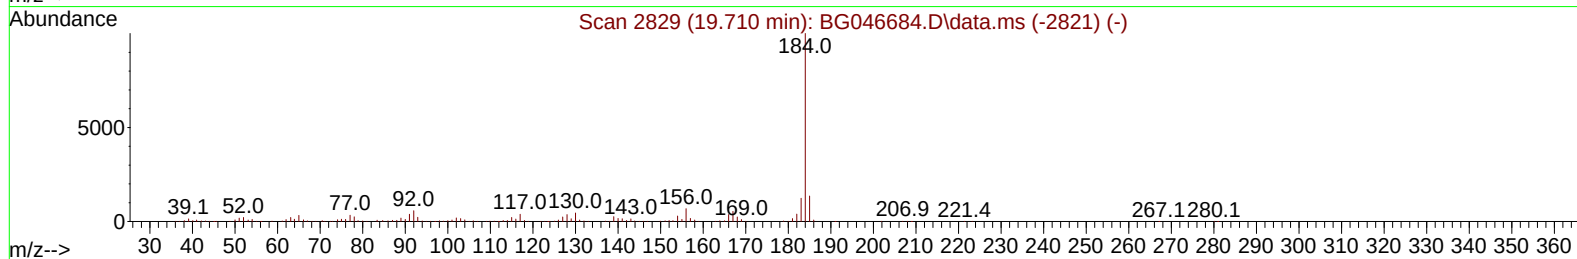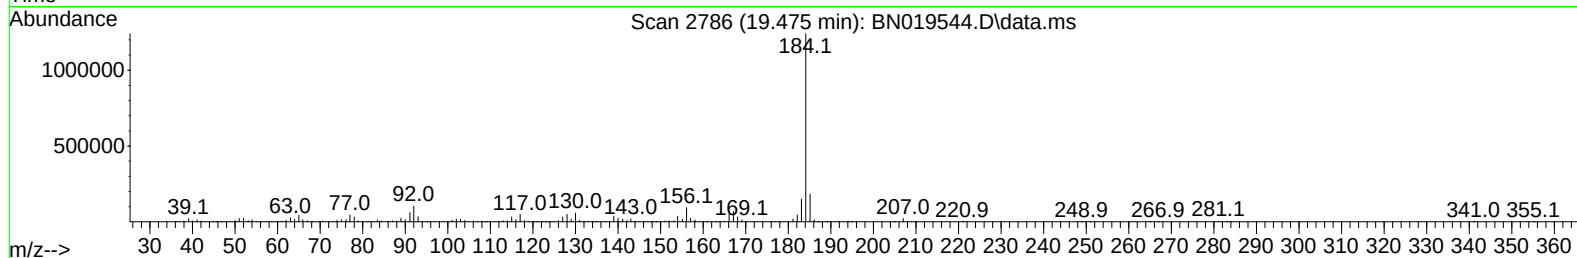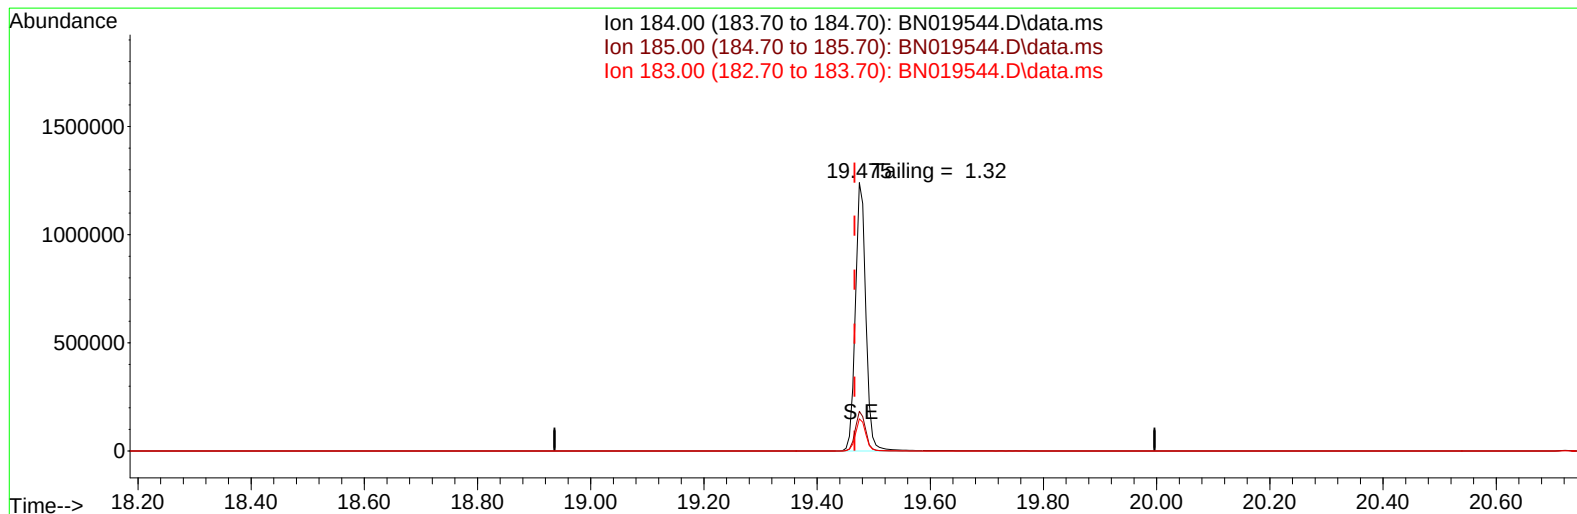

TIC: BN019544.D\data.ms

(77) Benzidine

19.475min (+ 0.009) 0.00 ng

response 1603037

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.78
183.00	13.20	12.02
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/28/2022	BNA_N	<u>BN019544.D</u>
Compound Name	Response	Retention Time
DDT	705763	20.722
DDD	7242	20.28
DDE	0	19.9
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7242	713005	1.02