
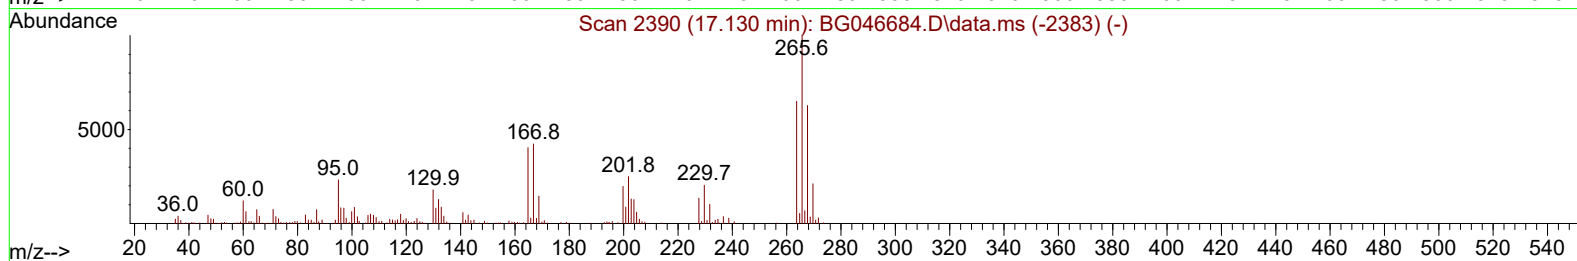
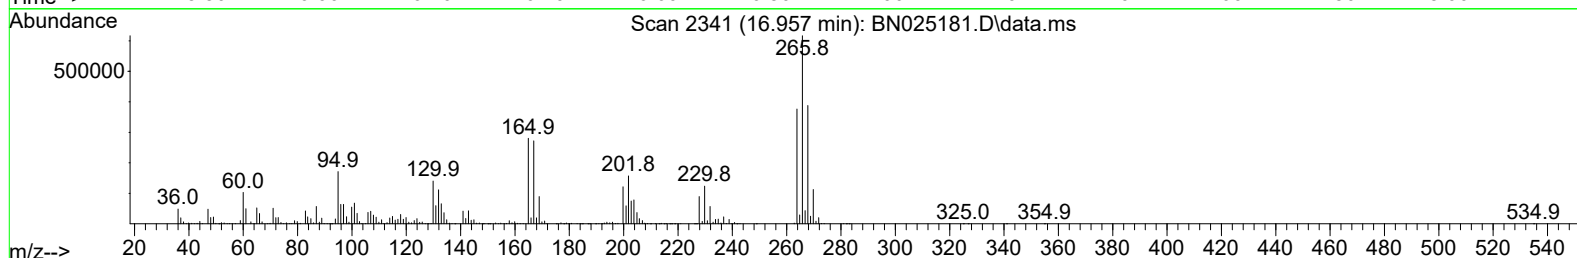


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042823\
Data File : BN025181.D
Acq On : 28 Apr 2023 08:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 01 06:00:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 01 06:00:29 2023
Response via : Initial Calibration

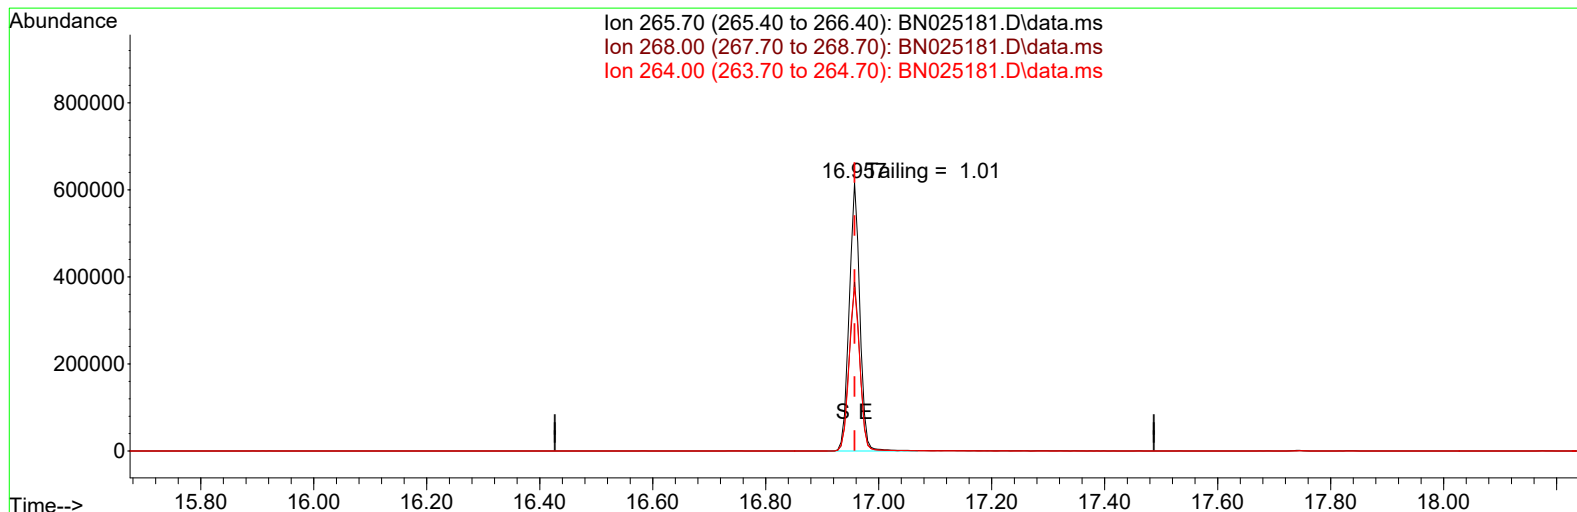

TIC: BN025181.D\data.ms

(70) Pentachlorophenol (C)




16.957min (0.000) 23335.58 ng

response 813105

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.93
264.00	61.60	61.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042823\
Data File : BN025181.D
Acq On : 28 Apr 2023 08:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 01 06:00:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 01 06:00:29 2023
Response via : Initial Calibration

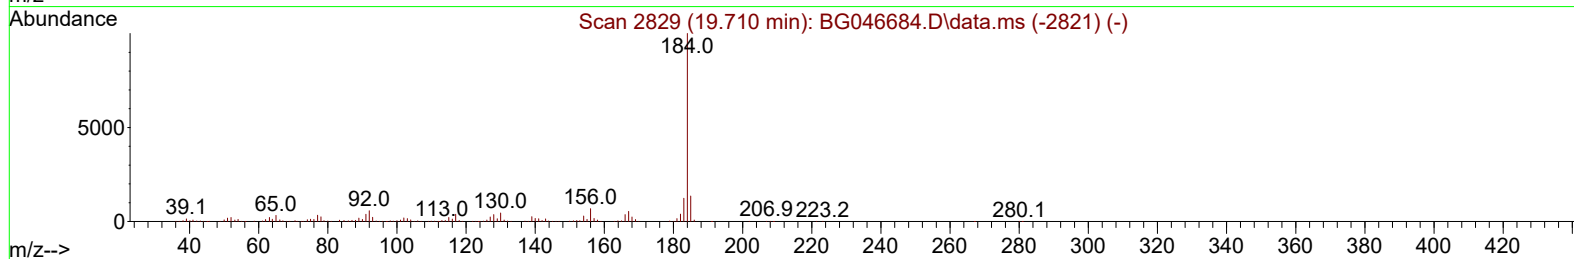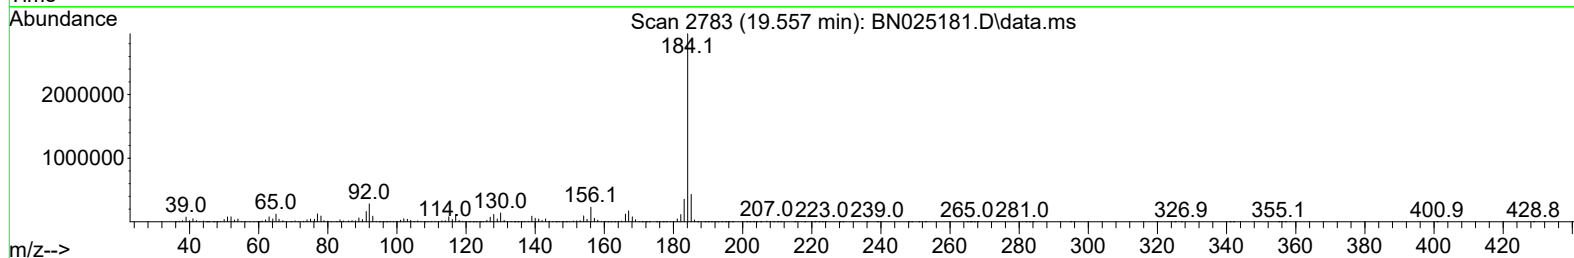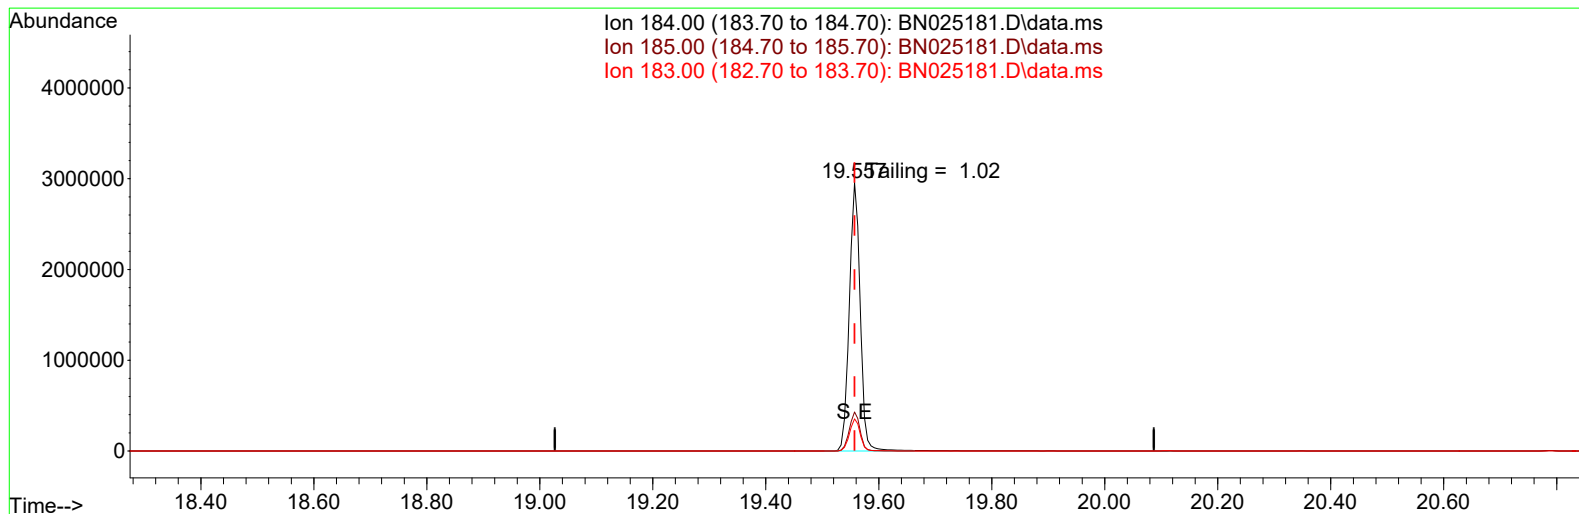

TIC: BN025181.D\data.ms

(77) Benzidine**19.557min (0.000) 709994.38 ng****response 3983223**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.58
183.00	13.20	11.98
0.00	0.00	0.00