

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042921\
 Data File : BN014488.D
 Acq On : 29 Apr 2021 13:16
 Operator : CG/JU
 Sample : SSTDICC1.6
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6

Quant Time: Apr 29 13:47:50 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 29 12:40:58 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.668	152	7471	0.40	ng	0.00
7) Naphthalene-d8	10.442	136	26159	0.40	ng	0.00
13) Acenaphthene-d10	14.295	164	13677	0.40	ng	0.00
19) Phenanthrene-d10	17.043	188	27031	0.40	ng	0.00
29) Chrysene-d12	21.250	240	26484	0.40	ng	0.00
35) Perylene-d12	23.465	264	20674	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.276	112	21840	1.55	ng	0.00
5) Phenol-d6	6.839	99	26839	1.54	ng	0.00
8) Nitrobenzene-d5	8.807	82	22790	1.31	ng	0.00
11) 2-Methylnaphthalene-d10	12.035	152	88717	2.25	ng	0.00
14) 2,4,6-Tribromophenol	15.793	330	6248	1.39	ng	0.00
15) 2-Fluorobiphenyl	12.925	172	88000	1.71	ng	0.00
27) Fluoranthene-d10	19.084	212	163140	2.20	ng	0.00
31) Terphenyl-d14	19.690	244	98977	1.87	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.231	88	13715	1.65	ng	97
3) n-Nitrosodimethylamine	3.569	42	6852	1.70	ng	# 95
6) bis(2-Chloroethyl)ether	7.104	93	30097	1.69	ng	99
9) Naphthalene	10.492	128	113932	1.76	ng	99
10) Hexachlorobutadiene	10.784	225	21533	1.72	ng	# 99
12) 2-Methylnaphthalene	12.111	142	74742	1.76	ng	99
16) Acenaphthylene	14.016	152	84606	1.58	ng	99
17) Acenaphthene	14.359	154	64556	1.71	ng	98
18) Fluorene	15.349	166	80386	1.70	ng	100
20) 4,6-Dinitro-2-methylph...	15.437	198	4098	1.73	ng	# 25
21) 4-Bromophenyl-phenylether	16.252	248	24767	1.75	ng	99
22) Hexachlorobenzene	16.362	284	32503	1.78	ng	100
23) Atrazine	16.520	200	12072	1.35	ng	97
24) Pentachlorophenol	16.702	266	5485	1.47	ng	98
25) Phenanthrene	17.092	178	132305	1.76	ng	100
26) Anthracene	17.177	178	101765	1.72	ng	100
28) Fluoranthene	19.114	202	149588	1.80	ng	99
30) Pyrene	19.481	202	140639	1.80	ng	100
32) Benzo(a)anthracene	21.229	228	118307	1.62	ng	99
33) Chrysene	21.282	228	147553	1.86	ng	100
34) Bis(2-ethylhexyl)phtha...	21.176	149	28836	0.93	ng	99
36) Indeno(1,2,3-cd)pyrene	25.687	276	149687	1.88	ng	100
37) Benzo(b)fluoranthene	22.801	252	134582	1.83	ng	95
38) Benzo(k)fluoranthene	22.846	252	152105	2.00	ng	95
39) Benzo(a)pyrene	23.369	252	116517	1.76	ng	# 93
40) Dibenzo(a,h)anthracene	25.704	278	127329	1.92	ng	96
41) Benzo(g,h,i)perylene	26.368	276	134152	1.91	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042921\
Data File : BN014488.D
Acq On : 29 Apr 2021 13:16
Operator : CG/JU
Sample : SSTDICC1.6
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Quant Time: Apr 29 13:47:50 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 29 12:40:58 2021
Response via : Initial Calibration




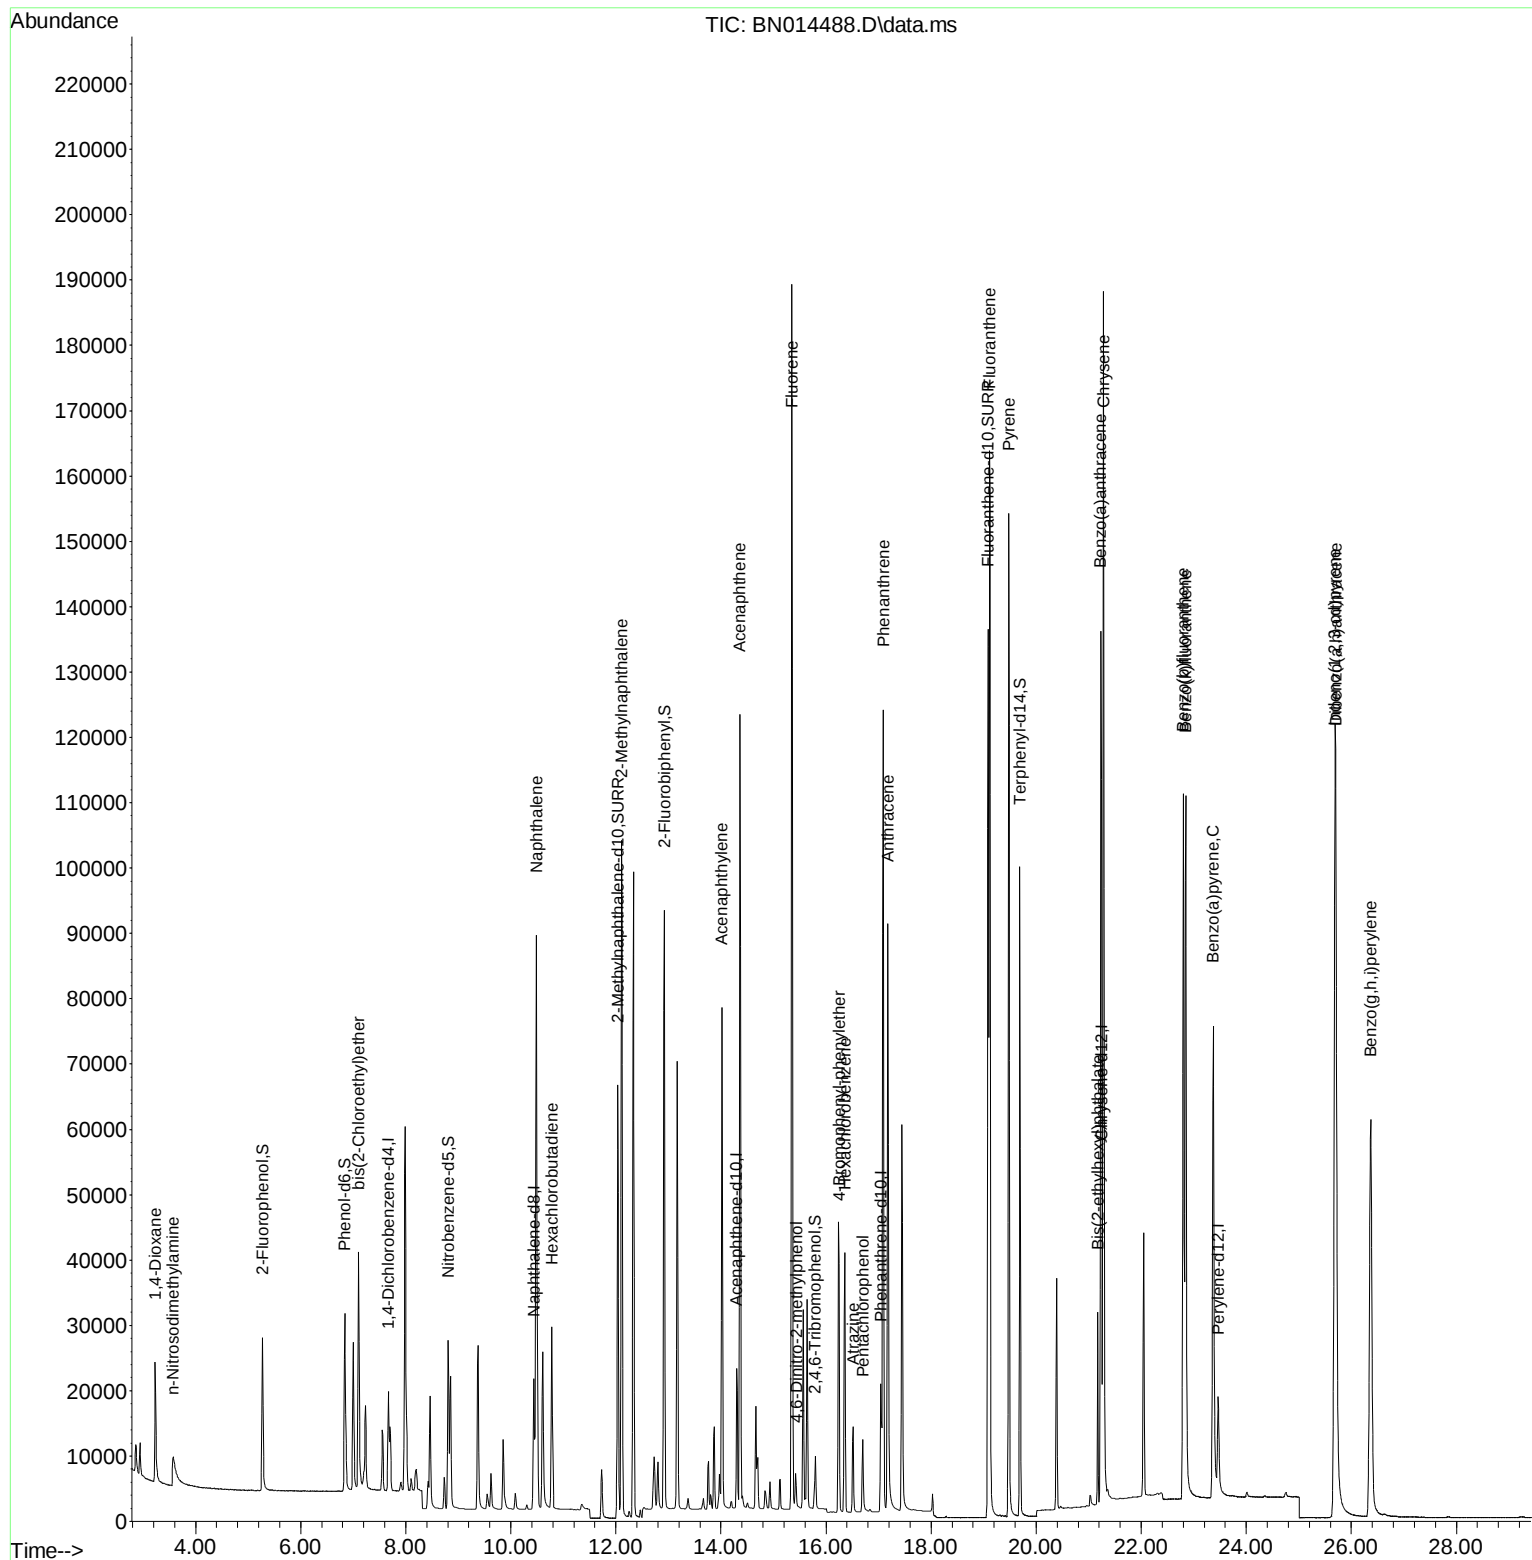


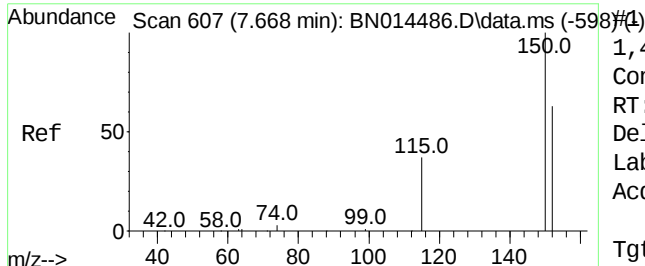

1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.668 min Scan# 607
 Delta R.T. 0.000 min
 Lab File: BN014488.D
 Acq: 29 Apr 2021 13:16




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6


Tgt Ion:	152	Resp:	7471
Ion	Ratio	Lower	Upper
152	100		
150	157.4	126.6	189.8
115	59.1	47.7	71.5

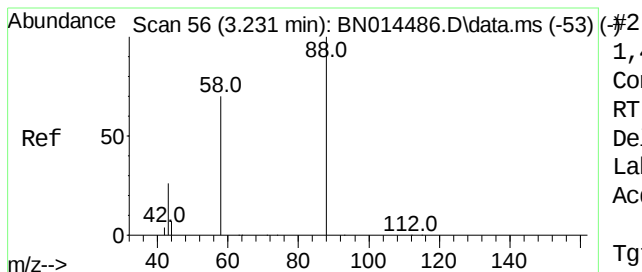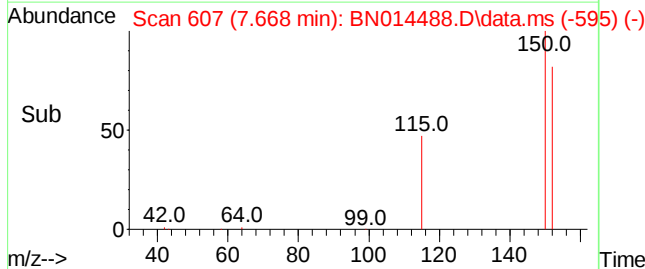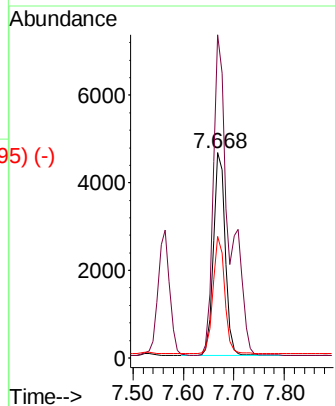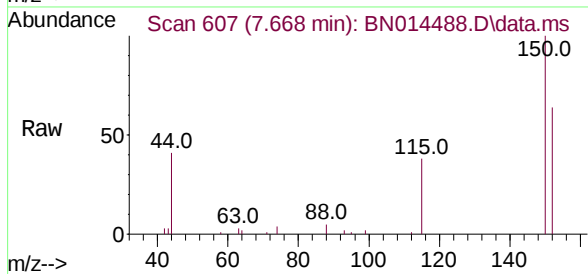

1,4-Dioxane
 Concen: 1.65 ng
 RT: 3.231 min Scan# 56
 Delta R.T. 0.000 min
 Lab File: BN014488.D
 Acq: 29 Apr 2021 13:16

Tgt Ion:	88	Resp:	13715
Ion	Ratio	Lower	Upper
88	100		
58	66.7	55.4	83.0
43	24.9	21.6	32.4


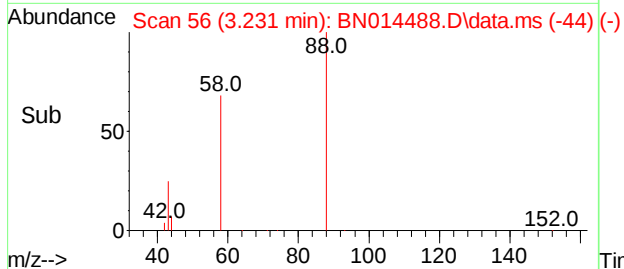
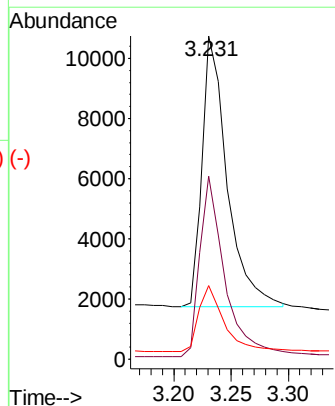
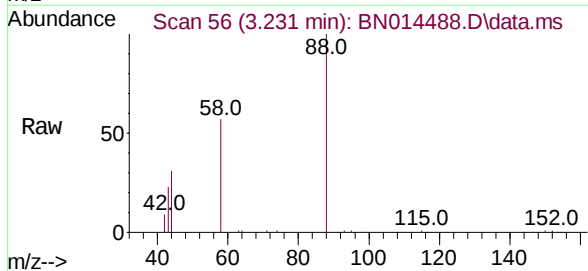


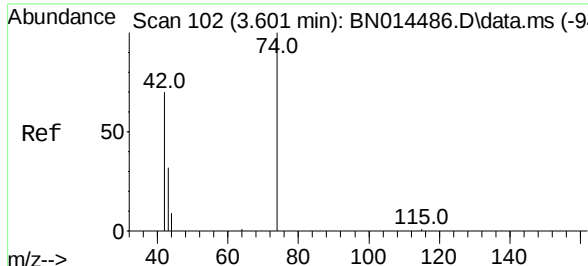

Scan 102 (3.601 min): BN014486.D\data.ms (-94) #3
 n-Nitrosodimethylamine
 Concen: 1.70 ng
 RT: 3.569 min Scan# 98
 Delta R.T. -0.032 min
 Lab File: BN014488.D
 Acq: 29 Apr 2021 13:16




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6


Tgt Ion:	42	Resp:	6852
Ion	Ratio	Lower	Upper
42	100		
74	144.2	120.3	180.5
44	4.8	6.7	10.1#

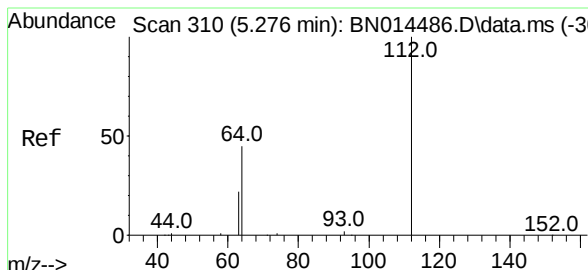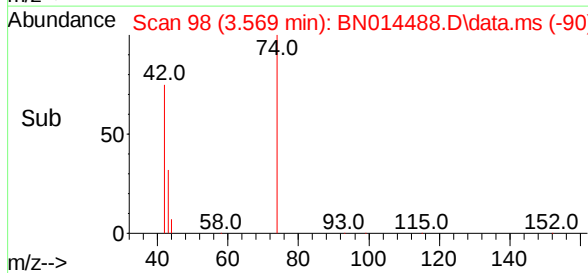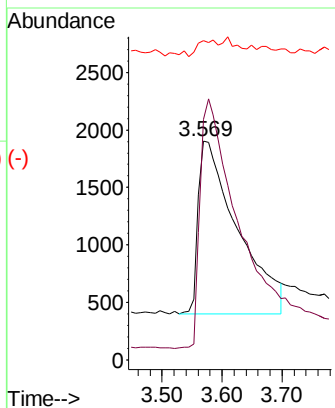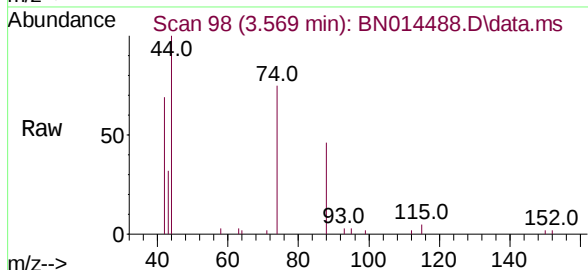

Scan 310 (5.276 min): BN014486.D\data.ms (-300) #4
 2-Fluorophenol
 Concen: 1.55 ng
 RT: 5.276 min Scan# 310
 Delta R.T. 0.000 min
 Lab File: BN014488.D
 Acq: 29 Apr 2021 13:16

Tgt Ion:	112	Resp:	21840
Ion	Ratio	Lower	Upper
112	100		
64	52.6	42.4	63.6
63	27.5	22.2	33.4


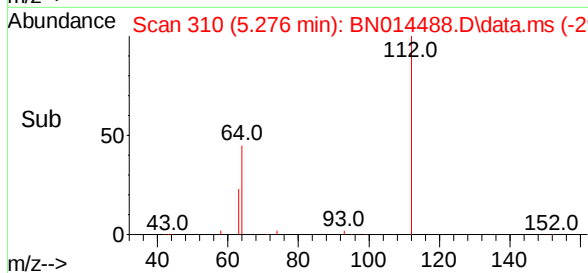
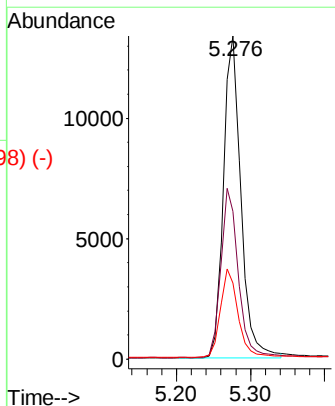
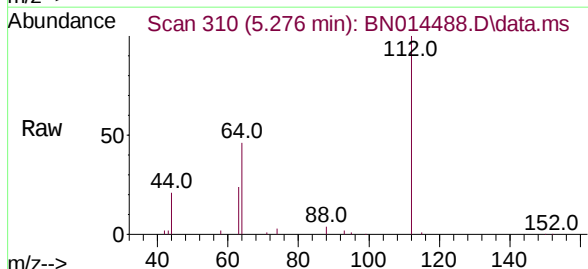


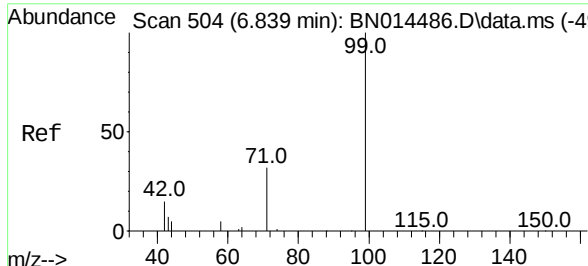

Phenol-d6
 Concen: 1.54 ng
 RT: 6.839 min Scan# 504
 Delta R.T. 0.000 min
 Lab File: BN014488.D
 Acq: 29 Apr 2021 13:16




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6

Tgt Ion:	99	Resp:	26839
Ion	Ratio	Lower	Upper
99	100		
42	17.2	13.8	20.8
71	32.1	26.0	39.0

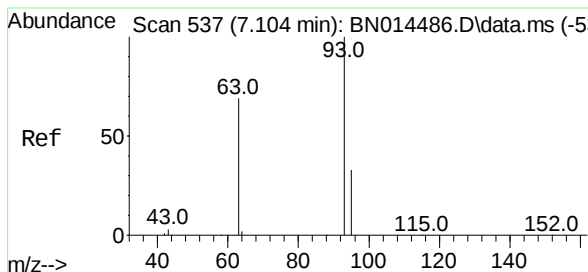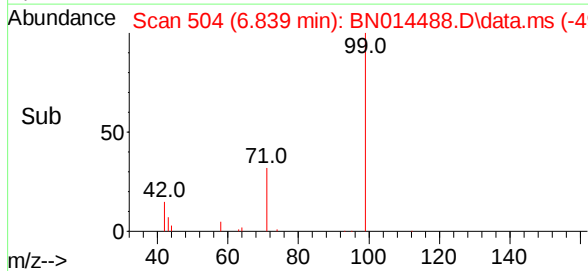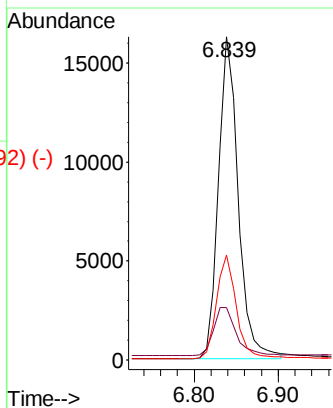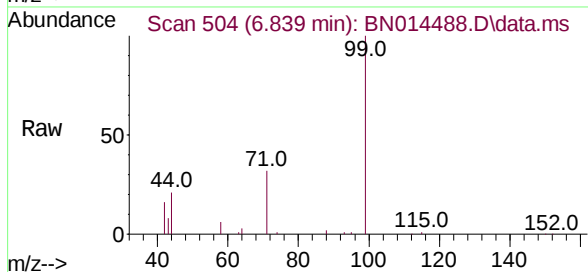

bis(2-Chloroethyl)ether
 Concen: 1.69 ng
 RT: 7.104 min Scan# 537
 Delta R.T. 0.000 min
 Lab File: BN014488.D
 Acq: 29 Apr 2021 13:16


Tgt Ion:	93	Resp:	30097
Ion	Ratio	Lower	Upper
93	100		
63	71.9	58.3	87.5
95	33.4	27.0	40.6

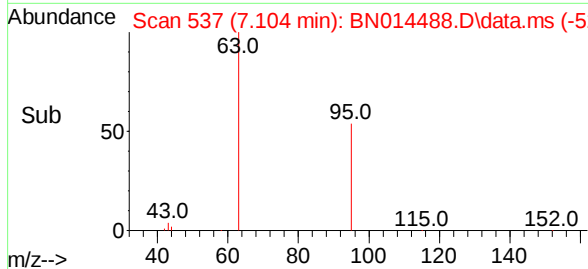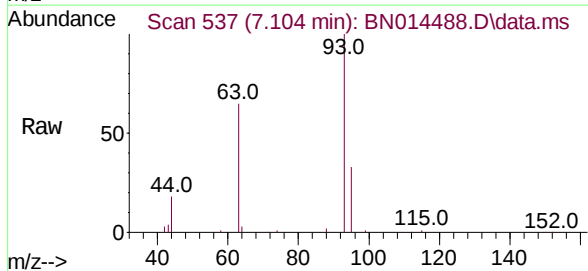




Abundance Scan 855 (10.442 min): BN014488.D\data.ms (-847) (-)

Naphthalene-d8
Concen: 0.40 ng
RT: 10.442 min Scan# 855
Delta R.T. 0.000 min
Lab File: BN014488.D
Acq: 29 Apr 2021 13:16

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

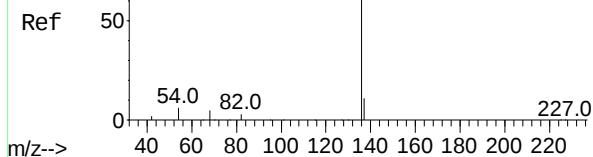




Tgt Ion:	136	Resp:	26159
Ion Ratio	Lower	Upper	
136	100		
137	11.0	9.0	13.6
54	5.7	4.8	7.2
68	5.6	4.6	6.8

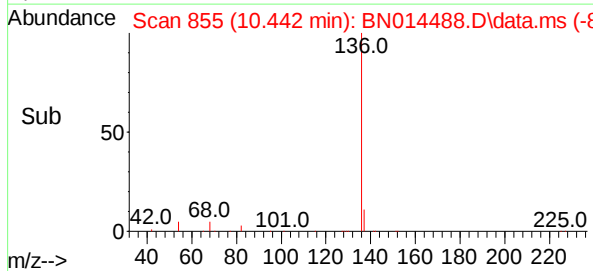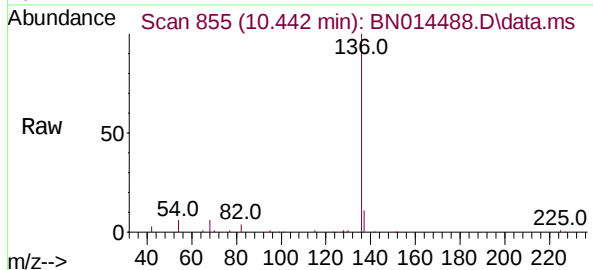


Abundance Scan 726 (8.807 min): BN014488.D\data.ms (-723) (-)

Nitrobenzene-d5
Concen: 1.31 ng
RT: 8.807 min Scan# 726
Delta R.T. 0.000 min
Lab File: BN014488.D
Acq: 29 Apr 2021 13:16

Tgt Ion:	82	Resp:	22790
Ion Ratio	Lower	Upper	
82	100		
128	33.8	26.0	39.0
54	47.5	39.5	59.3

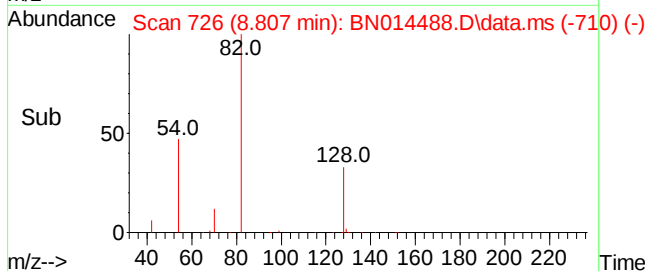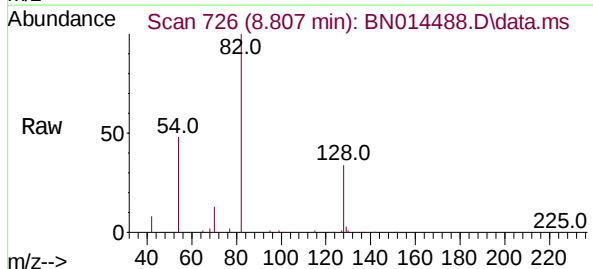




Abundance Scan 859 (10.492 min): BN014486.D\data.ms (-854) (-)




Naphthalene
Concen: 1.76 ng
RT: 10.492 min Scan# 859
Delta R.T. 0.000 min
Lab File: BN014488.D
Acq: 29 Apr 2021 13:16

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Tgt Ion:	128	Resp:	113932
Ion Ratio	Lower	Upper	
128	100		
129	11.0	9.0	13.6
127	12.6	10.2	15.4

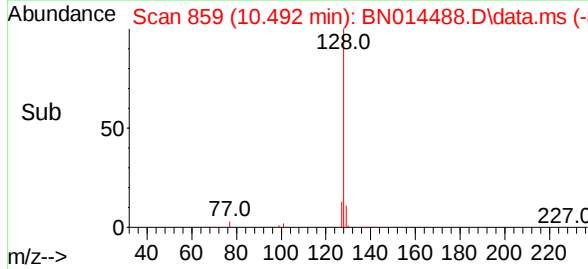
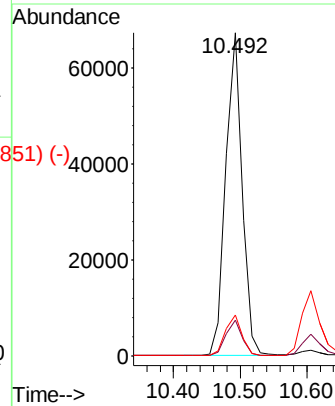
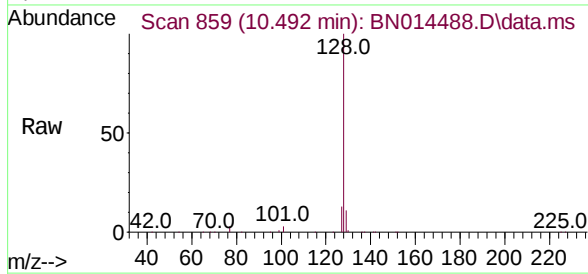


Abundance Scan 882 (10.784 min): BN014486.D\data.ms (-876) (-)



Hexachlorobutadiene
Concen: 1.72 ng
RT: 10.784 min Scan# 882
Delta R.T. 0.000 min
Lab File: BN014488.D
Acq: 29 Apr 2021 13:16


Tgt Ion:	225	Resp:	21533
Ion Ratio	Lower	Upper	
225	100		
223	0.0	0.0	0.0
227	64.0	51.8	77.6

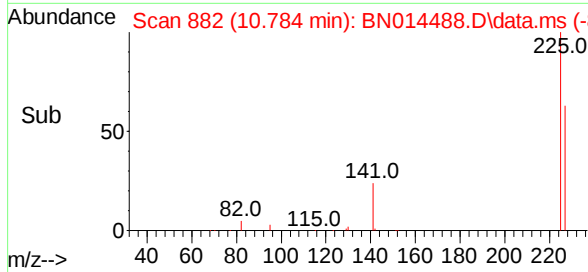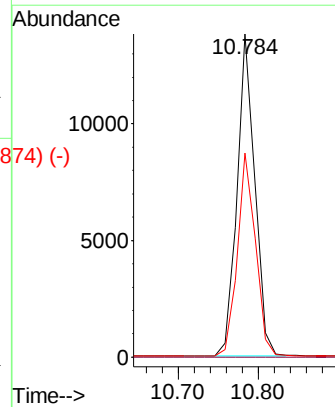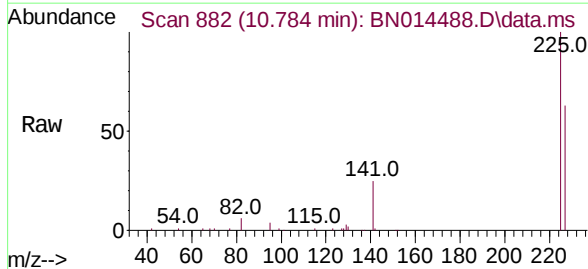




Abundance Scan 1058 (12.035 min): BN014488.D\data.ms (-1015) (-)

2-Methylnaphthalene-d10
Concen: 2.25 ng
RT: 12.035 min Scan# 1058
Delta R.T. 0.000 min
Lab File: BN014488.D
Acq: 29 Apr 2021 13:16

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

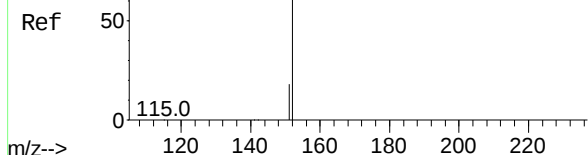





Tgt Ion:152 Resp: 88717
Ion Ratio Lower Upper
152 100
151 20.3 16.3 24.5

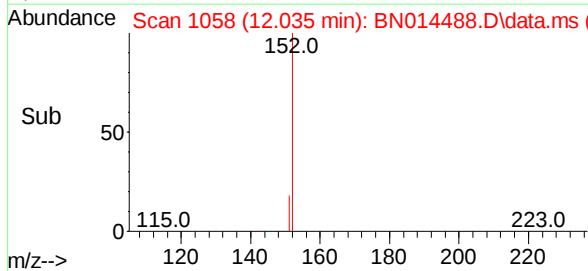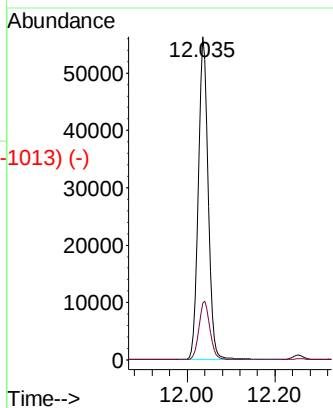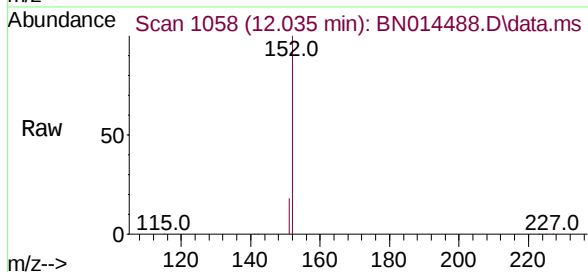

Abundance Scan 1075 (12.111 min): BN014488.D\data.ms (-1015) (-)

2-Methylnaphthalene
Concen: 1.76 ng
RT: 12.111 min Scan# 1075
Delta R.T. 0.000 min
Lab File: BN014488.D
Acq: 29 Apr 2021 13:16


Tgt Ion:142 Resp: 74742
Ion Ratio Lower Upper
142 100
141 87.6 70.5 105.7
115 33.7 27.5 41.3

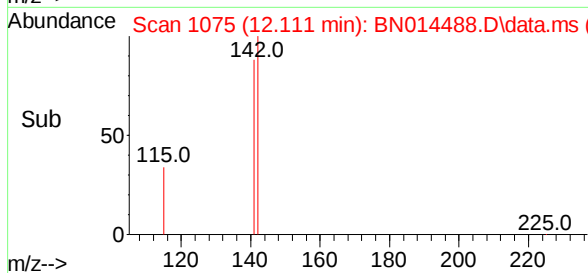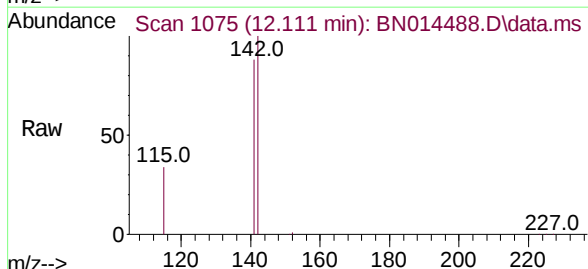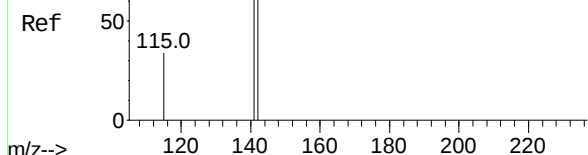



Abundance Scan 1305 (14.295 min): BN014488.D\data.ms (-1305) (-)

Acenaphthene-d10
Concen: 0.40 ng
RT: 14.295 min Scan# 1305
Delta R.T. 0.000 min
Lab File: BN014488.D
Acq: 29 Apr 2021 13:16


Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

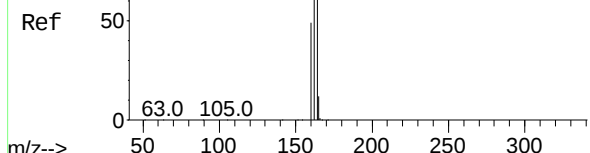

Tgt Ion:	164	Resp:	13677
Ion	Ratio	Lower	Upper
164	100		
162	102.9	82.4	123.6
160	49.7	40.5	60.7

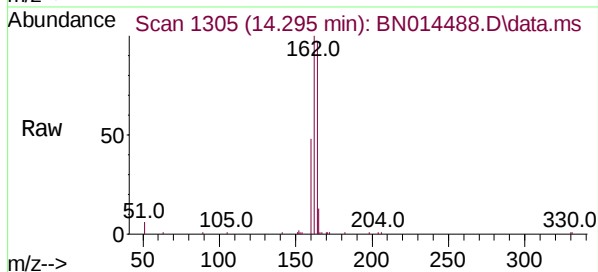



Abundance Scan 1305 (14.295 min): BN014488.D\data.ms (-1289) (-)

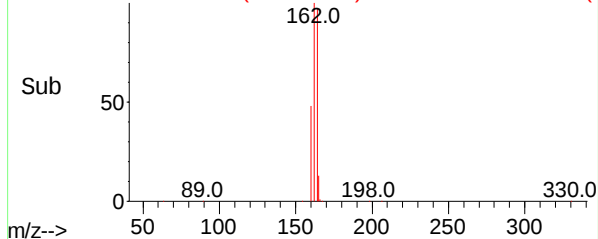


Abundance Scan 1423 (15.793 min): BN014488.D\data.ms (-1415) (-)

2,4,6-Tribromophenol
Concen: 1.39 ng
RT: 15.793 min Scan# 1423
Delta R.T. 0.000 min
Lab File: BN014488.D
Acq: 29 Apr 2021 13:16


Tgt Ion:	330	Resp:	6248
Ion	Ratio	Lower	Upper
330	100		
332	0.0	0.0	0.0
141	35.4	28.5	42.7

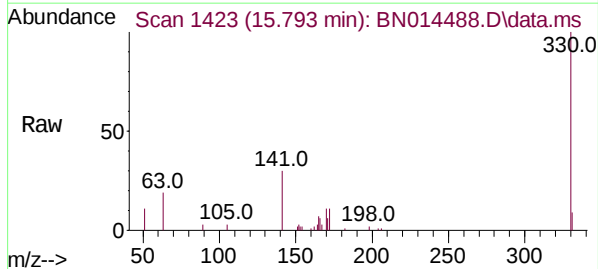

Abundance Scan 1423 (15.793 min): BN014488.D\data.ms (-1415) (-)

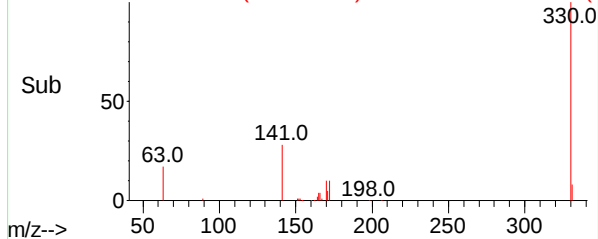



Abundance Scan 1197 (12.925 min): BN014488.D\data.ms (-1189) (-)

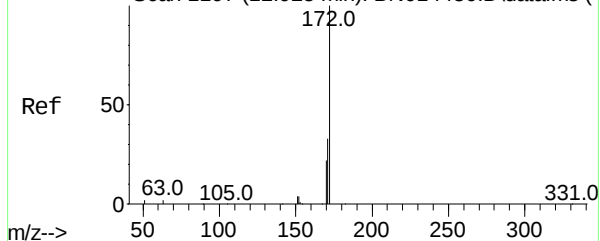


2-Fluorobiphenyl
Concen: 1.71 ng
RT: 12.925 min Scan# 1197
Delta R.T. 0.000 min
Lab File: BN014488.D
Acq: 29 Apr 2021 13:16

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:	172	Resp:	88000
Ion	Ratio	Lower	Upper
172	100		
171	33.3	26.6	40.0
170	21.8	18.2	27.2

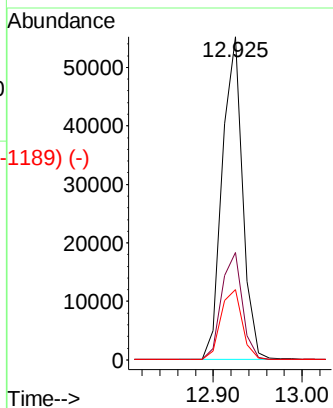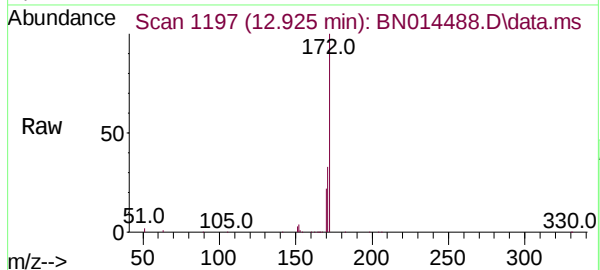

Abundance Scan 1197 (12.925 min): BN014488.D\data.ms (-1189) (-)


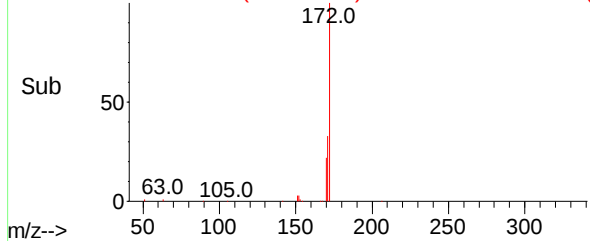


Abundance Scan 1283 (14.016 min): BN014488.D\data.ms (-1267) (-)

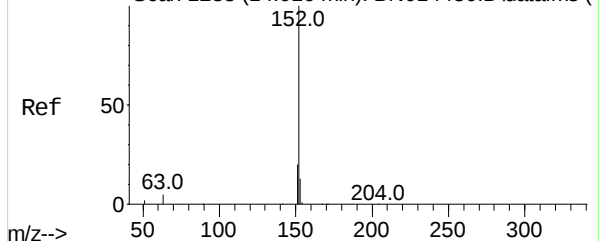


Acenaphthylene
Concen: 1.58 ng
RT: 14.016 min Scan# 1283
Delta R.T. 0.000 min
Lab File: BN014488.D
Acq: 29 Apr 2021 13:16


Tgt Ion:	152	Resp:	84606
Ion	Ratio	Lower	Upper
152	100		
151	19.2	15.6	23.4
153	13.0	10.7	16.1

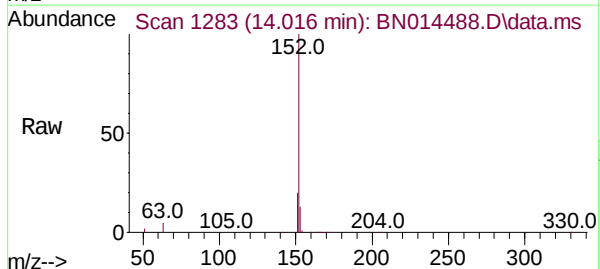

Abundance Scan 1283 (14.016 min): BN014488.D\data.ms (-1267) (-)

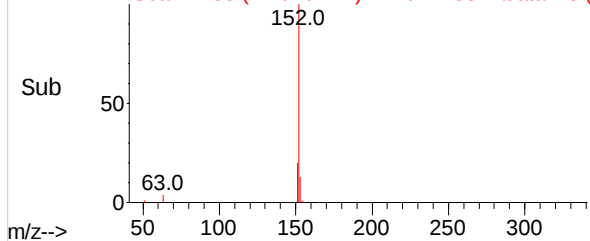



Abundance Scan 1310 (14.359 min): BN014488.D\data.ms (-1302) (-)




Acenaphthene
Concen: 1.71 ng
RT: 14.359 min Scan# 1310
Delta R.T. 0.000 min
Lab File: BN014488.D
Acq: 29 Apr 2021 13:16

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:	154	Resp:	64556
Ion	Ratio	Lower	Upper
154	100		
153	110.9	90.3	135.5
152	56.8	47.3	70.9

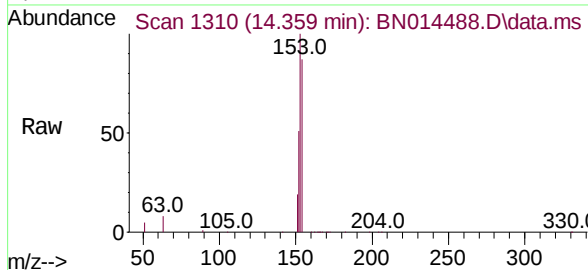

Abundance Scan 1310 (14.359 min): BN014488.D\data.ms (-1302) (-)


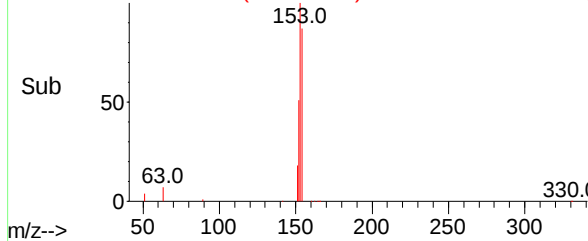


Abundance Scan 1388 (15.349 min): BN014488.D\data.ms (-1372) (-)




Fluorene
Concen: 1.70 ng
RT: 15.349 min Scan# 1388
Delta R.T. 0.000 min
Lab File: BN014488.D
Acq: 29 Apr 2021 13:16

Tgt Ion:	166	Resp:	80386
Ion	Ratio	Lower	Upper
166	100		
165	97.2	78.2	117.2
167	13.4	10.9	16.3

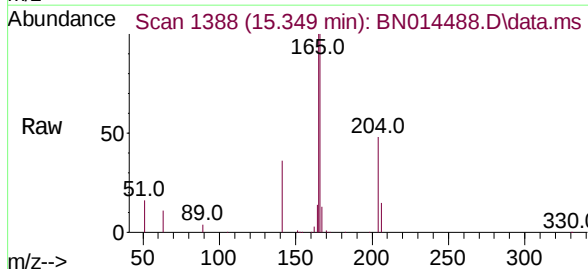


Abundance Scan 1388 (15.349 min): BN014488.D\data.ms (-1372) (-)

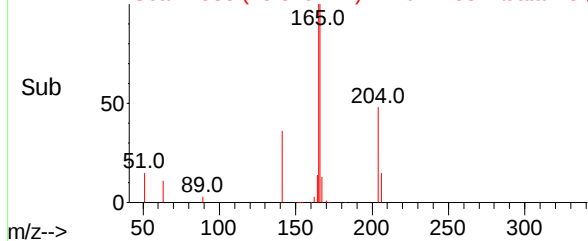




Abundance Scan 1525 (17.043 min): BN014488.D\data.ms (-1529) (-)

Phenanthrene-d10
Concen: 0.40 ng
RT: 17.043 min Scan# 1525
Delta R.T. 0.000 min
Lab File: BN014488.D
Acq: 29 Apr 2021 13:16

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

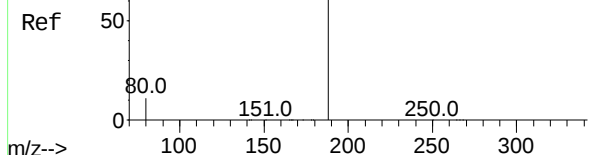


Tgt Ion:	188	Resp:	27031
Ion Ratio	Lower	Upper	
188	100		
94	0.0	0.0	0.0
80	11.3	8.8	13.2

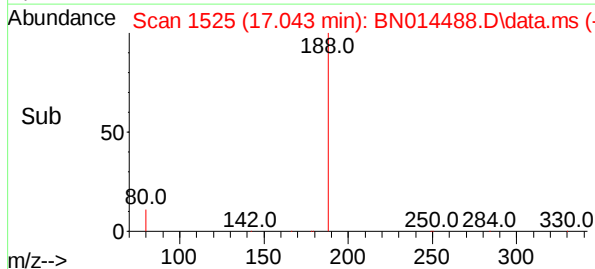

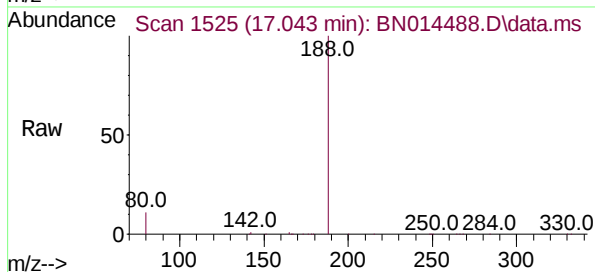


Abundance Scan 1395 (15.437 min): BN014488.D\data.ms (-1320) (-)


4,6-Dinitro-2-methylphenol
Concen: 1.73 ng
RT: 15.437 min Scan# 1395
Delta R.T. 0.000 min
Lab File: BN014488.D
Acq: 29 Apr 2021 13:16

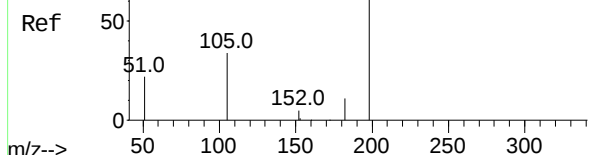

Tgt Ion:	198	Resp:	4098
Ion Ratio	Lower	Upper	
198	100		
51	36.0	116.0	174.0#
105	26.1	45.3	67.9#

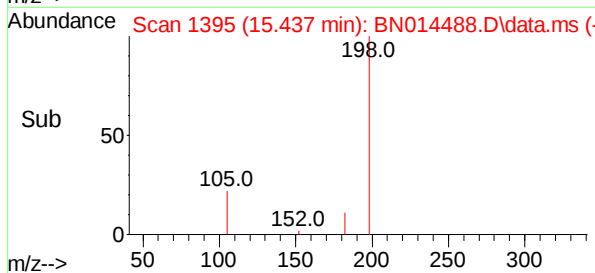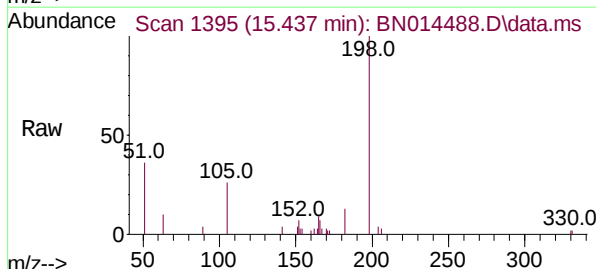




Abundance Scan 1460 (16.252 min): BN014486.D\data.ms (-1424) (-)

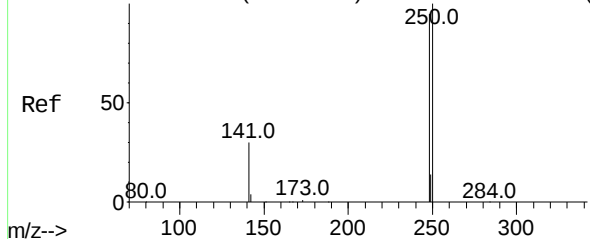


4-Bromophenyl-phenylether
Concen: 1.75 ng
RT: 16.252 min Scan# 1460
Delta R.T. 0.000 min
Lab File: BN014488.D
Acq: 29 Apr 2021 13:16

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Tgt Ion:	248	Resp:	24767
Ion	Ratio	Lower	Upper
248	100		
250	105.5	84.6	126.8
141	30.7	26.7	40.1

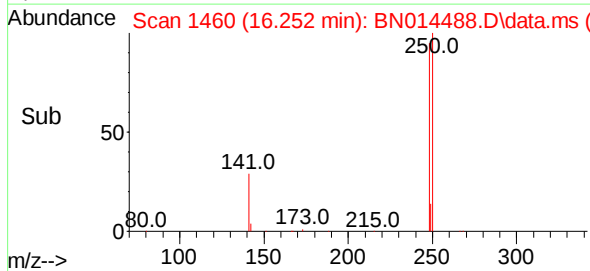
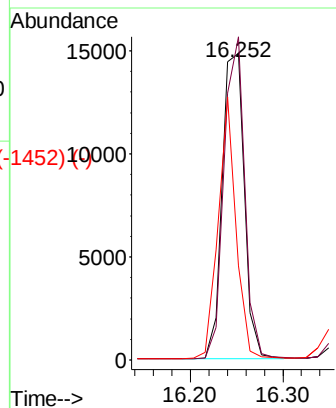
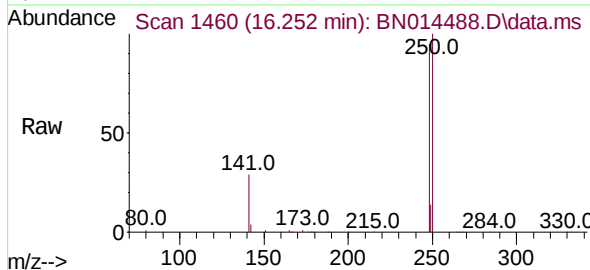


Abundance Scan 1469 (16.362 min): BN014486.D\data.ms (-1422) (-)

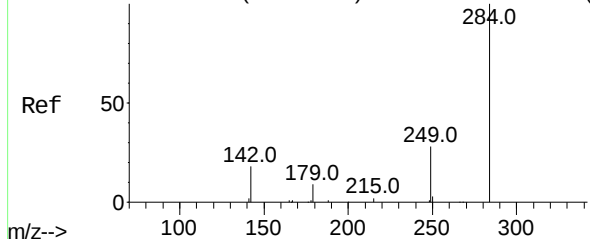

Hexachlorobenzene
Concen: 1.78 ng
RT: 16.362 min Scan# 1469
Delta R.T. 0.000 min
Lab File: BN014488.D
Acq: 29 Apr 2021 13:16


Tgt Ion:	284	Resp:	32503
Ion	Ratio	Lower	Upper
284	100		
142	34.1	27.0	40.6
249	29.7	23.6	35.4

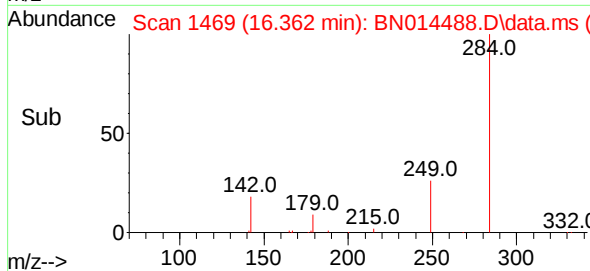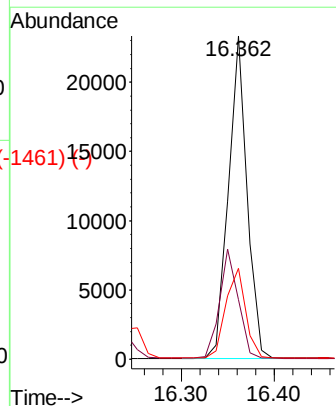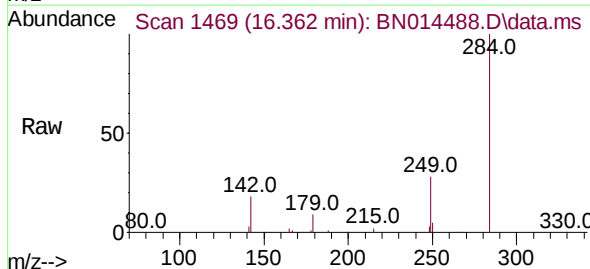



Abundance Scan 1482 (16.520 min): BN014486.D\data.ms (-1428) (-)

Atrazine
Concen: 1.35 ng
RT: 16.520 min Scan# 1482
Delta R.T. 0.000 min
Lab File: BN014488.D
Acq: 29 Apr 2021 13:16


Instrument :
BNA_N
ClientSampleId :
SSTDIC1.6

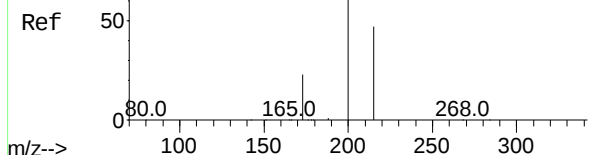

Tgt Ion	Ratio	Lower	Upper
200	100		
173	21.8	20.0	30.0
215	50.0	39.0	58.6

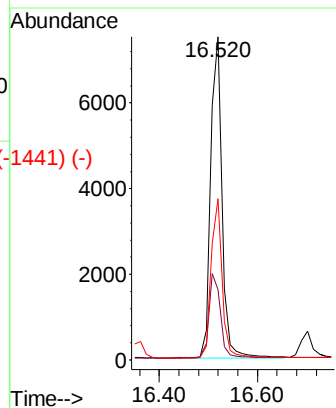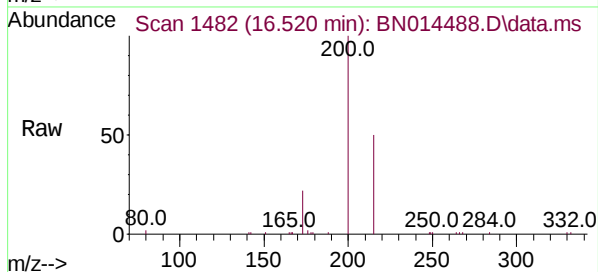




Abundance Scan 1482 (16.520 min): BN014488.D\data.ms (-1441) (-)

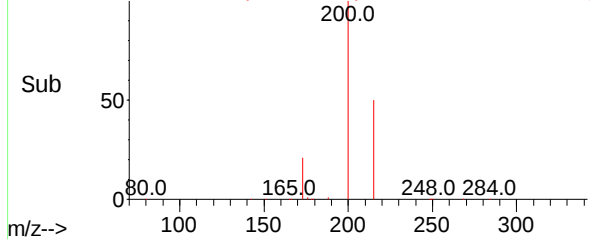


Abundance Scan 1497 (16.702 min): BN014486.D\data.ms (-1424) (-)

Pentachlorophenol
Concen: 1.47 ng
RT: 16.702 min Scan# 1497
Delta R.T. 0.000 min
Lab File: BN014488.D
Acq: 29 Apr 2021 13:16

Tgt Ion	Ratio	Lower	Upper
266	100		
264	63.2	49.9	74.9
268	64.0	49.9	74.9

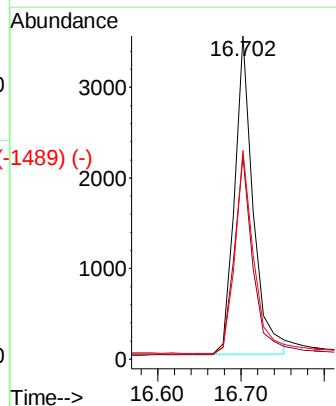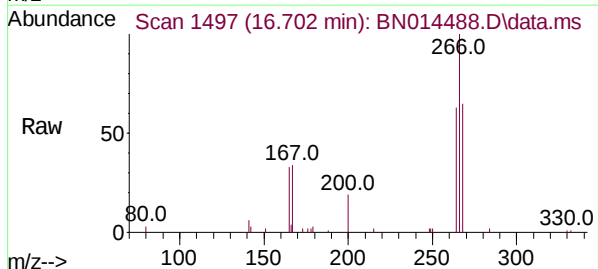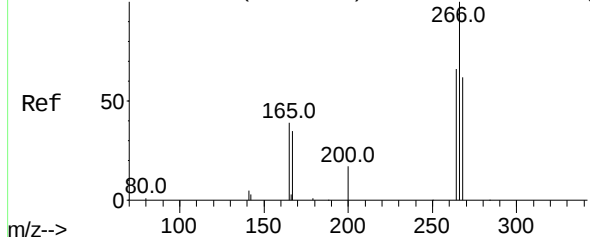


Abundance Scan 1497 (16.702 min): BN014488.D\data.ms (-1489) (-)

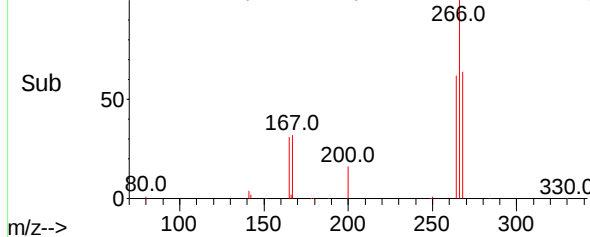



Abundance Scan 1529 (17.092 min): BN014486.D\data.ms (-1525) (-)

Phenanthrene
Concen: 1.76 ng
RT: 17.092 min Scan# 1529
Delta R.T. 0.000 min
Lab File: BN014488.D
Acq: 29 Apr 2021 13:16


Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

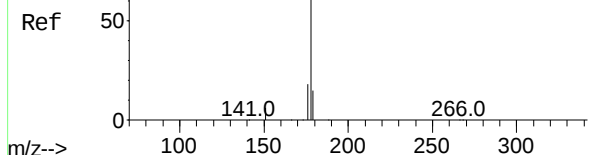

Tgt Ion	Ratio	Lower	Upper
178	100		
176	18.8	15.1	22.7
179	15.2	12.2	18.4

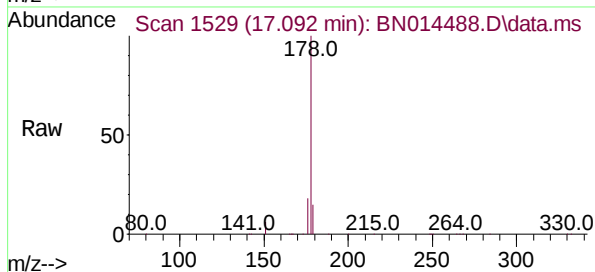




Abundance Scan 1529 (17.092 min): BN014488.D\data.ms (-1504) (-)

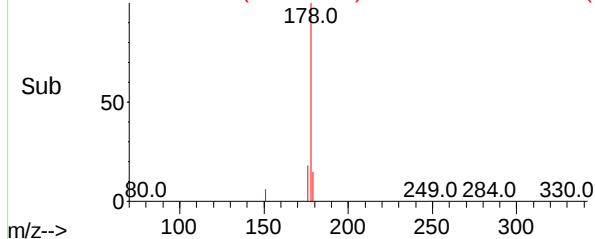


Abundance Scan 1536 (17.177 min): BN014486.D\data.ms (-1525) (-)

Anthracene
Concen: 1.72 ng
RT: 17.177 min Scan# 1536
Delta R.T. 0.000 min
Lab File: BN014488.D
Acq: 29 Apr 2021 13:16


Tgt Ion	Ratio	Lower	Upper
178	100		
176	18.3	14.6	22.0
179	15.4	12.2	18.2

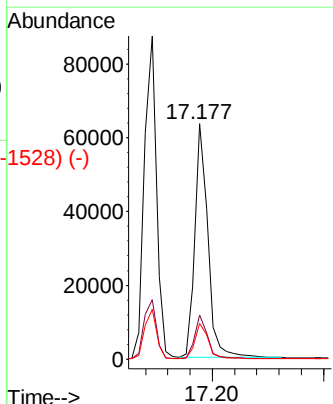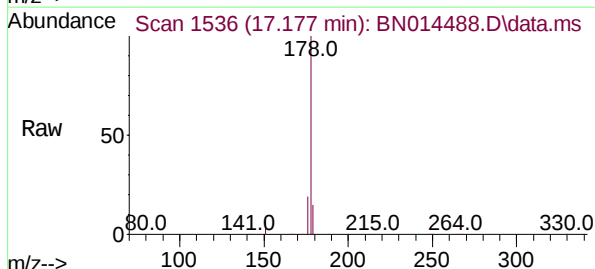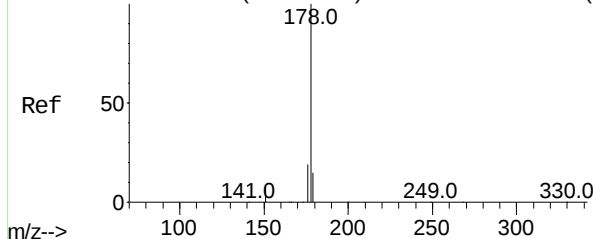

Abundance Scan 1536 (17.177 min): BN014488.D\data.ms (-1528) (-)

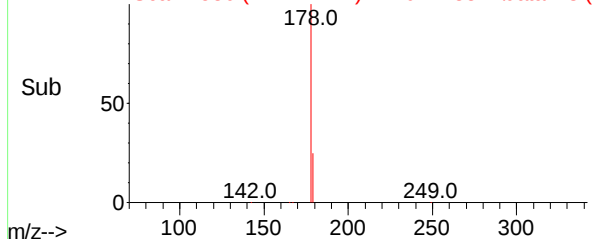



Abundance Scan 1820 (19.084 min): BN014486.D\data.ms (-1820) (-)




Fluoranthene-d10
Concen: 2.20 ng
RT: 19.084 min Scan# 1820
Delta R.T. 0.000 min
Lab File: BN014488.D
Acq: 29 Apr 2021 13:16

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:	212	Resp:	163140
Ion Ratio	Lower	Upper	
212	100		
106	12.7	10.2	15.4
104	6.9	5.6	8.4

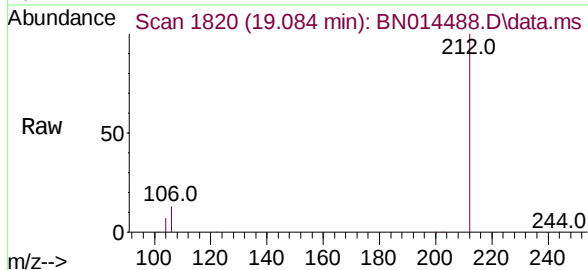

Abundance Scan 1820 (19.084 min): BN014488.D\data.ms (-1780) (-)


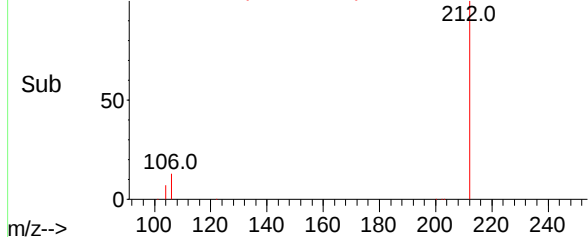


Abundance Scan 1826 (19.114 min): BN014486.D\data.ms (-1826) (-)




Fluoranthene
Concen: 1.80 ng
RT: 19.114 min Scan# 1826
Delta R.T. 0.000 min
Lab File: BN014488.D
Acq: 29 Apr 2021 13:16


Tgt Ion:	202	Resp:	149588
Ion Ratio	Lower	Upper	
202	100		
101	10.8	8.7	13.1
203	17.3	13.6	20.4

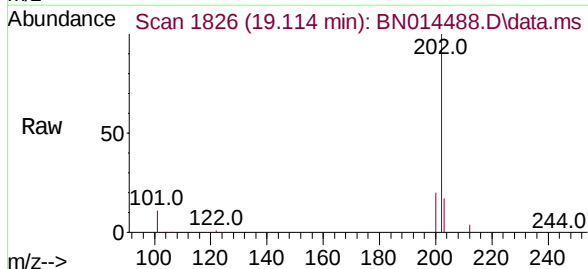

Abundance Scan 1826 (19.114 min): BN014488.D\data.ms (-1786) (-)






Abundance Scan 2123 (21.250 min): BN014486.D\data.ms (-2123) (-)

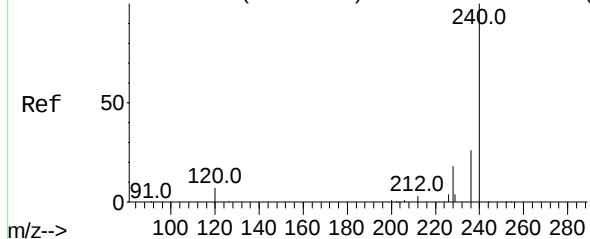


Chrysene-d12
Concen: 0.40 ng
RT: 21.250 min Scan# 2123
Delta R.T. 0.000 min
Lab File: BN014488.D
Acq: 29 Apr 2021 13:16

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Tgt Ion:240 Resp: 26484
Ion Ratio Lower Upper
240 100
120 7.4 6.3 9.5
236 25.5 20.9 31.3

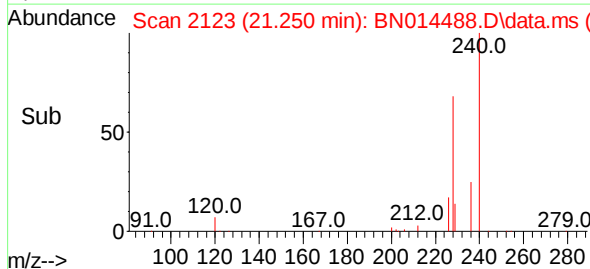
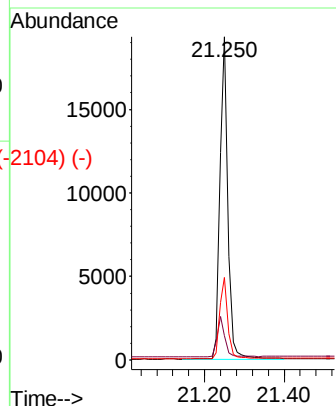
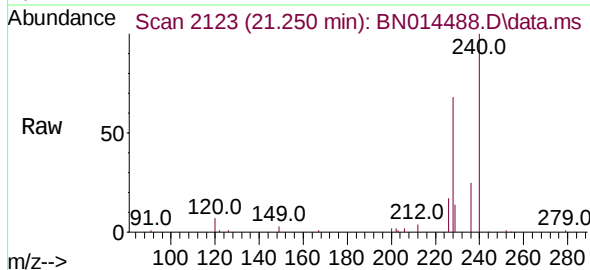


Abundance Scan 1900 (19.481 min): BN014486.D\data.ms (-1900) (-)

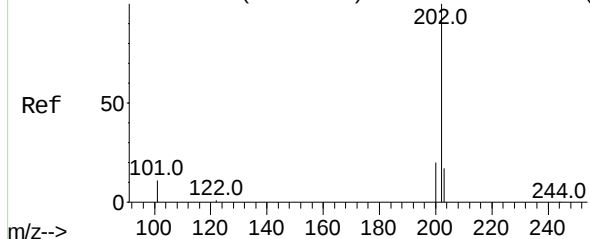


Pyrene
Concen: 1.80 ng
RT: 19.481 min Scan# 1900
Delta R.T. 0.000 min
Lab File: BN014488.D
Acq: 29 Apr 2021 13:16

Tgt Ion:202 Resp: 140639
Ion Ratio Lower Upper
202 100
200 20.5 16.4 24.6
203 17.4 13.9 20.9

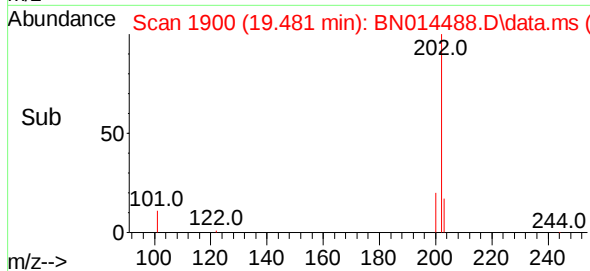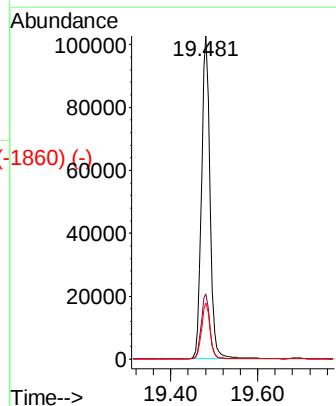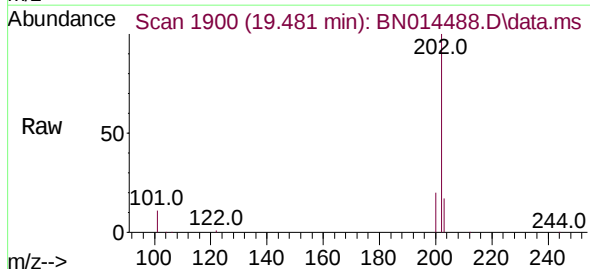



Abundance Scan 1942 (19.690 min): BN014488.D\data.ms (-1912) (-)




Terphenyl-d14
Concen: 1.87 ng
RT: 19.690 min Scan# 1942
Delta R.T. 0.000 min
Lab File: BN014488.D
Acq: 29 Apr 2021 13:16

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion	Ratio	Lower	Upper
244	100		
212	7.5	6.3	9.5
122	12.4	10.6	16.0

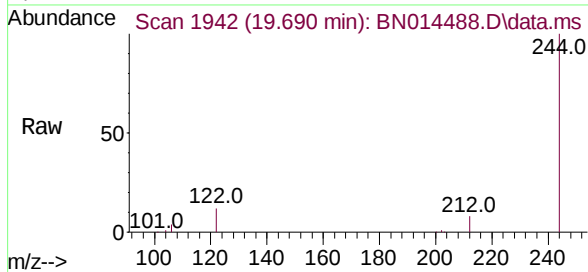

Abundance Scan 1942 (19.690 min): BN014488.D\data.ms (-1912) (-)





Abundance Scan 2121 (21.229 min): BN014488.D\data.ms (-2102) (-)




Benzo(a)anthracene
Concen: 1.62 ng
RT: 21.229 min Scan# 2121
Delta R.T. 0.000 min
Lab File: BN014488.D
Acq: 29 Apr 2021 13:16


Tgt Ion	Ratio	Lower	Upper
228	100		
226	27.5	21.8	32.8
229	19.0	15.8	23.6

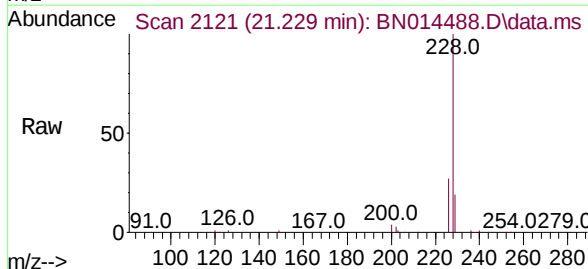

Abundance Scan 2121 (21.229 min): BN014488.D\data.ms (-2102) (-)



Abundance Scan 2126 (21.282 min): BN014486.D\data.ms (-2126) (-)

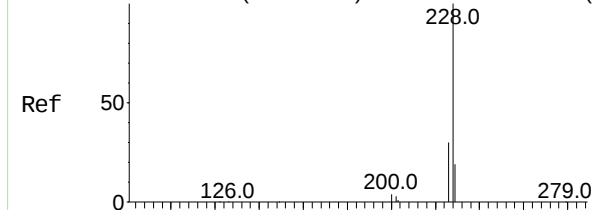


Chrysene
Concen: 1.86 ng
RT: 21.282 min Scan# 2126
Delta R.T. 0.000 min
Lab File: BN014488.D
Acq: 29 Apr 2021 13:16

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


m/z-->

Abundance Scan 2126 (21.282 min): BN014488.D\data.ms

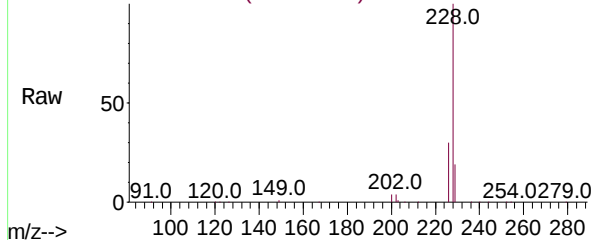


m/z-->


Abundance Scan 2126 (21.282 min): BN014488.D\data.ms (-2117) (-)

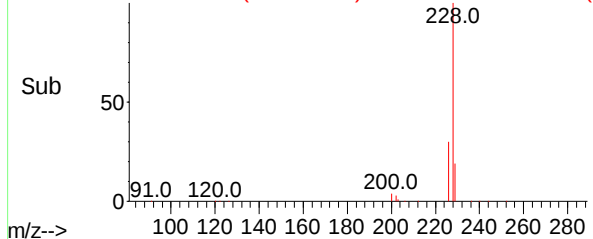

m/z-->




Abundance Scan 2116 (21.176 min): BN014486.D\data.ms (-2116) (-)

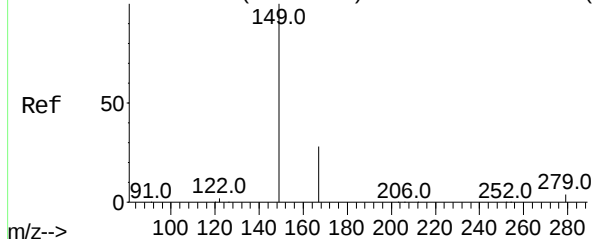

Bis(2-ethylhexyl)phthalate
Concen: 0.93 ng
RT: 21.176 min Scan# 2116
Delta R.T. 0.000 min
Lab File: BN014488.D
Acq: 29 Apr 2021 13:16


m/z-->

Abundance Scan 2116 (21.176 min): BN014488.D\data.ms

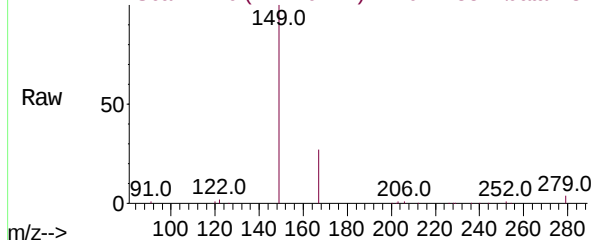


m/z-->

Abundance Scan 2116 (21.176 min): BN014488.D\data.ms (-2107) (-)

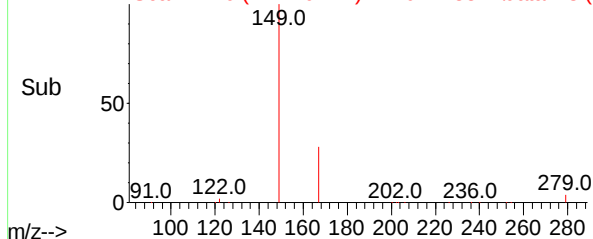


m/z-->

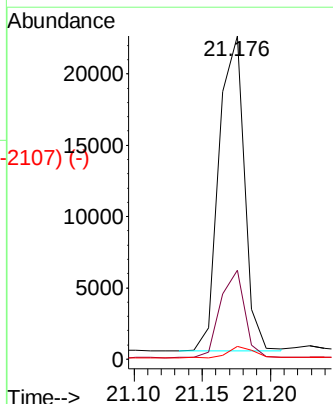




Abundance Scan 2541 (23.465 min): BN014488.D\data.ms (-2525) (-)

Perylene-d12
Concen: 0.40 ng
RT: 23.465 min Scan# 2541
Delta R.T. 0.000 min
Lab File: BN014488.D
Acq: 29 Apr 2021 13:16

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

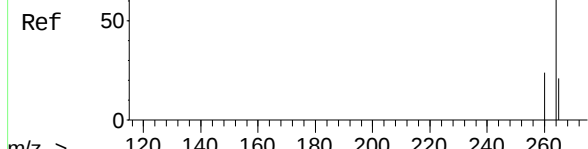





Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.9	19.6	29.4
265	42.7	35.5	53.3

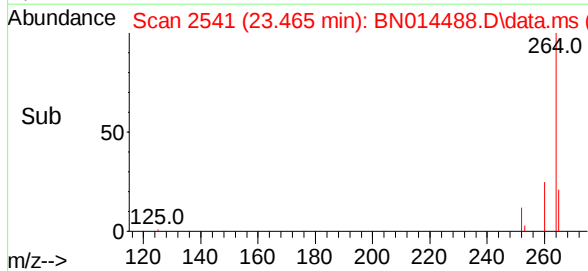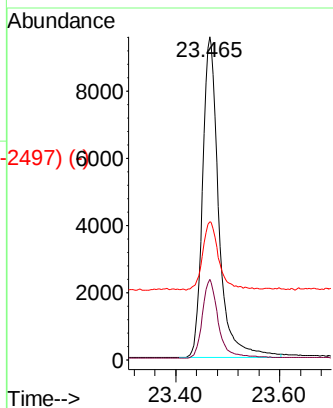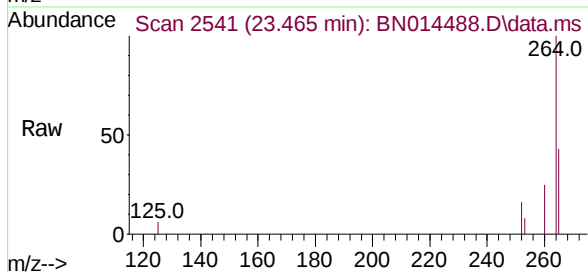


Abundance Scan 3190 (25.687 min): BN014488.D\data.ms (-3136) (-)

Indeno(1,2,3-cd)pyrene
Concen: 1.88 ng
RT: 25.687 min Scan# 3190
Delta R.T. 0.000 min
Lab File: BN014488.D
Acq: 29 Apr 2021 13:16

Tgt Ion	Ratio	Lower	Upper
276	100		
138	25.0	20.1	30.1
277	24.8	19.8	29.8

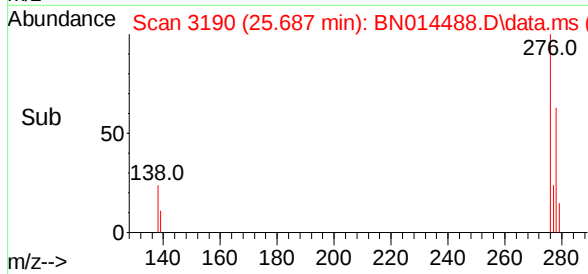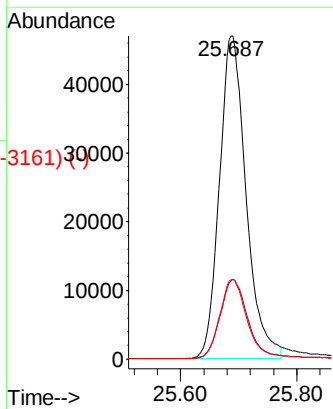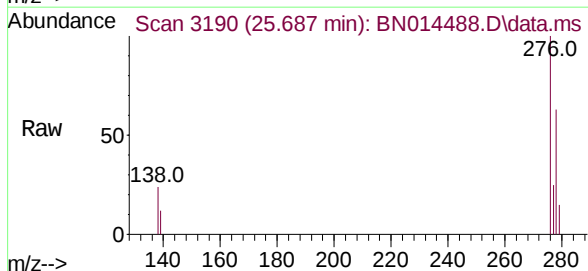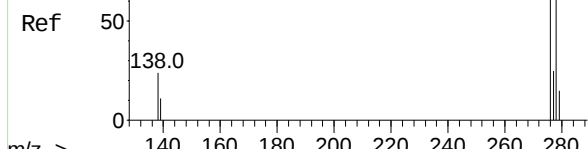



Abundance Scan 2347 (22.801 min): BN014488.D\data.ms (-2337) (-)

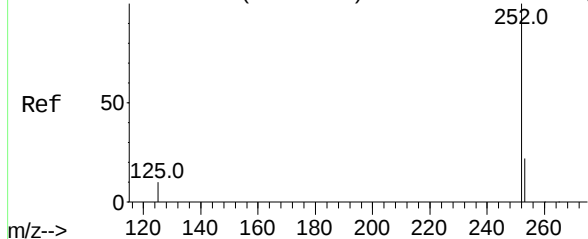


Benzo(b)fluoranthene
Concen: 1.83 ng
RT: 22.801 min Scan# 2347
Delta R.T. 0.000 min
Lab File: BN014488.D
Acq: 29 Apr 2021 13:16

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:	252	Resp:	134582
Ion	Ratio	Lower	Upper
252	100		
253	22.3	19.7	29.5
125	10.5	10.0	15.0

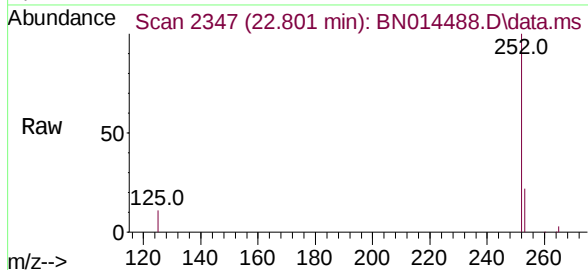

Abundance Scan 2347 (22.801 min): BN014488.D\data.ms (-2289) (-)


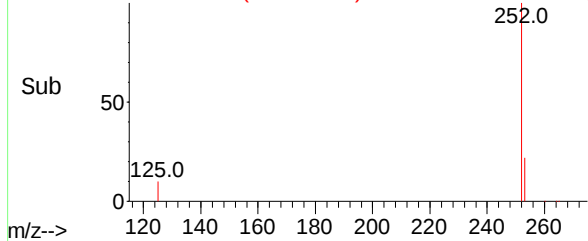


Abundance Scan 2360 (22.846 min): BN014488.D\data.ms (-2338) (-)

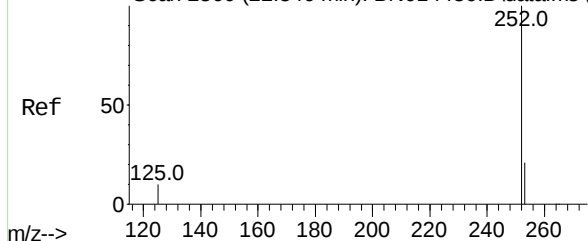


Benzo(k)fluoranthene
Concen: 2.00 ng
RT: 22.846 min Scan# 2360
Delta R.T. 0.000 min
Lab File: BN014488.D
Acq: 29 Apr 2021 13:16

Tgt Ion:	252	Resp:	152105
Ion	Ratio	Lower	Upper
252	100		
253	22.2	19.4	29.2
125	10.1	10.0	15.0

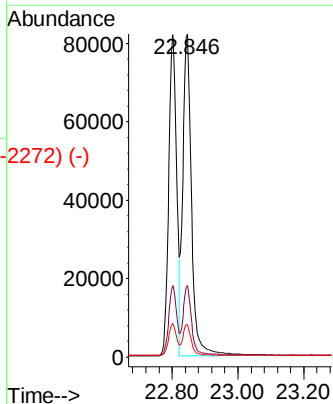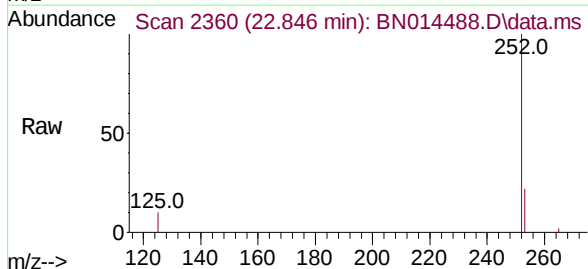


Abundance Scan 2360 (22.846 min): BN014488.D\data.ms (-2272) (-)

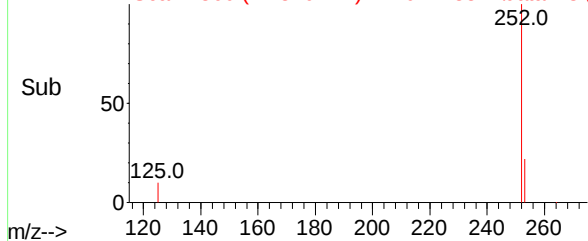




Abundance Scan 2513 (23.369 min): BN014488.D\data.ms (-2455) (-)

Benzo(a)pyrene
Concen: 1.76 ng
RT: 23.369 min Scan# 2513
Delta R.T. 0.000 min
Lab File: BN014488.D
Acq: 29 Apr 2021 13:16

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

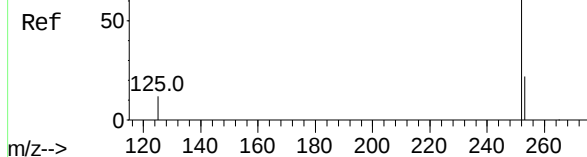





Tgt Ion:	252	Resp:	116517
Ion Ratio	Lower	Upper	
252	100		
253	22.6	20.8	31.2
125	12.4	12.6	19.0#

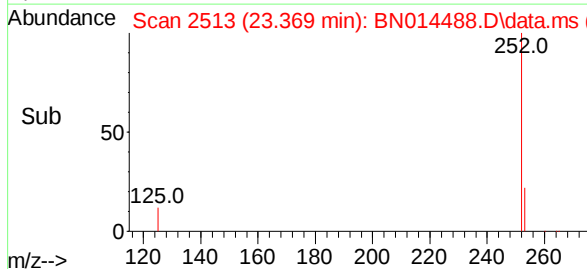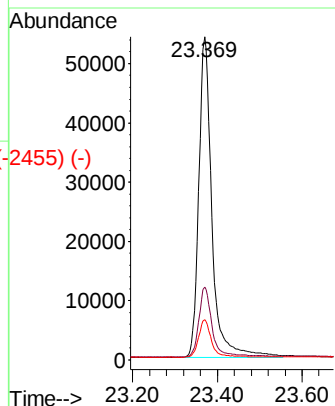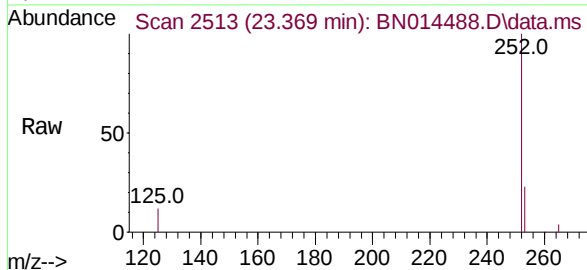


Abundance Scan 3194 (25.700 min): BN014488.D\data.ms (-3171) (-)

Dibenzo(a,h)anthracene
Concen: 1.92 ng
RT: 25.704 min Scan# 3195
Delta R.T. 0.003 min
Lab File: BN014488.D
Acq: 29 Apr 2021 13:16

Tgt Ion:	278	Resp:	127329
Ion Ratio	Lower	Upper	
278	100		
139	16.5	14.2	21.4
279	23.5	21.0	31.4

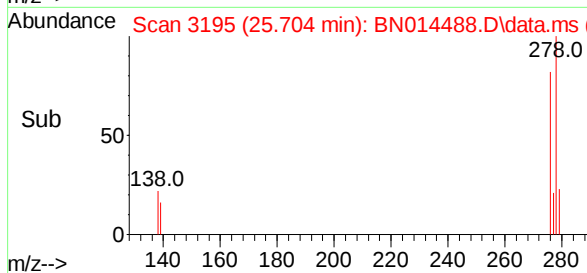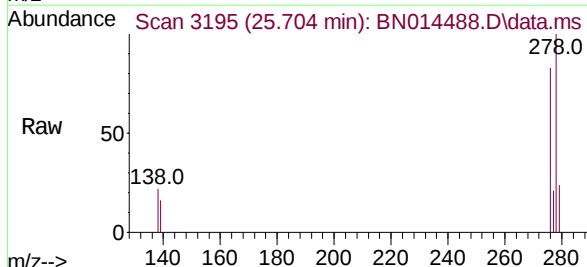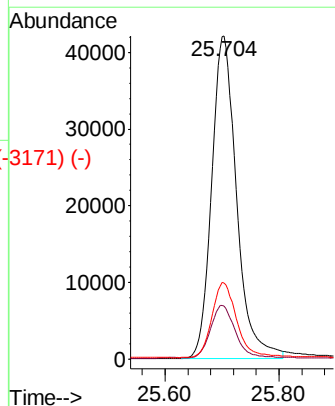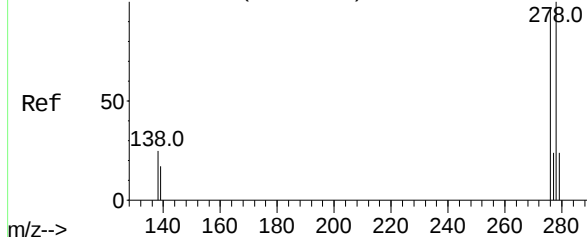


Abundance Scan 3388 (26.364 min): BN014486.D\data.ms (-3388) (-)

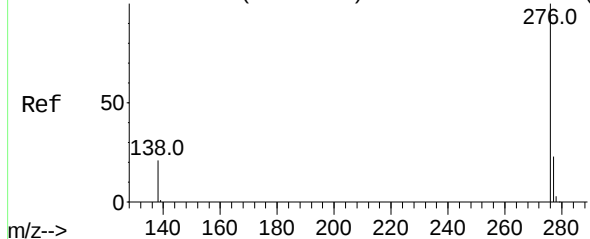

Benzo(g,h,i)perylene
Concen: 1.91 ng
RT: 26.368 min Scan# 3389
Delta R.T. 0.003 min
Lab File: BN014488.D
Acq: 29 Apr 2021 13:16

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Tgt Ion:276 Resp: 134152
Ion Ratio Lower Upper
276 100
277 23.7 19.4 29.2
138 21.6 17.5 26.3

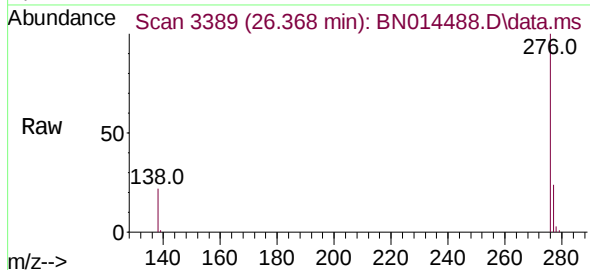

Abundance Scan 3389 (26.368 min): BN014488.D\data.ms (-3330) (-)

