

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042921\
 Data File : BN014498.D
 Acq On : 29 Apr 2021 20:08
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Quant Time: Apr 30 02:34:47 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 29 15:11:14 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.668	152	8008	0.40	ng	0.00
7) Naphthalene-d8	10.441	136	29698	0.40	ng	0.00
13) Acenaphthene-d10	14.295	164	16191	0.40	ng	0.00
19) Phenanthrene-d10	17.043	188	34165	0.40	ng	0.00
29) Chrysene-d12	21.247	240	31355	0.40	ng	0.00
35) Perylene-d12	23.462	264	27634	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.276	112	5972	0.42	ng	0.00
5) Phenol-d6	6.839	99	7013	0.40	ng	0.00
8) Nitrobenzene-d5	8.807	82	5756	0.38	ng	0.00
11) 2-Methylnaphthalene-d10	12.035	152	22445	0.37	ng	0.00
14) 2,4,6-Tribromophenol	15.792	330	1665	0.40	ng	0.00
15) 2-Fluorobiphenyl	12.925	172	22567	0.36	ng	0.00
27) Fluoranthene-d10	19.086	212	43241	0.36	ng	0.00
31) Terphenyl-d14	19.692	244	27021	0.37	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.231	88	3134	0.35	ng	98
3) n-Nitrosodimethylamine	3.609	42	1249	0.40	ng	98
6) bis(2-Chloroethyl)ether	7.104	93	7565	0.39	ng	98
9) Naphthalene	10.492	128	28835	0.37	ng	100
10) Hexachlorobutadiene	10.784	225	5469	0.36	ng	# 99
12) 2-Methylnaphthalene	12.111	142	18891	0.37	ng	100
16) Acenaphthylene	14.016	152	20695	0.34	ng	99
17) Acenaphthene	14.359	154	16647	0.36	ng	97
18) Fluorene	15.348	166	20469	0.36	ng	100
20) 4,6-Dinitro-2-methylph...	15.437	198	1062	0.48	ng	# 68
21) 4-Bromophenyl-phenylether	16.252	248	6353	0.34	ng	98
22) Hexachlorobenzene	16.361	284	8461	0.34	ng	99
23) Atrazine	16.519	200	3366	0.39	ng	98
24) Pentachlorophenol	16.702	266	1401	0.52	ng	98
25) Phenanthrene	17.091	178	35459	0.36	ng	100
26) Anthracene	17.176	178	26365	0.35	ng	100
28) Fluoranthene	19.116	202	37870	0.35	ng	100
30) Pyrene	19.478	202	37324	0.36	ng	100
32) Benzo(a)anthracene	21.226	228	29895	0.36	ng	100
33) Chrysene	21.279	228	37426	0.36	ng	100
34) Bis(2-ethylhexyl)phtha...	21.173	149	8761	0.38	ng	99
36) Indeno(1,2,3-cd)pyrene	25.684	276	39385	0.35	ng	98
37) Benzo(b)fluoranthene	22.798	252	36232	0.34	ng	99
38) Benzo(k)fluoranthene	22.843	252	40076	0.35	ng	99
39) Benzo(a)pyrene	23.367	252	32835	0.36	ng	# 95
40) Dibenzo(a,h)anthracene	25.701	278	32712	0.35	ng	98
41) Benzo(g,h,i)perylene	26.362	276	35357	0.34	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042921\
Data File : BN014498.D
Acq On : 29 Apr 2021 20:08
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Quant Time: Apr 30 02:34:47 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 29 15:11:14 2021
Response via : Initial Calibration




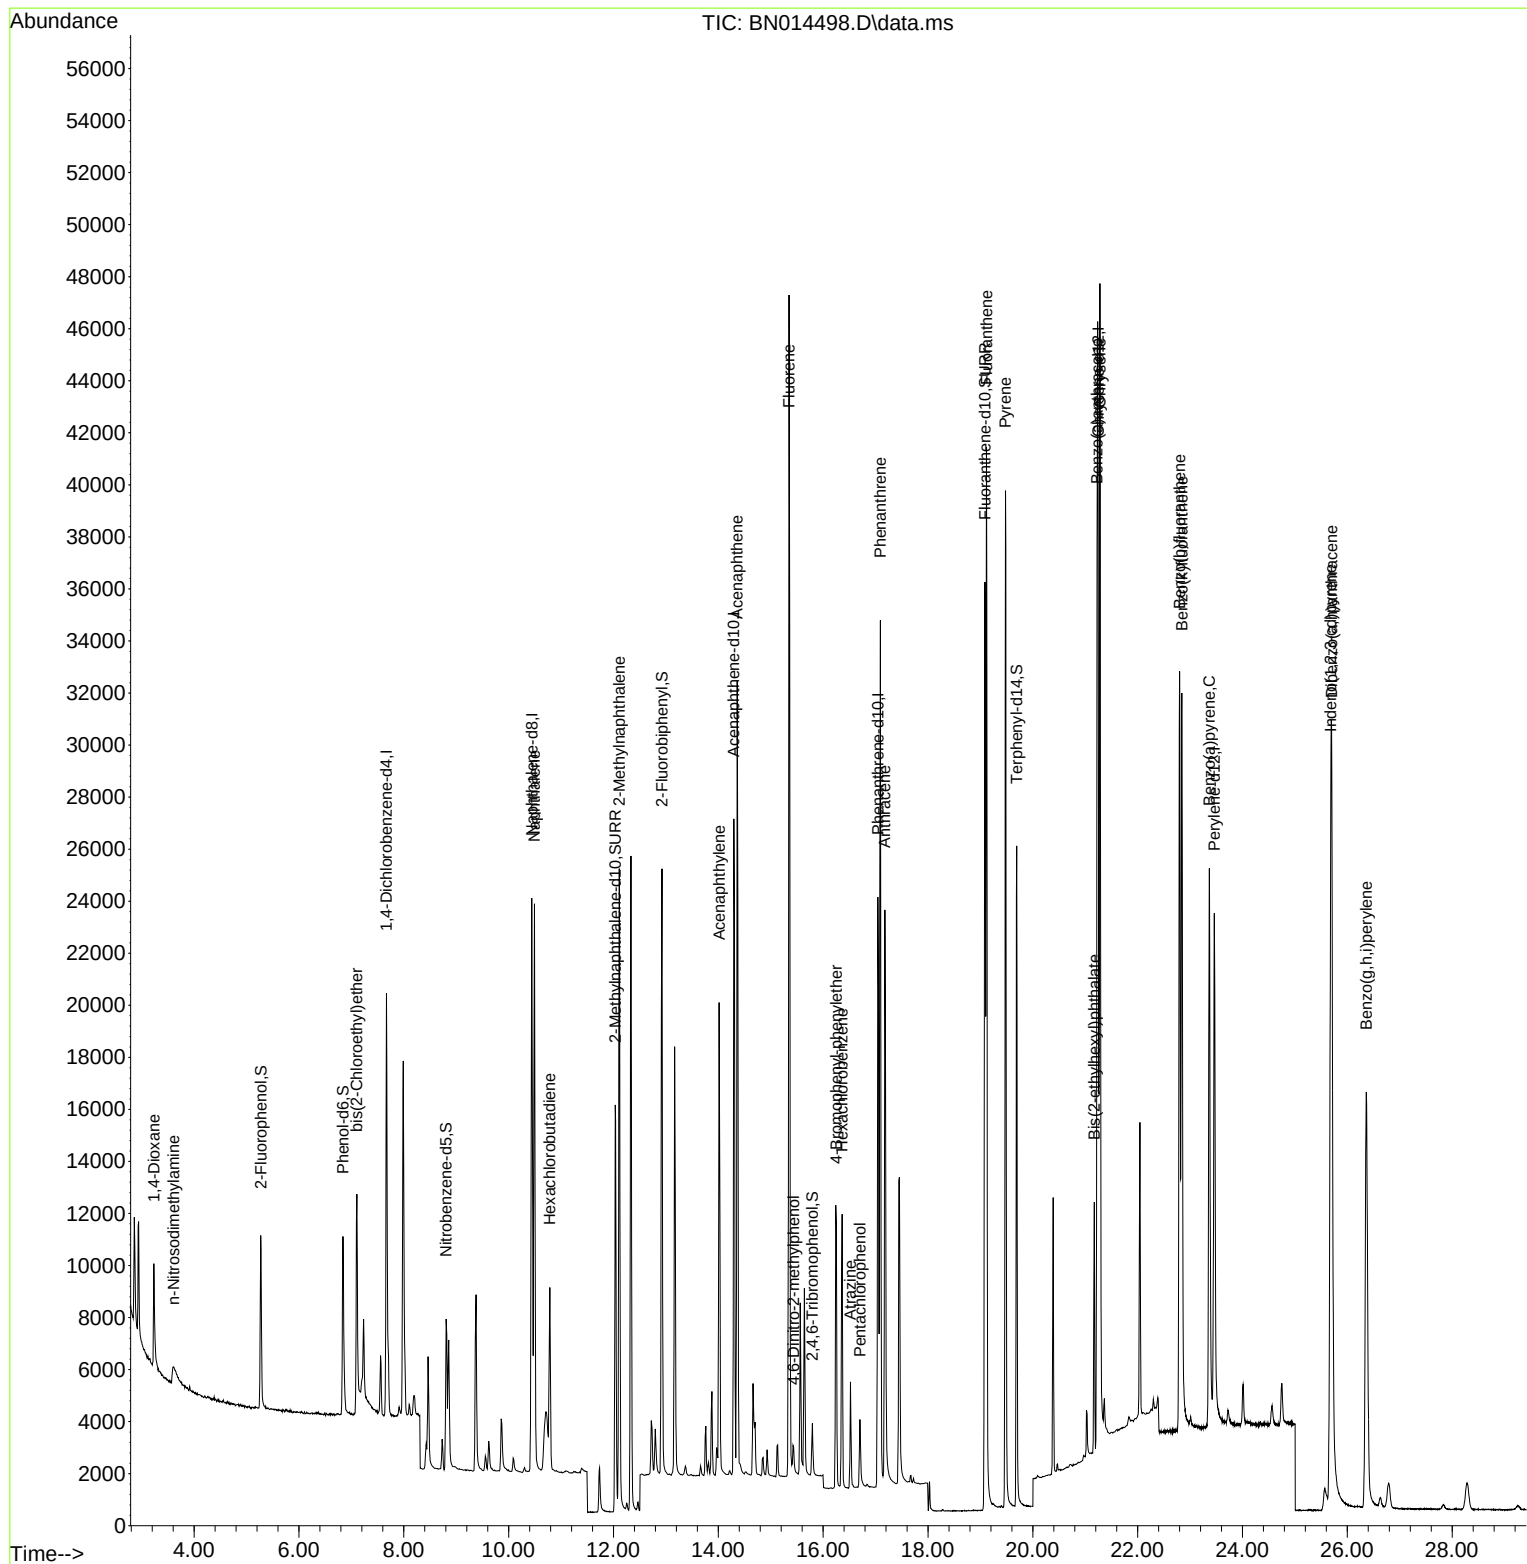




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.668 min Scan# 607
 Delta R.T. 0.000 min
 Lab File: BN014498.D
 Acq: 29 Apr 2021 20:08




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC


Tgt Ion:152 Resp: 8008
 Ion Ratio Lower Upper
 152 100
 150 156.8 126.6 189.8
 115 59.6 47.7 71.5

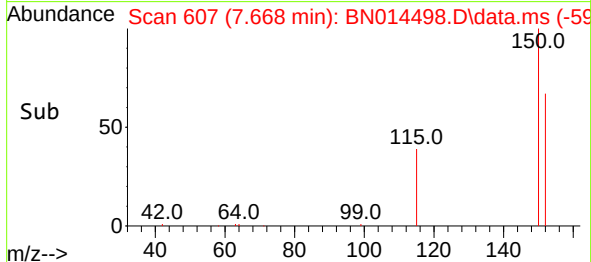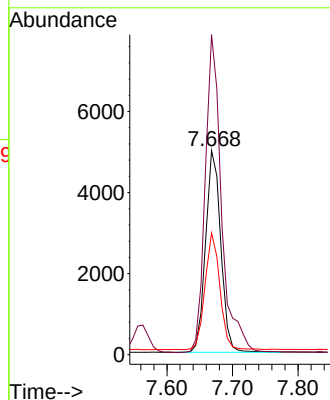

#2
 1,4-Dioxane
 Concen: 0.35 ng
 RT: 3.231 min Scan# 56
 Delta R.T. -0.000 min
 Lab File: BN014498.D
 Acq: 29 Apr 2021 20:08

Tgt Ion: 88 Resp: 3134
 Ion Ratio Lower Upper
 88 100
 58 68.0 55.4 83.0
 43 24.7 21.6 32.4



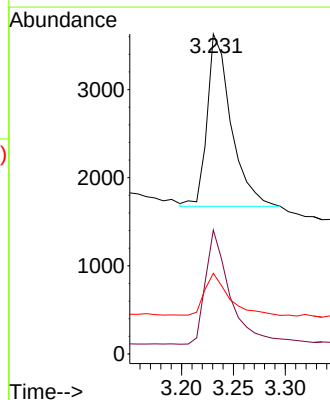
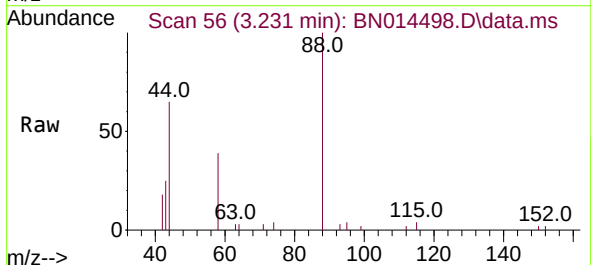




#3
n-Nitrosodimethylamine
Concen: 0.40 ng
RT: 3.609 min Scan# 103
Delta R.T. 0.008 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion: 42 Resp: 1249
Ion Ratio Lower Upper
42 100
74 152.6 120.3 180.5
44 8.2 6.7 10.1

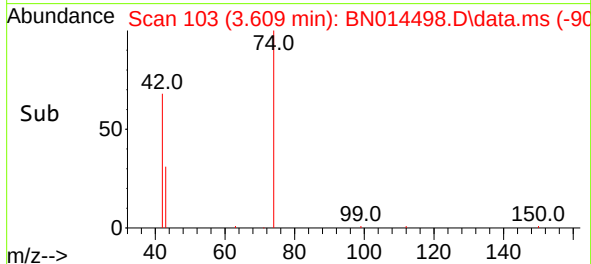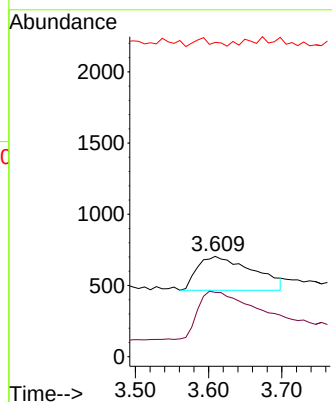

#4
2-Fluorophenol
Concen: 0.42 ng
RT: 5.276 min Scan# 310
Delta R.T. -0.000 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08

Tgt Ion: 112 Resp: 5972
Ion Ratio Lower Upper
112 100
64 52.8 42.4 63.6
63 27.4 22.2 33.4







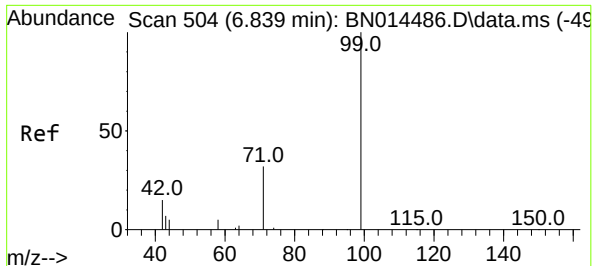

#5
Phenol-d6
Concen: 0.40 ng
RT: 6.839 min Scan# 504
Delta R.T. -0.000 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:	99	Resp:	7013
Ion	Ratio	Lower	Upper
99	100		
42	17.1	13.8	20.8
71	32.3	26.0	39.0

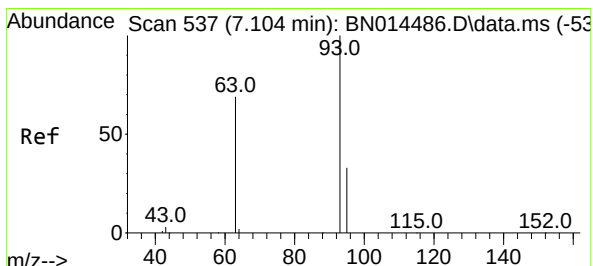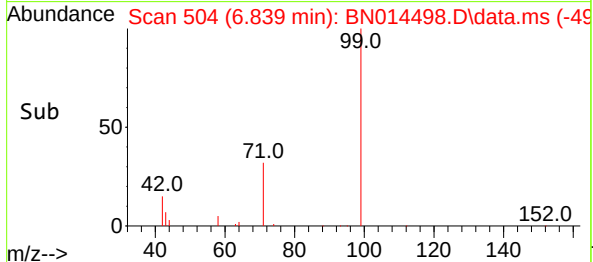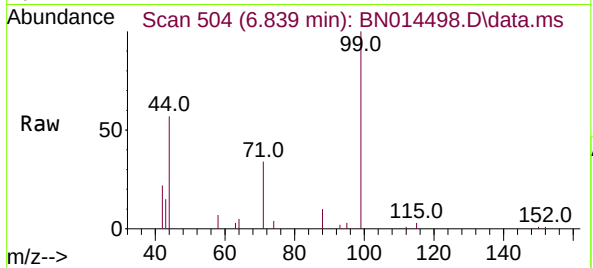

#6
bis(2-Chloroethyl)ether
Concen: 0.39 ng
RT: 7.104 min Scan# 537
Delta R.T. -0.000 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08

Tgt Ion:	93	Resp:	7565
Ion	Ratio	Lower	Upper
93	100		
63	71.4	58.3	87.5
95	32.6	27.0	40.6


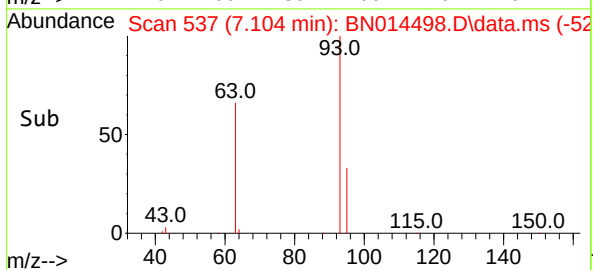

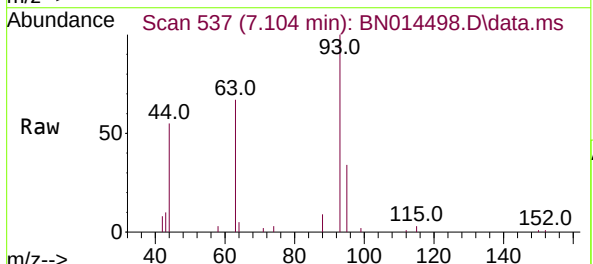




#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.441 min Scan# 855
Delta R.T. -0.000 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:136	Resp:	29698
Ion Ratio	Lower	Upper
136	100	
137	11.1	9.0 13.6
54	5.9	4.8 7.2
68	5.6	4.6 6.8

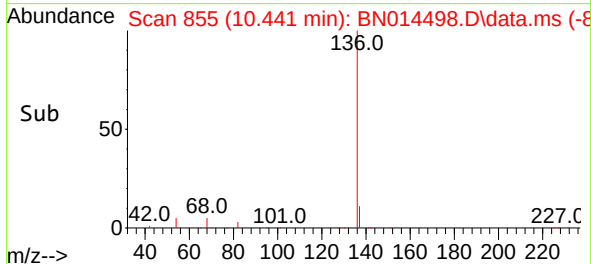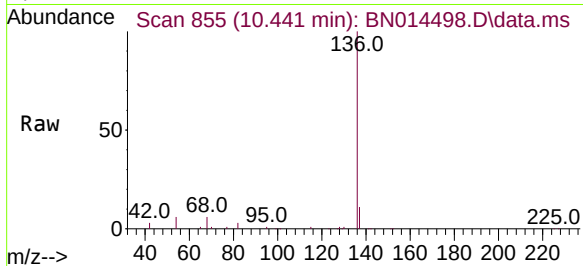

#8
Nitrobenzene-d5
Concen: 0.38 ng
RT: 8.807 min Scan# 726
Delta R.T. -0.000 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08

Tgt Ion: 82	Resp:	5756
Ion Ratio	Lower	Upper
82	100	
128	35.0	26.0 39.0
54	49.3	39.5 59.3




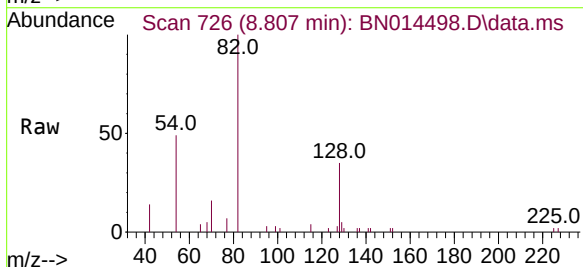


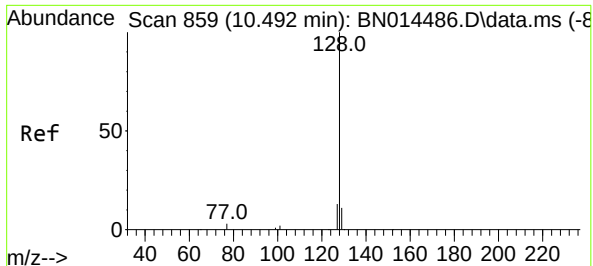

#9
Naphthalene
Concen: 0.37 ng
RT: 10.492 min Scan# 859
Delta R.T. -0.000 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:	128	Resp:	28835
Ion Ratio	Lower	Upper	
128	100		
129	11.3	9.0	13.6
127	12.9	10.2	15.4

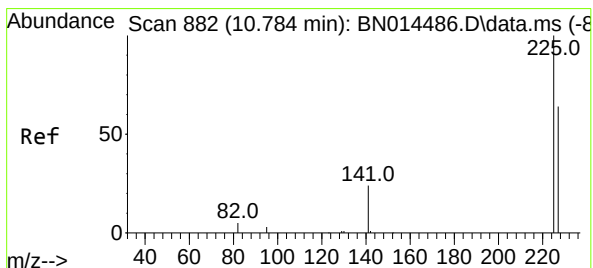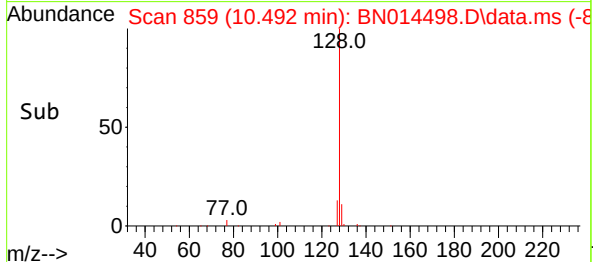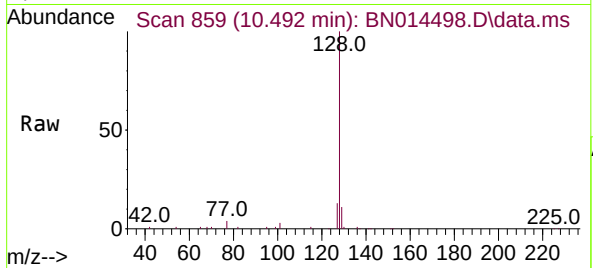

#10
Hexachlorobutadiene
Concen: 0.36 ng
RT: 10.784 min Scan# 882
Delta R.T. -0.000 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08

Tgt Ion:	225	Resp:	5469
Ion Ratio	Lower	Upper	
225	100		
223	0.0	0.0	0.0
227	63.6	51.8	77.6


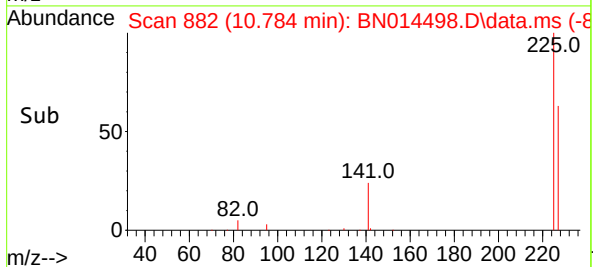

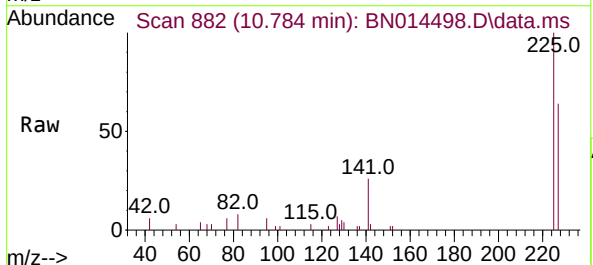




#11
2-Methylnaphthalene-d10
Concen: 0.37 ng
RT: 12.035 min Scan# 1058
Delta R.T. -0.000 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:152 Resp: 22445
Ion Ratio Lower Upper
152 100
151 20.6 16.3 24.5

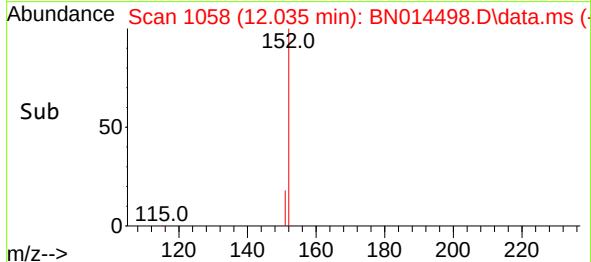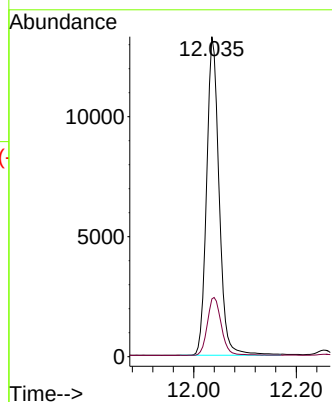

#12
2-Methylnaphthalene
Concen: 0.37 ng
RT: 12.111 min Scan# 1075
Delta R.T. -0.000 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08

Tgt Ion:142 Resp: 18891
Ion Ratio Lower Upper
142 100
141 87.7 70.5 105.7
115 34.1 27.5 41.3


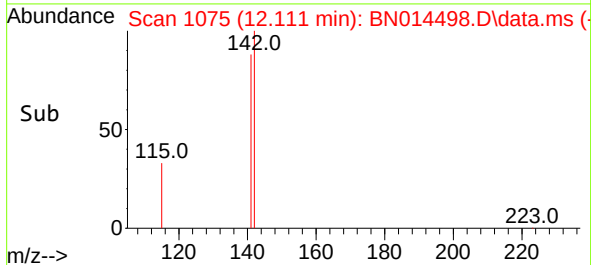






#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.295 min Scan# 1305
Delta R.T. -0.000 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:164 Resp: 16191
Ion Ratio Lower Upper
164 100
162 102.2 82.4 123.6
160 50.0 40.5 60.7

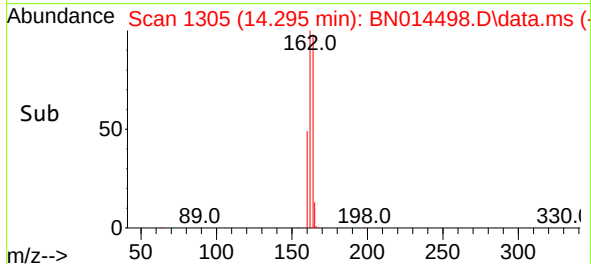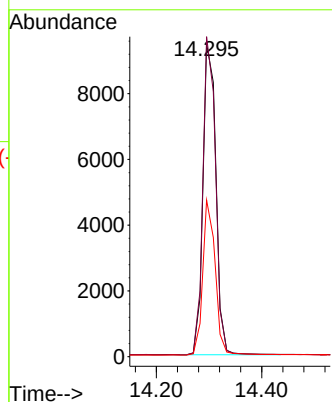

#14
2,4,6-Tribromophenol
Concen: 0.40 ng
RT: 15.792 min Scan# 1423
Delta R.T. -0.000 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08

Tgt Ion:330 Resp: 1665
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 33.8 28.5 42.7


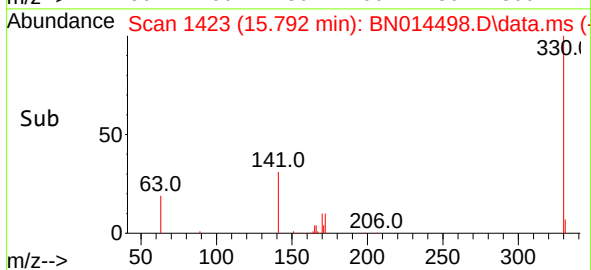






#15
2-Fluorobiphenyl
Concen: 0.36 ng
RT: 12.925 min Scan# 1197
Delta R.T. -0.000 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:172	Resp:	22567
Ion Ratio	Lower	Upper
172	100	
171	33.8	26.6 40.0
170	22.4	18.2 27.2

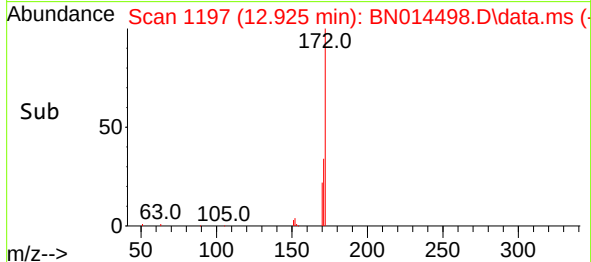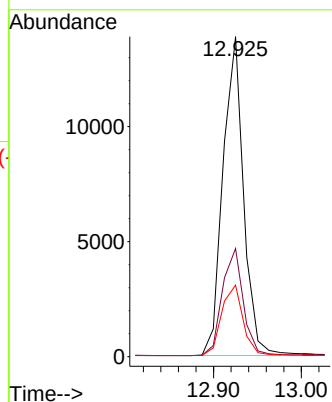

#16
Acenaphthylene
Concen: 0.34 ng
RT: 14.016 min Scan# 1283
Delta R.T. -0.000 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08

Tgt Ion:152	Resp:	20695
Ion Ratio	Lower	Upper
152	100	
151	19.4	15.6 23.4
153	12.9	10.7 16.1




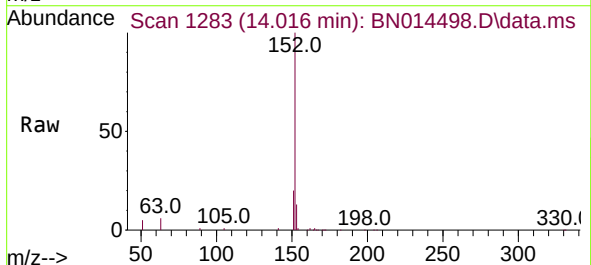




#17
Acenaphthene
Concen: 0.36 ng
RT: 14.359 min Scan# 1310
Delta R.T. -0.000 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:154 Resp: 16647
Ion Ratio Lower Upper
154 100
153 110.4 90.3 135.5
152 56.3 47.3 70.9

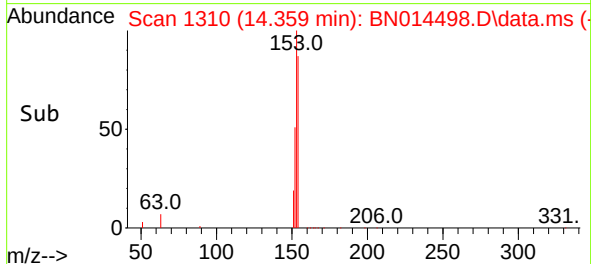

#18
Fluorene
Concen: 0.36 ng
RT: 15.348 min Scan# 1388
Delta R.T. -0.000 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08

Tgt Ion:166 Resp: 20469
Ion Ratio Lower Upper
166 100
165 97.7 78.2 117.2
167 13.5 10.9 16.3







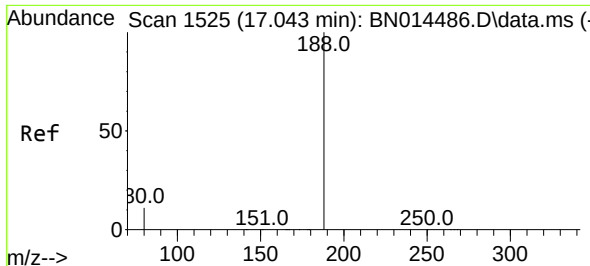

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.043 min Scan# 1525
Delta R.T. -0.001 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:188 Resp: 34165
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 11.9 8.8 13.2

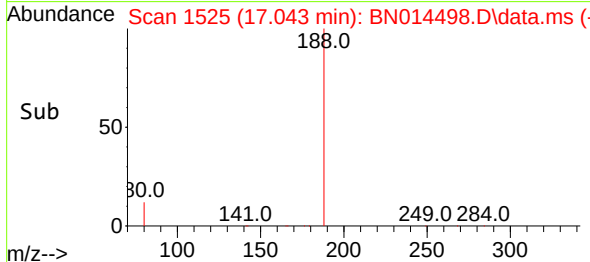

#20
4,6-Dinitro-2-methylphenol
Concen: 0.48 ng
RT: 15.437 min Scan# 1395
Delta R.T. 0.000 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08

Tgt Ion:198 Resp: 1062
Ion Ratio Lower Upper
198 100
51 97.1 116.0 174.0#
105 44.4 45.3 67.9#


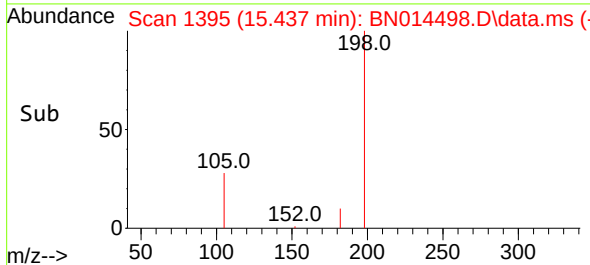

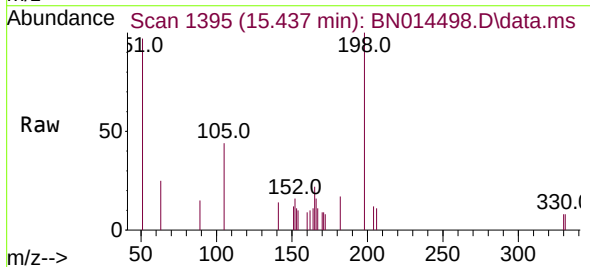


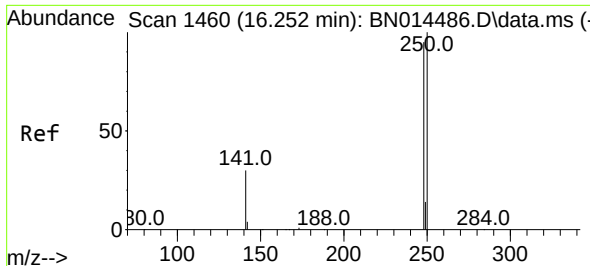

#21
4-Bromophenyl-phenylether
Concen: 0.34 ng
RT: 16.252 min Scan# 1460
Delta R.T. -0.001 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:	248	Resp:	6353
Ion	Ratio	Lower	Upper
248	100		
250	105.4	84.6	126.8
141	36.7	26.7	40.1

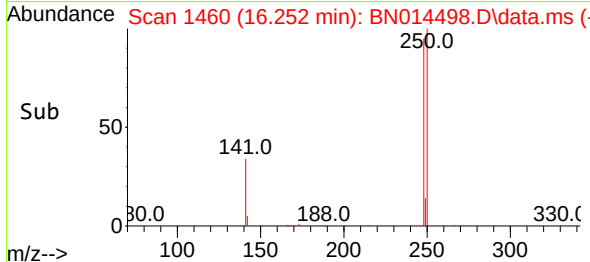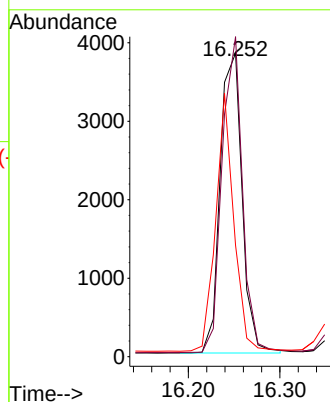

#22
Hexachlorobenzene
Concen: 0.34 ng
RT: 16.361 min Scan# 1469
Delta R.T. -0.001 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08

Tgt Ion:	284	Resp:	8461
Ion	Ratio	Lower	Upper
284	100		
142	33.7	27.0	40.6
249	30.0	23.6	35.4


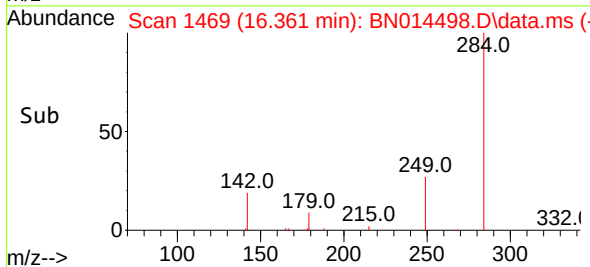
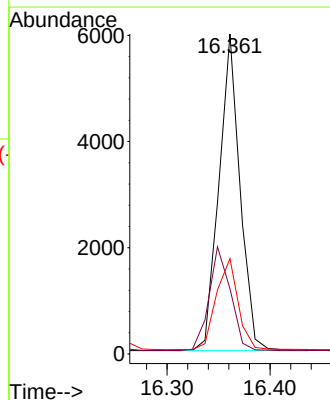
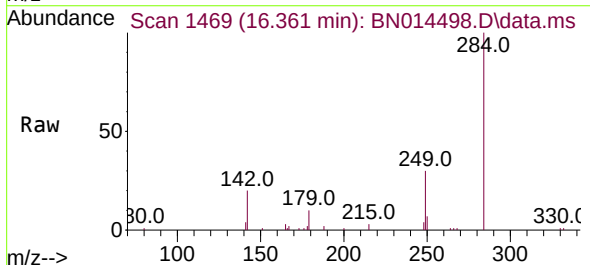


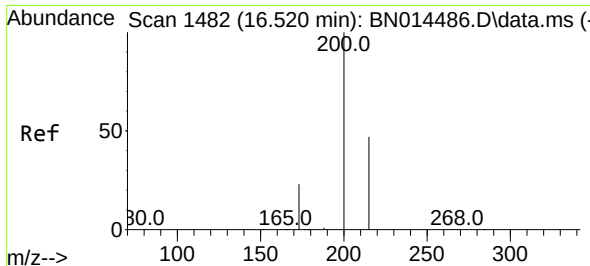

#23
Atrazine
Concen: 0.39 ng
RT: 16.519 min Scan# 1482
Delta R.T. -0.001 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:	200	Resp:	3366
Ion Ratio	Lower	Upper	
200	100		
173	28.6	20.0	30.0
215	48.8	39.0	58.6

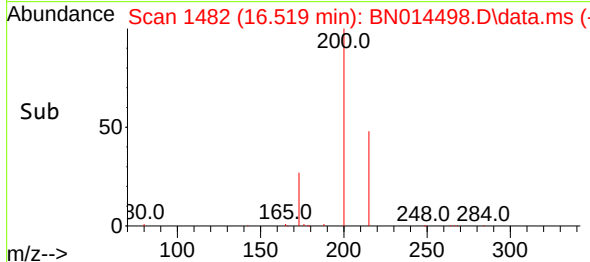

#24
Pentachlorophenol
Concen: 0.52 ng
RT: 16.702 min Scan# 1497
Delta R.T. -0.000 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08

Tgt Ion:	266	Resp:	1401
Ion Ratio	Lower	Upper	
266	100		
264	62.7	49.9	74.9
268	64.7	49.9	74.9


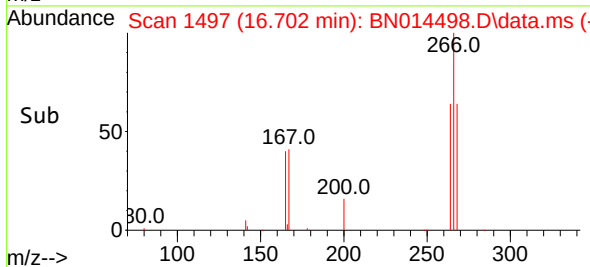

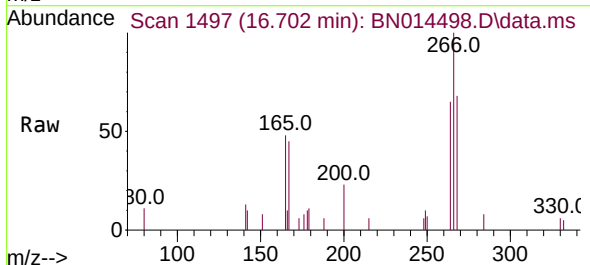


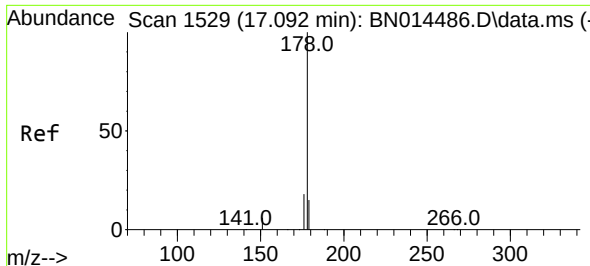

#25
Phenanthrene
Concen: 0.36 ng
RT: 17.091 min Scan# 1529
Delta R.T. -0.001 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:178 Resp: 35459
Ion Ratio Lower Upper
178 100
176 18.9 15.1 22.7
179 15.3 12.2 18.4

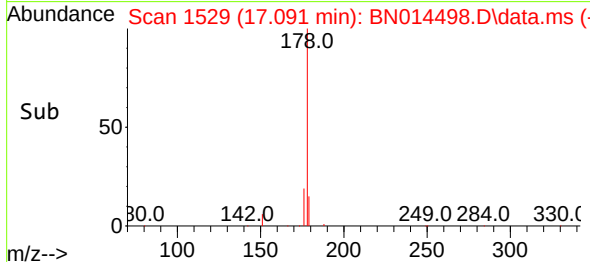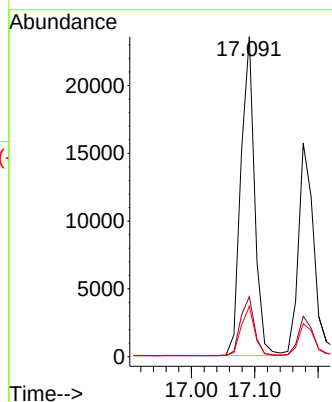

#26
Anthracene
Concen: 0.35 ng
RT: 17.176 min Scan# 1536
Delta R.T. -0.001 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08

Tgt Ion:178 Resp: 26365
Ion Ratio Lower Upper
178 100
176 18.4 14.6 22.0
179 15.3 12.2 18.2


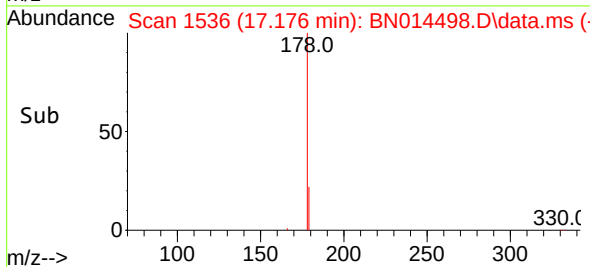

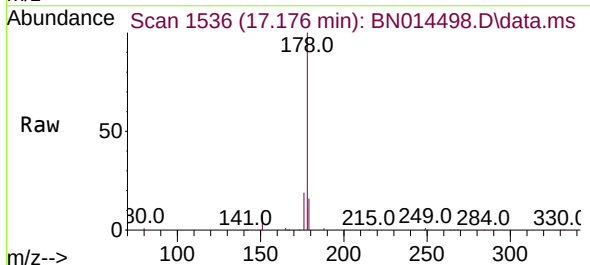


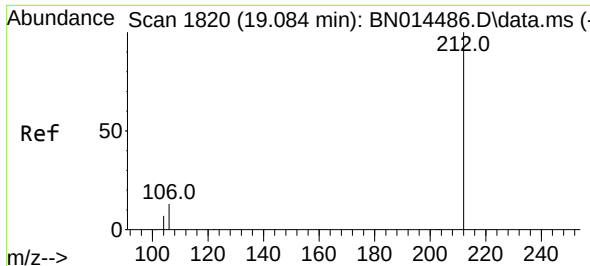

#27
Fluoranthene-d10
Concen: 0.36 ng
RT: 19.086 min Scan# 1822
Delta R.T. 0.002 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:212 Resp: 43241
Ion Ratio Lower Upper
212 100
106 12.4 10.2 15.4
104 6.9 5.6 8.4

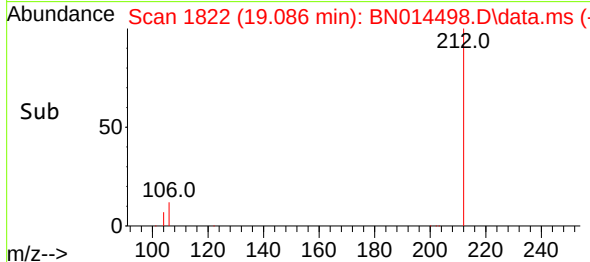

#28
Fluoranthene
Concen: 0.35 ng
RT: 19.116 min Scan# 1828
Delta R.T. 0.002 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08

Tgt Ion:202 Resp: 37870
Ion Ratio Lower Upper
202 100
101 10.8 8.7 13.1
203 17.1 13.6 20.4


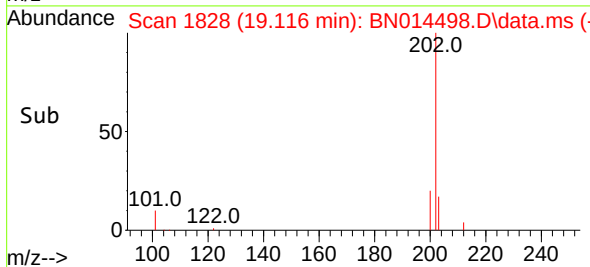

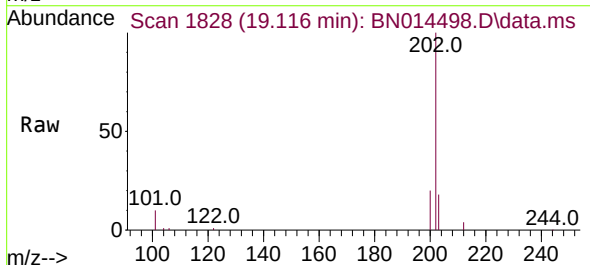




#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.247 min Scan# 2124
Delta R.T. -0.003 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:240 Resp: 31355
Ion Ratio Lower Upper
240 100
120 7.7 6.3 9.5
236 25.7 20.9 31.3

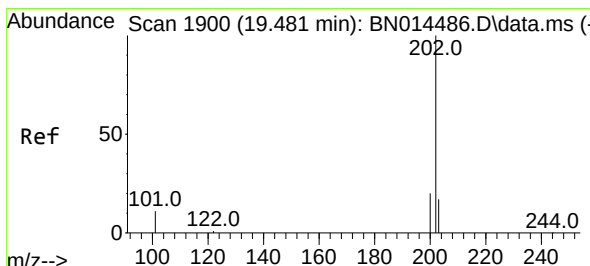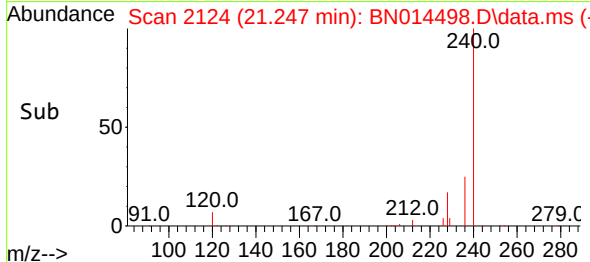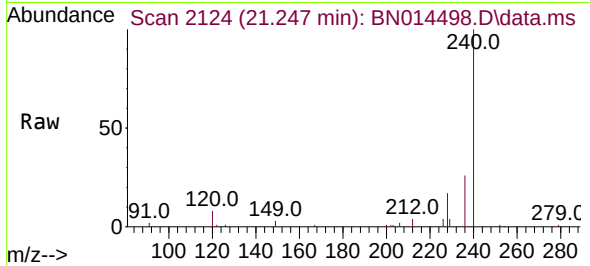

#30
Pyrene
Concen: 0.36 ng
RT: 19.478 min Scan# 1901
Delta R.T. -0.003 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08


Tgt Ion:202 Resp: 37324
Ion Ratio Lower Upper
202 100
200 20.5 16.4 24.6
203 17.5 13.9 20.9

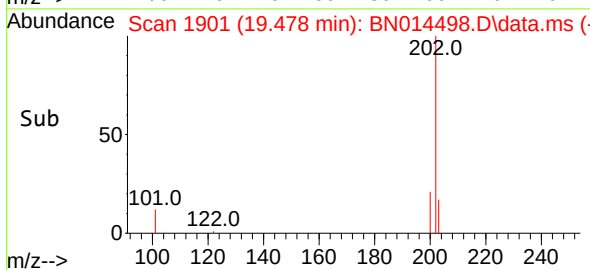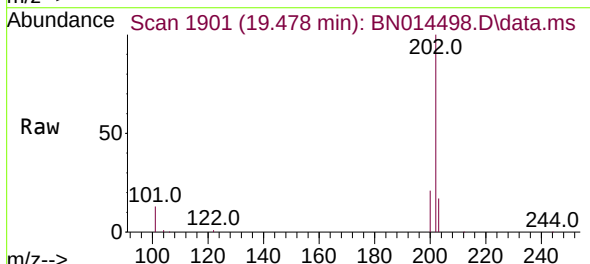






#31
Terphenyl-d14
Concen: 0.37 ng
RT: 19.692 min Scan# 1944
Delta R.T. 0.002 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC







Tgt Ion:244 Resp: 27021
Ion Ratio Lower Upper
244 100
212 7.6 6.3 9.5
122 11.6 10.6 16.0

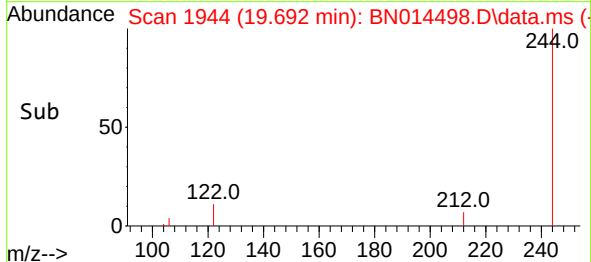

#32
Benzo(a)anthracene
Concen: 0.36 ng
RT: 21.226 min Scan# 2122
Delta R.T. -0.003 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08

Tgt Ion:228 Resp: 29895
Ion Ratio Lower Upper
228 100
226 27.5 21.8 32.8
229 19.8 15.8 23.6


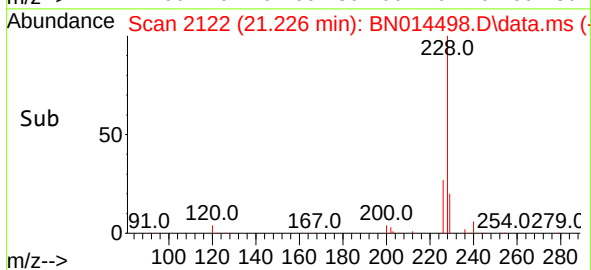

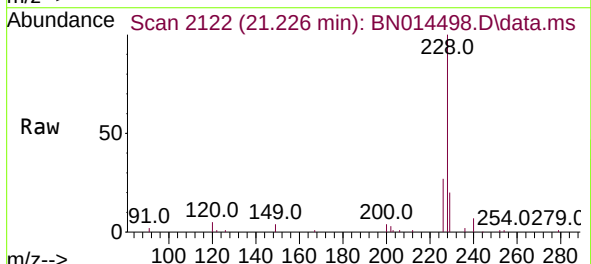


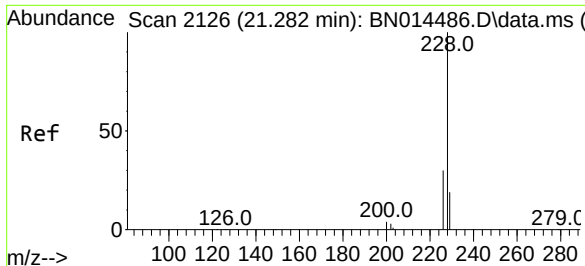

#33
Chrysene
Concen: 0.36 ng
RT: 21.279 min Scan# 2127
Delta R.T. -0.003 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:228	Resp:	37426
Ion Ratio	Lower	Upper
228	100	
226	29.9	23.9 35.9
229	19.4	15.5 23.3

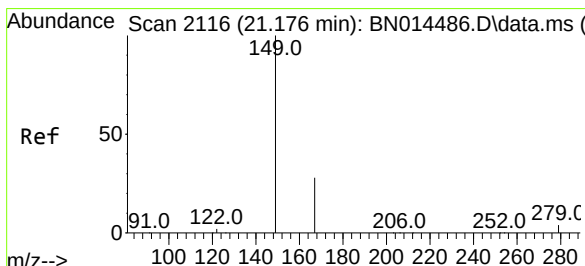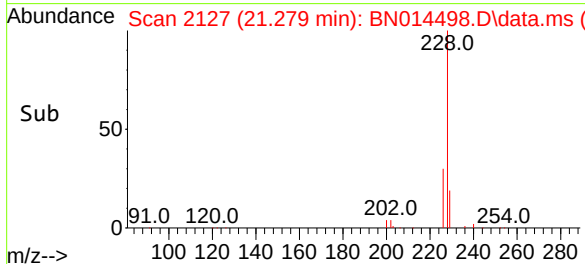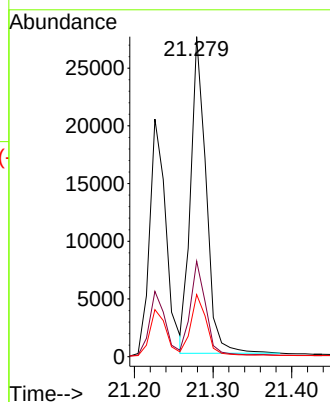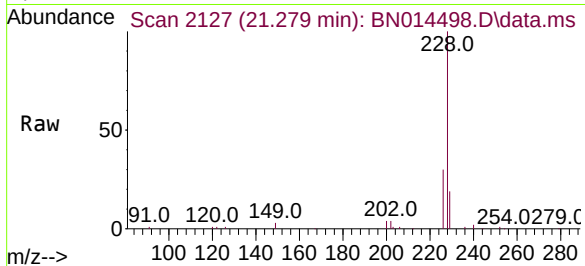

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.38 ng
RT: 21.173 min Scan# 2117
Delta R.T. -0.003 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08

Tgt Ion:149	Resp:	8761
Ion Ratio	Lower	Upper
149	100	
167	27.3	21.4 32.2
279	4.3	3.3 4.9


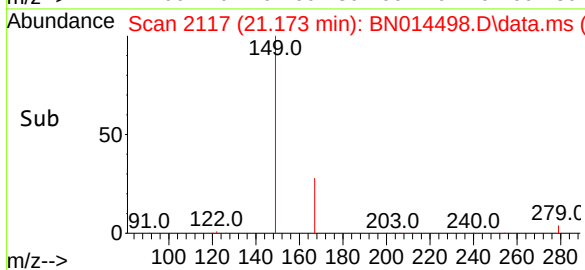
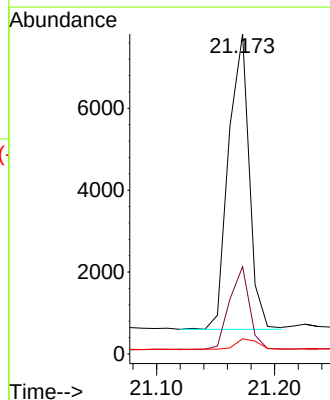
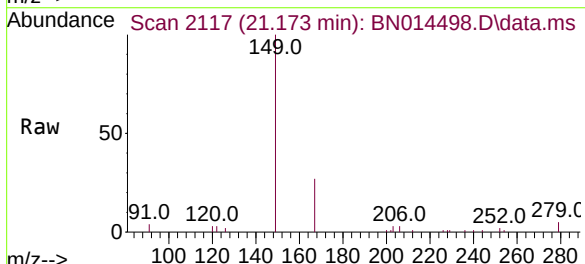




#35
 Perylene-d12
 Concen: 0.40 ng
 RT: 23.462 min Scan# 2542
 Delta R.T. -0.003 min
 Lab File: BN014498.D
 Acq: 29 Apr 2021 20:08




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC


Tgt Ion:264	Resp:	27634
Ion Ratio	Lower	Upper
264	100	
260	24.7	19.6 29.4
265	37.6	35.5 53.3

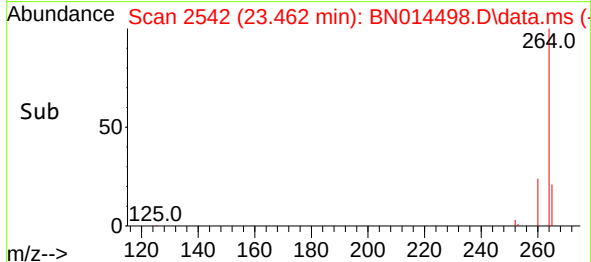

#36
 Indeno(1,2,3-cd)pyrene
 Concen: 0.35 ng
 RT: 25.684 min Scan# 3191
 Delta R.T. -0.003 min
 Lab File: BN014498.D
 Acq: 29 Apr 2021 20:08

Tgt Ion:276	Resp:	39385
Ion Ratio	Lower	Upper
276	100	
138	22.8	20.1 30.1
277	24.7	19.8 29.8




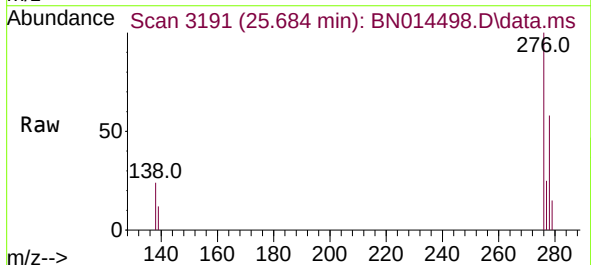




#37
Benzo(b)fluoranthene
Concen: 0.34 ng
RT: 22.798 min Scan# 2348
Delta R.T. -0.003 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:252 Resp: 36232
Ion Ratio Lower Upper
252 100
253 24.2 19.7 29.5
125 13.5 10.0 15.0

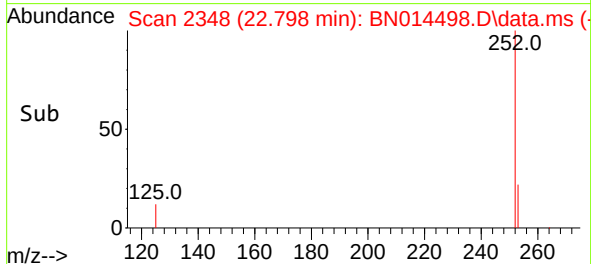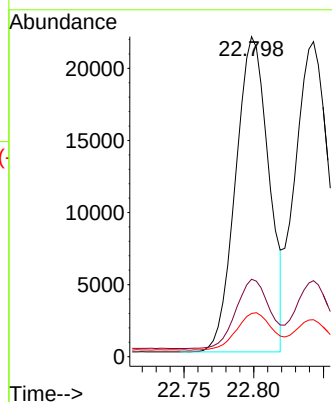

#38
Benzo(k)fluoranthene
Concen: 0.35 ng
RT: 22.843 min Scan# 2361
Delta R.T. -0.003 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08


Tgt Ion:252 Resp: 40076
Ion Ratio Lower Upper
252 100
253 24.1 19.4 29.2
125 11.7 10.0 15.0

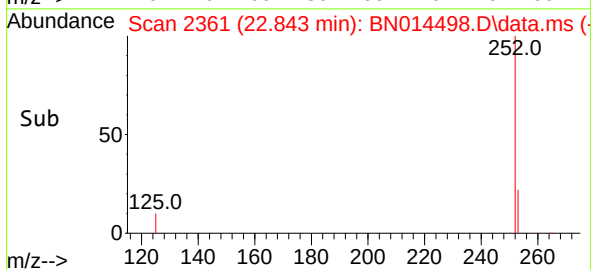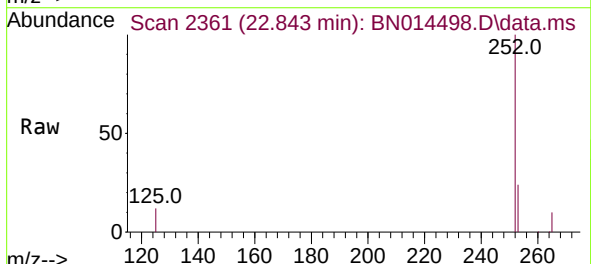






#39
Benzo(a)pyrene
Concen: 0.36 ng
RT: 23.367 min Scan# 2514
Delta R.T. -0.003 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08


Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

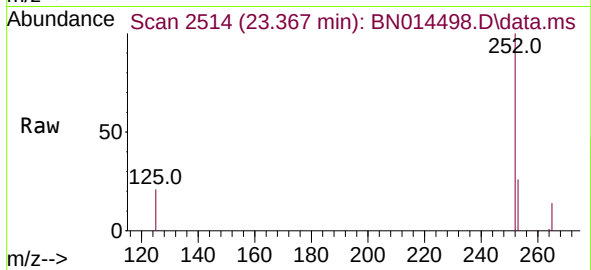



Tgt Ion:252 Resp: 32835
Ion Ratio Lower Upper
252 100
253 26.1 20.8 31.2
125 20.8 12.6 19.0#

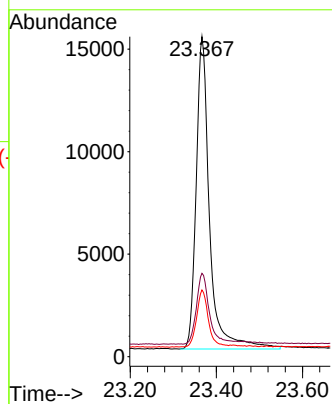


#40
Dibenzo(a,h)anthracene
Concen: 0.35 ng
RT: 25.701 min Scan# 3196
Delta R.T. 0.001 min
Lab File: BN014498.D
Acq: 29 Apr 2021 20:08



Tgt Ion:278 Resp: 32712
Ion Ratio Lower Upper
278 100
139 17.2 14.2 21.4
279 25.4 21.0 31.4



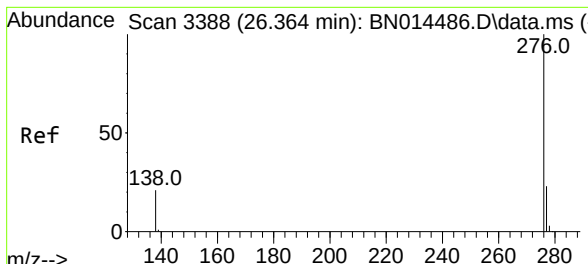

#41
 Benzo(g,h,i)perylene
 Concen: 0.34 ng
 RT: 26.362 min Scan# 3389
 Delta R.T. -0.003 min
 Lab File: BN014498.D
 Acq: 29 Apr 2021 20:08

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Tgt Ion:	276	Resp:	35357
Ion Ratio	Lower	Upper	
276	100		
277	24.3	19.4	29.2
138	21.8	17.5	26.3

