
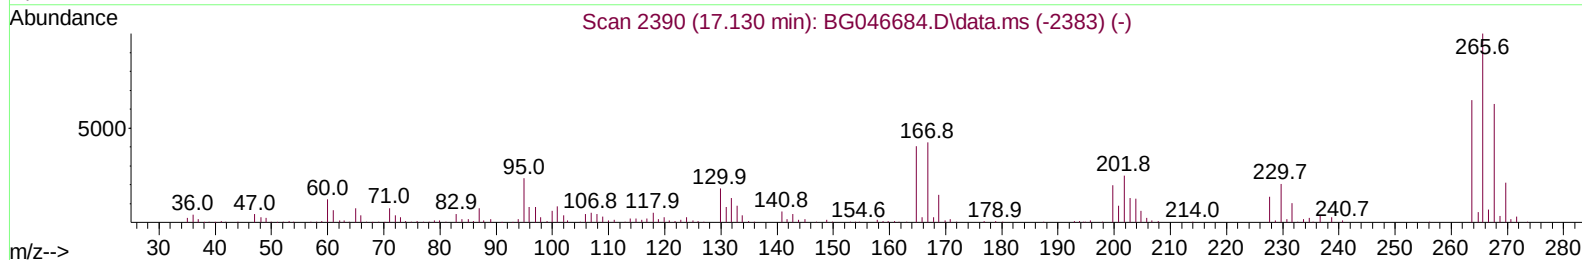
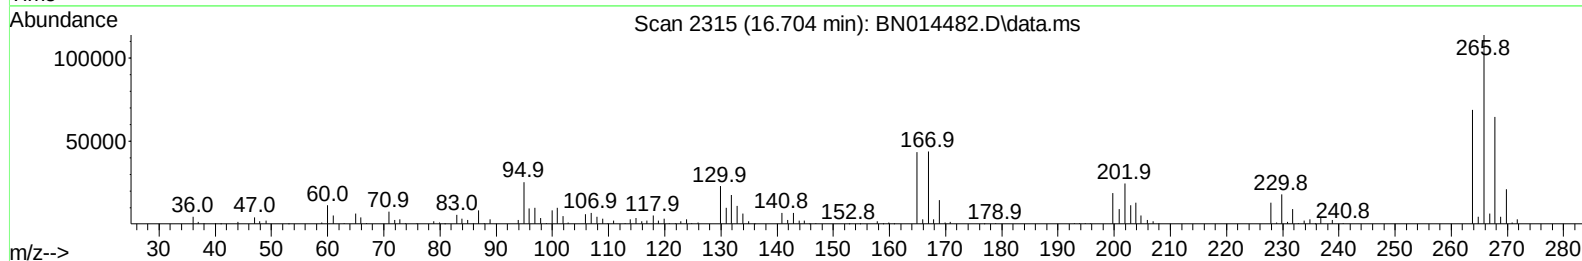


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042921\
Data File : BN014482.D
Acq On : 29 Apr 2021 09:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 10:56:40 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 09 09:55:03 2021
Response via : Initial Calibration

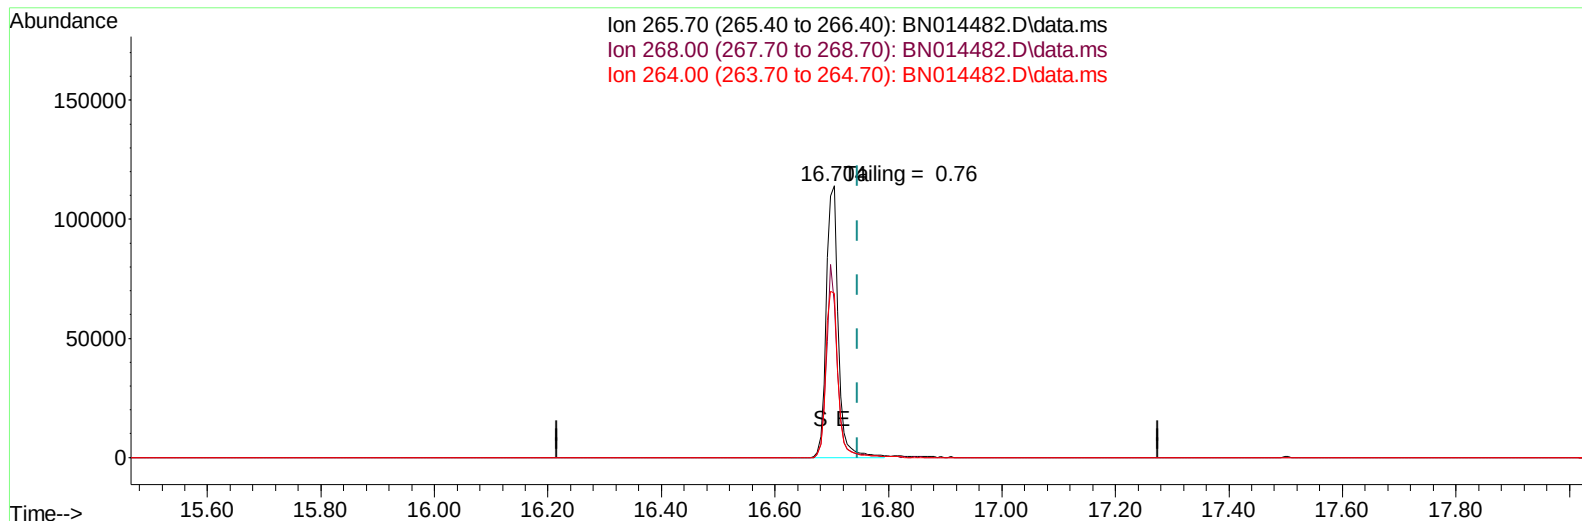




TIC: BN014482.D\data.ms

(70) Pentachlorophenol (C)**16.704min (-0.041) 18618.01 ng****response 166857**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	56.59
264.00	61.60	60.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042921\
Data File : BN014482.D
Acq On : 29 Apr 2021 09:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 10:56:40 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 09 09:55:03 2021
Response via : Initial Calibration

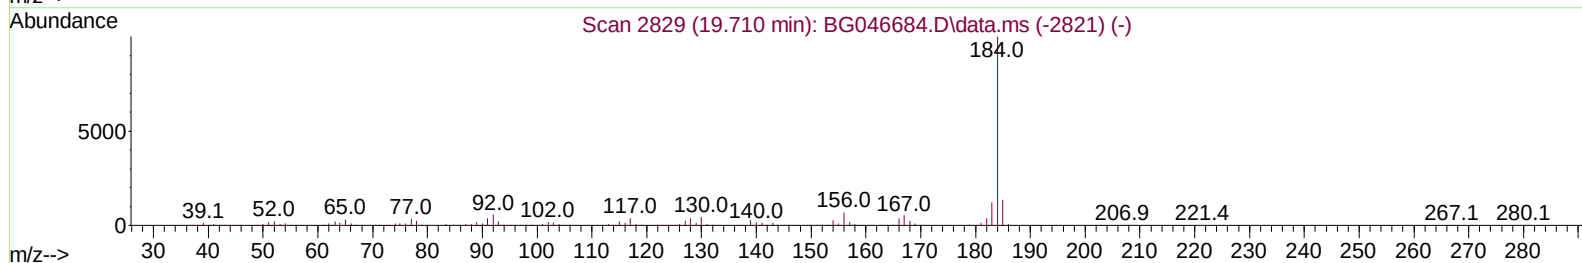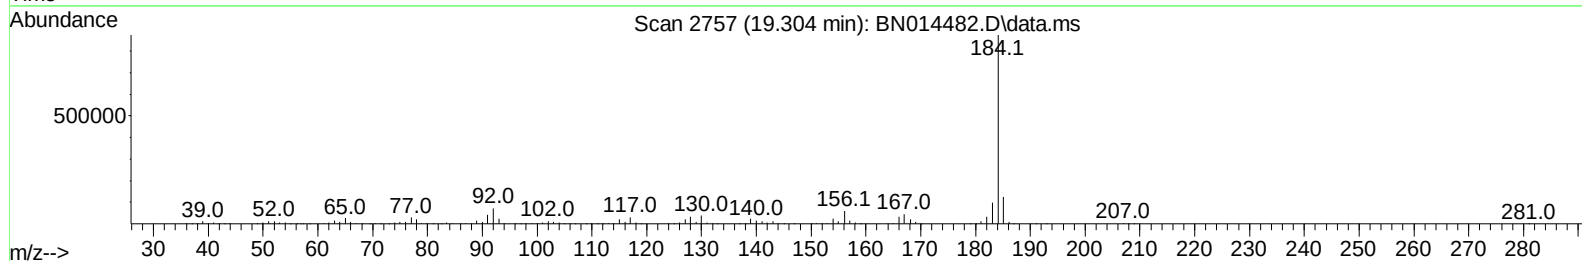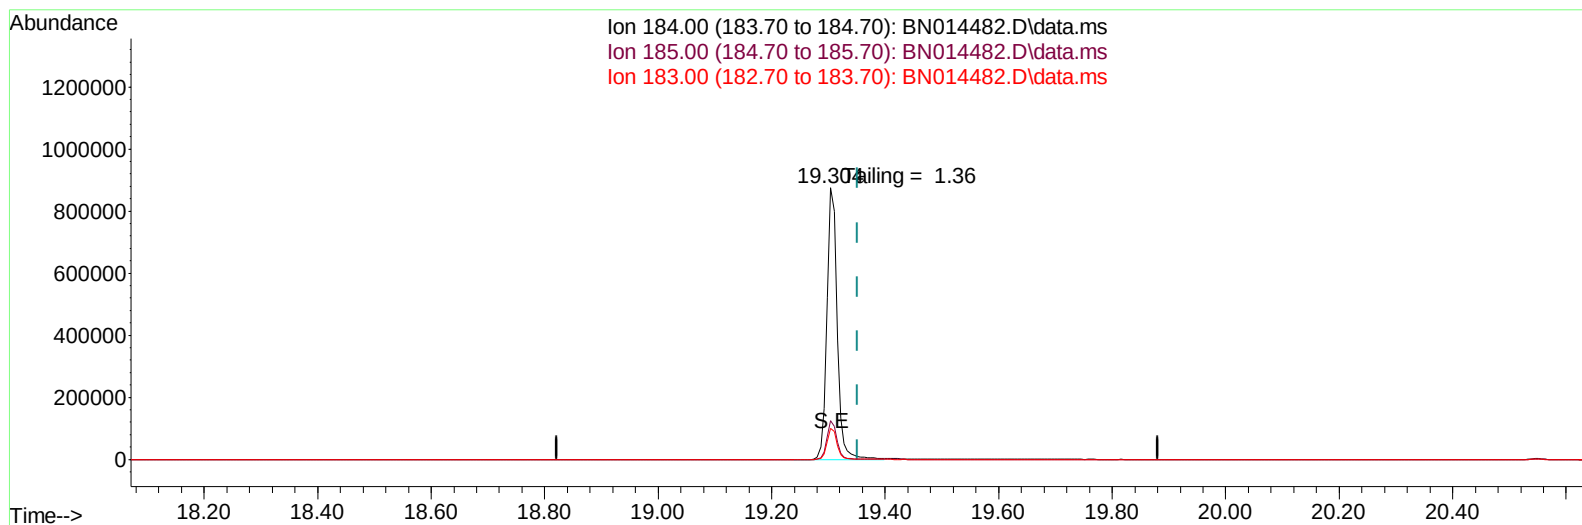

TIC: BN014482.D\data.ms

(77) Benzidine**19.304min (-0.047) 16215.12 ng****response 1088645**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.33
183.00	13.20	11.38
0.00	0.00	0.00