

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042921\
 Data File : BN014486.D
 Acq On : 29 Apr 2021 12:05
 Operator : CG/JU
 Sample : SSTDICCC0.4
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICCC0.4

Quant Time: Apr 29 12:41:17 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 29 12:40:58 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.668	152	8126	0.40	ng	0.00
7) Naphthalene-d8	10.442	136	29958	0.40	ng	0.00
13) Acenaphthene-d10	14.295	164	15211	0.40	ng	0.00
19) Phenanthrene-d10	17.043	188	31524	0.40	ng	0.00
29) Chrysene-d12	21.250	240	25522	0.40	ng	0.00
35) Perylene-d12	23.465	264	19972	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.276	112	5066	0.33	ng	0.00
5) Phenol-d6	6.839	99	6067	0.32	ng	0.00
8) Nitrobenzene-d5	8.807	82	5265	0.26	ng	0.00
11) 2-Methylnaphthalene-d10	12.035	152	22097	0.49	ng	0.00
14) 2,4,6-Tribromophenol	15.793	330	1270	0.25	ng	0.00
15) 2-Fluorobiphenyl	12.925	172	22266	0.39	ng	0.00
27) Fluoranthene-d10	19.084	212	36925	0.43	ng	0.00
31) Terphenyl-d14	19.690	244	22959	0.45	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.231	88	3178	0.35	ng	100
3) n-Nitrosodimethylamine	3.601	42	1131	0.26	ng	100
6) bis(2-Chloroethyl)ether	7.104	93	7289	0.38	ng	100
9) Naphthalene	10.492	128	29145	0.39	ng	100
10) Hexachlorobutadiene	10.784	225	5550	0.39	ng	# 100
12) 2-Methylnaphthalene	12.111	142	18477	0.38	ng	100
16) Acenaphthylene	14.016	152	19002	0.32	ng	100
17) Acenaphthene	14.359	154	15587	0.37	ng	100
18) Fluorene	15.349	166	18890	0.36	ng	100
20) 4,6-Dinitro-2-methylph...	15.437	198	690	0.25	ng	100
21) 4-Bromophenyl-phenylether	16.252	248	5914	0.36	ng	100
22) Hexachlorobenzene	16.362	284	8303	0.39	ng	100
23) Atrazine	16.520	200	2600	0.25	ng	100
24) Pentachlorophenol	16.702	266	874	0.20	ng	100
25) Phenanthrene	17.092	178	32091	0.37	ng	100
26) Anthracene	17.177	178	22864	0.33	ng	100
28) Fluoranthene	19.114	202	32702	0.34	ng	100
30) Pyrene	19.481	202	31551	0.42	ng	100
32) Benzo(a)anthracene	21.229	228	23350	0.33	ng	100
33) Chrysene	21.282	228	31345	0.41	ng	100
34) Bis(2-ethylhexyl)phtha...	21.176	149	6662	0.22	ng	100
36) Indeno(1,2,3-cd)pyrene	25.687	276	26453	0.34	ng	100
37) Benzo(b)fluoranthene	22.801	252	27072	0.38	ng	100
38) Benzo(k)fluoranthene	22.846	252	29743	0.40	ng	100
39) Benzo(a)pyrene	23.369	252	22188	0.35	ng	100
40) Dibenzo(a,h)anthracene	25.700	278	22235	0.35	ng	100
41) Benzo(g,h,i)perylene	26.364	276	27074	0.40	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042921\
Data File : BN014486.D
Acq On : 29 Apr 2021 12:05
Operator : CG/JU
Sample : SSTDICCC0.4
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Quant Time: Apr 29 12:41:17 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 29 12:40:58 2021
Response via : Initial Calibration




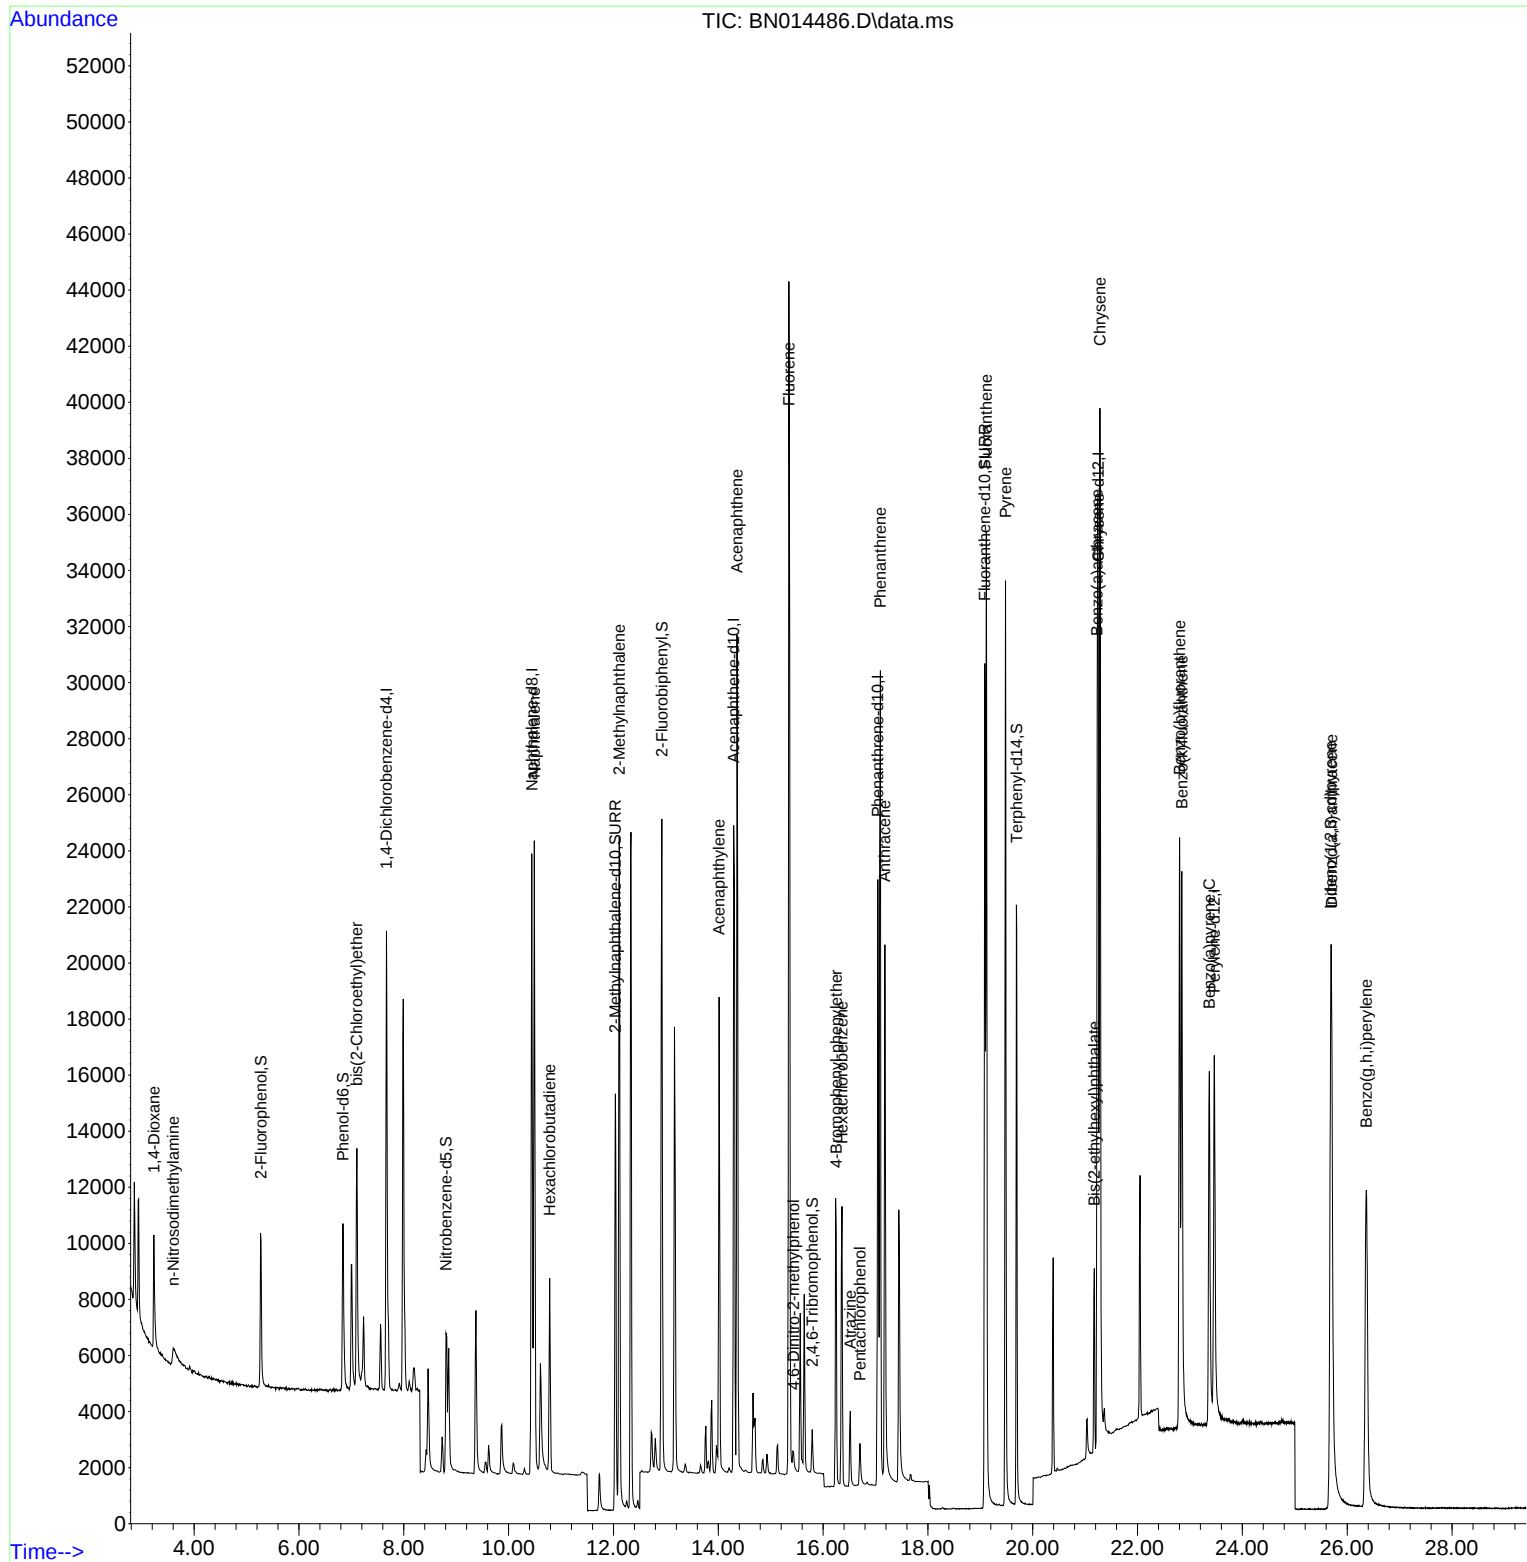




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.668 min Scan# 607
 Delta R.T. 0.000 min
 Lab File: BN014486.D
 Acq: 29 Apr 2021 12:05




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.4


Tgt Ion:152 Resp: 8126
 Ion Ratio Lower Upper
 152 100
 150 158.2 126.6 189.8
 115 59.6 47.7 71.5

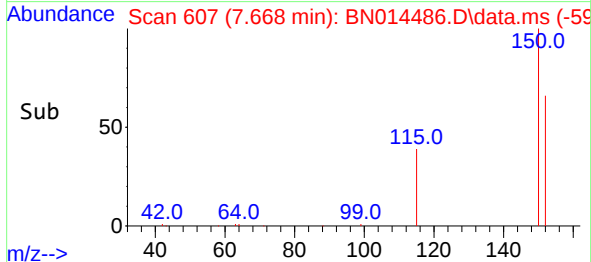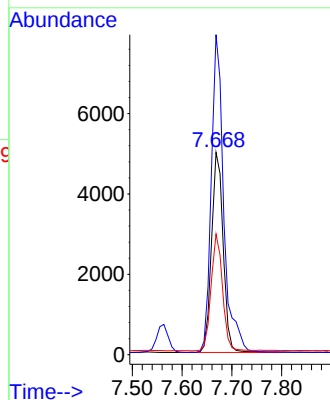

#2
 1,4-Dioxane
 Concen: 0.35 ng
 RT: 3.231 min Scan# 56
 Delta R.T. 0.000 min
 Lab File: BN014486.D
 Acq: 29 Apr 2021 12:05

Tgt Ion: 88 Resp: 3178
 Ion Ratio Lower Upper
 88 100
 58 69.2 55.4 83.0
 43 27.0 21.6 32.4



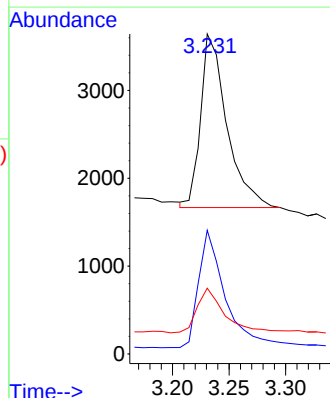





#3
n-Nitrosodimethylamine
Concen: 0.26 ng
RT: 3.601 min Scan# 102
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05




Instrument :
BNA_N
ClientSampled :
SSTDICCC0.4


Tgt Ion: 42 Resp: 1131
Ion Ratio Lower Upper
42 100
74 150.9 120.3 180.5
44 8.0 6.7 10.1

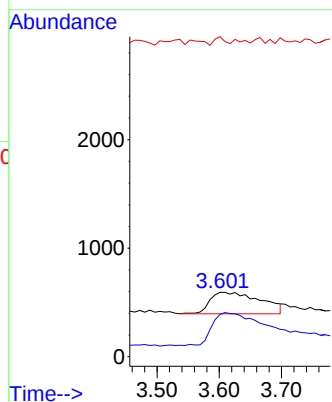

#4
2-Fluorophenol
Concen: 0.33 ng
RT: 5.276 min Scan# 310
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05

Tgt Ion: 112 Resp: 5066
Ion Ratio Lower Upper
112 100
64 53.0 42.4 63.6
63 27.8 22.2 33.4









#5
Phenol-d6
Concen: 0.32 ng
RT: 6.839 min Scan# 504
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05

Instrument :
BNA_N
ClientSampled :
SSTDICCC0.4

Tgt Ion: 99 Resp: 6067




Ion	Ratio	Lower	Upper
99	100		
42	17.3	13.8	20.8
71	32.5	26.0	39.0




#6
bis(2-Chloroethyl)ether
Concen: 0.38 ng
RT: 7.104 min Scan# 537
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05

Tgt Ion: 93 Resp: 7289

Ion	Ratio	Lower	Upper
93	100		
63	72.9	58.3	87.5
95	33.8	27.0	40.6


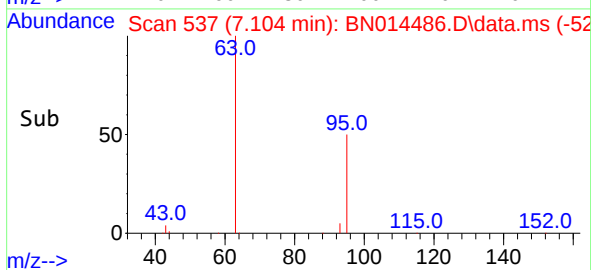






#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.442 min Scan# 855
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:	136	Resp:	29958
Ion Ratio	Lower	Upper	
136	100		
137	11.3	9.0	13.6
54	6.0	4.8	7.2
68	5.7	4.6	6.8

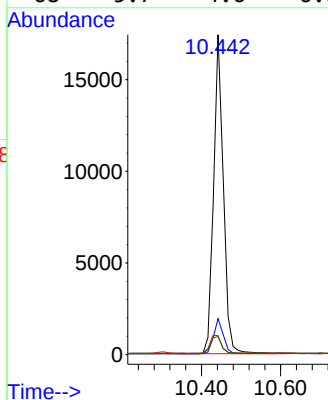

#8
Nitrobenzene-d5
Concen: 0.26 ng
RT: 8.807 min Scan# 726
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05

Tgt Ion:	82	Resp:	5265
Ion Ratio	Lower	Upper	
82	100		
128	32.5	26.0	39.0
54	49.4	39.5	59.3



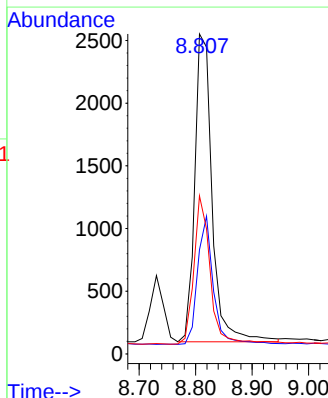



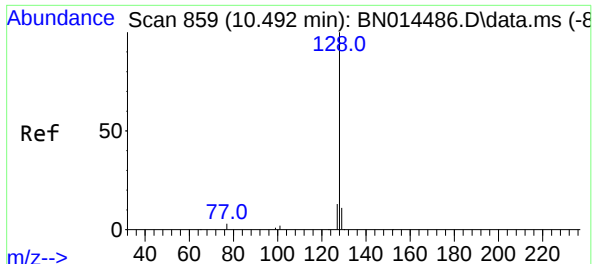

#9
Naphthalene
Concen: 0.39 ng
RT: 10.492 min Scan# 859
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:	128	Resp:	29145
Ion	Ratio	Lower	Upper
128	100		
129	11.3	9.0	13.6
127	12.8	10.2	15.4

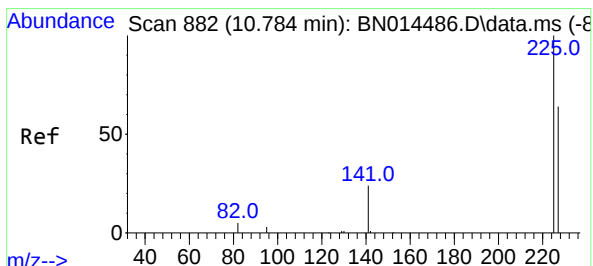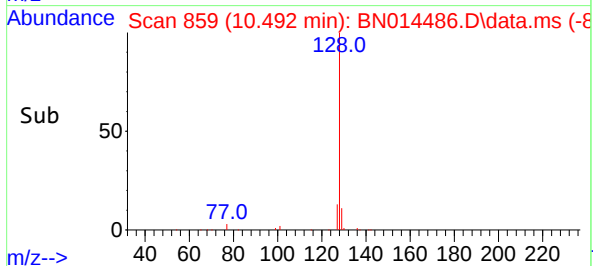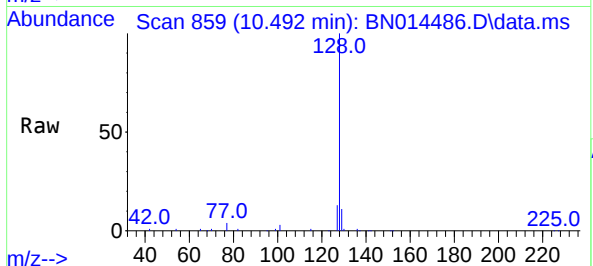

#10
Hexachlorobutadiene
Concen: 0.39 ng
RT: 10.784 min Scan# 882
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05

Tgt Ion:	225	Resp:	5550
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	64.7	51.8	77.6


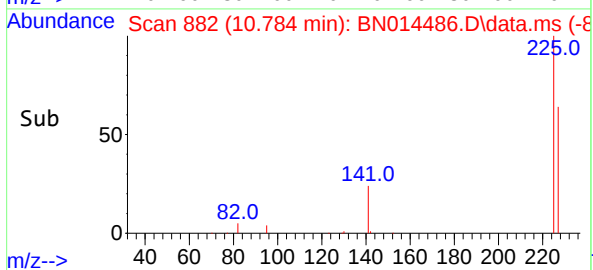

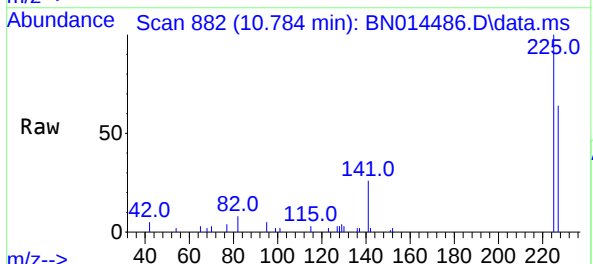




#11
2-Methylnaphthalene-d10
Concen: 0.49 ng
RT: 12.035 min Scan# 1058
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:152 Resp: 22097
Ion Ratio Lower Upper
152 100
151 20.4 16.3 24.5

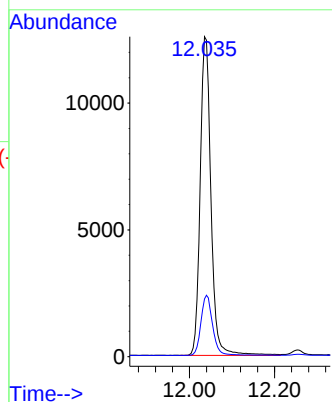

#12
2-Methylnaphthalene
Concen: 0.38 ng
RT: 12.111 min Scan# 1075
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05

Tgt Ion:142 Resp: 18477
Ion Ratio Lower Upper
142 100
141 88.1 70.5 105.7
115 34.4 27.5 41.3



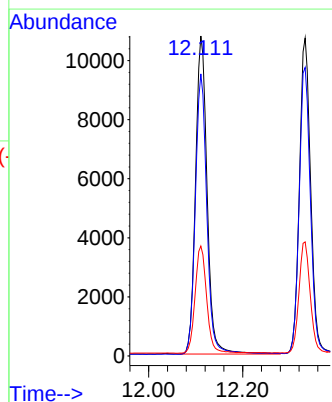
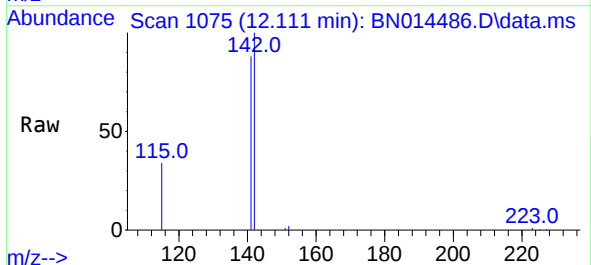




#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.295 min Scan# 1305
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:164 Resp: 15211
Ion Ratio Lower Upper
164 100
162 103.0 82.4 123.6
160 50.6 40.5 60.7

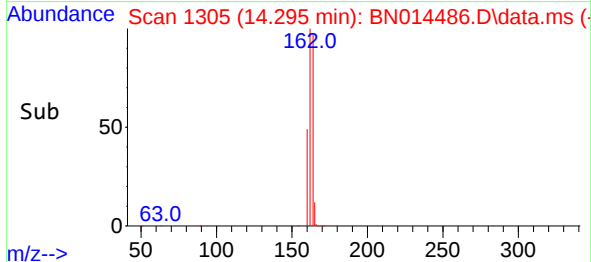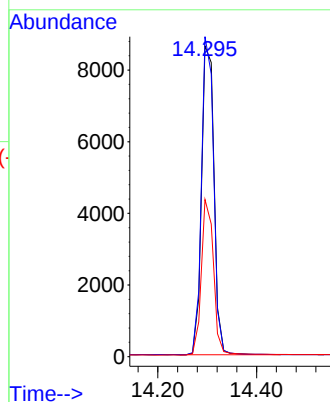

#14
2,4,6-Tribromophenol
Concen: 0.25 ng
RT: 15.793 min Scan# 1423
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05

Tgt Ion:330 Resp: 1270
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 35.3 28.5 42.7


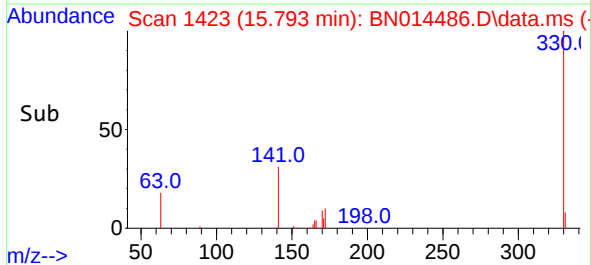
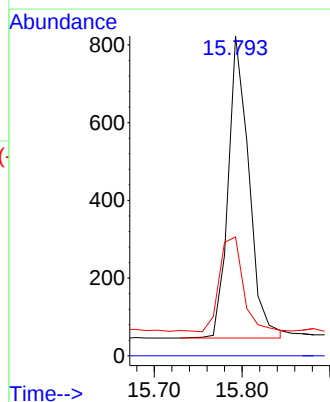





#15
2-Fluorobiphenyl
Concen: 0.39 ng
RT: 12.925 min Scan# 1197
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:172	Resp:	22266
Ion Ratio	Lower	Upper
172	100	
171	33.3	26.6 40.0
170	22.7	18.2 27.2

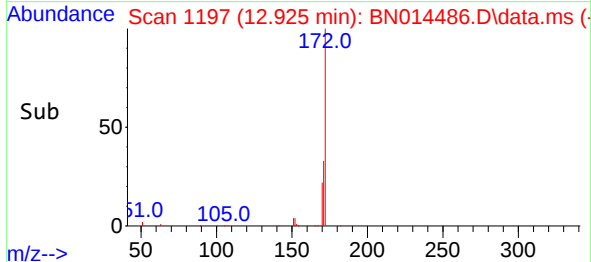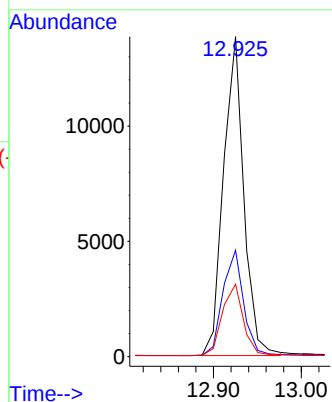

#16
Acenaphthylene
Concen: 0.32 ng
RT: 14.016 min Scan# 1283
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05

Tgt Ion:152	Resp:	19002
Ion Ratio	Lower	Upper
152	100	
151	19.4	15.6 23.4
153	13.4	10.7 16.1




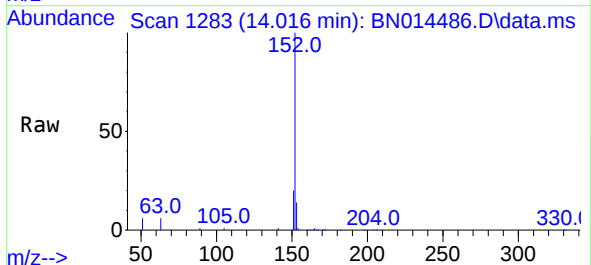




#17
Acenaphthene
Concen: 0.37 ng
RT: 14.359 min Scan# 1310
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:154 Resp: 15587
Ion Ratio Lower Upper
154 100
153 112.9 90.3 135.5
152 59.1 47.3 70.9

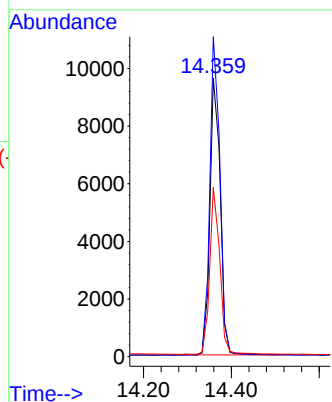

#18
Fluorene
Concen: 0.36 ng
RT: 15.349 min Scan# 1388
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05

Tgt Ion:166 Resp: 18890
Ion Ratio Lower Upper
166 100
165 97.7 78.2 117.2
167 13.6 10.9 16.3


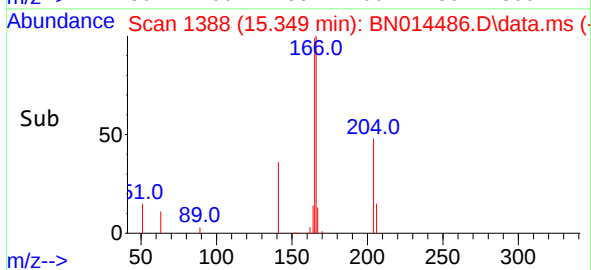
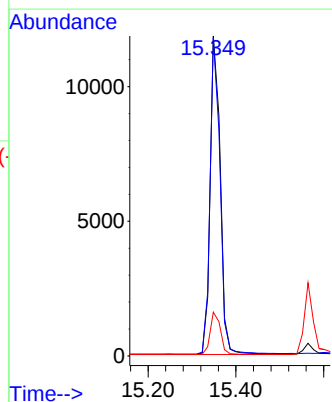





#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.043 min Scan# 1525
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:188 Resp: 31524
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 11.0 8.8 13.2

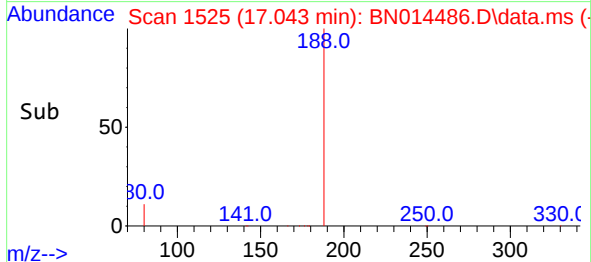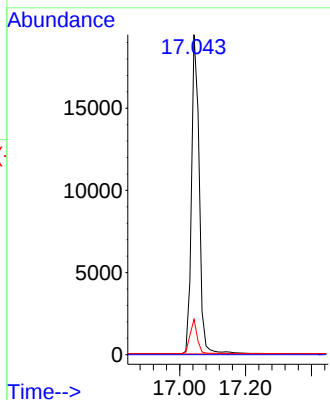

#20
4,6-Dinitro-2-methylphenol
Concen: 0.25 ng
RT: 15.437 min Scan# 1395
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05

Tgt Ion:198 Resp: 690
Ion Ratio Lower Upper
198 100
51 145.0 116.0 174.0
105 56.6 45.3 67.9



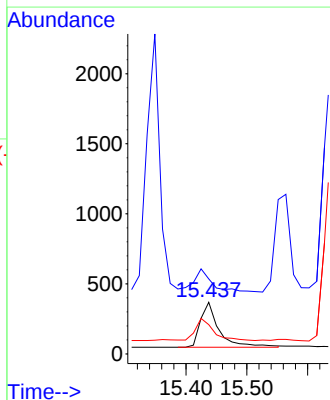
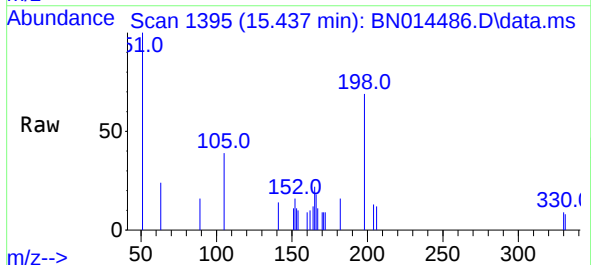




#21
4-Bromophenyl-phenylether
Concen: 0.36 ng
RT: 16.252 min Scan# 1460
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05




Instrument :
BNA_N
ClientSampled :
SSTDICCC0.4


Tgt Ion:248 Resp: 5914
Ion Ratio Lower Upper
248 100
250 105.7 84.6 126.8
141 33.4 26.7 40.1

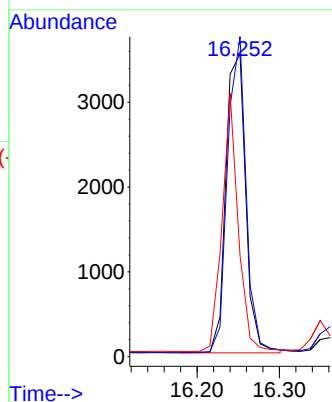

#22
Hexachlorobenzene
Concen: 0.39 ng
RT: 16.362 min Scan# 1469
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05

Tgt Ion:284 Resp: 8303
Ion Ratio Lower Upper
284 100
142 33.8 27.0 40.6
249 29.6 23.6 35.4


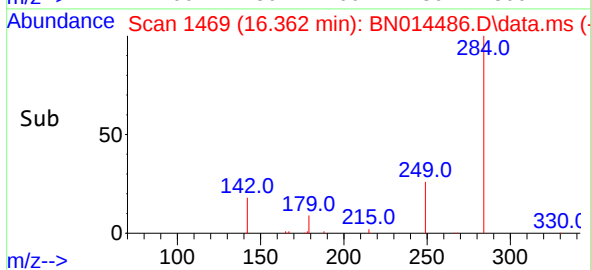






#23
Atrazine
Concen: 0.25 ng
RT: 16.520 min Scan# 1482
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:	200	Resp:	2600
Ion	Ratio	Lower	Upper
200	100		
173	25.0	20.0	30.0
215	48.8	39.0	58.6



#24
Pentachlorophenol
Concen: 0.20 ng
RT: 16.702 min Scan# 1497
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05

Tgt Ion:	266	Resp:	874
Ion	Ratio	Lower	Upper
266	100		
264	62.4	49.9	74.9
268	62.4	49.9	74.9


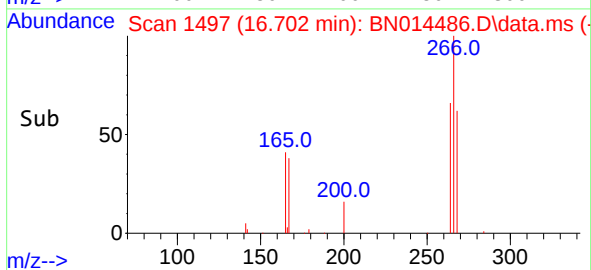






#25
Phenanthrene
Concen: 0.37 ng
RT: 17.092 min Scan# 1529
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:	178	Resp:	32091
Ion	Ratio	Lower	Upper
178	100		
176	18.9	15.1	22.7
179	15.3	12.2	18.4

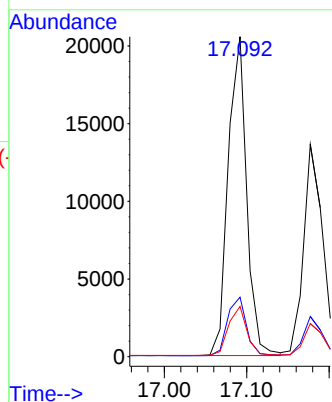

#26
Anthracene
Concen: 0.33 ng
RT: 17.177 min Scan# 1536
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05

Tgt Ion:	178	Resp:	22864
Ion	Ratio	Lower	Upper
178	100		
176	18.3	14.6	22.0
179	15.1	12.2	18.2


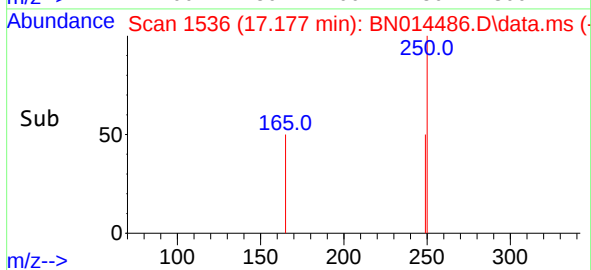






#27
Fluoranthene-d10
Concen: 0.43 ng
RT: 19.084 min Scan# 1820
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:212 Resp: 36925
Ion Ratio Lower Upper
212 100
106 12.8 10.2 15.4
104 7.0 5.6 8.4

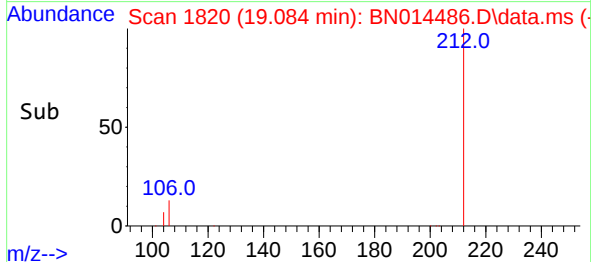

#28
Fluoranthene
Concen: 0.34 ng
RT: 19.114 min Scan# 1826
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05

Tgt Ion:202 Resp: 32702
Ion Ratio Lower Upper
202 100
101 10.9 8.7 13.1
203 17.0 13.6 20.4









#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.250 min Scan# 2123
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:240 Resp: 25522
Ion Ratio Lower Upper
240 100
120 7.9 6.3 9.5
236 26.1 20.9 31.3

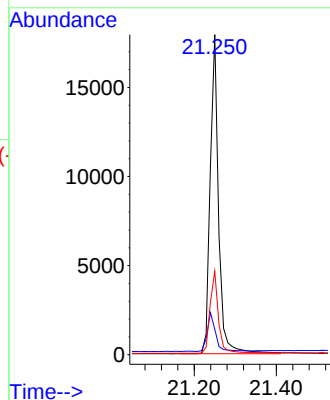

#30
Pyrene
Concen: 0.42 ng
RT: 19.481 min Scan# 1900
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05

Tgt Ion:202 Resp: 31551
Ion Ratio Lower Upper
202 100
200 20.5 16.4 24.6
203 17.4 13.9 20.9



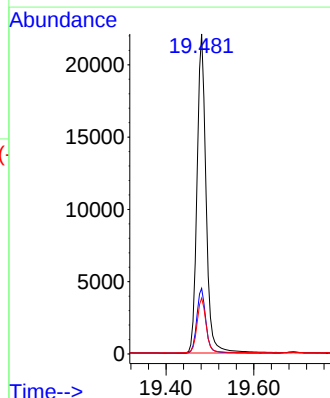





#31
 Terphenyl-d14
 Concen: 0.45 ng
 RT: 19.690 min Scan# 1942
 Delta R.T. 0.000 min
 Lab File: BN014486.D
 Acq: 29 Apr 2021 12:05




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.4


Tgt Ion:244 Resp: 22959
 Ion Ratio Lower Upper
 244 100
 212 7.9 6.3 9.5
 122 13.3 10.6 16.0

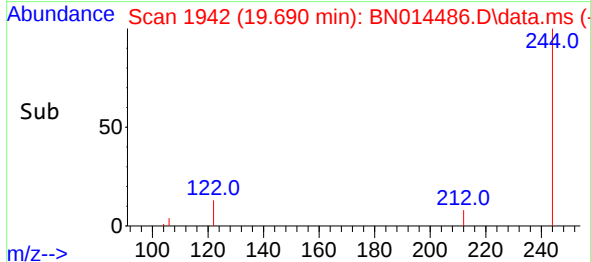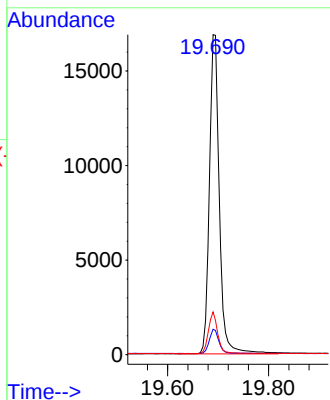

#32
 Benzo(a)anthracene
 Concen: 0.33 ng
 RT: 21.229 min Scan# 2121
 Delta R.T. 0.000 min
 Lab File: BN014486.D
 Acq: 29 Apr 2021 12:05

Tgt Ion:228 Resp: 23350
 Ion Ratio Lower Upper
 228 100
 226 27.3 21.8 32.8
 229 19.7 15.8 23.6


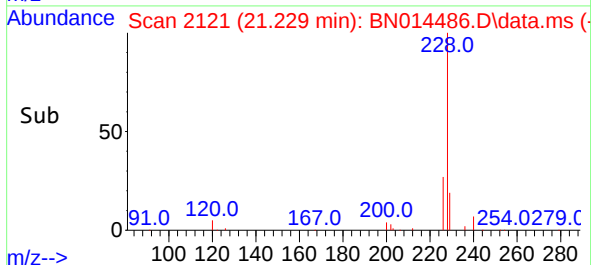
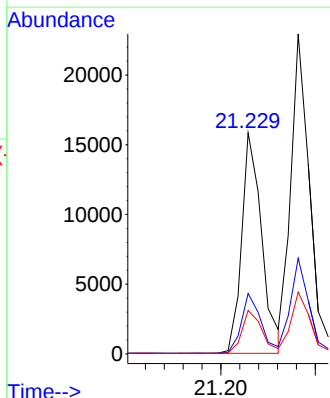



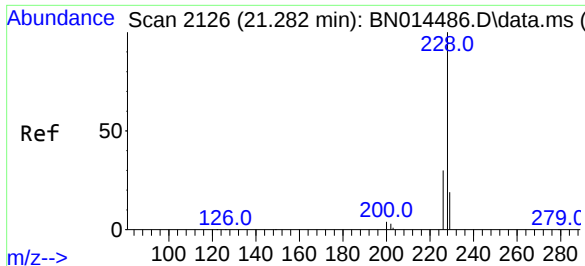

#33
Chrysene
Concen: 0.41 ng
RT: 21.282 min Scan# 2126
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:	228	Resp:	31345
Ion Ratio	Lower	Upper	
228	100		
226	29.9	23.9	35.9
229	19.4	15.5	23.3

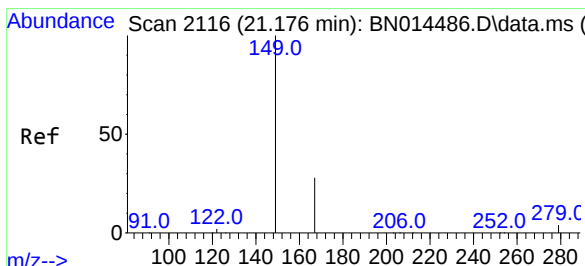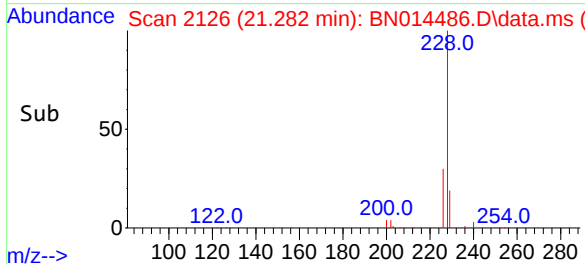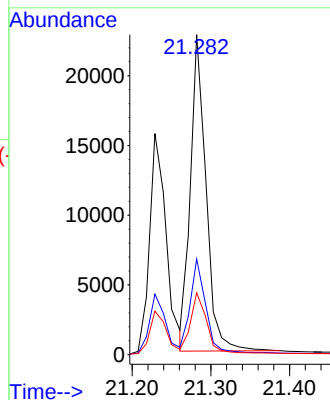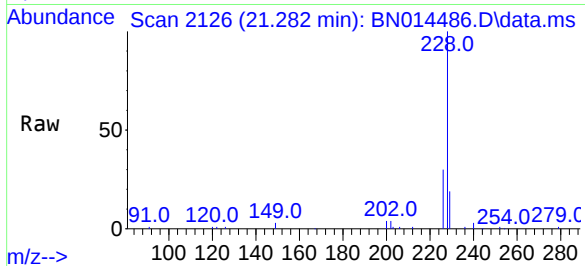

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.22 ng
RT: 21.176 min Scan# 2116
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05

Tgt Ion:	149	Resp:	6662
Ion Ratio	Lower	Upper	
149	100		
167	26.8	21.4	32.2
279	4.1	3.3	4.9


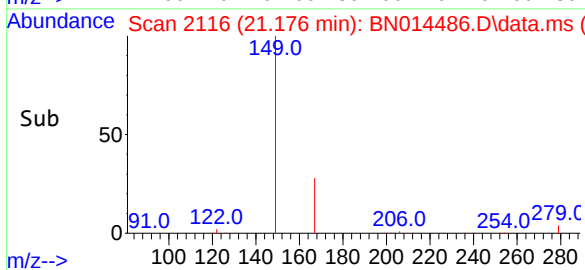
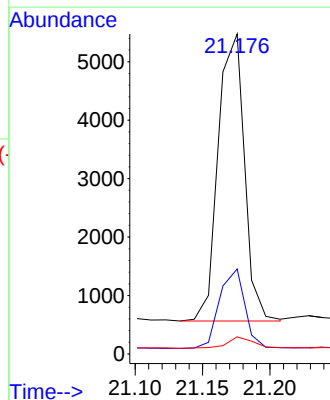
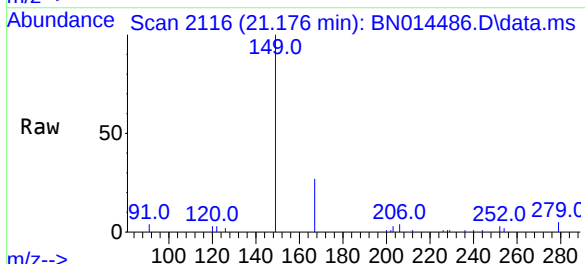




#35
Perylene-d12
Concen: 0.40 ng
RT: 23.465 min Scan# 2541
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:264	Resp:	19972
Ion Ratio	Lower	Upper
264	100	
260	24.5	19.6 29.4
265	44.4	35.5 53.3

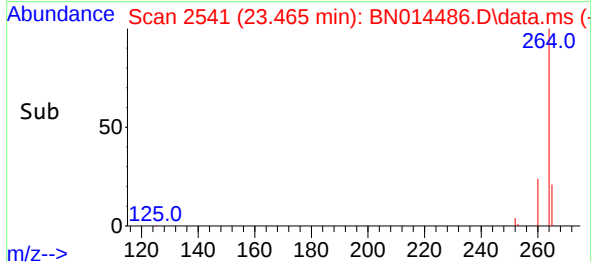

#36
Indeno(1,2,3-cd)pyrene
Concen: 0.34 ng
RT: 25.687 min Scan# 3190
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05

Tgt Ion:276	Resp:	26453
Ion Ratio	Lower	Upper
276	100	
138	25.1	20.1 30.1
277	24.7	19.8 29.8




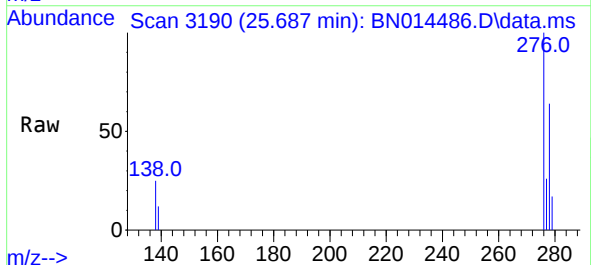




#37
Benzo(b)fluoranthene
Concen: 0.38 ng
RT: 22.801 min Scan# 2347
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:252 Resp: 27072
Ion Ratio Lower Upper
252 100
253 24.6 19.7 29.5
125 12.5 10.0 15.0

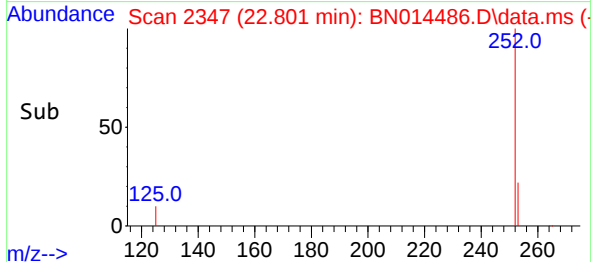

#38
Benzo(k)fluoranthene
Concen: 0.40 ng
RT: 22.846 min Scan# 2360
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05

Tgt Ion:252 Resp: 29743
Ion Ratio Lower Upper
252 100
253 24.3 19.4 29.2
125 12.5 10.0 15.0


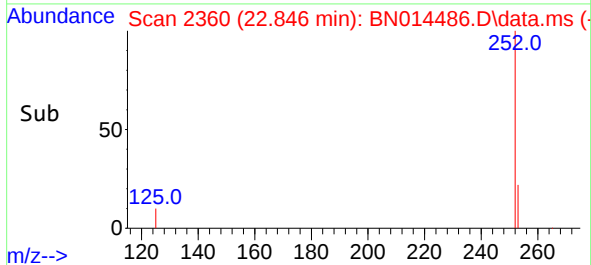






#39
Benzo(a)pyrene
Concen: 0.35 ng
RT: 23.369 min Scan# 2513
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:	252	Resp:	22188
Ion Ratio	Lower	Upper	
252	100		
253	26.0	20.8	31.2
125	15.8	12.6	19.0

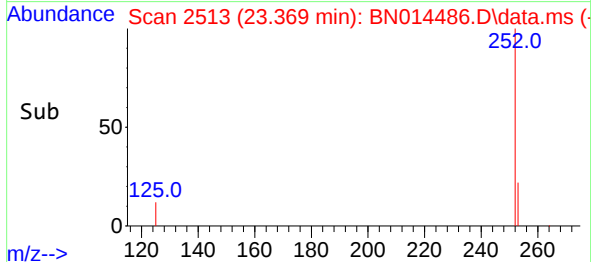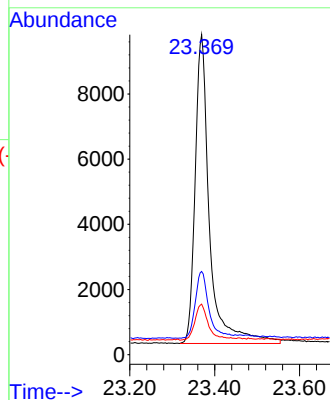

#40
Dibenzo(a,h)anthracene
Concen: 0.35 ng
RT: 25.700 min Scan# 3194
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05


Tgt Ion:	278	Resp:	22235
Ion Ratio	Lower	Upper	
278	100		
139	17.8	14.2	21.4
279	26.2	21.0	31.4

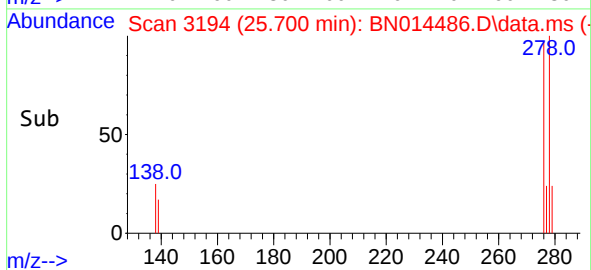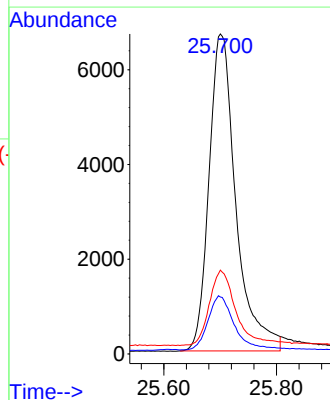

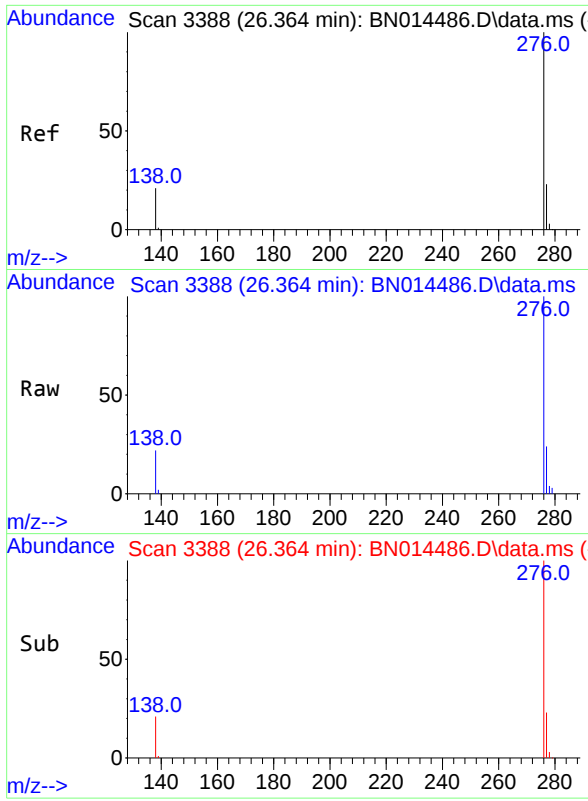

#41
Benzo(g,h,i)perylene
Concen: 0.40 ng
RT: 26.364 min Scan# 3388
Delta R.T. 0.000 min
Lab File: BN014486.D
Acq: 29 Apr 2021 12:05

Tgt Ion:	276	Resp:	27074
Ion	Ratio	Lower	Upper
276	100		
277	24.3	19.4	29.2
138	21.9	17.5	26.3

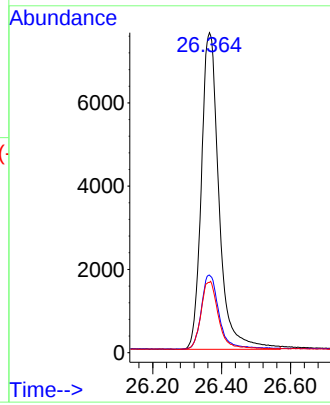

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4