

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042921\
 Data File : BN014489.D
 Acq On : 29 Apr 2021 13:52
 Operator : CG/JU
 Sample : SSTDICC3.2
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2

Quant Time: Apr 29 14:21:36 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 29 12:40:58 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.668	152	7687	0.40	ng	0.00
7) Naphthalene-d8	10.442	136	25955	0.40	ng	0.00
13) Acenaphthene-d10	14.295	164	14041	0.40	ng	0.00
19) Phenanthrene-d10	17.043	188	27308	0.40	ng	0.00
29) Chrysene-d12	21.250	240	28450	0.40	ng	0.00
35) Perylene-d12	23.465	264	21345	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.276	112	46829	3.24	ng	0.00
5) Phenol-d6	6.839	99	60092	3.36	ng	0.00
8) Nitrobenzene-d5	8.807	82	49567	2.86	ng	0.00
11) 2-Methylnaphthalene-d10	12.035	152	181177	4.62	ng	0.00
14) 2,4,6-Tribromophenol	15.793	330	15045	3.25	ng	0.00
15) 2-Fluorobiphenyl	12.925	172	178306	3.37	ng	0.00
27) Fluoranthene-d10	19.084	212	348734	4.66	ng	0.00
31) Terphenyl-d14	19.690	244	207896	3.65	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.231	88	27394	3.20	ng	96
3) n-Nitrosodimethylamine	3.561	42	15657	3.77	ng	96
6) bis(2-Chloroethyl)ether	7.104	93	61254	3.34	ng	98
9) Naphthalene	10.492	128	227650	3.55	ng	99
10) Hexachlorobutadiene	10.784	225	42629	3.43	ng	# 99
12) 2-Methylnaphthalene	12.111	142	150972	3.58	ng	99
16) Acenaphthylene	14.016	152	193069	3.50	ng	99
17) Acenaphthene	14.359	154	136633	3.54	ng	96
18) Fluorene	15.349	166	169225	3.49	ng	100
20) 4,6-Dinitro-2-methylph...	15.425	198	10178	4.26	ng	# 47
21) 4-Bromophenyl-phenylether	16.240	248	51797	3.63	ng	# 67
22) Hexachlorobenzene	16.362	284	66544	3.61	ng	99
23) Atrazine	16.520	200	28379	3.15	ng	96
24) Pentachlorophenol	16.702	266	13936	3.69	ng	99
25) Phenanthrene	17.092	178	274461	3.62	ng	100
26) Anthracene	17.177	178	225244	3.76	ng	100
28) Fluoranthene	19.114	202	313938	3.74	ng	99
30) Pyrene	19.481	202	302803	3.61	ng	100
32) Benzo(a)anthracene	21.229	228	275091	3.51	ng	100
33) Chrysene	21.282	228	312918	3.66	ng	100
34) Bis(2-ethylhexyl)phtha...	21.176	149	64992	1.96	ng	100
36) Indeno(1,2,3-cd)pyrene	25.690	276	319659	3.89	ng	100
37) Benzo(b)fluoranthene	22.801	252	288621	3.80	ng	# 94
38) Benzo(k)fluoranthene	22.846	252	316437	4.03	ng	# 95
39) Benzo(a)pyrene	23.369	252	253425	3.70	ng	# 91
40) Dibenzo(a,h)anthracene	25.700	278	271454	3.97	ng	96
41) Benzo(g,h,i)perylene	26.364	276	282708	3.90	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042921\
Data File : BN014489.D
Acq On : 29 Apr 2021 13:52
Operator : CG/JU
Sample : SSTDIC3.2
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Quant Time: Apr 29 14:21:36 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 29 12:40:58 2021
Response via : Initial Calibration









#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.668 min Scan# 607
 Delta R.T. 0.000 min
 Lab File: BN014489.D
 Acq: 29 Apr 2021 13:52

Instrument :
 BNA_N
 ClientSampleId :
 SSTDIC3.2

Tgt Ion:152 Resp: 7687




Ion	Ratio	Lower	Upper
152	100		
150	154.8	126.6	189.8
115	58.3	47.7	71.5




#2
 1,4-Dioxane
 Concen: 3.20 ng
 RT: 3.231 min Scan# 56
 Delta R.T. 0.000 min
 Lab File: BN014489.D
 Acq: 29 Apr 2021 13:52

Tgt Ion: 88 Resp: 27394

Ion	Ratio	Lower	Upper
88	100		
58	65.8	55.4	83.0
43	24.5	21.6	32.4









#3
n-Nitrosodimethylamine
Concen: 3.77 ng
RT: 3.561 min Scan# 97
Delta R.T. -0.040 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Tgt Ion: 42 Resp: 15657




Ion	Ratio	Lower	Upper
42	100		
74	145.7	120.3	180.5
44	7.4	6.7	10.1




#4
2-Fluorophenol
Concen: 3.24 ng
RT: 5.276 min Scan# 310
Delta R.T. 0.000 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52

Tgt Ion: 112 Resp: 46829

Ion	Ratio	Lower	Upper
112	100		
64	52.3	42.4	63.6
63	27.2	22.2	33.4









#5
Phenol-d6
Concen: 3.36 ng
RT: 6.839 min Scan# 504
Delta R.T. 0.000 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion: 99 Resp: 60092
Ion Ratio Lower Upper
99 100
42 16.7 13.8 20.8
71 31.9 26.0 39.0



#6
bis(2-Chloroethyl)ether
Concen: 3.34 ng
RT: 7.104 min Scan# 537
Delta R.T. 0.000 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52

Tgt Ion: 93 Resp: 61254
Ion Ratio Lower Upper
93 100
63 70.9 58.3 87.5
95 33.1 27.0 40.6









#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.442 min Scan# 855
Delta R.T. 0.000 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:	136	Resp:	25955
Ion Ratio	Lower	Upper	
136	100		
137	11.2	9.0	13.6
54	5.8	4.8	7.2
68	5.6	4.6	6.8



#8
Nitrobenzene-d5
Concen: 2.86 ng
RT: 8.807 min Scan# 726
Delta R.T. 0.000 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52

Tgt Ion:	82	Resp:	49567
Ion Ratio	Lower	Upper	
82	100		
128	35.0	26.0	39.0
54	46.0	39.5	59.3







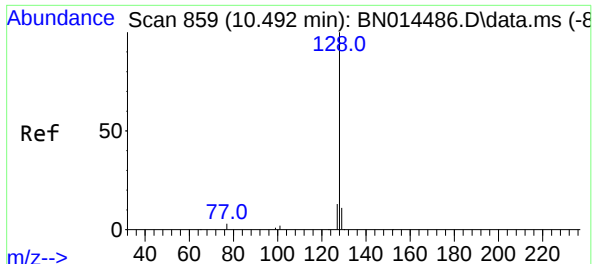

#9
Naphthalene
Concen: 3.55 ng
RT: 10.492 min Scan# 859
Delta R.T. 0.000 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:128 Resp: 227650
Ion Ratio Lower Upper
128 100
129 11.0 9.0 13.6
127 12.7 10.2 15.4



#10
Hexachlorobutadiene
Concen: 3.43 ng
RT: 10.784 min Scan# 882
Delta R.T. 0.000 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52

Tgt Ion:225 Resp: 42629
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.7 51.8 77.6









#11
2-Methylnaphthalene-d10
Concen: 4.62 ng
RT: 12.035 min Scan# 1058
Delta R.T. 0.000 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:152 Resp: 181177
Ion Ratio Lower Upper
152 100
151 20.2 16.3 24.5



#12
2-Methylnaphthalene
Concen: 3.58 ng
RT: 12.111 min Scan# 1075
Delta R.T. 0.000 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52

Tgt Ion:142 Resp: 150972
Ion Ratio Lower Upper
142 100
141 87.2 70.5 105.7
115 33.2 27.5 41.3









#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.295 min Scan# 1305
Delta R.T. 0.000 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:164 Resp: 14041
Ion Ratio Lower Upper
164 100
162 102.8 82.4 123.6
160 48.8 40.5 60.7



#14
2,4,6-Tribromophenol
Concen: 3.25 ng
RT: 15.793 min Scan# 1423
Delta R.T. 0.000 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52

Tgt Ion:330 Resp: 15045
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 34.9 28.5 42.7









#15
2-Fluorobiphenyl
Concen: 3.37 ng
RT: 12.925 min Scan# 1197
Delta R.T. 0.000 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:172 Resp: 178306
Ion Ratio Lower Upper
172 100
171 32.9 26.6 40.0
170 21.5 18.2 27.2



#16
Acenaphthylene
Concen: 3.50 ng
RT: 14.016 min Scan# 1283
Delta R.T. 0.000 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52

Tgt Ion:152 Resp: 193069
Ion Ratio Lower Upper
152 100
151 19.2 15.6 23.4
153 13.0 10.7 16.1









#17
Acenaphthene
Concen: 3.54 ng
RT: 14.359 min Scan# 1310
Delta R.T. 0.000 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:154 Resp: 136633
Ion Ratio Lower Upper
154 100
153 109.5 90.3 135.5
152 55.2 47.3 70.9



#18
Fluorene
Concen: 3.49 ng
RT: 15.349 min Scan# 1388
Delta R.T. 0.000 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52

Tgt Ion:166 Resp: 169225
Ion Ratio Lower Upper
166 100
165 97.4 78.2 117.2
167 13.5 10.9 16.3









#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.043 min Scan# 1525
Delta R.T. 0.000 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:188 Resp: 27308
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 10.5 8.8 13.2



#20
4,6-Dinitro-2-methylphenol
Concen: 4.26 ng
RT: 15.425 min Scan# 1394
Delta R.T. -0.013 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52

Tgt Ion:198 Resp: 10178
Ion Ratio Lower Upper
198 100
51 54.8 116.0 174.0#
105 58.0 45.3 67.9









#21
4-Bromophenyl-phenylether
Concen: 3.63 ng
RT: 16.240 min Scan# 1459
Delta R.T. -0.012 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:248 Resp: 51797
Ion Ratio Lower Upper
248 100
250 90.1 84.6 126.8
141 84.7 26.7 40.1#



#22
Hexachlorobenzene
Concen: 3.61 ng
RT: 16.362 min Scan# 1469
Delta R.T. 0.000 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52

Tgt Ion:284 Resp: 66544
Ion Ratio Lower Upper
284 100
142 33.2 27.0 40.6
249 29.1 23.6 35.4









#23
Atrazine
Concen: 3.15 ng
RT: 16.520 min Scan# 1482
Delta R.T. 0.000 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:200 Resp: 28379
Ion Ratio Lower Upper
200 100
173 20.7 20.0 30.0
215 50.0 39.0 58.6



#24
Pentachlorophenol
Concen: 3.69 ng
RT: 16.702 min Scan# 1497
Delta R.T. 0.000 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52

Tgt Ion:266 Resp: 13936
Ion Ratio Lower Upper
266 100
264 62.5 49.9 74.9
268 63.7 49.9 74.9









#25
Phenanthrene
Concen: 3.62 ng
RT: 17.092 min Scan# 1529
Delta R.T. 0.000 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52




Instrument :
BNA_N
ClientSampleId :
SSTDIC3.2


Tgt Ion:178 Resp: 274461
Ion Ratio Lower Upper
178 100
176 18.8 15.1 22.7
179 15.3 12.2 18.4



#26
Anthracene
Concen: 3.76 ng
RT: 17.177 min Scan# 1536
Delta R.T. 0.000 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52

Tgt Ion:178 Resp: 225244
Ion Ratio Lower Upper
178 100
176 18.3 14.6 22.0
179 15.3 12.2 18.2









#27
Fluoranthene-d10
Concen: 4.66 ng
RT: 19.084 min Scan# 1820
Delta R.T. 0.000 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:212 Resp: 348734
Ion Ratio Lower Upper
212 100
106 12.6 10.2 15.4
104 6.9 5.6 8.4



#28
Fluoranthene
Concen: 3.74 ng
RT: 19.114 min Scan# 1826
Delta R.T. 0.000 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52

Tgt Ion:202 Resp: 313938
Ion Ratio Lower Upper
202 100
101 10.8 8.7 13.1
203 17.5 13.6 20.4









#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.250 min Scan# 2123
Delta R.T. 0.000 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:240 Resp: 28450
Ion Ratio Lower Upper
240 100
120 7.5 6.3 9.5
236 25.9 20.9 31.3



#30
Pyrene
Concen: 3.61 ng
RT: 19.481 min Scan# 1900
Delta R.T. 0.000 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52

Tgt Ion:202 Resp: 302803
Ion Ratio Lower Upper
202 100
200 20.5 16.4 24.6
203 17.5 13.9 20.9









#31
 Terphenyl-d14
 Concen: 3.65 ng
 RT: 19.690 min Scan# 1942
 Delta R.T. 0.000 min
 Lab File: BN014489.D
 Acq: 29 Apr 2021 13:52




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2


Tgt Ion:244 Resp: 207896
 Ion Ratio Lower Upper
 244 100
 212 7.4 6.3 9.5
 122 12.1 10.6 16.0



#32
 Benzo(a)anthracene
 Concen: 3.51 ng
 RT: 21.229 min Scan# 2121
 Delta R.T. 0.000 min
 Lab File: BN014489.D
 Acq: 29 Apr 2021 13:52

Tgt Ion:228 Resp: 275091
 Ion Ratio Lower Upper
 228 100
 226 27.3 21.8 32.8
 229 19.2 15.8 23.6









#33
Chrysene
Concen: 3.66 ng
RT: 21.282 min Scan# 2126
Delta R.T. 0.000 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:228 Resp: 312918
Ion Ratio Lower Upper
228 100
226 29.9 23.9 35.9
229 19.4 15.5 23.3



#34
Bis(2-ethylhexyl)phthalate
Concen: 1.96 ng
RT: 21.176 min Scan# 2116
Delta R.T. 0.000 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52

Tgt Ion:149 Resp: 64992
Ion Ratio Lower Upper
149 100
167 26.8 21.4 32.2
279 3.5 3.3 4.9









#35
Perylene-d12
Concen: 0.40 ng
RT: 23.465 min Scan# 2541
Delta R.T. 0.000 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:264	Resp:	21345
Ion Ratio	Lower	Upper
264	100	
260	24.8	19.6 29.4
265	42.3	35.5 53.3



#36
Indeno(1,2,3-cd)pyrene
Concen: 3.89 ng
RT: 25.690 min Scan# 3191
Delta R.T. 0.003 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52

Tgt Ion:276	Resp:	319659
Ion Ratio	Lower	Upper
276	100	
138	25.0	20.1 30.1
277	24.8	19.8 29.8









#37
Benzo(b)fluoranthene
Concen: 3.80 ng
RT: 22.801 min Scan# 2347
Delta R.T. 0.000 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:252 Resp: 288621
Ion Ratio Lower Upper
252 100
253 22.0 19.7 29.5
125 10.0 10.0 15.0#



#38
Benzo(k)fluoranthene
Concen: 4.03 ng
RT: 22.846 min Scan# 2360
Delta R.T. 0.000 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52

Tgt Ion:252 Resp: 316437
Ion Ratio Lower Upper
252 100
253 22.1 19.4 29.2
125 9.7 10.0 15.0#









#39
Benzo(a)pyrene
Concen: 3.70 ng
RT: 23.369 min Scan# 2513
Delta R.T. 0.000 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:252 Resp: 253425
Ion Ratio Lower Upper
252 100
253 21.9 20.8 31.2
125 11.2 12.6 19.0#



#40
Dibenzo(a,h)anthracene
Concen: 3.97 ng
RT: 25.700 min Scan# 3194
Delta R.T. 0.000 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52


Tgt Ion:278 Resp: 271454
Ion Ratio Lower Upper
278 100
139 16.6 14.2 21.4
279 23.3 21.0 31.4





#41
Benzo(g,h,i)perylene
Concen: 3.90 ng
RT: 26.364 min Scan# 3388
Delta R.T. 0.000 min
Lab File: BN014489.D
Acq: 29 Apr 2021 13:52

Tgt Ion: 276 Resp: 282708
Ion Ratio Lower Upper
276 100
277 23.6 19.4 29.2
138 21.6 17.5 26.3



Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2